

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulate Liquid for Head 750

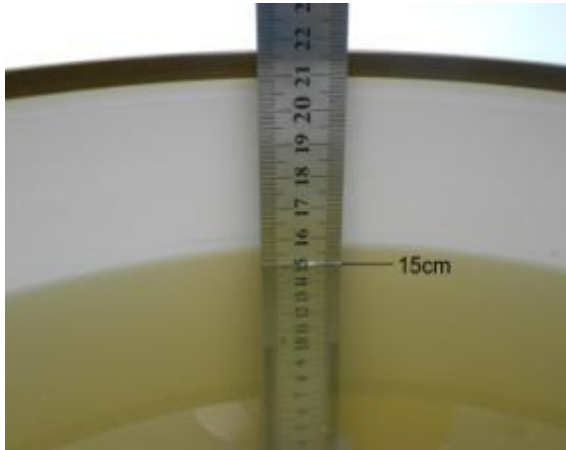


Photo 2: Tissue Simulate Liquid for Head 835

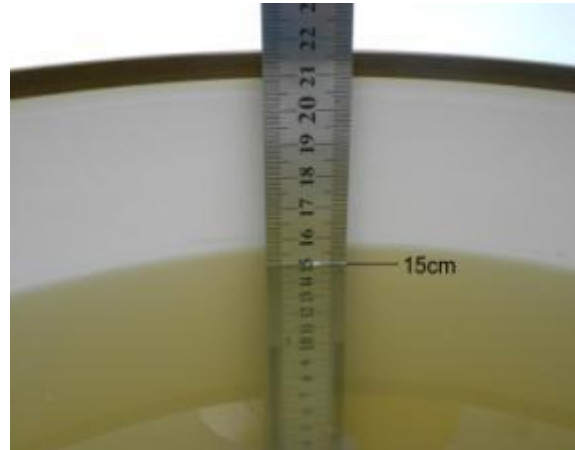


Photo 3: Tissue Simulate Liquid for Head 1800

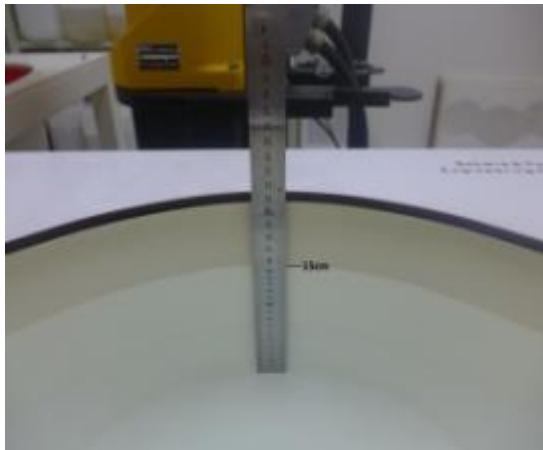


Photo 4: Tissue Simulate Liquid for Head 1900

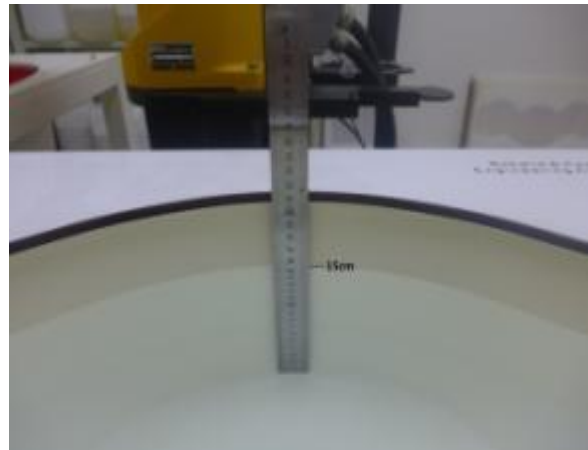


Photo 5: Tissue Simulate Liquid for Head 2450


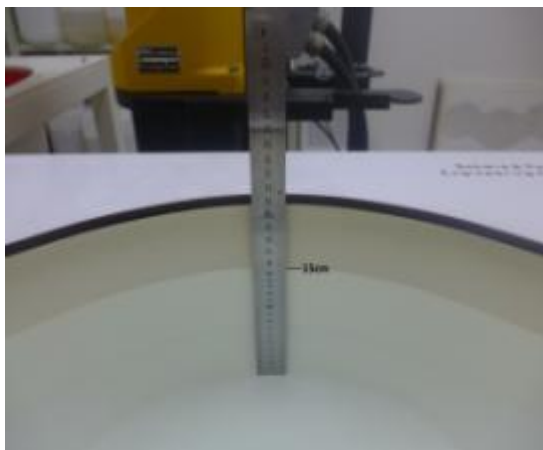

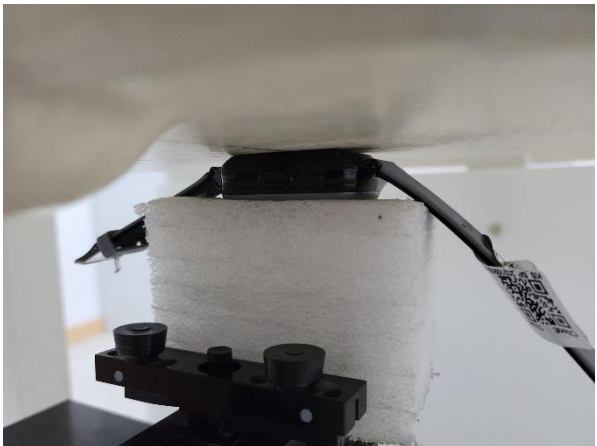


Photo 6: Tissue Simulate Liquid for Head 2450

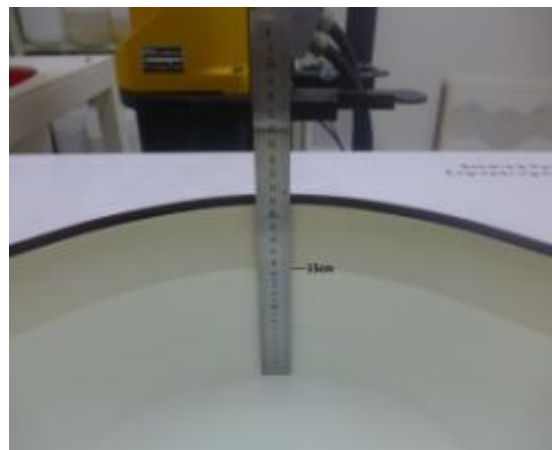

3. Photographs of EUT test position

Photo 7: Next to the Mouth 10mm	Photo 8: Back side 0mm
	

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.