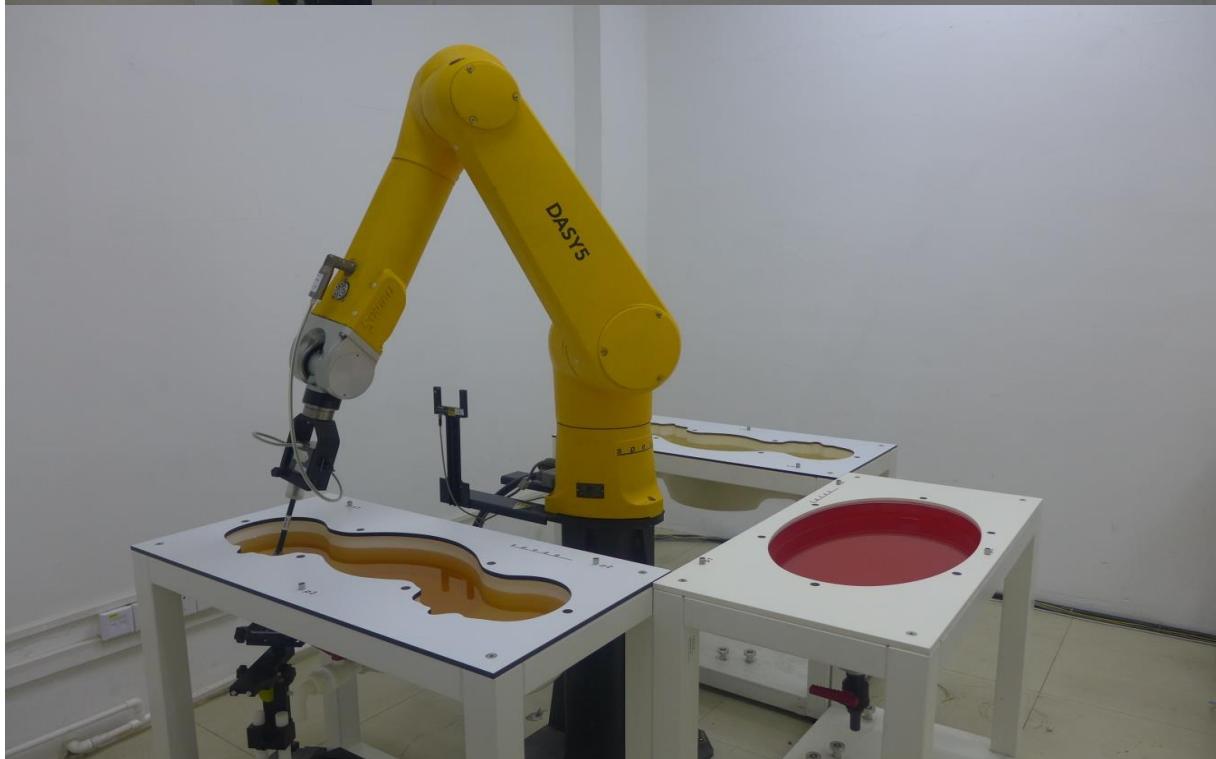
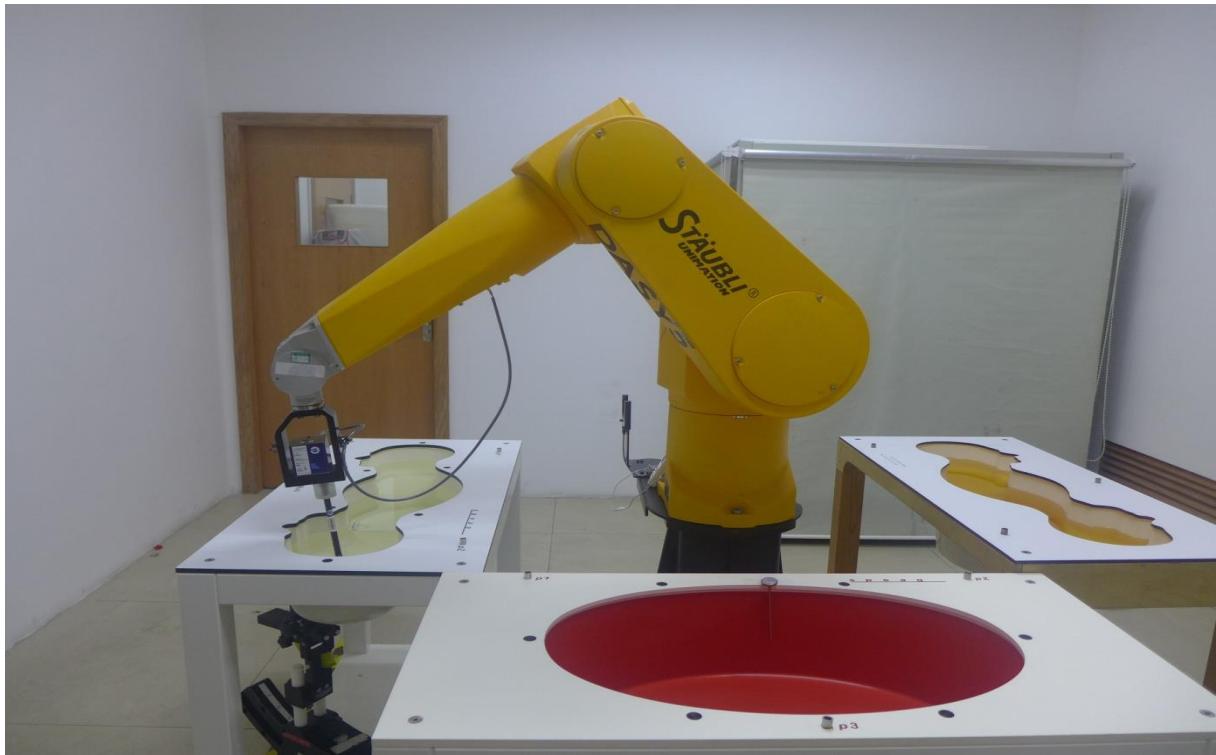


Appendix D

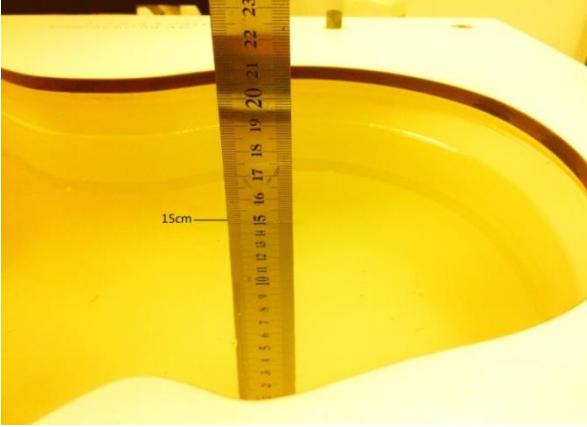
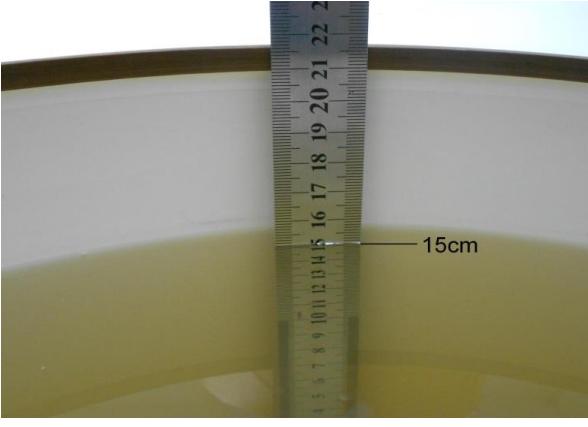
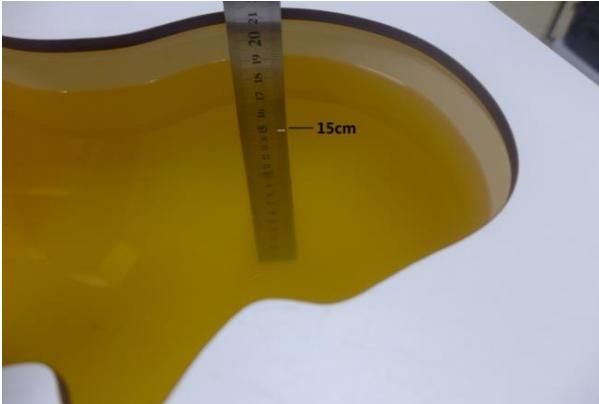
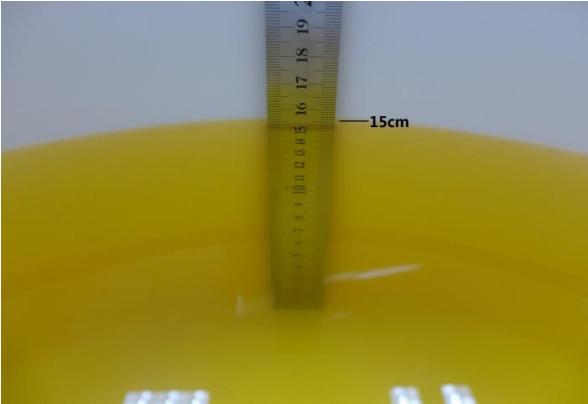
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Body 835
	
Photo 3: Tissue Simulant Liquid for Head 1900	Photo 4: Tissue Simulant Liquid for Body 1900
	

3. Photographs of EUT test position

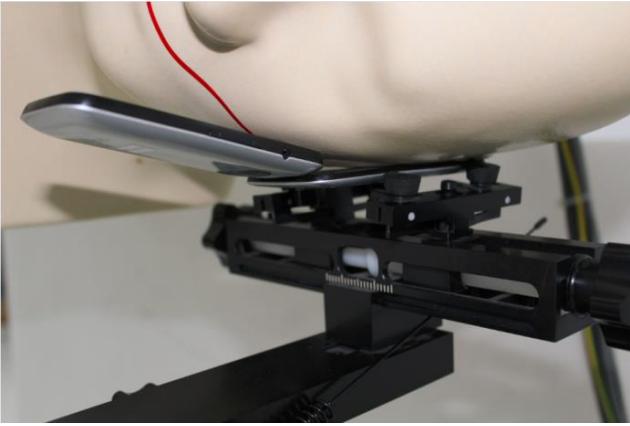
Photo 5: Left touch cheek	Photo 6: Left tilted 15 degree
	
Photo 7: Right touch cheek	Photo 8: Right tilted 15 degree
	
Photo 9: Front side 10mm with cover close	Photo 10: Back side 10mm with cover close
	

Photo 11: Back side 10mm With Cover Open	NA
	NA

4. EUT Constructional Details

Photo 12: Front View	Photo 13: Back View
	
Photo 14: Front View With Cover Open	Photo 15: Back View With Cover Open
	