

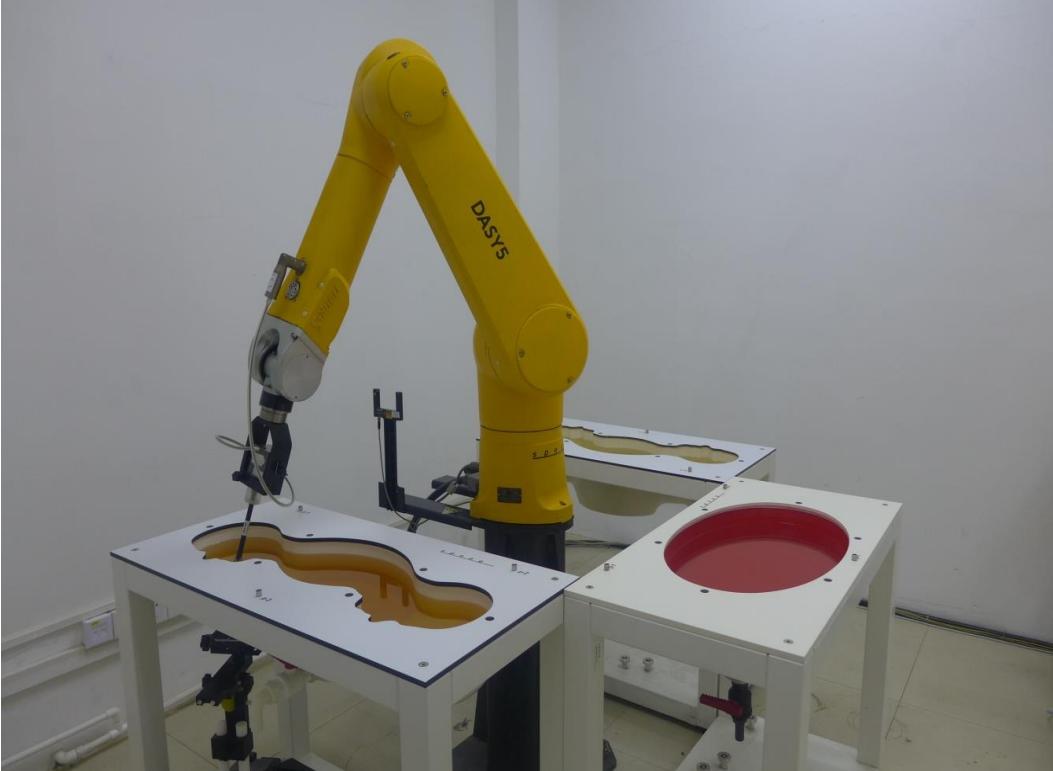
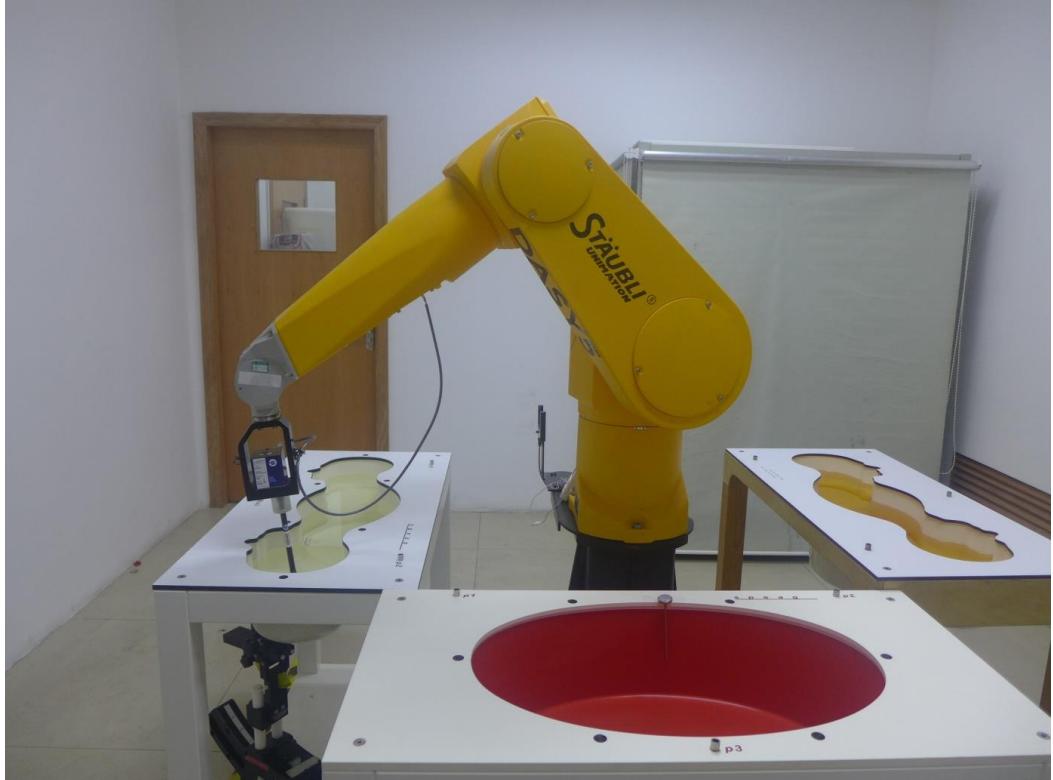


# **Appendix D**

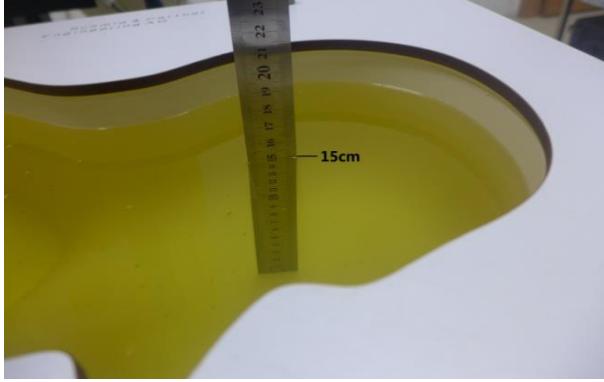
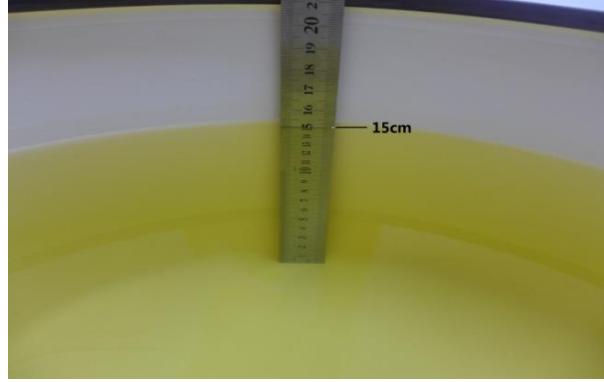
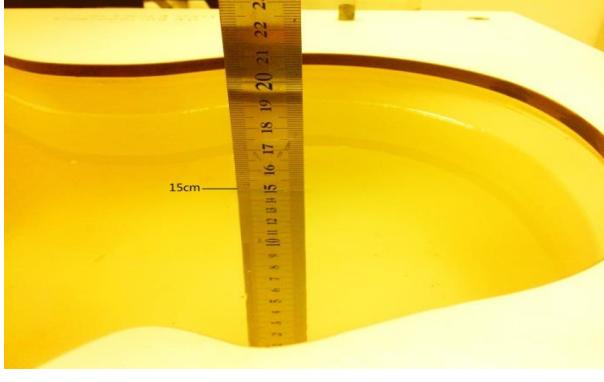
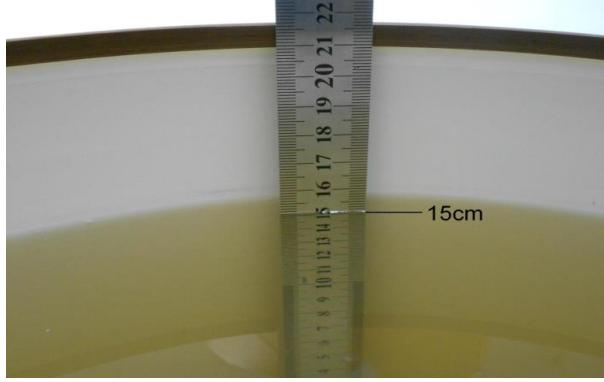
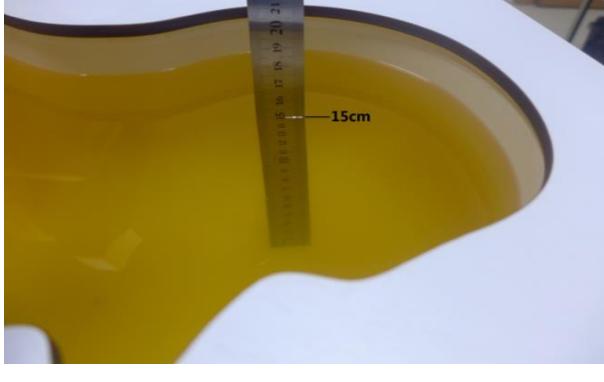
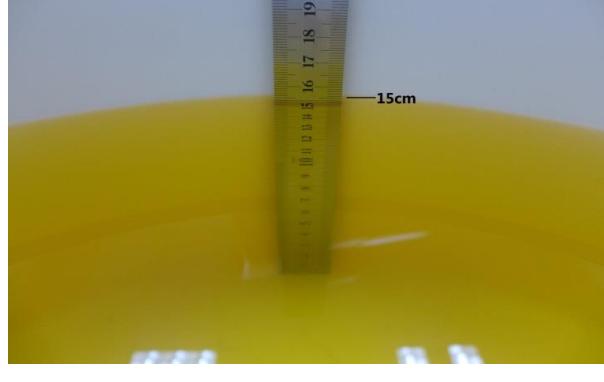
## **Photographs**

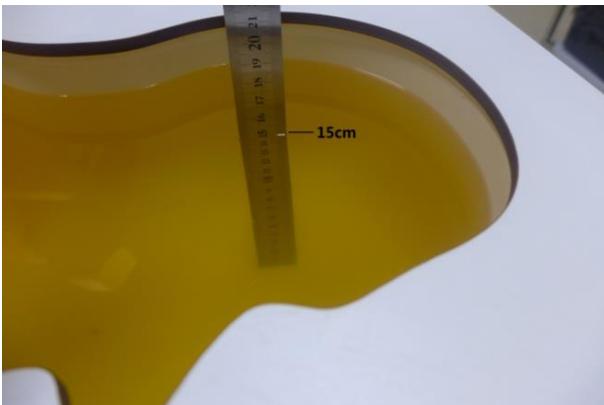
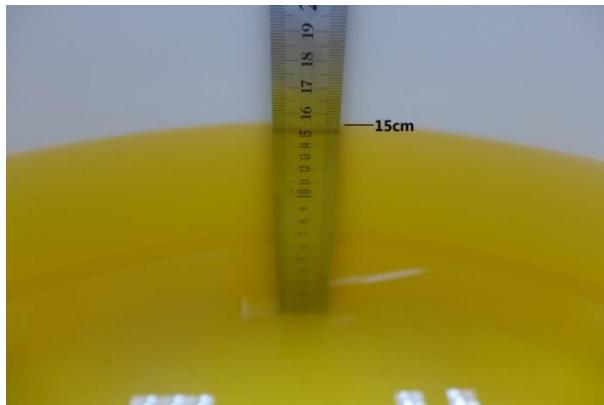
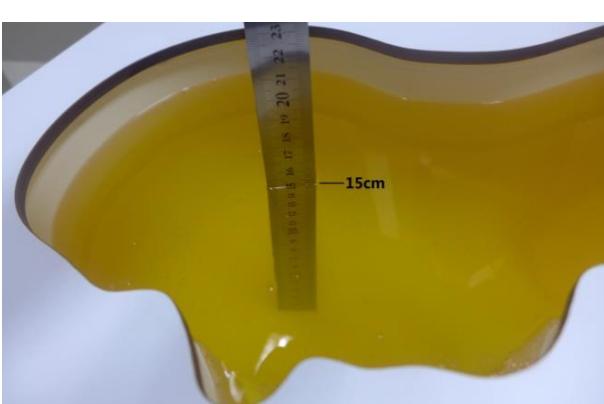
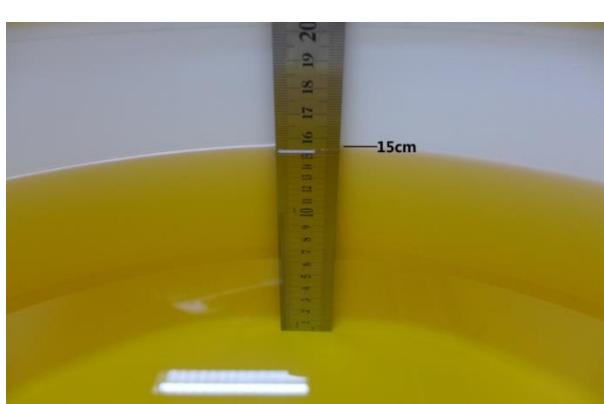
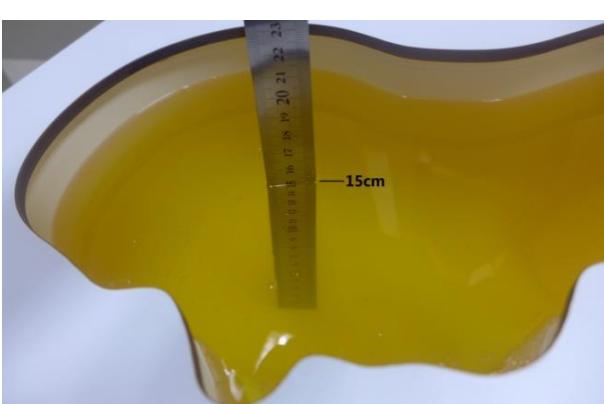
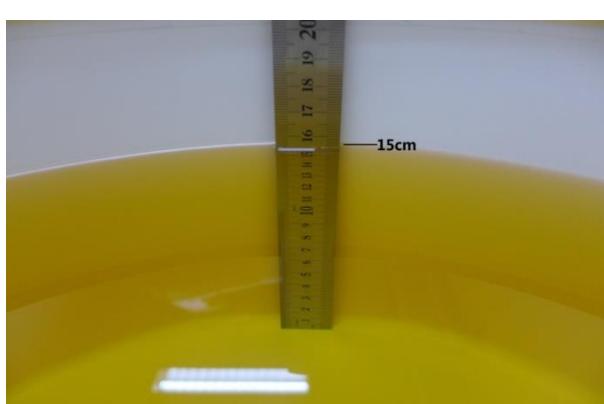
1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details
5. Serial Number of EUT

## 1. SAR measurement System

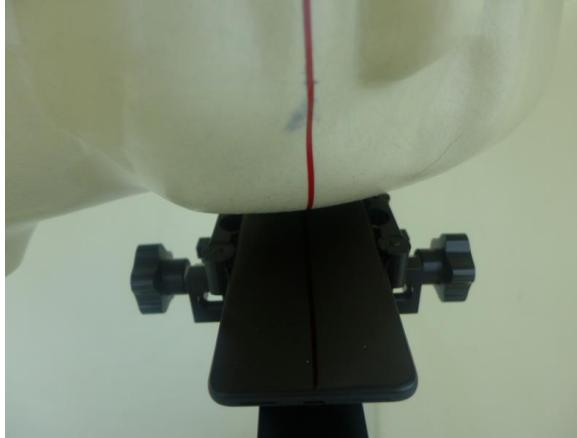
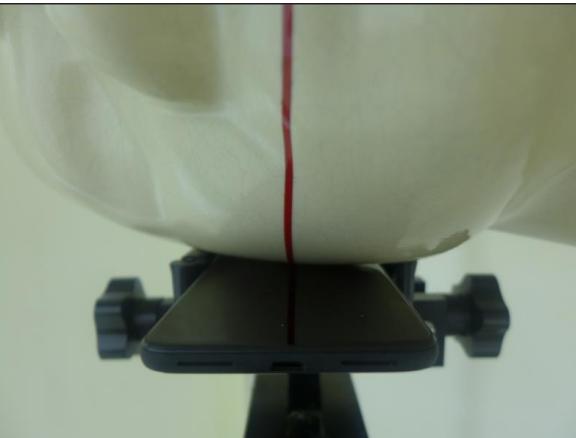
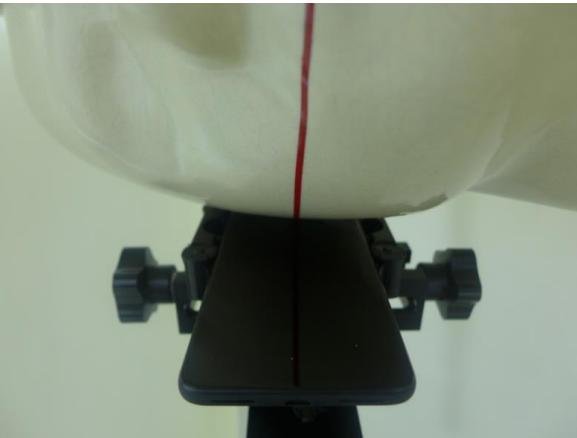


## 2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Body 750
	
Photo 3: Tissue Simulant Liquid for Head 835	Photo 4: Tissue Simulant Liquid for Body 835
	
Photo 5: Tissue Simulant Liquid for Head 1750	Photo 6: Tissue Simulant Liquid for Body 1750
	

<b>Photo 7: Tissue Simulant Liquid for Head 1900</b>	<b>Photo 8: Tissue Simulant Liquid for Body 1900</b>
 A photograph showing a yellow, viscous liquid in a shallow, irregularly shaped container. A metal ruler is placed vertically next to the container, with the '15cm' mark indicated by an arrow.	 A photograph showing a yellow, viscous liquid in a shallow, irregularly shaped container. A metal ruler is placed vertically next to the container, with the '15cm' mark indicated by an arrow.
<b>Photo 9: Tissue Simulant Liquid for Head 2450</b>	<b>Photo 10: Tissue Simulant Liquid for Body 2450</b>
 A photograph showing a yellow, viscous liquid in a shallow, irregularly shaped container. A metal ruler is placed vertically next to the container, with the '15cm' mark indicated by an arrow.	 A photograph showing a yellow, viscous liquid in a shallow, irregularly shaped container. A metal ruler is placed vertically next to the container, with the '15cm' mark indicated by an arrow.
<b>Photo 11: Tissue Simulant Liquid for Head 2600</b>	<b>Photo 12: Tissue Simulant Liquid for Body 2600</b>
 A photograph showing a yellow, viscous liquid in a shallow, irregularly shaped container. A metal ruler is placed vertically next to the container, with the '15cm' mark indicated by an arrow.	 A photograph showing a yellow, viscous liquid in a shallow, irregularly shaped container. A metal ruler is placed vertically next to the container, with the '15cm' mark indicated by an arrow.

**3. Photographs of EUT test position**

<b>Photo 13: Left cheek</b>	<b>Photo 14: Left tilted</b>
	
<b>Photo 15: Right cheek</b>	<b>Photo 16: Right tilted</b>
	
<b>Photo 17: Front side 15mm</b>	<b>Photo 18: Back side 15mm</b>
	

<b>Photo 19: Front side 10mm</b>	<b>Photo 20: Back side 10mm</b>
	
<b>Photo 21: Left side 10mm</b>	<b>Photo 22: Right side 10mm</b>
	
<b>Photo 23: Top side 10mm</b>	<b>Photo 24: Bottom side 10mm</b>
	

**4. EUT Constructional Details**

Photo 25: Front View	Photo 26: Back View
	
Photo 27: Accessory	NA
	NA