




Appendix D







Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

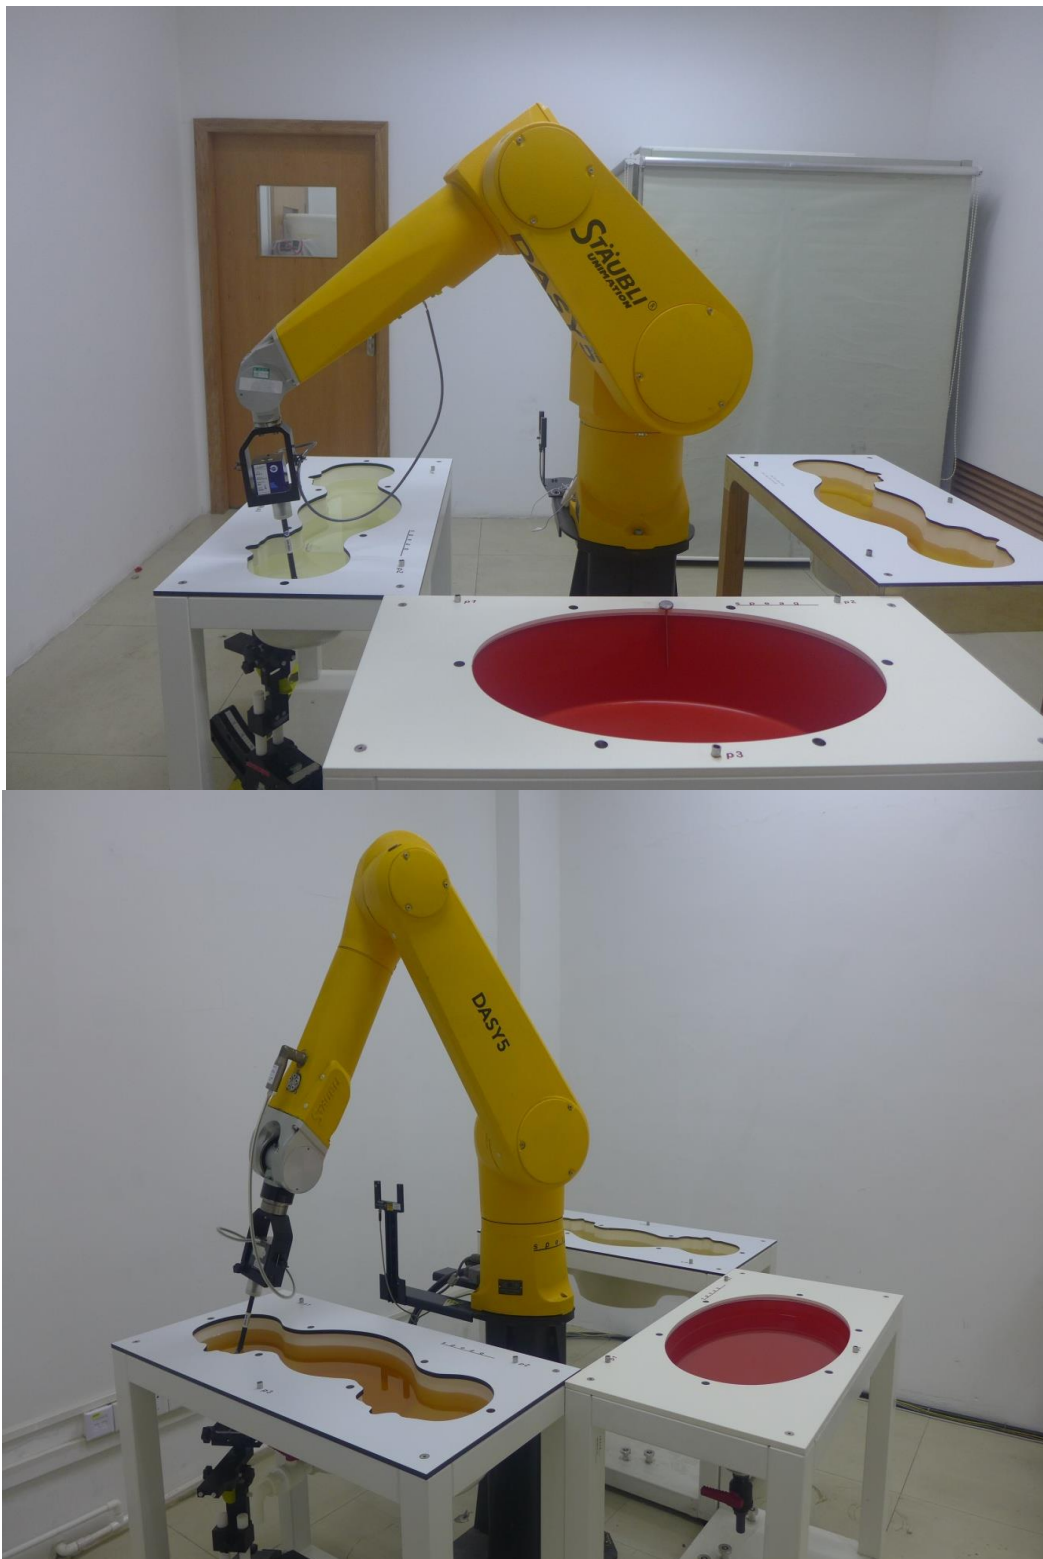

2. Photographs of Tissue Simulate Liquid

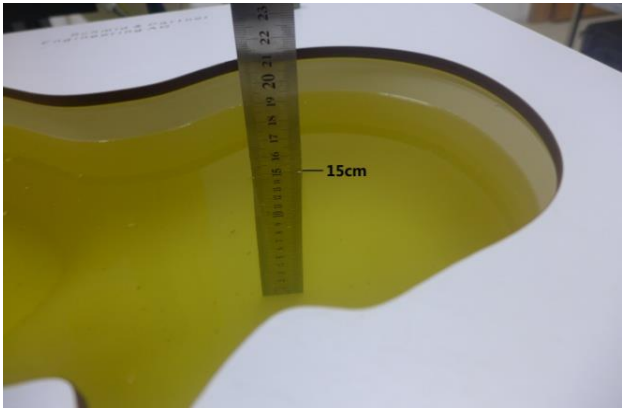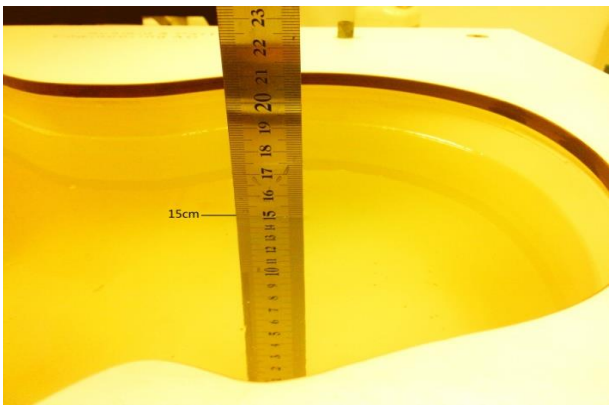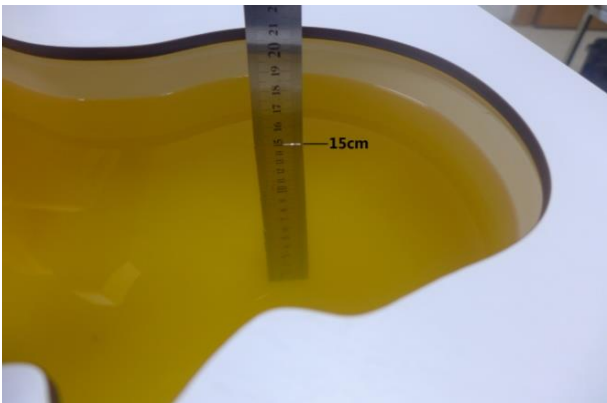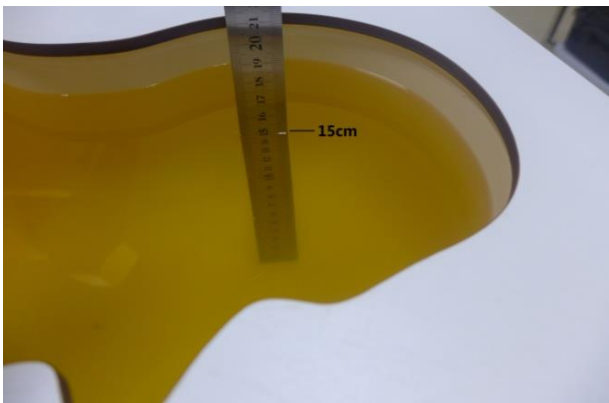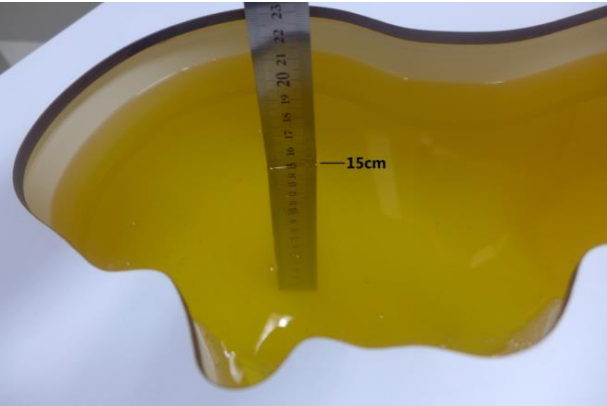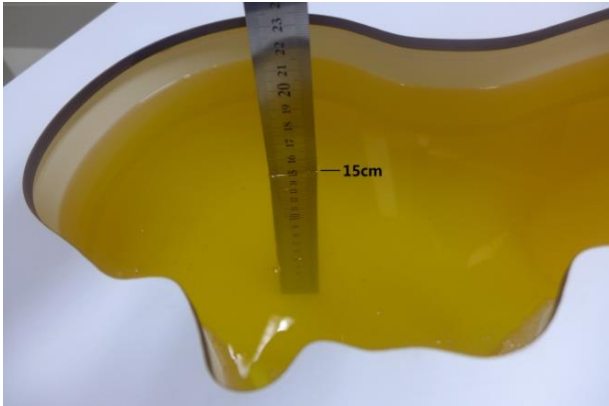Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 2600
	

3. Photographs of EUT test position

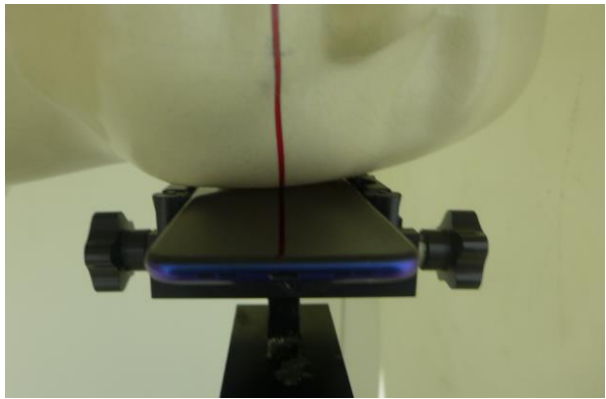
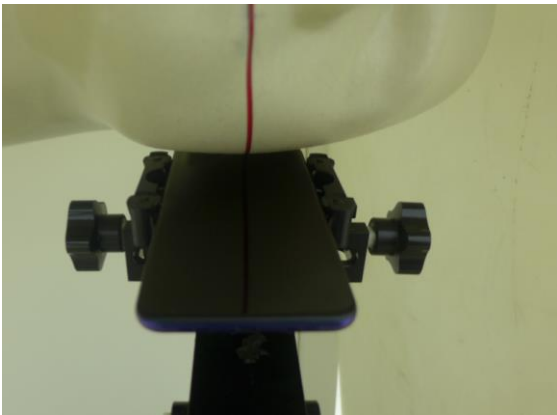
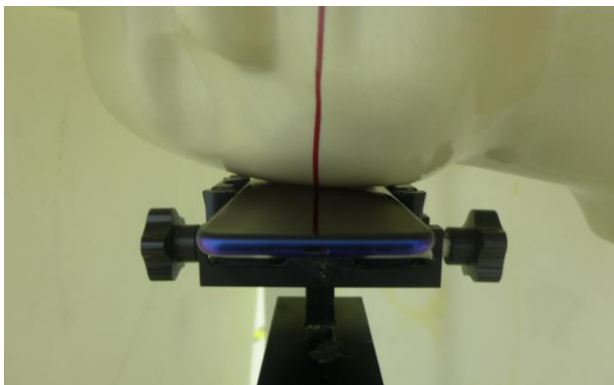
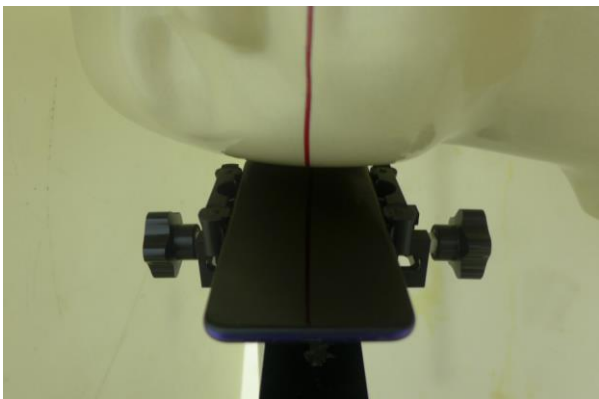
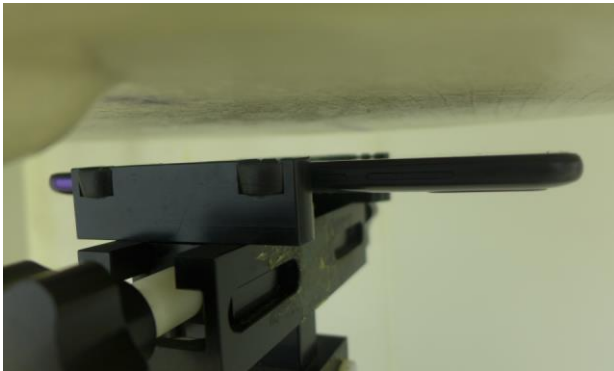
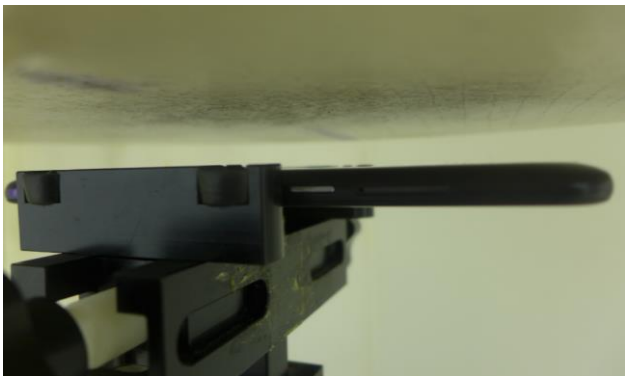
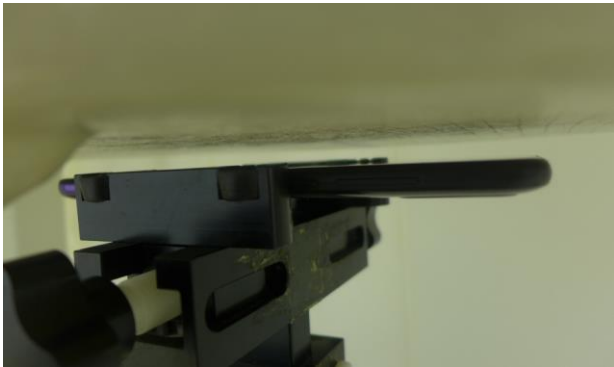
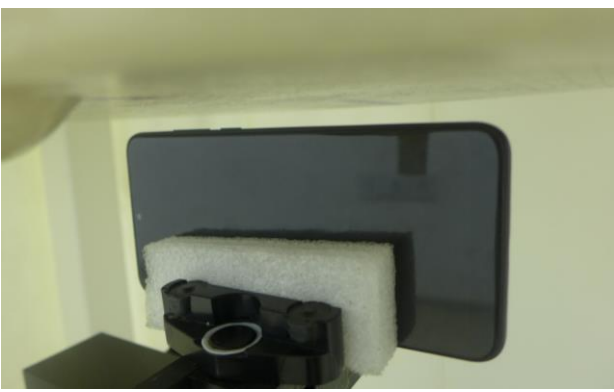
Photo 7: Left cheek	Photo 8: Left tilted
	
Photo 9: Right cheek	Photo 10: Right tilted
	
Photo 11: Front side 15mm	Photo 12: Back side 15mm
	

Photo 13: Front side 10mm	Photo 14: Back side 10mm
	
Photo 15: Left side 10mm	Photo 16: Right side 10mm
	
Photo 17: Top side 10mm	Photo 18: Bottom side 10mm
	

4. EUT Constructional Details

Photo 19: Front View	Photo 20: Back View
 A black smartphone is shown from the front, lying flat on a blue surface. A white ruler is placed vertically to the left of the phone, showing a height of approximately 15 cm. Another white ruler is placed horizontally below the phone, showing a width of approximately 7 cm.	 A blue smartphone is shown from the back, lying flat on a blue surface. A white ruler is placed vertically to the left of the phone, showing a height of approximately 15 cm. Another white ruler is placed horizontally below the phone, showing a width of approximately 7 cm. The back of the phone features a camera lens, a flash, and a circular logo with the text 'COCORAMA' below it.