

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

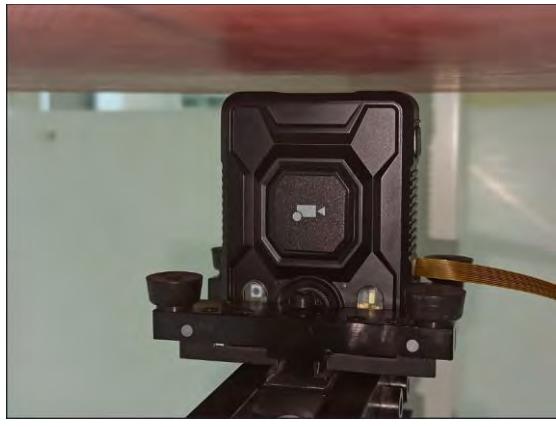


2. Photographs of Tissue Simulate Liquid

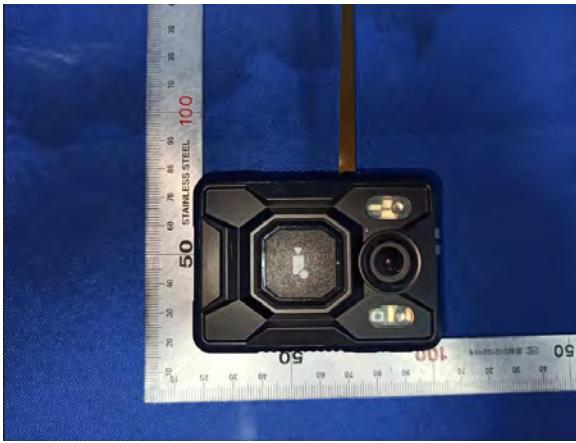
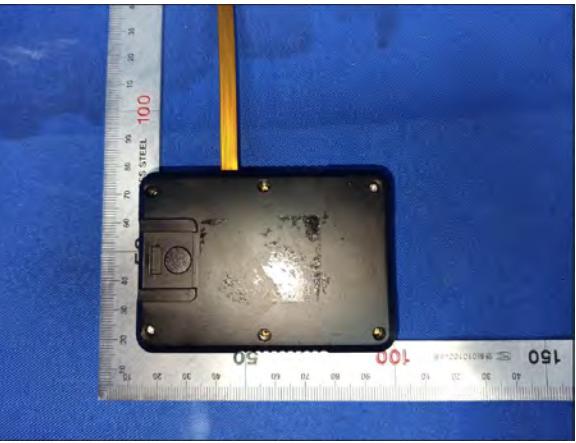
Photo 1: Tissue Simulant Liquid for Body 2450



3. Photographs of EUT test position

Photo 2: Front side 5mm	Photo 3: Back side 5mm
	
Photo 4: Left side 5mm	Photo 5: Right side 5mm
	
Photo 6: Top side 5mm	Photo 7: Bottom side 5mm
	

4. EUT Constructional Details

Photo 8: Front View	Photo 9: Back View
 A photograph showing the front view of the EUT (Equipment Under Test). It is a black rectangular device with a prominent camera lens and a small display or sensor area in the center. It is placed on a blue surface next to a metal ruler for scale. The ruler is marked in centimeters, with '100' clearly visible on the right side.	 A photograph showing the back view of the EUT. The device is a dark, rectangular metal plate with several small circular holes or mounting points. It is positioned on a blue surface next to a metal ruler for scale. The ruler is marked in centimeters, with '100' clearly visible on the right side.