


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

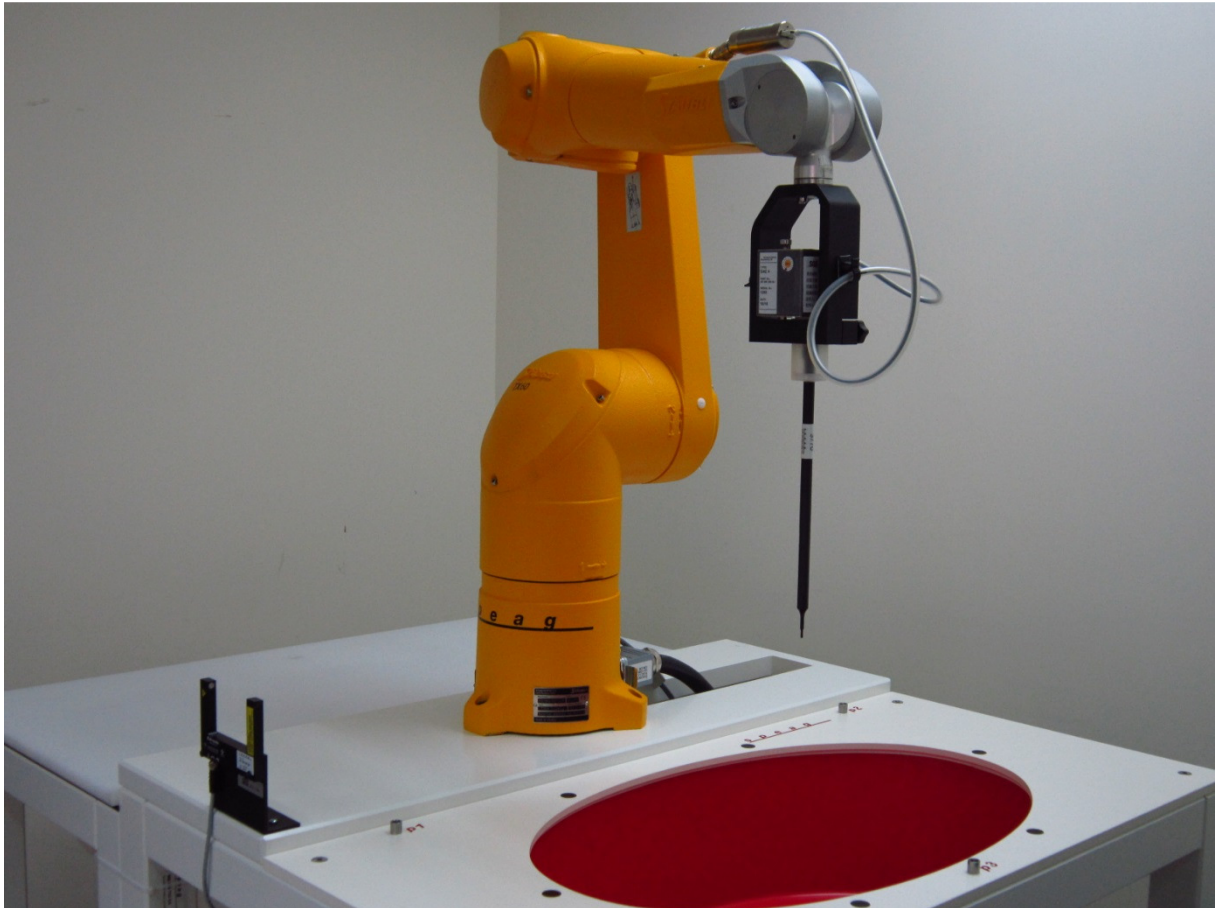

2. Photographs of Tissue Simulate Liquid






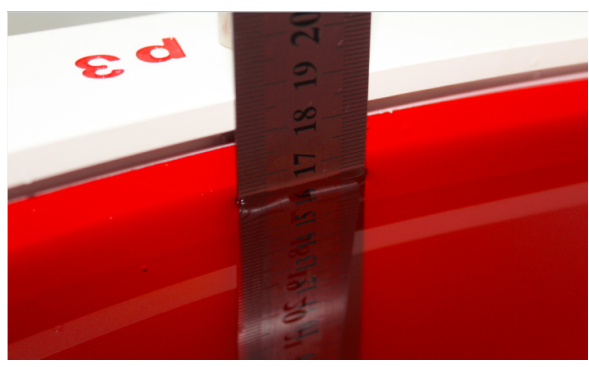
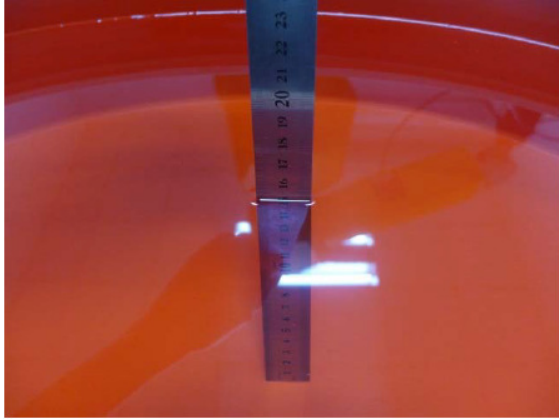
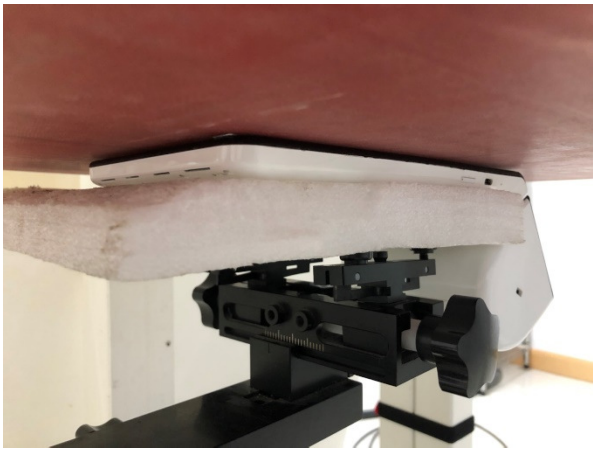
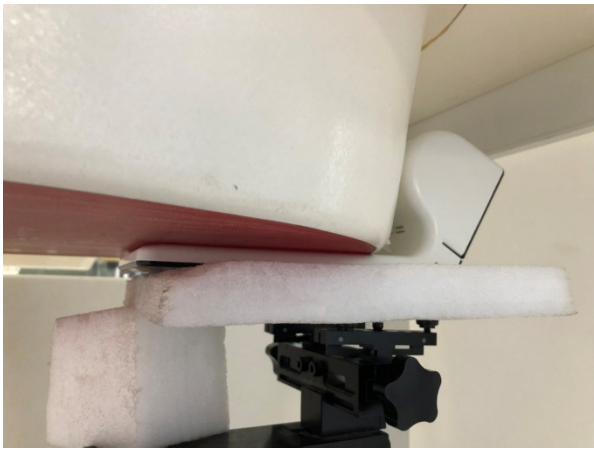
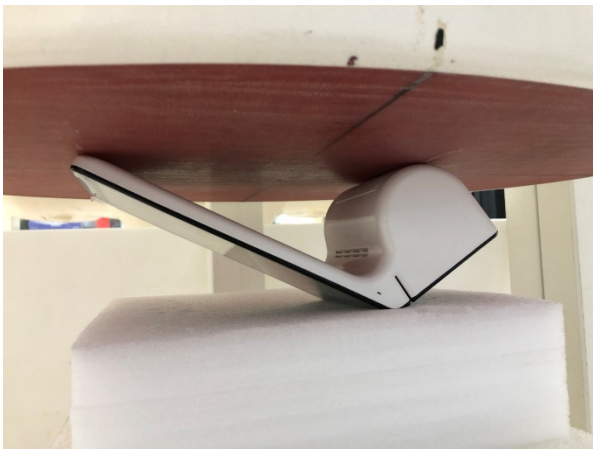



Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1800	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 2600
	

Photo 7: Tissue Simulant Liquid for Head 5GHz



3. Photographs of EUT test position

Photo 8: Front side 0mm	Photo 9: Back side 0mm
	
Photo 10: Back-1 side 0mm	Photo 11: Left side 0mm
	
Photo 12: Right side 0mm	Photo 13: Top side 0mm
	


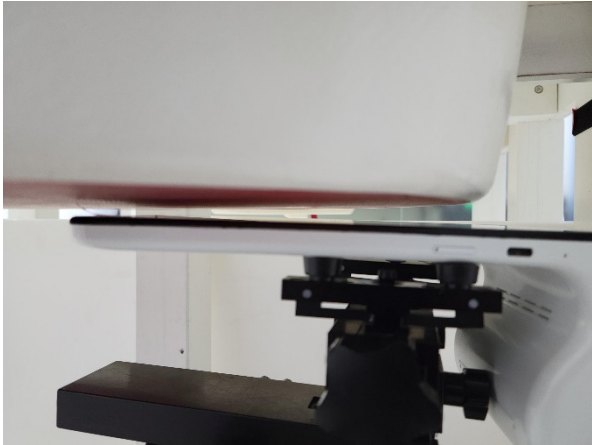



<p>Photo 14: Bottom side 0mm</p>	
	
<p>Photo 15: Front side 10mm</p>	<p>Photo 16: Back side 10mm</p>
	
<p>Photo 17: Back-1 side 10mm</p>	<p>Photo 18: Left side 10mm</p>
	

Photo 19: Right side 10mm



Photo 20: Top side 10mm



Photo 21: Bottom side 10mm



4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.