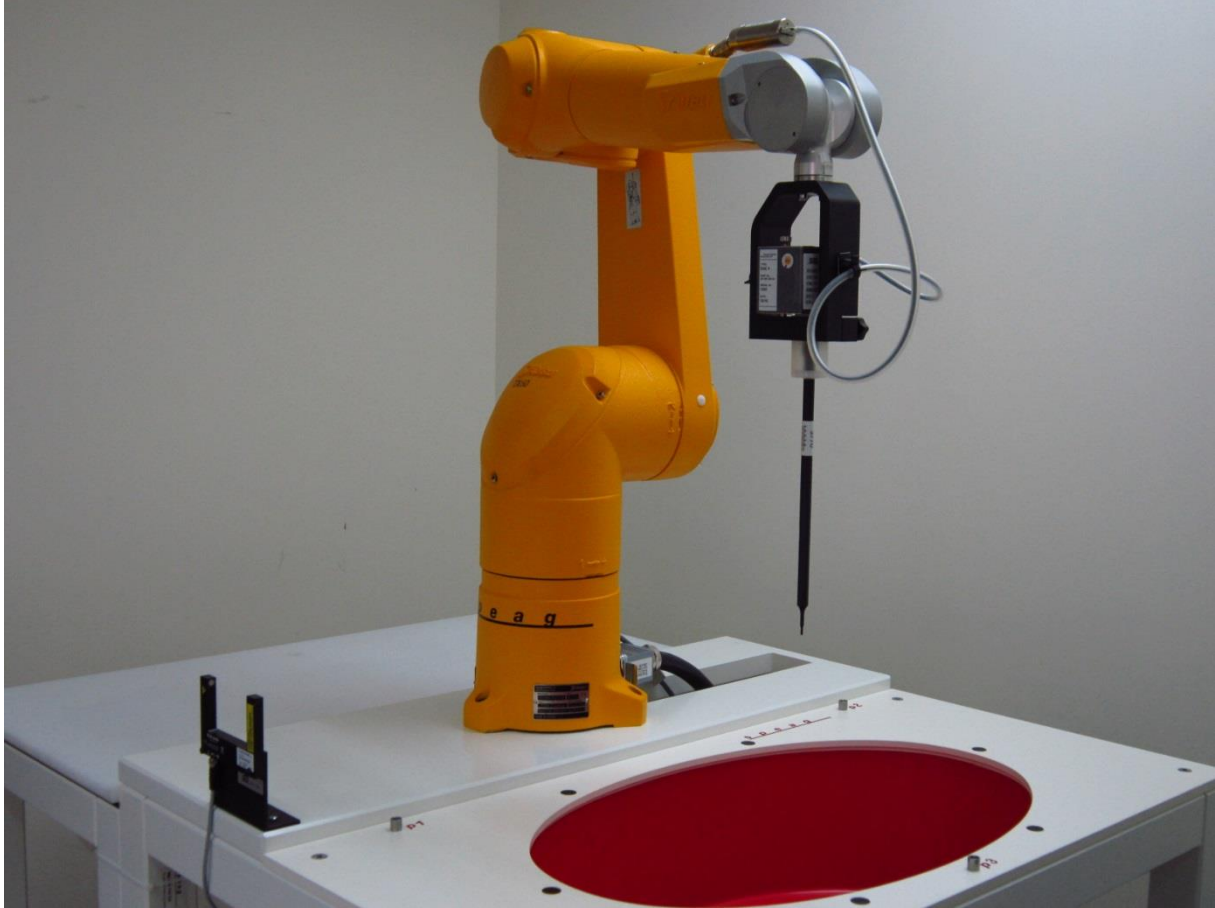


Appendix D

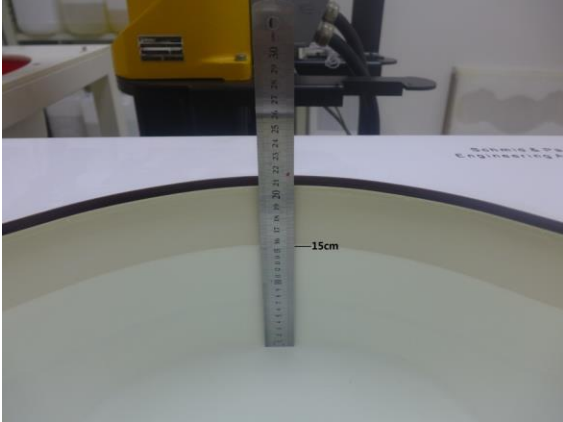

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details





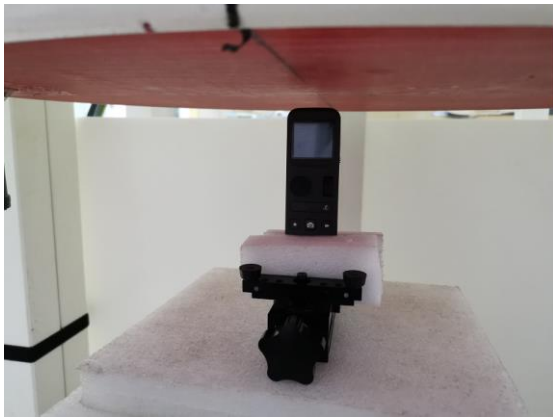

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Body 2450	Photo 2: Tissue Simulant Liquid for Body 5G
	

3. Photographs of EUT test position




<p>Photo 3: Front side 10mm</p>	<p>Photo 4: Back side 10mm_Wifi2</p>
	
<p>Photo 5: Left side 10mm</p>	<p>Photo 6: Right side 10mm</p>
	
<p>Photo 7: Top side 10mm</p>	<p>Photo 8: Bottom side 10mm</p>
	

<p>Photo 9: Back side 10mm_Wifi1</p>	<p>Photo 10: Front side 0mm_Wifi1</p>
	
<p>Photo 11: Back side 0mm_Wifi1</p>	<p>Photo 12: Left side 0mm_Wifi1</p>
	
<p>Photo 13: Right side 0mm_Wifi1</p>	<p>Photo 14: Top side 0mm_Wifi1</p>
	

Photo 15: Bottom side 0mm_Wifi1



4. EUT Constructional Details

Photo 16: Front View	Photo 17: Back View
 A photograph showing the front view of a black mobile phone. The phone is positioned horizontally on a blue background. A white ruler is placed below the phone, showing measurements in centimeters. The phone's screen, camera, and keypad are visible.	 A photograph showing the back view of a black mobile phone. The phone is positioned horizontally on a blue background. A white ruler is placed below the phone, showing measurements in centimeters. The back cover, camera lens, and flash are visible.
Photo 18: Front View with Front Splint	
 A photograph showing the front view of a black mobile phone with a front splint. The phone is positioned horizontally on a blue background. A white ruler is placed below the phone, showing measurements in centimeters. The front splint is visible over the keypad area.	