



# **Appendix D**

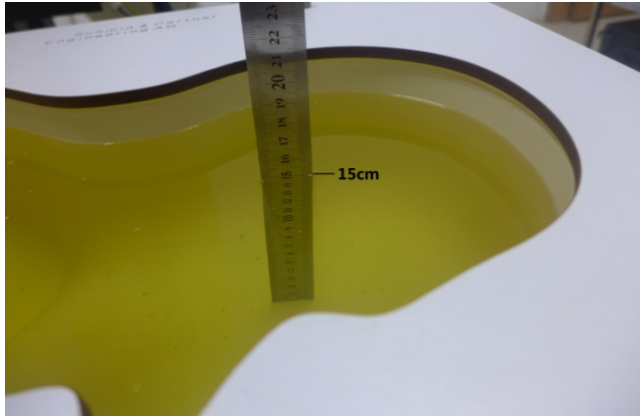
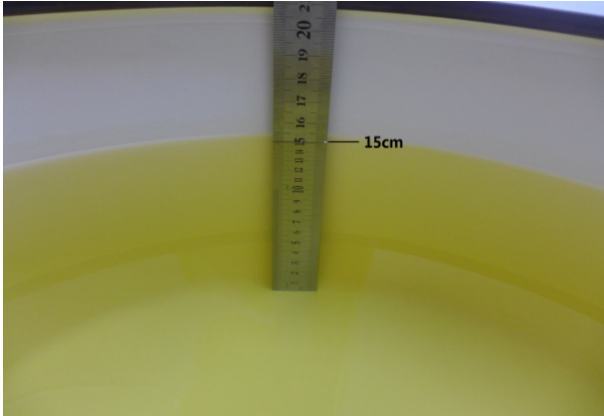
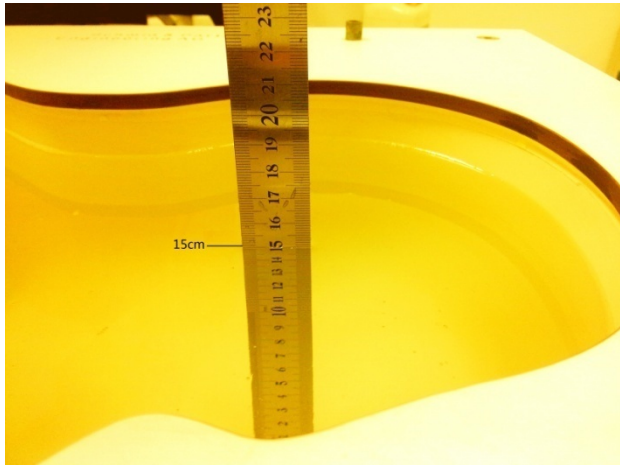
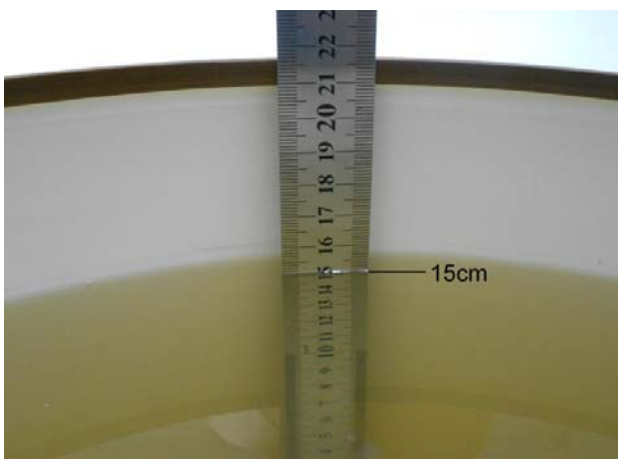
## **Photographs**

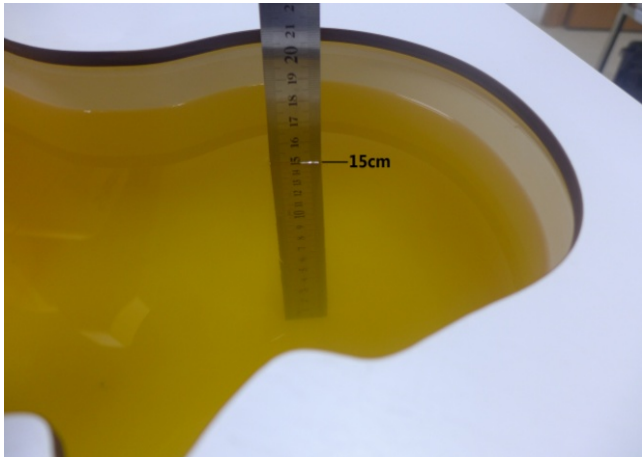
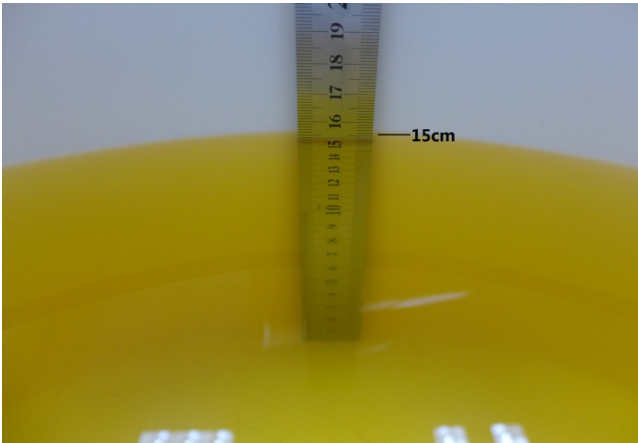
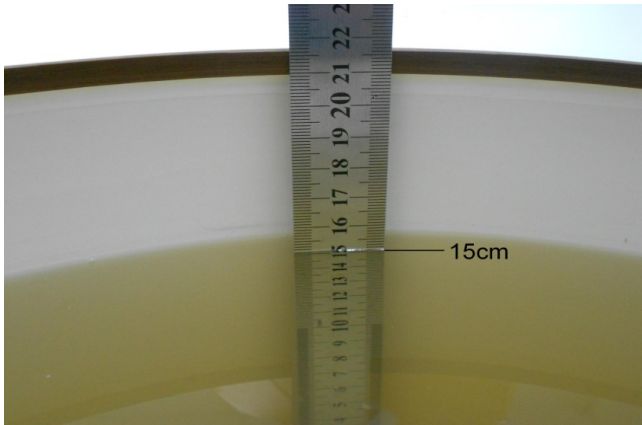
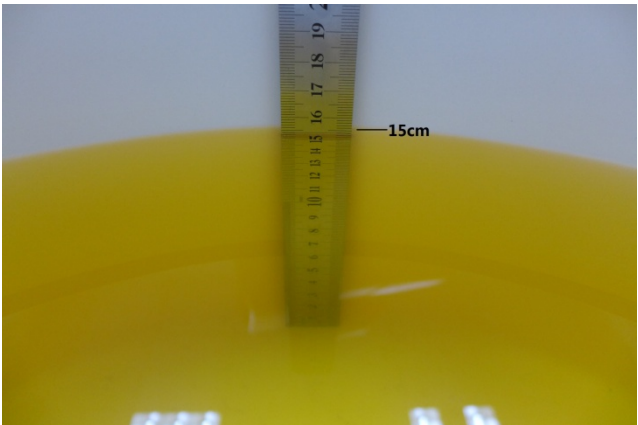
1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System

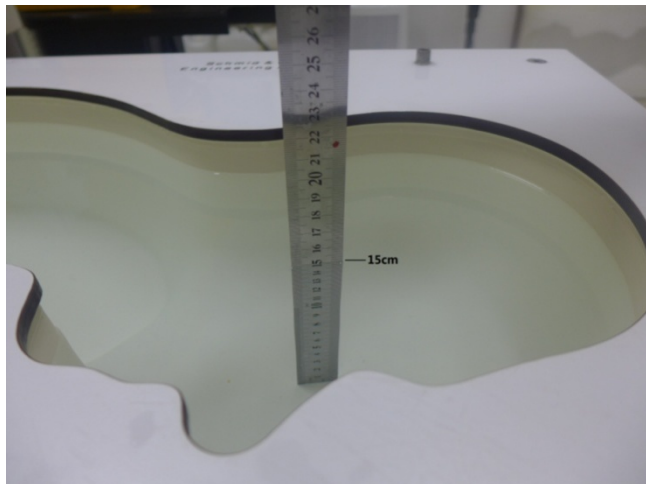


## 2. Photographs of Tissue Simulate Liquid

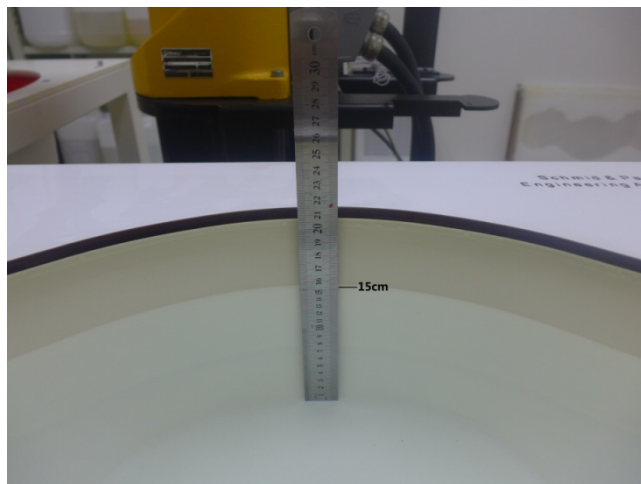
<p><b>Photo 1: Tissue Simulant Liquid for Head 750</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Body 750</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 835</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Body 835</b></p>
	

<p><b>Photo 5: Tissue Simulant Liquid for Head 1750</b></p>	<p><b>Photo 6: Tissue Simulant Liquid for Body 1750</b></p>
	
<p><b>Photo 7: Tissue Simulant Liquid for Head 1900</b></p>	<p><b>Photo 8: Tissue Simulant Liquid for Body 1900</b></p>
	

**Photo 9: Tissue Simulant Liquid for Head 5G**

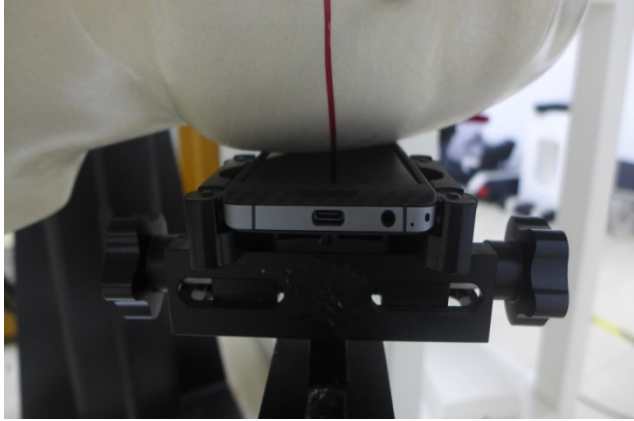
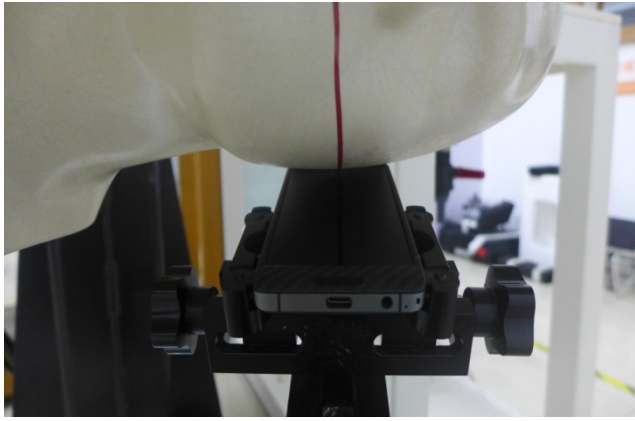
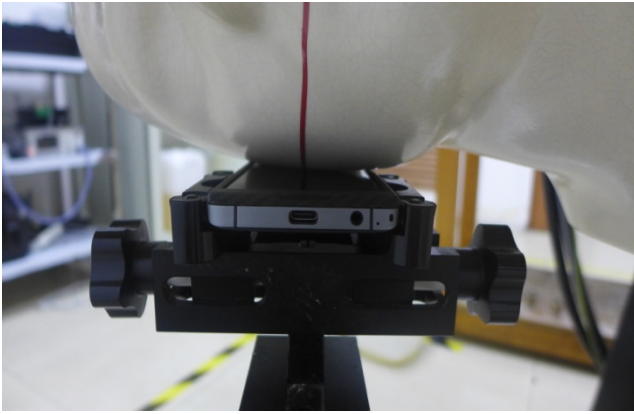
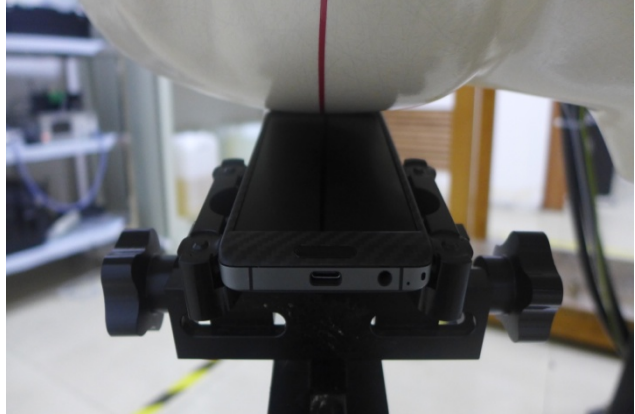




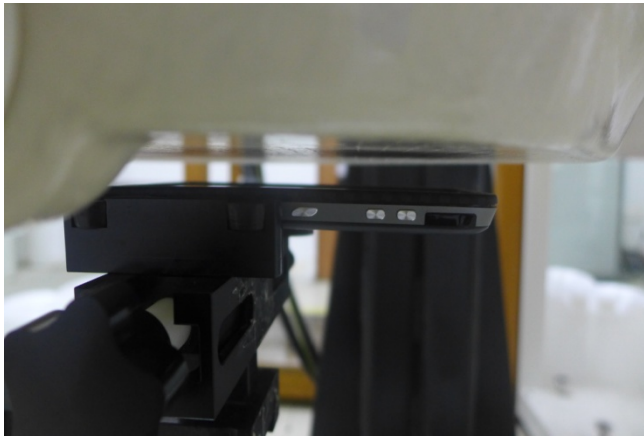
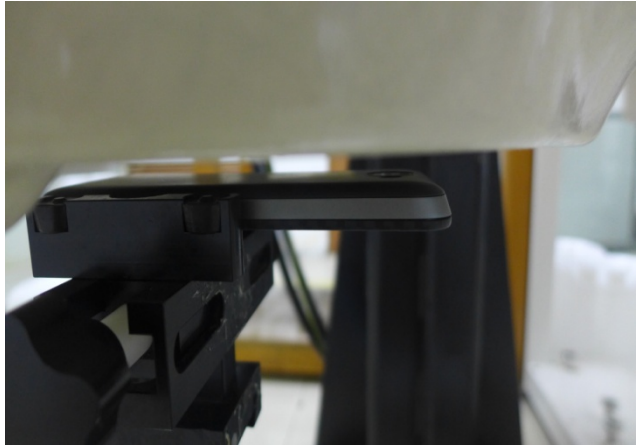
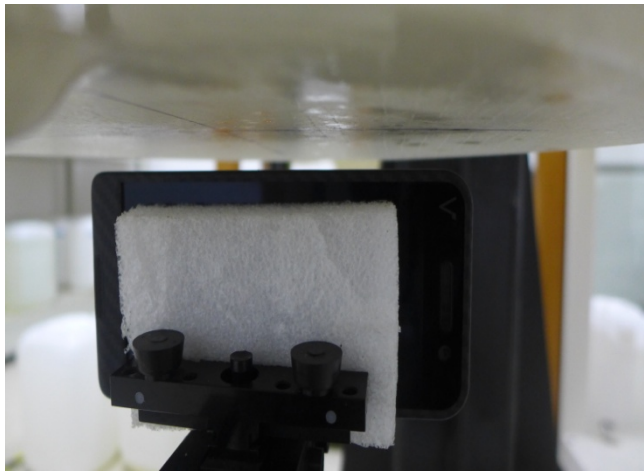
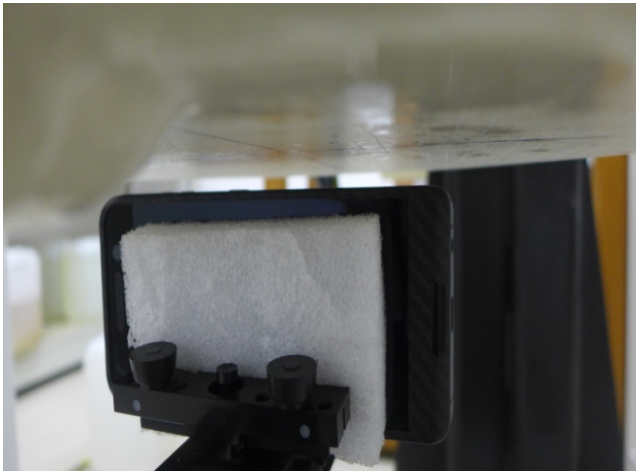
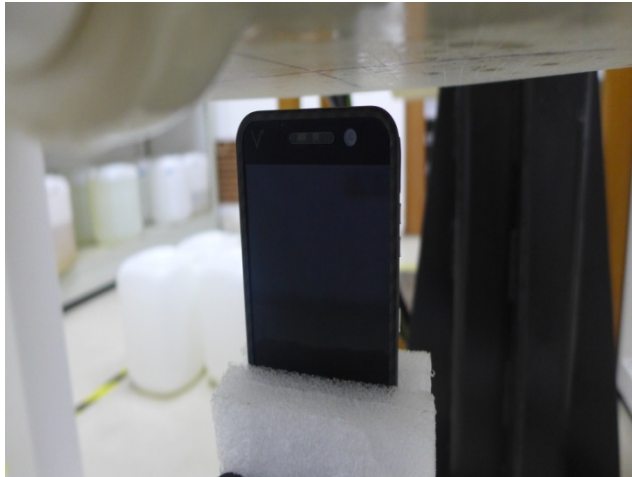
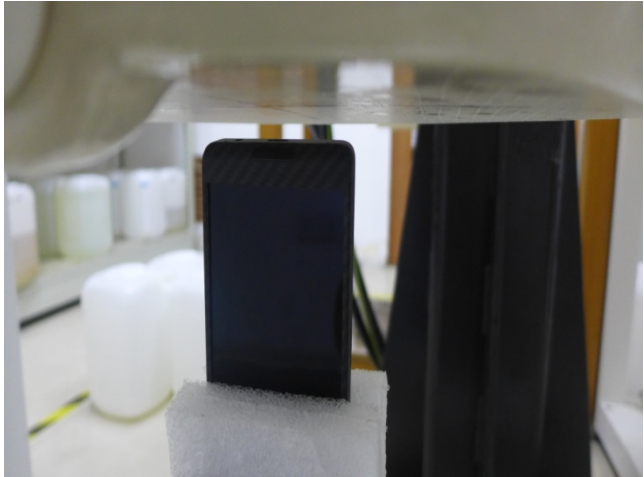
**Photo 10: Tissue Simulant Liquid for Body 5G**







### 3. Photographs of EUT test position

<p>Photo 11: Left touch cheek</p> 	<p>Photo 12: Left tilted 15 degree</p> 
<p>Photo 13: Right touch cheek</p> 	<p>Photo 14: Right tilted 15 degree</p> 
<p>Photo 15: Front side 15mm</p> 	<p>Photo 16: Back side 15mm</p> 

<p><b>Photo 17: Front side 10mm</b></p> 	<p><b>Photo 18: Back side 10mm</b></p> 
<p><b>Photo 19: Left side 10mm</b></p> 	<p><b>Photo 20: Right side 10mm</b></p> 
<p><b>Photo 21: Top side 10mm</b></p> 	<p><b>Photo 22: Bottom side 10mm</b></p> 

## 4. EUT Constructional Details

Photo 23: Front View	Photo 24: Back View
	
Photo 25: Accessory	N/A
	<p>N/A</p>