Report No.: SZEM171001110307

Appendix D

Photographs

- 1. SAR measurement System
- 2. Photographs of Tissue Simulate Liquid
- 3. Photographs of EUT test position
- 4. EUT Constructional Details



Report No.: SZEM171001110307

1. SAR measurement System









Report No.: SZEM171001110307


2. Photographs of Tissue Simulate Liquid

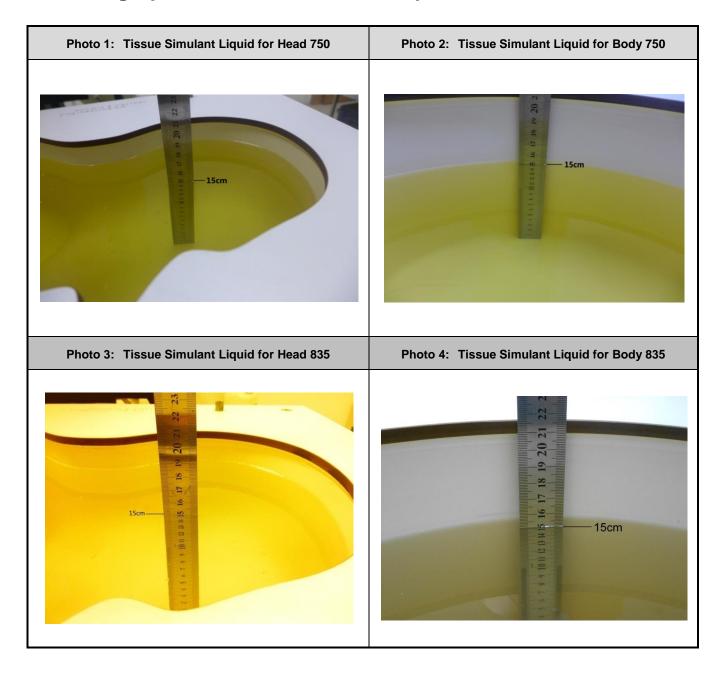




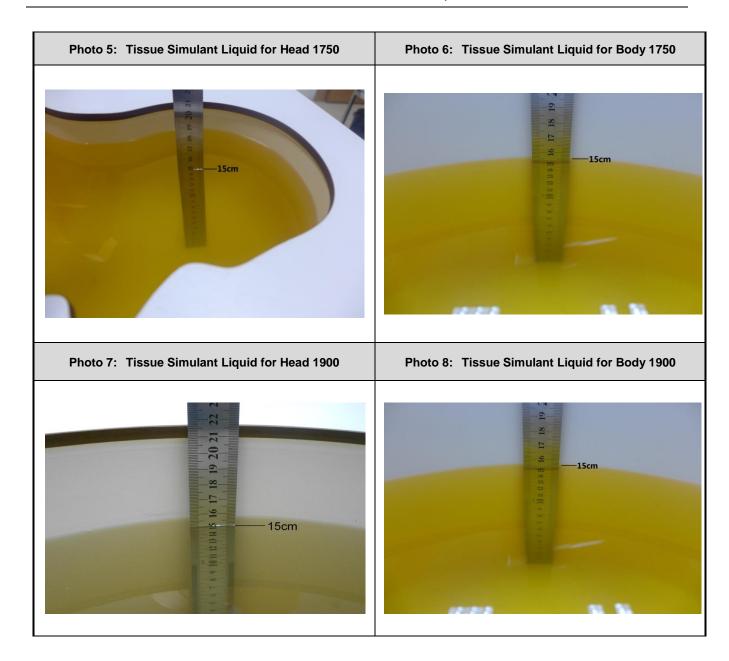



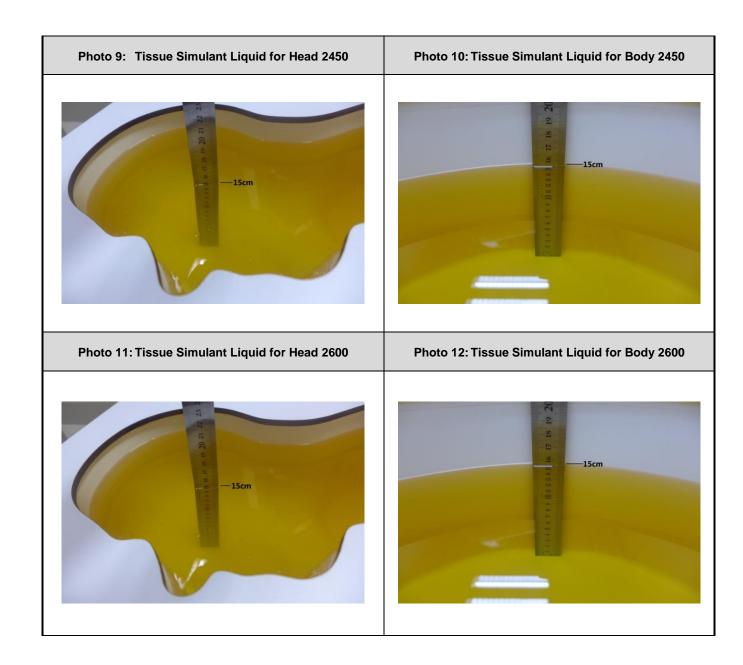



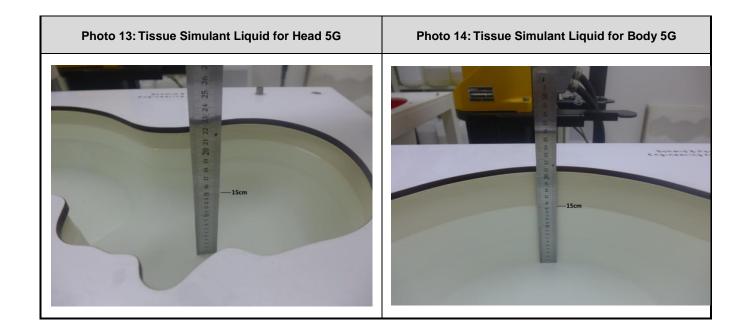



Report No.: SZEM171001110307

3. Photographs of EUT test position

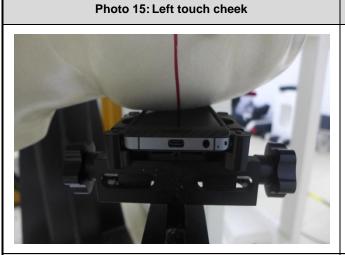


Photo 16: Left tilted 15 degree

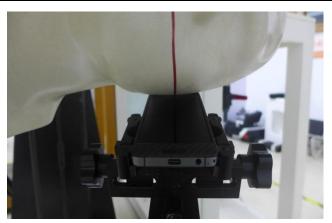


Photo 17: Right touch cheek

Photo 18: Right tilted 15 degree

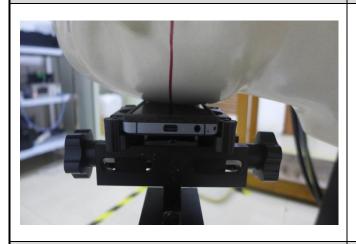


Photo 19: Front side 15mm

Photo 20: Back side 15mm







Report No.: SZEM171001110307

Photo 22: Back side 10mm

Photo 21: Front side 10mm



Photo 23: Left side 10mm



Photo 24: Right side 10mm

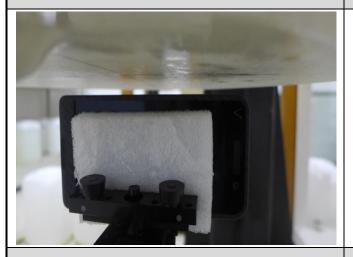


Photo 25: Top side 10mm



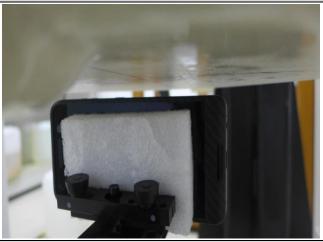


Photo 26: Bottom side 10mm



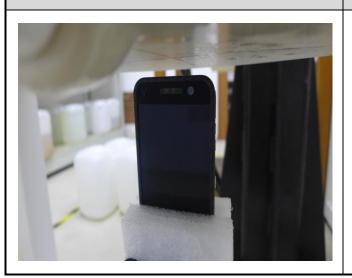

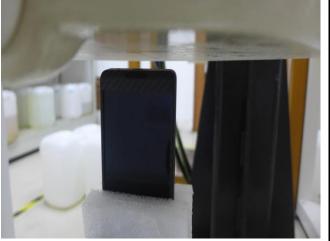

Report No.: SZEM171001110307

4. EUT Constructional Details

Photo 27: Front View	Photo 28: Back View
En 2 3 4 5 6 7 3 9 10 11 12 13 14 15 16 17 18	C 1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17
Photo 29: Accessory	N/A
THE	N/A