


Minimum Emission Bandwidth 6 dB (5180 MHz; 0 (0 dBm); 20 MHz)

6 dB Bandwidth

DUT Frequency (MHz)	Bandwidth (MHz)	Limit Min (MHz)	Limit Max (MHz)	Band Edge Left (MHz)	Band Edge Right (MHz)	Max Level (dBm)
5180.000000	16.658354	---	---	5171.620948	5188.279302	-2.7

(continuation of the "6 dB Bandwidth" table from column 7 ...)

DUT Frequency (MHz)	Result
5180.000000	PASS

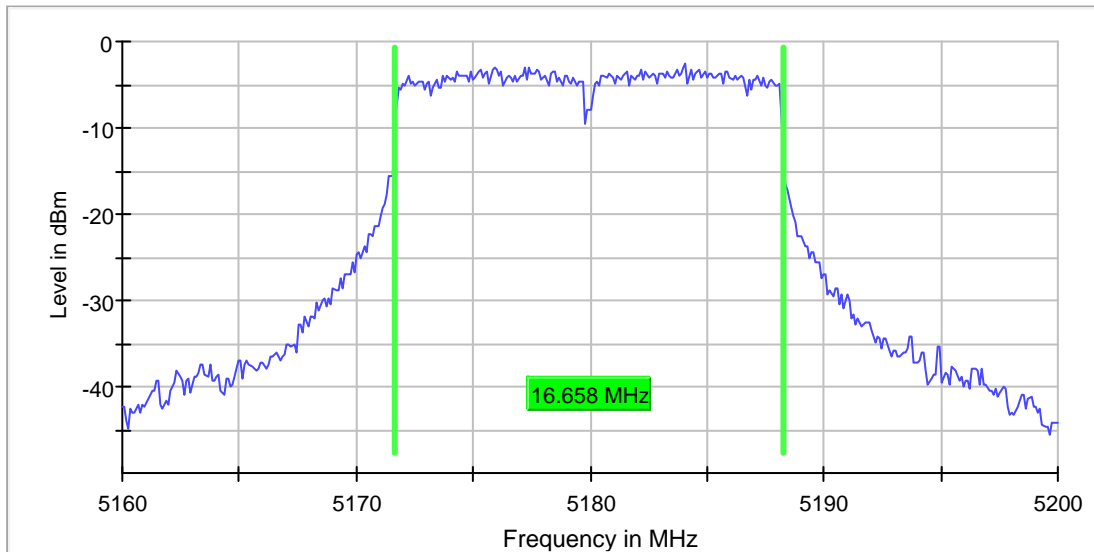

Measurement

Setting	Instrument Value	Target Value
Start Frequency	5.16000 GHz	5.16000 GHz
Stop Frequency	5.20000 GHz	5.20000 GHz
Span	40.000 MHz	40.000 MHz
RBW	100.000 kHz	~ 100.000 kHz
VBW	300.000 kHz	~ 300.000 kHz
SweepPoints	400	~ 400
Sweeptime	56.886 μ s	AUTO
Reference Level	-10.000 dBm	-10.000 dBm
Attenuation	10.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	200	200
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
Sweeptype	FFT	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.30 dB	0.30 dB
Run	11 / max. 150	max. 150
Stable	5 / 5	5
Max Stable Difference	0.21 dB	0.30 dB


Minimum Emission Bandwidth 6 dB (5220 MHz; 0 (0 dBm); 20 MHz)

6 dB Bandwidth

DUT Frequency (MHz)	Bandwidth (MHz)	Limit Min (MHz)	Limit Max (MHz)	Band Edge Left (MHz)	Band Edge Right (MHz)	Max Level (dBm)
5220.000000	16.658354	---	---	5211.620948	5228.279302	-2.5

(continuation of the "6 dB Bandwidth" table from column 7 ...)

DUT Frequency (MHz)	Result
5220.000000	PASS

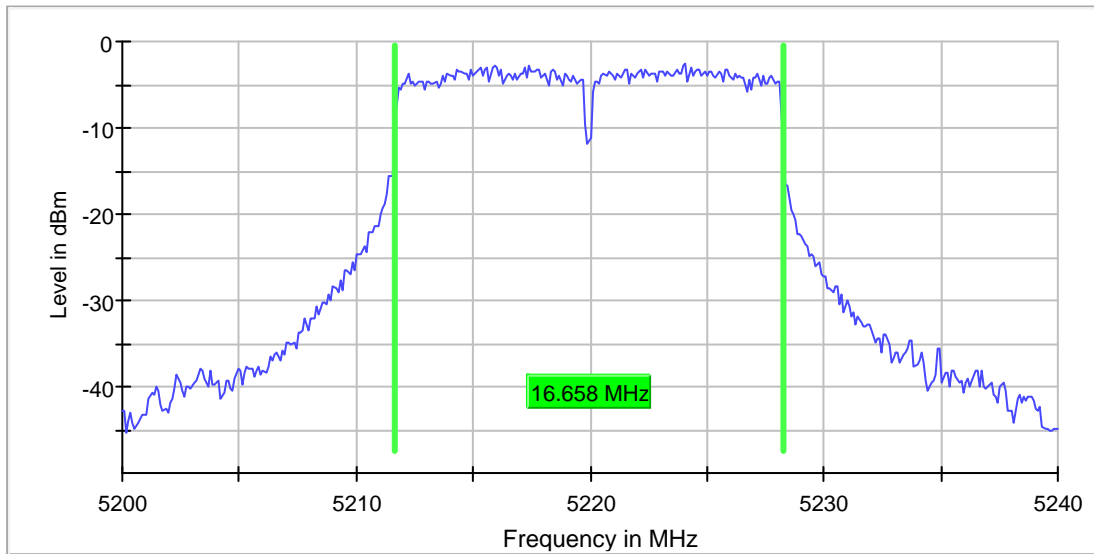

Measurement

Setting	Instrument Value	Target Value
Start Frequency	5.20000 GHz	5.20000 GHz
Stop Frequency	5.24000 GHz	5.24000 GHz
Span	40.000 MHz	40.000 MHz
RBW	100.000 kHz	~ 100.000 kHz
VBW	300.000 kHz	~ 300.000 kHz
SweepPoints	400	~ 400
Sweeptime	56.886 μ s	AUTO
Reference Level	-10.000 dBm	-10.000 dBm
Attenuation	10.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	200	200
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
Sweeptype	FFT	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.30 dB	0.30 dB
Run	12 / max. 150	max. 150
Stable	5 / 5	5
Max Stable Difference	0.03 dB	0.30 dB


Minimum Emission Bandwidth 6 dB (5240 MHz; 0 (0 dBm); 20 MHz)

6 dB Bandwidth

DUT Frequency (MHz)	Bandwidth (MHz)	Limit Min (MHz)	Limit Max (MHz)	Band Edge Left (MHz)	Band Edge Right (MHz)	Max Level (dBm)
5240.000000	16.658354	---	---	5231.620948	5248.279302	-2.3

(continuation of the "6 dB Bandwidth" table from column 7 ...)

DUT Frequency (MHz)	Result
5240.000000	PASS

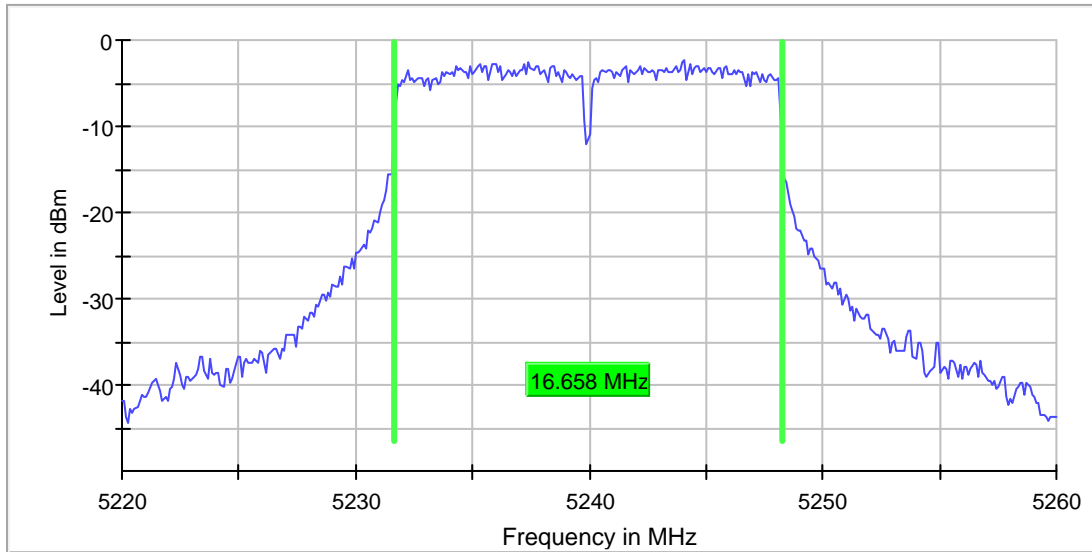

Measurement

Setting	Instrument Value	Target Value
Start Frequency	5.22000 GHz	5.22000 GHz
Stop Frequency	5.26000 GHz	5.26000 GHz
Span	40.000 MHz	40.000 MHz
RBW	100.000 kHz	~ 100.000 kHz
VBW	300.000 kHz	~ 300.000 kHz
SweepPoints	400	~ 400
Sweeptime	56.886 μ s	AUTO
Reference Level	-10.000 dBm	-10.000 dBm
Attenuation	10.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	200	200
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	FFT	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.30 dB	0.30 dB
Run	16 / max. 150	max. 150
Stable	5 / 5	5
Max Stable Difference	0.08 dB	0.30 dB


Power Spectral Density (5180 MHz; 0 (0 dBm); 20 MHz)

Result

DUT Frequency (MHz)	Frequency (MHz)	PSD (dBm)	Limit Max (dBm)	Result
5180.000000	5184.019608	-0.050	17.0	PASS

Ports

Port	Duty Cycle (%)
1	100.000

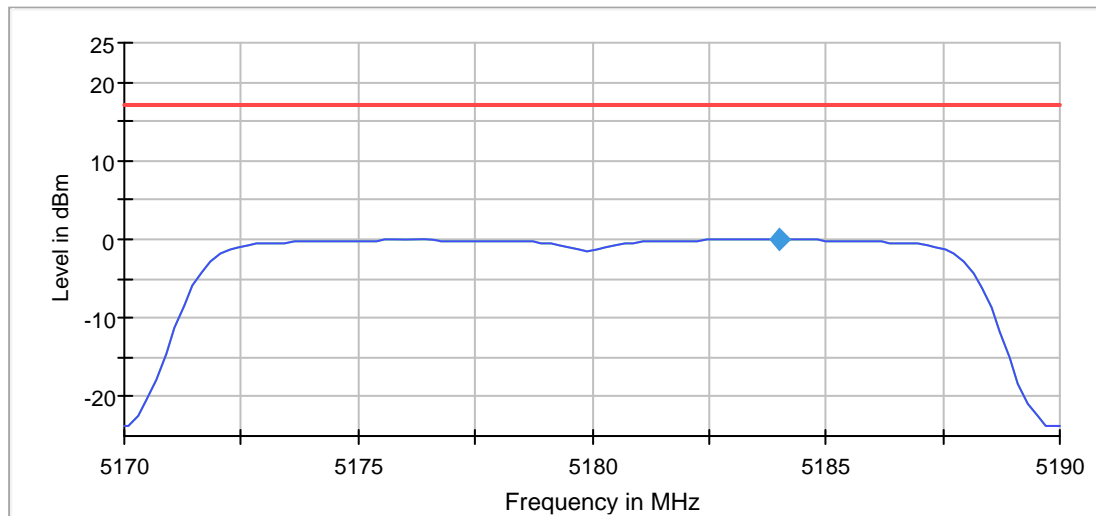

— Connector 1 — Sum Level — Limit ◆ PSD

Measurement

Setting	Instrument Value	Target Value
Start Frequency	5.17000 GHz	5.17000 GHz
Stop Frequency	5.19000 GHz	5.19000 GHz
Span	20.000 MHz	20.000 MHz
RBW	1.000 MHz	<= 1.000 MHz
VBW	3.000 MHz	>= 3.000 MHz
SweepPoints	101	~ 40
SweepTime	2.020 s	2.020 s
Reference Level	0.000 dBm	0.000 dBm
Attenuation	20.000 dB	AUTO
Detector	RMS	RMS
SweepCount	3	3
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.30 dB	0.30 dB
Run	3 / max. 3	max. 3
Stable	2 / 3	3
Max Stable Difference	0.00 dB	0.30 dB


Power Spectral Density (5220 MHz; 0 (0 dBm); 20 MHz)

Result

DUT Frequency (MHz)	Frequency (MHz)	PSD (dBm)	Limit Max (dBm)	Result
5220.000000	5224.019608	0.031	17.0	PASS

Ports

Port	Duty Cycle (%)
1	100.000

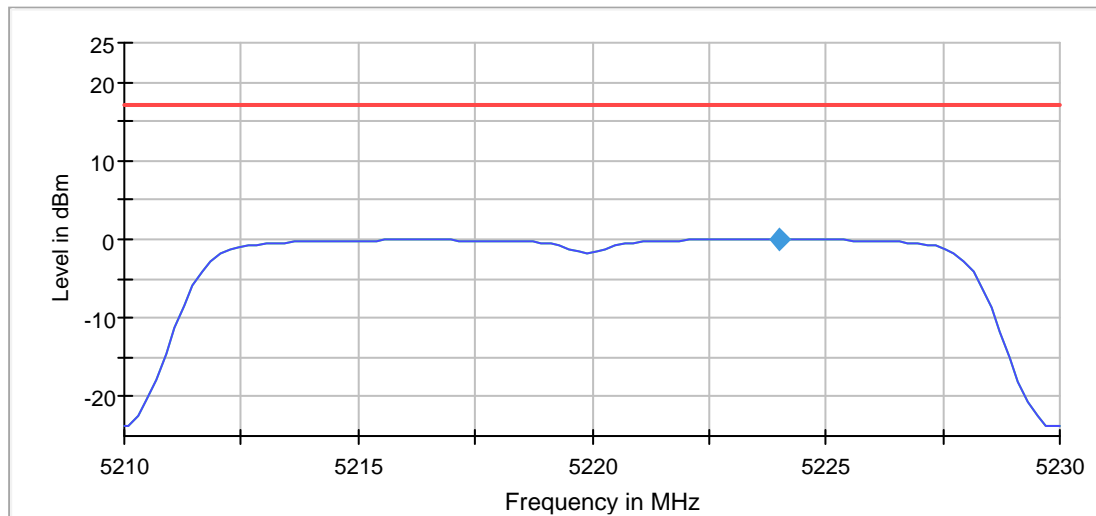

— Connector 1 — Sum Level — Limit ◆ PSD

Measurement

Setting	Instrument Value	Target Value
Start Frequency	5.21000 GHz	5.21000 GHz
Stop Frequency	5.23000 GHz	5.23000 GHz
Span	20.000 MHz	20.000 MHz
RBW	1.000 MHz	<= 1.000 MHz
VBW	3.000 MHz	>= 3.000 MHz
SweepPoints	101	~ 40
SweepTime	2.020 s	2.020 s
Reference Level	0.000 dBm	0.000 dBm
Attenuation	20.000 dB	AUTO
Detector	RMS	RMS
SweepCount	3	3
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.30 dB	0.30 dB
Run	3 / max. 3	max. 3
Stable	2 / 3	3
Max Stable Difference	0.00 dB	0.30 dB


Power Spectral Density (5240 MHz; 0 (0 dBm); 20 MHz)

Result

DUT Frequency (MHz)	Frequency (MHz)	PSD (dBm)	Limit Max (dBm)	Result
5240.000000	5244.019608	0.240	17.0	PASS

Ports

Port	Duty Cycle (%)
1	100.000

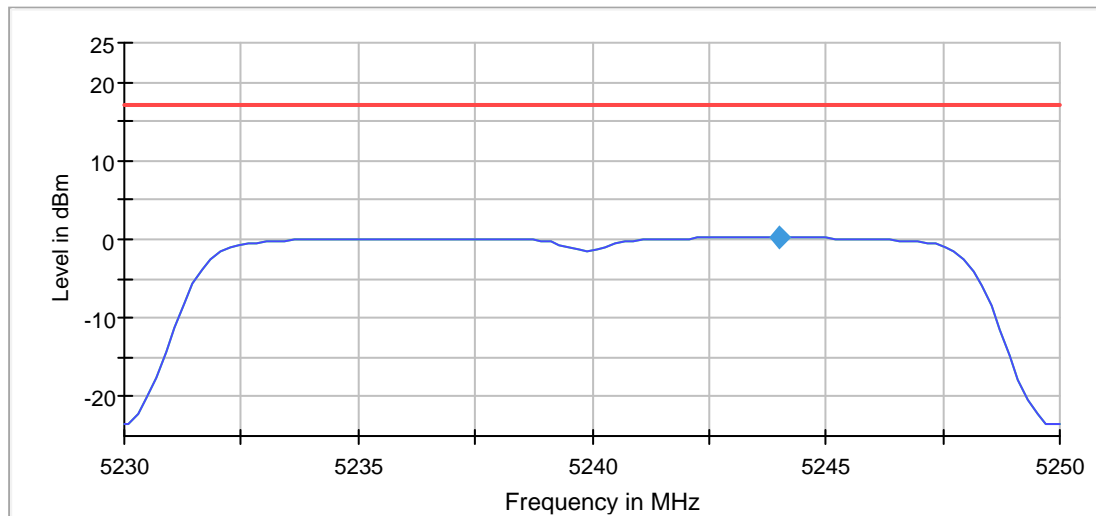

— Connector 1 — Sum Level — Limit ◆ PSD

Measurement

Setting	Instrument Value	Target Value
Start Frequency	5.23000 GHz	5.23000 GHz
Stop Frequency	5.25000 GHz	5.25000 GHz
Span	20.000 MHz	20.000 MHz
RBW	1.000 MHz	<= 1.000 MHz
VBW	3.000 MHz	>= 3.000 MHz
SweepPoints	101	~ 40
SweepTime	2.020 s	2.020 s
Reference Level	0.000 dBm	0.000 dBm
Attenuation	20.000 dB	AUTO
Detector	RMS	RMS
SweepCount	3	3
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.30 dB	0.30 dB
Run	3 / max. 3	max. 3
Stable	2 / 3	3
Max Stable Difference	0.00 dB	0.30 dB

Tx Spurious Emission (5180 MHz; 0 (0 dBm); 20 MHz)

Result

DUT Frequency (MHz)	Result
5180.000000	PASS

Final measurements


Frequency (MHz)	Level Pre Measurement (dBm)	level (dBm)	Limit (dBm)	Margin (dB)	Result
4945.549265	-46.0	-55.0	-41.2	13.8	PASS
5021.530956	-43.5	-52.8	-41.2	11.6	PASS
5143.501566	-42.3	-54.9	-41.2	13.7	PASS
5423.884298	-44.2	-53.5	-41.2	12.3	PASS
10360.323141	-32.1	-42.6	-27.0	15.6	PASS
36497.750161	-46.3	-57.1	-41.2	15.9	PASS

Pre Measurements

Frequency (MHz)	Level (dBm)	Margin (dB)	Limit (dBm)
5143.501566	-42.3	1.1	-41.2
5145.501084	-42.3	1.1	-41.2
5144.501325	-42.4	1.2	-41.2
5021.530956	-43.5	2.3	-41.2
5147.500602	-43.7	2.5	-41.2
5146.500843	-43.7	2.5	-41.2
5013.532884	-43.8	2.6	-41.2
5016.532161	-43.8	2.6	-41.2
5012.533125	-44.0	2.8	-41.2
5015.532402	-44.1	2.9	-41.2
5020.531197	-44.1	2.9	-41.2
5423.884298	-44.2	3.0	-41.2
5018.531679	-44.3	3.1	-41.2
5148.500361	-44.3	3.1	-41.2
5142.501807	-44.4	3.2	-41.2

Measurement Settings

Start Frequency (MHz)	Stop Frequency (MHz)	Pre Measurement	Final Measurement
30.000000	1000.000000	1	1
1000.000000	5150.000000	2	2
5150.000000	5250.000000	2	2
5250.000000	5350.000000	2	2
5350.000000	5470.000000	2	2
5470.000000	5725.000000	2	2
5725.000000	5850.000000	2	2
5850.000000	7000.000000	2	2
7000.000000	26000.000000	2	2
26000.000000	40000.000000	2	2

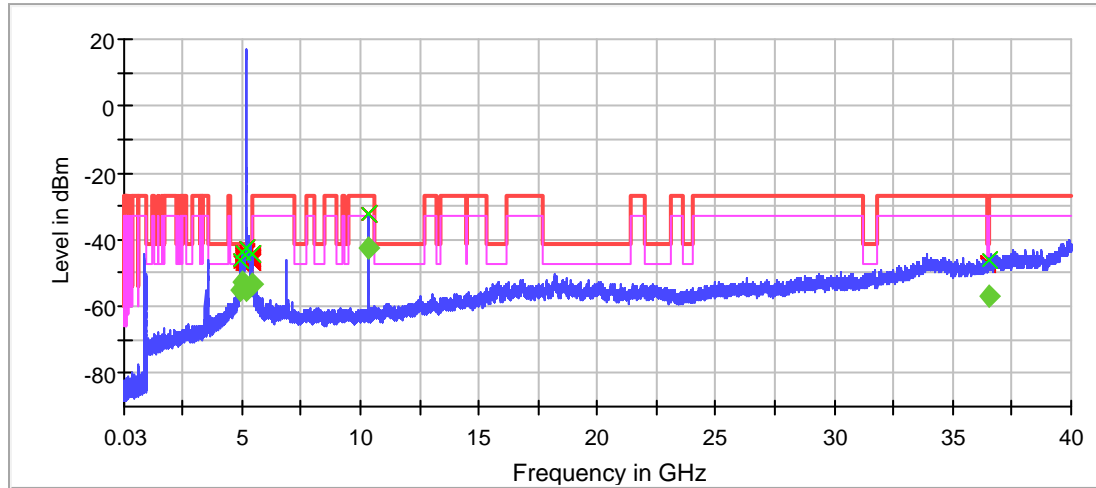

✗ Limit Final Critical
 ◆ Threshold Fail
 ✗ Critical Pass
 — Sum Level

Pre Measurement 1

Setting	Instrument Value	Target Value
RBW	100.000 kHz	<= 100.000 kHz
VBW	300.000 kHz	>= 300.000 kHz
SweepPoints	9700	~ 9700
SweepTime	9.700 ms	AUTO
Reference Level	-30.000 dBm	-30.000 dBm
Attenuation	0.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	30	30
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.50 dB	0.50 dB
Run	3 / max. 3	max. 3
Stable	0 / 3	3
Max Stable Difference	6.21 dB	0.50 dB

Pre Measurement 2

Setting	Instrument Value	Target Value
RBW	1.000 MHz	<= 1.000 MHz
VBW	3.000 MHz	>= 3.000 MHz
SweepPoints	4150	~ 4150
SweepTime	4.150 ms	AUTO
Reference Level	-30.000 dBm	-30.000 dBm
Attenuation	0.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	30	30
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.50 dB	0.50 dB
Run	3 / max. 3	max. 3
Stable	0 / 3	3
Max Stable Difference	0.51 dB	0.50 dB

Final Measurement 2

Setting	Instrument Value	Target Value
Span	ZeroSpan	ZeroSpan
RBW	1.000 MHz	~ 1.000 MHz
VBW	3.000 MHz	~ 3.000 MHz
SweepPoints	10001	~ 10001
SweepTime	50.000 ms	50.000 ms
Reference Level	-10.000 dBm	-10.000 dBm
Attenuation	0.000 dB	0.000 dB
Detector	RMS	RMS
SweepCount	1	1
Filter	3 dB	3 dB
Trace Mode	Clear Write	Clear Write
SweepType	Sweep	AUTO
Preamp	off	off

Tx Spurious Emission (5220 MHz; 0 (0 dBm); 20 MHz)

Result

DUT Frequency (MHz)	Result
5220.000000	PASS

Final measurements


Frequency (MHz)	Level Pre Measurement (dBm)	level (dBm)	Limit (dBm)	Margin (dB)	Result
1015.496266	-40.3	-51.7	-41.2	10.5	PASS
3625.867261	-44.9	-58.6	-41.2	17.4	PASS
4976.541797	-44.4	-52.9	-41.2	11.7	PASS
5064.520597	-46.1	-55.3	-41.2	14.1	PASS
5121.506866	-44.6	-55.6	-41.2	14.4	PASS
5373.305785	-43.2	-52.4	-41.2	11.2	PASS
5456.611570	-45.6	-53.1	-41.2	11.9	PASS
36491.750589	-46.3	-57.2	-41.2	16.0	PASS

Pre Measurements

Frequency (MHz)	Level (dBm)	Margin (dB)	Limit (dBm)
1015.496266	-40.3	-0.9	-41.2
1014.496507	-40.5	-0.7	-41.2
1017.495784	-43.0	1.8	-41.2
1013.496748	-43.1	1.9	-41.2
1012.496989	-43.1	1.9	-41.2
5373.305785	-43.2	2.0	-41.2
1016.496025	-43.3	2.1	-41.2
1020.495061	-43.5	2.3	-41.2
1011.497230	-43.9	2.7	-41.2
5372.314050	-44.3	3.1	-41.2
5374.297521	-44.3	3.1	-41.2
1018.495543	-44.4	3.2	-41.2
4976.541797	-44.4	3.2	-41.2
4983.540111	-44.4	3.2	-41.2
4974.542279	-44.4	3.2	-41.2

Measurement Settings

Start Frequency (MHz)	Stop Frequency (MHz)	Pre Measurement	Final Measurement
30.000000	1000.000000	1	1
1000.000000	5150.000000	2	2
5150.000000	5250.000000	2	2
5250.000000	5350.000000	2	2
5350.000000	5470.000000	2	2
5470.000000	5725.000000	2	2
5725.000000	5850.000000	2	2
5850.000000	7000.000000	2	2
7000.000000	26000.000000	2	2
26000.000000	40000.000000	2	2

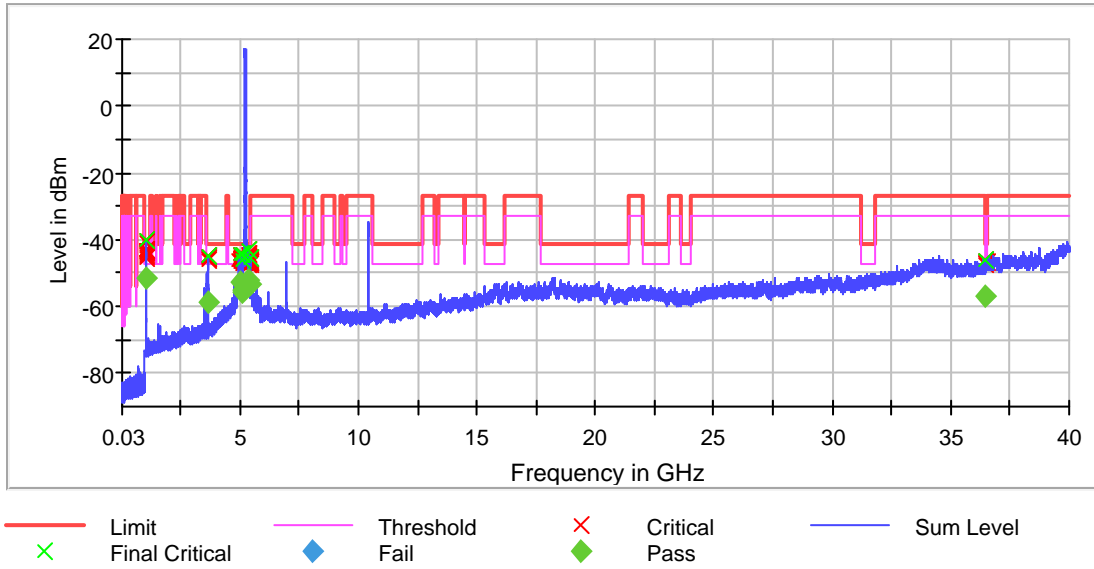

Pre Measurement 1

Setting	Instrument Value	Target Value
RBW	100.000 kHz	<= 100.000 kHz
VBW	300.000 kHz	>= 300.000 kHz
SweepPoints	9700	~ 9700
Sweeptime	9.700 ms	AUTO
Reference Level	-30.000 dBm	-30.000 dBm
Attenuation	0.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	30	30
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.50 dB	0.50 dB
Run	3 / max. 3	max. 3
Stable	2 / 3	3
Max Stable Difference	0.00 dB	0.50 dB

Pre Measurement 2

Setting	Instrument Value	Target Value
RBW	1.000 MHz	<= 1.000 MHz
VBW	3.000 MHz	>= 3.000 MHz
SweepPoints	4150	~ 4150
SweepTime	4.150 ms	AUTO
Reference Level	-30.000 dBm	-30.000 dBm
Attenuation	0.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	30	30
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.50 dB	0.50 dB
Run	3 / max. 3	max. 3
Stable	0 / 3	3
Max Stable Difference	2.65 dB	0.50 dB

Final Measurement 2

Setting	Instrument Value	Target Value
Span	ZeroSpan	ZeroSpan
RBW	1.000 MHz	~ 1.000 MHz
VBW	3.000 MHz	~ 3.000 MHz
SweepPoints	10001	~ 10001
SweepTime	50.000 ms	50.000 ms
Reference Level	-10.000 dBm	-10.000 dBm
Attenuation	0.000 dB	0.000 dB
Detector	RMS	RMS
SweepCount	1	1
Filter	3 dB	3 dB
Trace Mode	Clear Write	Clear Write
SweepType	Sweep	AUTO
Preamp	off	off

Tx Spurious Emission (5240 MHz; 0 (0 dBm); 20 MHz)

Result

DUT Frequency (MHz)	Result
5240.000000	PASS

Final measurements


Frequency (MHz)	Level Pre Measurement (dBm)	level (dBm)	Limit (dBm)	Margin (dB)	Result
1036.491207	-39.0	-51.5	-41.2	10.3	PASS
3655.860034	-41.5	-58.1	-41.2	16.9	PASS
4994.537461	-44.5	-52.7	-41.2	11.5	PASS
5083.516020	-43.4	-52.0	-41.2	10.8	PASS
5351.487603	-42.6	-52.7	-41.2	11.5	PASS
36474.751803	-46.3	-57.4	-41.2	16.2	PASS

Pre Measurements

Frequency (MHz)	Level (dBm)	Margin (dB)	Limit (dBm)
1036.491207	-39.0	-2.2	-41.2
1035.491448	-40.9	-0.3	-41.2
1037.490966	-41.1	-0.1	-41.2
3655.860034	-41.5	0.3	-41.2
1034.491689	-41.7	0.5	-41.2
3654.860275	-42.0	0.8	-41.2
5351.487603	-42.6	1.4	-41.2
1032.492171	-42.6	1.4	-41.2
5083.516020	-43.4	2.2	-41.2
5082.516261	-43.4	2.2	-41.2
1031.492411	-43.4	2.2	-41.2
5350.495868	-43.5	2.3	-41.2
5352.479339	-43.7	2.5	-41.2
5085.515538	-43.7	2.5	-41.2
1033.491930	-43.7	2.5	-41.2

Measurement Settings

Start Frequency (MHz)	Stop Frequency (MHz)	Pre Measurement	Final Measurement
30.000000	1000.000000	1	1
1000.000000	5150.000000	2	2
5150.000000	5250.000000	2	2
5250.000000	5350.000000	2	2
5350.000000	5470.000000	2	2
5470.000000	5725.000000	2	2
5725.000000	5850.000000	2	2
5850.000000	7000.000000	2	2
7000.000000	26000.000000	2	2
26000.000000	40000.000000	2	2

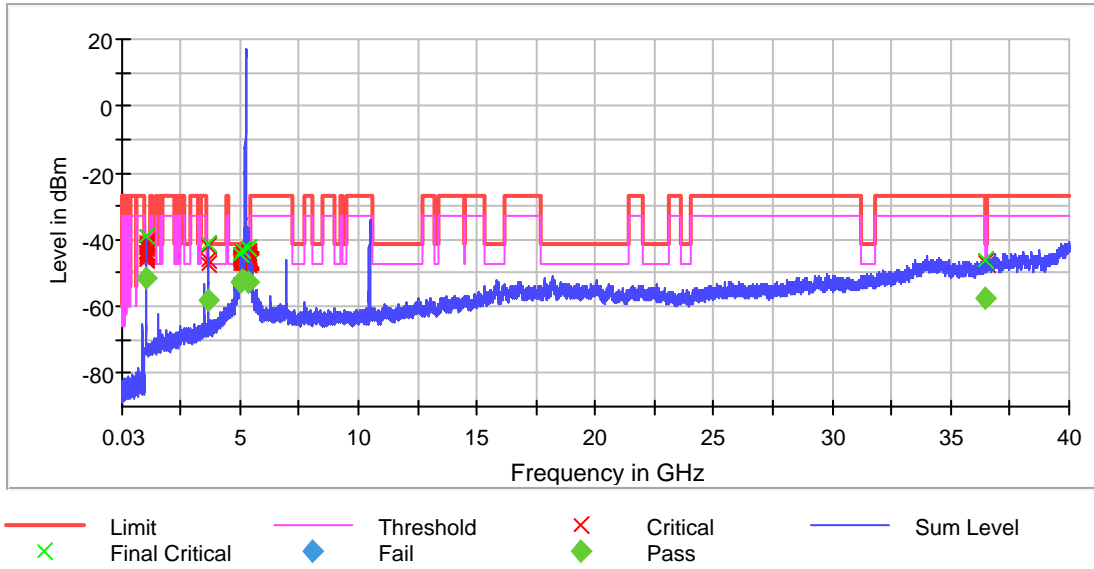

Pre Measurement 1

Setting	Instrument Value	Target Value
RBW	100.000 kHz	<= 100.000 kHz
VBW	300.000 kHz	>= 300.000 kHz
SweepPoints	9700	~ 9700
SweepTime	9.700 ms	AUTO
Reference Level	-30.000 dBm	-30.000 dBm
Attenuation	0.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	30	30
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.50 dB	0.50 dB
Run	3 / max. 3	max. 3
Stable	0 / 3	3
Max Stable Difference	2.12 dB	0.50 dB

Pre Measurement 2

Setting	Instrument Value	Target Value
RBW	1.000 MHz	<= 1.000 MHz
VBW	3.000 MHz	>= 3.000 MHz
SweepPoints	4150	~ 4150
SweepTime	4.150 ms	AUTO
Reference Level	-30.000 dBm	-30.000 dBm
Attenuation	0.000 dB	AUTO
Detector	MaxPeak	MaxPeak
SweepCount	30	30
Filter	3 dB	3 dB
Trace Mode	Max Hold	Max Hold
SweepType	Sweep	AUTO
Preamp	off	off
Stablemode	Trace	Trace
Stablevalue	0.50 dB	0.50 dB
Run	3 / max. 3	max. 3
Stable	0 / 3	3
Max Stable Difference	1.06 dB	0.50 dB

Final Measurement 2

Setting	Instrument Value	Target Value
Span	ZeroSpan	ZeroSpan
RBW	1.000 MHz	~ 1.000 MHz
VBW	3.000 MHz	~ 3.000 MHz
SweepPoints	10001	~ 10001
SweepTime	50.000 ms	50.000 ms
Reference Level	-10.000 dBm	-10.000 dBm
Attenuation	0.000 dB	0.000 dB
Detector	RMS	RMS
SweepCount	1	1
Filter	3 dB	3 dB
Trace Mode	Clear Write	Clear Write
SweepType	Sweep	AUTO
Preamp	off	off