

Appendix D

Photographs


1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System






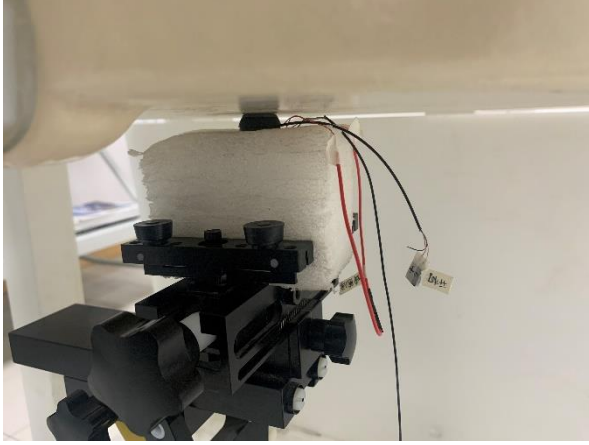


2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450

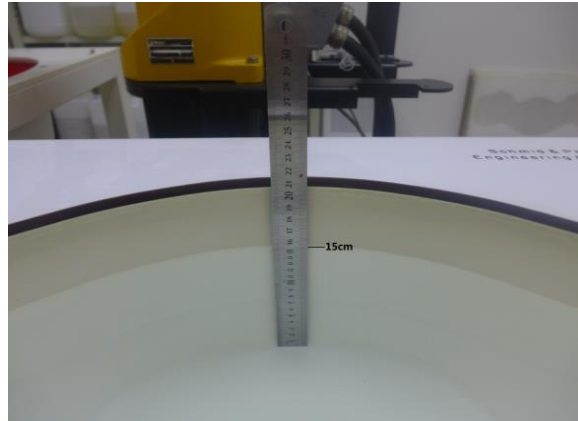

3. Photographs of EUT test position
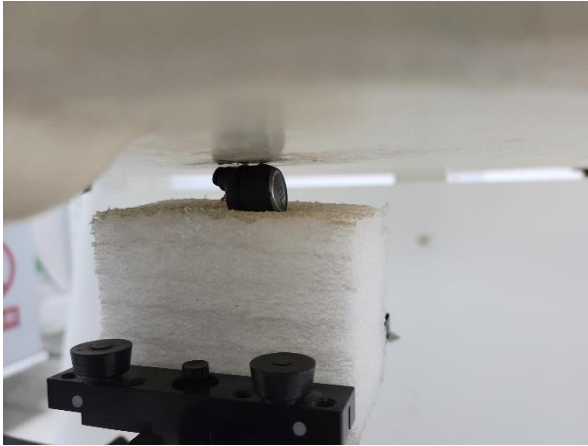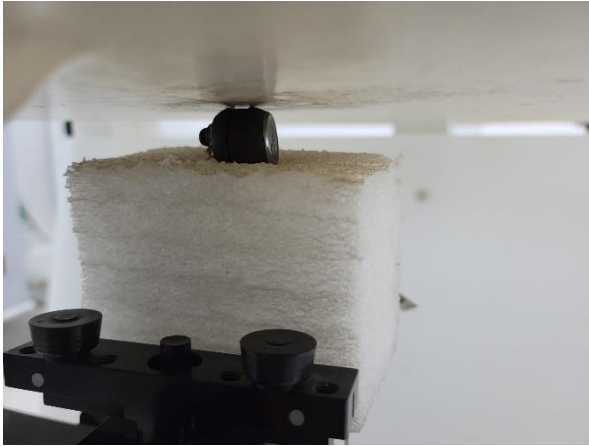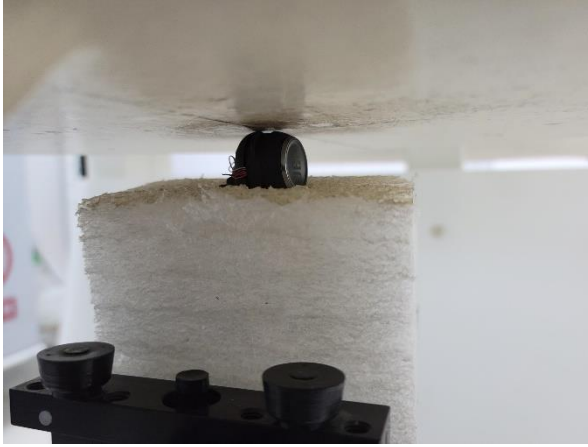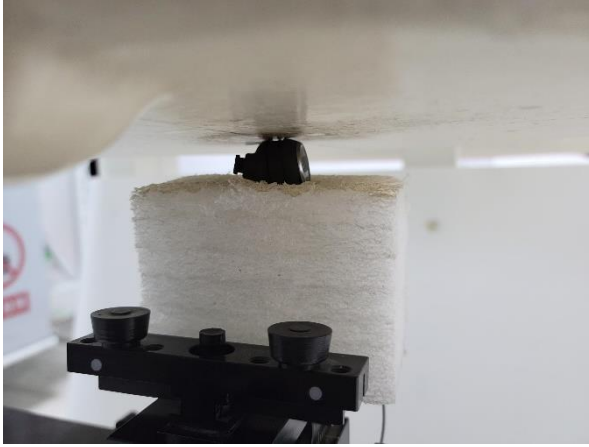
<p align="center">Photo 2: Side1 0mm</p>	<p align="center">Photo 3: Side2 0mm</p>
	
<p align="center">Photo 4: Side3 0mm</p>	<p align="center">Photo 5: Side4 0mm</p>
	
<p align="center">Photo 6: Side5 0mm</p>	<p align="center">Photo 7: Side6 0mm</p>
	
<p align="center">Photo 8: Side7 0mm</p>	<p align="center">Photo 9: Side8 0mm</p>

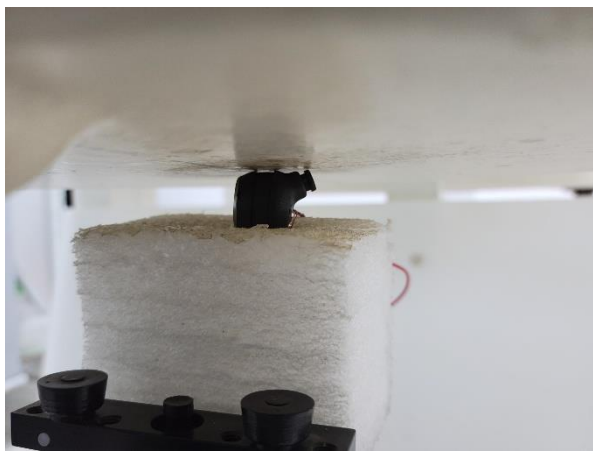


Photo 10: Side9 0mm

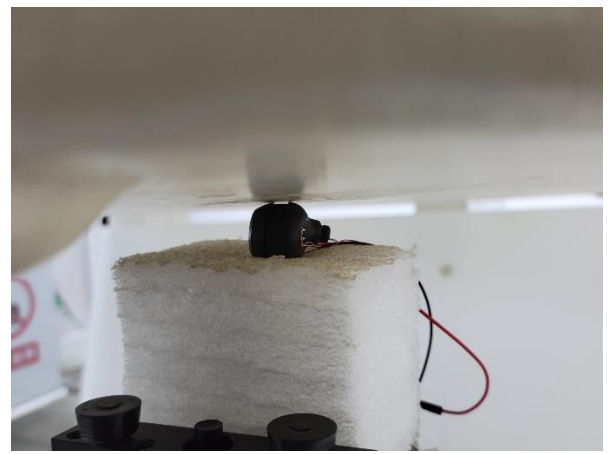


Photo 11: Side10 0mm

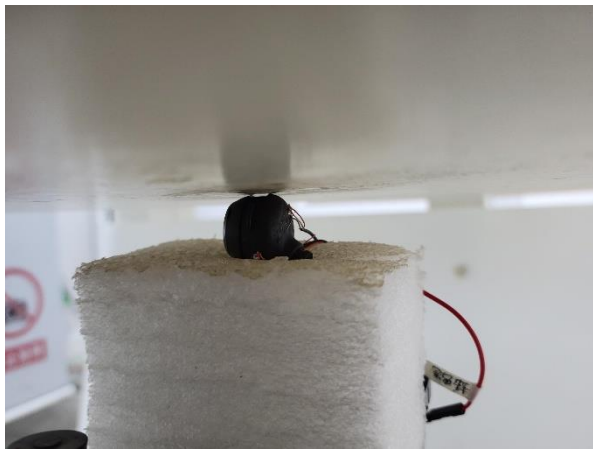


Photo 12: Side11 0mm


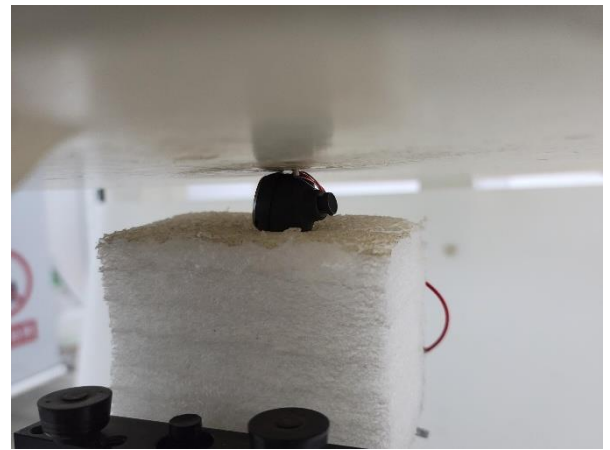


Photo 13: Side12 0mm



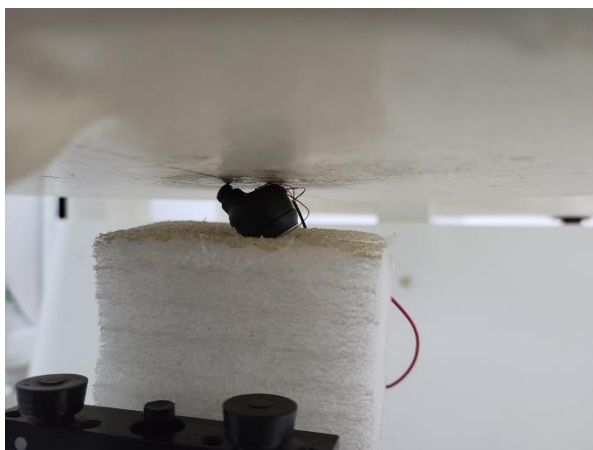

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.