

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 13.0 MHz; Type: CLA-13 - SN1004

Communication System: UID: 0, CW; Frequency: 13.0 MHz
Medium: 30 Head; Medium parameters used:
 $f = 13.0$ MHz; $\text{cond} = 0.761$ S/m; $\text{perm} = 54.6$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 0 mm

Test Date: 07/13/2025; Ambient Temp: 21.4°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN3746; ConvF:(15.27,15.58,17.13); Calibrated: 2024-10-15
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn1237; Calibrated: 2024-10-10
Phantom: ELI V6.0; Serial: 2003
Measurement SW: DASY Module SAR V16.4.0.5005

13.0 MHz System Verification at 30.0 dBm (1000 mW)


Area Scan (40.0 x 90.0): Measurement grid: $dx=10.0$ mm, $dy=15.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=6.0$ mm, $dy=6.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 1.17 W/kg

SAR(10 g) = 0.350 W/kg

Deviation (10 g) = -1.41%

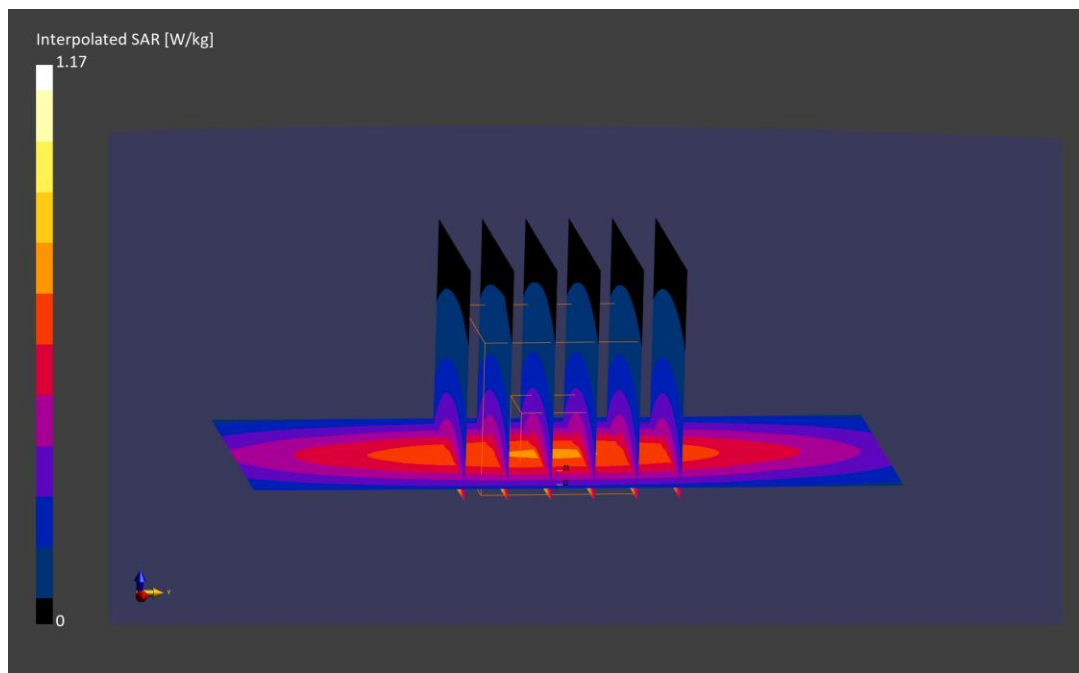

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\text{cond} = 1.78$ S/m; $\text{perm} = 40.0$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/02/2025; Ambient Temp: 19.6°C; Tissue Temp: 19.5°C

Probe: EX3DV4 - SN7551; ConvF:(6.98,6.91,7.1); Calibrated: 2025-04-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1323; Calibrated: 2025-04-15

Phantom: Twin-SAM V5.0; Serial: 1647

Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)

Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.1 W/kg

SAR(1 g) = 5.02 W/kg; SAR(10 g) = 2.36 W/kg

Deviation (1 g) = -5.82%; Deviation (10 g) = -5.98%

