

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 13.000 MHz; Type: CLA-13 - SN1004

Communication System: UID: 0, CW; Frequency: 13.000 MHz

Medium: 30 Head; Medium parameters used:

$f = 13.000$ MHz; $\text{cond} = 0.746$ S/m; $\text{perm} = 55.6$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 0 mm

Test Date: 07/09/2025; Ambient Temp: 22.3°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN3746; ConvF:(15.27,15.58,17.13); Calibrated: 2024-10-15

Sensor-Surface: 1.4mm (All points)

Electronics: DAE4 Sn1237; Calibrated: 2024-10-10

Phantom: ELI V6.0; Serial: 2003

Measurement SW: DASY Module SAR V16.4.0.5005

13.0 MHz System Verification at 30.0 dBm (1000 mW)


Area Scan (40.0 x 90.0): Measurement grid: $dx=10.0$ mm, $dy=15.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=6.0$ mm, $dy=6.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 1.22 W/kg

SAR(10 g) = 0.365 W/kg

Deviation (10 g) = 2.82%

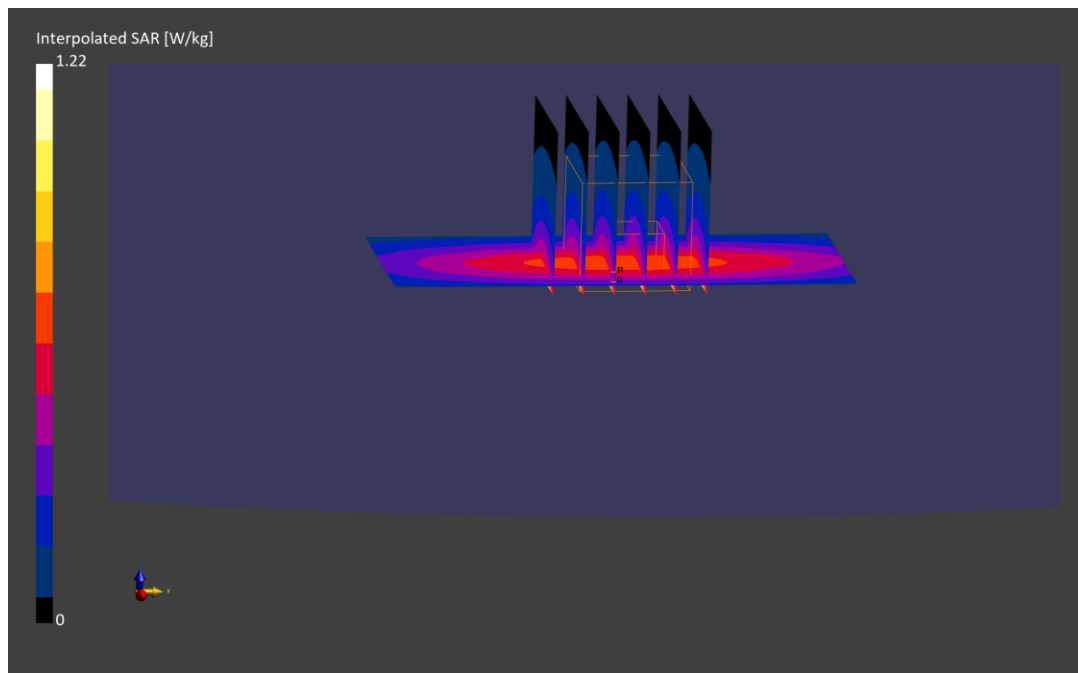

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.000 MHz
Medium: 2450 Head; Medium parameters used:
 $f = 2450.000$ MHz; $\text{cond} = 1.79$ S/m; $\text{perm} = 38.4$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/18/2025; Ambient Temp: 19.9°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7551; ConvF:(6.98,6.91,7.1); Calibrated: 2025-04-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1323; Calibrated: 2025-04-15
Phantom: Twin-SAM V4.0; Serial: 1447
Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.3 W/kg

SAR(1 g) = 5.14 W/kg; SAR(10 g) = 2.40 W/kg

Deviation (1 g) = -3.56%; Deviation (10 g) = -4.38%

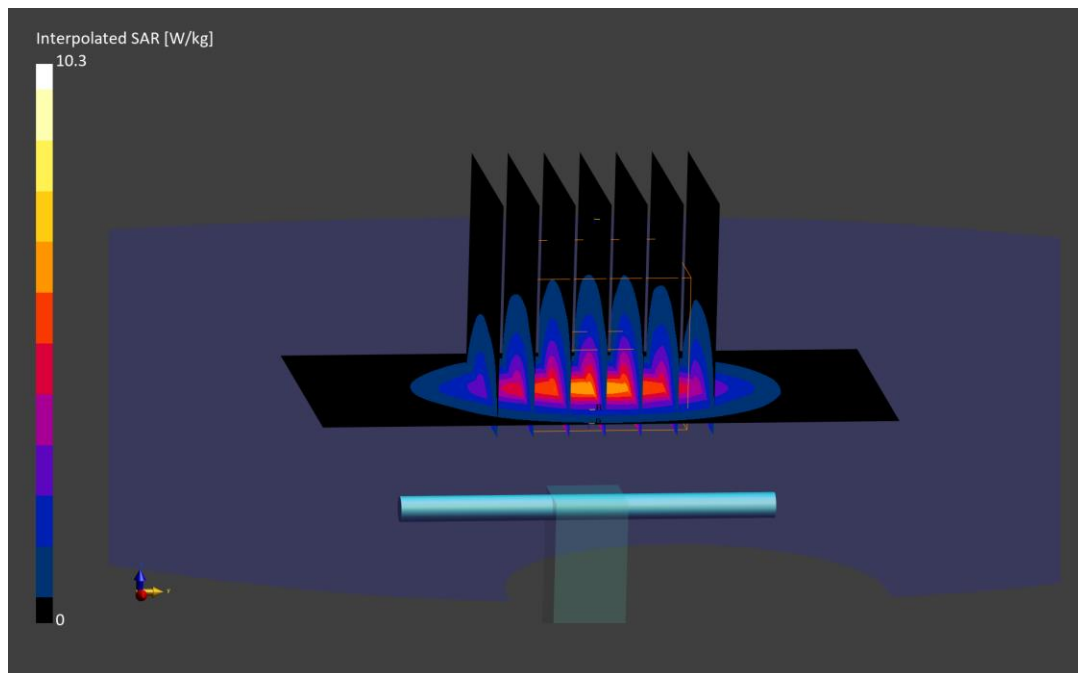

ELEMENT

DUT: Dipole 2450.000 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.000 MHz
Medium: 2450 Head; Medium parameters used:
 $f = 2450.000$ MHz; $\text{cond} = 1.85$ S/m; $\text{perm} = 38.7$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/23/2025; Ambient Temp: 21.0°C; Tissue Temp: 23.4°C

Probe: EX3DV4 - SN7532; ConvF:(6.89,6.81,7.65); Calibrated: 2025-04-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn501; Calibrated: 2025-04-09
Phantom: Twin-SAM V8.0; Serial: 2058
Measurement SW: DASY Module SAR V16.4.0.5005

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 31.2): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

SAR(10 g) = 2.40 W/kg

Deviation (10 g) = -4.38%

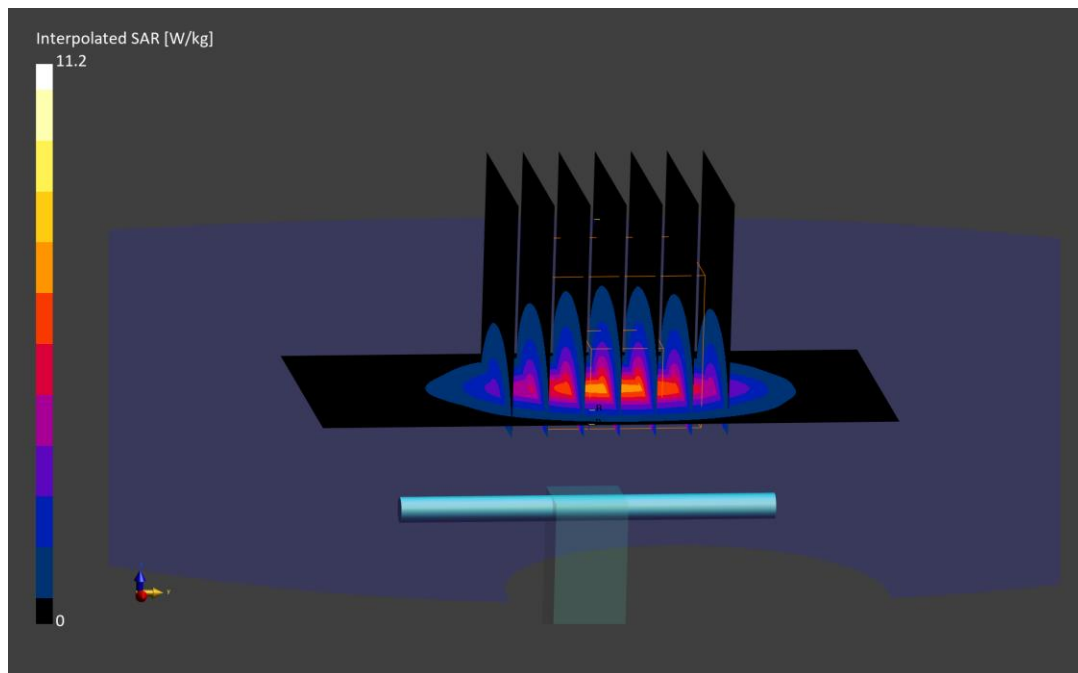

ELEMENT

DUT: Dipole 5250.000 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5250.000 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5250.000$ MHz; $\text{cond} = 4.61$ S/m; $\text{perm} = 35.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/24/2025; Ambient Temp: 21.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7782; ConvF:(5.91,5.17,5.06); Calibrated: 2024-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2024-09-03
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (32.0 x 32.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.1 W/kg

SAR(1 g) = 3.95 W/kg; SAR(10 g) = 1.13 W/kg

Deviation (1 g) = 1.41%; Deviation (10 g) = 0.44%

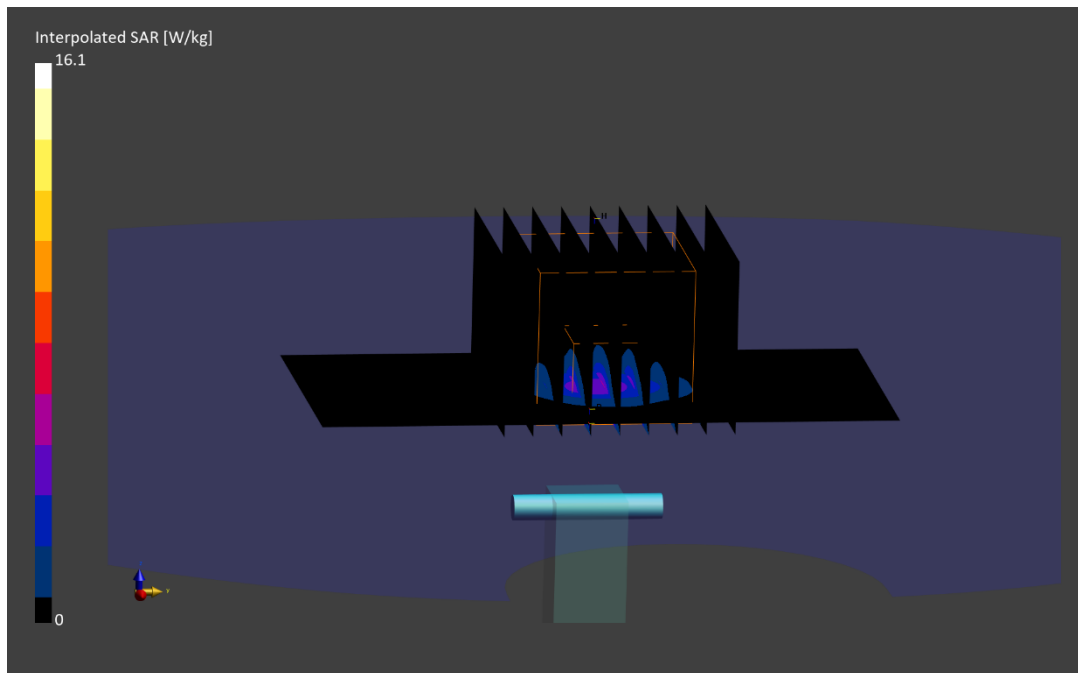

ELEMENT

DUT: Dipole 5250.000 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5250.000 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5250.000$ MHz; $\text{cond} = 4.65$ S/m; $\text{perm} = 36.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/11/2025; Ambient Temp: 20.4°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7499; ConvF:(5.42,5.54,5.73); Calibrated: 2025-01-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1465; Calibrated: 2025-01-08
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.4.0.5005

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.7 W/kg

SAR(1 g) = 3.82 W/kg

Deviation (1 g) = -1.93%

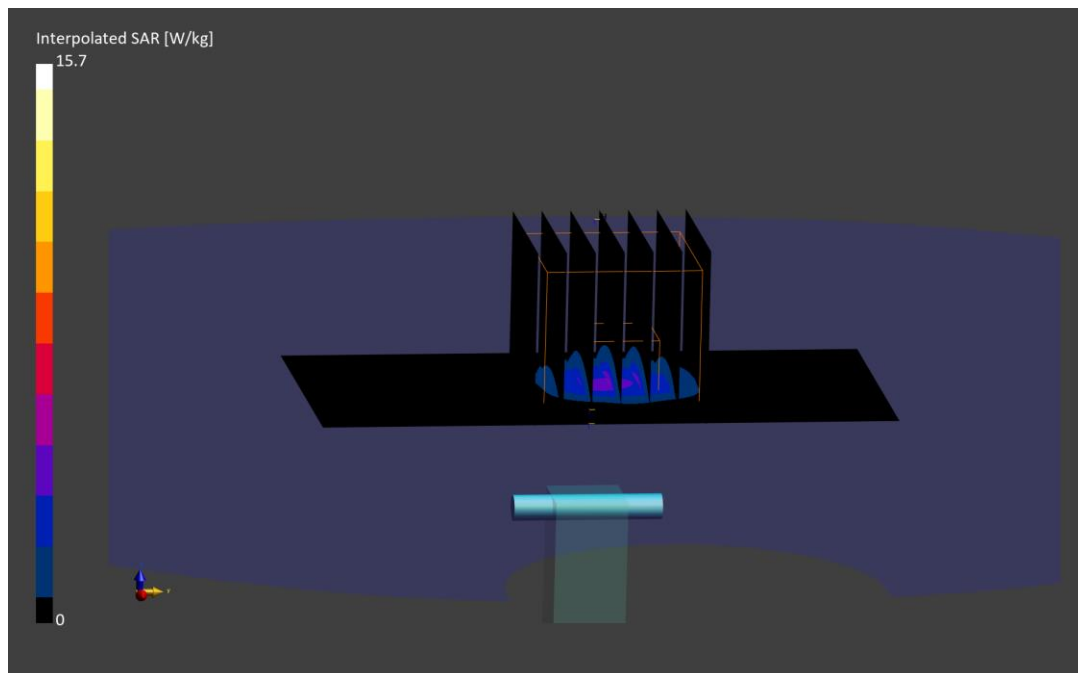

ELEMENT

DUT: Dipole 5600.000 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5600.000 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5600.000$ MHz; $\text{cond} = 5.01$ S/m; $\text{perm} = 34.3$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/24/2025; Ambient Temp: 21.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7782; ConvF:(5.12,4.48,4.38); Calibrated: 2024-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2024-09-03
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.6 W/kg

SAR(1 g) = 4.24 W/kg; SAR(10 g) = 1.21 W/kg

Deviation (1 g) = 3.67%; Deviation (10 g) = 2.11%

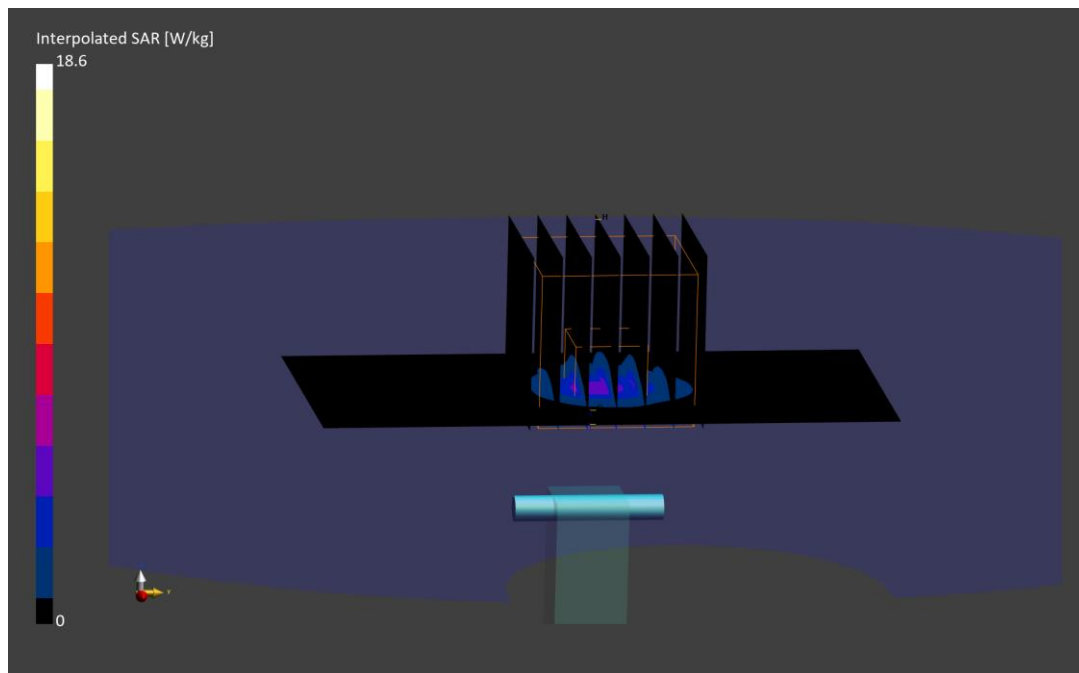

ELEMENT

DUT: Dipole 5600.000 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5600.000 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5600.000$ MHz; $\text{cond} = 5.04$ S/m; $\text{perm} = 35.4$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/11/2025; Ambient Temp: 20.4°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7499; ConvF:(4.83,4.94,5.11); Calibrated: 2025-01-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1465; Calibrated: 2025-01-08
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.4.0.5005

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 19.3 W/kg

SAR(1 g) = 4.34 W/kg

Deviation (1 g) = 6.11%

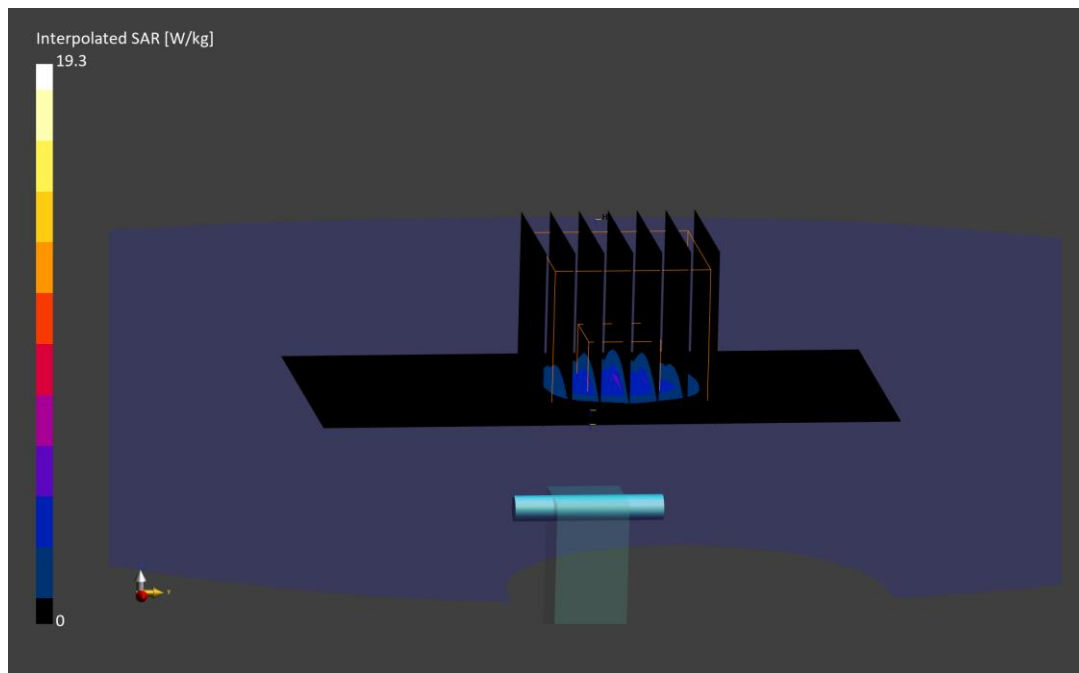

ELEMENT

DUT: Dipole 5750.000 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5750.000 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5750.000$ MHz; $\text{cond} = 5.20$ S/m; $\text{perm} = 34.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/24/2025; Ambient Temp: 21.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7782; ConvF:(5.28,4.62,4.52); Calibrated: 2024-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2024-09-03
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 3.96 W/kg; SAR(10 g) = 1.13 W/kg

Deviation (1 g) = -1.86%; Deviation (10 g) = -2.59%

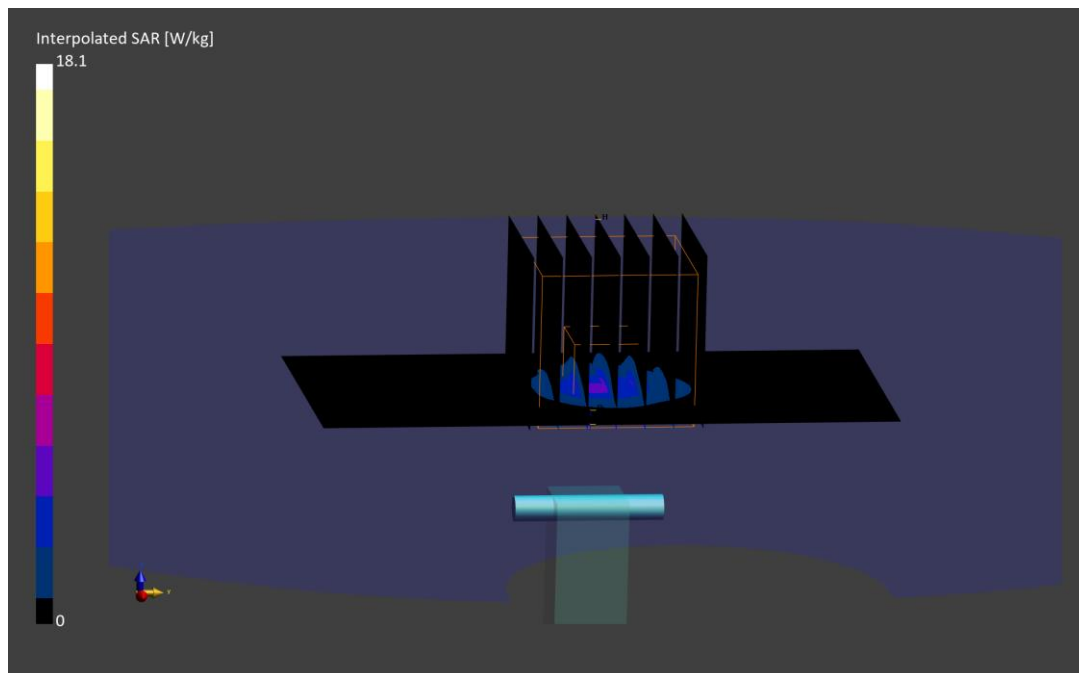

ELEMENT

DUT: Dipole 5750.000 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5750.000 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5750.000$ MHz; $\text{cond} = 5.22$ S/m; $\text{perm} = 35.1$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/11/2025; Ambient Temp: 20.4°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7499; ConvF:(4.93,5.05,5.22); Calibrated: 2025-01-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1465; Calibrated: 2025-01-08
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.4.0.5005

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.2 W/kg

SAR(1 g) = 3.96 W/kg

Deviation (1 g) = -1.86%

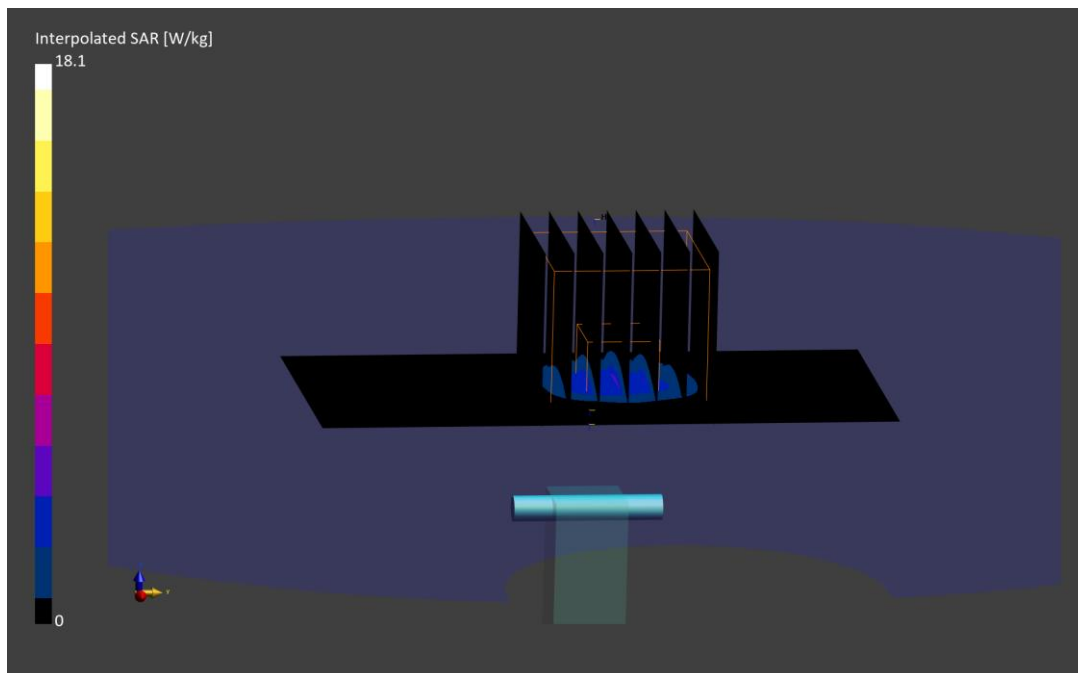

ELEMENT

DUT: Dipole 5850.000 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5850.000 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5850.000 MHz; cond = 5.31 S/m; perm = 33.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/24/2025; Ambient Temp: 21.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7782; ConvF:(5.08,4.44,4.35); Calibrated: 2024-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2024-09-03
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.5 W/kg

SAR(1 g) = 3.95 W/kg; SAR(10 g) = 1.10 W/kg

Deviation (1 g) = 2.07%; Deviation (10 g) = -0.90%

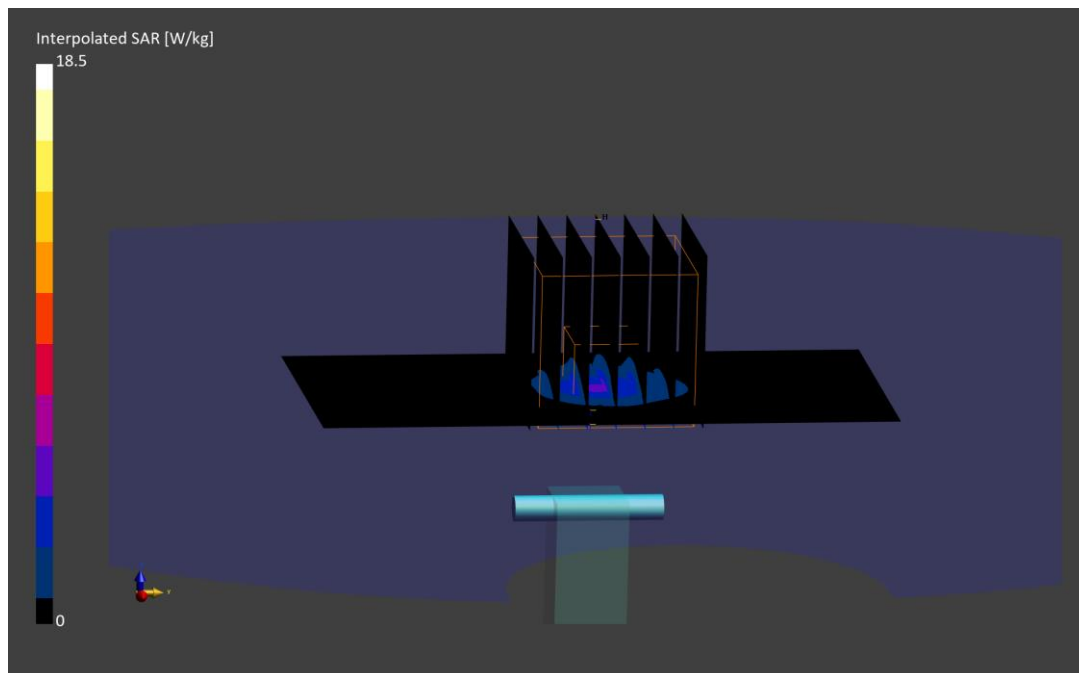

ELEMENT

DUT: Dipole 5850.000 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5850.000 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5850.000$ MHz; $\text{cond} = 5.33$ S/m; $\text{perm} = 35.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/11/2025; Ambient Temp: 20.4°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7499; ConvF:(4.9,5.02,5.19); Calibrated: 2025-01-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1465; Calibrated: 2025-01-08
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.4.0.5005

5850.0 MHz System Verification at 17.0 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (24.0 x 24.0 x 22.9): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 19.4 W/kg

SAR(1 g) = 4.10 W/kg

Deviation (1 g) = 5.94%

