


[Return to List of Scans](#) [Previous Scan](#) [Next Scan](#)

Blue Room
CISPR Class B
BCGA1041
Line 1 BCGA1041 using inverted F antenna

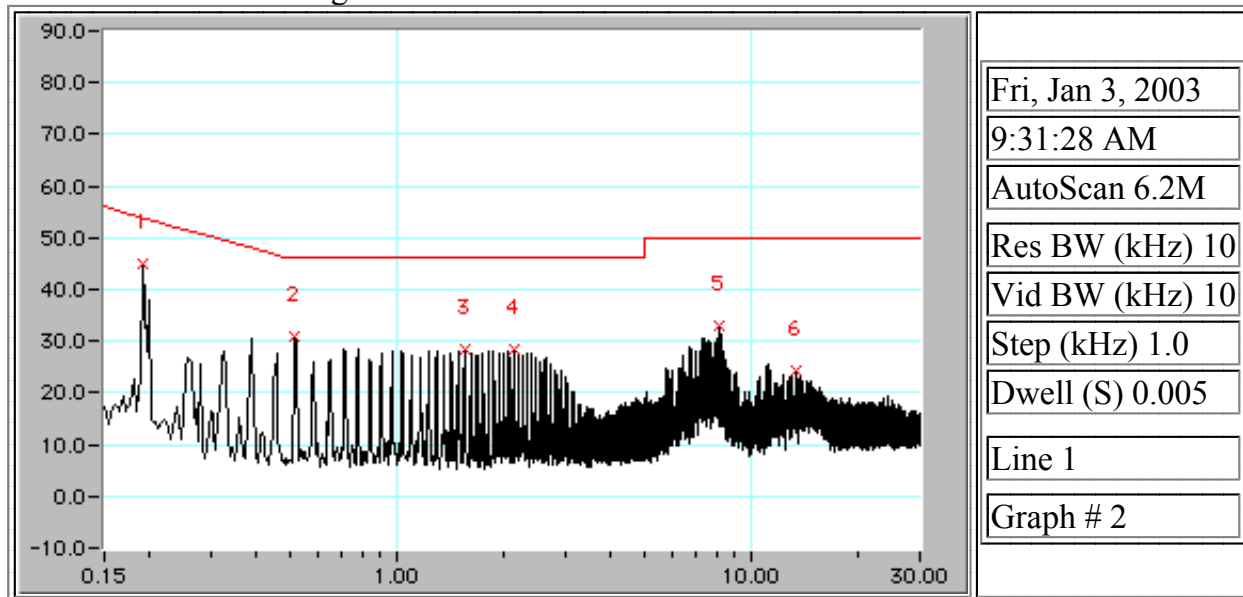


Frequency	Level	Limit	Delta	Raw	LISN	Cable	Xducer	All Factors
No.	MHz	dBuV	dB	dBuV	dB	dB	dB	dB
1	0.193	44.8 Av	53.9 -9.2	42.72	1.99	0.06	0.00	-2.05
2	0.517	30.9 Av	46.0 -15.1	30.14	0.69	0.07	0.00	-0.76
3	1.556	28.4 Av	46.0 -17.6	27.88	0.38	0.12	0.00	-0.50
4	2.142	28.4 Av	46.0 -17.6	27.88	0.34	0.14	0.00	-0.48
5	8.161	33.0 Av	50.0 -17.0	32.33	0.44	0.27	0.00	-0.71
6	13.466	24.2 Av	50.0 -25.8	23.35	0.52	0.36	0.00	-0.89

Equipment Description	Model Number	Serial Number	Last Calibration	Next Calibration
Spectrum Analyzer	HP 8568	AOU107886	22 Apr 2002	22 Apr 2003
Receiver	Rohde & Schwarz ESCS 30	100115	4 Apr 2002	4 Apr 2003
LISN	R&S ESHS3-Z5	153874	28 May 2002	28 May 2003
Cable	Blue Room Cable	CE#2	28 May 2002	28 May 2003

[Return to List of Scans](#) [Previous Scan](#) [Next Scan](#)

Blue Room
CISPR Class B
BCGA1041
Line 1 BCGA1041 using inverted F antenna

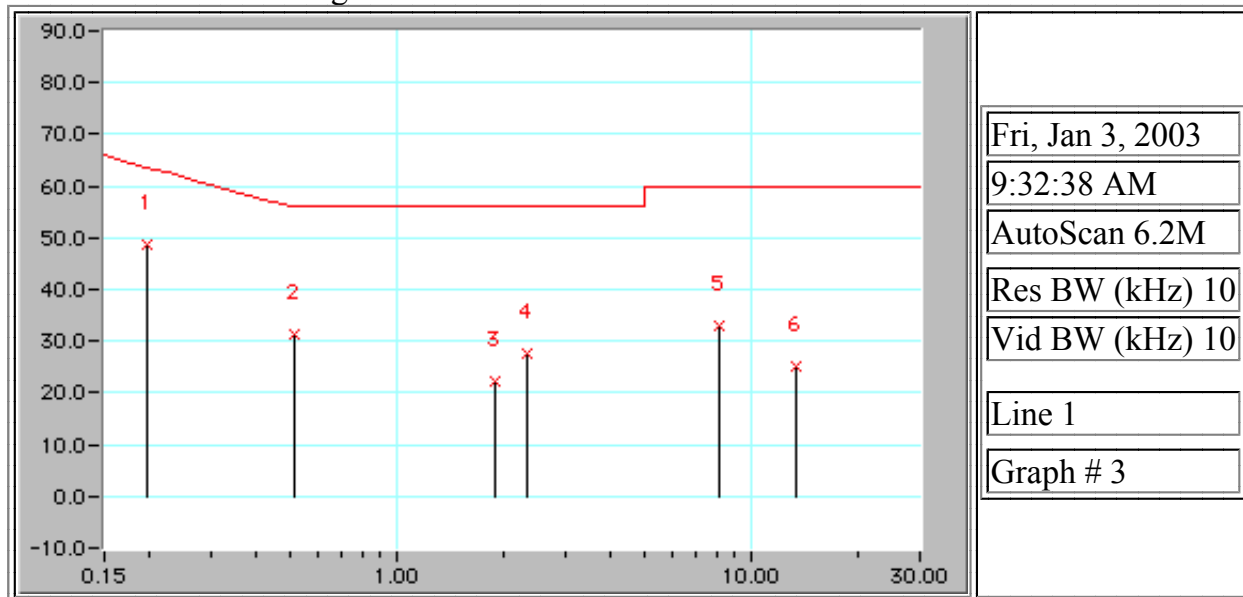


Frequency	Level	Limit	Delta	Raw	LISN	Cable	Xducer	All Factors
No. MHz	dBuV	dBuV	dB	dBuV	dB	dB	dB	dB
1 0.197	48.6 QP	63.8	-15.1	46.65	1.94	0.06	0.00	-2.00
2 0.517	31.3 QP	56.0	-24.7	30.87	0.31	0.17	0.00	-0.47
3 1.888	22.2 QP	56.0	-33.8	21.65	0.32	0.23	0.00	-0.55
4 2.337	27.8 QP	56.0	-28.2	27.09	0.44	0.27	0.00	-0.71
5 8.161	32.9 QP	60.0	-27.1	32.11	0.46	0.32	0.00	-0.79
6 13.466	25.2 QP	60.0	-34.8	24.31	0.52	0.36	0.00	-0.89

Equipment Description	Model Number	Serial Number	Last Calibration	Next Calibration
Spectrum Analyzer	HP 8568	AOU107886	22 Apr 2002	22 Apr 2003
Receiver	Rohde & Schwarz ESCS 30	100115	4 Apr 2002	4 Apr 2003
LISN	R&S ESHS3-Z5	153874	28 May 2002	28 May 2003
Cable	Blue Room Cable	CE#2	28 May 2002	28 May 2003

[Return to List of Scans](#) [Previous Scan](#) [Next Scan](#)

Blue Room
CISPR Class B
BCGA1041
Line 2 BCGA1041 using inverted F antenna

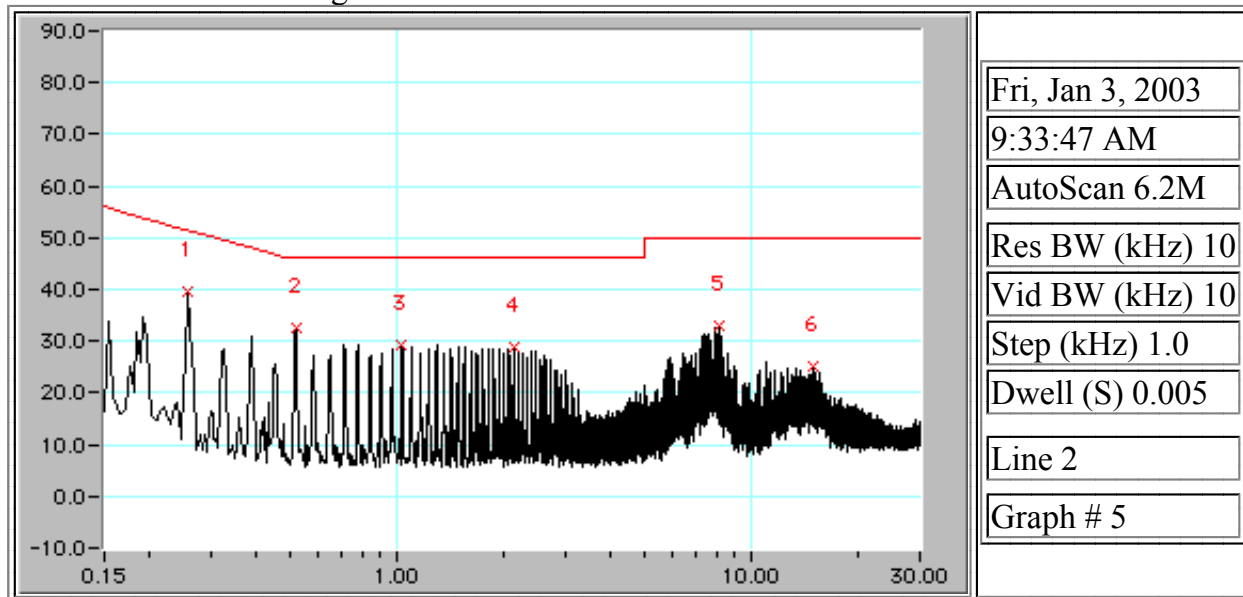

Frequency	Level	Limit	Delta	Raw	LISN	Cable	Xducer	All Factors	
No.	MHz	dBuV	dBuV	dB	dBuV	dB	dB	dB	
1	0.259	39.7	Av 51.5	-11.8	38.14	1.47	0.07	0.00	-1.54
2	0.521	32.6	Av 46.0	-13.4	31.85	0.67	0.07	0.00	-0.74
3	1.037	29.3	Av 46.0	-16.7	28.79	0.41	0.10	0.00	-0.51
4	2.142	28.7	Av 46.0	-17.3	28.26	0.30	0.14	0.00	-0.45
5	8.165	32.9	Av 50.0	-17.1	32.25	0.42	0.27	0.00	-0.69
6	14.927	25.0	Av 50.0	-25.0	24.18	0.47	0.39	0.00	-0.86

Equipment Description	Model Number	Serial Number	Last Calibration	Next Calibration
Spectrum Analyzer	HP 8568	AOU107886	22 Apr 2002	22 Apr 2003
Receiver	Rohde & Schwarz ESCS 30	100115	4 Apr 2002	4 Apr 2003
LISN	R&S ESHS3-Z5	153874	28 May 2002	28 May 2003
Cable	Blue Room Cable	CE#2	28 May 2002	28 May 2003


[Return to List of Scans](#) [Previous Scan](#) [Next Scan](#)

Blue Room

CISPR Class B

BCGA1041

Line 2 BCGA1041 using inverted F antenna

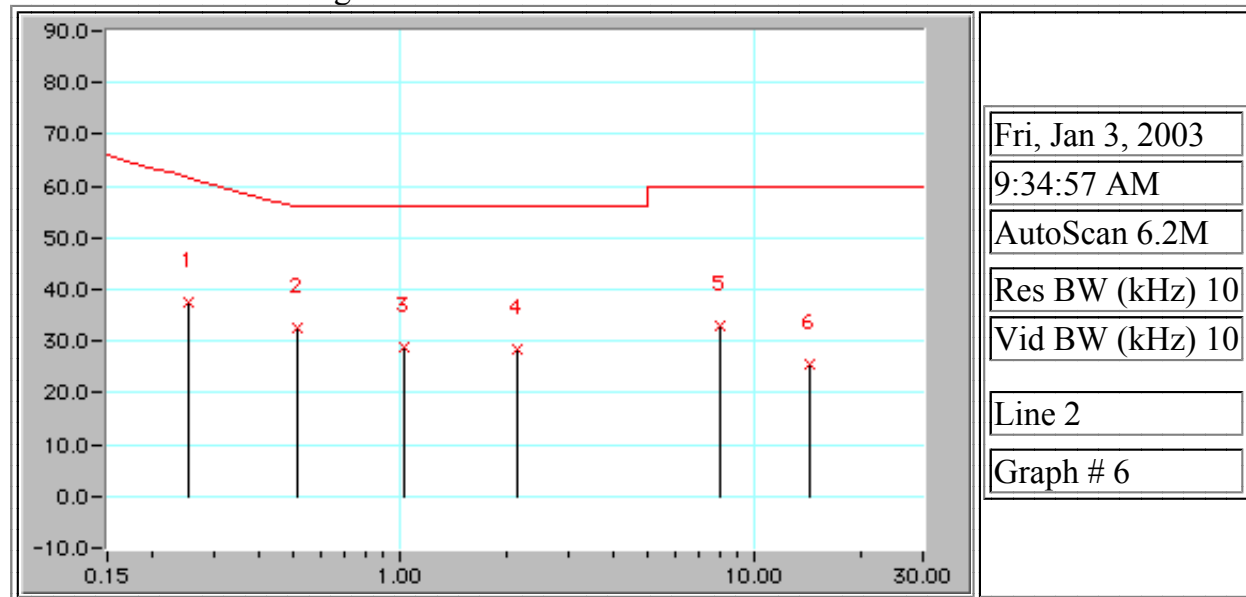

Frequency Level Limit Delta Raw LISN Cable Xducer All Factors

No.	MHz	dBuV	QP	dBuV	dB	dB	dB	dB	dB
1	0.255	37.7	QP	61.6	-24.0	36.10	1.50	0.07	0.00
2	0.517	32.6	QP	56.0	-23.4	32.10	0.31	0.17	0.00
3	1.037	28.7	QP	56.0	-27.3	28.12	0.33	0.24	0.00
4	2.142	28.3	QP	56.0	-27.7	27.59	0.43	0.29	0.00
5	8.064	33.2	QP	60.0	-26.8	32.35	0.48	0.33	0.00
6	14.298	25.5	QP	60.0	-34.5	24.68	0.47	0.38	0.00

Equipment Description	Model Number	Serial Number	Last Calibration	Next Calibration
Spectrum Analyzer	HP 8568	AOU107886	22 Apr 2002	22 Apr 2003
Receiver	Rohde & Schwarz ESCS 30	100115	4 Apr 2002	4 Apr 2003
LISN	R&S ESHS3-Z5	153874	28 May 2002	28 May 2003
Cable	Blue Room Cable	CE#2	28 May 2002	28 May 2003