

20120224_System Check D1750V2 SN 1053

Frequency: 1750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
Medium parameters used: $f = 1750$ MHz; $\sigma = 1.481$ mho/m; $\epsilon_r = 51.598$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Electronics: DAE4 Sn1239; Calibrated: 11/17/2010
- Probe: EX3DV4 - SN3772; ConvF(7.55, 7.55, 7.55); Calibrated: 2/16/2012
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (B); Type: QDOVA001BB; Serial: 1099

D1750V2/Pin=100 mW/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 4.861 mW/g


D1750V2/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.341 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 6.4340

SAR(1 g) = 3.62 mW/g; SAR(10 g) = 1.92 mW/g

Maximum value of SAR (measured) = 4.832 mW/g

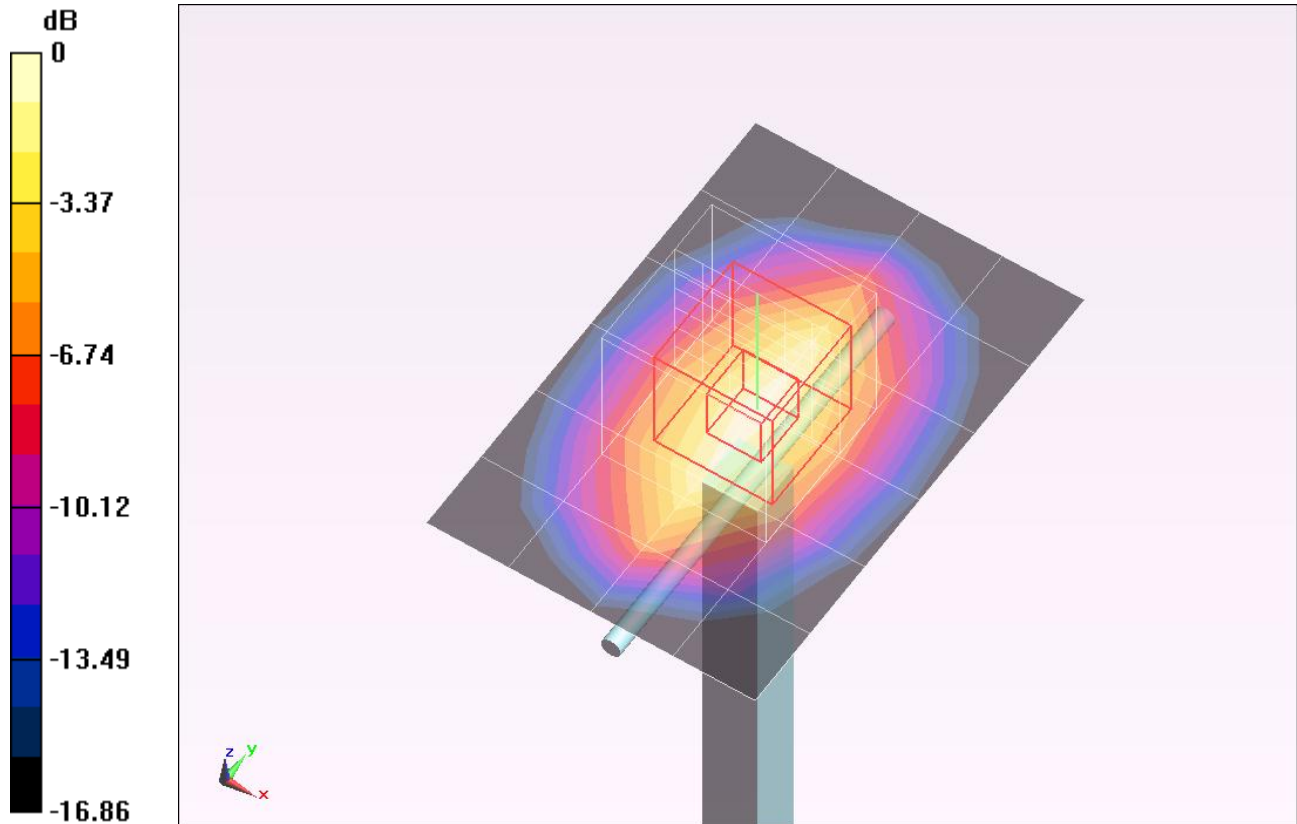


0 dB = 4.830mW/g = 13.68 dB mW/g

20120224_System Check D1750V2 SN 1053

Frequency: 1750 MHz; Duty Cycle: 1:1

D1750V2/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm

Maximum value of SAR (measured) = 4.853 mW/g

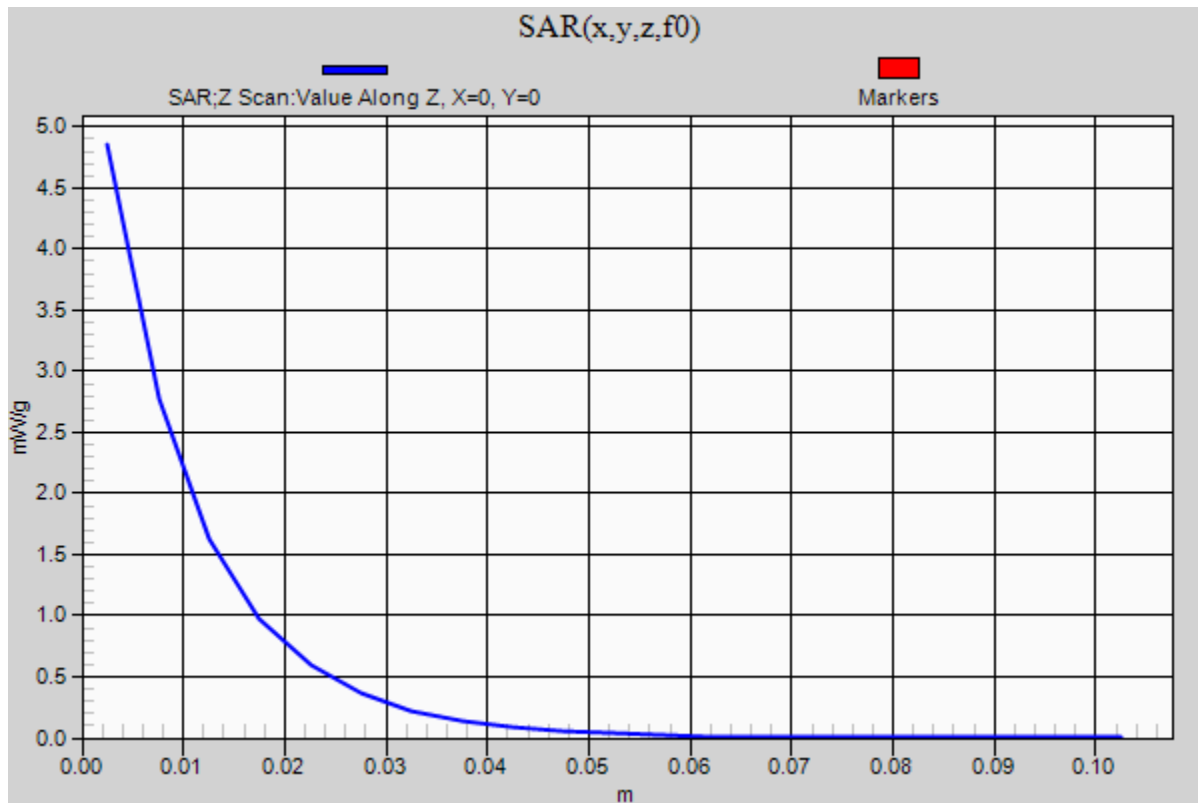

20120225_System Check D1750V2 SN 1053

Frequency: 1750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
Medium parameters used: $f = 1750$ MHz; $\sigma = 1.496$ mho/m; $\epsilon_r = 51.538$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Electronics: DAE4 Sn1239; Calibrated: 11/17/2010
- Probe: EX3DV4 - SN3772; ConvF(7.55, 7.55, 7.55); Calibrated: 2/16/2012
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (B); Type: QDOVA001BB; Serial: 1099

D1750V2/Pin=100 mW/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 4.920 mW/g


D1750V2/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.002 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 6.5920

SAR(1 g) = 3.69 mW/g; SAR(10 g) = 1.96 mW/g


Maximum value of SAR (measured) = 4.925 mW/g

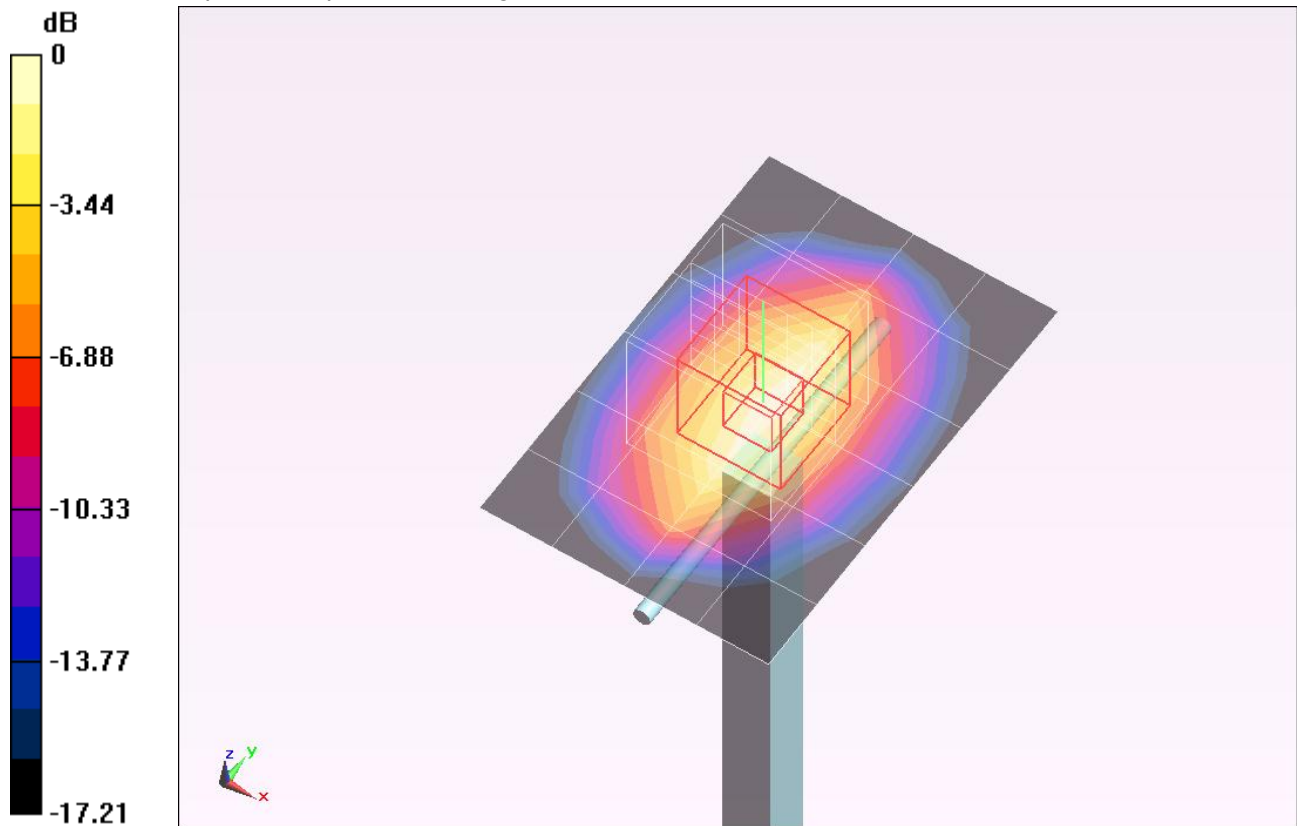

0 dB = 4.920mW/g = 13.84 dB mW/g

20120225_System Check D1750V2 SN 1053

Frequency: 1750 MHz; Duty Cycle: 1:1

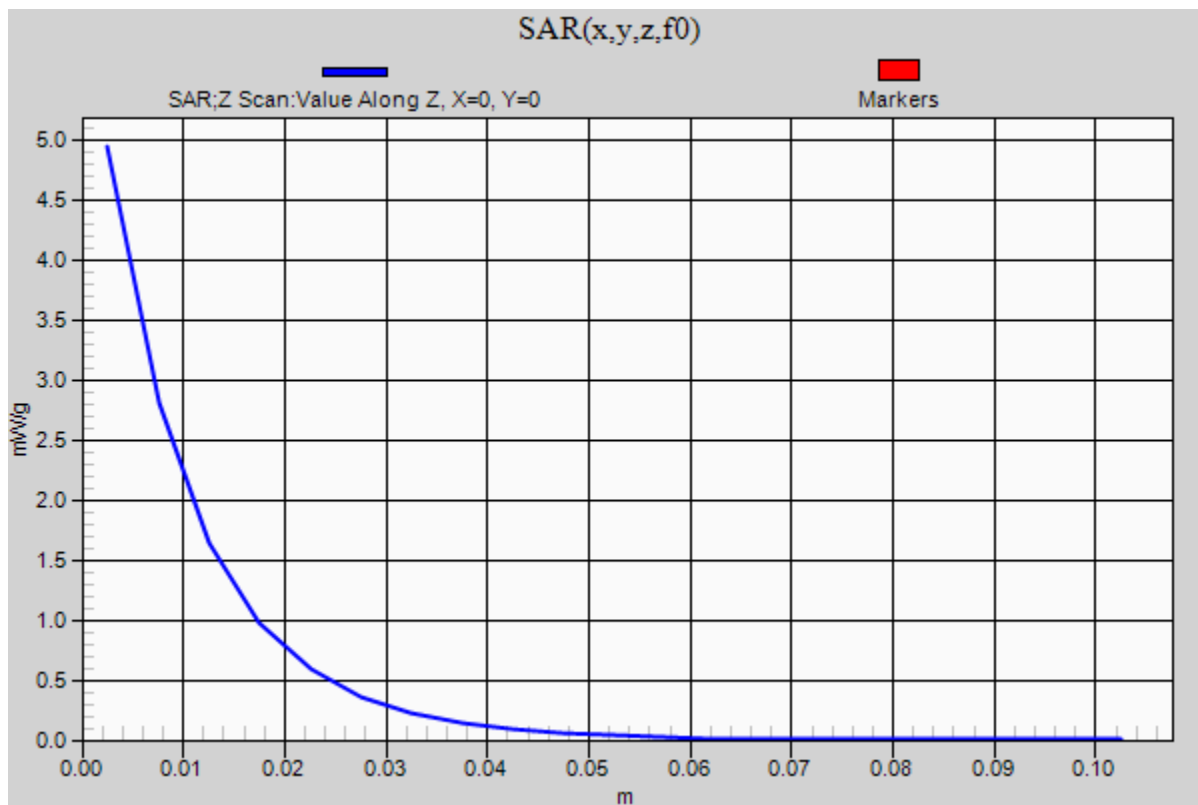D1750V2/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 4.946 mW/g

20120226_System Check D1750V2 SN 1053

Frequency: 1750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
Medium parameters used: $f = 1750$ MHz; $\sigma = 1.466$ mho/m; $\epsilon_r = 51.668$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Electronics: DAE4 Sn1239; Calibrated: 11/17/2010
- Probe: EX3DV4 - SN3772; ConvF(7.55, 7.55, 7.55); Calibrated: 2/16/2012
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (B); Type: QDOVA001BB; Serial: 1099

D1750V2/Pin=100 mW/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 4.915 mW/g


D1750V2/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.709 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 6.5640

SAR(1 g) = 3.66 mW/g; SAR(10 g) = 1.93 mW/g

Maximum value of SAR (measured) = 4.912 mW/g

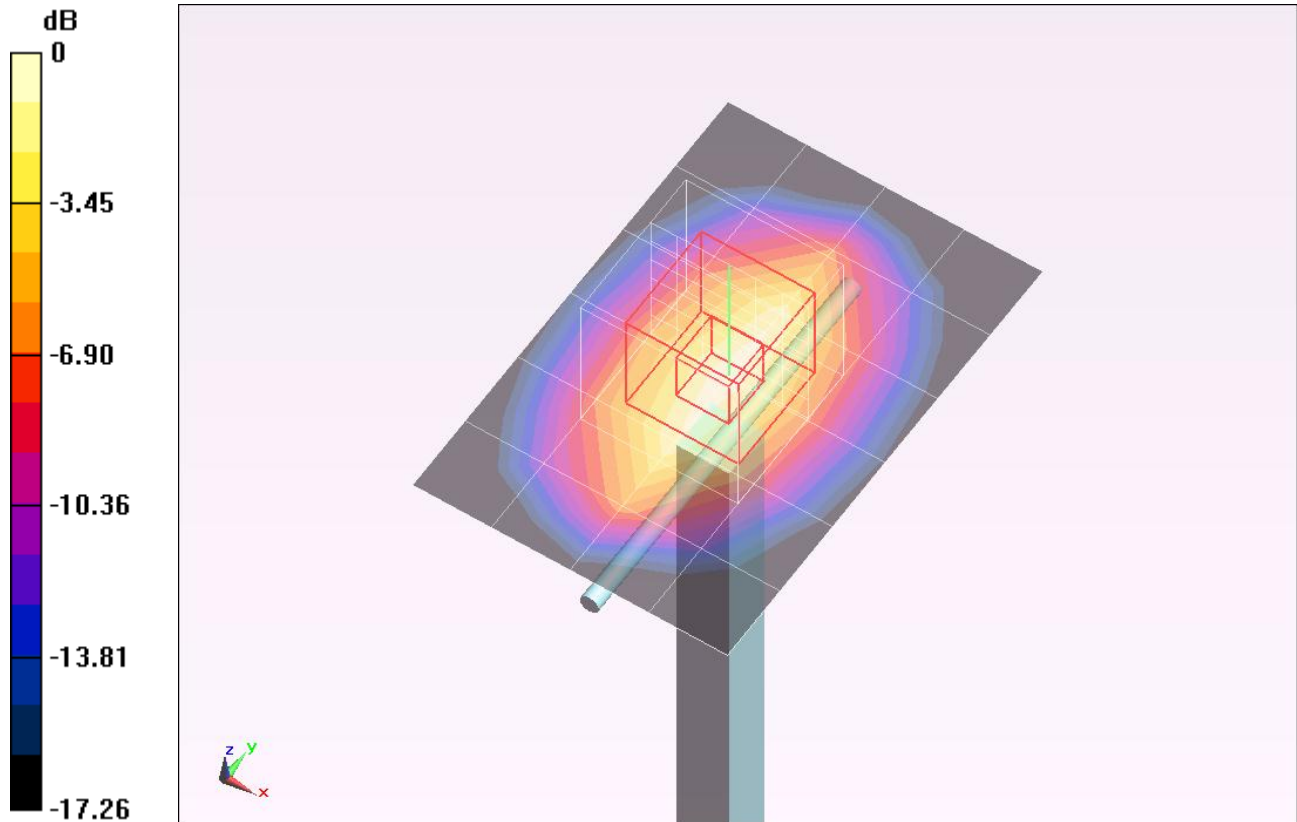


0 dB = 4.910mW/g = 13.82 dB mW/g

20120226_System Check D1750V2 SN 1053

Frequency: 1750 MHz; Duty Cycle: 1:1

D1750V2/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm

Maximum value of SAR (measured) = 4.901 mW/g

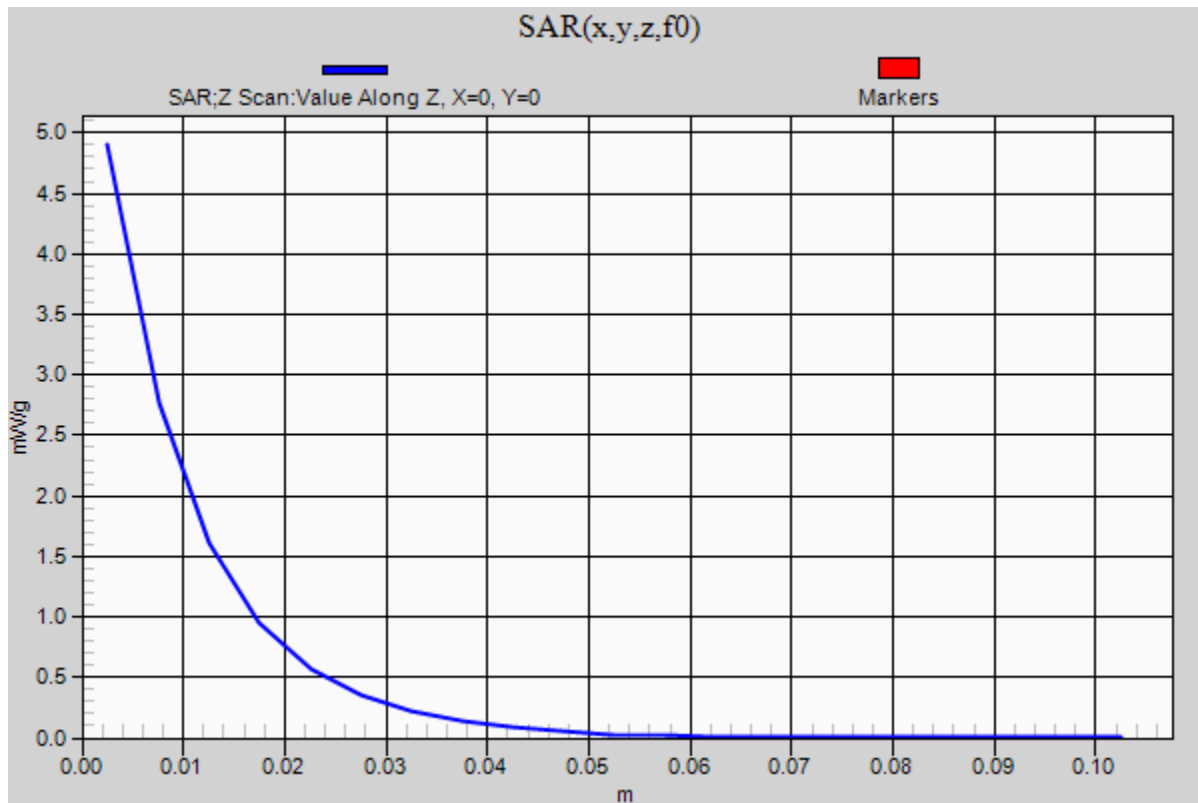

20120227_System Check D1750V2 SN 1053

Frequency: 1750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.464$ mho/m; $\epsilon_r = 51.952$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Electronics: DAE4 Sn1239; Calibrated: 11/17/2010
- Probe: EX3DV4 - SN3772; ConvF(7.55, 7.55, 7.55); Calibrated: 2/16/2012
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (B); Type: QDOVA001BB; Serial: 1099

D1750V2/Pin=100 mW/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 4.941 mW/g


D1750V2/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.363 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 6.6430

SAR(1 g) = 3.68 mW/g; SAR(10 g) = 1.94 mW/g

Maximum value of SAR (measured) = 4.962 mW/g

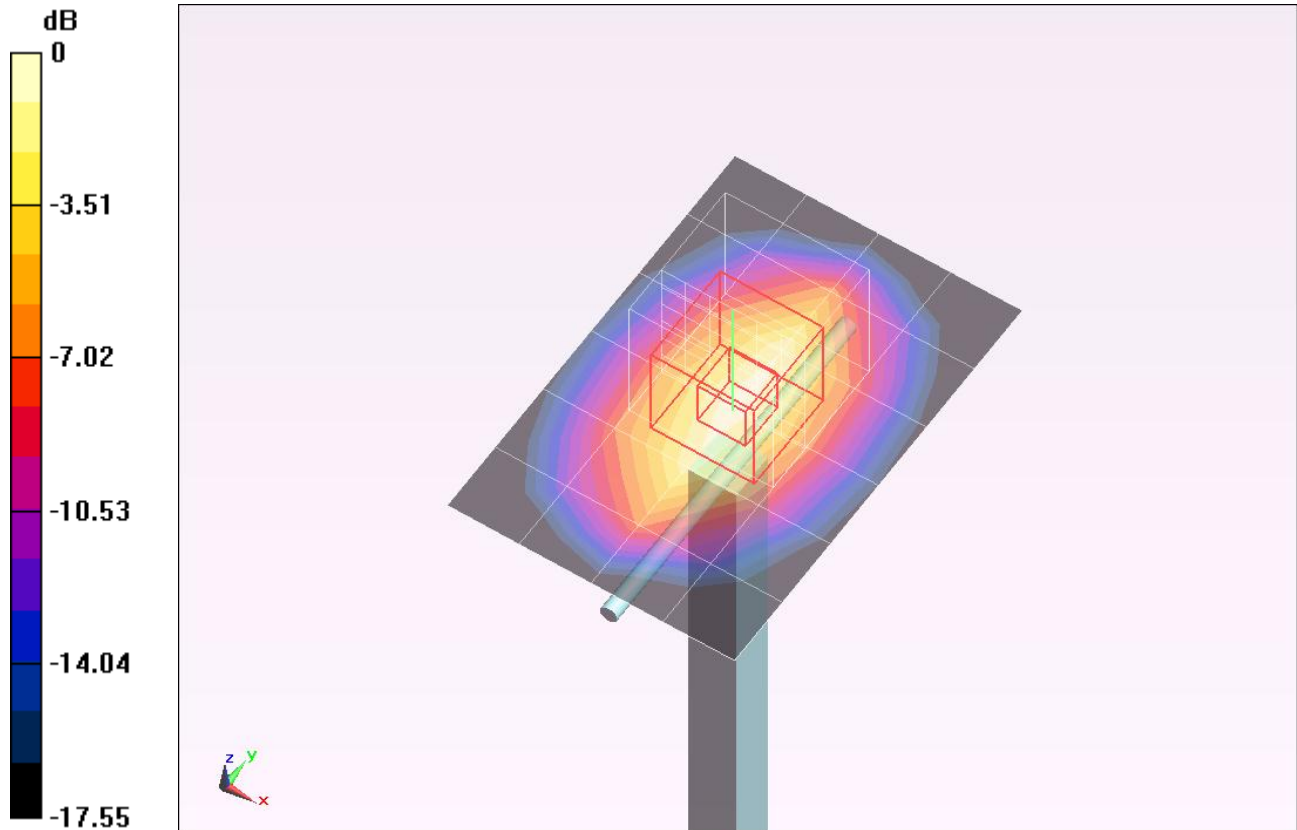


0 dB = 4.960mW/g = 13.91 dB mW/g

20120227_System Check D1750V2 SN 1053

Frequency: 1750 MHz; Duty Cycle: 1:1

D1750V2/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm

Maximum value of SAR (measured) = 4.922 mW/g

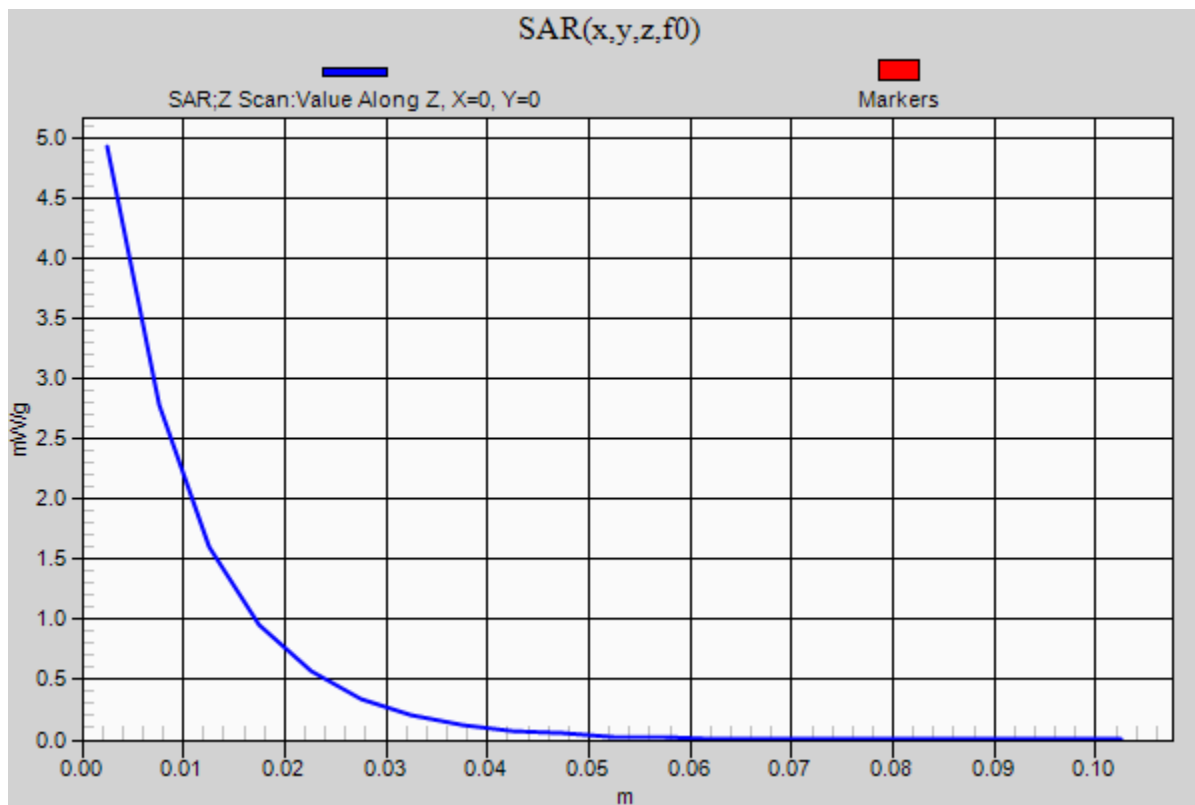

20120227_SystemPerformanceCheck-D1750V2 SN 1050

Frequency: 1750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
Medium parameters used: $f = 1750$ MHz; $\sigma = 1.45$ mho/m; $\epsilon_r = 51.6$; $\rho = 1000$ kg/m³;

DASY4 Configuration:

- Electronics: DAE3 Sn427; Calibrated: 1/17/2012
- Probe: EX3DV4 - SN3749; ConvF(7.23, 7.23, 7.23); Calibrated: 1/27/2012
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: Flat Phantom ELI4.0; Type: QDOVA001BA; Serial: SN:1003

Body, Pin=100mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 4.18 mW/g


Body, Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 61.0 V/m; Power Drift = -0.077 dB

Peak SAR (extrapolated) = 7.13 W/kg


SAR(1 g) = 3.91 mW/g; SAR(10 g) = 2.06 mW/g

Maximum value of SAR (measured) = 5.27 mW/g

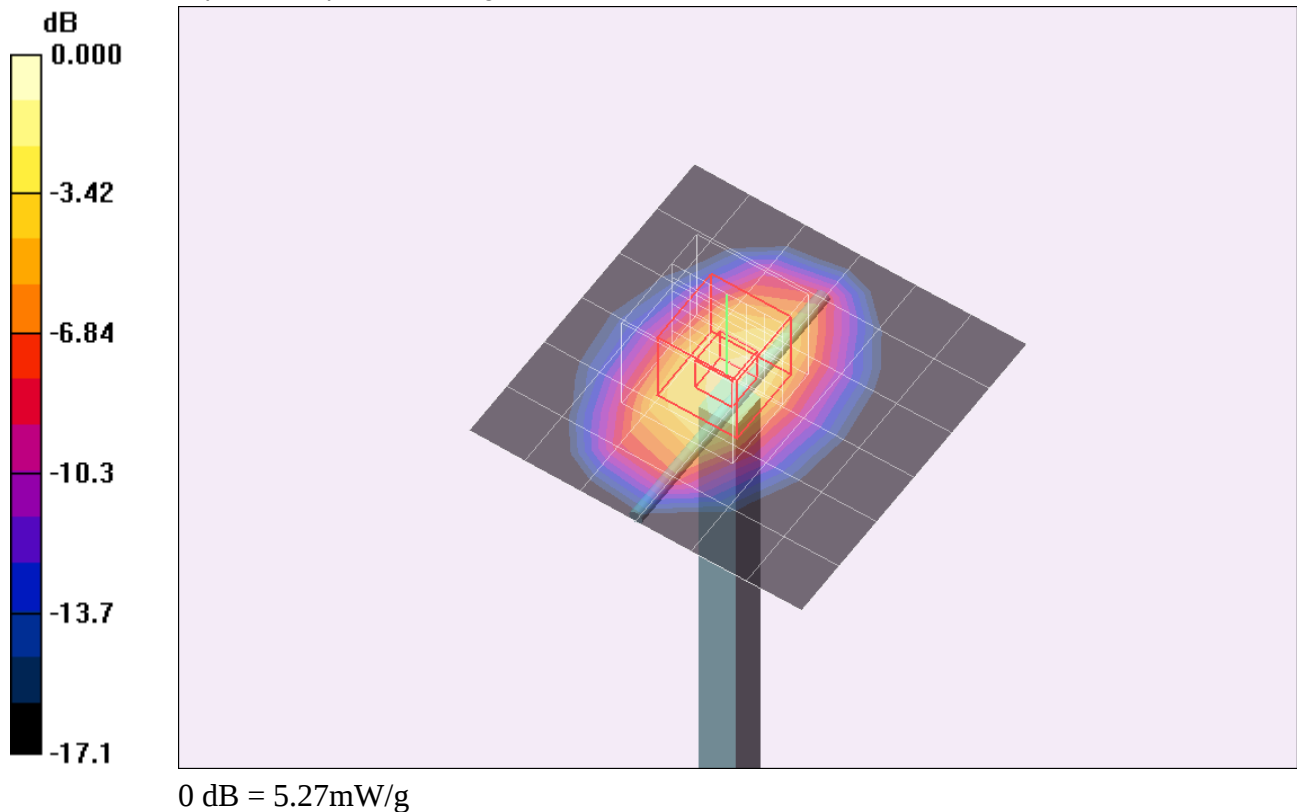

20120227_SystemPerformanceCheck-D1750V2 SN 1050

Frequency: 1750 MHz; Duty Cycle: 1:1

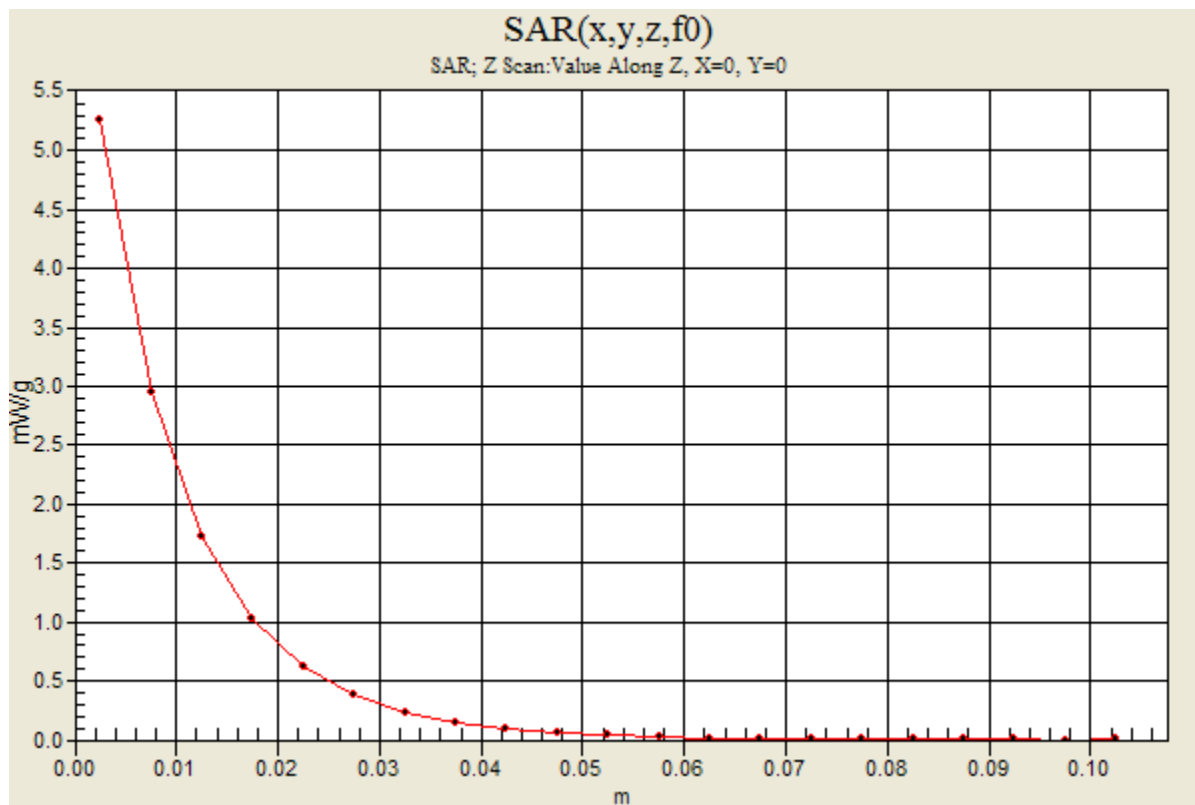Body, Pin=100mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 5.26 mW/g

20120228_System Check D1750V2 SN 1050

Frequency: 1750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
Medium parameters used: $f = 1750$ MHz; $\sigma = 1.465$ mho/m; $\epsilon_r = 51.132$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Electronics: DAE4 Sn1239; Calibrated: 11/17/2010
- Probe: EX3DV4 - SN3772; ConvF(7.55, 7.55, 7.55); Calibrated: 2/16/2012
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (B); Type: QDOVA001BB; Serial: 1099

D1750V2/Pin=100 mW/Area Scan (5x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 5.006 mW/g


D1750V2/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 59.048 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 6.6980

SAR(1 g) = 3.75 mW/g; SAR(10 g) = 1.98 mW/g


Maximum value of SAR (measured) = 5.017 mW/g

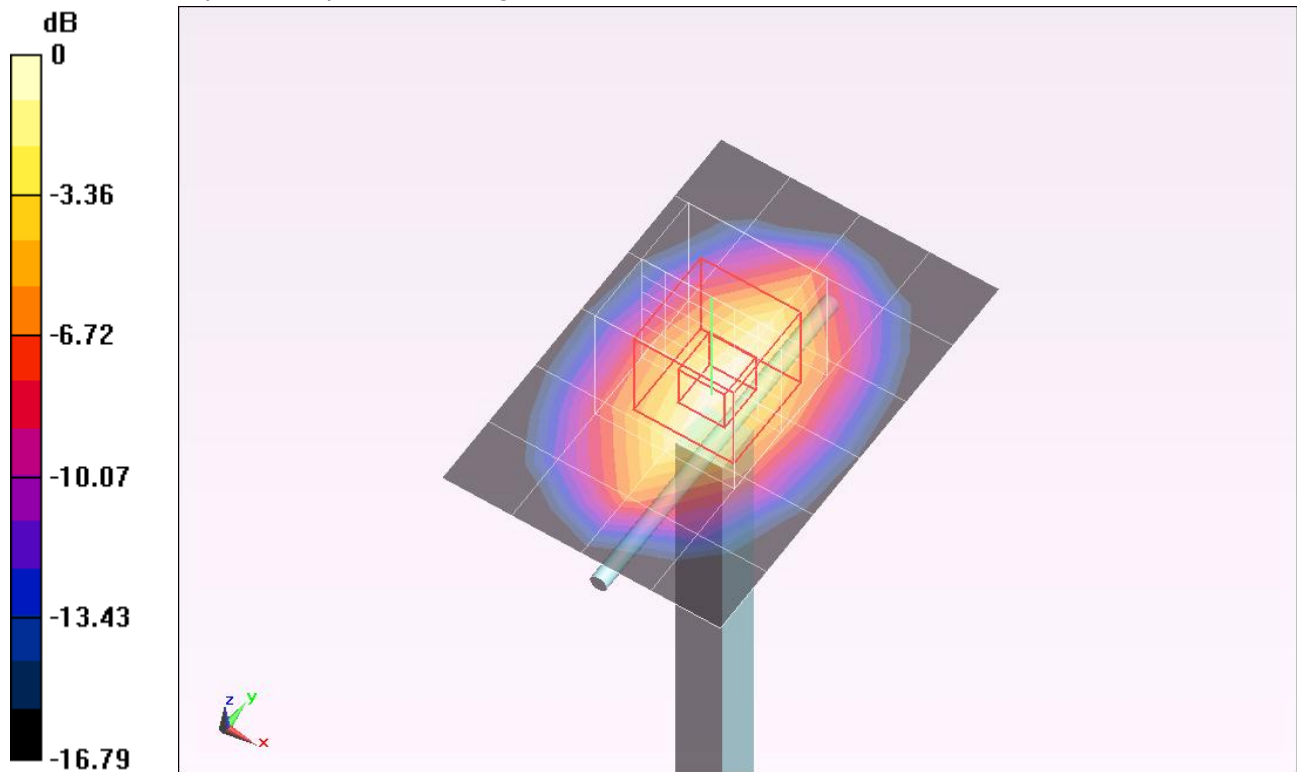

0 dB = 5.020mW/g = 14.01 dB mW/g

20120228_System Check D1750V2 SN 1050

Frequency: 1750 MHz; Duty Cycle: 1:1

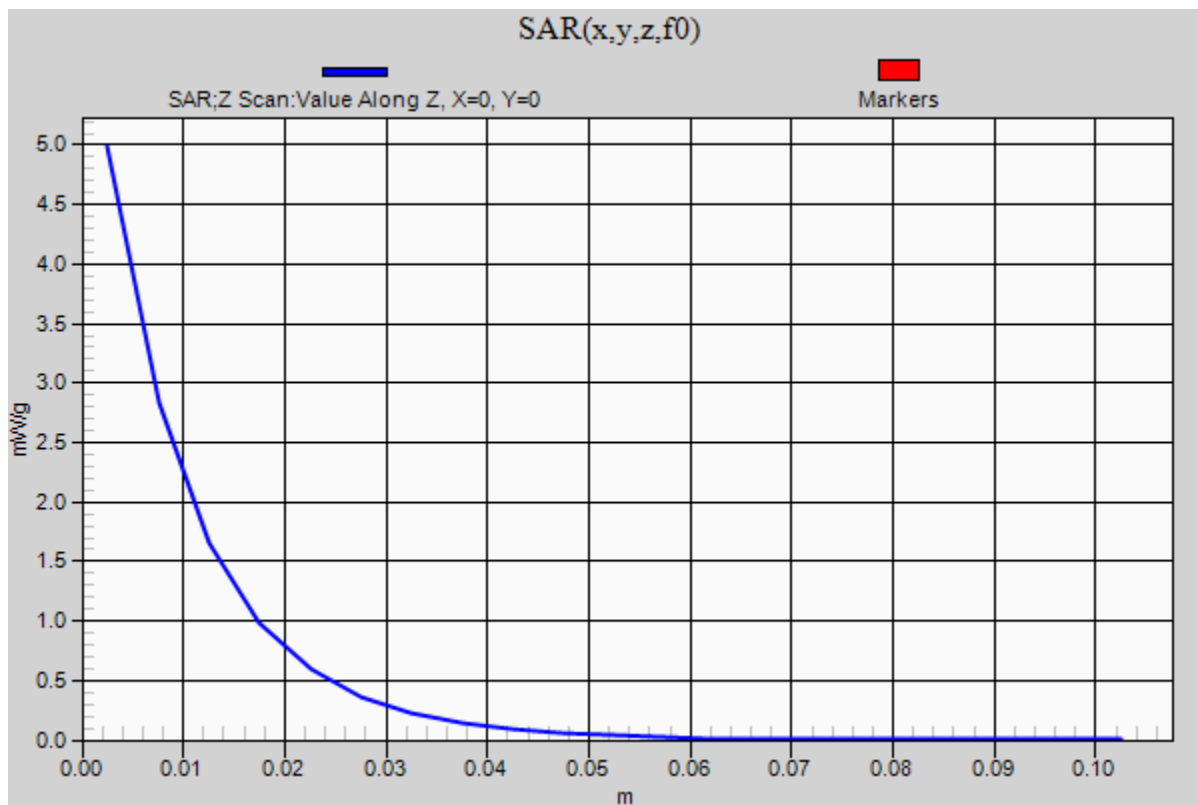D1750V2/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 4.986 mW/g

20120228_SystemPerformanceCheck-D1750V2 SN 1050

Frequency: 1750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
Medium parameters used: $f = 1750$ MHz; $\sigma = 1.47$ mho/m; $\epsilon_r = 50.9$; $\rho = 1000$ kg/m³;

DASY4 Configuration:

- Electronics: DAE3 Sn427; Calibrated: 1/17/2012
- Probe: EX3DV4 - SN3749; ConvF(7.23, 7.23, 7.23); Calibrated: 1/27/2012
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: Flat Phantom ELI4.0; Type: QDOVA001BA; Serial: SN:1003

Body, Pin=100mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 4.15 mW/g


Body, Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 60.4 V/m; Power Drift = -0.023 dB

Peak SAR (extrapolated) = 7.19 W/kg

SAR(1 g) = 3.91 mW/g; SAR(10 g) = 2.06 mW/g

Maximum value of SAR (measured) = 5.26 mW/g

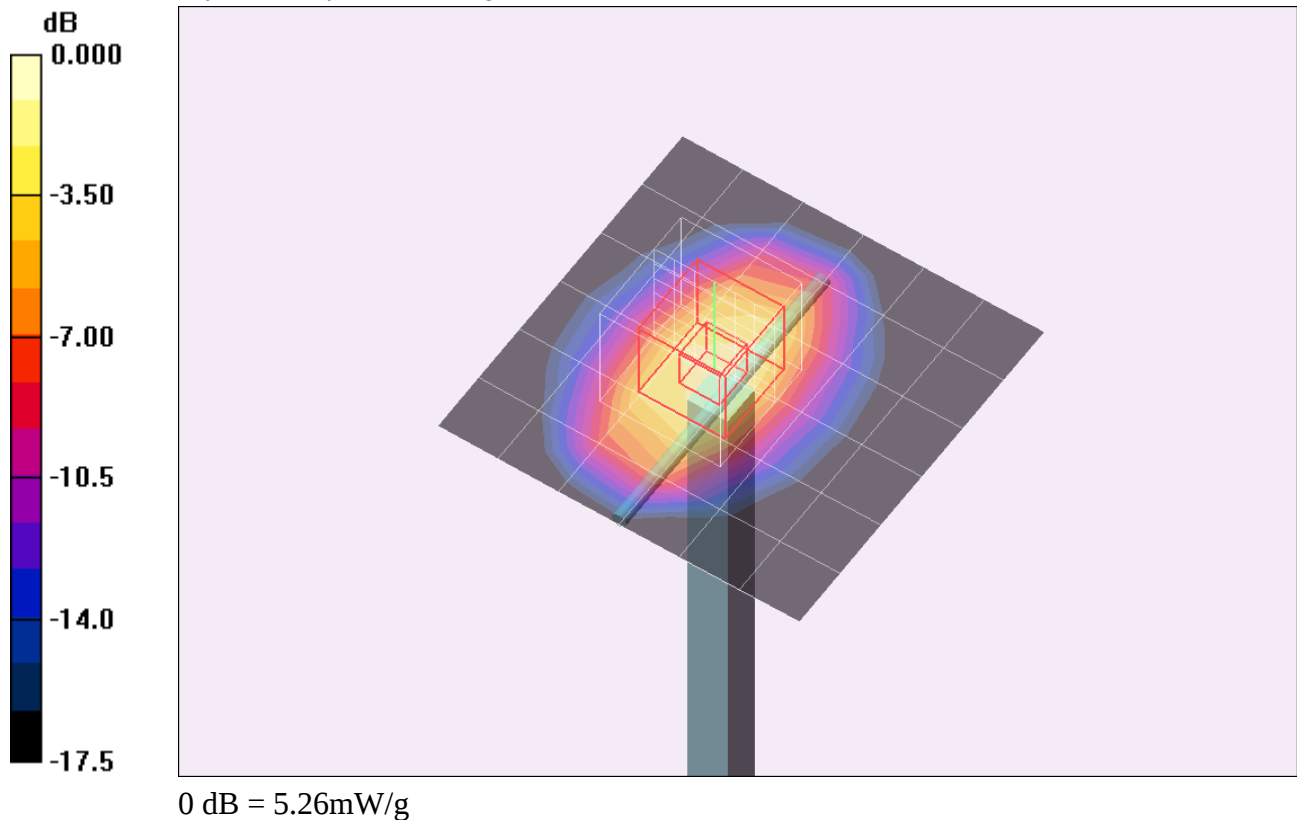

20120228_SystemPerformanceCheck-D1750V2 SN 1050

Frequency: 1750 MHz; Duty Cycle: 1:1

Body, Pin=100mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 5.22 mW/g