

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\text{cond} = 1.83$ S/m; $\text{perm} = 38.7$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/26/2024; Ambient Temp: 21.9°C; Tissue Temp: 23.1°C

Probe: EX3DV4 - SN7499; ConvF:(7.13,7.46,7.69); Calibrated: 2024-01-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1644; Calibrated: 2023-12-07

Phantom: Twin-SAM V8.0; Serial: 1357

Measurement SW: DASY Module SAR V16.2.4.2524

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.3 W/kg

SAR(1 g) = 5.58 W/kg

Deviation (1 g) = 6.08%

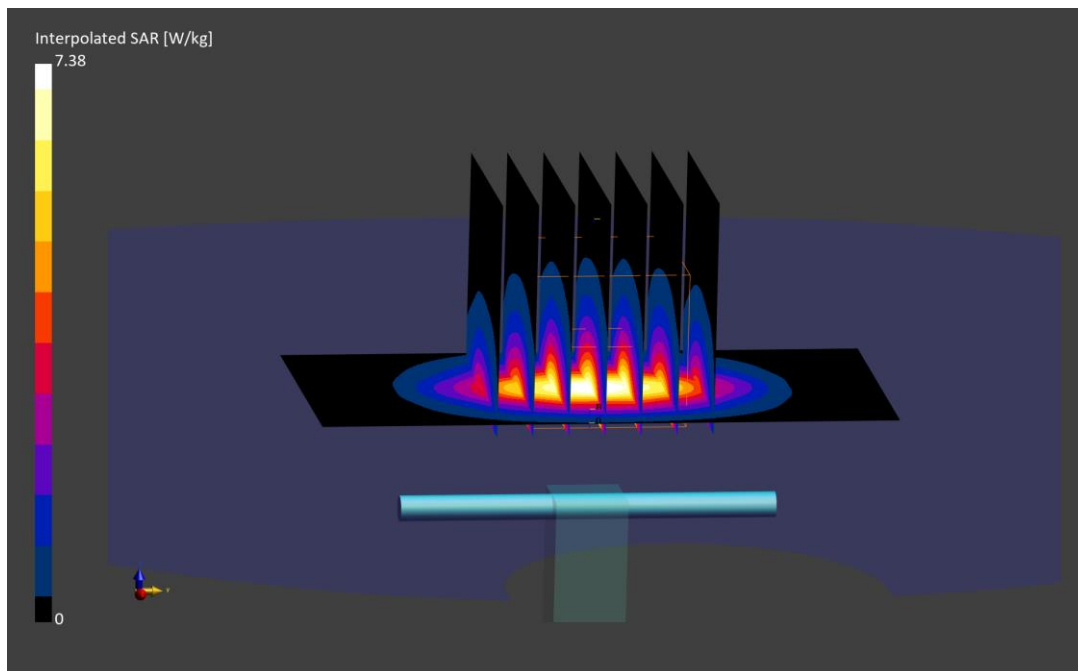

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5250.0$ MHz; $\text{cond} = 4.63$ S/m; $\text{perm} = 35.2$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/02/2024; Ambient Temp: 21.2°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.73,5.26,5.35); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.1 W/kg

SAR(1 g) = 3.82 W/kg

Deviation (1 g) = -3.78%

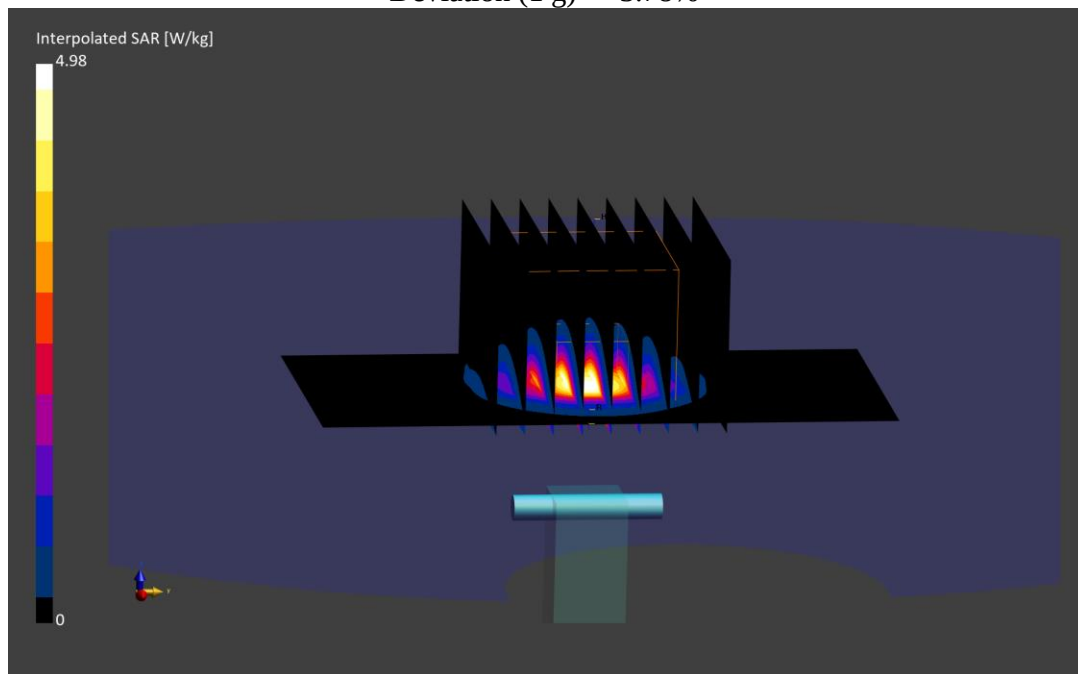

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5250.0$ MHz; $\text{cond} = 4.59$ S/m; $\text{perm} = 34.6$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/13/2024; Ambient Temp: 20.9°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.73,5.26,5.35); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.4 W/kg

SAR(1 g) = 3.86 W/kg

Deviation (1 g) = -3.02%

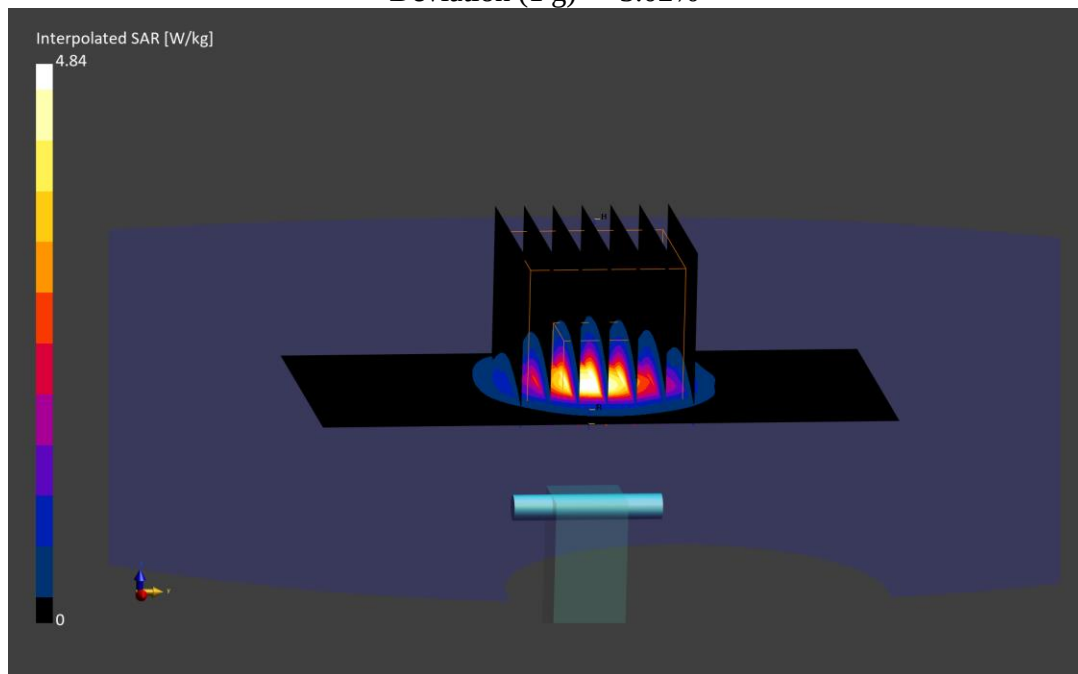

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5600.0$ MHz; $\text{cond} = 5.01$ S/m; $\text{perm} = 34.6$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/02/2024; Ambient Temp: 21.2°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.18,4.62,4.72); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.9 W/kg

SAR(1 g) = 4.08 W/kg

Deviation (1 g) = -1.09%

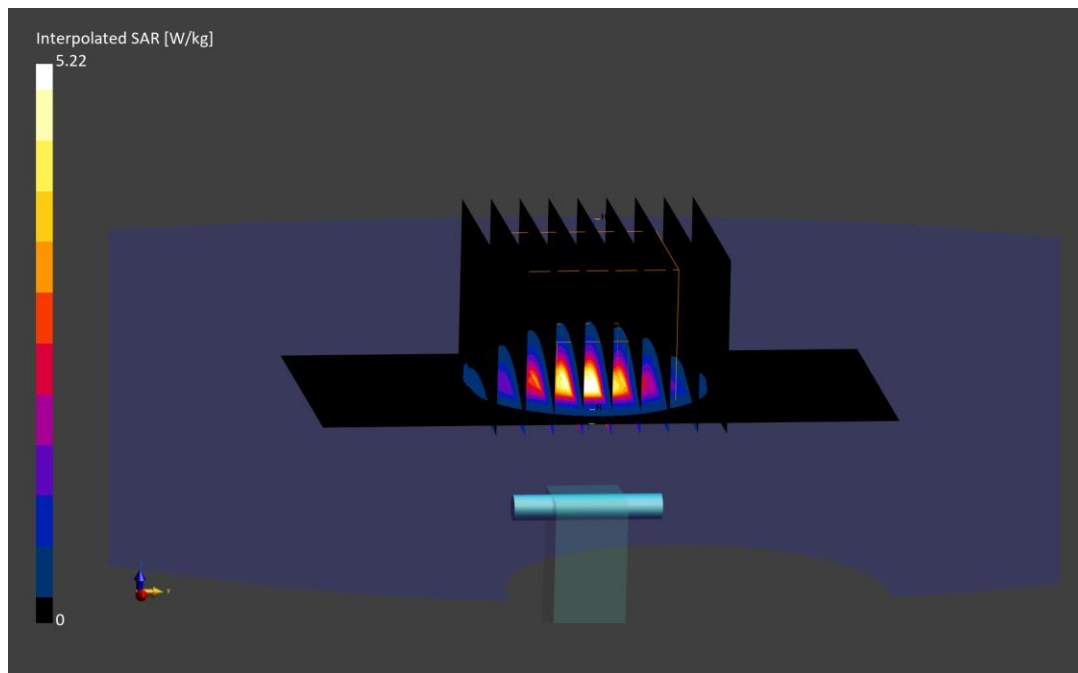

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5600.0$ MHz; $\text{cond} = 4.95$ S/m; $\text{perm} = 34.0$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/13/2024; Ambient Temp: 20.9°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.18,4.62,4.72); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.6 W/kg

SAR(1 g) = 4.22 W/kg

Deviation (1 g) = 1.93%

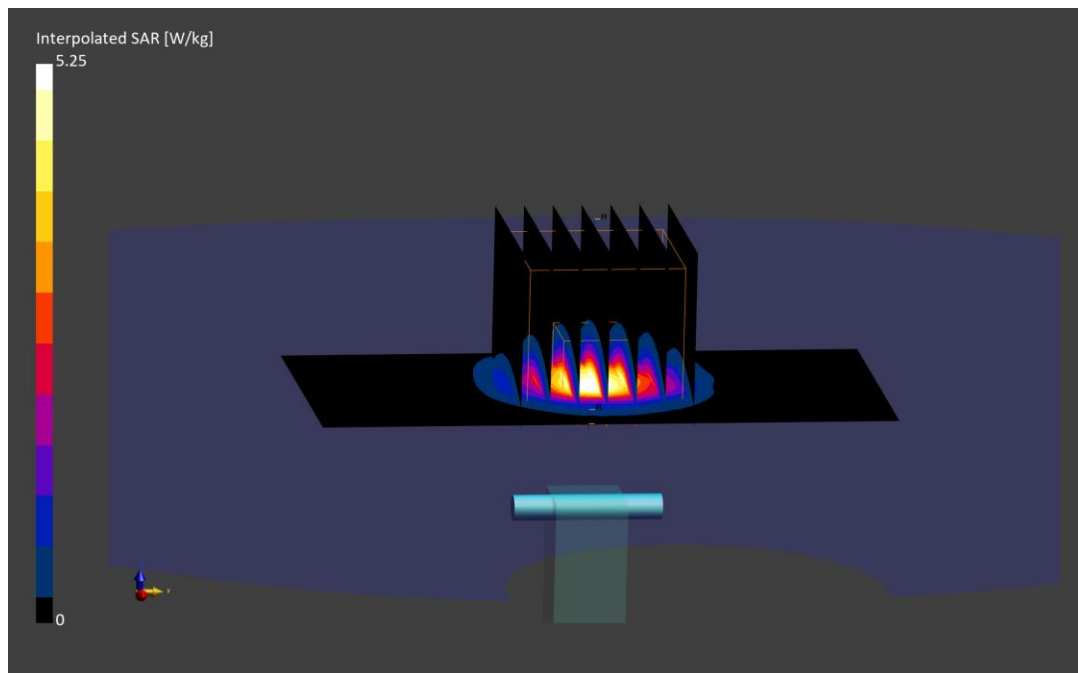

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5750.0$ MHz; $\text{cond} = 5.18$ S/m; $\text{perm} = 34.4$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/02/2024; Ambient Temp: 21.2°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.35,4.78,4.93); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.8 W/kg

SAR(1 g) = 3.69 W/kg

Deviation (1 g) = -7.05%

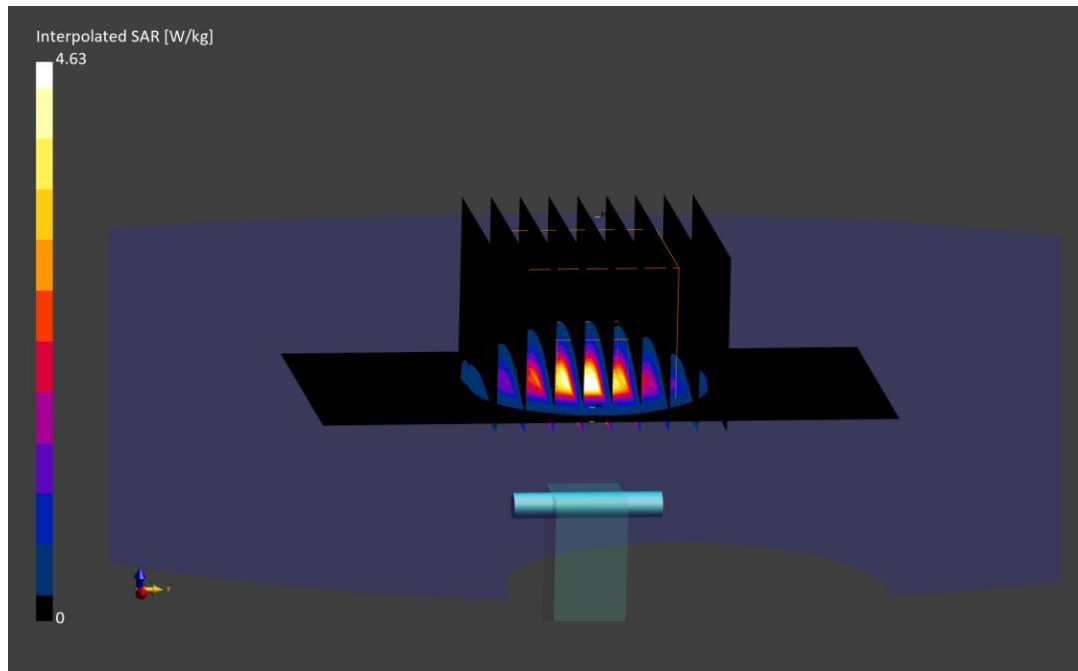

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5750.0$ MHz; $\text{cond} = 5.12$ S/m; $\text{perm} = 33.8$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/13/2024; Ambient Temp: 20.9°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.35,4.78,4.93); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 3.77 W/kg

Deviation (1 g) = -7.03%

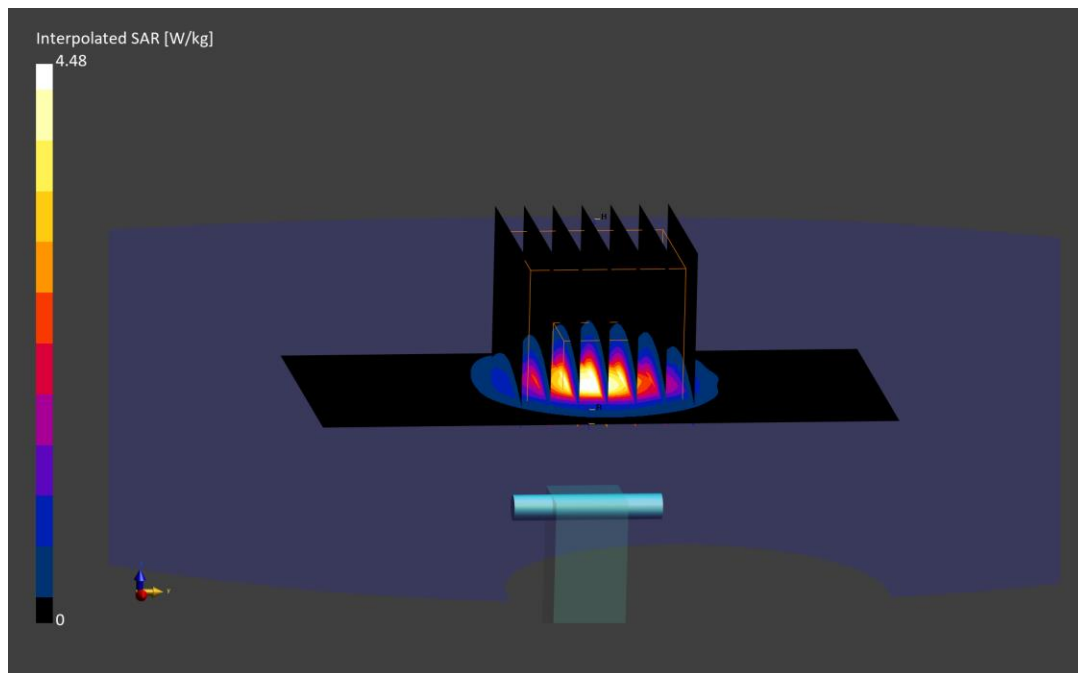

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5850.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5850.0$ MHz; $\text{cond} = 5.29$ S/m; $\text{perm} = 34.2$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/02/2024; Ambient Temp: 21.2°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.04,4.57,4.63); Calibrated: 2024-02-09

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn467; Calibrated: 2024-02-09

Phantom: Twin-SAM V8.0; Serial: 2070

Measurement SW: DASY Module SAR V16.2.4.2524

5850.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.6 W/kg

SAR(1 g) = 4.09 W/kg

Deviation (1 g) = 3.54%

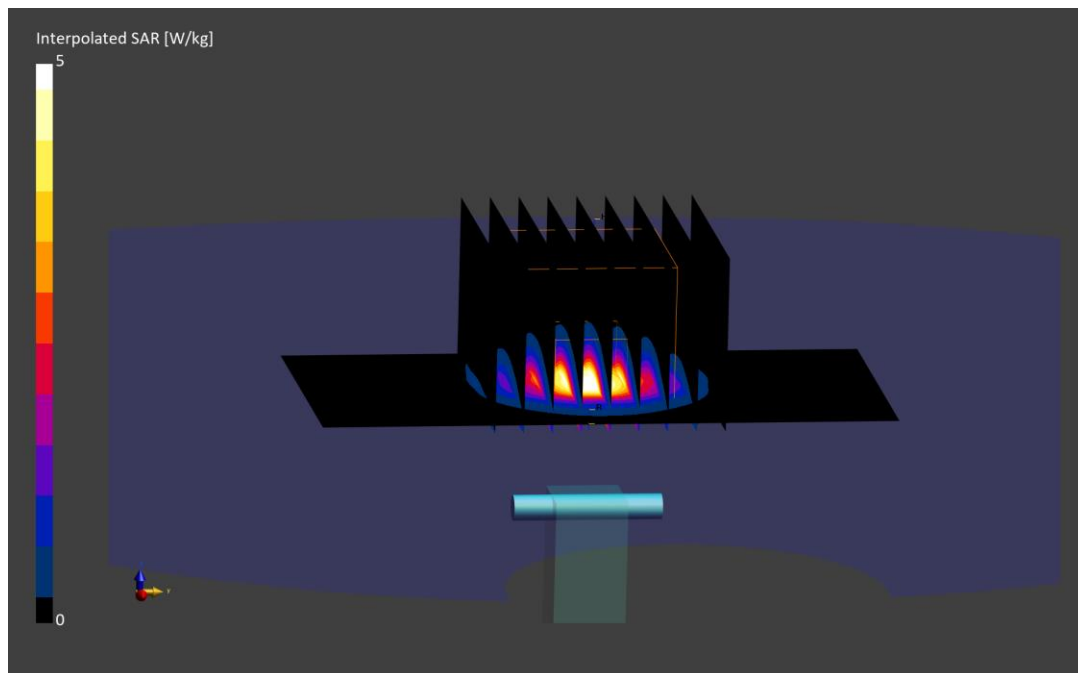

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1163

Communication System: UID: 0, CW; Frequency: 5850.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5850.0$ MHz; $\text{cond} = 5.23$ S/m; $\text{perm} = 33.6$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/13/2024; Ambient Temp: 20.9°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.04,4.57,4.63); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5850.0 MHz System Verification at 17.0 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.2 W/kg

SAR(1 g) = 3.96 W/kg

Deviation (1 g) = 0.25%

