

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

$f = 2450.0$ MHz; $\text{cond} = 1.80$ S/m; $\text{perm} = 38.2$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/24/2024; Ambient Temp: 20.0°C; Tissue Temp: 23.7°C

Probe: EX3DV4 - SN7499; ConvF:(7.13,7.46,7.69); Calibrated: 2024-01-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1644; Calibrated: 2023-12-07

Phantom: Twin-SAM V8.0; Serial: 1357

Measurement SW: DASY Module SAR V16.2.4.2524

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: $dx=5.0$ mm, $dy=5.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

SAR(1 g) = 5.04 W/kg

Deviation (1 g) = -4.18%

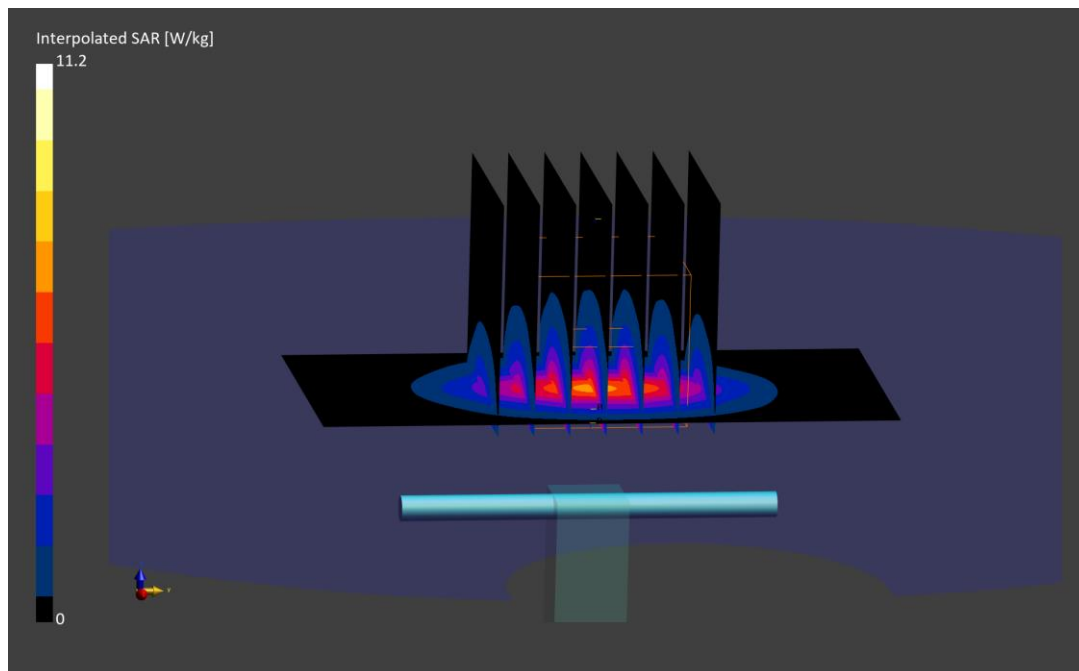

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5250.0$ MHz; $\text{cond} = 4.72$ S/m; $\text{perm} = 35.0$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/08/2024; Ambient Temp: 22.8°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.73,5.26,5.35); Calibrated: 2024-02-09

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn467; Calibrated: 2024-02-09

Phantom: Twin-SAM V8.0; Serial: 2070

Measurement SW: DASY Module SAR V16.2.4.2524

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.4 W/kg

SAR(1 g) = 3.90 W/kg

Deviation (1 g) = -2.86%

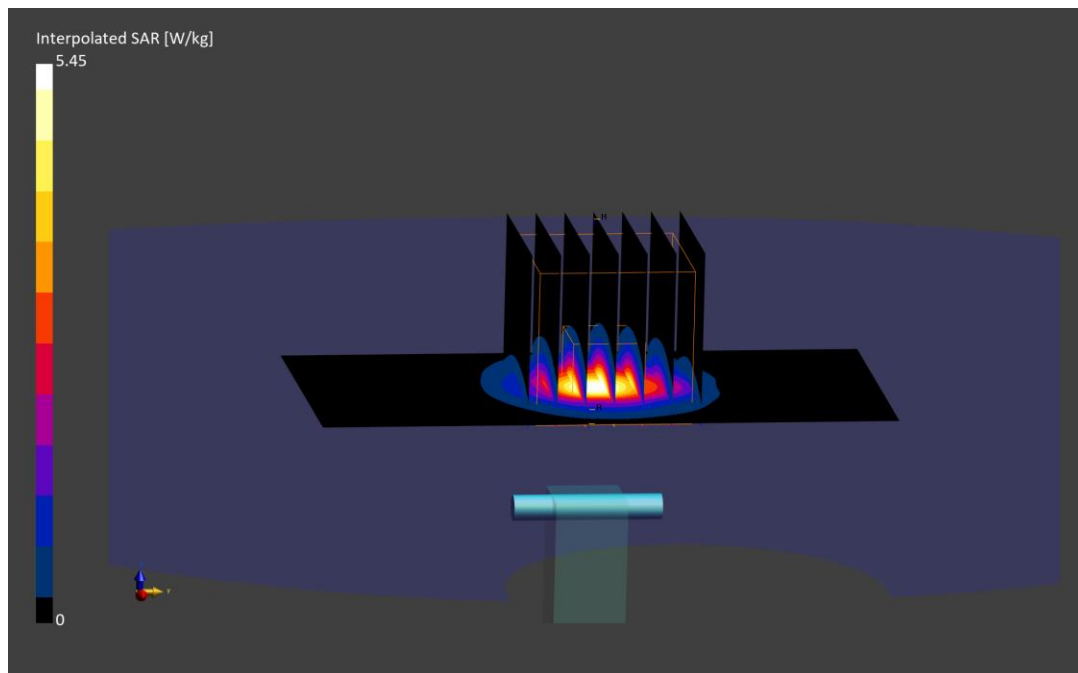

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5600.0$ MHz; $\text{cond} = 5.11$ S/m; $\text{perm} = 34.4$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/08/2024; Ambient Temp: 22.8°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.18,4.62,4.72); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.2 W/kg

SAR(1 g) = 4.12 W/kg

Deviation (1 g) = -1.79%

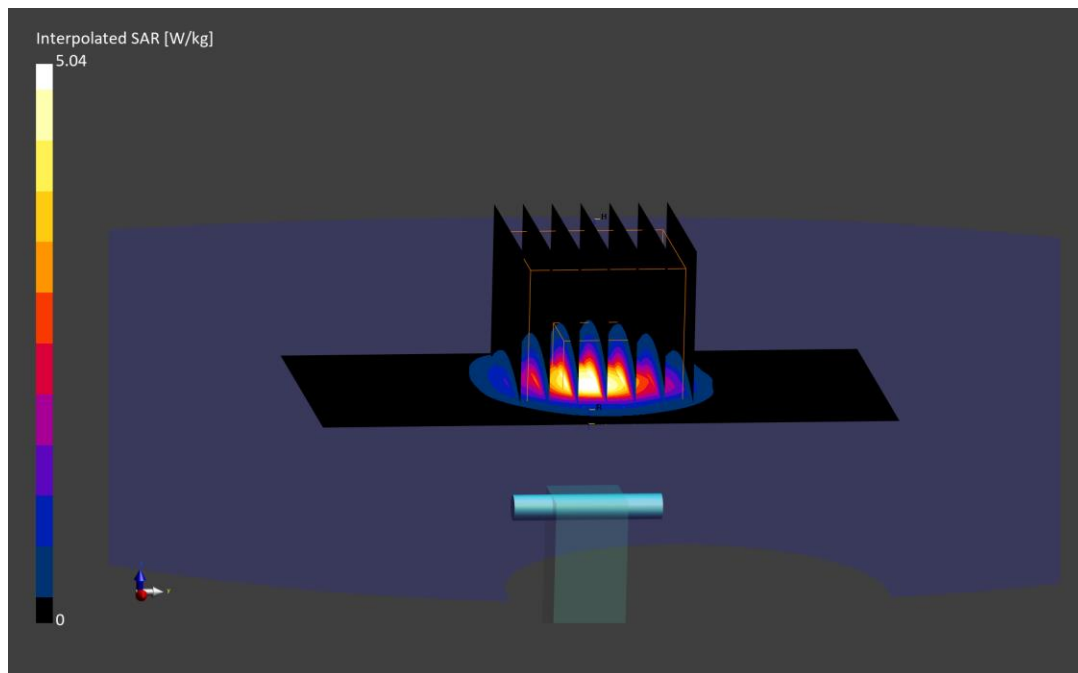

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
 $f = 5750.0$ MHz; $\text{cond} = 5.28$ S/m; $\text{perm} = 34.2$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/08/2024; Ambient Temp: 22.8°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.35,4.78,4.93); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 3.78 W/kg

Deviation (1 g) = -4.91%

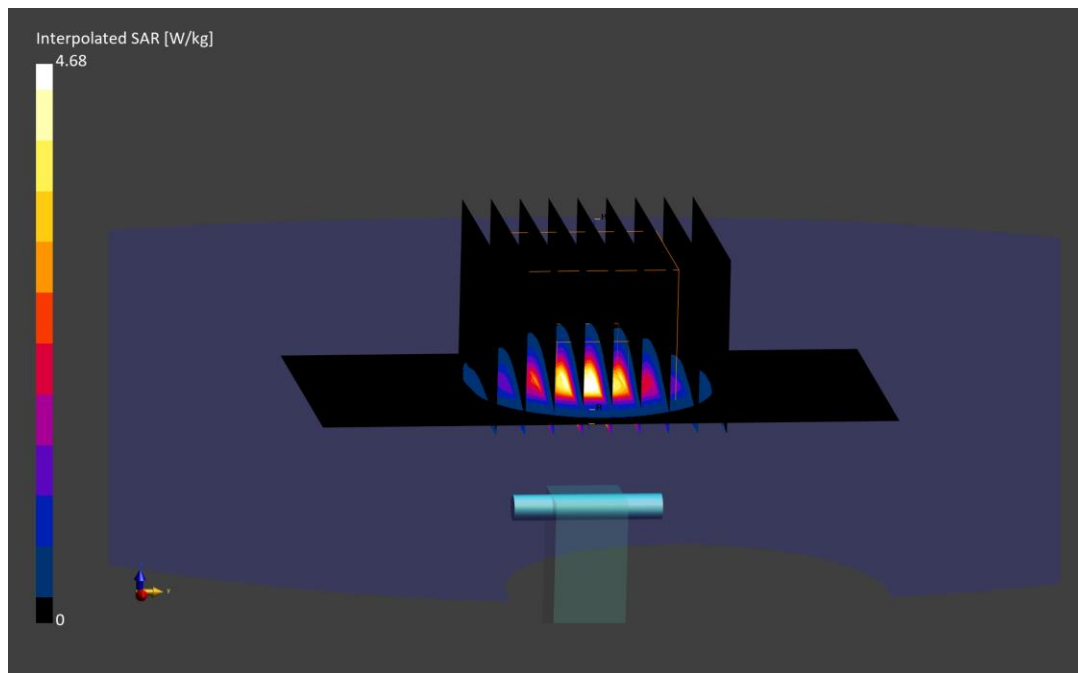

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5850.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

$f = 5850.0$ MHz; $\text{cond} = 5.39$ S/m; $\text{perm} = 34.0$; $\text{density} = 1000$ kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/08/2024; Ambient Temp: 22.8°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7427; ConvF:(4.04,4.57,4.63); Calibrated: 2024-02-09

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn467; Calibrated: 2024-02-09

Phantom: Twin-SAM V8.0; Serial: 2070

Measurement SW: DASY Module SAR V16.2.4.2524

5850.0 MHz System Verification at 17.0 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: $dx=10.0$ mm, $dy=10.0$ mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: $dx=4.0$ mm, $dy=4.0$ mm, $dz=1.4$ mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 3.97 W/kg

Deviation (1 g) = -3.41%

