

**Appendix C**  
**Calibration Files**  
**&**  
**Antenna Information**



## NCL CALIBRATION LABORATORIES

Calibration File No: DC-890  
Project Number: APREL-ALSAS 10U

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

APREL Validation Dipole


Manufacturer: APREL Laboratories  
Part number: ALS-D-5258-S-2  
Frequency: 5.2GHz to 5.8GHz  
Serial No: 5258-235-00802

Customer: APREL

Serial Number: ALS-BB-001

Calibrated: 24<sup>th</sup> May 2008  
Released on: 24<sup>th</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

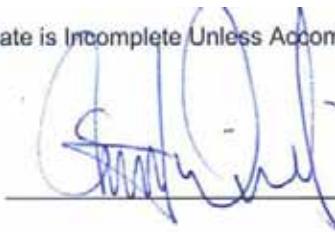Released By: 

**NCL** CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4162

## **NCL Calibration Laboratories**

---


Division of APREL Laboratories.

### **Conditions**

Dipole 5258-235-00802 was new and taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



C. Teodorian

## Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions


**Length:** 23.3 mm  
**Height:** 20.3 mm

### Electrical Specification

**SWR:** 1.22 U  
**Return Loss:** -20.0 dB  
**Impedance:** 50.0  $\Omega$

### System Validation Results


Frequency	1 Gram	10 Gram	Peak
5200 MHz	51.9	17.9	223.1

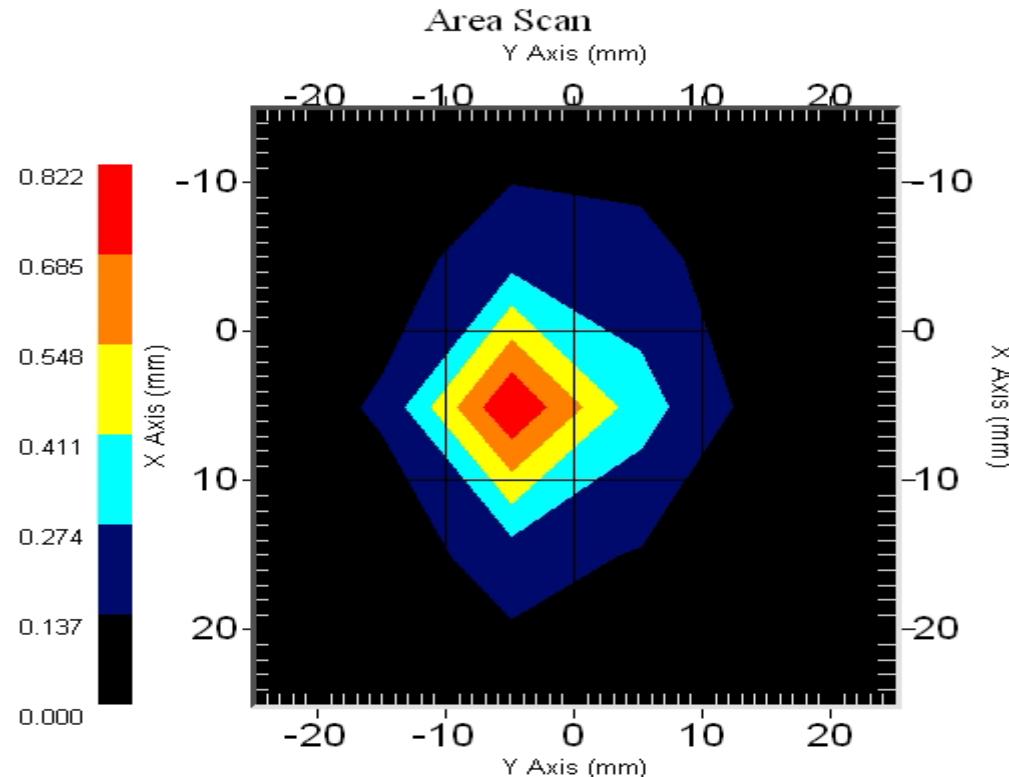

# NCL Calibration Laboratories

Division of APREL Laboratories.


Frequency	1 Gram	10 Gram	Peak
5600 MHz	52.97	18.2	243.1

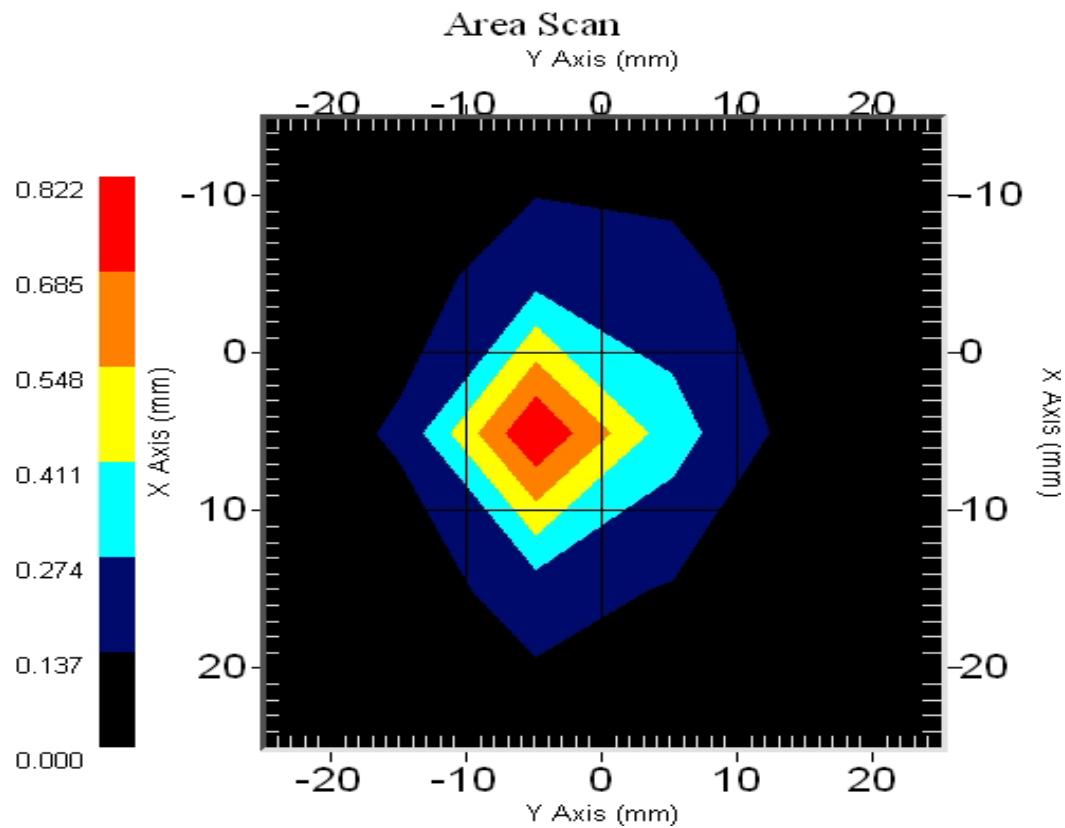

# NCL Calibration Laboratories

Division of APREL Laboratories.

Frequency	1 Gram	10 Gram	Peak
5800 MHz	48.97	17.2	207.1

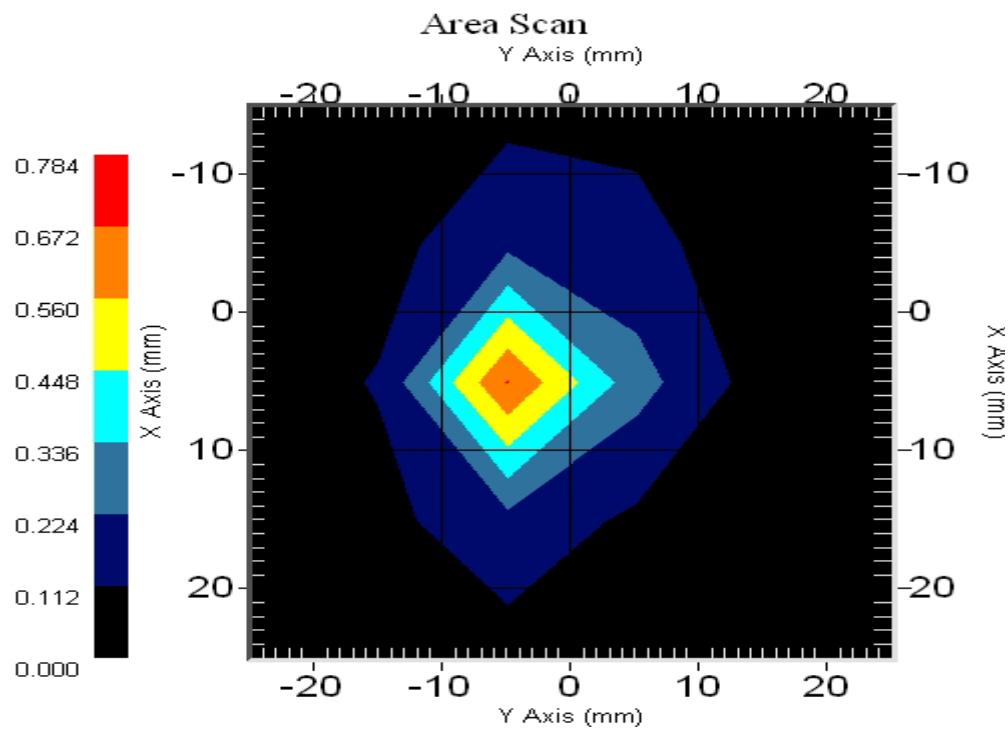

## Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 5258-235-00802. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-030 018 E-Field Probe.

## References

SSI-TP-018-ALSAS Dipole Calibration Procedure

SSI-TP-016 Tissue Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

## Conditions

Dipole 5258-235-00802 was new taken from stock.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C

**Temperature of the Tissue:** 20 °C +/- 0.5°C

# **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Dipole Calibration Results**

### **Tissue Validation**

<b>Head Tissue 5200 MHz</b>	<b>Measured</b>
<b>Dielectric constant, <math>\epsilon_r</math></b>	47.0
<b>Conductivity, <math>\sigma</math> [S/m]</b>	5.30

<b>Head Tissue 5600 MHz</b>	<b>Measured</b>
<b>Dielectric constant, <math>\epsilon_r</math></b>	46.1
<b>Conductivity, <math>\sigma</math> [S/m]</b>	5.78

<b>Head Tissue 5800 MHz</b>	<b>Measured</b>
<b>Dielectric constant, <math>\epsilon_r</math></b>	46.7
<b>Conductivity, <math>\sigma</math> [S/m]</b>	6.22

### **Mechanical Verification**

<b>APREL Length</b>	<b>APREL Height</b>	<b>Measured Length</b>	<b>Measured Height</b>
23.1 mm	20.7 mm	23.3 mm	20.3 mm

### **Electrical Calibration**

<b>S11</b>	<b>5200MHz</b>	<b>5800MHz</b>
<b>RL (dB)</b>	-21.16	-22.34
<b>SWR</b>	1.2	1.17
<b>Impedance (ohms)</b>	51.38	43.92

The Following Graphs are the results as displayed on the Vector Network Analyzer.


**S11 Parameter Return Loss**

S22 REVERSE REFLECTION

LOG MAGNITUDE

REF = -20.000 dB

5.000 dB/DIV

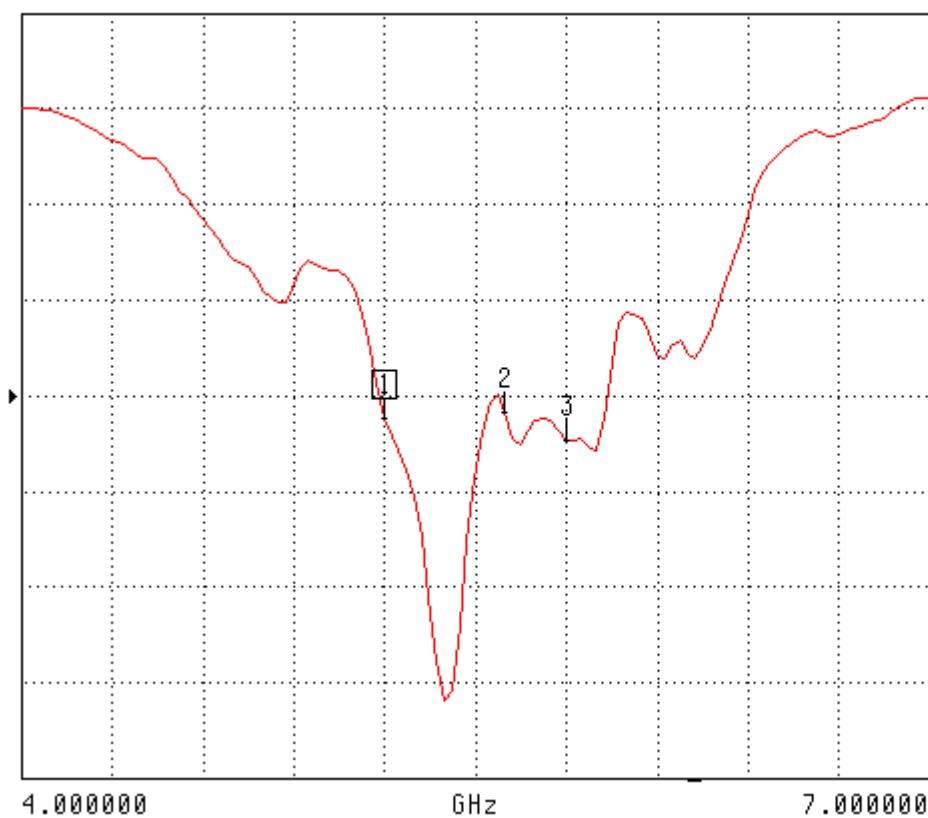CH 4 - S22  
REFERENCE PLANE  
0.0000 mmMARKER 1  
5.200000 GHz  
-21.160 dBMARKER TO MAX  
► MARKER TO MIN2 5.600000 GHz  
-20.906 dB3 5.800000 GHz  
-22.337 dBMARKER READOUT  
FUNCTIONS


## SWR

S22 REVERSE REFLECTION

SWR

►REF=2.500 U

500.000 mU/DIV

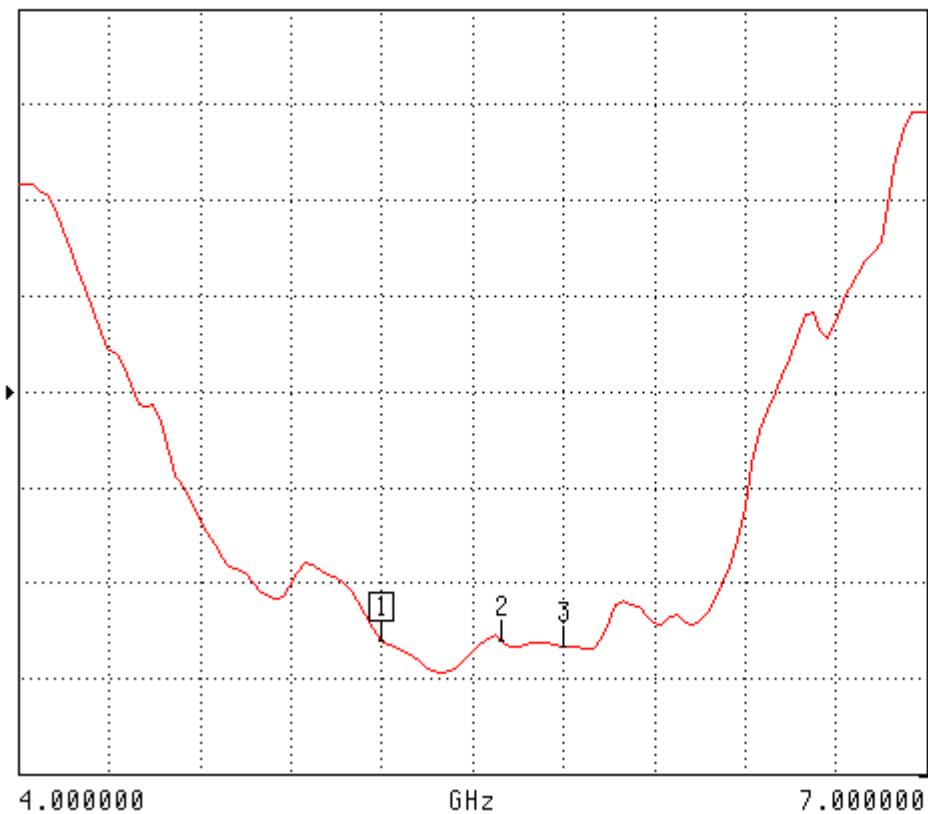

CH 4 - S22  
REFERENCE PLANE  
0.0000 mm

MARKER 1  
5.200000 GHz  
1.199 U


► MARKER TO MAX  
► MARKER TO MIN

2 5.600000 GHz  
1.200 U

3 5.800000 GHz  
1.165 U

MARKER READOUT  
FUNCTIONS

## Smith Chart Dipole Impedance

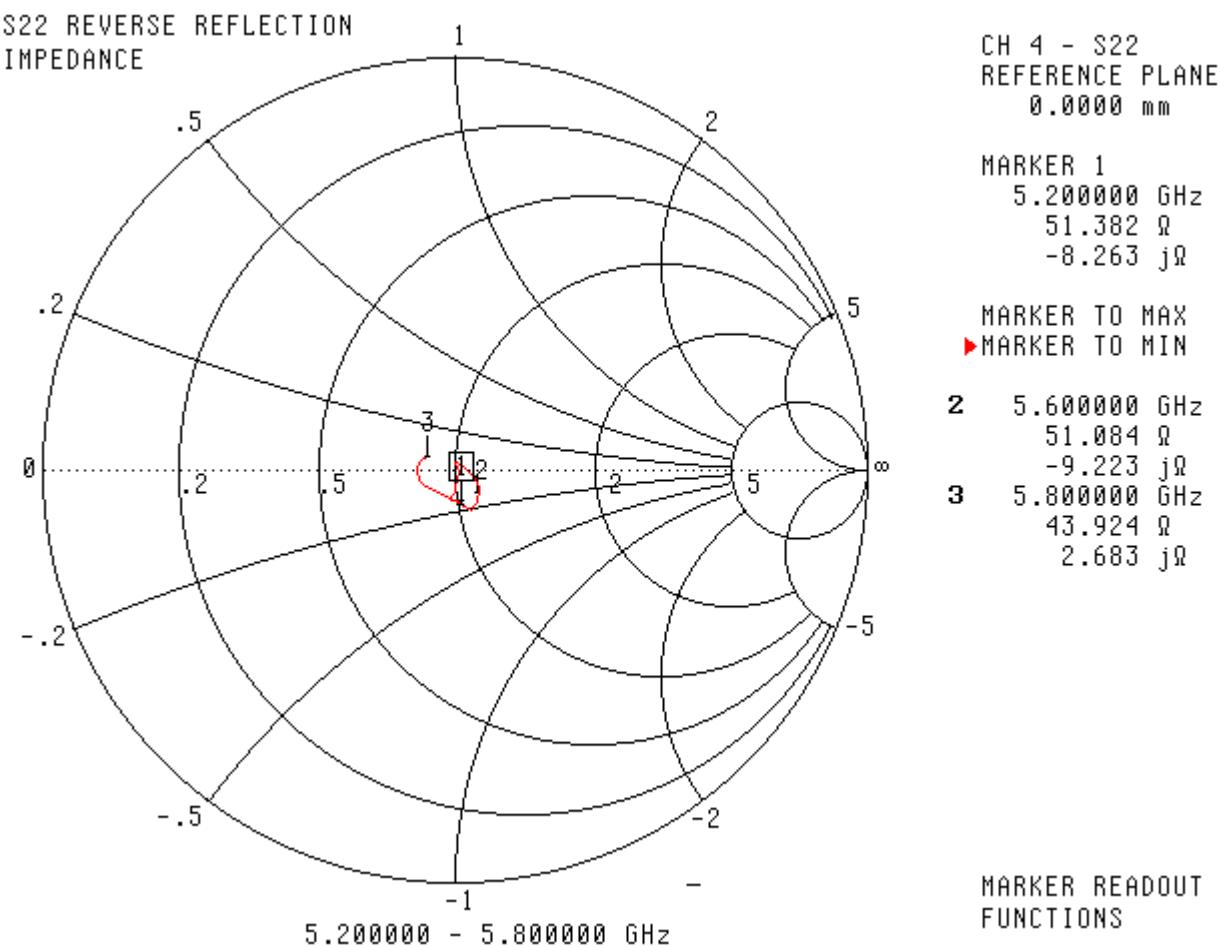

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

## NCL CALIBRATION LABORATORIES

Calibration File No: DC-889  
Project Number: APREL-ALSAS10U

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

APREL Validation Dipole

Manufacturer: APREL Laboratories

Part number: ALS-D-2450-S-2

Frequency: 2450 MHz


Serial No: 301581

Customer: APREL

Calibrated: 4<sup>th</sup> May 2008  
Released on: 4<sup>th</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

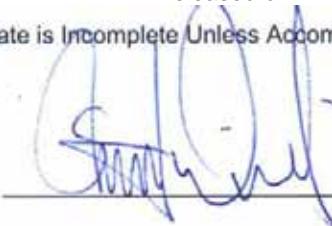

## NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4162

## **NCL Calibration Laboratories**

---


Division of APREL Laboratories.

### **Conditions**

Dipole 301581 was new and taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



C. Teodorian

## Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

## Mechanical Dimensions


**Length:** 52.4 mm  
**Height:** 30.3 mm

## Electrical Specification

**SWR:** 1.056 U  
**Return Loss:** -32.0 dB  
**Impedance:** 50.2  $\Omega$

## System Validation Results

Frequency	1 Gram	10 Gram	Peak
2450 MHz	53.1	24.4	101.8

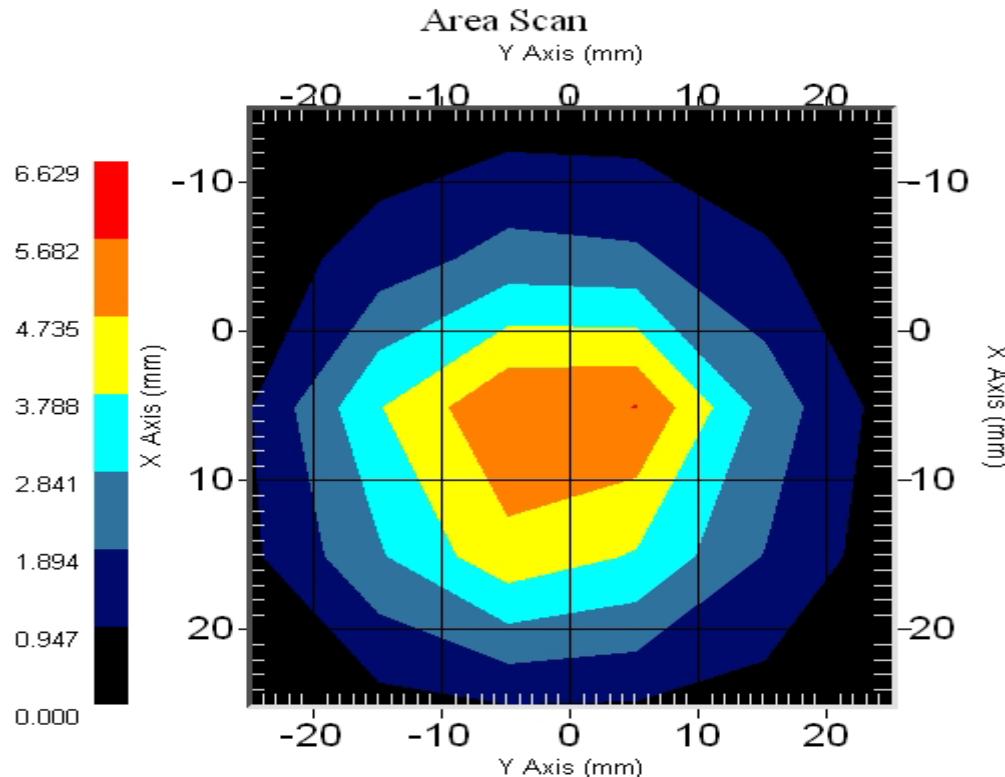

## Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 301581. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

## References

SSI-TP-018-ALSAS Dipole Calibration Procedure

SSI-TP-016 Tissue Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

IEC-62209 "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures"

Part 1: "Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity of the ear (frequency range of 300 MHz to 3 GHz)"

IEC-62209 "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures"

Part 2 *Draft*: "Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity of the ear (frequency range of 30 MHz to 6 GHz)"

## Conditions

Dipole 301581 was new taken from stock.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 20 °C +/- 0.5°C

## **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Dipole Calibration Results**

### **Mechanical Verification**

<b>APREL Length</b>	<b>APREL Height</b>	<b>Measured Length</b>	<b>Measured Height</b>
51.5 mm	30.4 mm	52.4 mm	30.3 mm

### **Tissue Validation**

<b>Head Tissue 2450 MHz</b>	<b>Measured</b>
<b>Dielectric constant, <math>\epsilon_r</math></b>	39.2
<b>Conductivity, <math>\sigma</math> [S/m]</b>	1.80

# NCL Calibration Laboratories


Division of APREL Laboratories.

## Electrical Calibration

Test	Result
S11 R/L	-32.0 dB
SWR	1.05 U
Impedance	50.2 $\Omega$

The Following Graphs are the results as displayed on the Vector Network Analyzer.

### S11 Parameter Return Loss

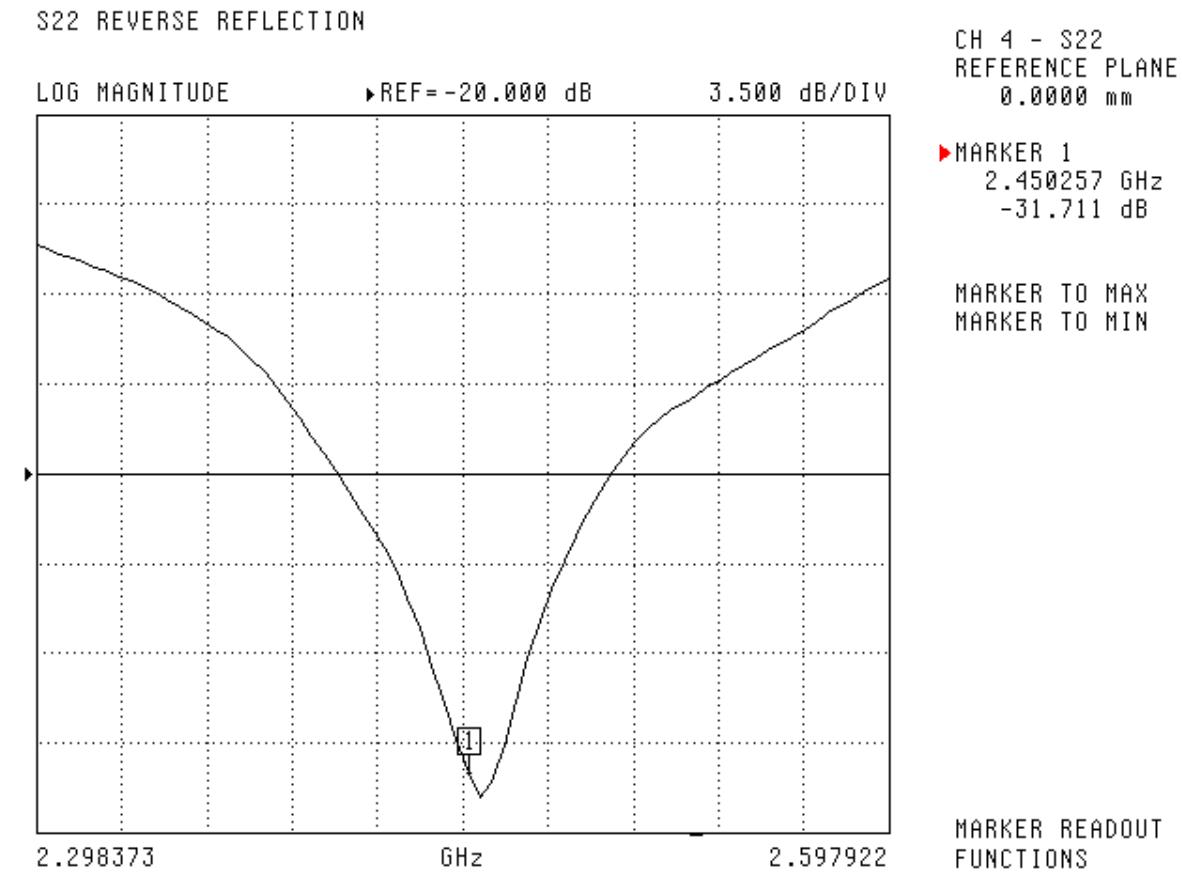

# NCL Calibration Laboratories

Division of APREL Laboratories.


## SWR

S22 REVERSE REFLECTION

SWR

►REF= 1.100 U

100.000 mU/DIV

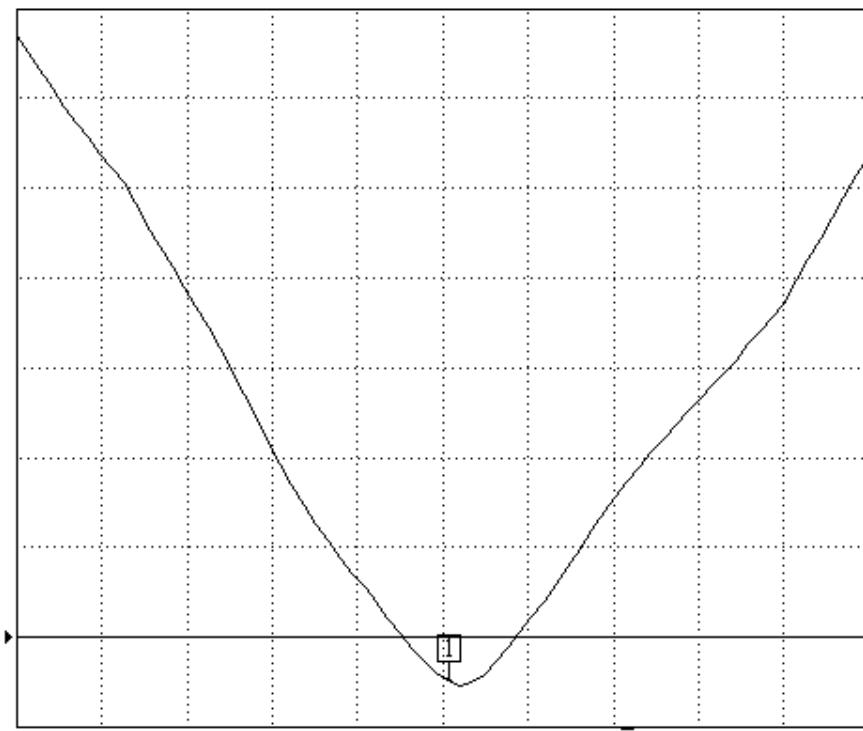


CH 4 - S22  
REFERENCE PLANE  
0.0000 mm

►MARKER 1  
2.450257 GHz  
1.051 U

MARKER TO MAX  
MARKER TO MIN


MARKER READOUT  
FUNCTIONS

## Smith Chart Dipole Impedance

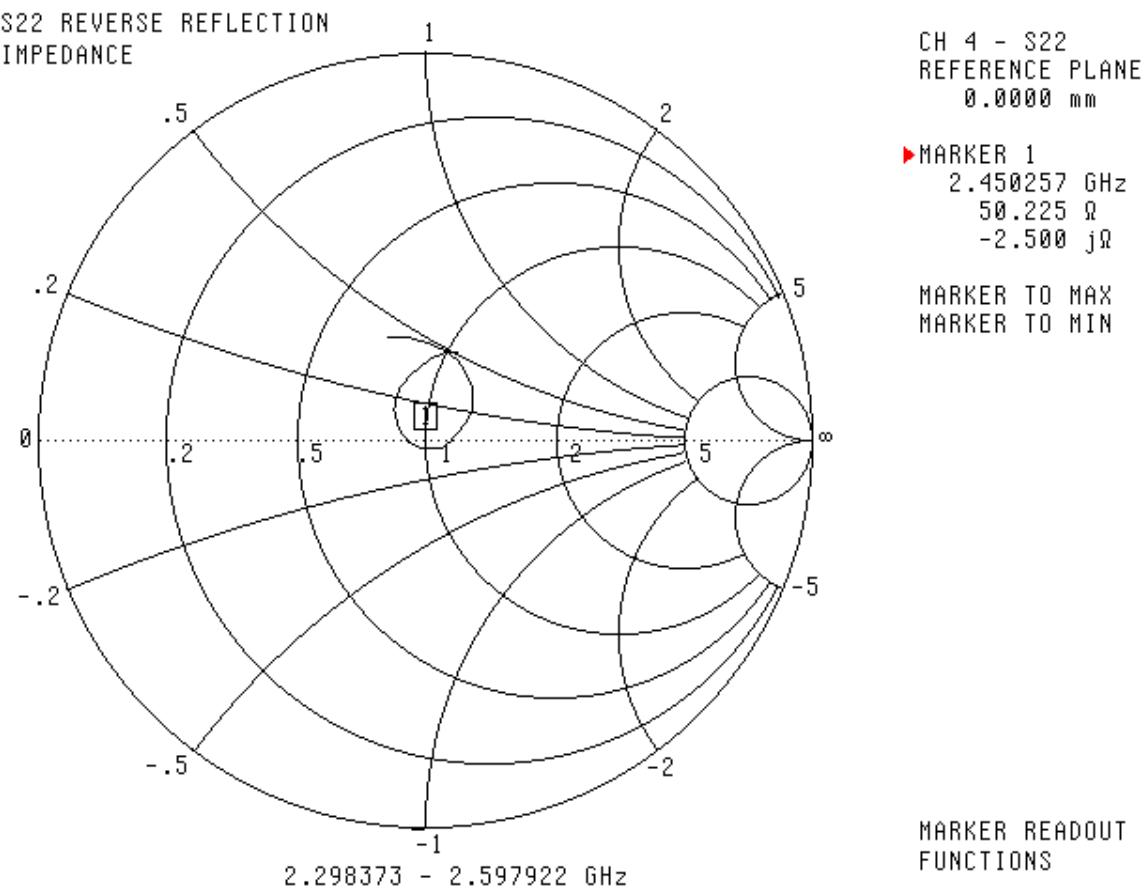

## System Validation Results Using the Electrically Calibrated Dipole

Frequency	1 Gram	10 Gram	Peak
2450 MHz	53.1	24.4	101.8

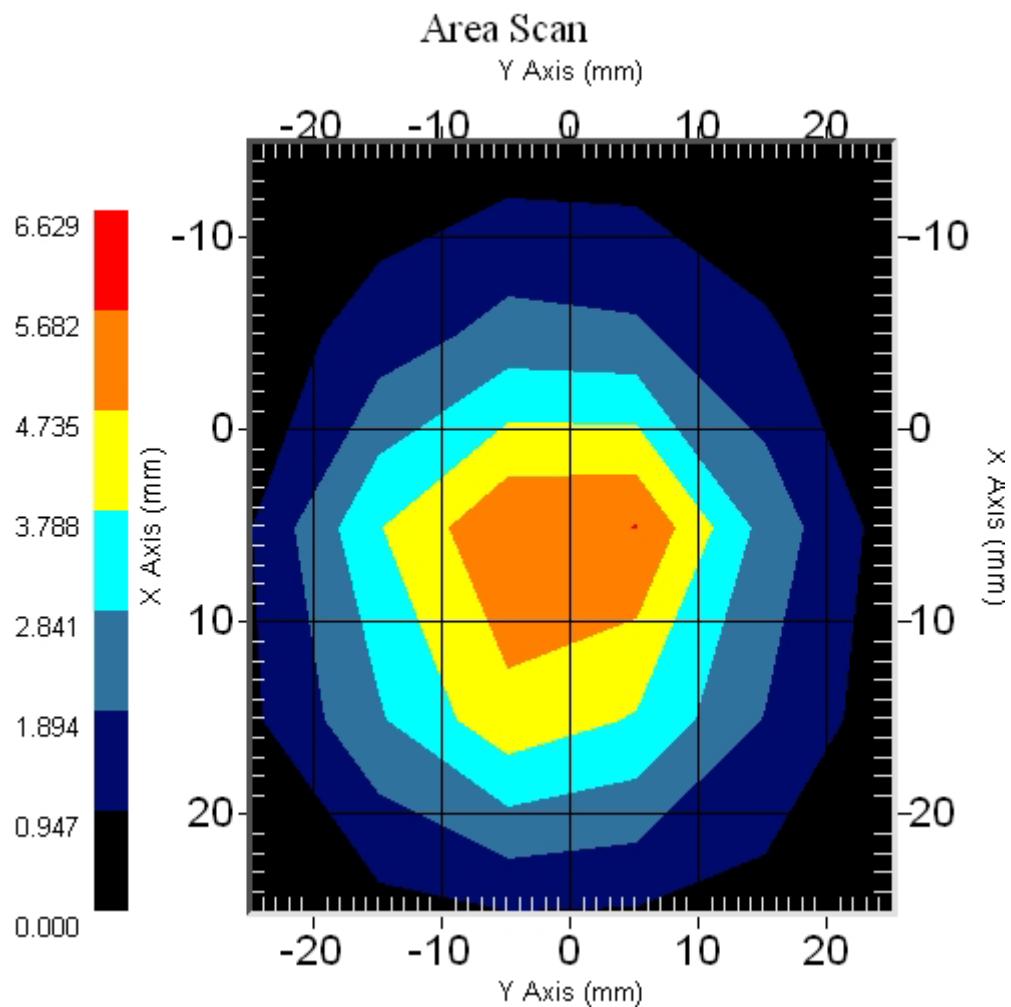

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-887

Client.: APREL

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5600 MHz

Manufacturer: APREL Laboratories

Model No.: E-030

Serial No.: 018

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: Internal APREL

Calibrated: 3<sup>rd</sup> May 2008  
Released on: 3<sup>rd</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-030 018.

## **References**

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure

## **Conditions**

Probe 018 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**

Stuart Nicol

Jesse Hones

## Calibration Results Summary

**Probe Type:** E-Field Probe E-030

**Serial Number:** 018

**Frequency:** 5600 MHz

**Sensor Offset:** 0.44 mm

**Sensor Length:** 2.5 mm

**Tip Enclosure:** Ertalyte\*

**Tip Diameter:** <2.9 mm

**Tip Length:** 60 mm

**Total Length:** 290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

### Sensitivity in Air

**Channel X:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Channel Y:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Channel Z:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Diode Compression Point:** 95 mV

**Sensitivity in Body Tissue Measured****Frequency:** 5600 MHz**Epsilon:** 46.0 (+/-10%) **Sigma:** 5.85 S/m (+/-10%)**ConvF****Channel X:** 3.3**Channel Y:** 3.3**Channel Z:** 3.3

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

**Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

**Spatial Resolution:**


The measured probe tip diameter is 2.9 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.



**Broad Band Calibration:**

The probe was assessed for sensitivity and conversion factor using a +/- 40MHz deviation from the centre frequency.

**Deviation at -40MHz:** -3.77%**Deviation at +40MHz:** +4.28%


## Receiving Pattern 5600 MHz (Air)

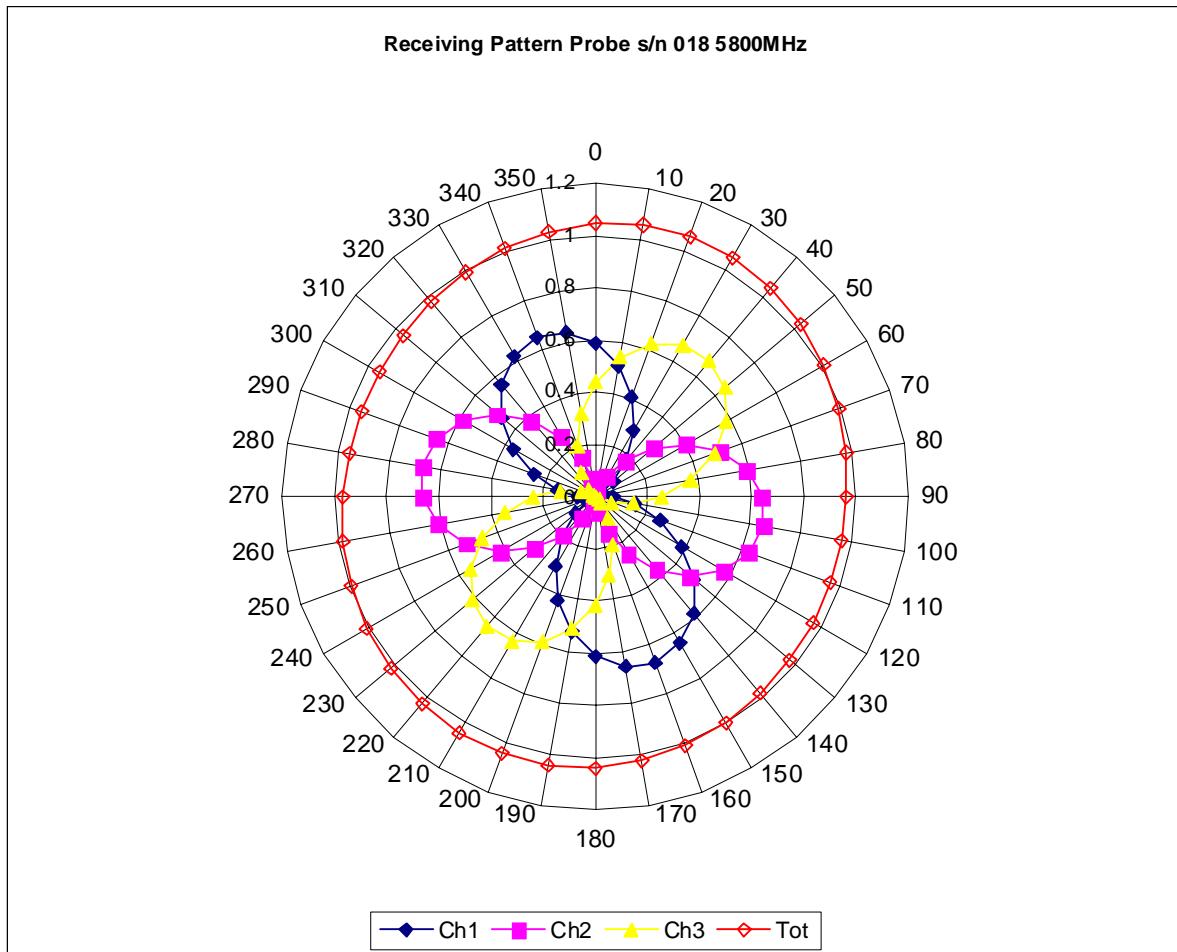

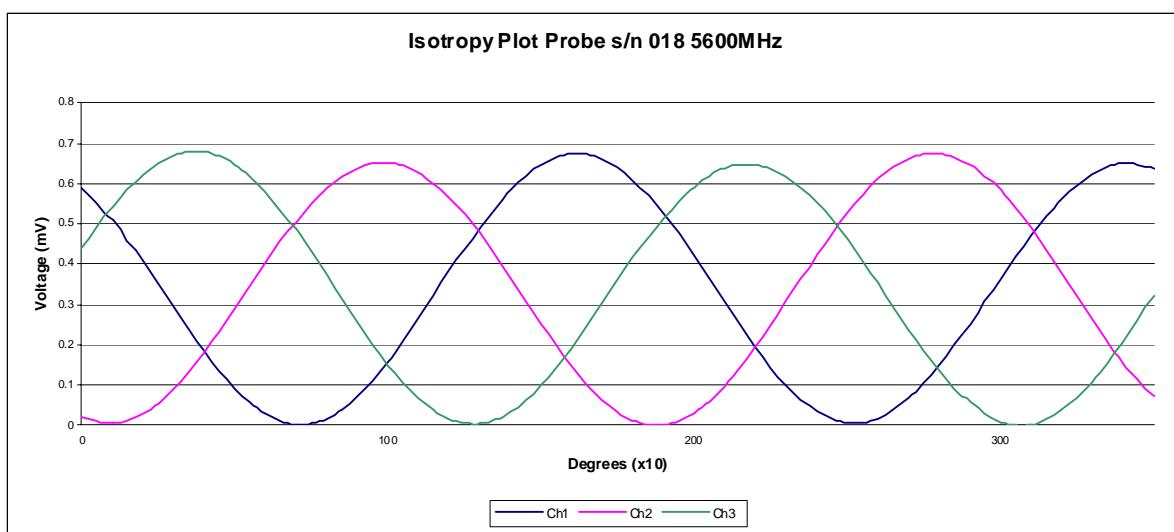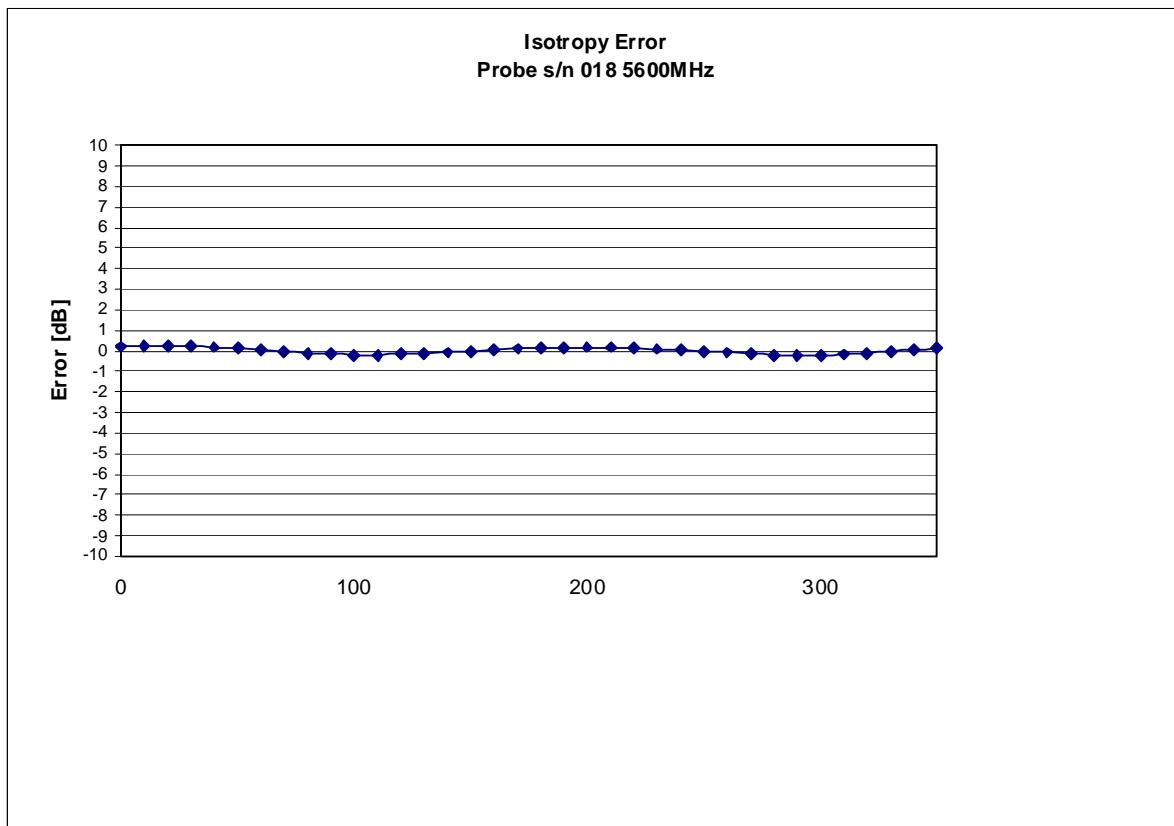
**Isotropy Error 5600 MHz (Air)****Isotropicity in Tissue:**

0.10 dB

## Dynamic Range

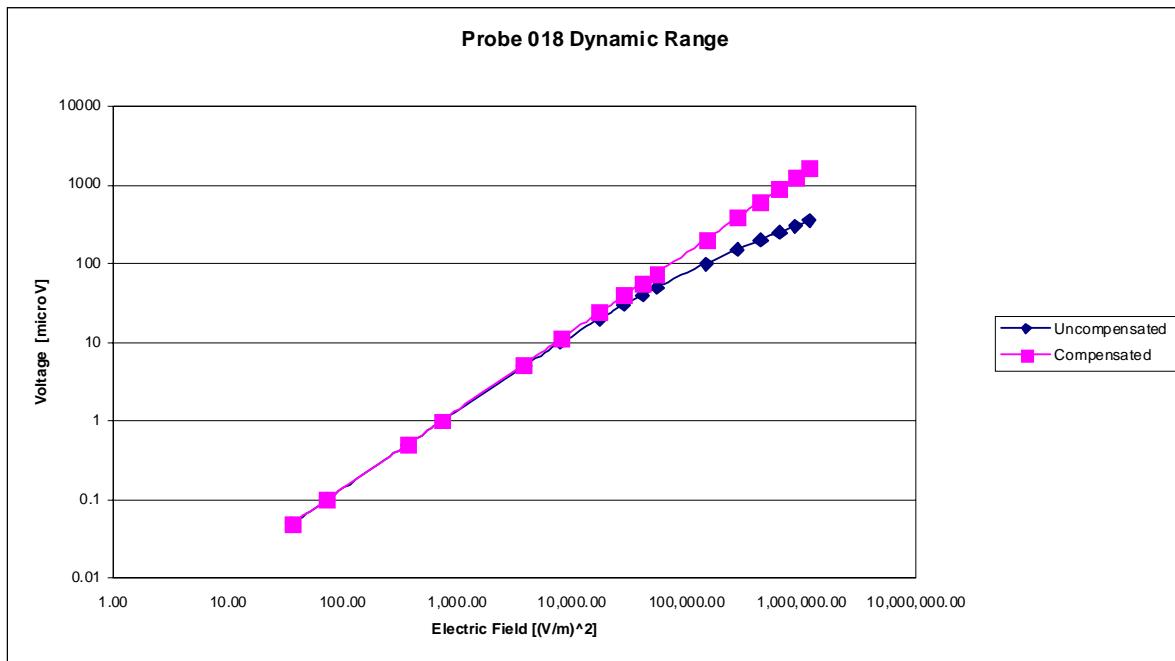

## Video Bandwidth

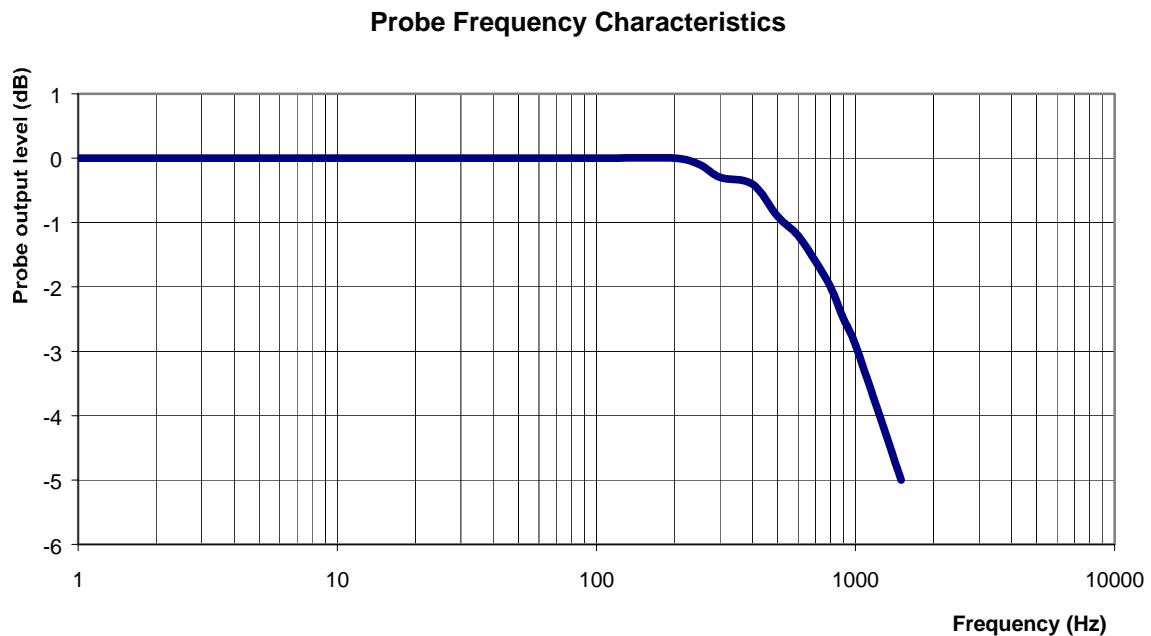

**Video Bandwidth at 500 Hz** 1 dB  
**Video Bandwidth at 1.02 KHz:** 3 dB

## **Conversion Factor Uncertainty Assessment**

### **Sensitivity in Body Tissue Measured**

**Frequency:** 5600 MHz

**Epsilon:** 46.0 (+/-10%) **Sigma:** 5.85 S/m (+/-10%)

#### **ConvF**

**Channel X:** 3.3 7%(K=2)

**Channel Y:** 3.3 7%(K=2)

**Channel Z:** 3.3 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

#### **Boundary Effect:**

For a distance of 0.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-886

Client.: APREL

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5200 MHz

Manufacturer: APREL Laboratories

Model No.: E-030

Serial No.: 018

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: Internal APREL

Calibrated: 3<sup>rd</sup> May 2008  
Released on: 3<sup>rd</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-030 018.

## **References**

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure

## **Conditions**

Probe 018 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**

Stuart Nicol

Jesse Hones

## Calibration Results Summary

**Probe Type:** E-Field Probe E-030

**Serial Number:** 018

**Frequency:** 5200 MHz

**Sensor Offset:** 0.44 mm

**Sensor Length:** 2.5 mm

**Tip Enclosure:** Ertalyte\*

**Tip Diameter:** <2.9 mm

**Tip Length:** 60 mm

**Total Length:** 290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

### Sensitivity in Air

**Channel X:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Channel Y:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Channel Z:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Diode Compression Point:** 95 mV

## **Sensitivity in Body Tissue**

**Frequency:** 5200 MHz

**Epsilon:** 43.0 (+/-10%) **Sigma:** 5.75 S/m (+/-10%)

### **ConvF**

**Channel X:** 3.2

**Channel Y:** 3.2

**Channel Z:** 3.2

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

### **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

### **Spatial Resolution:**

The measured probe tip diameter is 2.9 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


### **Broad Band Calibration:**



The probe was assessed for sensitivity and conversion factor using a +/- 40MHz deviation from the centre frequency.

**Deviation at -40MHz:** -4.16%

**Deviation at +40MHz:** +2.78%


## Receiving Pattern 5200 MHz (Air)

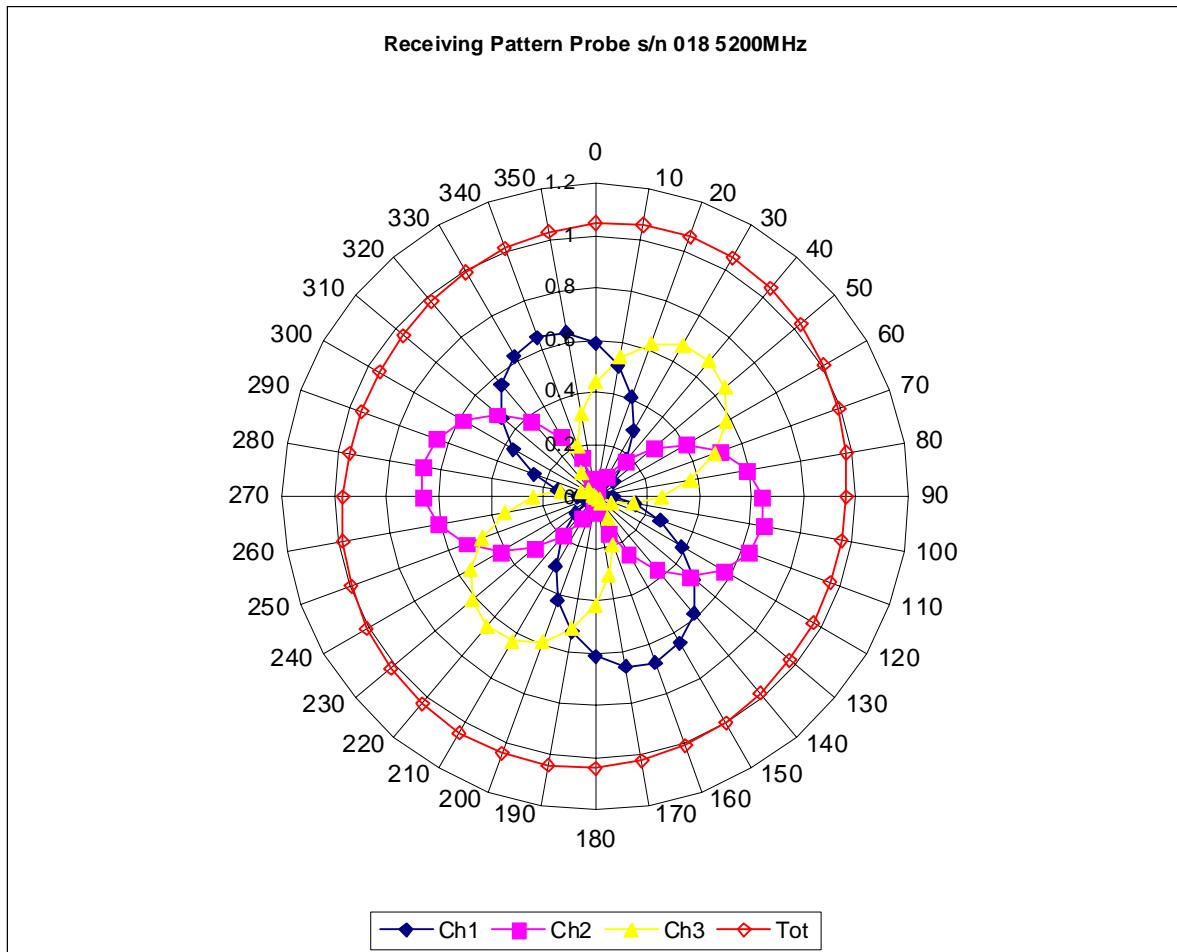

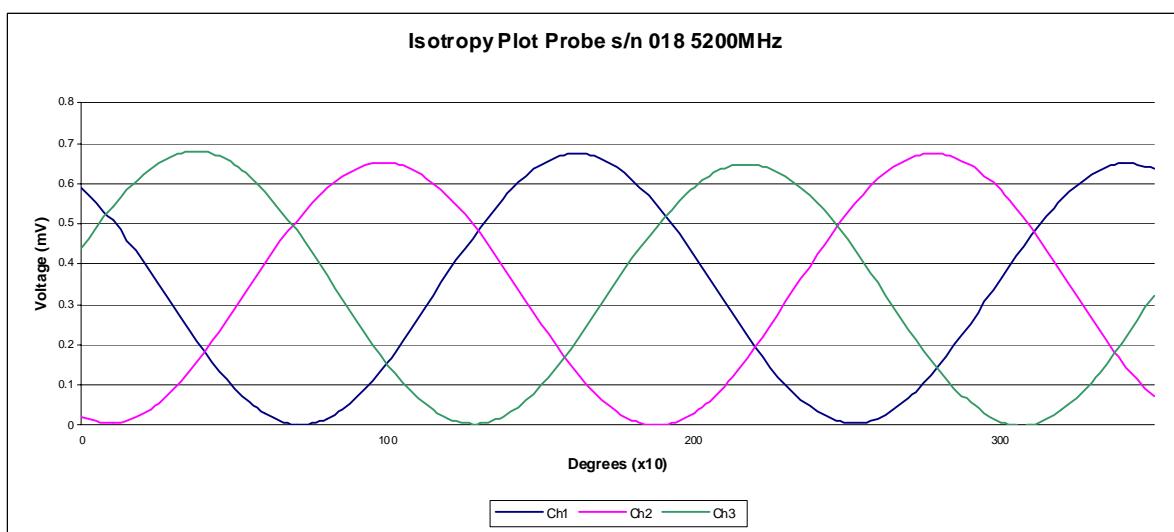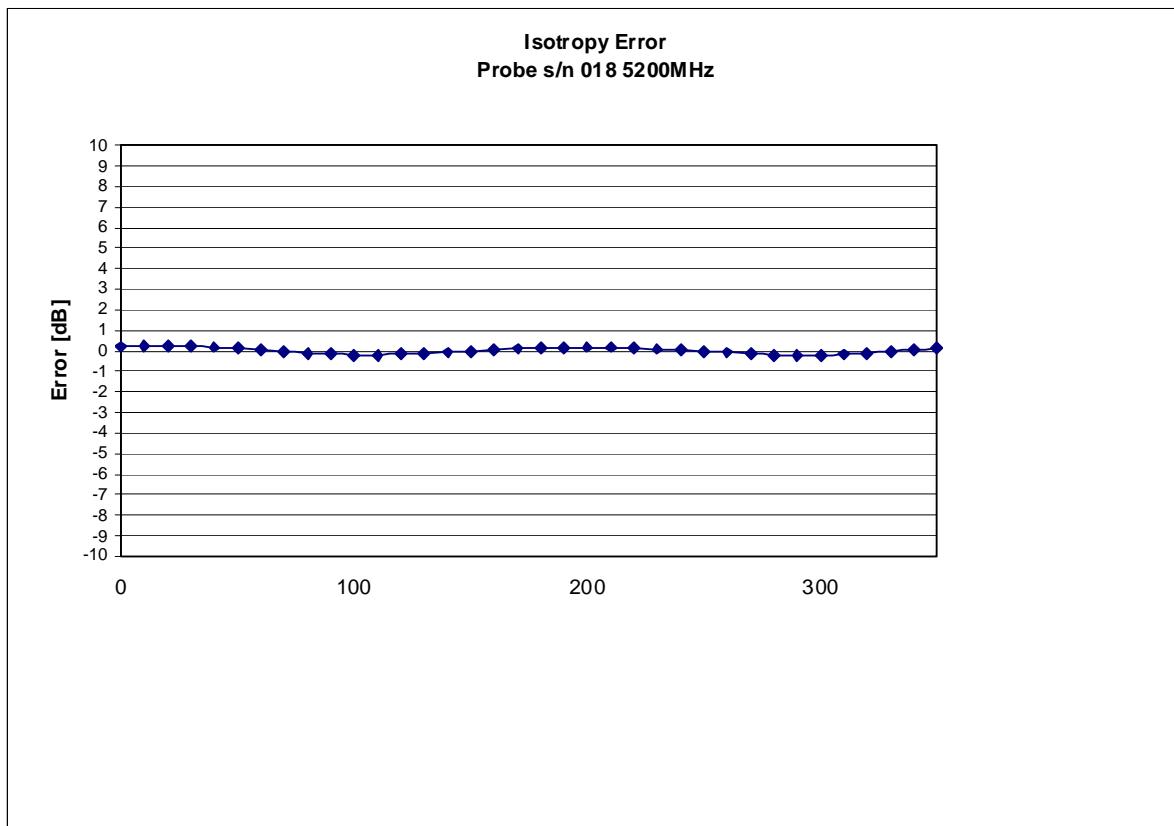
**Isotropy Error 5200 MHz (Air)****Isotropicity in Tissue:**

0.10 dB

## Dynamic Range

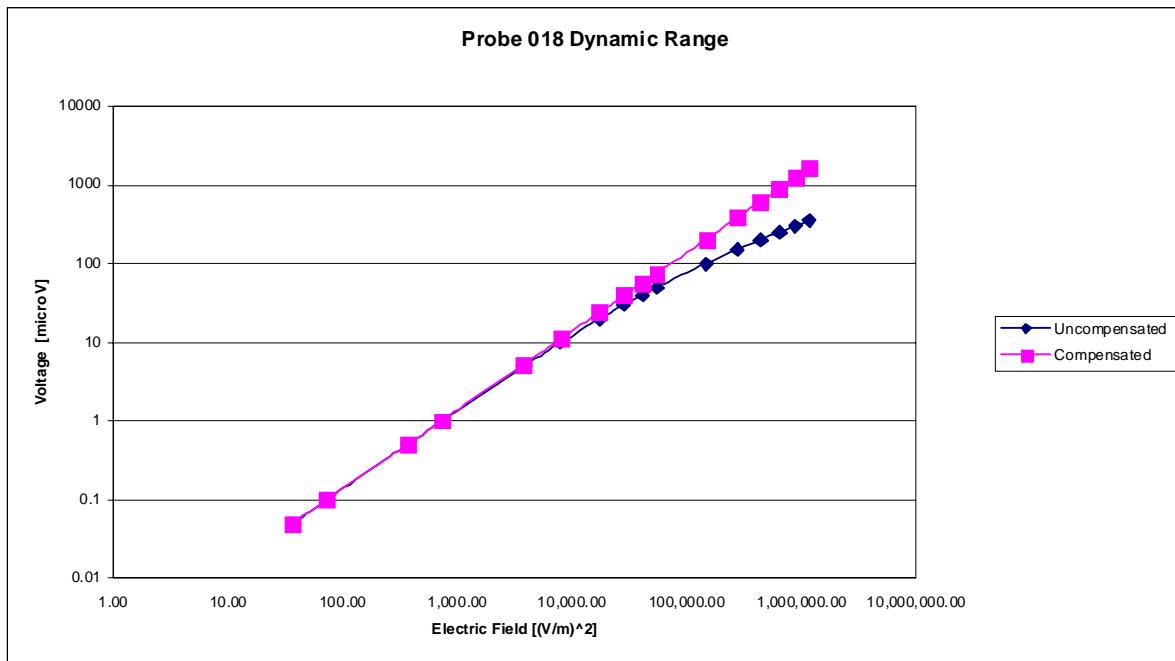

## Video Bandwidth

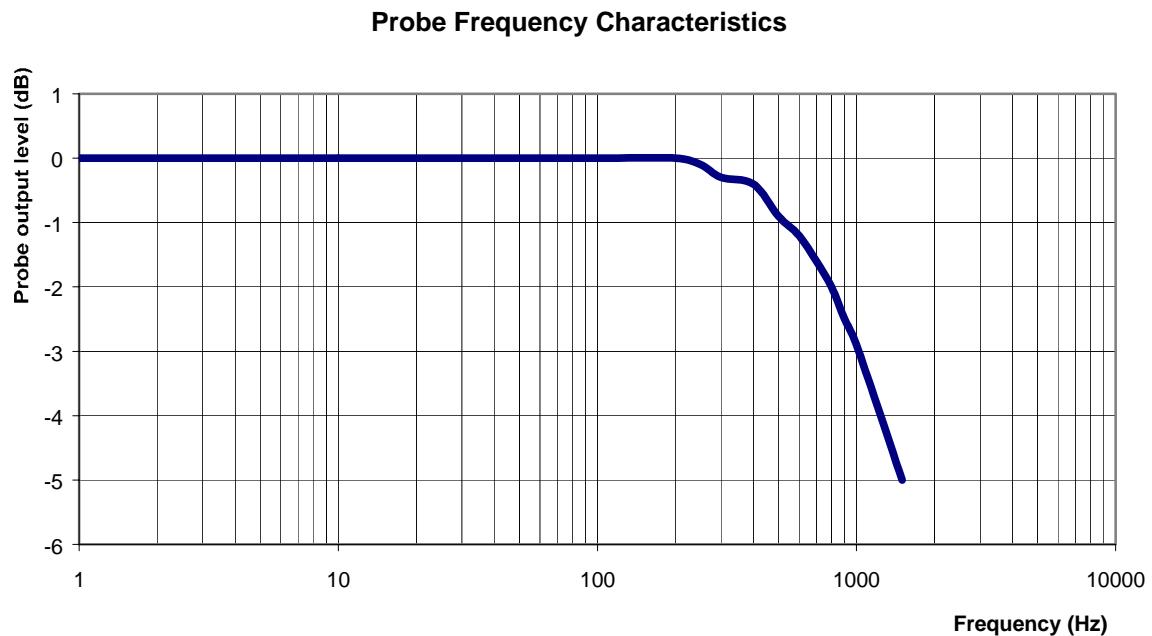

**Video Bandwidth at 500 Hz** 1 dB  
**Video Bandwidth at 1.02 KHz:** 3 dB

## **Conversion Factor Uncertainty Assessment**

**Frequency:** 5200MHz

**Epsilon:** 43.0 (+/-10%) **Sigma:** 5.75 S/m (+/-10%)

### **ConvF**

**Channel X:** 3.2 7%(K=2)

**Channel Y:** 3.2 7%(K=2)

**Channel Z:** 3.2 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

### **Boundary Effect:**

For a distance of 0.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-885

Client.: APREL

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 2450 MHz

Manufacturer: APREL Laboratories

Model No.: E-030

Serial No.: 018

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: Internal APREL

Calibrated: 3<sup>rd</sup> May 2008  
Released on: 3<sup>rd</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-030 018.

## **References**

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure

## **Conditions**

Probe 018 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**

Stuart Nicol

Jesse Hones

## **NCL Calibration Laboratories**

---

Division of APREL Laboratories.

### **Calibration Results Summary**

**Probe Type:** E-Field Probe E-030

**Serial Number:** 018

**Frequency:** 2450 MHz

**Sensor Offset:** 0.44 mm

**Sensor Length:** 2.5 mm

**Tip Enclosure:** Ertalyte\*

**Tip Diameter:** <2.9 mm

**Tip Length:** 60 mm

**Total Length:** 290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

### **Sensitivity in Air**

**Channel X:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Channel Y:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Channel Z:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Diode Compression Point:** 95 mV

## Sensitivity in Body Tissue

**Frequency:** 2450 MHz

**Epsilon:** 52.7 (+/-5%) **Sigma:** 1.95 S/m (+/-5%)

### ConvF

**Channel X:** 4.01

**Channel Y:** 4.01

**Channel Z:** 4.01

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq and corrected for broadband calibration factor.

### Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 1.44mm.

### Spatial Resolution:

The measured probe tip diameter is 2.9 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


### Broad Band Calibration:



The probe was assessed for sensitivity and conversion factor using a +/- 40MHz deviation from the centre frequency.

**Deviation at -40MHz:** -1.56%

**Deviation at +40MHz:** +1.3%


## Receiving Pattern 2450 MHz (Air)

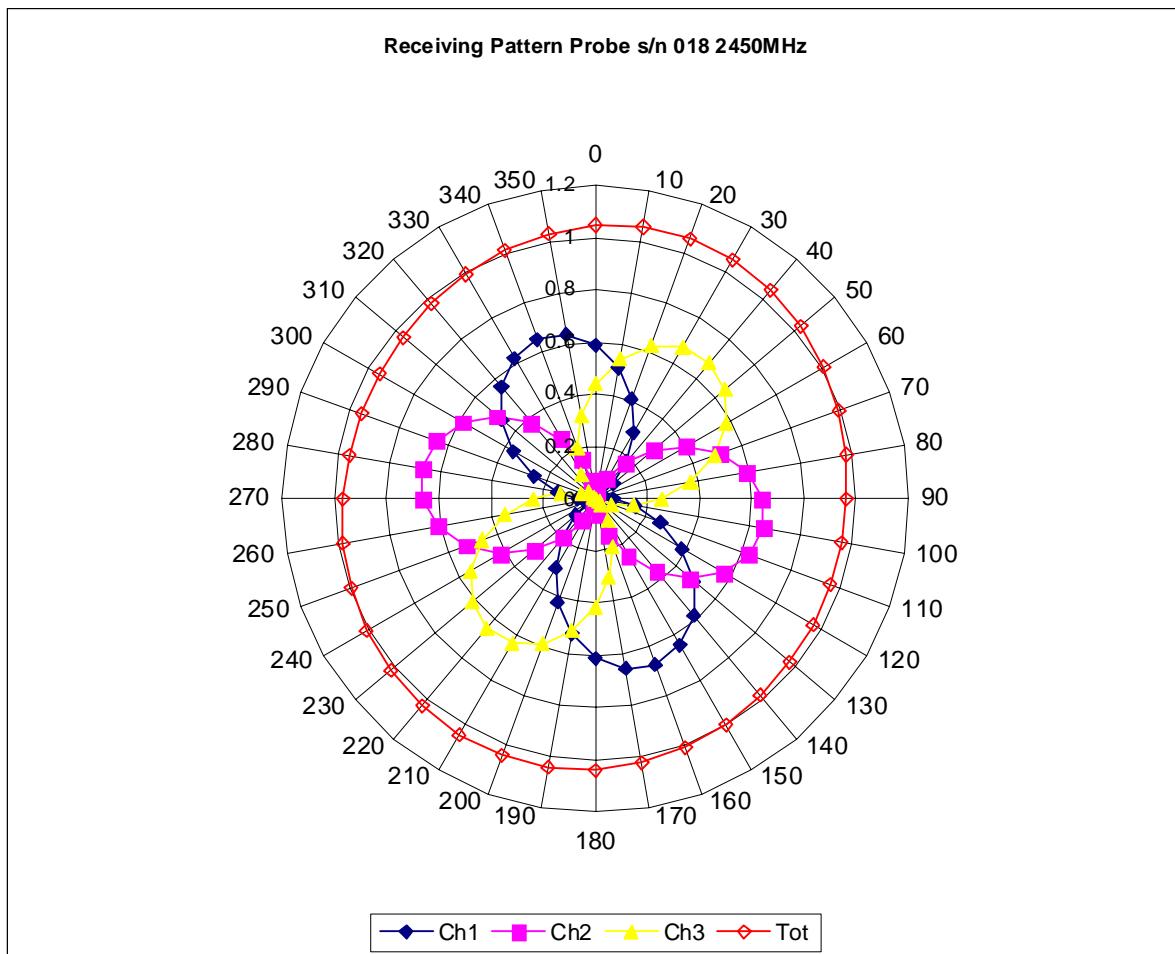

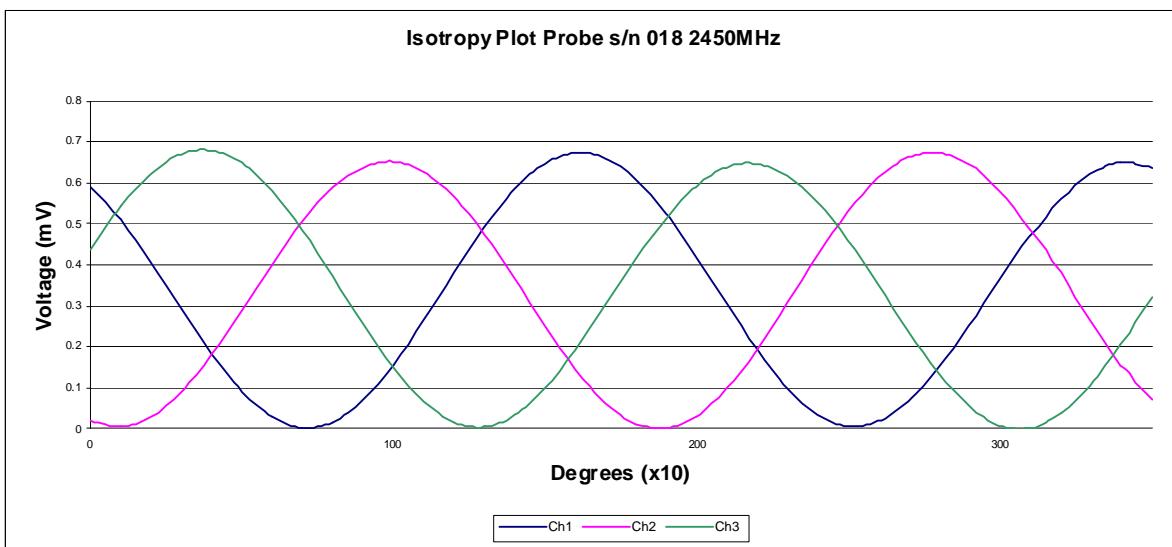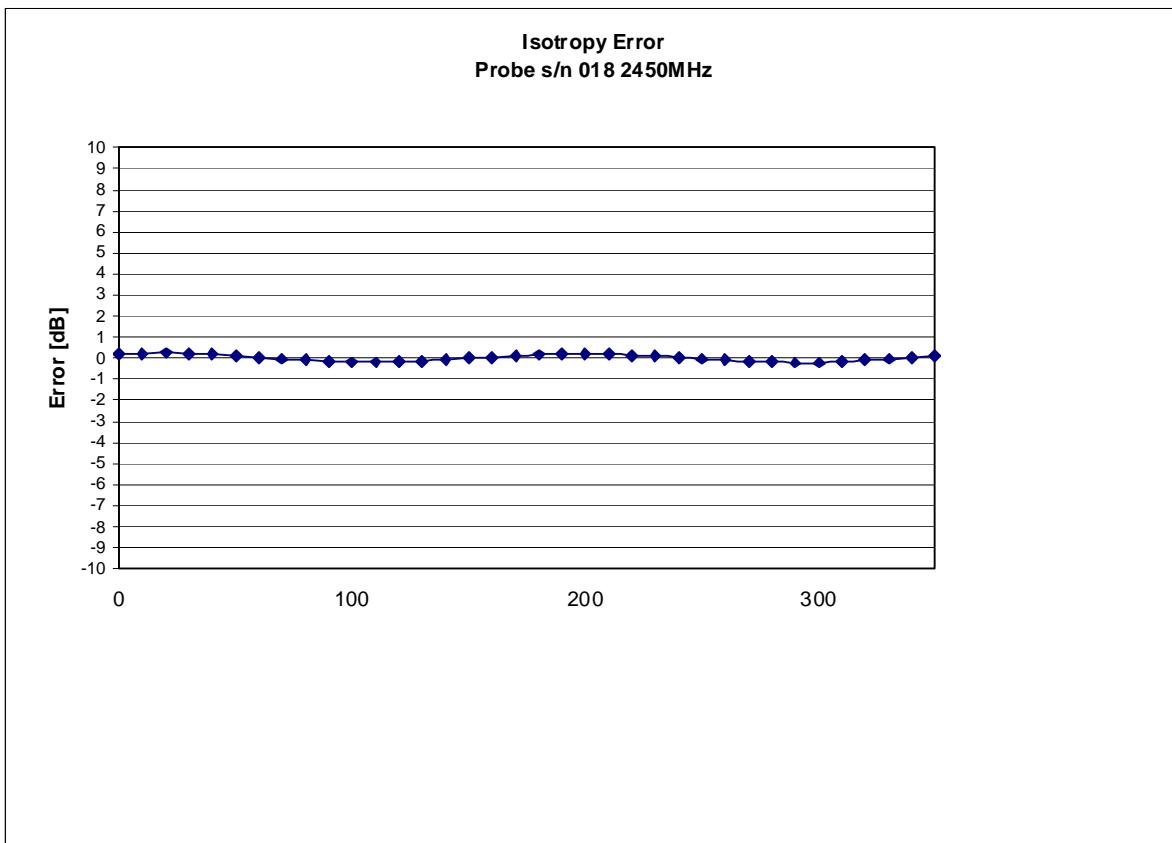
**Isotropy Error 2450 MHz (Air)****Isotropicity in Tissue:**

0.10 dB

## Dynamic Range

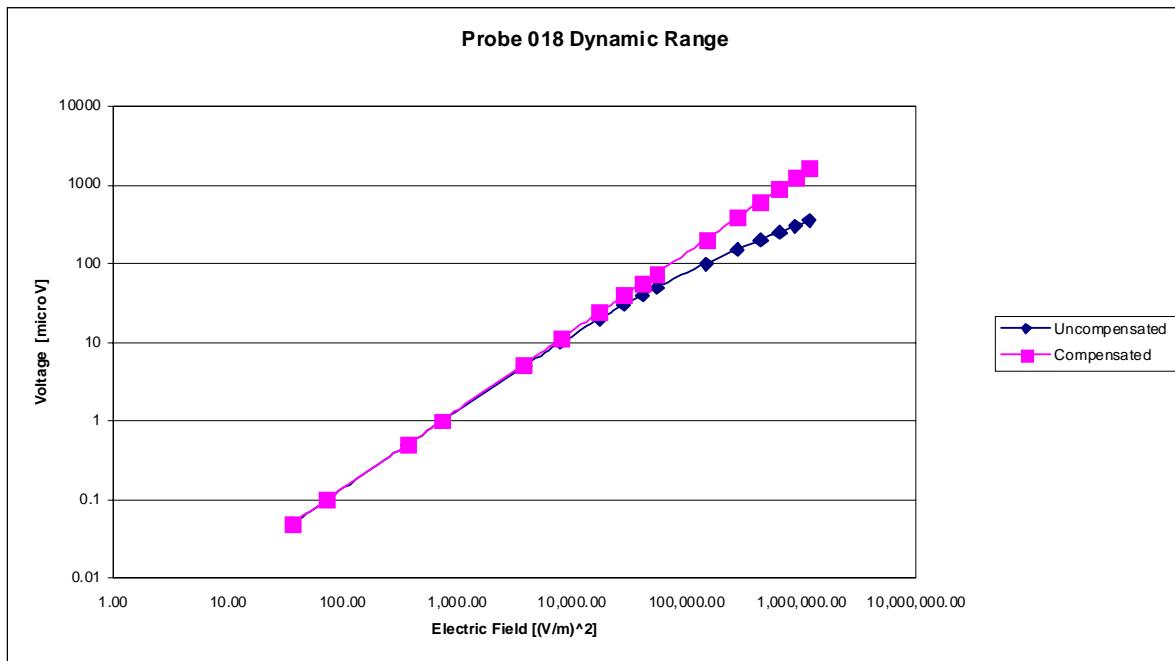

## Video Bandwidth

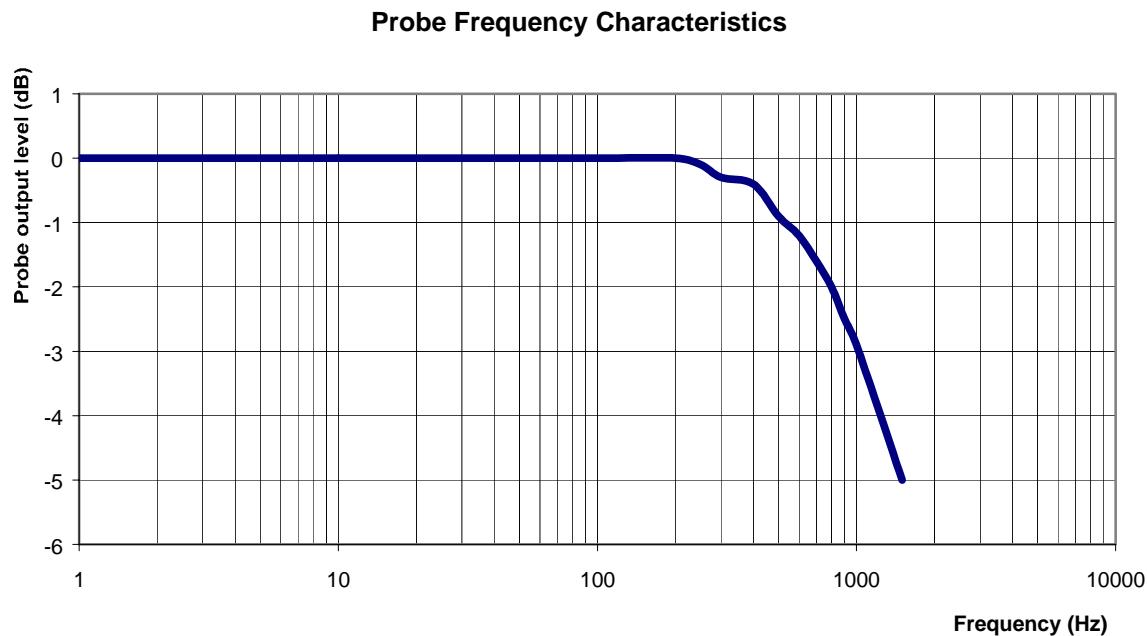

**Video Bandwidth at 500 Hz** 1 dB  
**Video Bandwidth at 1.02 KHz:** 3 dB

## **Conversion Factor Uncertainty Assessment**

**Frequency:** 2450MHz

**Epsilon:** 52.7 (+/-5%) **Sigma:** 1.95 S/m (+/-5%)

### **ConvF**

**Channel X:** 4.01 7%(K=2)

**Channel Y:** 4.01 7%(K=2)

**Channel Z:** 4.01 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

### **Boundary Effect:**

For a distance of 0.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

# NCL CALIBRATION LABORATORIES

Calibration File No.: CP-888

Client.: APREL

## C E R T I F I C A T E   O F   C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the  
**NCL CALIBRATION LABORATORIES** by qualified personnel following recognized  
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5800 MHz

Manufacturer: APREL Laboratories

Model No.: E-030

Serial No.: 018

Calibration in Body Tissue

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: Internal APREL

Calibrated: 3<sup>rd</sup> May 2008  
Released on: 3<sup>rd</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-030 018.

## **References**

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
SSI-TP-011 Tissue Calibration Procedure

## **Conditions**

Probe 018 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

**We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within this report has been reviewed for accuracy.**

Stuart Nicol

Jesse Hones

## Calibration Results Summary

**Probe Type:** E-Field Probe E-030

**Serial Number:** 018

**Frequency:** 5800 MHz

**Sensor Offset:** 0.44 mm

**Sensor Length:** 2.5 mm

**Tip Enclosure:** Ertalyte\*

**Tip Diameter:** <2.9 mm

**Tip Length:** 60 mm

**Total Length:** 290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

### Sensitivity in Air

**Channel X:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Channel Y:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Channel Z:**  $1.2 \mu\text{V}/(\text{V}/\text{m})^2$

**Diode Compression Point:** 95 mV

## Sensitivity in Body Tissue

**Frequency:** 5800 MHz

**Epsilon:** 48.2 (+/-10%) **Sigma:** 6.0 S/m (+/-10%)

### ConvF

**Channel X:** 3.2

**Channel Y:** 3.2

**Channel Z:** 3.2

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq and corrected for broadband calibration factor.

### Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.

### Spatial Resolution:

The measured probe tip diameter is 2.9 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


### Broad Band Calibration:



The probe was assessed for sensitivity and conversion factor using a +/- 40MHz deviation from the centre frequency.

**Deviation at -40MHz:** -3.07%

**Deviation at +40MHz:** +3.22%


## Receiving Pattern 5800 MHz (Air)

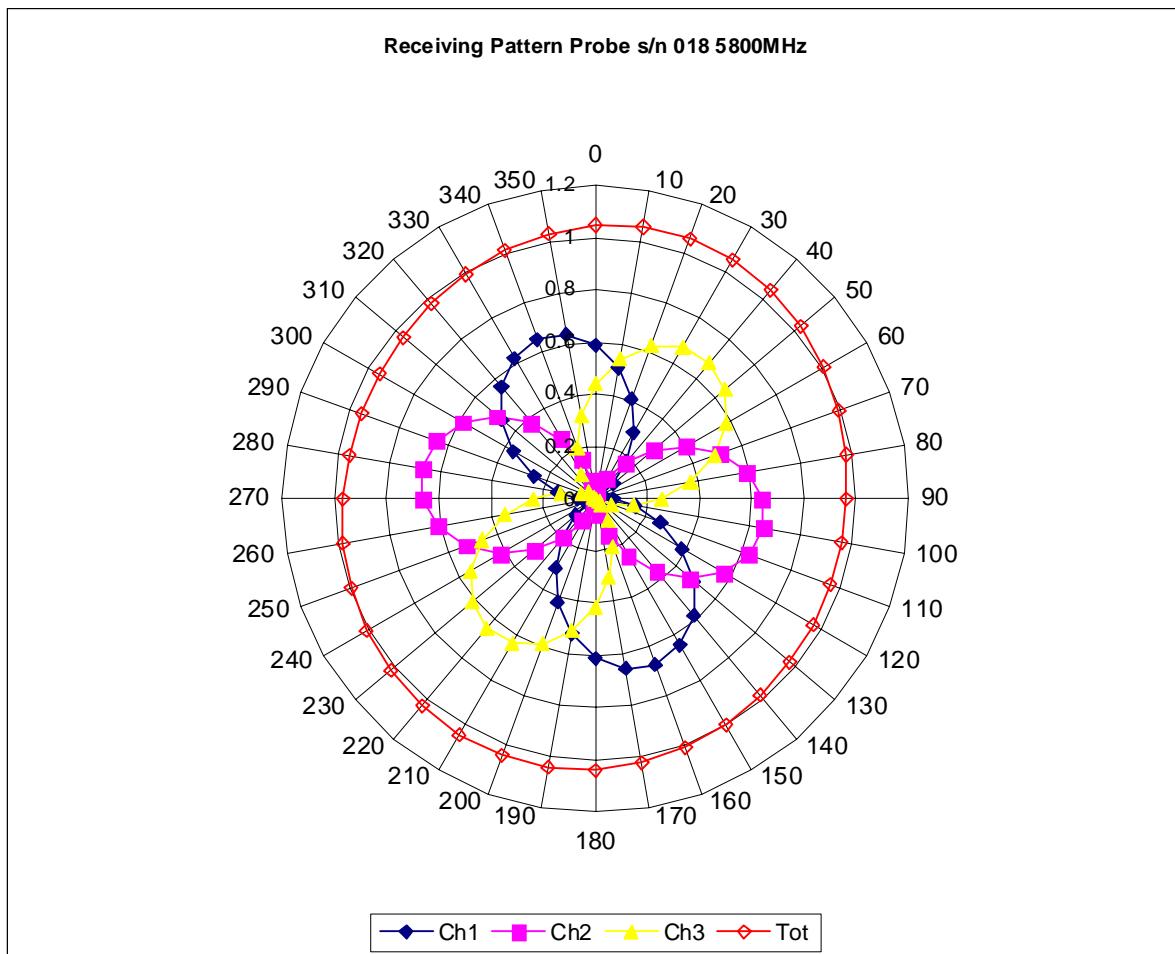

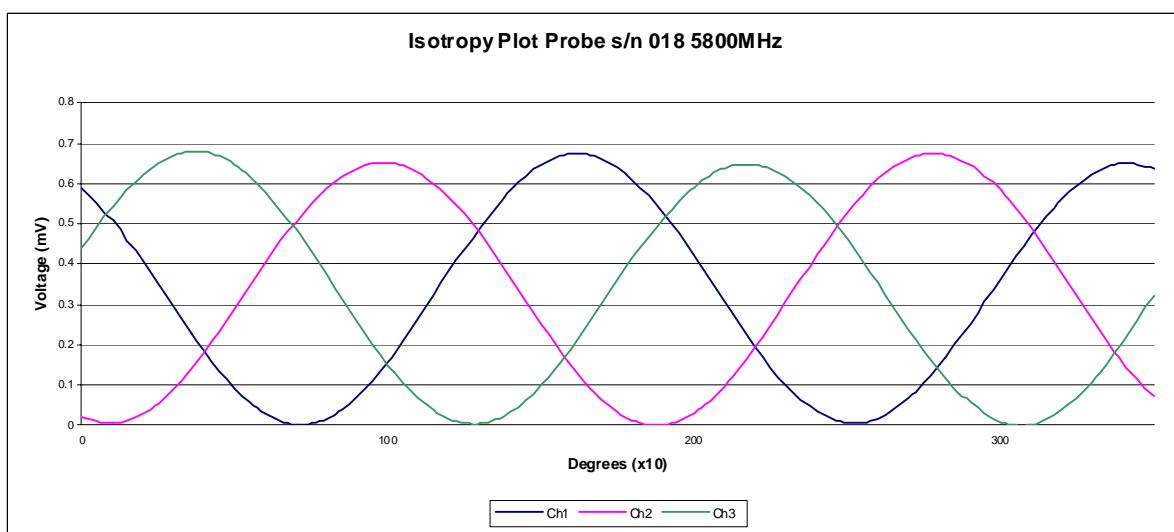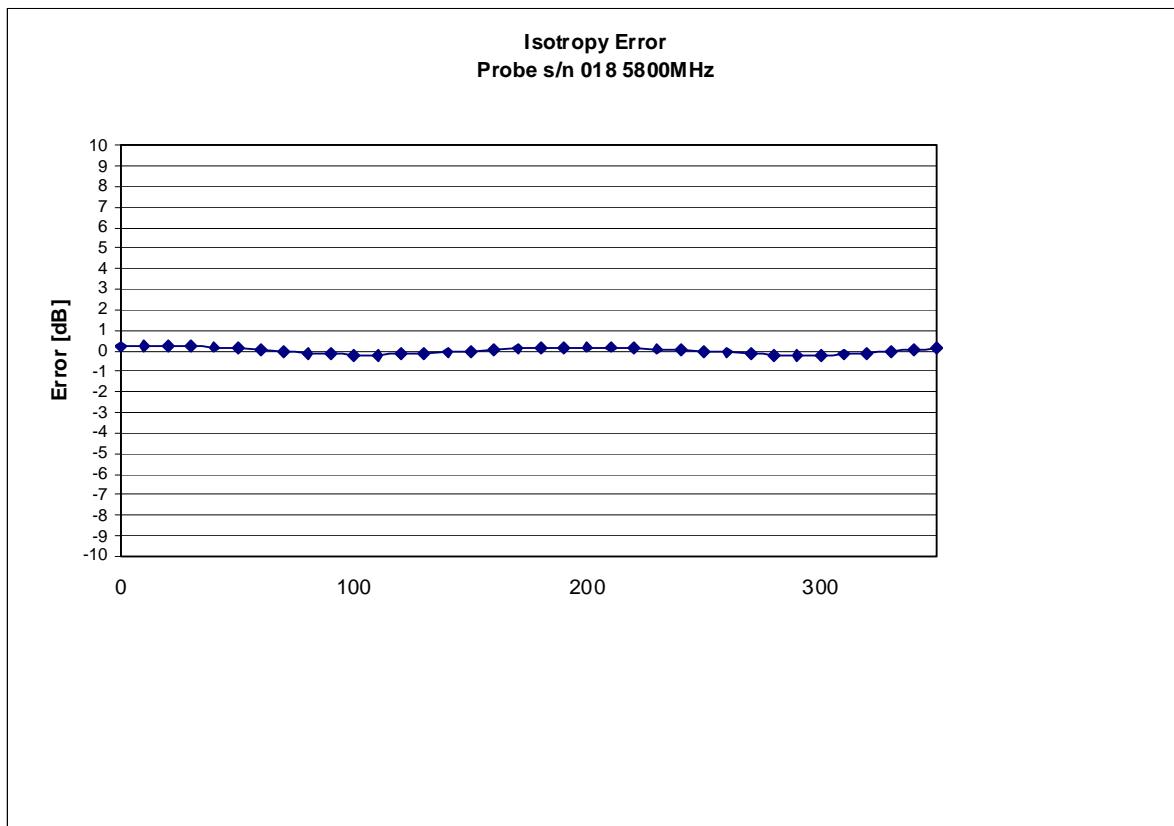
**Isotropy Error 5800 MHz (Air)****Isotropicity in Tissue:**

0.10 dB

## Dynamic Range

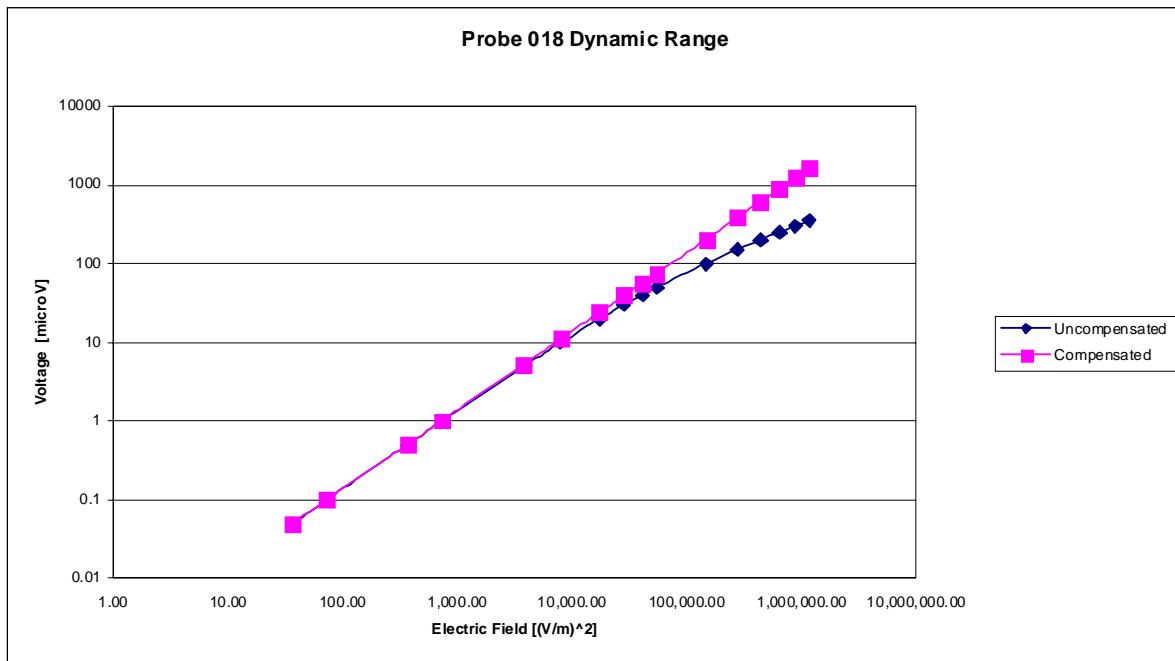

## Video Bandwidth

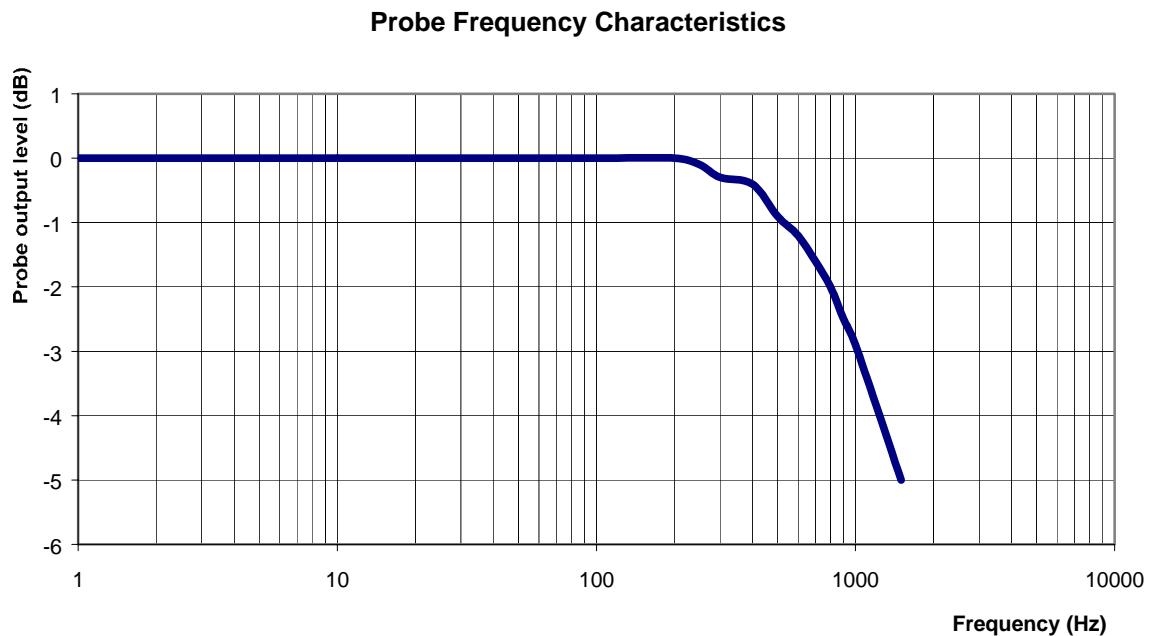

**Video Bandwidth at 500 Hz** 1 dB  
**Video Bandwidth at 1.02 KHz:** 3 dB

## **Conversion Factor Uncertainty Assessment**

**Frequency:** 5800MHz

**Epsilon:** 48.2 (+/-10%) **Sigma:** 6.0 S/m (+/-10%)

### **ConvF**

**Channel X:** 3.2 7%(K=2)

**Channel Y:** 3.2 7%(K=2)

**Channel Z:** 3.2 7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

### **Boundary Effect:**

For a distance of 0.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

# Regulatory WLAN Antenna Information

(English Language Required for Intel Regulatory Review / Approval)

**(OEM/ODM or antenna vendor is required to complete this document with platform antenna information.  
Remove Intel references and make this your own document)**

Platform	
Platform Owner	DELL
Brand Name	
Model Name	
ODM	COMPAL
Target Launch Date	(YYYY/ MM/ DD)
Antenna	
Brand Name	GALTRONICS
Antenna Set Name	WLAN_L
Antenna Set P/N	021020201NC3793-1
Part Number	<input type="checkbox"/> Tx1 Antenna: 06-7015-03 (MAIN) <input type="checkbox"/> Tx2 Antenna: 06-7016-03 (AUX)
Antenna Set Name	WLAN_R
Antenna Set P/N	021020201NC3793-2
Part Number	<input type="checkbox"/> Tx3 Antenna: 06-7014-03 (MIMO)
Module	
With WLAN Module	
(Check Box)	
	<input type="checkbox"/> 533ANX Family
	<input type="checkbox"/> 512ANX Family
	<input type="checkbox"/> 533AN Family
	<input type="checkbox"/> 512AN Family

# Antenna Sample / Antenna Data Requirements for worldwide regulatory approval

Section	Description of Required OEM / ODM Antenna Information	US / IC	EU	Japan	Taiwan	S.Korea
1A	Part Number for Antenna only	Required	Required	Required	Required	Required
1B	Antenna Manufacturer Name	Required	Required	Required	Required	Required
1C	Description of Antenna Type	Required	N/A	N/A	N/A	N/A
1D	Part number of Antenna Assembly / cable impedance, length & diameter.	Required	Desired	Desired	Desired	Desired
1E	Tx1, Tx2 & Tx3 antenna (Peak Gain W/ cable loss) *	Required	Required	Required	Required	Required
	1E OR 1F, 1G, 1H					
1F	Tx1, Tx2 & Tx3 antenna (Peak Gain only) *	Required	Required	Required	Required	Required
1G	VSWR of cable including connector	Required	Required	Required	Required	Required
1H	Tx1, Tx2 & Tx3 antenna (Cable loss W/ connector) *	Required	Required	Required	Required	Required
2	Dimensioned Photographs <u>and</u> Drawings of Tx1, Tx2, and Tx3 (or Rx3) antennas	Required	Required	Required	Required	Required
3	Radiation patterns of antennas loaded in the host platform.	Required	Desired	Required	N/A	Required
4	Platform model name / number - correlated to antenna manufacturer and antenna part number	Required	Required	Desired	Required	Desired
5	Photograph(s) or Drawings showing location of antennas in platform. <u>(S. Korea requires photographs of antennas for approval submission).</u> <u>Taiwan requires pictures of each antenna type shown in the system.</u>	Required	Required	Desired	Required (Photos)	Required (Photos)
6	Mech. drawings / photos with dimensions of antenna locations and distance from end-user (For evaluation of SAR testing requirement).	Required	N/A	N/A	N/A	N/A
7	Photograph(s) or Drawings showing the location of all antennas (WLAN, other) and distance between those transmitting antennas. Information will be used to evaluate whether co-location testing is required.	Required	N/A	N/A	N/A	N/A
8	Local representative contact information for LMA/ PARS process.	Required	N/A	N/A	N/A	N/A

**NOTE:**

(\*) if 3<sup>rd</sup> antenna is Rx only (e.g. receive only for 4965AGN) then peak gain and cable loss not required

# Antenna Information

## Section 1. Antenna Assembly Specifications

### Antenna Assembly Summary:

1A Antenna Part Number	1B Manufacture	1C Antenna Type	1D Cable Assembly Part Number and Information	1E *Peak Gain W/ Cable loss (dBi)	1F Peak Gain w/o Cable Loss (dBi)	1G VSWR	1H Cable Loss (dBi)
(P/N:06-7015-03) Tx1 antenna	Galtronics	PIFA	(P/N: 03-7007-01) 50 ohm Coaxial. length:53.9cm diameter: 1.13mm Connector: U.FL	2400-2500MHz <u>-2.49</u> dBi (peak)	2400-2500MHz <u>-1.15</u> dBi (peak)	2400-2500MHz <u>2.00</u> max	2400-2500MHz <u>-1.34</u> dBi (peak)
				2496-2690MHz <u>-2.19</u> dBi (peak)	2496-2690MHz <u>-0.85</u> dBi (peak)	2496-2690MHz <u>1.47</u> max	2496-2690MHz <u>-1.34</u> dBi (peak)
				5150-5350MHz <u>-1.88</u> dBi (peak)	5150-5350MHz <u>-0.36</u> dBi (peak)	5150-5350MHz <u>1.59</u> max	5150-5350MHz <u>-2.24</u> dBi (peak)
				5470-5725MHz <u>0.40</u> dBi (peak)	5470-5725MHz <u>1.84</u> dBi (peak)	5470-5725MHz <u>1.73</u> max	5470-5725MHz <u>-2.24</u> dBi (peak)
				5725-5850MHz <u>-0.52</u> dBi (peak)	5725-5850MHz <u>1.72</u> dBi (peak)	5725-5850MHz <u>2.00</u> max	5725-5850MHz <u>2.24</u> dBi (peak)
(P/N:06-7016-03) Tx2 antenna	Galtronics	PIFA	(P/N: 03-7008-01) 50 ohm Coaxial. length:49.1cm diameter: 1.13mm Connector: U.FL	2400-2500MHz <u>0.18</u> dBi (peak)*	2400-2500MHz <u>1.40</u> dBi (peak)*	2400-2500MHz <u>1.80</u> max*	2400-2500MHz <u>-1.22</u> dBi (peak)*
				2496-2690MHz <u>0.18</u> dBi (peak)*	2496-2690MHz <u>1.40</u> dBi (peak)*	2496-2690MHz <u>1.56</u> max*	2496-2690MHz <u>-1.22</u> dBi (peak)*
				5150-5350MHz <u>1.32</u> dBi (peak)*	5150-5350MHz <u>3.36</u> dBi (peak)*	5150-5350MHz <u>2.50</u> max*	5150-5350MHz <u>-2.04</u> dBi (peak)*
				5470-5725MHz <u>-0.60</u> dBi (peak)*	5470-5725MHz <u>1.44</u> dBi (peak)*	5470-5725MHz <u>2.03</u> max*	5470-5725MHz <u>-2.04</u> dBi (peak)*
				5725-5850MHz <u>-1.31</u> dBi (peak)*	5725-5850MHz <u>0.73</u> dBi (peak)*	5725-5850MHz <u>1.65</u> max*	5725-5850MHz <u>-2.04</u> dBi (peak)*
(P/N:06-7014-03) Tx3 antenna	Galtronics	PIFA	(P/N: 03-7009-01) 50 ohm Coaxial. length:32.9cm diameter: 1.13mm Connector: U.FL	2400-2500MHz <u>-1.8</u> dBi (peak)*	2400-2500MHz <u>-0.98</u> dBi (peak)*	2400-2500MHz <u>2.65</u> max*	2400-2500MHz <u>-0.82</u> dBi (peak)*
				2496-2690MHz <u>-1.28</u> dBi (peak)*	2496-2690MHz <u>-0.46</u> dBi (peak)*	2496-2690MHz <u>1.36</u> max*	2496-2690MHz <u>-0.82</u> dBi (peak)*
				5150-5350MHz <u>1.37</u> dBi (peak)*	5150-5350MHz <u>0</u> dBi (peak)*	5150-5350MHz <u>1.13</u> max*	5150-5350MHz <u>-1.37</u> dBi (peak)*
				5470-5725MHz <u>-0.87</u> dBi (peak)*	5470-5725MHz <u>0.50</u> dBi (peak)*	5470-5725MHz <u>1.21</u> max*	5470-5725MHz <u>-1.37</u> dBi (peak)*
				5725-5850MHz <u>-1.76</u> dBi (peak)*	5725-5850MHz <u>-0.39</u> dBi (peak)*	5725-5850MHz <u>1.73</u> max*	5725-5850MHz <u>-1.37</u> dBi (peak)*

### NOTE:

(\*) If Rx2/Rx3 only (2<sup>nd</sup> or 3<sup>rd</sup> antenna receives only, e.g. for 512 family & 4965AGN) then the information marked with \* is not required

### Antenna Peak Gain Table:


	Tx1 antenna		Tx2 Antenna		Tx3 Antenna	
Frequency (MHz)	Horizontal (dBi)	Vertical (dBi)	Horizontal (dBi)	Vertical (dBi)	Horizontal (dBi)	Vertical (dBi)
2400	-2.49	-4.62	-1.84	-6.34	-3.01	-3.40
2450	-2.84	-2.73	-2.76	-3.52	-0.69	-3.12
2500	-3.97	-2.69	-2.33	-2.41	-2.00	-2.87
2500	-3.97	-2.69	-2.33	-2.41	-2.00	-2.87
2600	-2.23	-3.06	-1.62	-5.19	-1.35	-3.63
2700	-2.78	-2.19	-3.20	-2.54	-2.75	-3.10
5150	-6.38	-1.88	-7.72	-1.07	-11.42	-3.46
5470	-4.66	0.30	-8.86	-1.71	-6.27	-0.83
5600	-6.23	0.40	-8.63	-2.10	-4.30	0.64
5785	-7.23	-2.04	-9.22	-4.54	-3.23	0.15
5850	-3.27	-0.52	-6.55	-2.48	-2.57	1.62

- Antenna Peak Gain required being test in system basis.
- 1E frame contend absolutely peak antenna gain include H/V

## Section 2. Dimensioned Photos or Drawings of Antennas

Include a dimensioned photo and dimensioned drawing of Tx1 antenna here.

### Tx1 Antenna Dimensioned Drawing: (MAIN)

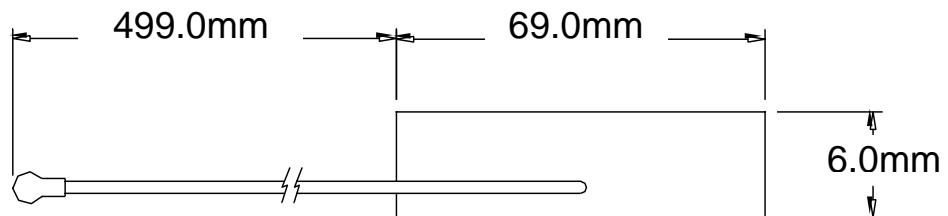


### Tx1 Antenna Photo:




**Include a dimensioned photo and dimensioned drawing of Tx2 antenna here.**

**Tx2 Antenna Dimensioned Drawing: (AUX)**

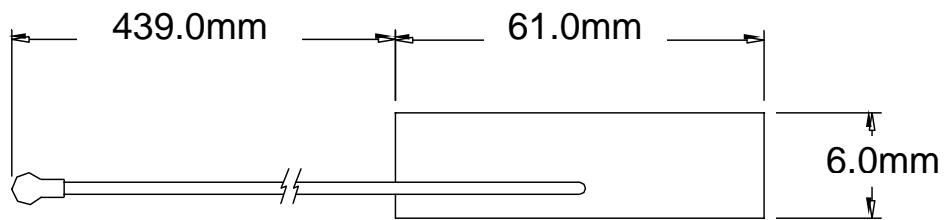


**Tx2 Antenna Photo:**

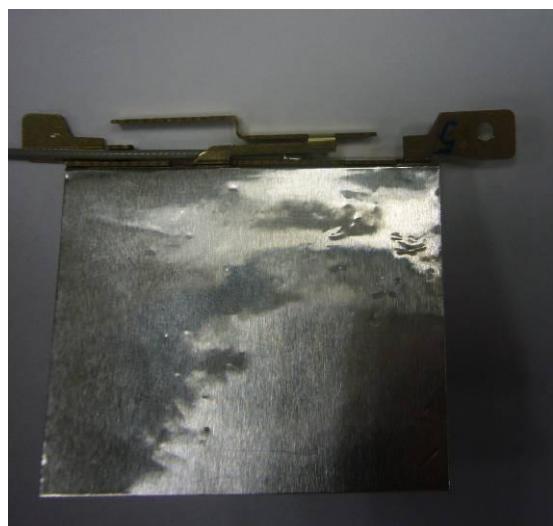

**Include a dimensioned photo and dimensioned drawing of Tx3 antenna here.**

**Tx3 Antenna Dimensioned Drawing: (MIMO)**

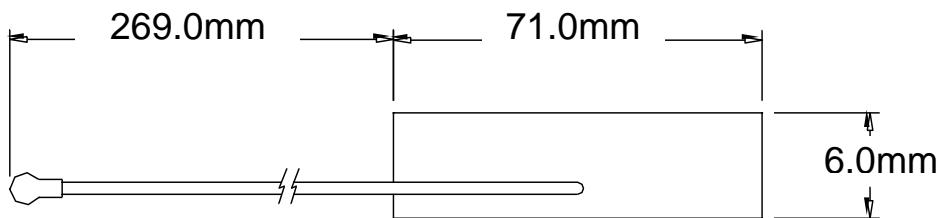

**Tx3 Antenna Photo:**



**Include front view photo of all 3 antennas here.**

Antenna Manufacturer: Galtronics

Antenna Part Number: 06-7015-03 (Tx1), 06-7016-03 (Tx2), 06-7014-03 (Tx3)



**Include back view photo of all 3 antennas here.**

Antenna Manufacturer: Galtronics


Antenna Part Number: 06-7015-03 (Main), 06-7016-03 (Aux), 06-7014-03 (MIMO)




## Section 3. Radiation characteristics of antennae Loaded in Host Platform

### 2400-2500MHz radiation characteristic


Tx1 antenna: 2400 MHz

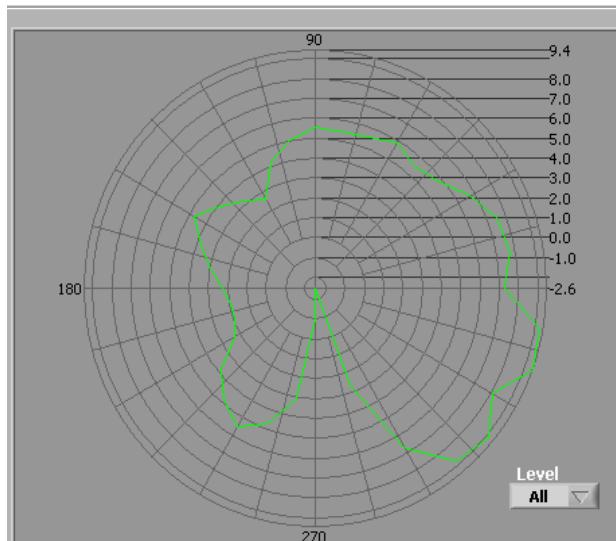

Total

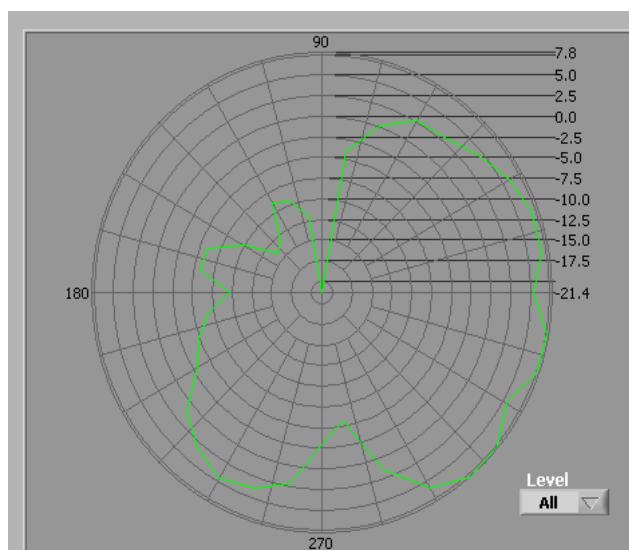


Horizontal

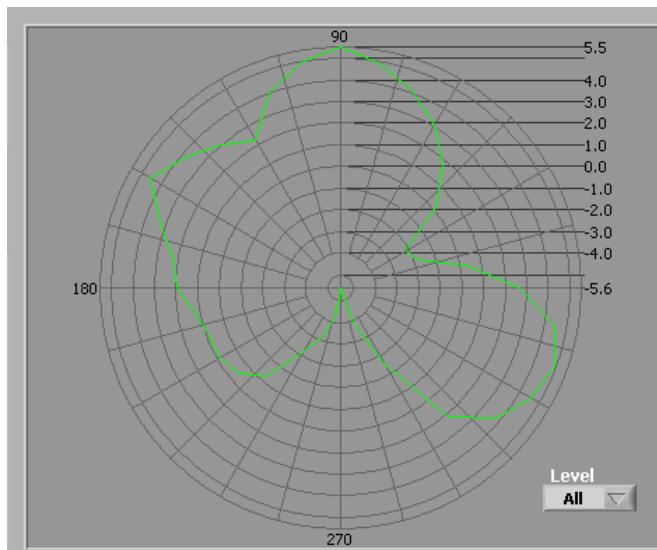


Vertical

Center Frequency	<b>2400 MHz</b>
Horizontal (dBi) peak	<b>-2.49</b>
Vertical (dBi) peak	<b>-4.62</b>


## Tx1 antenna: 2450 MHz

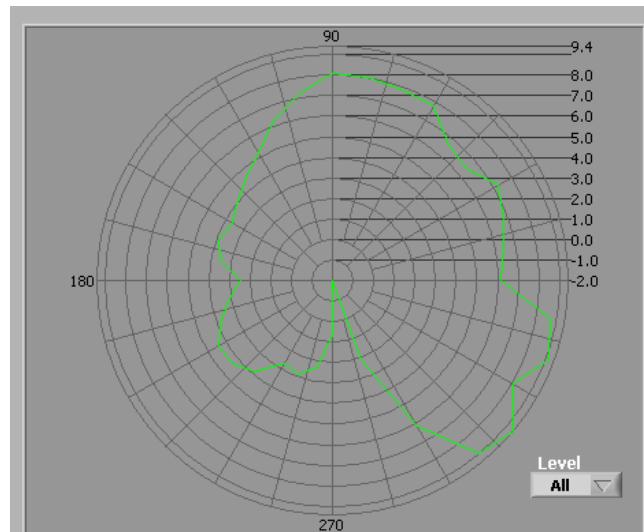

Total

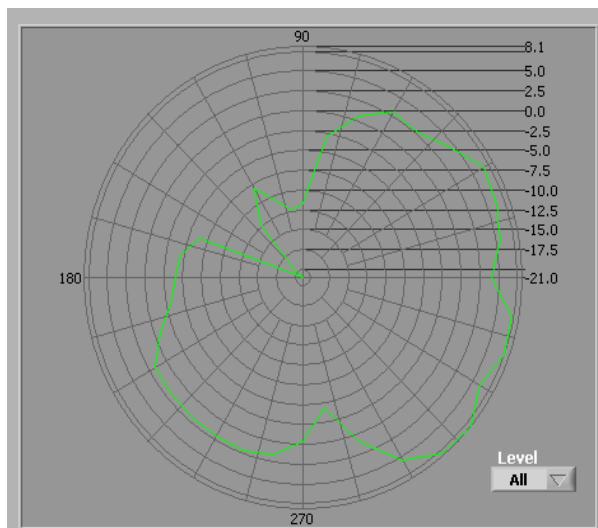


Horizontal

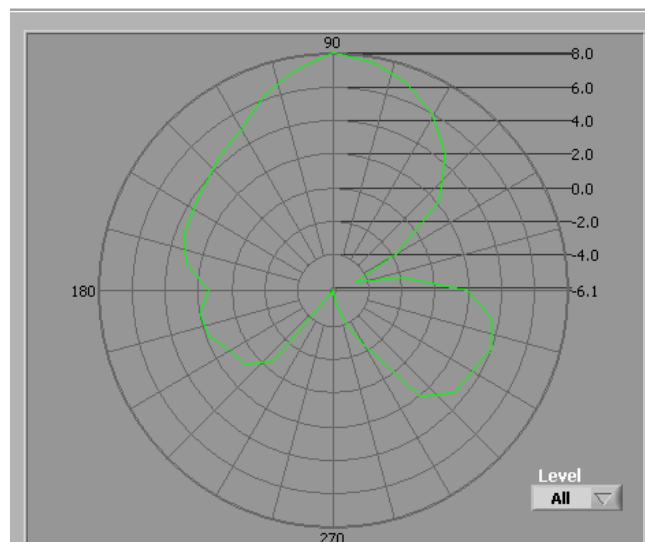


Vertical

Center Frequency	<b>2450 MHz</b>
Horizontal (dBi) peak	<b>-2.84</b>
Vertical (dBi) peak	<b>-2.73</b>


## Tx1 antenna: 2500 MHz

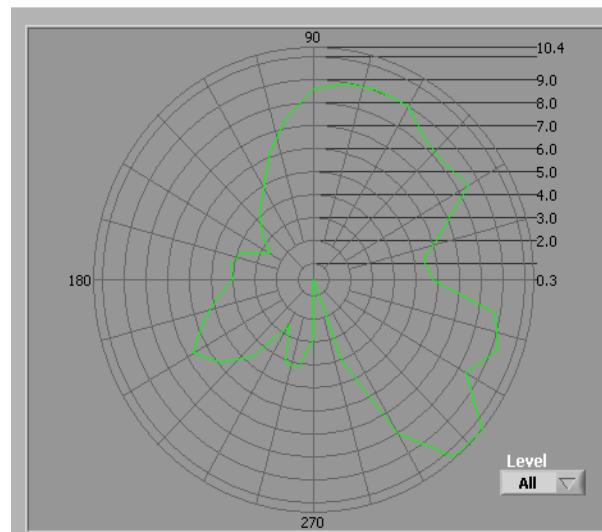

Total

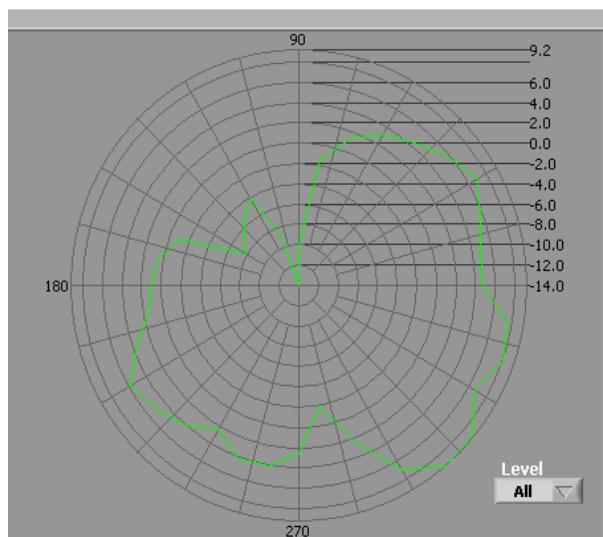


Horizontal

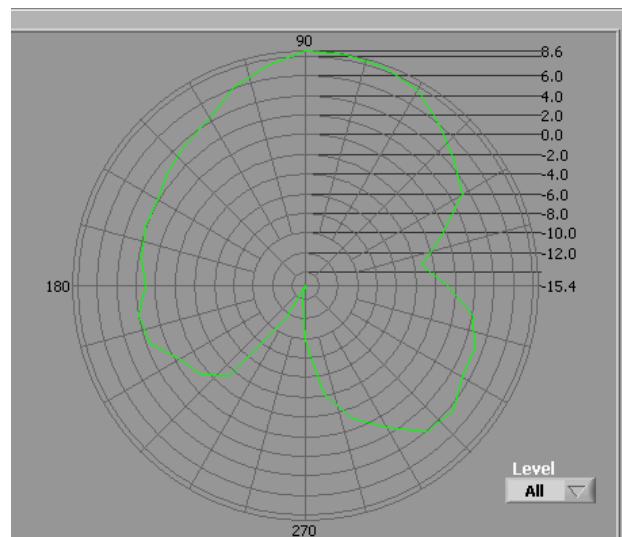


Vertical

Center Frequency	<b>2500 MHz</b>
Horizontal (dBi) peak	<b>-3.97</b>
Vertical (dBi) peak	<b>-2.69</b>


Tx2 (or Rx2) antenna: 2400 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)

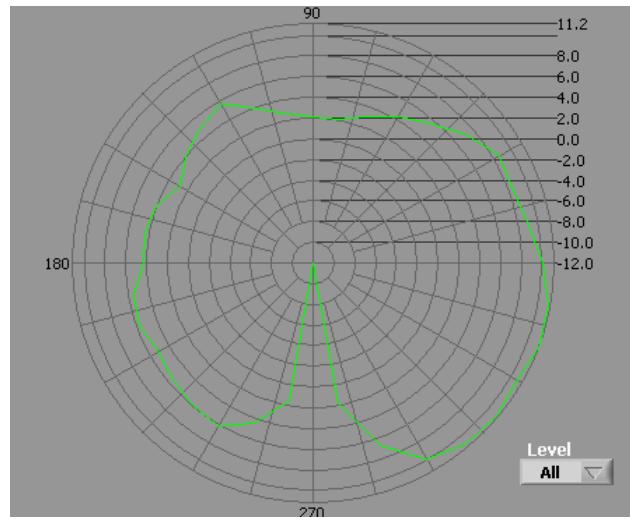

Total

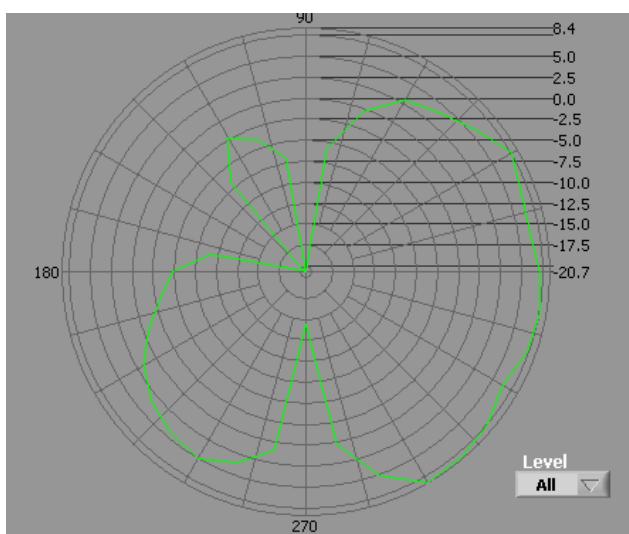


Horizontal

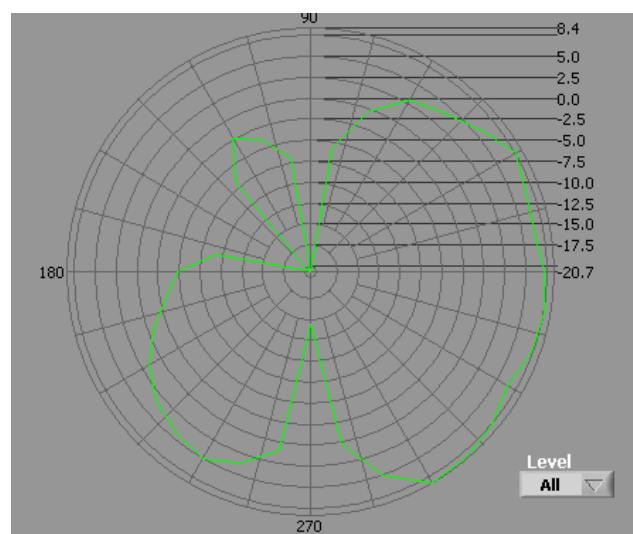


Vertical

Center Frequency	<b>2400 MHz</b>
Horizontal (dBi) peak	<b>-1.84</b>
Vertical (dBi) peak	<b>-6.34</b>

Tx2 (or Rx2) antenna: 2450 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)

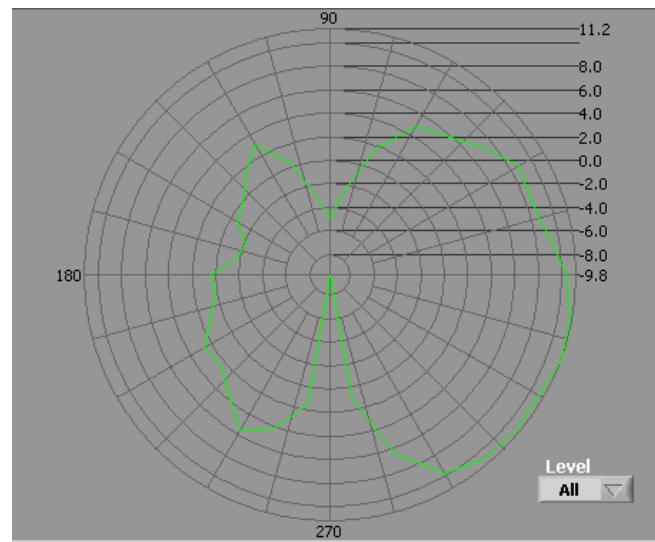


Total

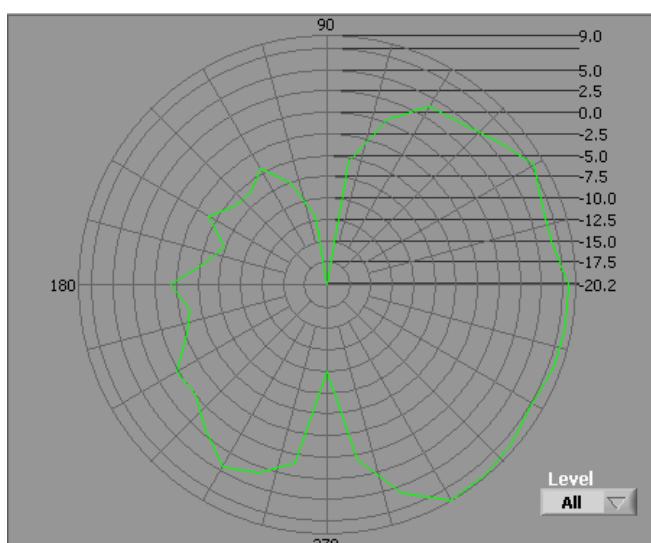

Level  
All

Horizontal

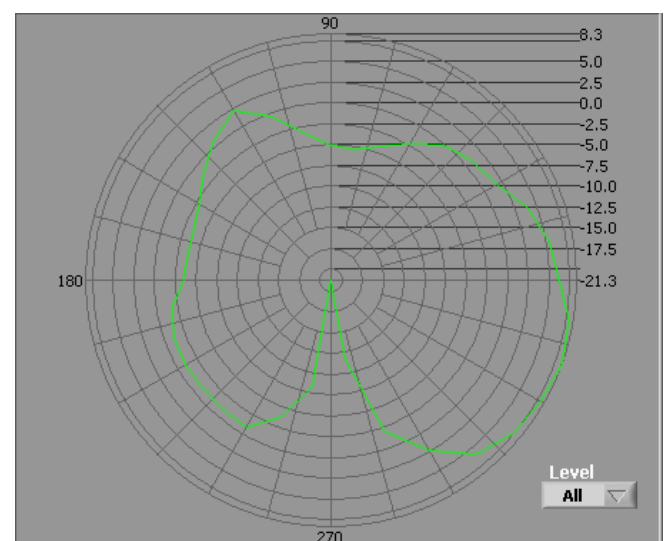


Level  
All


Vertical

Center Frequency	<b>2450 MHz</b>
Horizontal (dBi) peak	<b>-2.76</b>
Vertical (dBi) peak	<b>-3.52</b>


**Tx2 (or Rx2) antenna: 2500 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)**

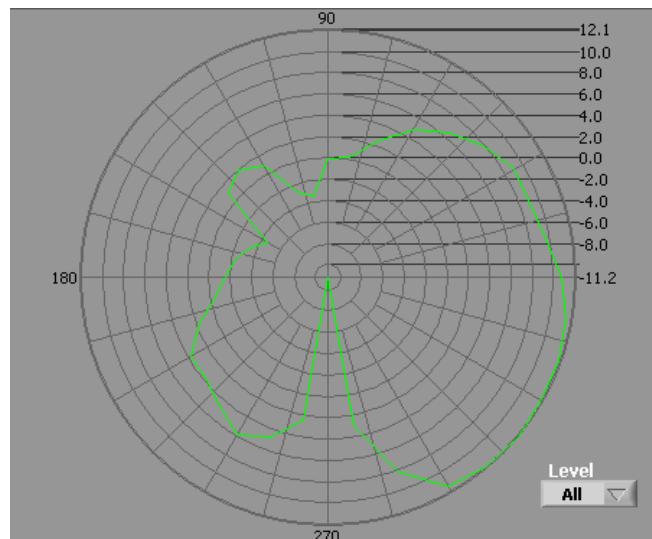

**Total**

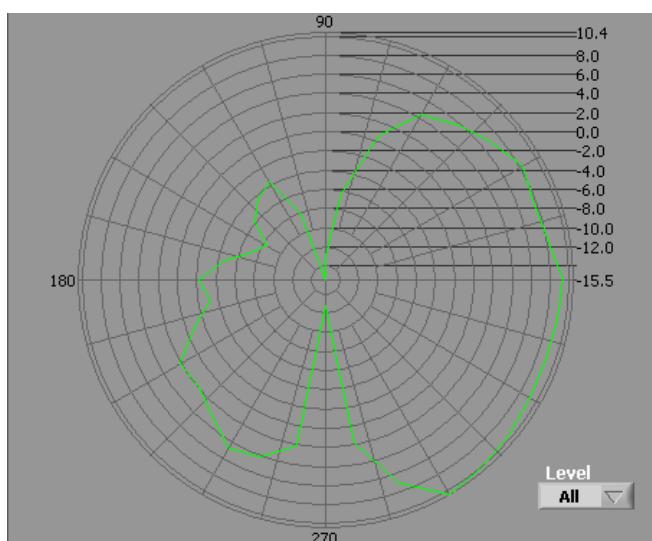


**Horizontal**

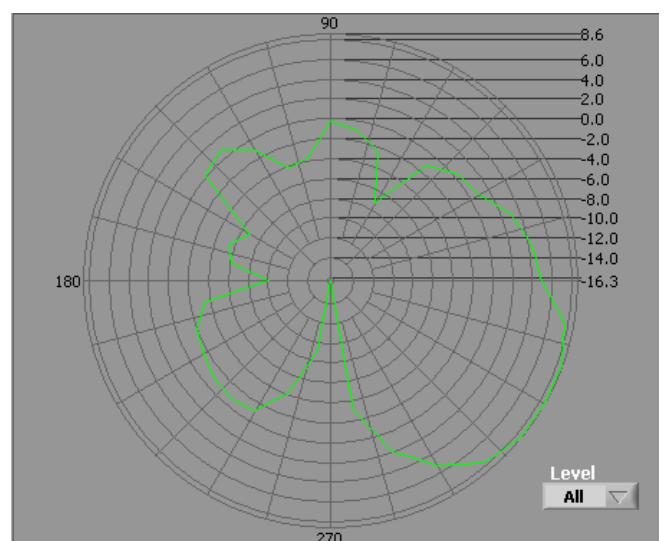


**Vertical**

Center Frequency	<b>2500 MHz</b>
Horizontal (dBi) peak	<b>-2.33</b>
Vertical (dBi) peak	<b>-2.41</b>


**Tx3 (or Rx3) antenna: 2400 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

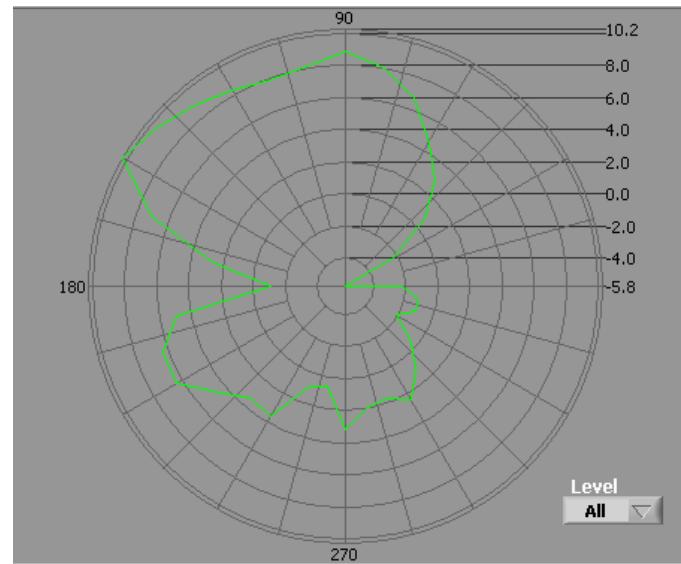

Total

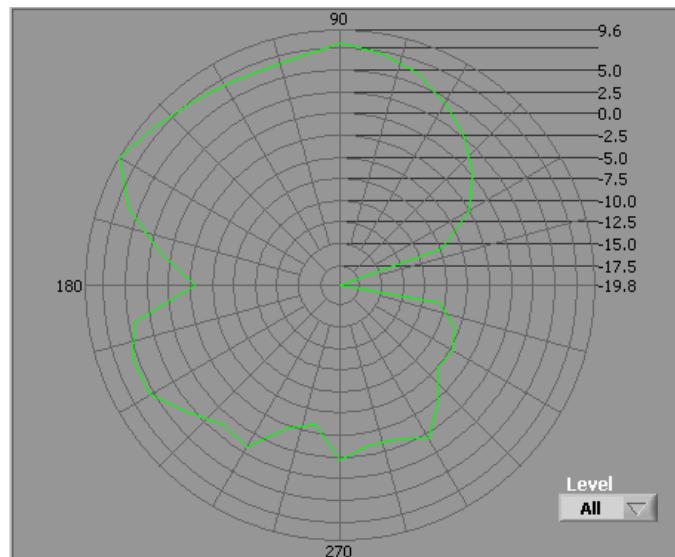


Horizontal

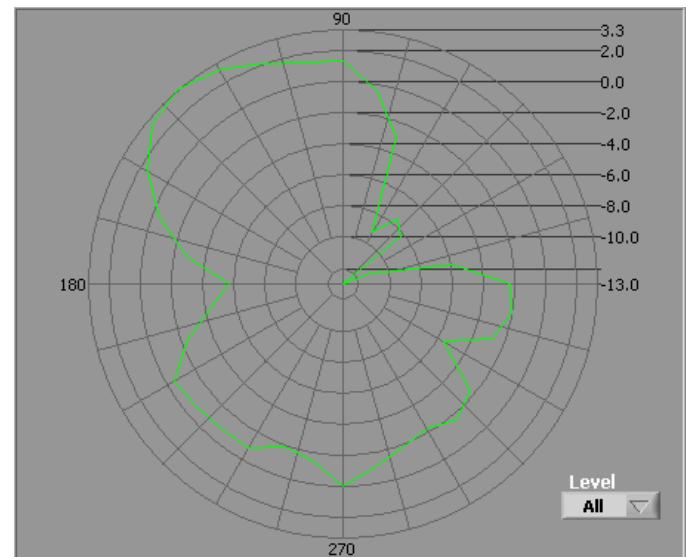


Vertical

Center Frequency	<b>2400 MHz</b>
Horizontal (dBi) peak	<b>-3.01</b>
Vertical (dBi) peak	<b>-3.70</b>


**Tx3 (or Rx3) antenna: 2450 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

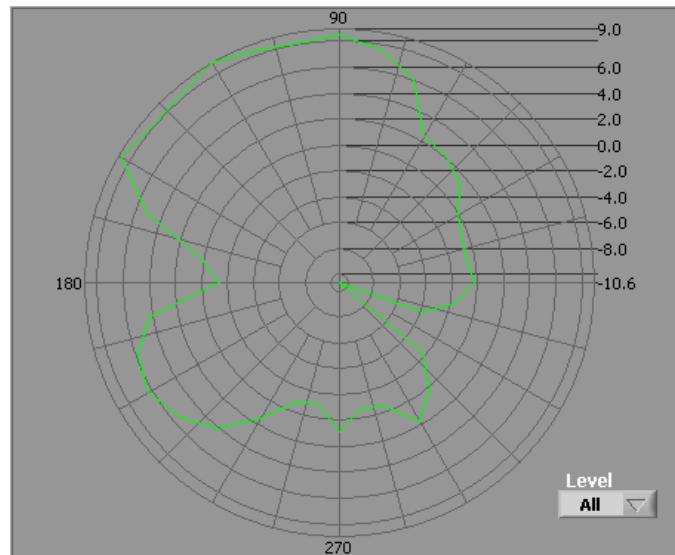

Total

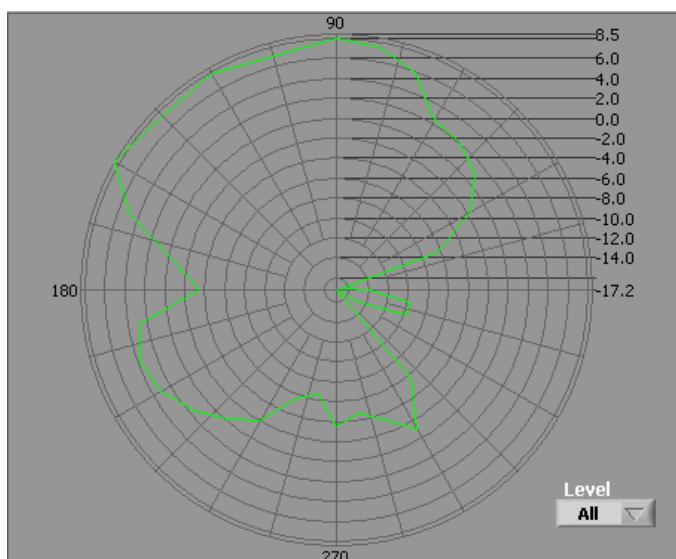


Horizontal

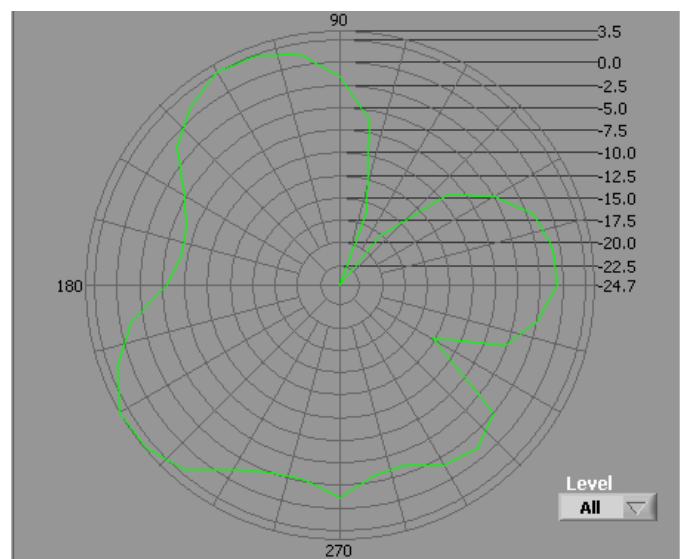


Vertical

Center Frequency	<b>2450 MHz</b>
Horizontal (dBi) peak	<b>-0.69</b>
Vertical (dBi) peak	<b>-3.12</b>


Tx3 (or Rx3) antenna: 2500 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for

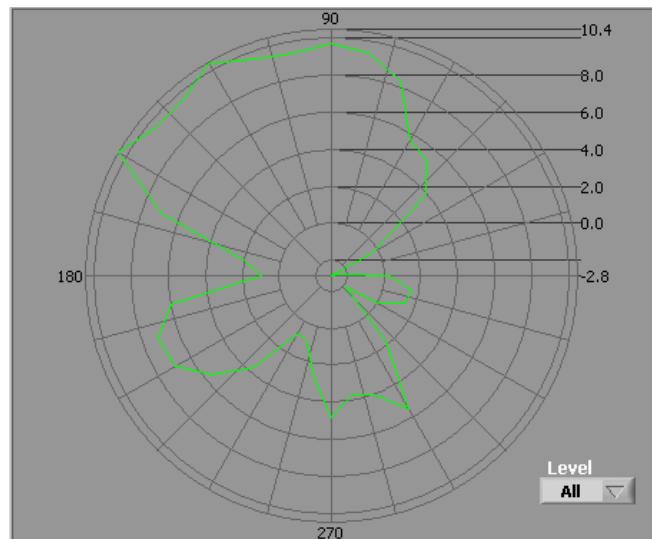

4965AGN)

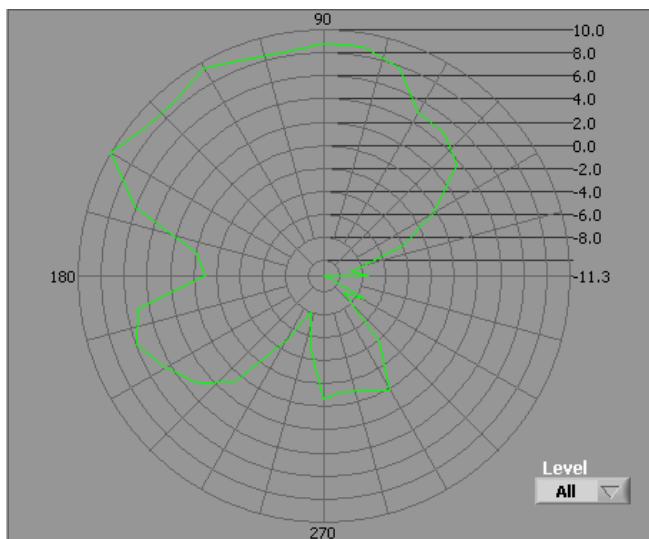

Horizontal



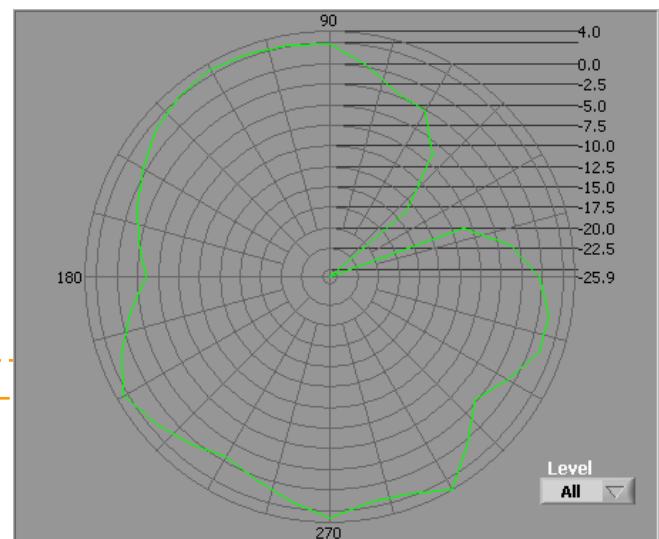


Vertical

Center Frequency	<b>2500 MHz</b>
Horizontal (dBi) peak	<b>-2</b>
Vertical (dBi) peak	<b>-2.87</b>


## 2490-2700MHz radiation characteristic

Tx1 antenna: 2500MHz

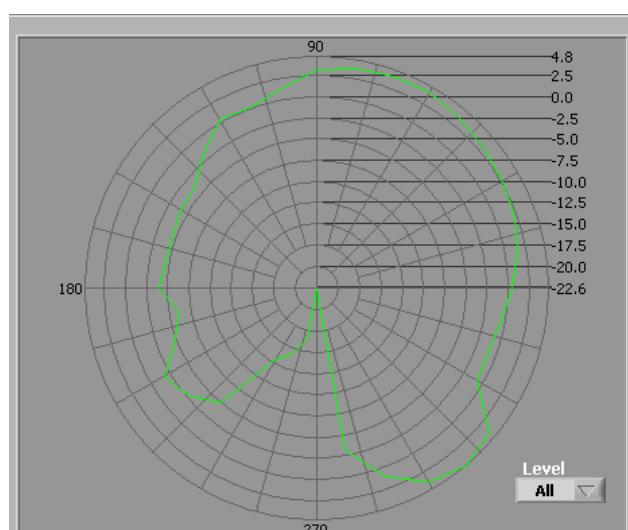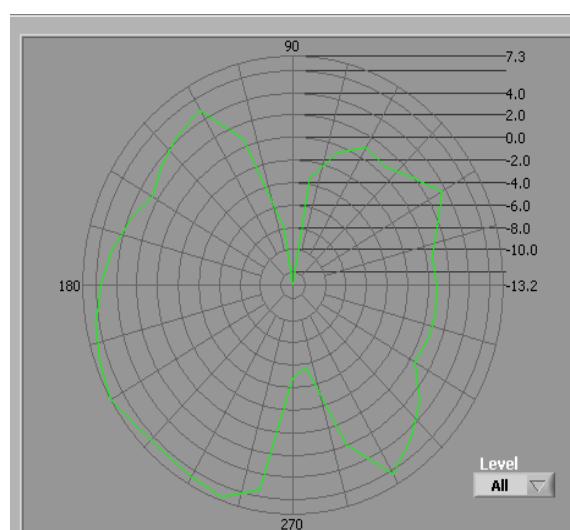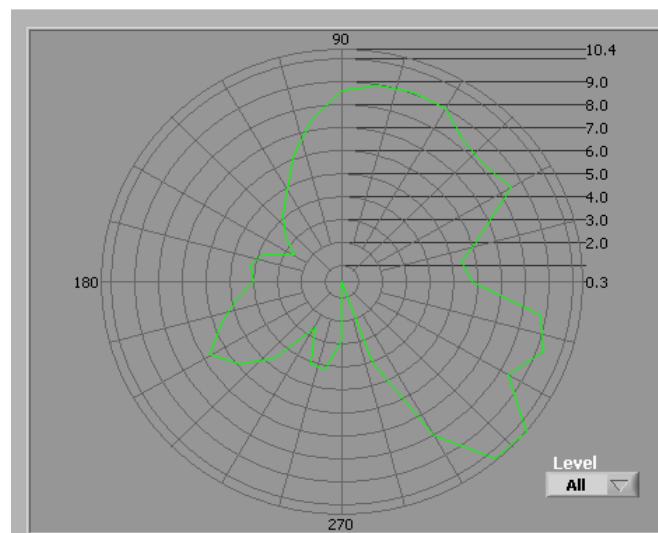


Center Frequency	<b>2500 MHz</b>
Horizontal (dBi) peak	<b>-3.97</b>
Vertical (dBi) peak	<b>-2.69</b>


## Tx1 antenna: 2600MHz

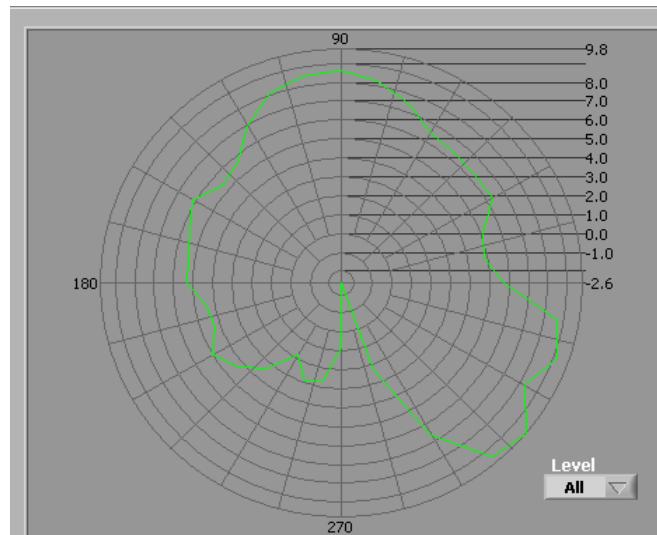

— Total —

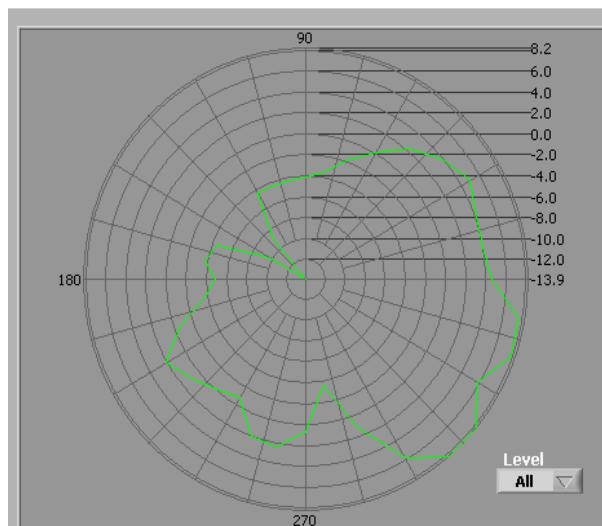


— Horizontal —

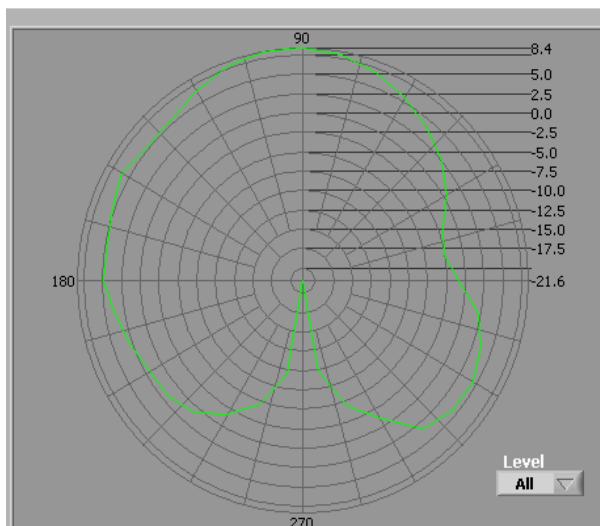


— Vertical —

Center Frequency	<b>2600 MHz</b>
Horizontal (dBi) peak	<b>-2.23</b>
Vertical (dBi) peak	<b>-3.06</b>


## Tx1 antenna: 2700 MHz

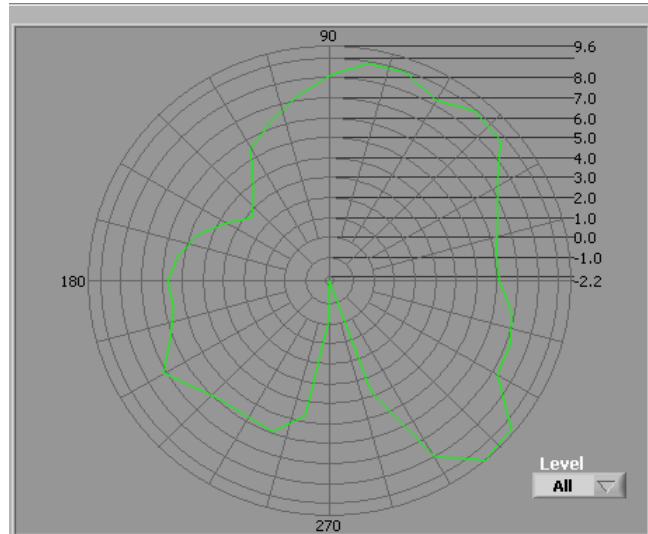

□ Total □

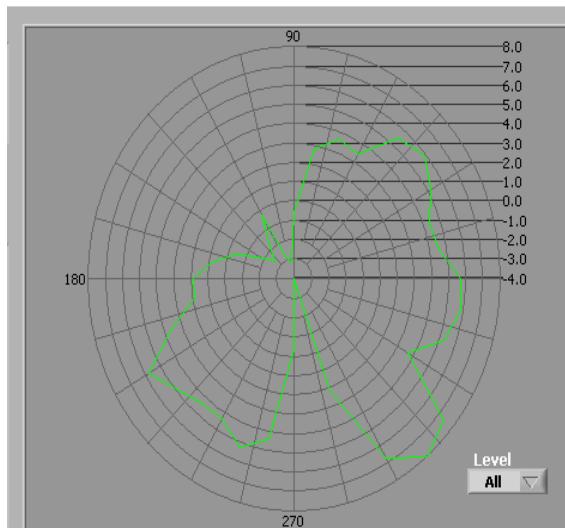


□ Horizontal □

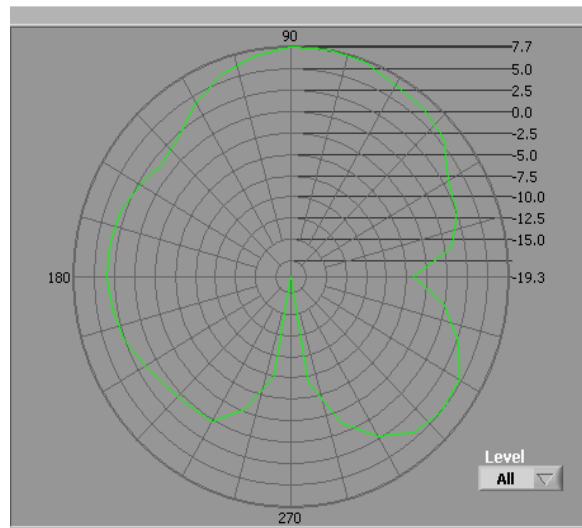


□ Vertical □

Center Frequency	<b>2700 MHz</b>
Horizontal (dBi) peak	<b>-2.78</b>
Vertical (dBi) peak	<b>-2.19</b>


Tx2 (or Rx2) antenna: 2500MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)

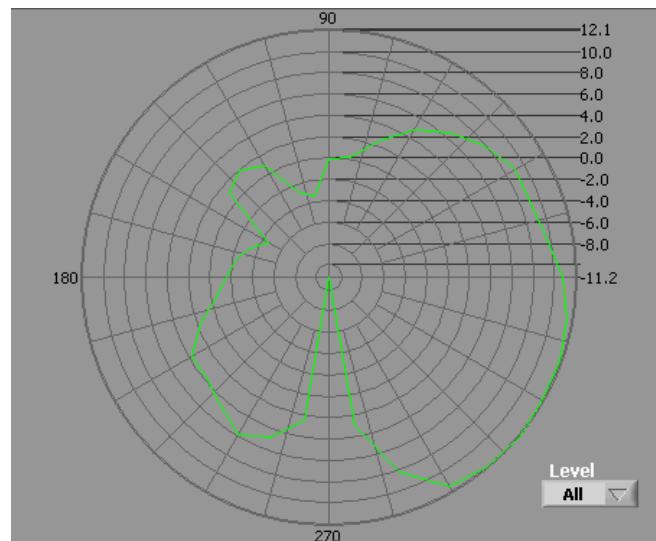

Total

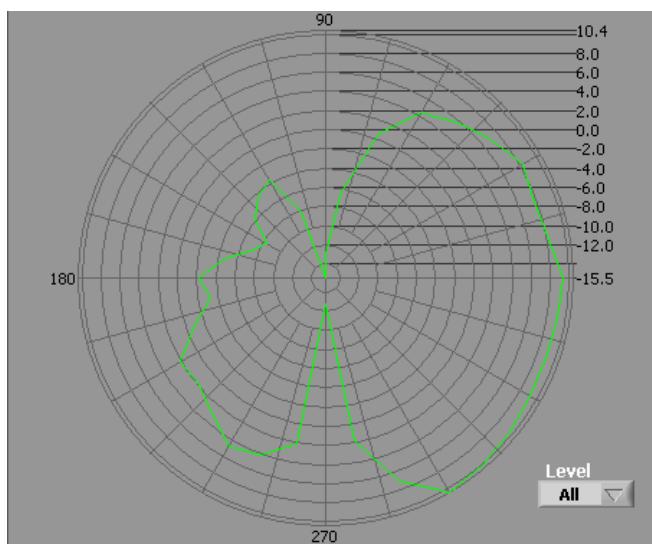

Horizontal

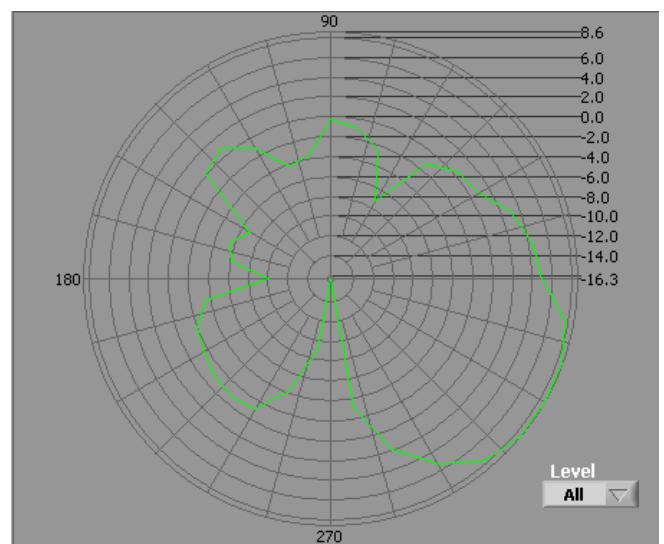


Vertical


Center Frequency	<b>2500 MHz</b>
Horizontal (dBi) peak	<b>-2.33</b>
Vertical (dBi) peak	<b>-2.41</b>

Tx2 (or Rx2) antenna: 2600MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)


1

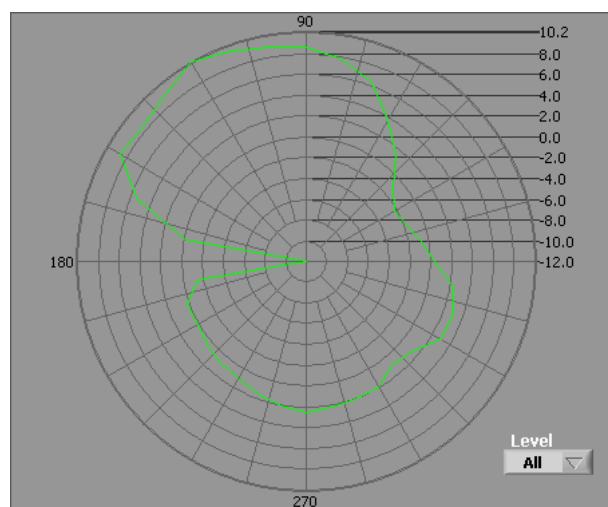

total

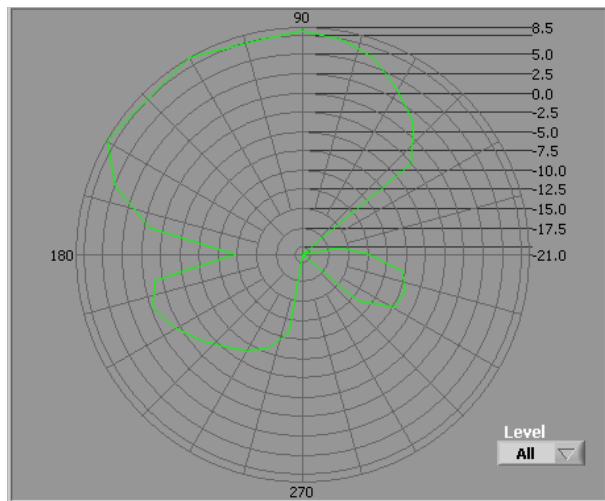


Horizontal

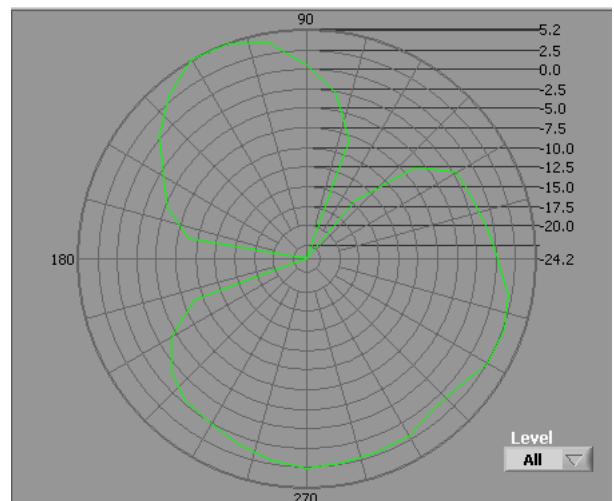


Vertical

Center Frequency	<b>2600 MHz</b>
Horizontal (dBi) peak	<b>-1.62</b>
Vertical (dBi) peak	<b>-5.19</b>


**Tx2 (or Rx2) antenna: 2700 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)**

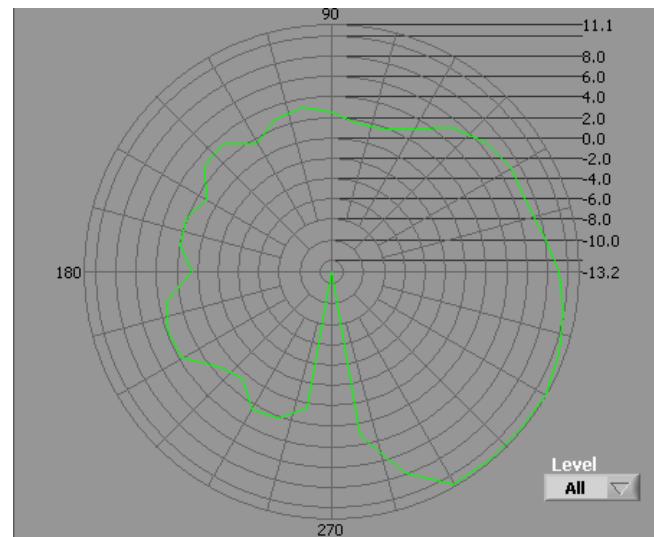

**Total**

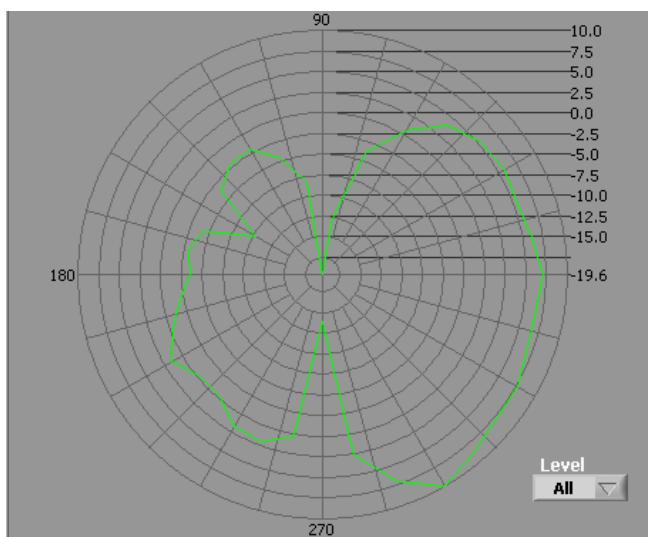


**Horizontal**

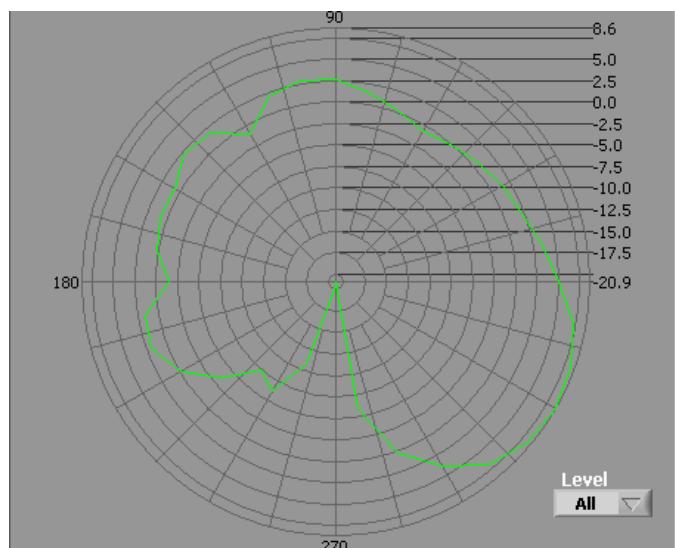


**Vertical**

Center Frequency	<b>2700 MHz</b>
Horizontal (dBi) peak	<b>-3.20</b>
Vertical (dBi) peak	<b>-2.54</b>


**Tx3 (or Rx3) antenna: 2500 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

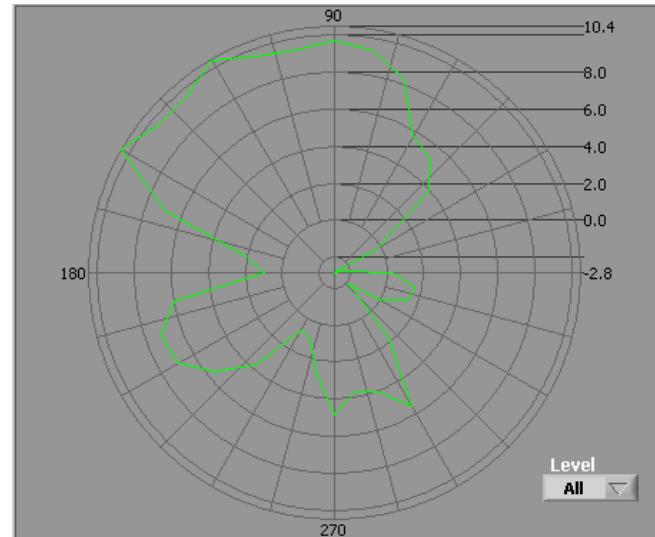

 Total

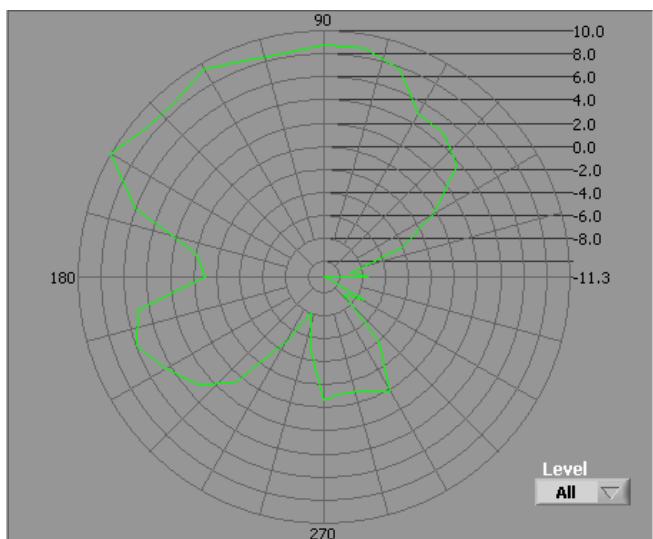


 Horizontal

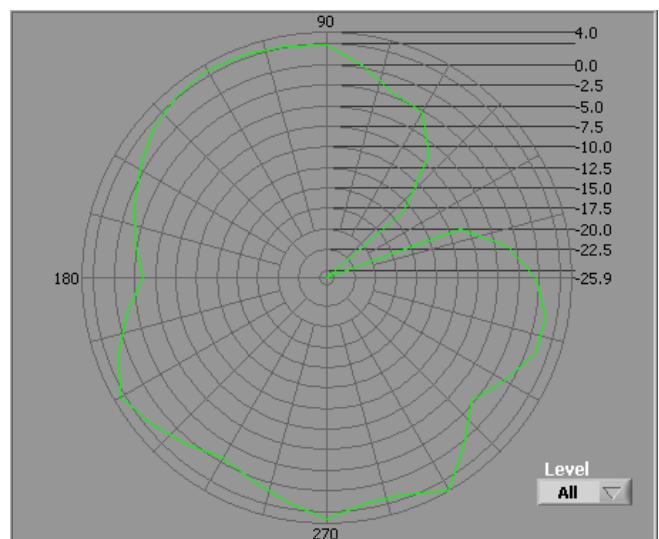


 Vertical

Center Frequency	<b>2500 MHz</b>
Horizontal (dBi) peak	<b>-2</b>
Vertical (dBi) peak	<b>-2.87</b>


**Tx3 (or Rx3) antenna: 2600MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

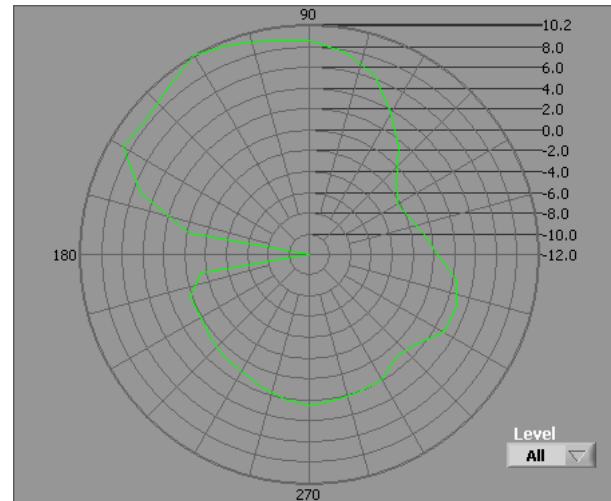

Total

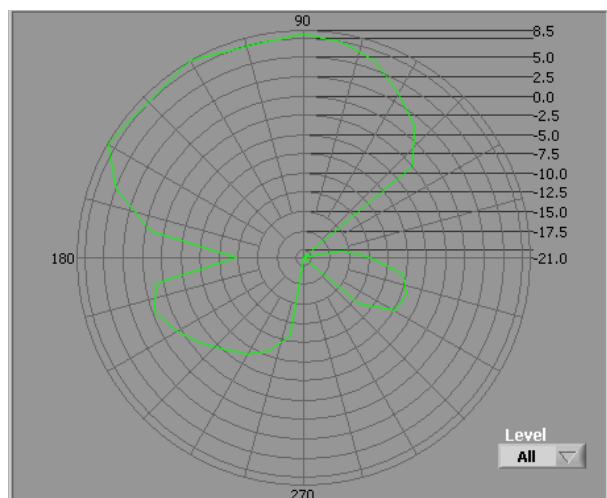


Horizontal

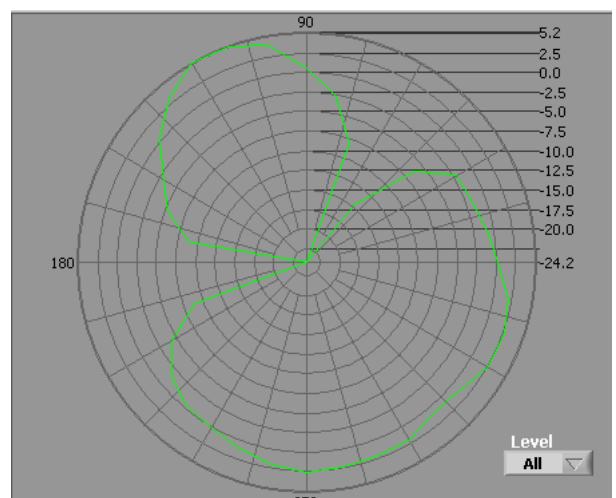


Vertical

Center Frequency	<b>2600 MHz</b>
Horizontal (dBi) peak	<b>-1.35</b>
Vertical (dBi) peak	<b>-3.63</b>


**Tx3 (or Rx3) antenna: 2700 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

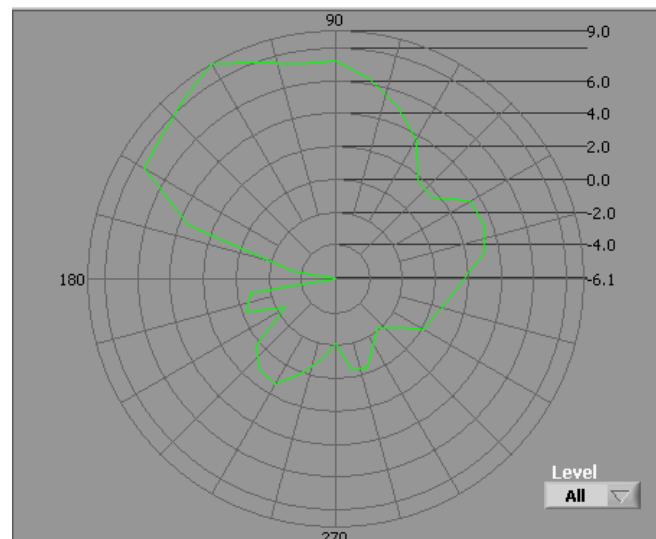

Total

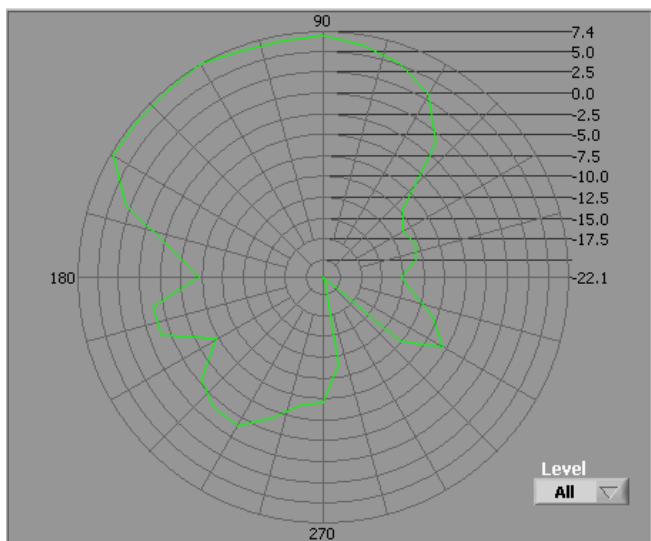

Horizontal


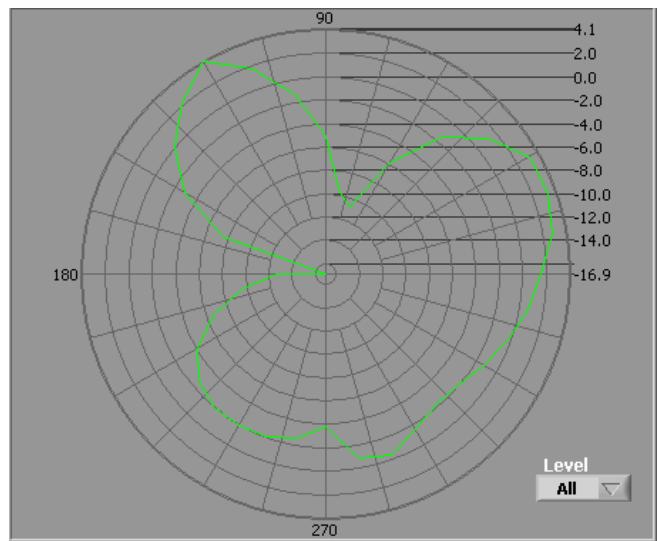


Vertical

Center Frequency	<b>2700 MHz</b>
Horizontal (dBi) peak	<b>-2.75</b>
Vertical (dBi) peak	<b>-3.1</b>



## 5150-5350 MHz radiation characteristic

### Tx1 antenna: 5150 MHz

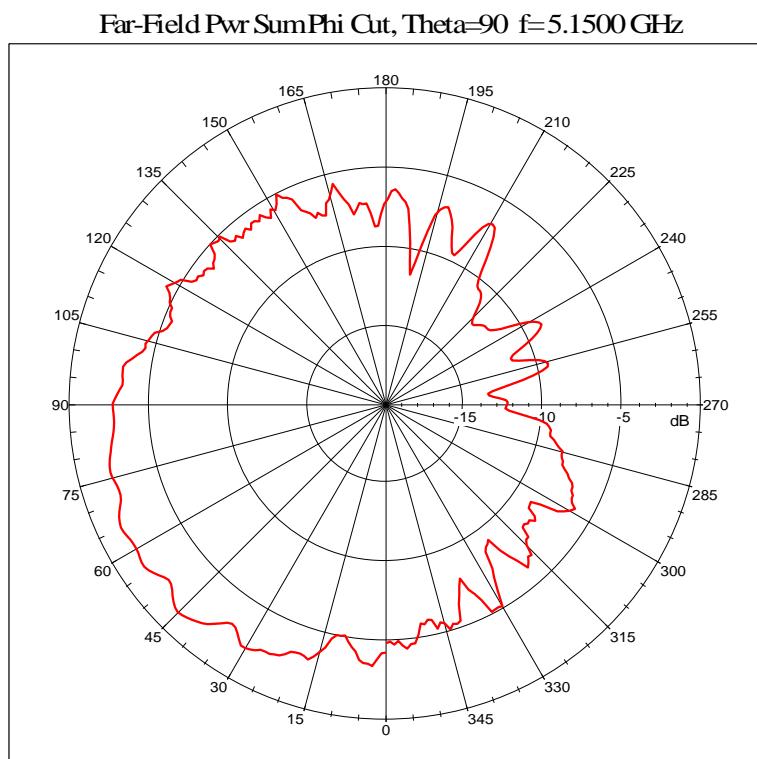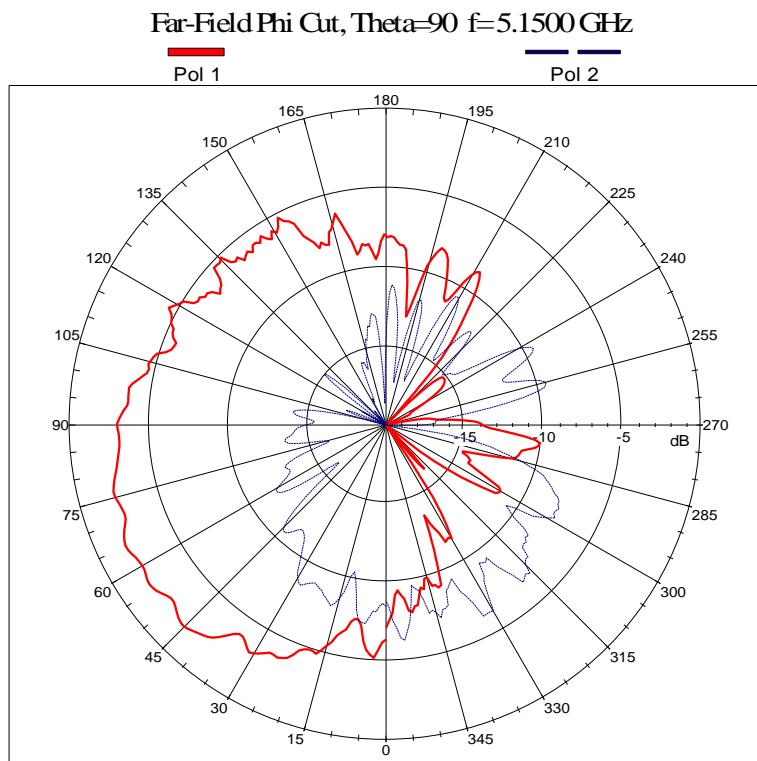



Center Frequency	<b>5150 MHz</b>
Horizontal (dBi) peak	<b>-6.38</b>
Vertical (dBi) peak	<b>-1.88</b>

**Tx2 (or Rx2) antenna: 5150 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)**

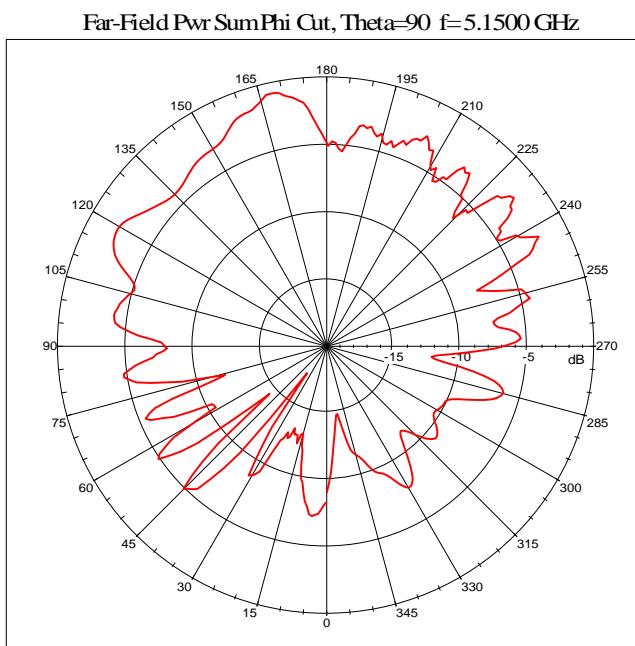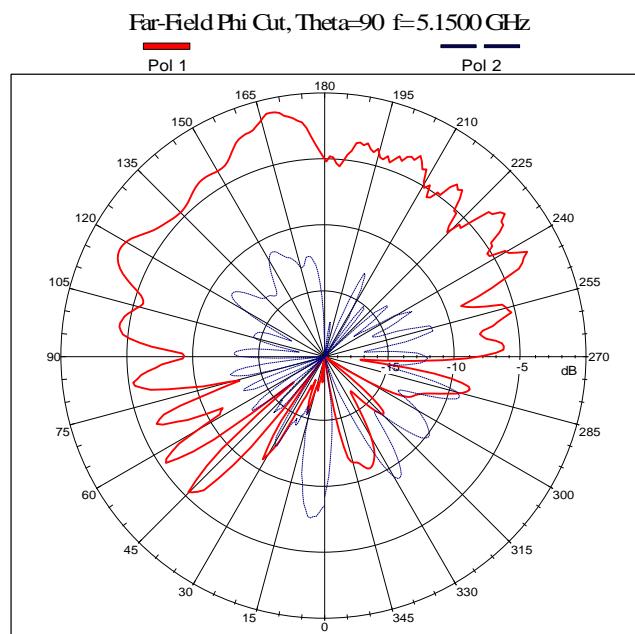

Center Frequency	<b>5150 MHz</b>
Horizontal (dBi) peak	-7.721
Vertical (dBi) peak	-1.071



**Tx3 (or Rx3) antenna: 5150 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

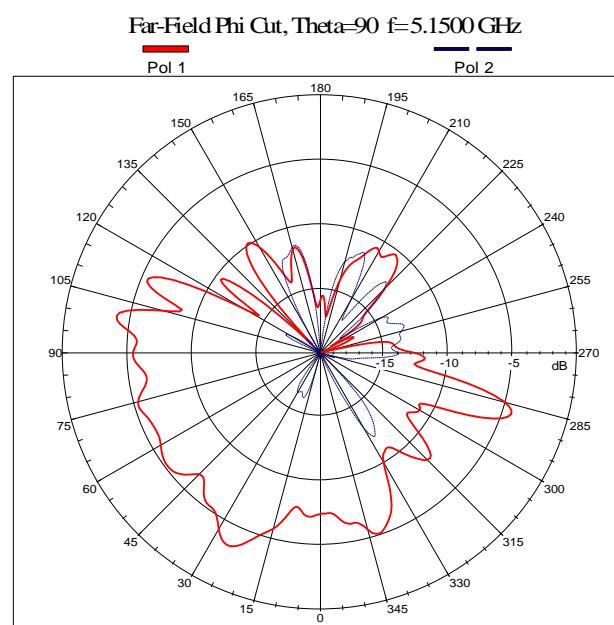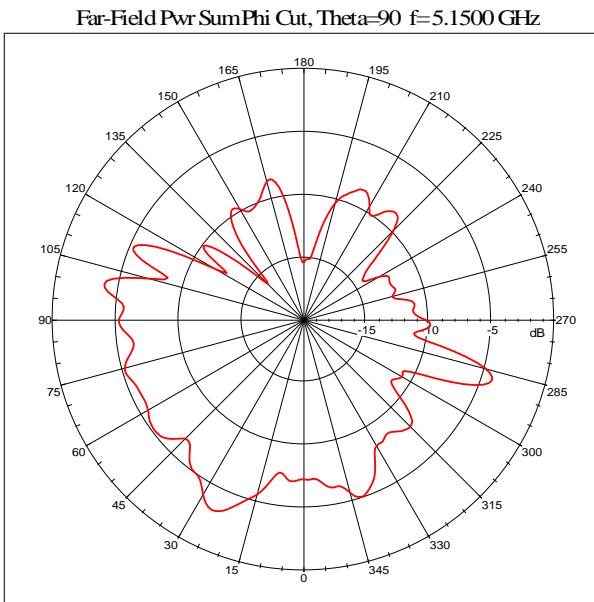

Center Frequency	<b>5150 MHz</b>
Horizontal (dBi) peak	<b>-11.4</b>
Vertical (dBi) peak	<b>-3.46</b>



## 5470-5725MHz radiation characteristic

### Tx1 antenna: 5470 MHz

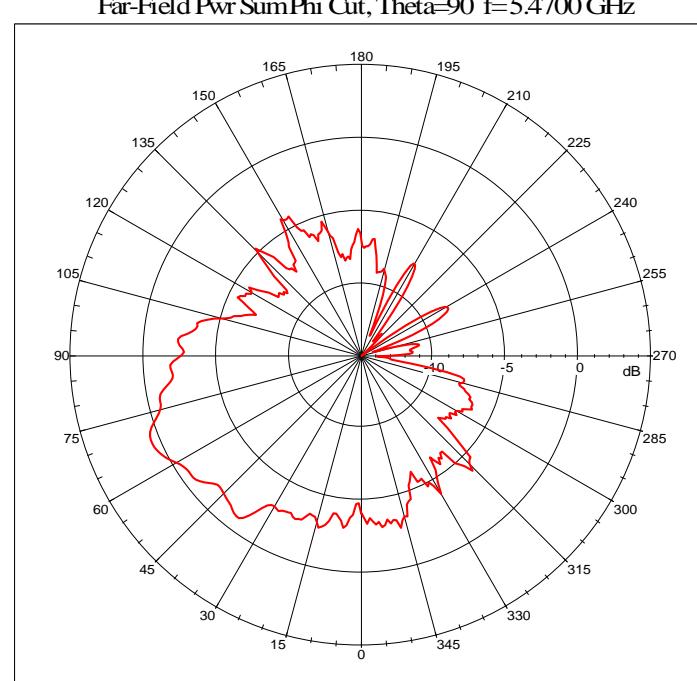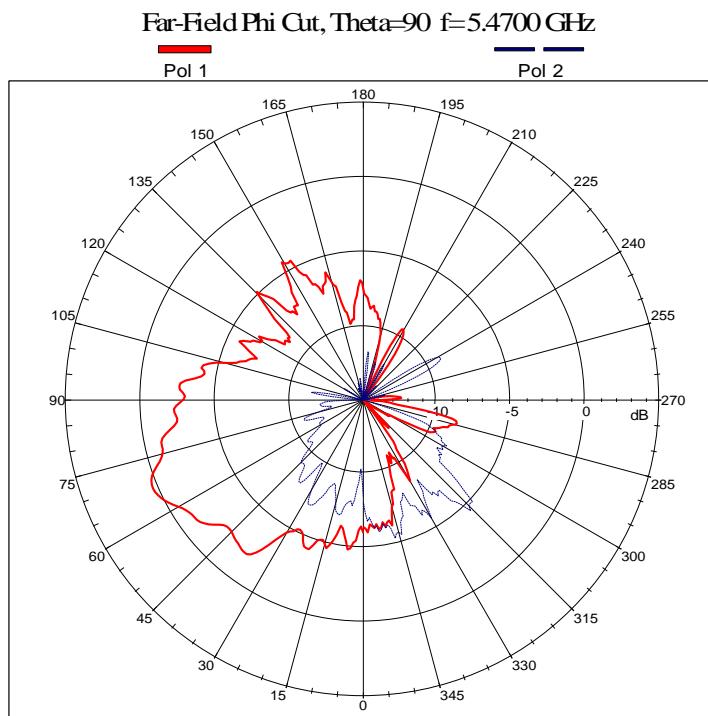

Center Frequency	<b>5470 MHz</b>
Horizontal (dBi) peak	<b>-4.66</b>
Vertical (dBi) peak	<b>0.30</b>


## Tx1 antenna: 5600 MHz

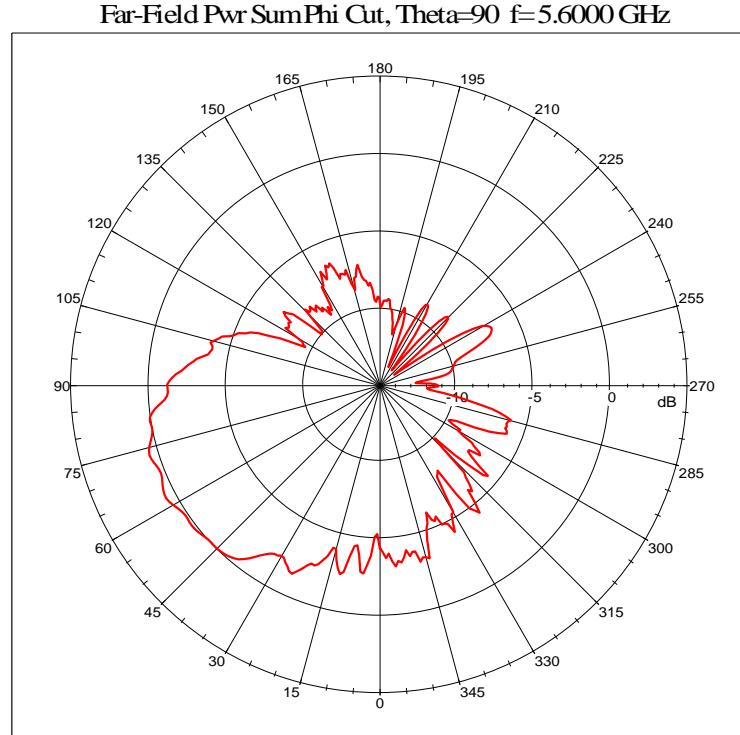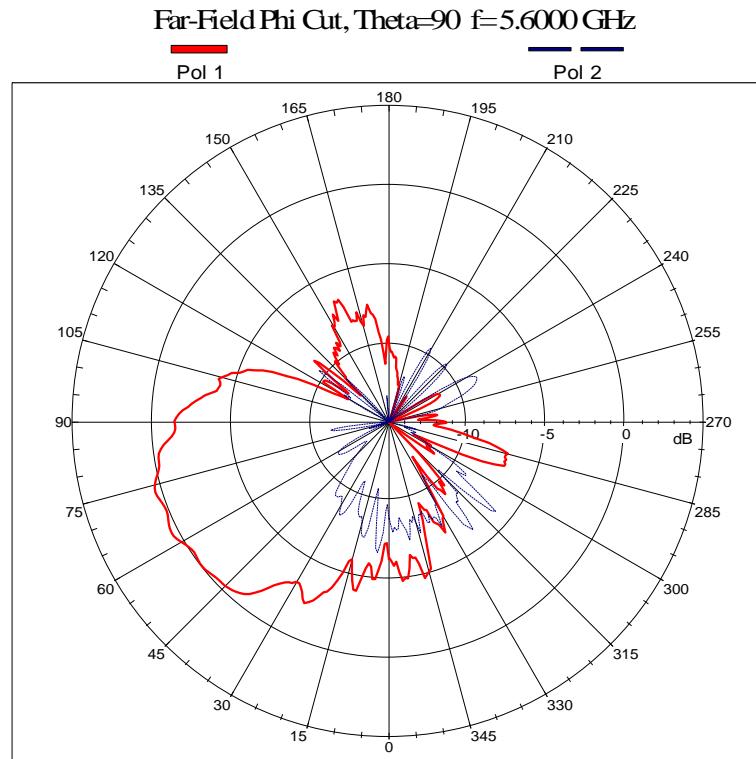


Center Frequency	<b>5600 MHz</b>
Horizontal (dBi) peak	<b>-6.23</b>
Vertical (dBi) peak	<b>0.40</b>

**Tx1 antenna: 5725 MHz**

Far-Field Phi Cut, Theta=90 f=5.7250 GHz


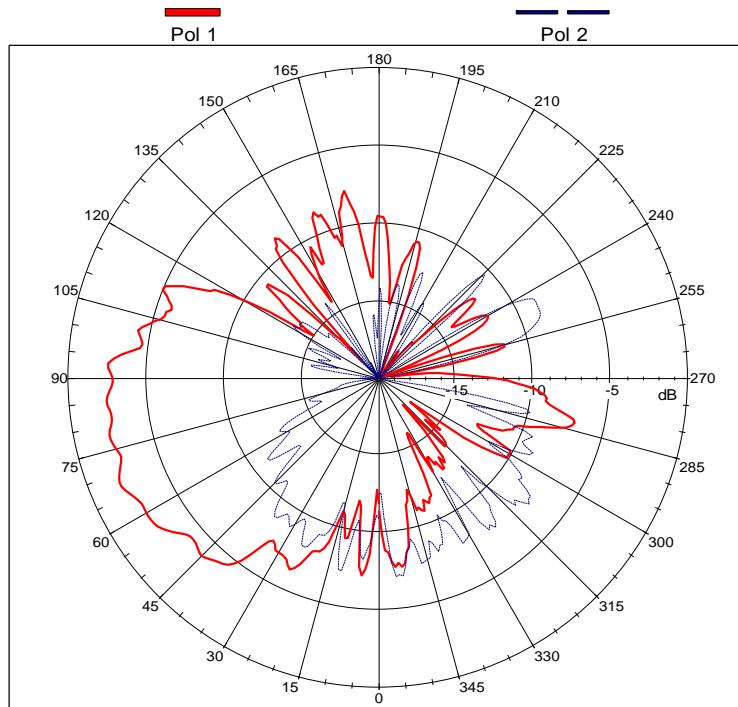


Far-Field Pwr SumPhi Cut, Theta=90 f=5.7250 GHz

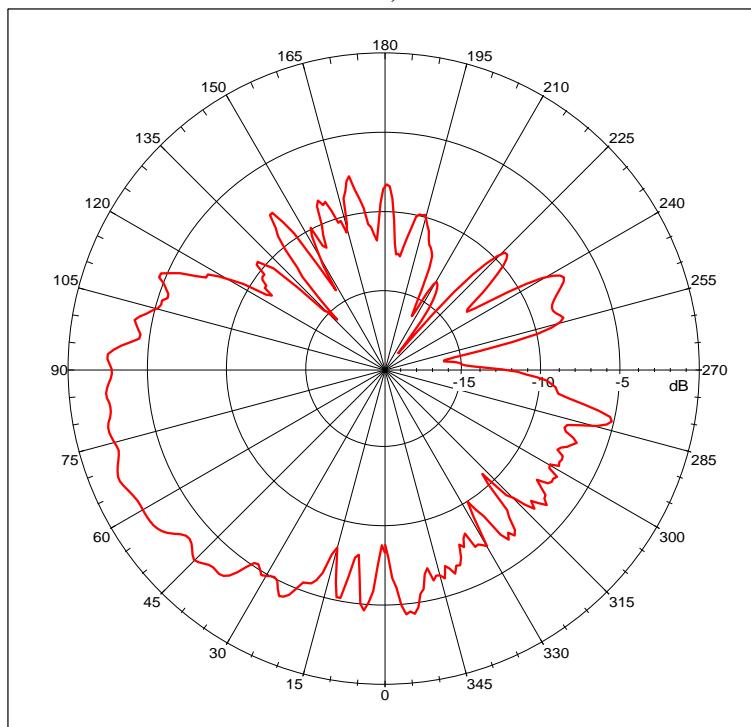



Center Frequency	<b>5725 MHz</b>
Horizontal (dBi) peak	<b>-7.23</b>
Vertical (dBi) peak	<b>-2.04</b>

**Tx2 (or Rx2) antenna: 5470 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)**

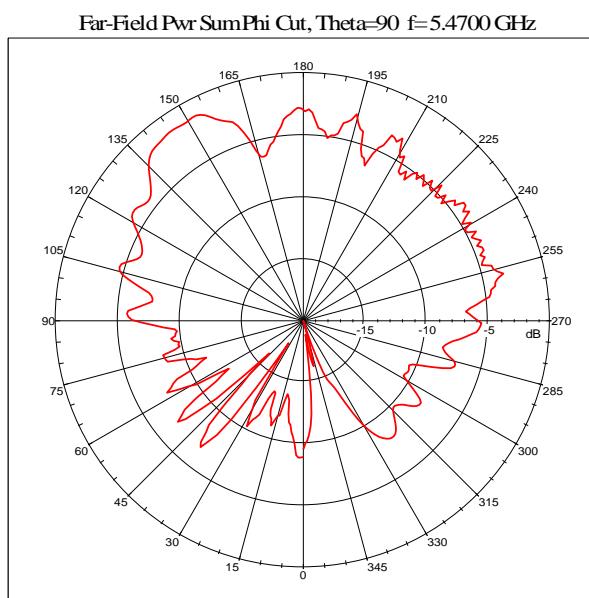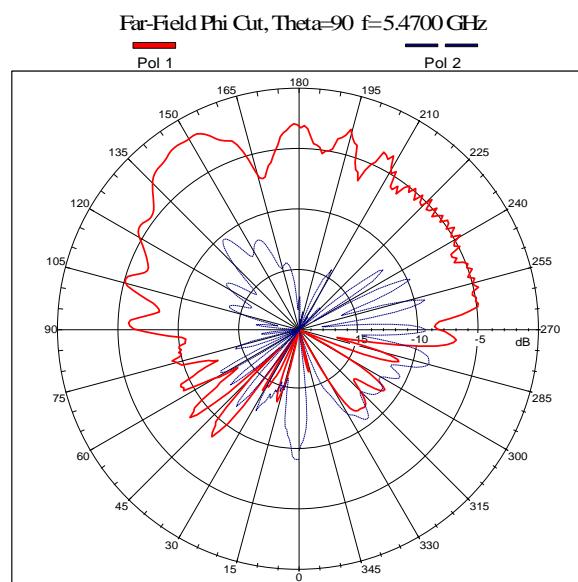



Center Frequency	<b>5470 MHz</b>
Horizontal (dBi) peak	<b>-8.86</b>
Vertical (dBi) peak	<b>-1.71</b>

**Tx2 (or Rx2) antenna: 5600 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)**

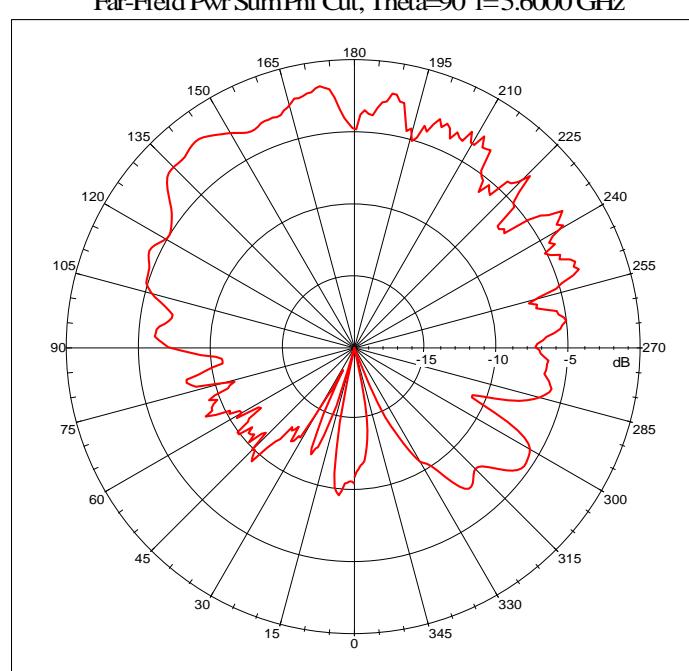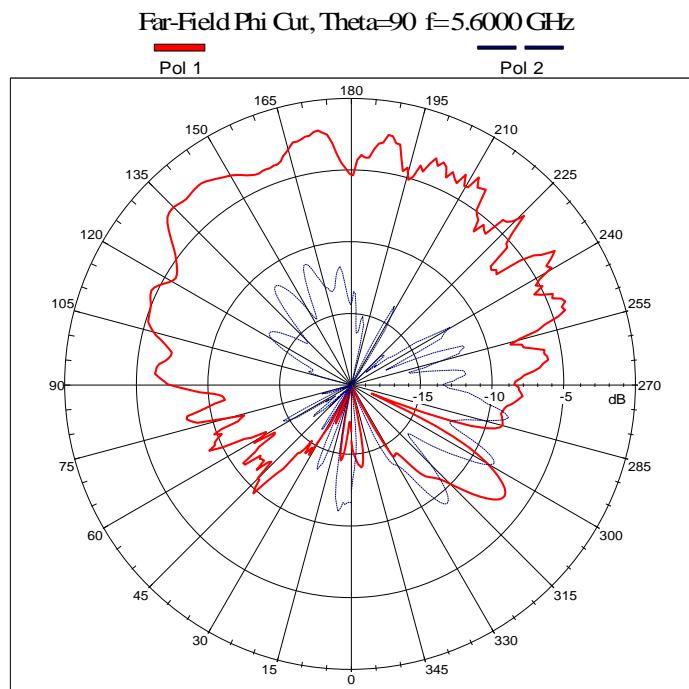

Center Frequency	<b>5600 MHz</b>
Horizontal (dBi) peak	<b>-8.63</b>
Vertical (dBi) peak	<b>-2.10</b>


**Tx2 (or Rx2) antenna: 5725 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)**

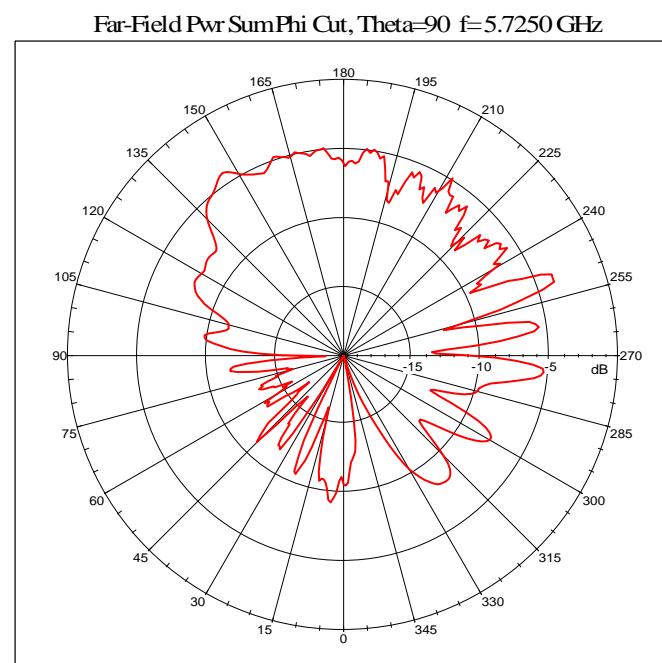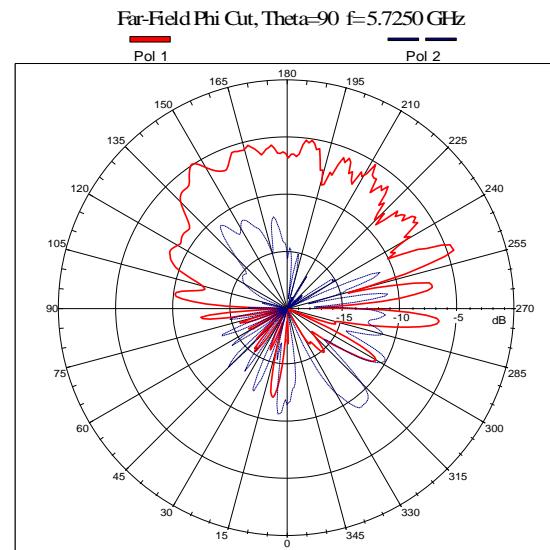


Center Frequency	<b>5725 MHz</b>
Horizontal (dBi) peak	<b>-9.22</b>
Vertical (dBi) peak	<b>-4.55</b>

**Tx3 (or Rx3) antenna: 5470 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

Far-Field Phi Cut, Theta=90 f=5.4700 GHz


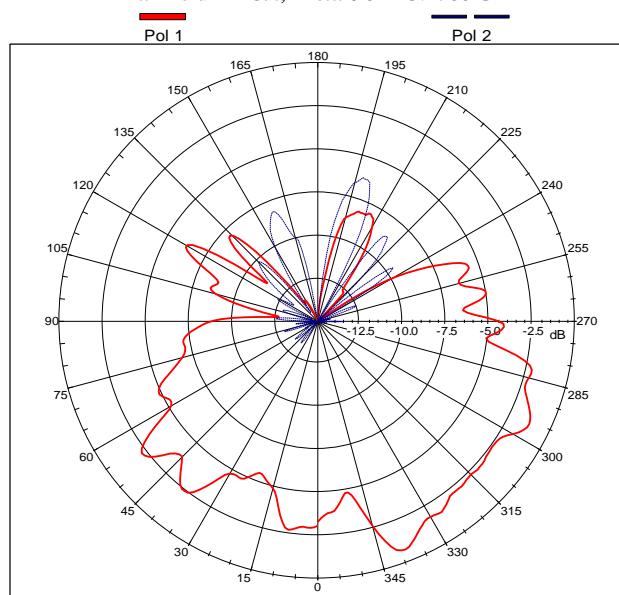


Far-Field Pwr SumPhi Cut, Theta=90 f=5.4700 GHz

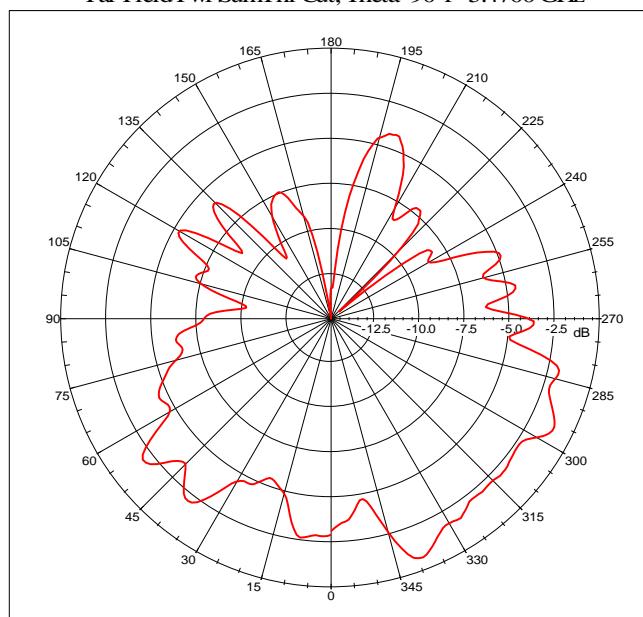



Center Frequency	<b>5470 MHz</b>
Horizontal (dBi) peak	<b>-6.28</b>
Vertical (dBi) peak	<b>-0.83</b>

**Tx3 (or Rx3) antenna: 5600 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

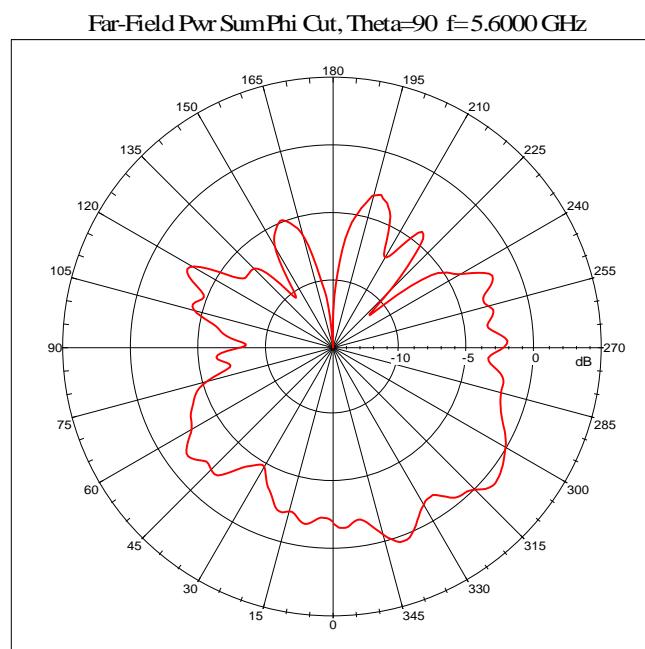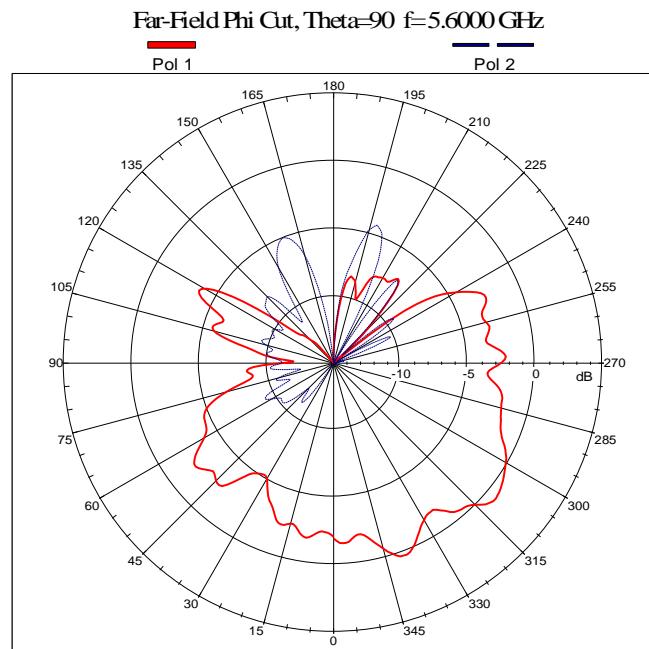

Center Frequency	<b>5600 MHz</b>
Horizontal (dBi) peak	<b>-4.3</b>
Vertical (dBi) peak	<b>-0.64</b>



**Tx3 (or Rx3) antenna: 5750 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

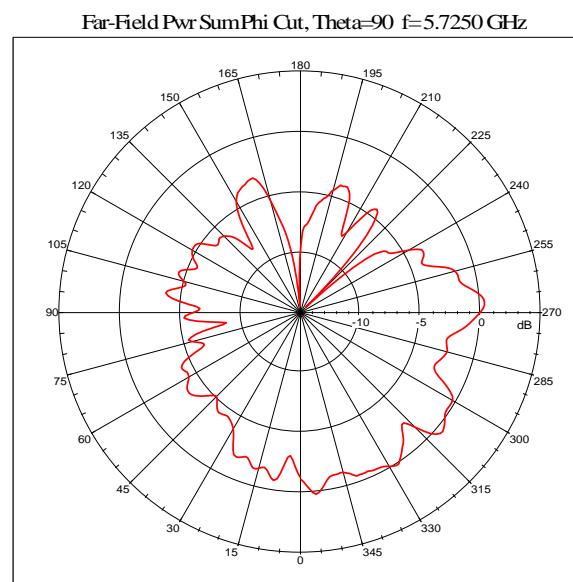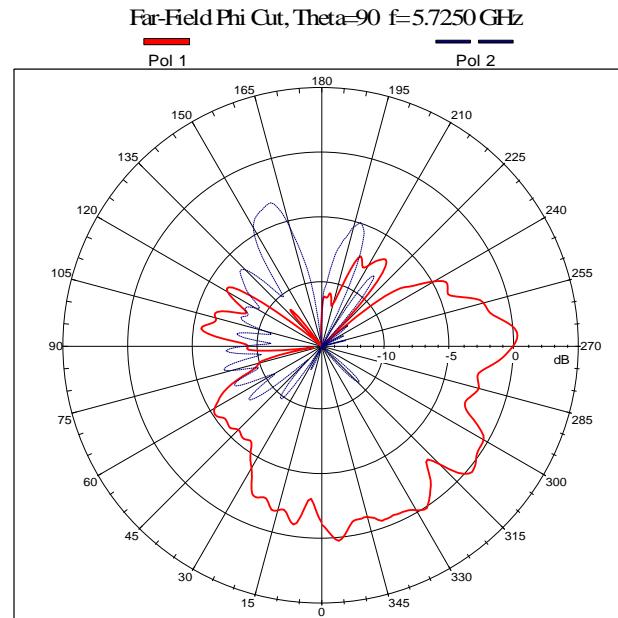

Center Frequency	<b>5725 MHz</b>
Horizontal (dBi) peak	<b>-3.24</b>
Vertical (dBi) peak	<b>0.15</b>

## 5725-5850 MHz radiation characteristic


### Tx1 antenna: 5725 MHz

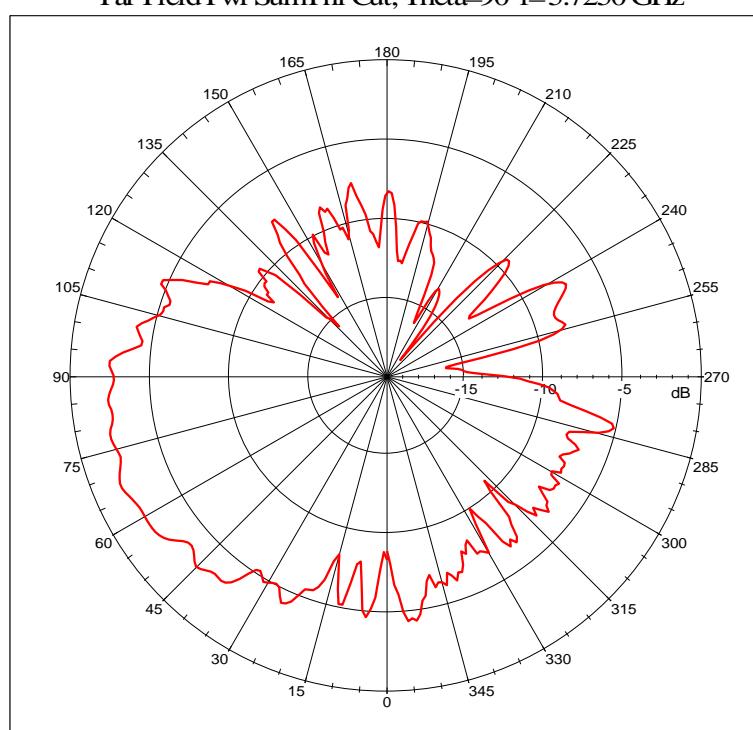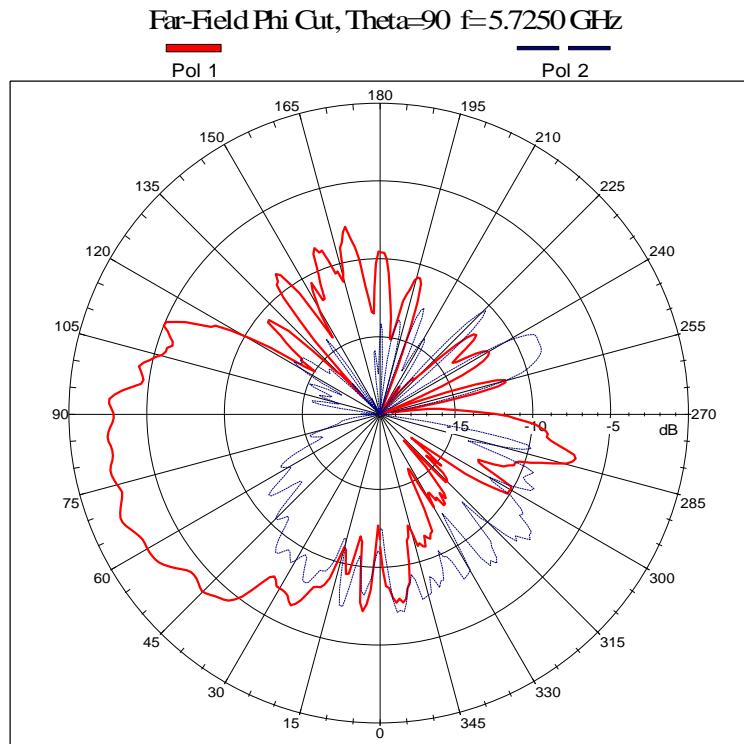


Center Frequency	<b>5725 MHz</b>
Horizontal (dBi) peak	<b>-7.23</b>
Vertical (dBi) peak	<b>-2.04</b>

## Tx1 antenna: 5850 MHz

Far-Field Phi Cut, Theta=90 f=5.8500 GHz


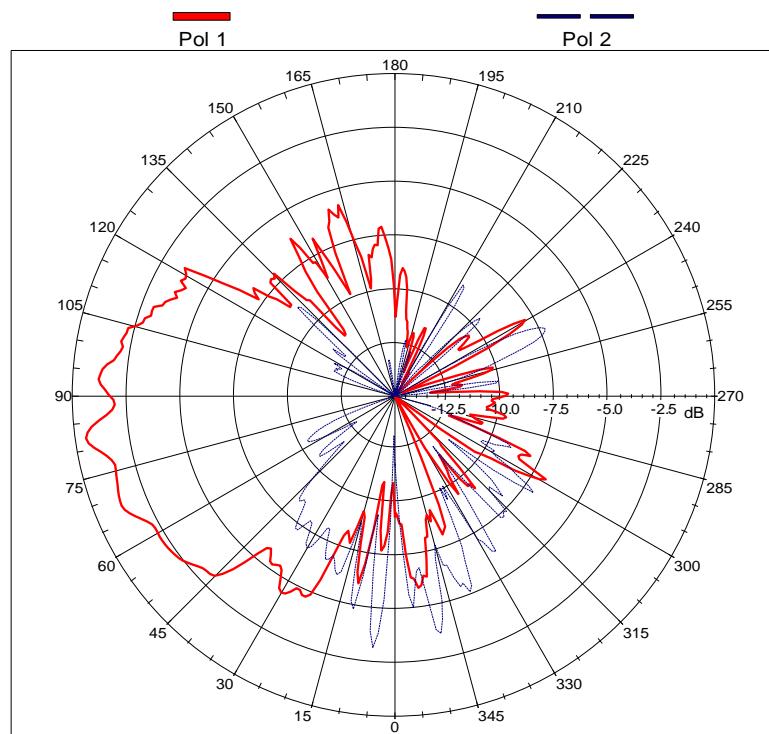


Far-Field Pwr SumPhi Cut, Theta=90 f=5.8500 GHz

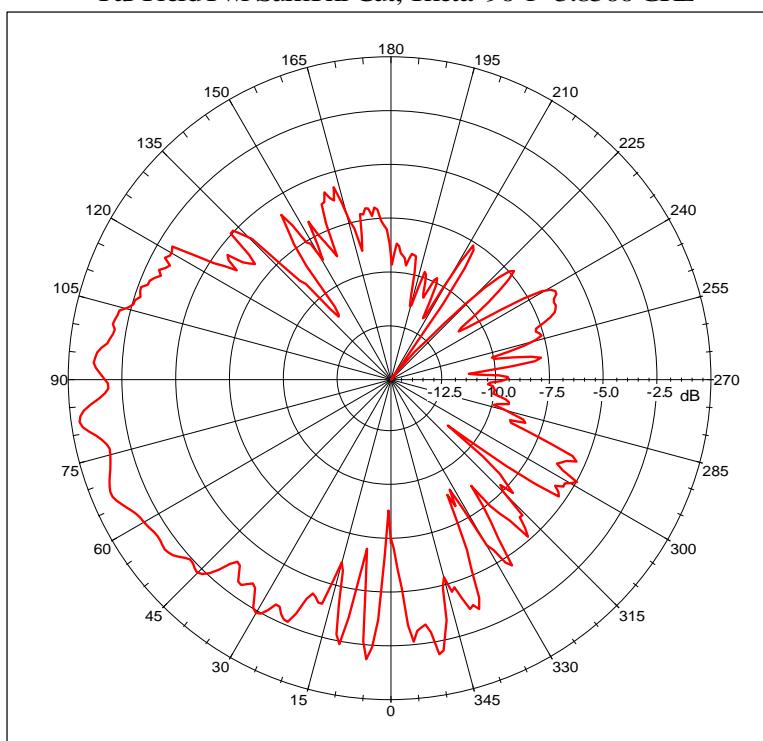



Center Frequency	<b>5850 MHz</b>
Horizontal (dBi) peak	<b>-3.27</b>
Vertical (dBi) peak	<b>-0.52</b>

**Tx2 (or Rx2) antenna: 5725 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)**

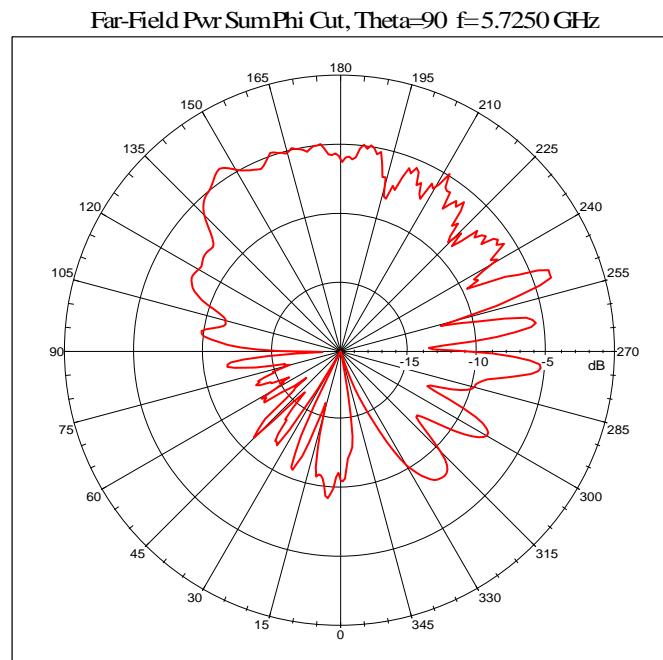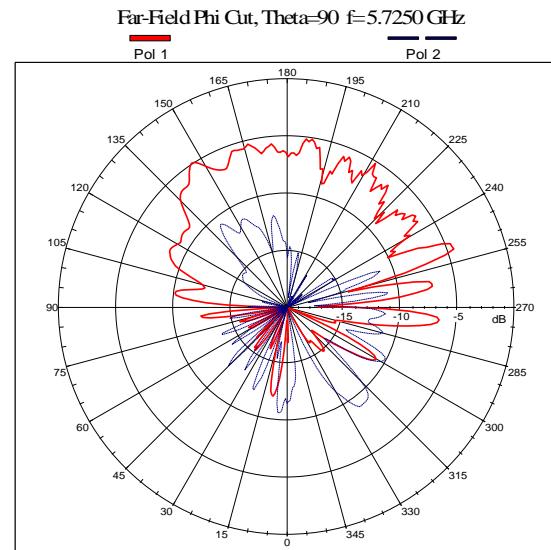



Center Frequency	<b>5725 MHz</b>
Horizontal (dBi) peak	<b>-9.22</b>
Vertical (dBi) peak	<b>-4.55</b>

**Tx2 (or Rx2) antenna: 5850 MHz (Plot is not required if 2<sup>nd</sup> Antenna is receive only e.g. Rx2 for 512 family)**

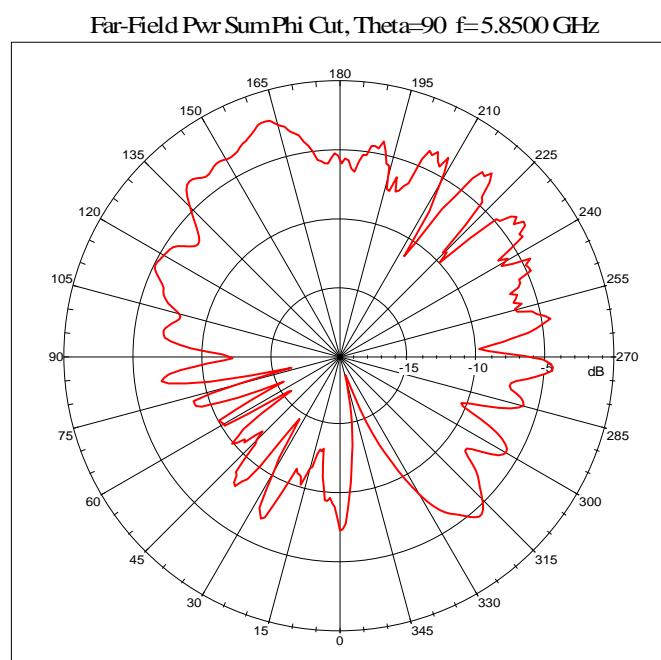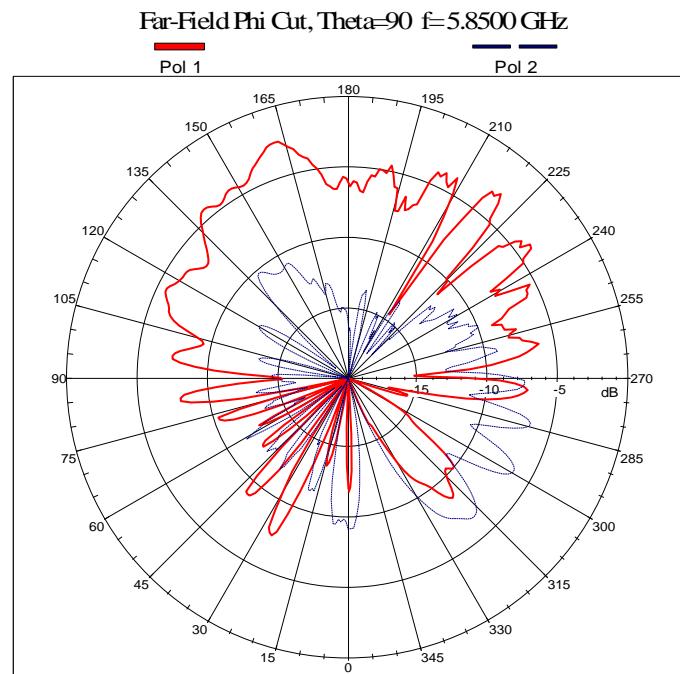



Center Frequency	<b>5850 MHz</b>
Horizontal (dBi) peak	<b>-6.55</b>
Vertical (dBi) peak	<b>-2.49</b>

**Tx3 (or Rx3) antenna: 5725 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

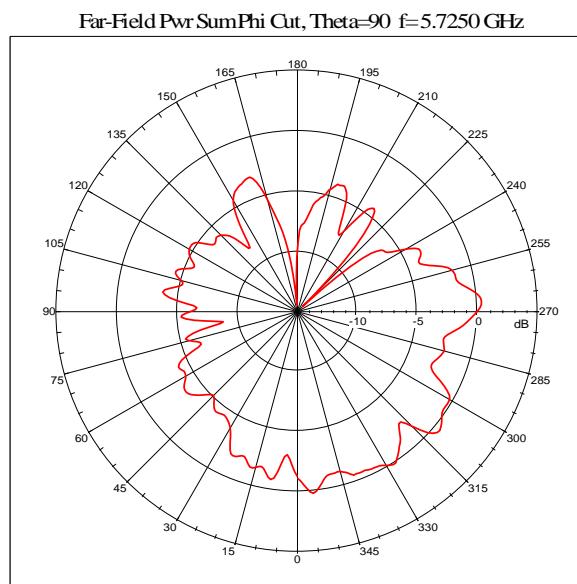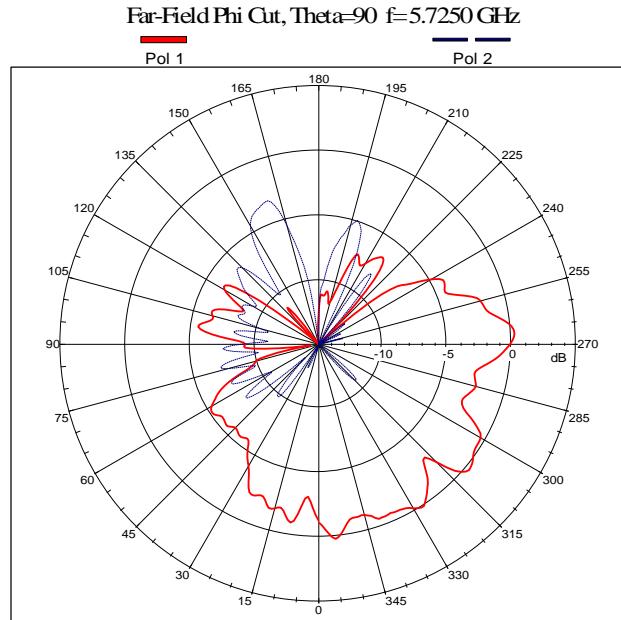

Center Frequency	<b>5725 MHz</b>
Horizontal (dBi) peak	<b>-3.24</b>
Vertical (dBi) peak	<b>0.15</b>

**Tx3 (or Rx3) antenna: 5850 MHz (Plot is not required if 3<sup>rd</sup> Antenna is receive only e.g. Rx3 for 4965AGN)**

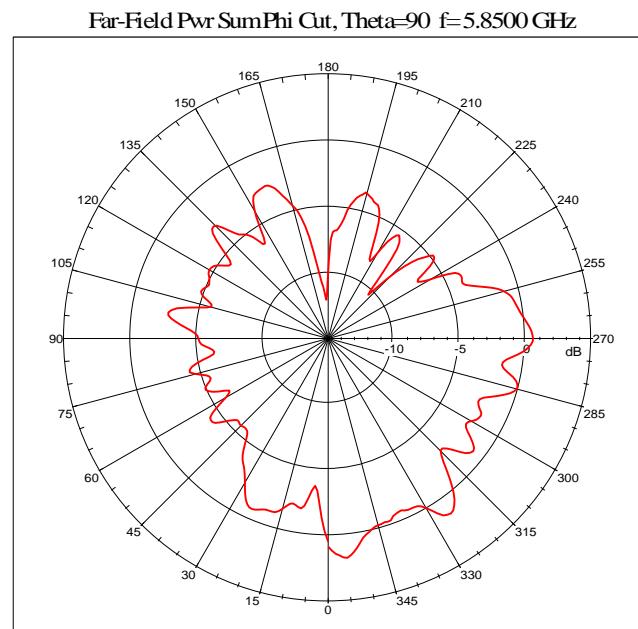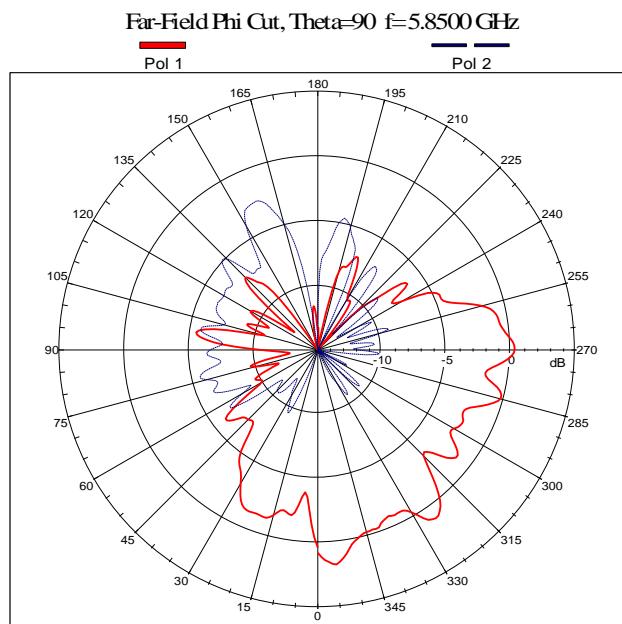

Center Frequency	<b>5850 MHz</b>
Horizontal (dBi) peak	<b>-2.57</b>
Vertical (dBi) peak	<b>-1.63</b>


## Section 4. Host Platform Information

OEM / ODM Host platform: (XXXXXXX) platform correlated to antenna data

Rating Label Photo:


## Section 5. Antenna Host Platform Location Information

Include a **dimensioned photo or dimensioned drawing** of Tx1, Tx2 and Tx3 antenna placements (measurements are not required for receive-only antenna). Any antenna that transmits must show dimensions to bottom of laptop.

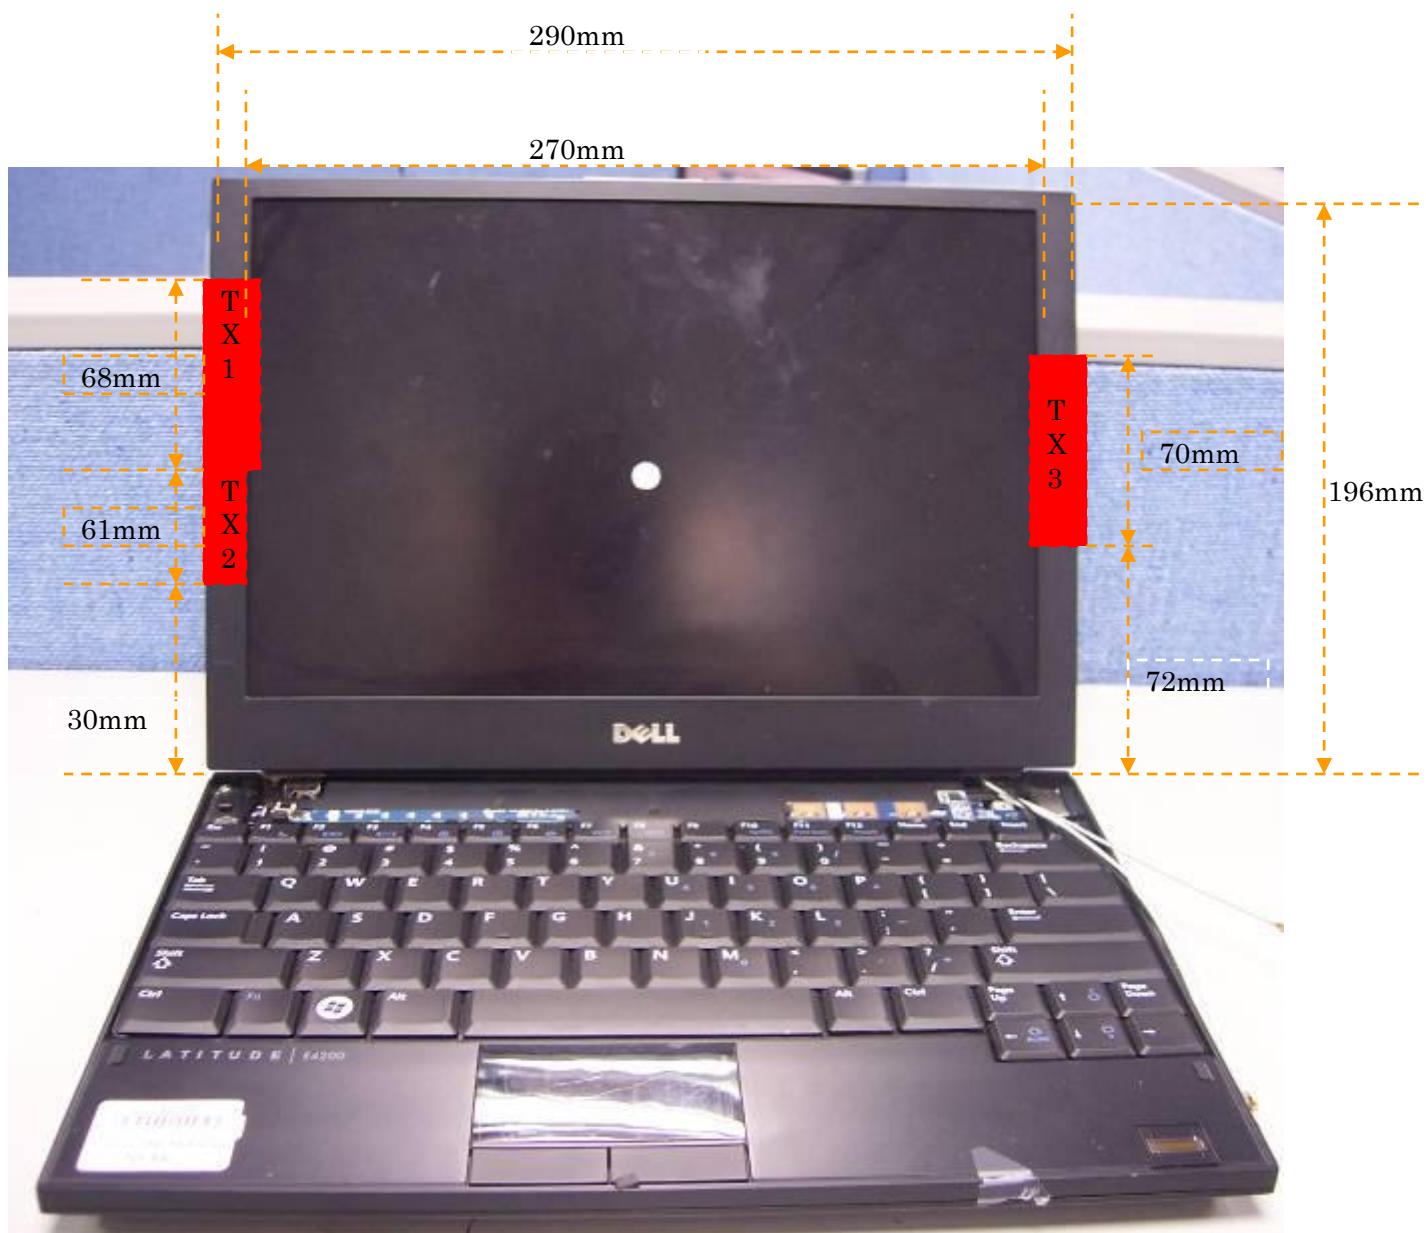

## Section 6. Antenna dimensional information for SAR evaluation


Include a **dimensioned photo or dimensioned drawing** showing the distance (mm) between the transmit antennas and the user (excluding hands, wrist, feet, lap/ thigh, and ankle)

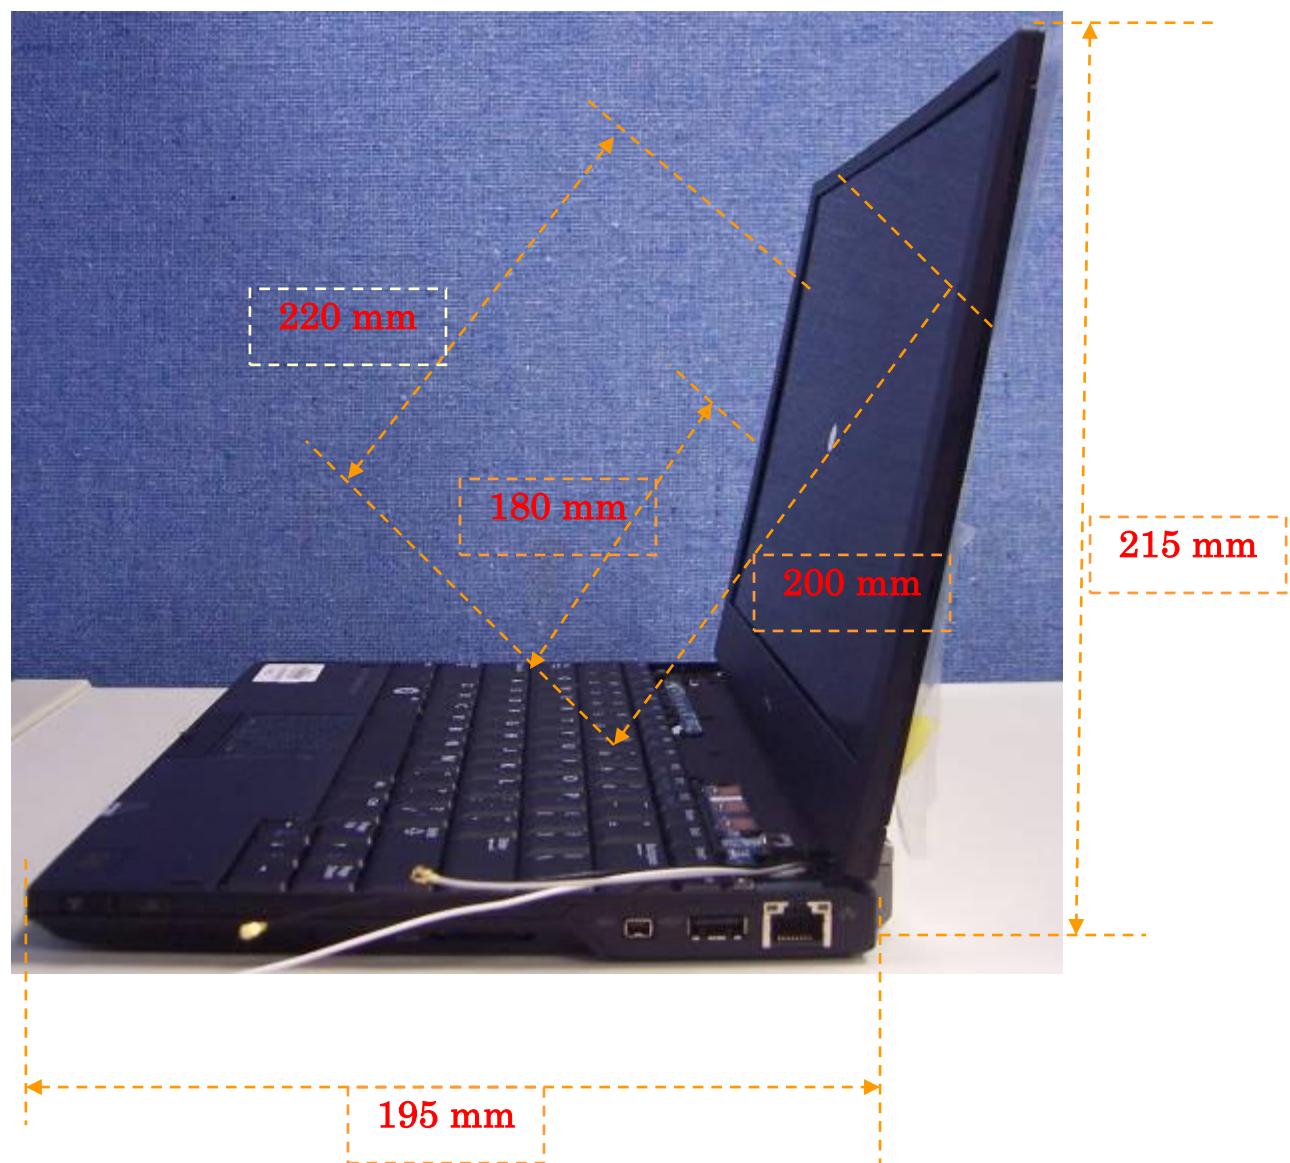

## Section 7. Diagram Example of Co-Location Antenna Separation

Include a **dimensioned photo** or **dimensioned drawing** showing the distance (mm) between all WLAN transmit antennas and other co-located radiator transmit antenna such as Bluetooth, WWAN,..

(Note: Due to the evolving rules regarding co-location, each platform will need to be reviewed on a case by case basis)

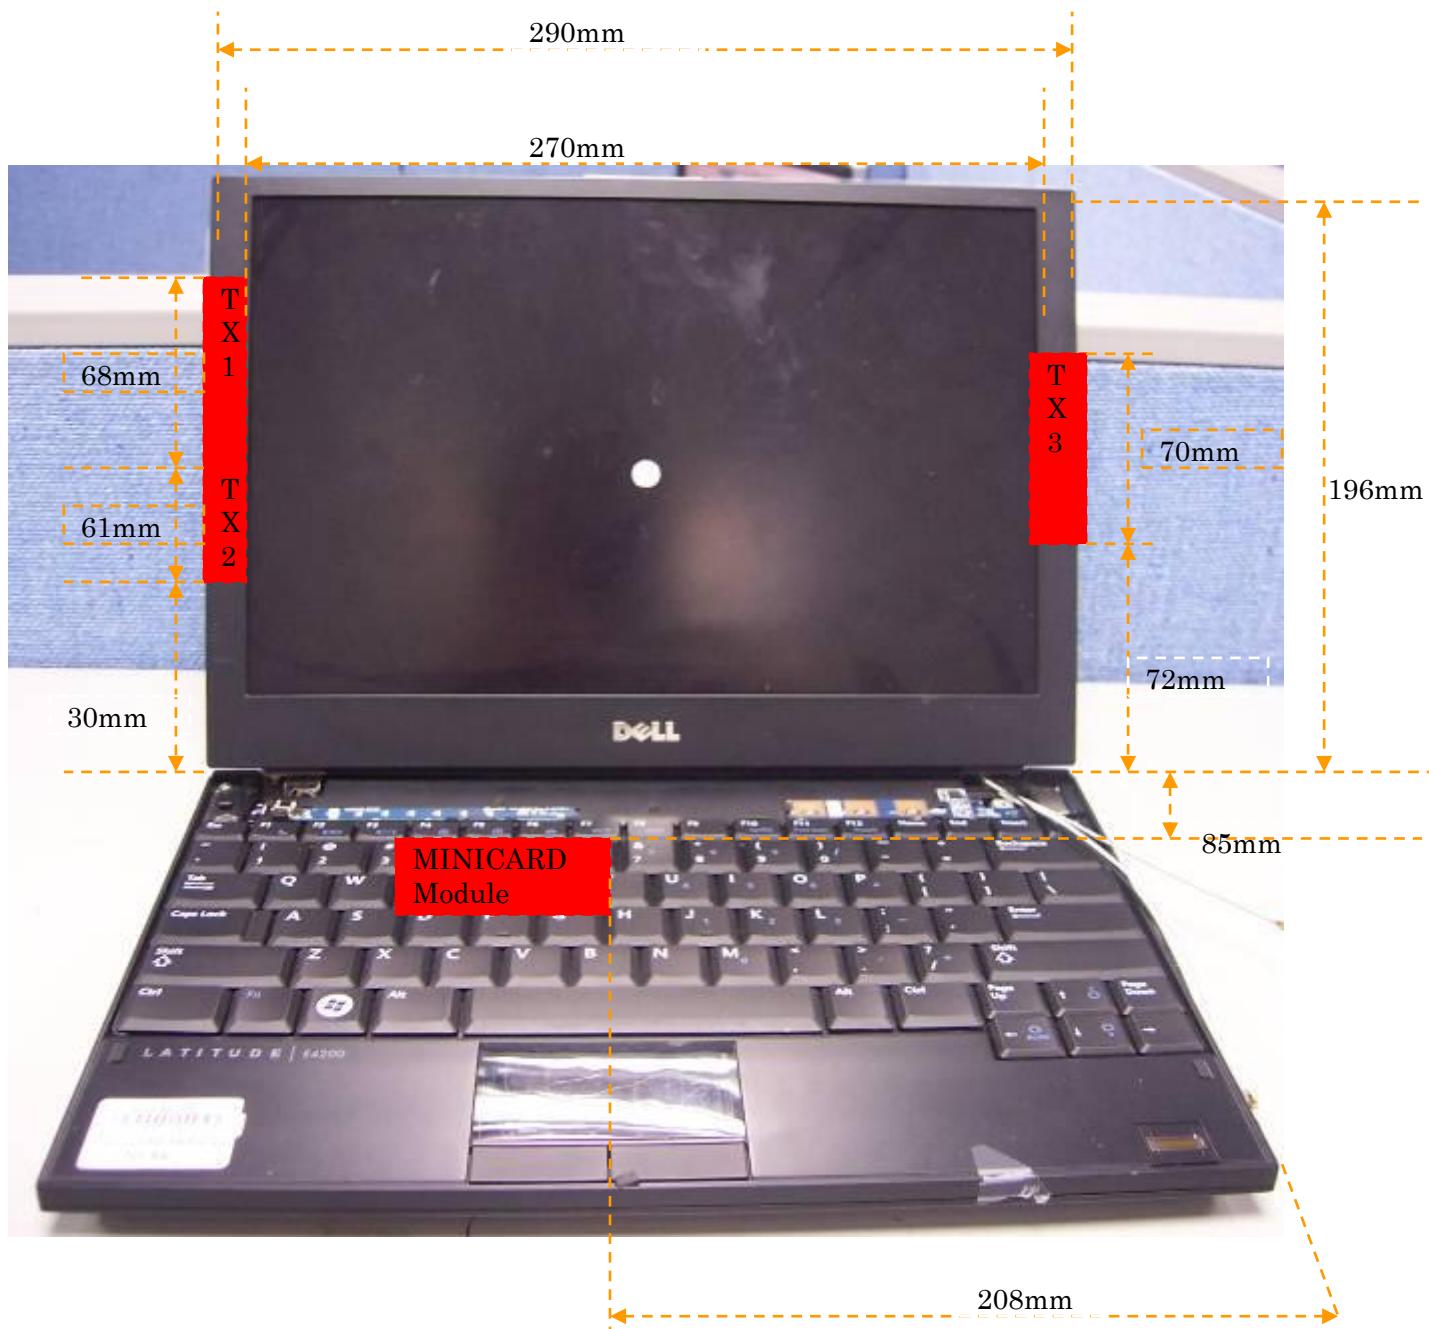

## Section 8. Local representative contact information

**Local representative contact information is required for regulatory support for target countries below.**

	Local company name	Contact name	Phone number	FAX Number	e-Mail Address	Notes
Argentina						
Brazil						
Indonesia						
Israel	Galtronics LTD	Doron Kenigsbuch	+972-46-739-812	+972-46-734-138	Doron.kenigsbuch@galtronics.coml	
Malaysia						
Mexico						
Singapore						Telecommunication Equipment Dealer License Required
South Africa						
USA, Canada						