

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL_750_231220 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.893$ S/m; $\epsilon_r = 43.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.84, 9.43, 10.43); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.279 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.418 W/kg; SAR (8g) = 0.297 W/kg; SAR (10g) = 0.282 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 90.2 %

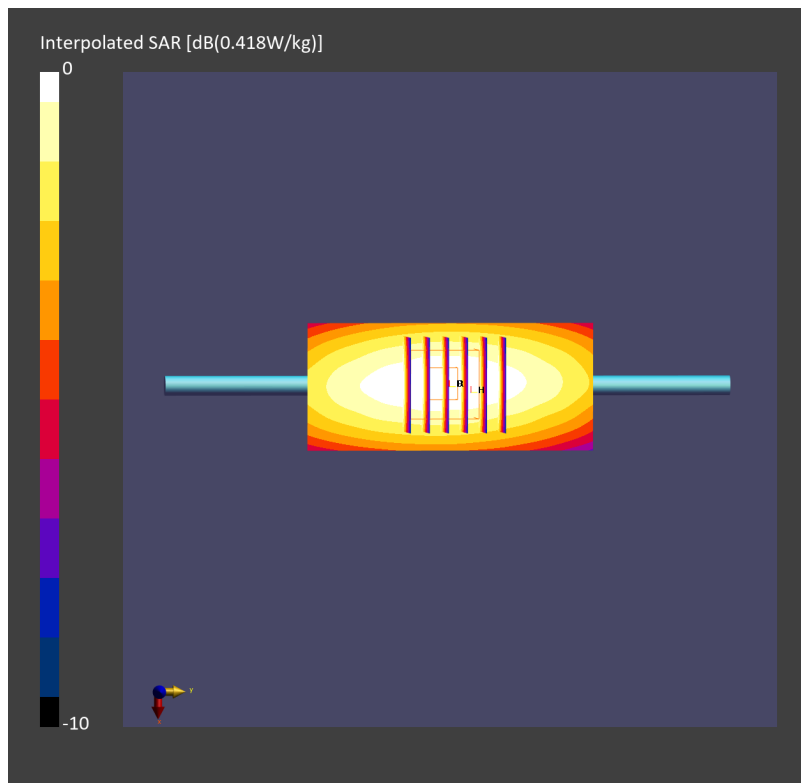

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL_750_231222 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.892$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.84, 9.43, 10.43); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.416 W/kg; SAR (10g) = 0.278 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 0.419 W/kg; SAR (8g) = 0.298 W/kg; SAR (10g) = 0.284 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 91.2 %

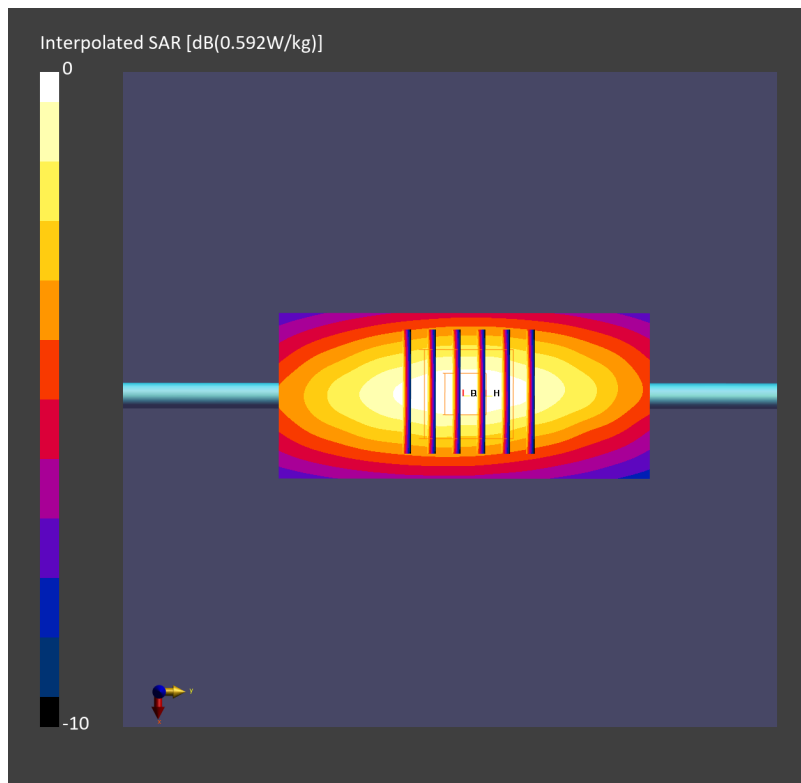

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz; Duty Cycle: 1:1

Medium: HSL_750_231231 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.84, 9.43, 10.43); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.413 W/kg; SAR (10g) = 0.276 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 0.414 W/kg; SAR (8g) = 0.295 W/kg; SAR (10g) = 0.281 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 90.4 %

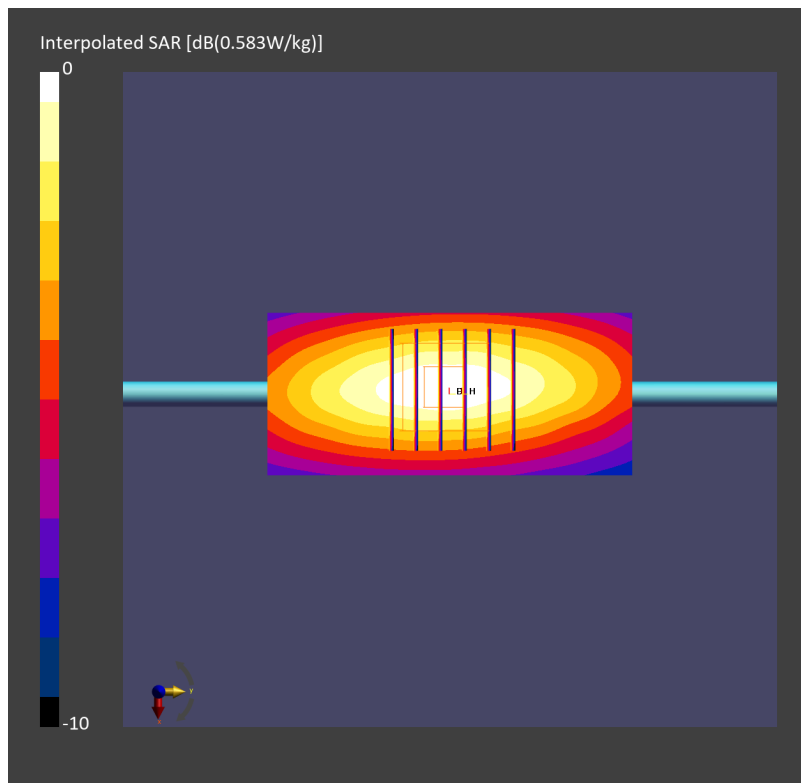

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_850_231219 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.920$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.35, 9.19, 10.14); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.496 W/kg; SAR (10g) = 0.327 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.05 dB

SAR (1g) = 0.502 W/kg; SAR (8g) = 0.354 W/kg; SAR (10g) = 0.336 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 89.4 %

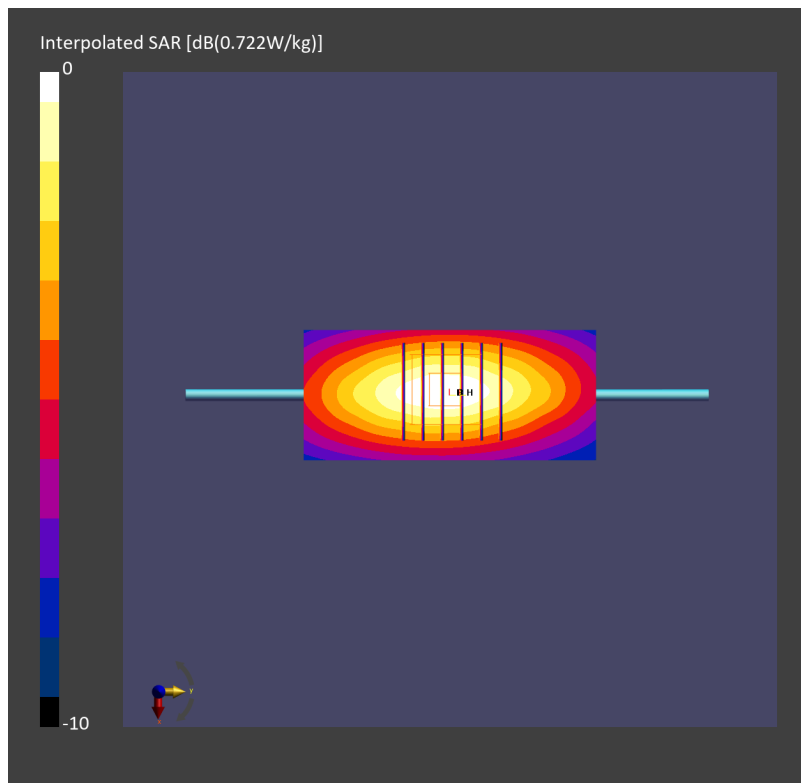

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz; Duty Cycle: 1:1

Medium: HSL_850_231221 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.930$ S/m; $\epsilon_r = 42.8$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(9.35, 9.19, 10.14); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.509 W/kg; SAR (10g) = 0.336 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.510 W/kg; SAR (8g) = 0.358 W/kg; SAR (10g) = 0.340 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 90.2 %

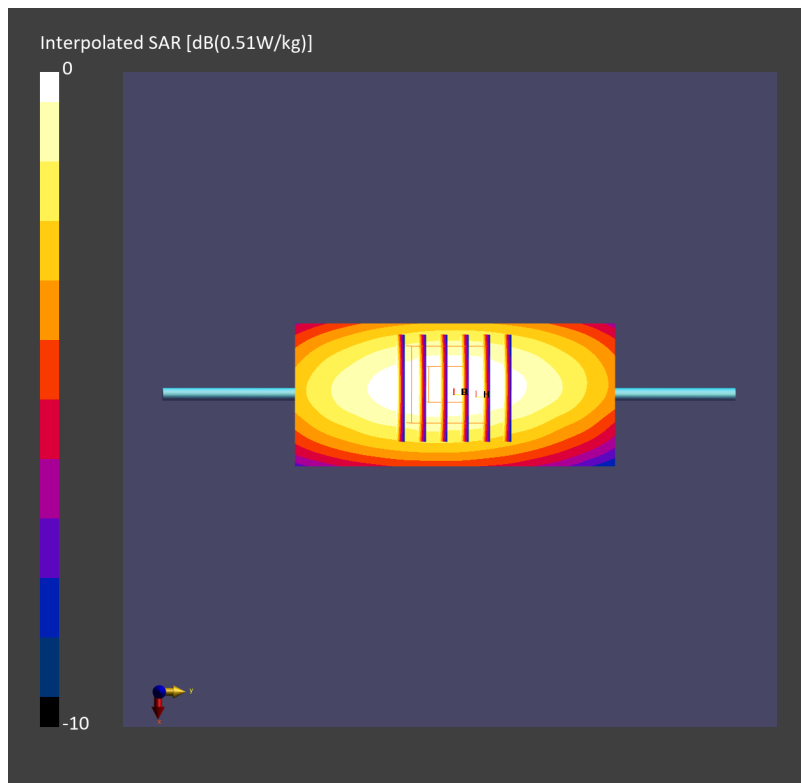

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: HSL_1750_231223 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(8.66, 8.71, 9.35); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.85 W/kg; SAR (10g) = 0.970 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.88 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.997 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

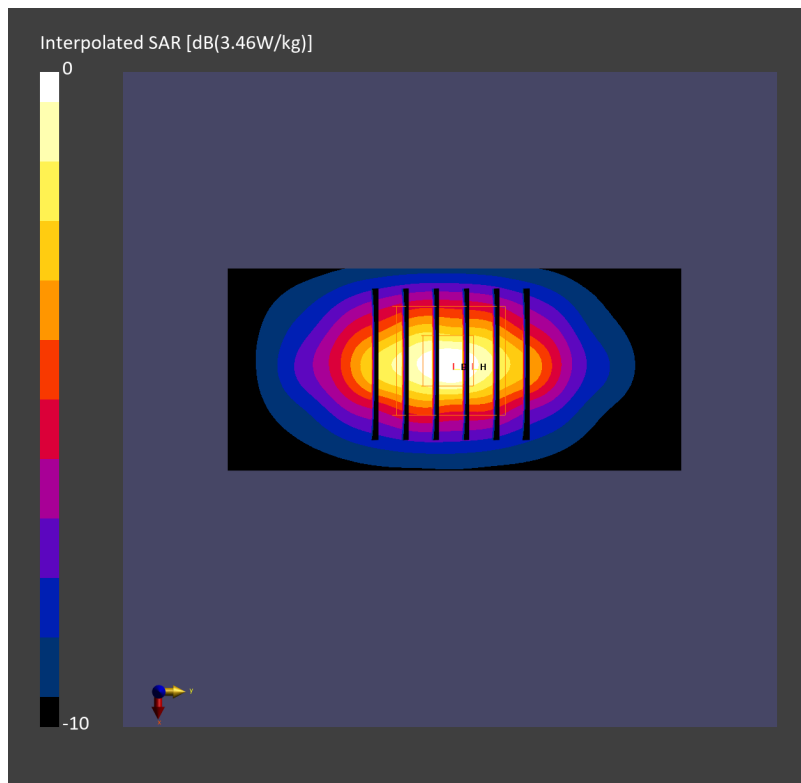

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz; Duty Cycle: 1:1

Medium: HSL_1750_240101 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(8.66, 8.71, 9.35); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 1.00 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.96 W/kg; SAR (8g) = 1.12 W/kg; SAR (10g) = 1.03 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 81.7 %

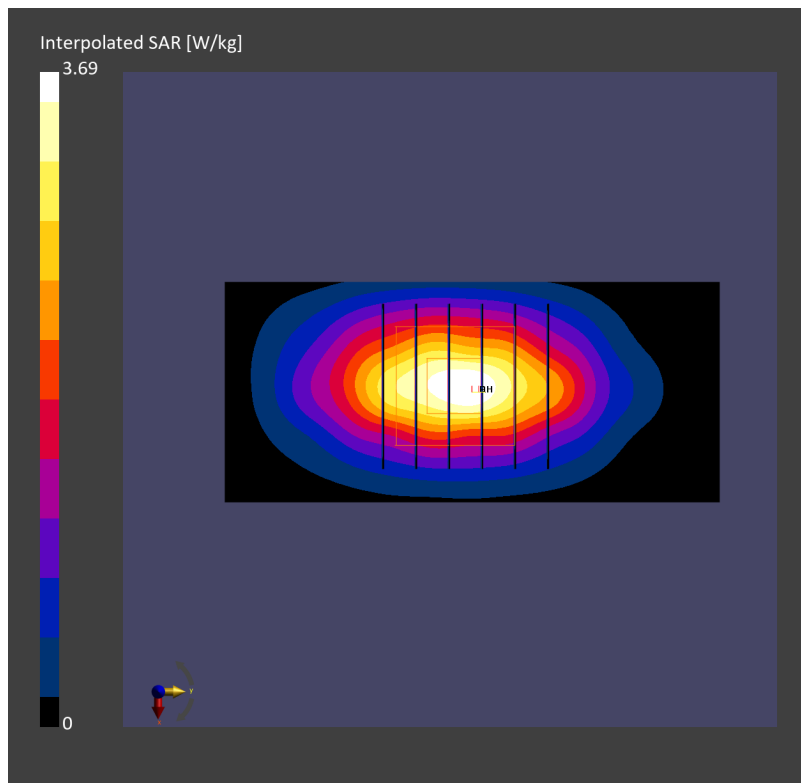

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL_1900_231219 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.40$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(8.0, 8.07, 8.72); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.78 W/kg; SAR (10g) = 0.921 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.77 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.938 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.6 %

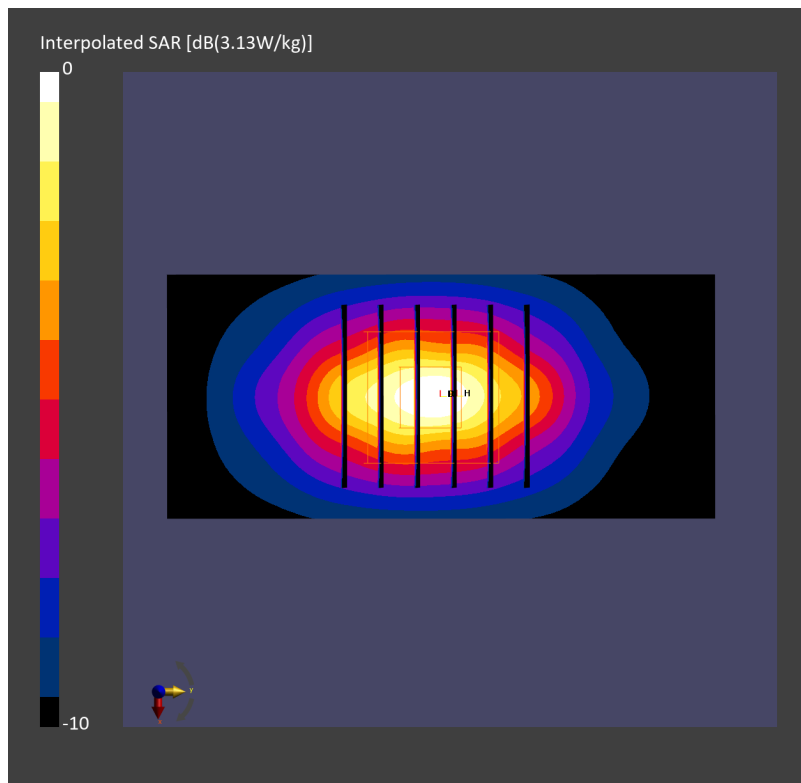

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz; Duty Cycle: 1:1

Medium: HSL_1900_231222 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(8.0, 8.07, 8.72); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.95 W/kg; SAR (10g) = 0.996 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.98 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

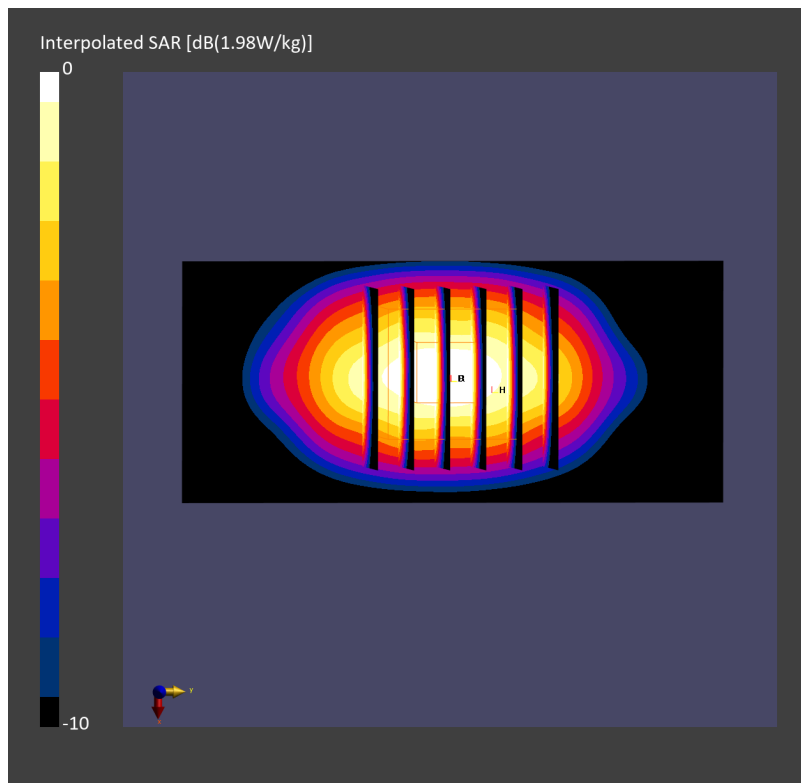

System Check_Head_2300MHz

DUT: D2300V2 - SN1006

Communication System: CW; Frequency: 2300.000 MHz; Duty Cycle: 1:1

Medium: HSL_2300_231226 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.64$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.71, 7.81, 8.42); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.35 W/kg; SAR (10g) = 1.16 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.49 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

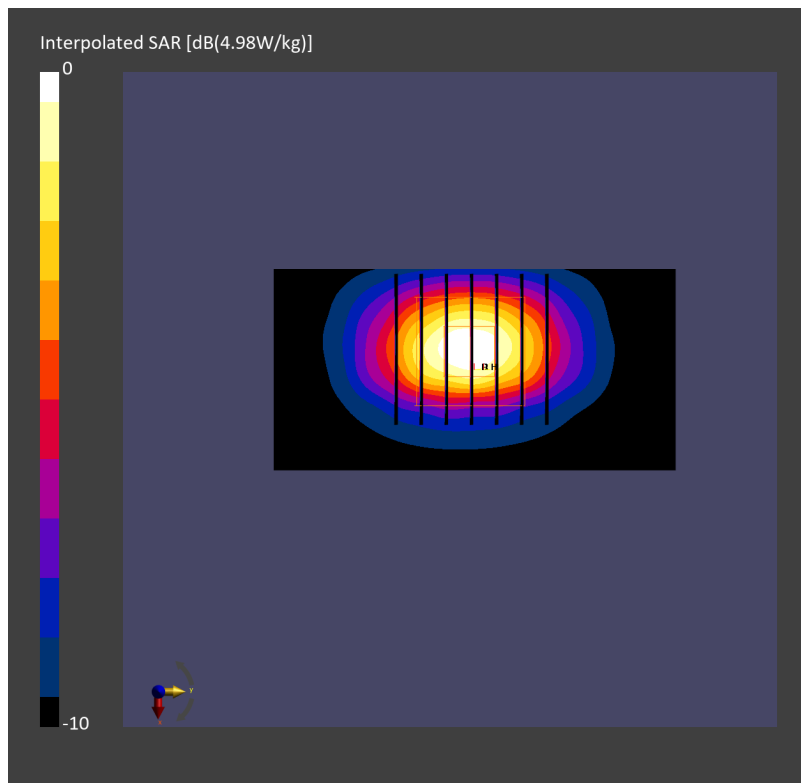

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600_231218 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.5, 7.6, 8.24); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.42 W/kg; SAR (10g) = 1.09 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 2.50 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.4 %

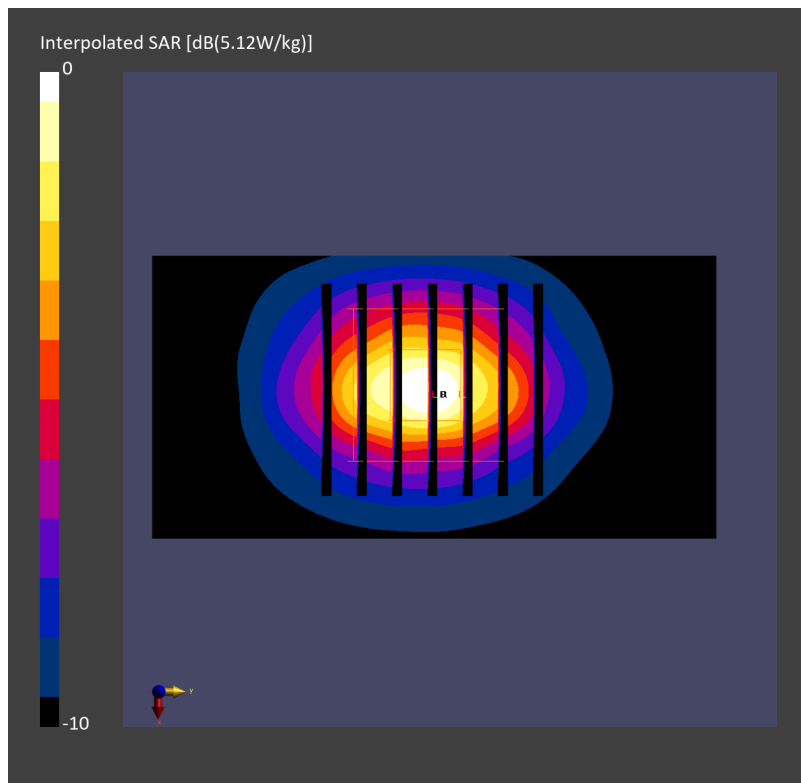

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600_231224 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.95$ S/m; $\epsilon_r = 39.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.5, 7.6, 8.24); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.77 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.84 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

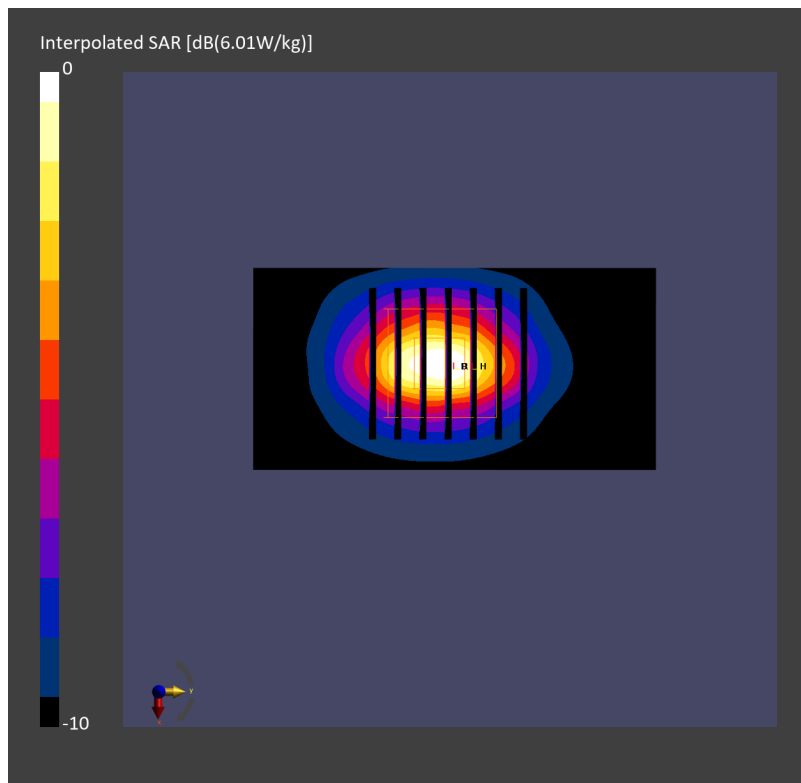

System Check_Head_2600MHz

DUT: D2600V2 - SN1078

Communication System: CW; Frequency: 2600.000 MHz; Duty Cycle: 1:1

Medium: HSL_2600_231225 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.5, 7.6, 8.24); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.79 W/kg; SAR (10g) = 1.24 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.87 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.9 %

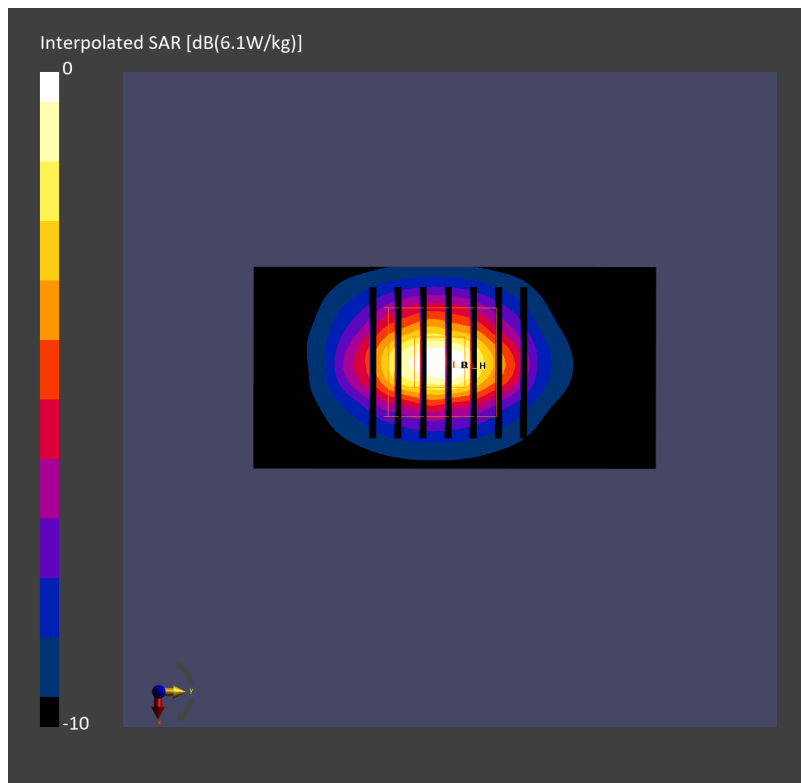

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500_231213 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 3.01$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.07, 7.19, 7.75); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 1.28 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.52 W/kg; SAR (8g) = 1.52 W/kg; SAR (10g) = 1.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

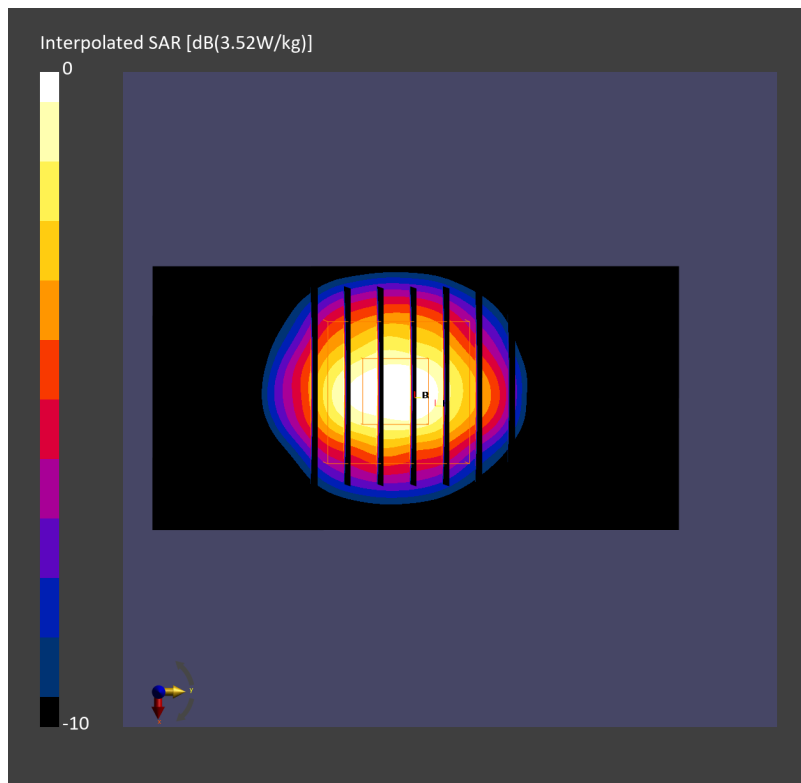

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500_231214 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.91$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.07, 7.19, 7.75); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.24 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.40 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.4 %

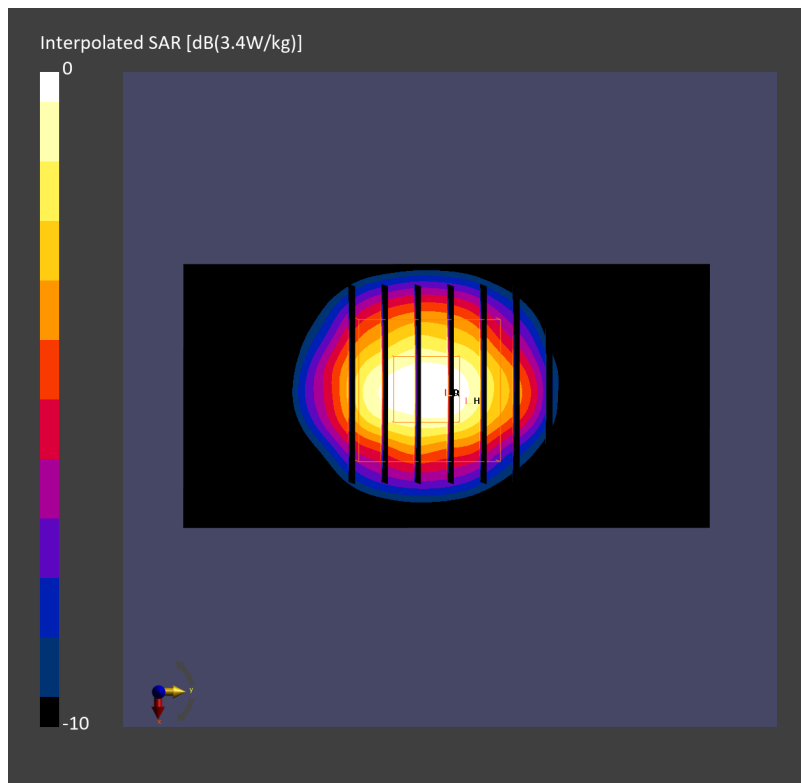

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500_231215 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.97$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.07, 7.19, 7.75); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.21 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.6 %

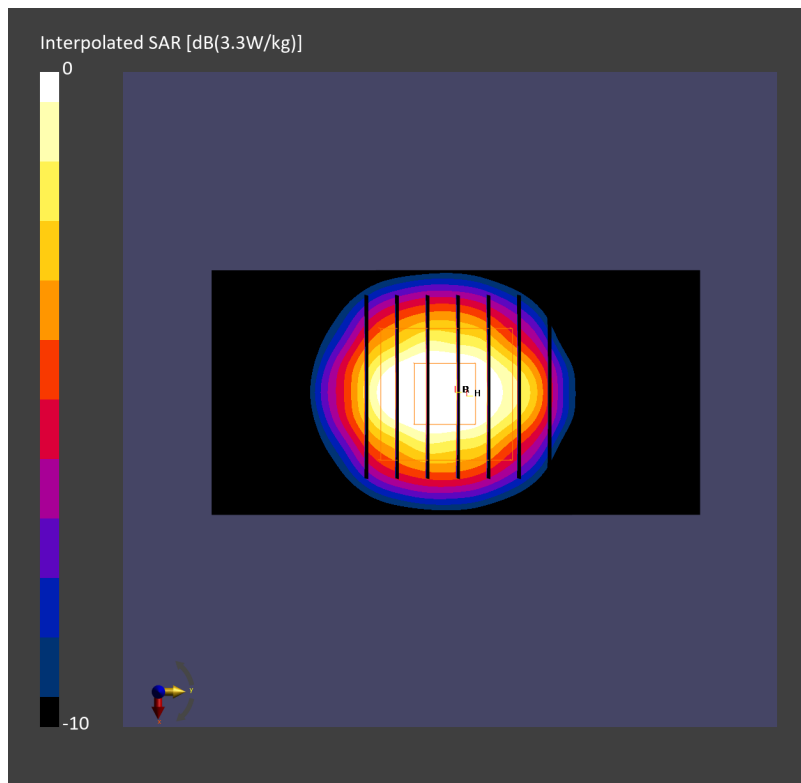

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500_231217 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 3.00$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.07, 7.19, 7.75); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.19 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.21 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 77.0 %

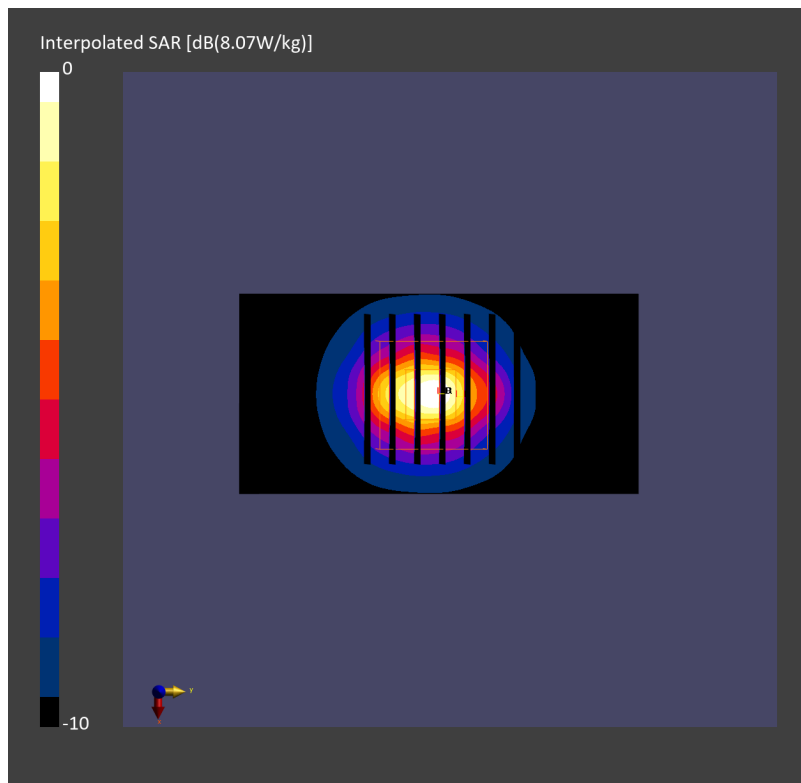

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500_231227 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.98$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.07, 7.19, 7.75); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.27 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.45 W/kg; SAR (8g) = 1.50 W/kg; SAR (10g) = 1.33 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

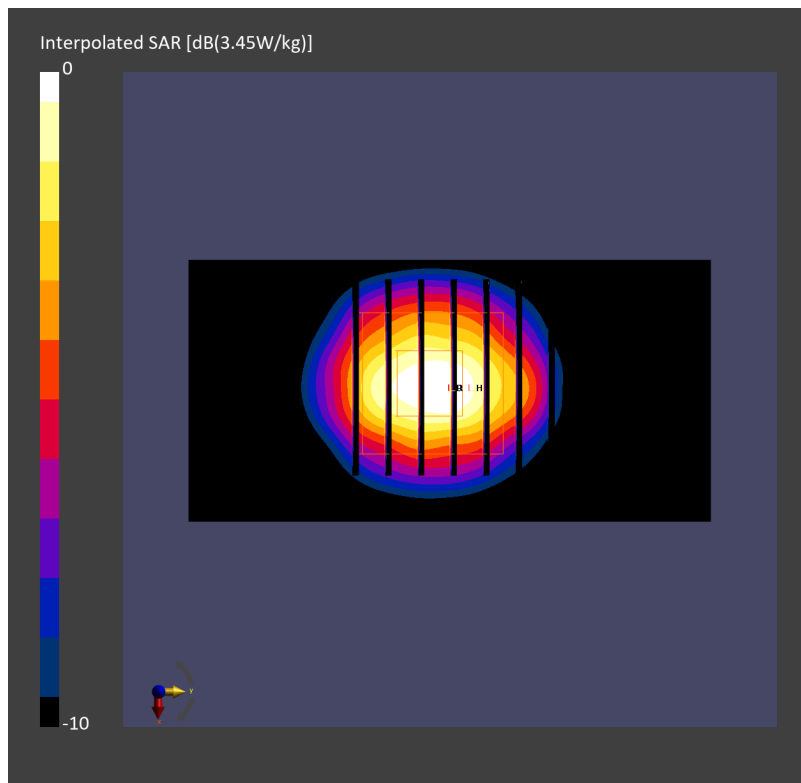

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500_231228 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.92$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.07, 7.19, 7.75); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.37 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.30 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.6 %

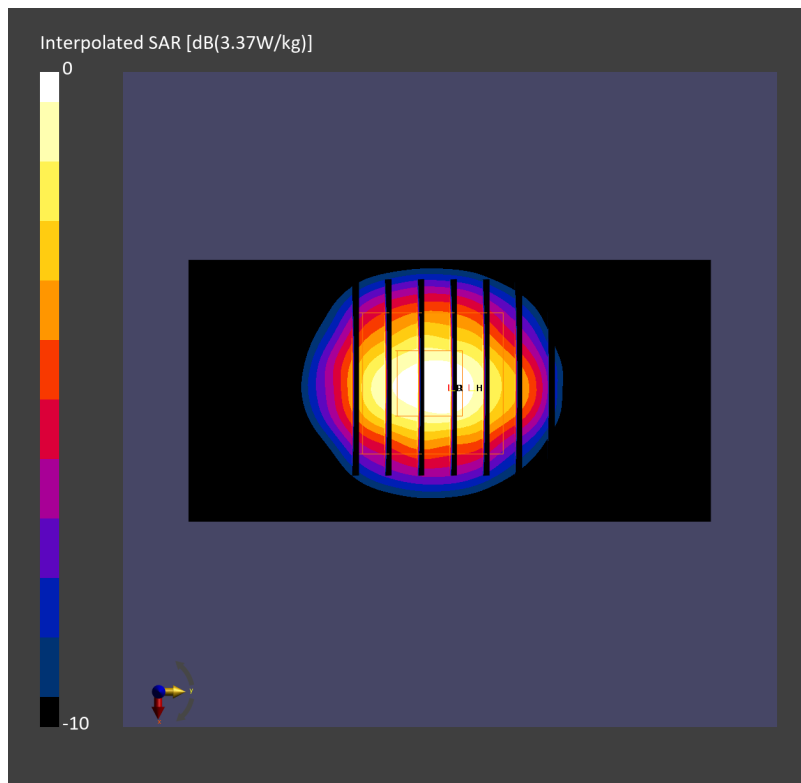

System Check_Head_3500MHz

DUT: D3500V2 - SN1036

Communication System: CW; Frequency: 3500.000 MHz; Duty Cycle: 1:1

Medium: HSL_3500_231230 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.95$ S/m; $\epsilon_r = 38.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(7.07, 7.19, 7.75); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.59 W/kg; SAR (10g) = 1.34 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.70 W/kg; SAR (8g) = 1.60 W/kg; SAR (10g) = 1.38 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.8 %

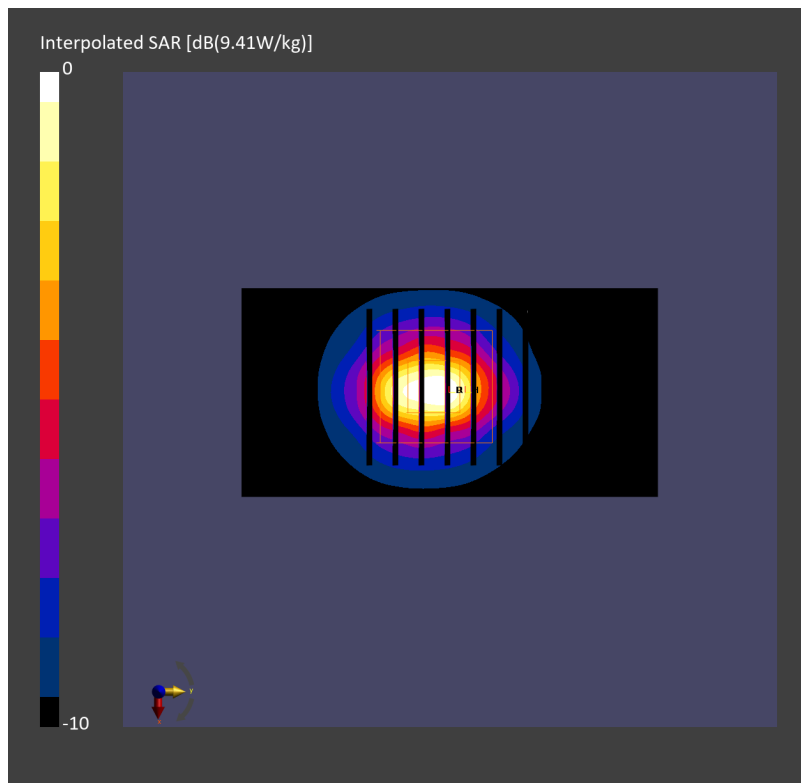

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: HSL_3700_231211 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.22$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.89, 7.01, 7.57); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.95 W/kg; SAR (10g) = 1.09 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.02 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.9 %

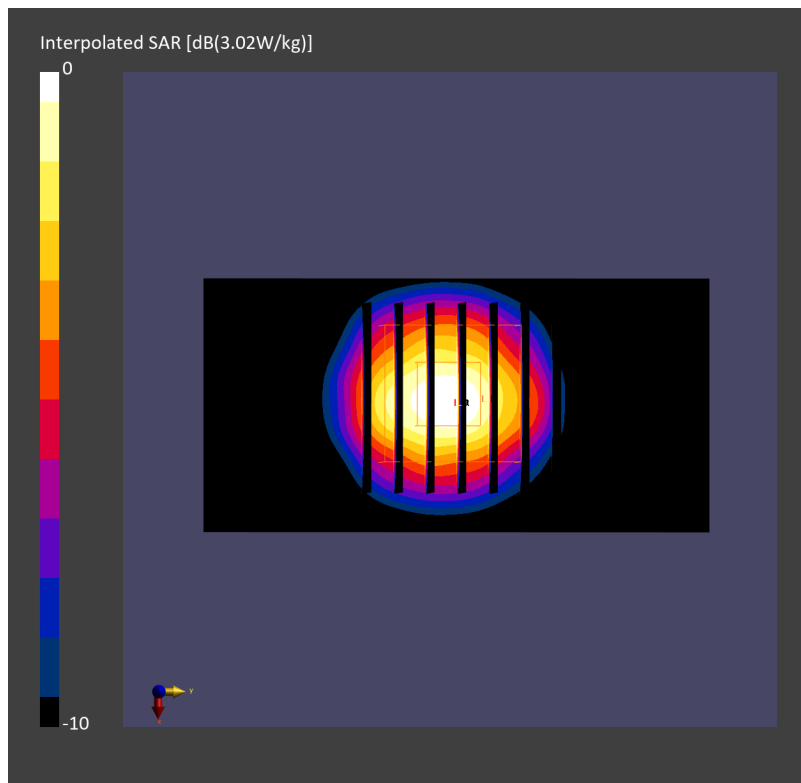

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: HSL_3700_231214 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 36.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.89, 7.01, 7.57); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.39 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.49 W/kg; SAR (8g) = 1.47 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

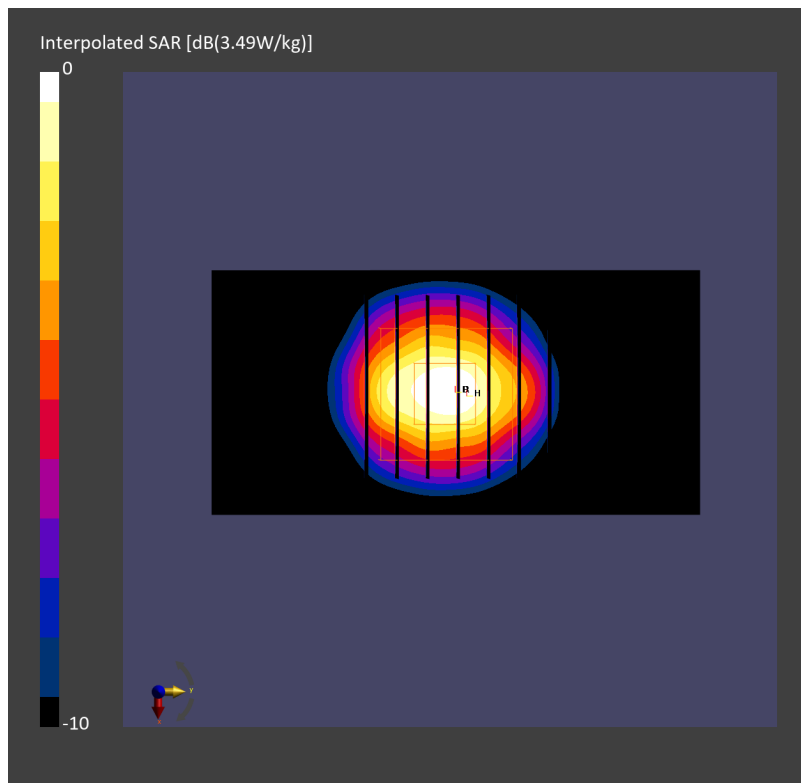

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: HSL_3700_231217 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.19$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.89, 7.01, 7.57); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.98 W/kg; SAR (10g) = 1.10 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.07 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.2 %

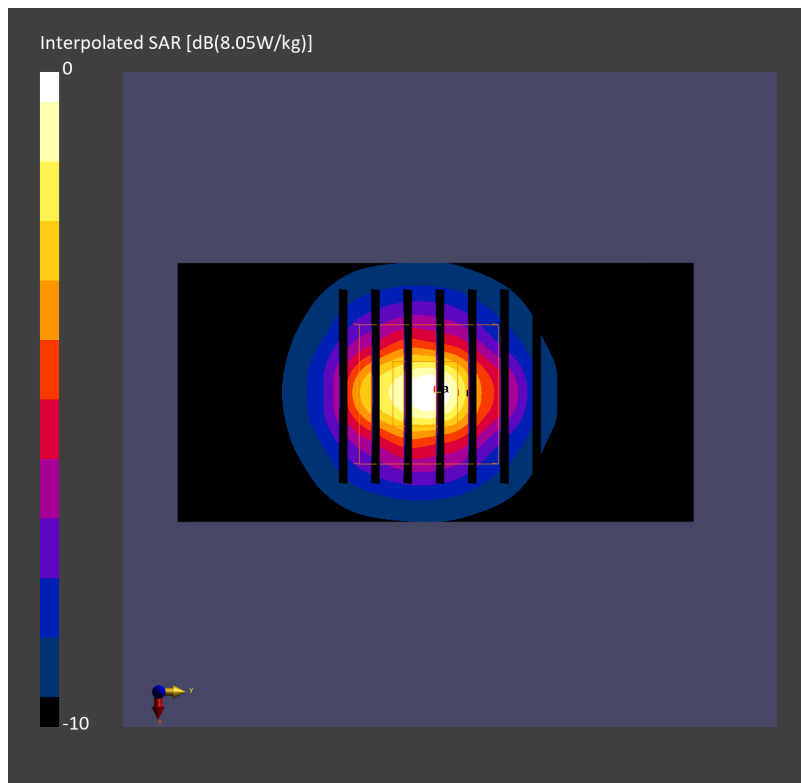

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: HSL_3700_231229 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.18$ S/m; $\epsilon_r = 38.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.89, 7.01, 7.57); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.01 W/kg; SAR (10g) = 1.15 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.20 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.2 %

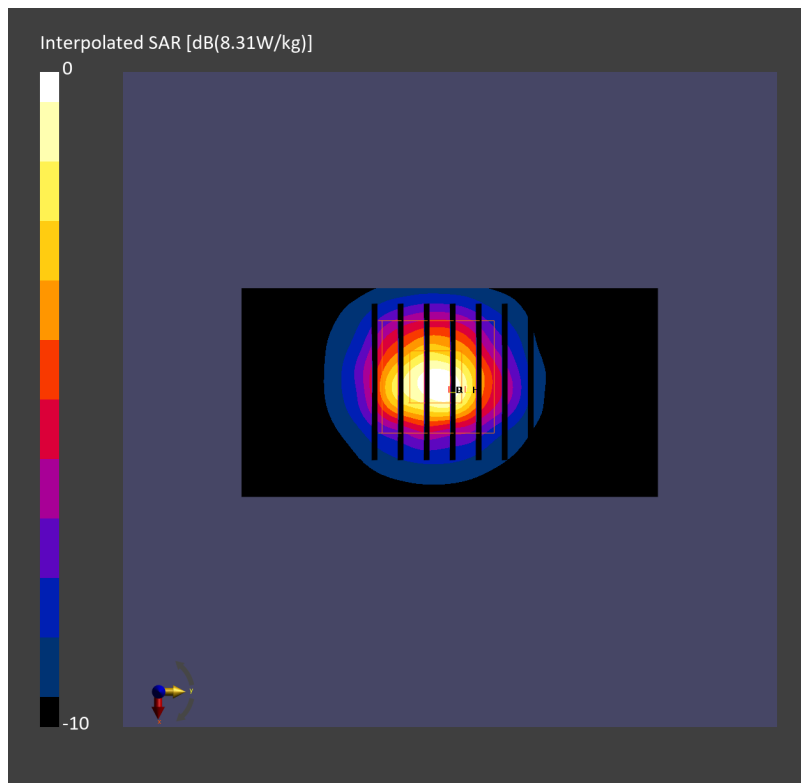

System Check_Head_3700MHz

DUT: D3700V2 - SN1006

Communication System: CW; Frequency: 3700.000 MHz; Duty Cycle: 1:1

Medium: HSL_3700_231230 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.10$ S/m; $\epsilon_r = 36.8$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.89, 7.01, 7.57); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.92 W/kg; SAR (10g) = 1.11 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.12 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.4 %

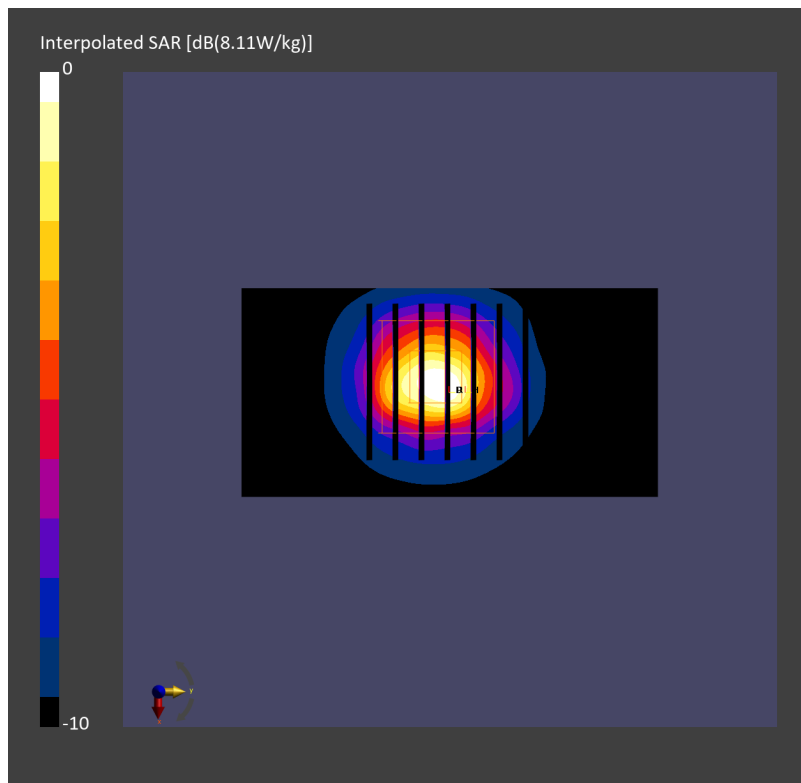

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: HSL_3900_231210 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.37$ S/m; $\epsilon_r = 37.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.88, 7.01, 7.55); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.79 W/kg; SAR (10g) = 1.04 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.06 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.1 %

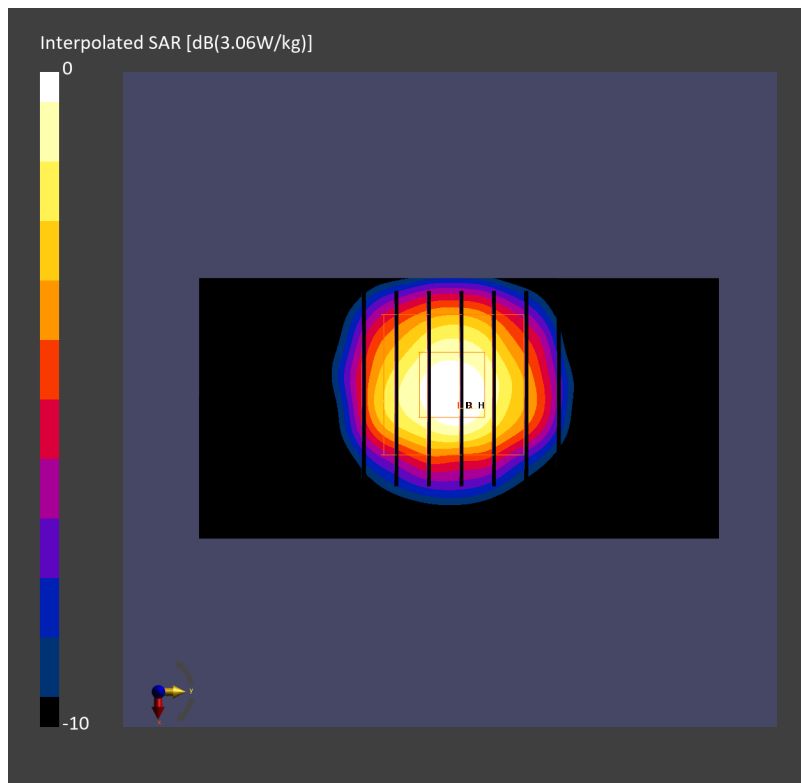

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: HSL_3900_231211 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.42$ S/m; $\epsilon_r = 37.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.88, 7.01, 7.55); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.83 W/kg; SAR (10g) = 1.06 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.11 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.2 %

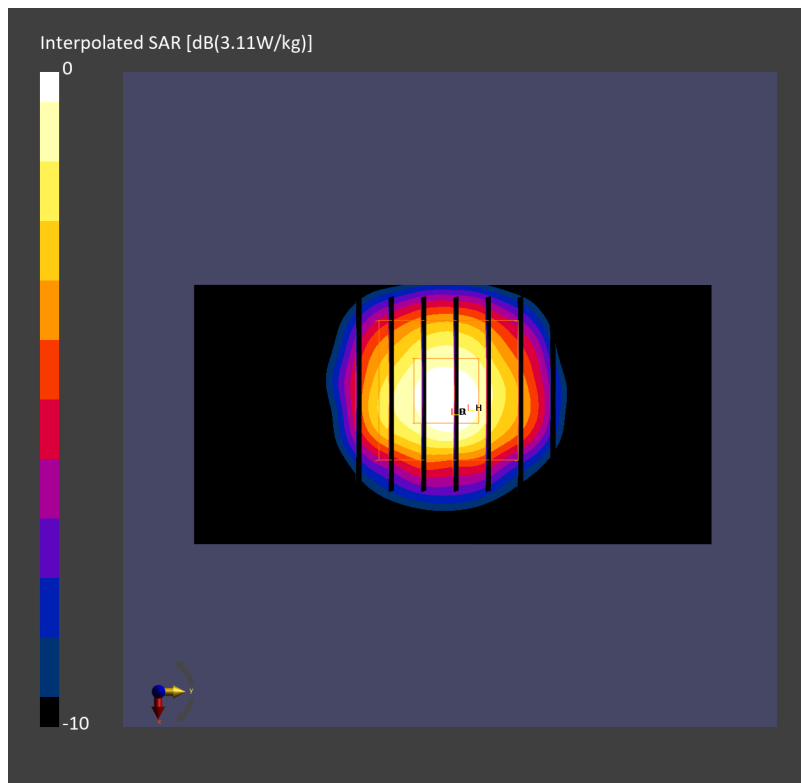

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: HSL_3900_231212 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.39$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.88, 7.01, 7.55); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.83 W/kg; SAR (10g) = 1.05 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.07 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.2 %

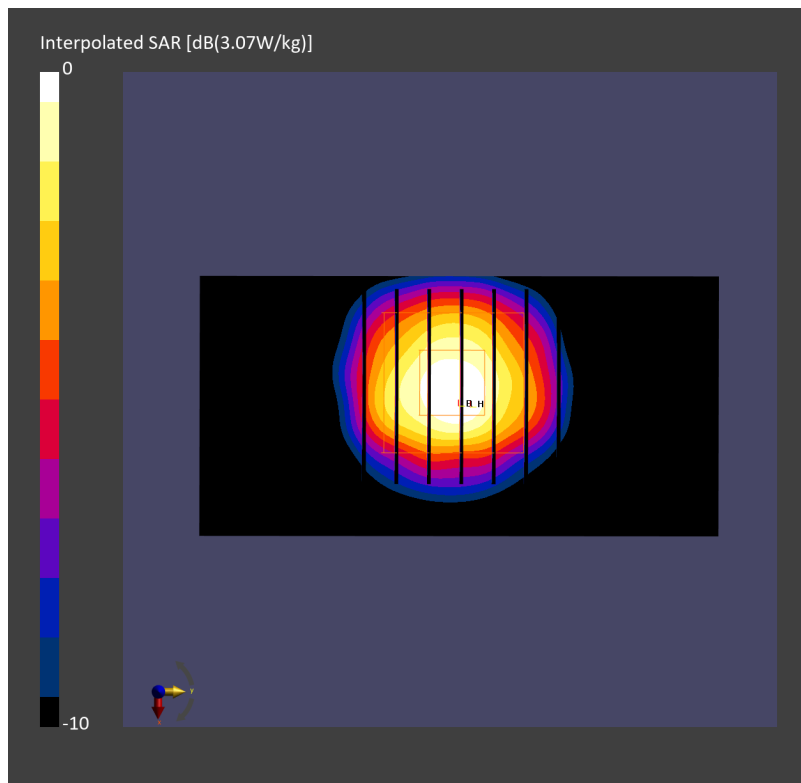

System Check_Head_3900MHz

DUT: D3900V2 - SN1092

Communication System: CW; Frequency: 3900.000 MHz; Duty Cycle: 1:1

Medium: HSL_3900_231216 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.41$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7695; ConvF(6.88, 7.01, 7.55); Calibrated: 2023-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1696; Calibrated: 2023-10-23
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2205; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.15 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.47 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.8 %

