

Date: 2024-10-11

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_241011 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.891$ S/m; $\epsilon_r = 41.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.94, 9.37, 8.85); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.436 W/kg; SAR (10g) = 0.291 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5


mm

Power Drift = -0.00 dB

SAR (1g) = 0.434 W/kg; SAR (8g) = 0.301 W/kg; SAR (10g) = 0.285 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 86.9 %

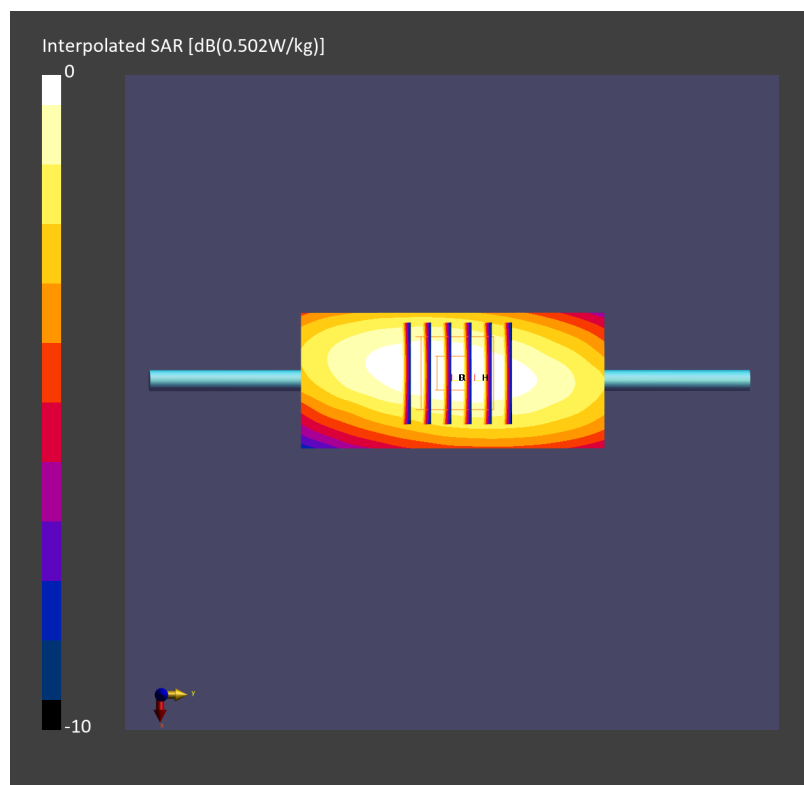

Date: 2024-10-13

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_241013 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.889$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.94, 9.37, 8.85); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.436 W/kg; SAR (10g) = 0.290 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5


mm

Power Drift = 0.01 dB

SAR (1g) = 0.433 W/kg; SAR (8g) = 0.301 W/kg; SAR (10g) = 0.285 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 86.7 %

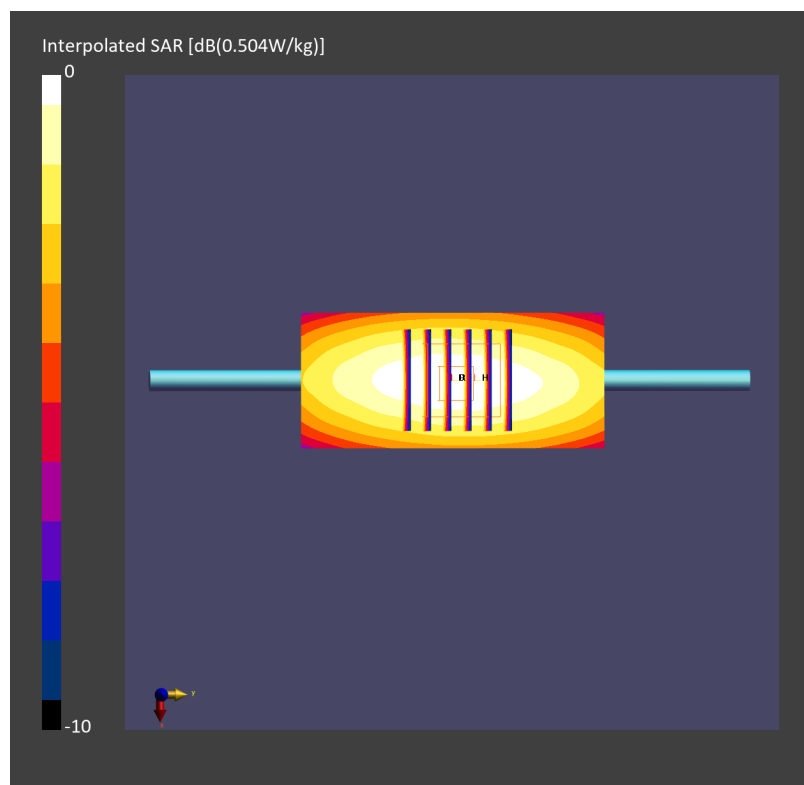

Date: 2024-10-17

System Check_Head_750MHz

DUT: D750V3 - SN1012

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_241017 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.902$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.94, 9.37, 8.85); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.429 W/kg; SAR (10g) = 0.286 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5


mm

Power Drift = -0.00 dB

SAR (1g) = 0.427 W/kg; SAR (8g) = 0.300 W/kg; SAR (10g) = 0.285 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.7 %

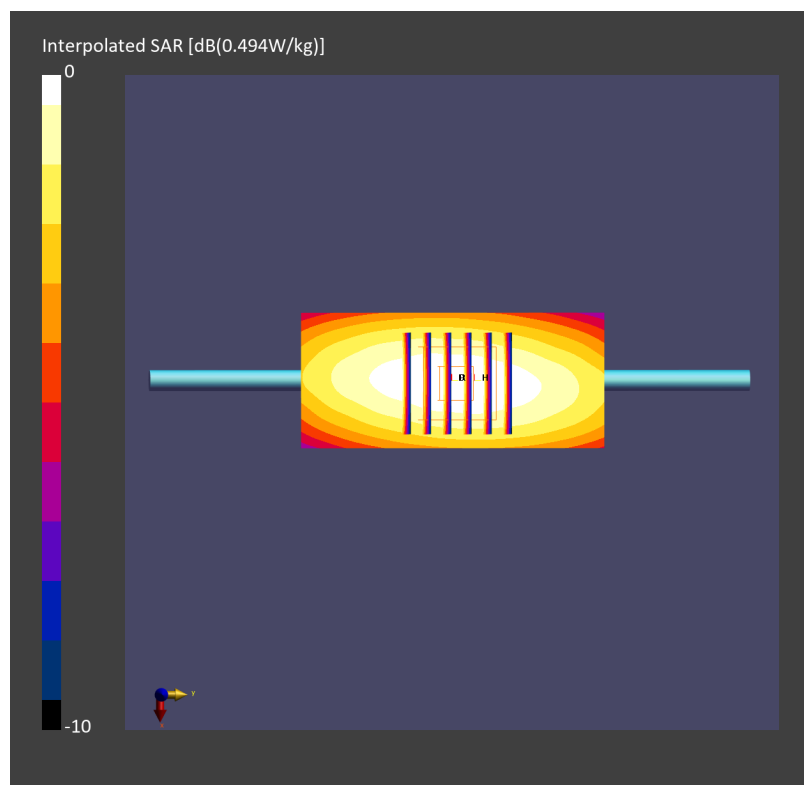

Date: 2024-10-19

System Check_Head_750MHz**DUT: D750V3 - SN1012**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_241019 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.898$ S/m; $\epsilon_r = 42.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.94, 9.37, 8.85); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.415 W/kg; SAR (10g) = 0.278 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 0.417 W/kg; SAR (8g) = 0.292 W/kg; SAR (10g) = 0.277 W/kg

Smallest distance from peaks to all points 3 dB below = > 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.4 %

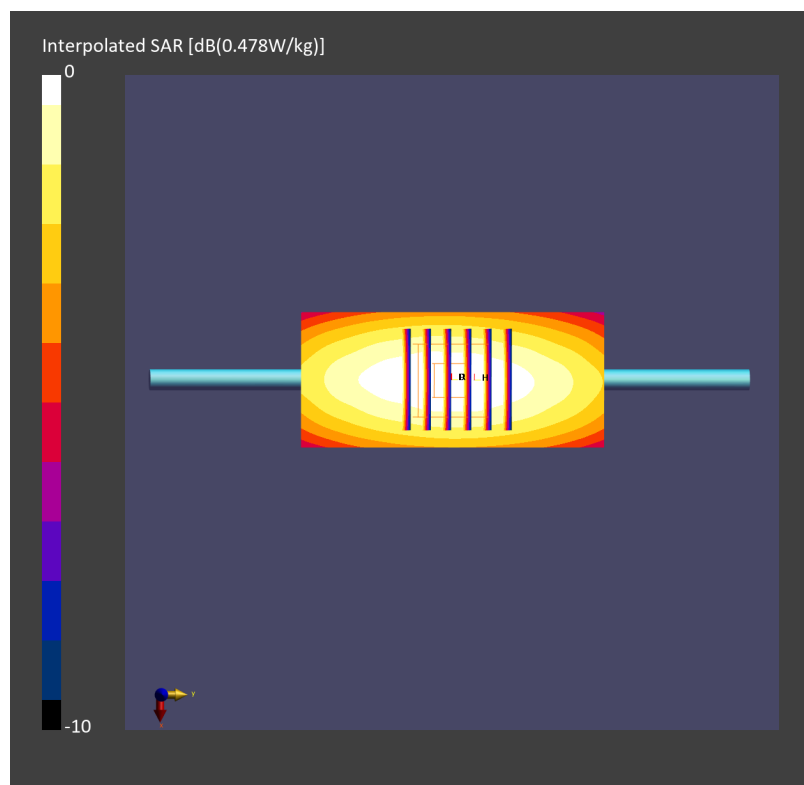

Date: 2024-10-13

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_241013 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.923$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.67, 9.09, 8.59); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.486 W/kg; SAR (10g) = 0.322 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5


mm

Power Drift = 0.00 dB

SAR (1g) = 0.490 W/kg; SAR (8g) = 0.340 W/kg; SAR (10g) = 0.322 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 85.1 %

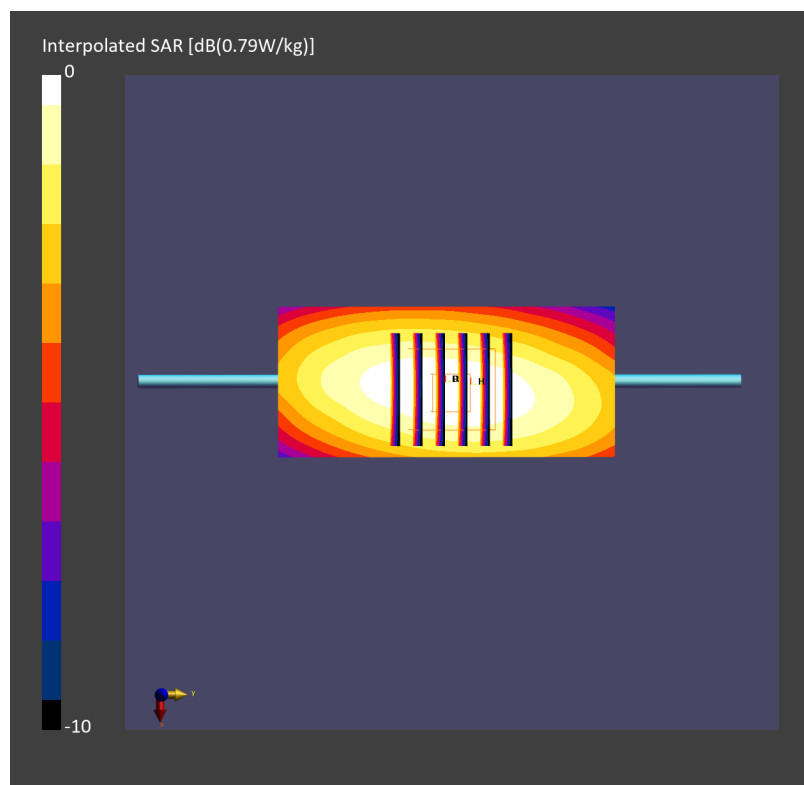

Date: 2024-10-19

System Check_Head_835MHz**DUT: D835V2 - SN4d060**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_241019 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.933$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(8.67, 9.09, 8.59); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.512 W/kg; SAR (10g) = 0.336 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5


mm

Power Drift = -0.01 dB

SAR (1g) = 0.509 W/kg; SAR (8g) = 0.351 W/kg; SAR (10g) = 0.333 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 86.8 %

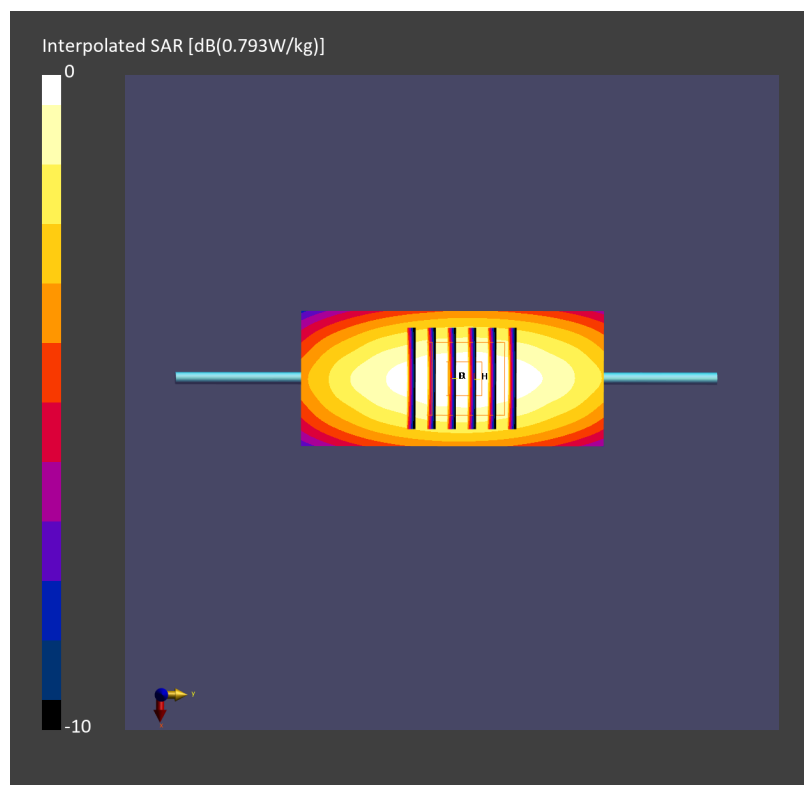

Date: 2024-10-12

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_241012 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.49, 7.86, 7.42); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.84 W/kg; SAR (10g) = 0.977 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.82 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.967 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

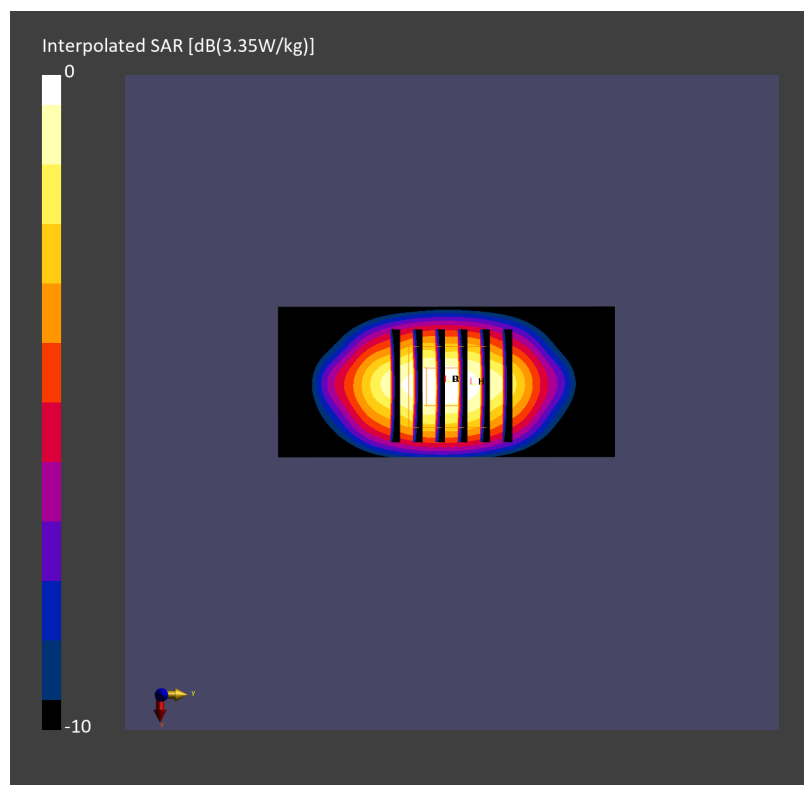

Date: 2024-10-18

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_241018 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.49, 7.86, 7.42); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.68 W/kg; SAR (10g) = 0.903 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5


mm

Power Drift = -0.00 dB

SAR (1g) = 1.69 W/kg; SAR (8g) = 0.980 W/kg; SAR (10g) = 0.905 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 81.8 %

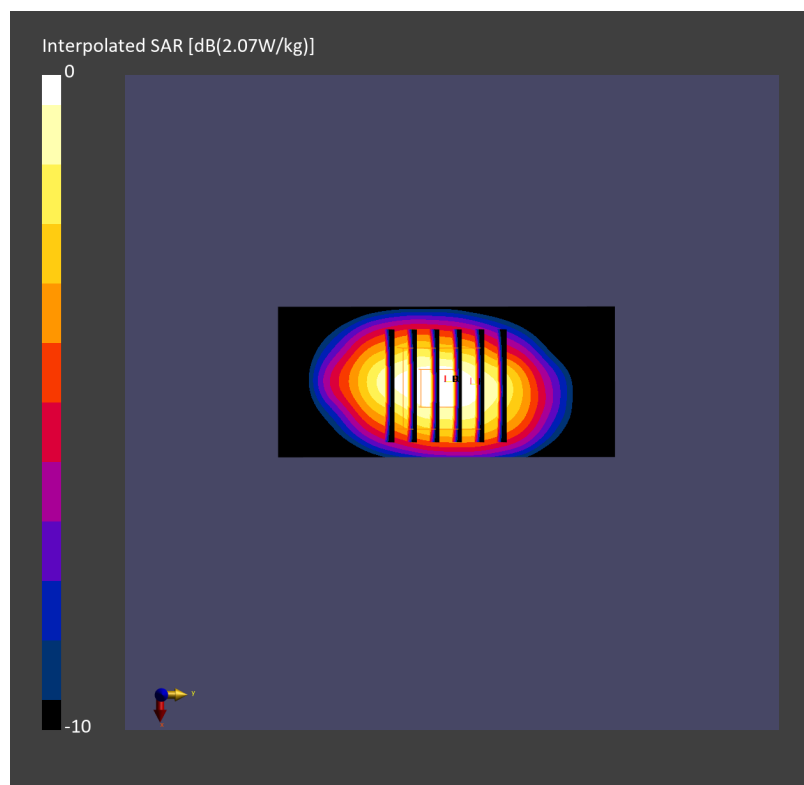

Date: 2024-10-25

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_241025 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.49, 7.86, 7.42); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.81 W/kg; SAR (10g) = 0.961 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.80 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.954 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

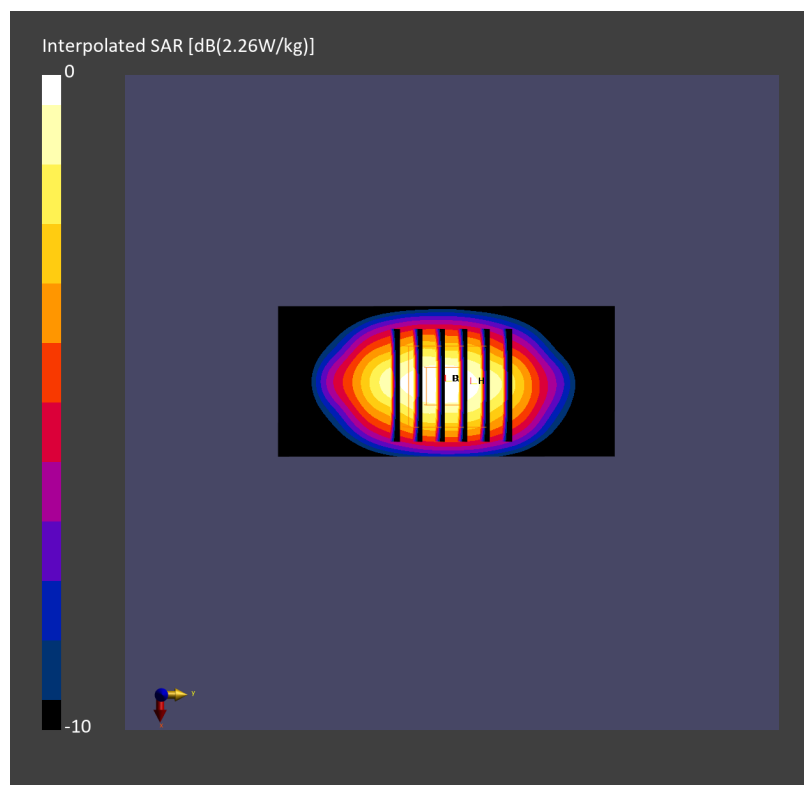

Date: 2024-11-01

System Check_Head_1750MHz**DUT: D1750V2 - SN1068**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_241101 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.49, 7.86, 7.42); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.82 W/kg; SAR (10g) = 0.964 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.80 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.957 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

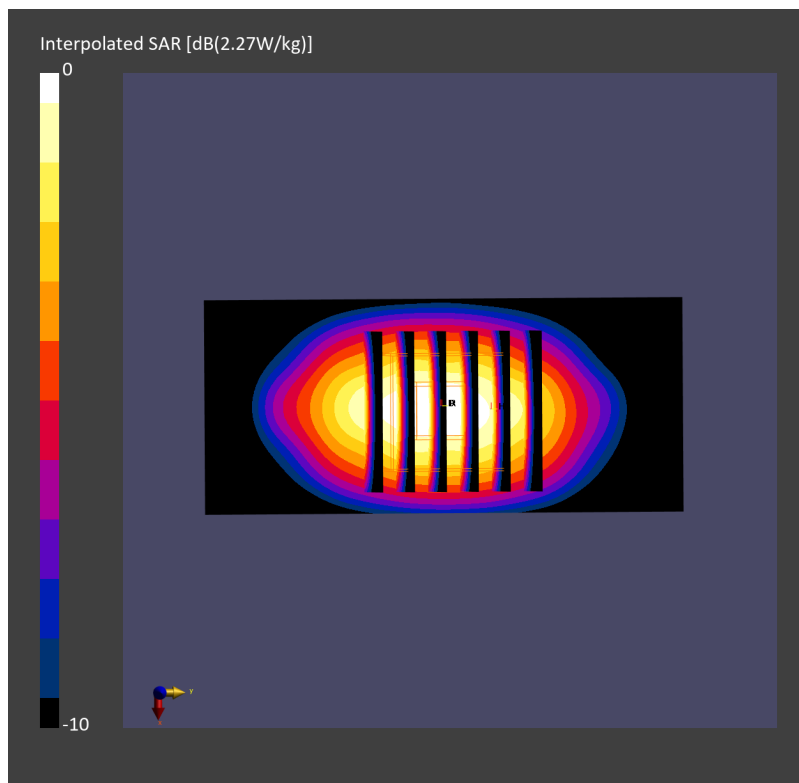

Date: 2024-10-15

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_241015 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.28, 7.63, 7.21); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.996 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 0.999 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 81.2 %

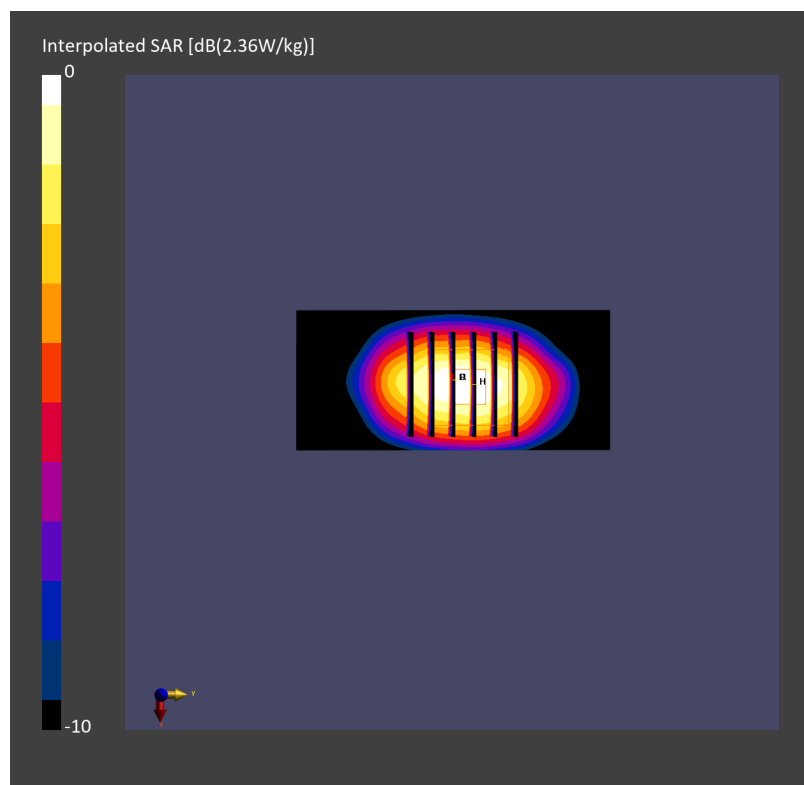

Date: 2024-10-18

System Check_Head_1900MHz**DUT: D1900V2 - SN5d041**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_241018 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.28, 7.63, 7.21); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.01 W/kg; SAR (10g) = 1.04 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5


mm

Power Drift = 0.01 dB

SAR (1g) = 1.99 W/kg; SAR (8g) = 1.13 W/kg; SAR (10g) = 1.04 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.4 %

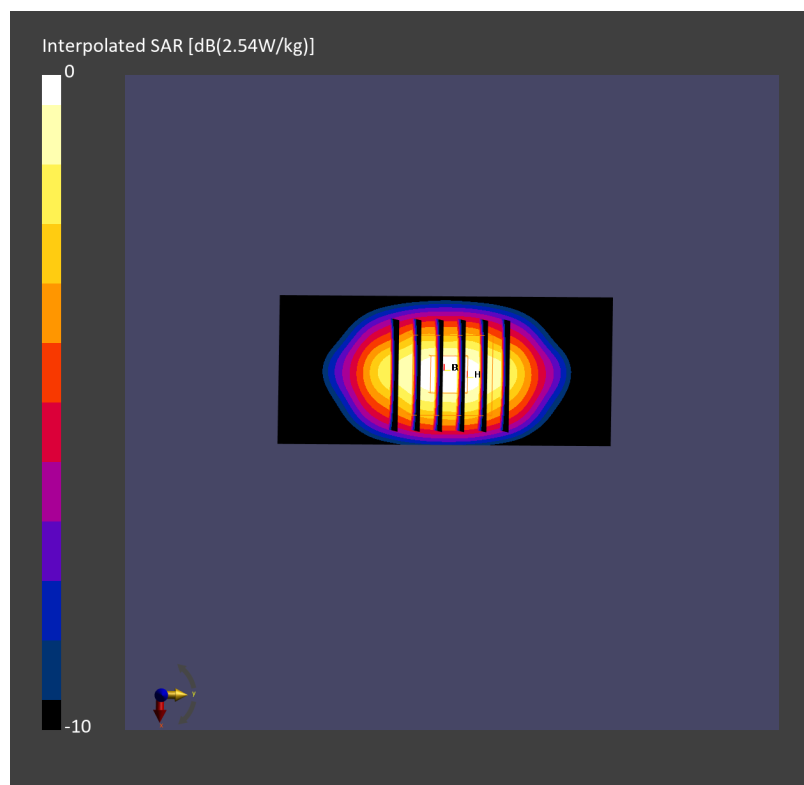

Date: 2024-10-20

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_241020 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.65$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.19, 7.54, 7.12); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.25 W/kg; SAR (10g) = 1.06 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5


mm

Power Drift = -0.00 dB

SAR (1g) = 2.22 W/kg; SAR (8g) = 1.16 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.4 %

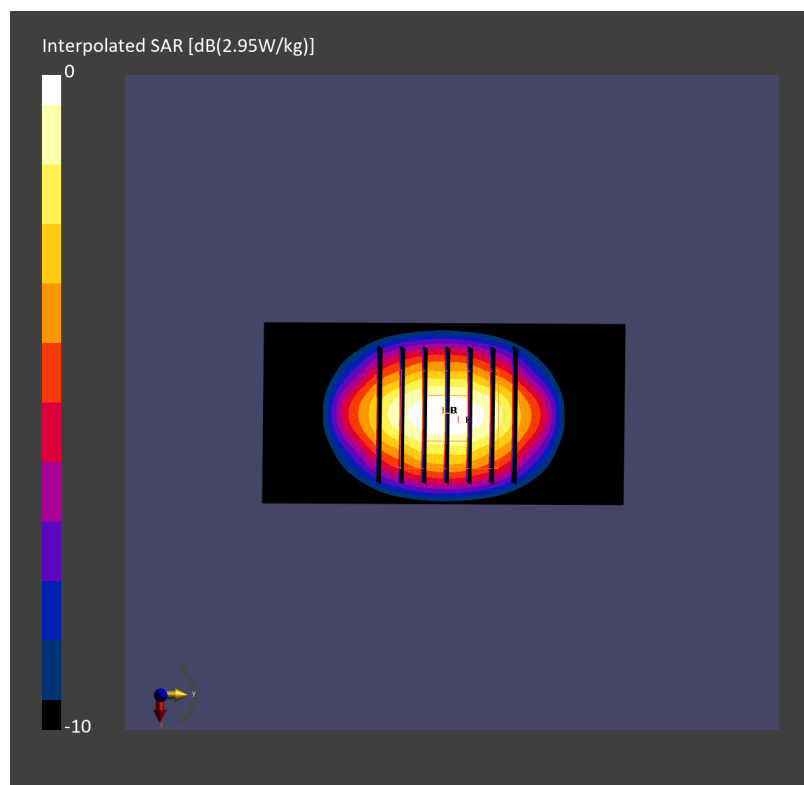

Date: 2024-10-26

System Check_Head_2300MHz**DUT: D2300V2 - SN1006**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL_2300_241026 Medium parameters used: $f = 2300.000$ MHz; $\sigma = 1.68$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.19, 7.54, 7.12); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.28 W/kg; SAR (10g) = 1.08 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.24 W/kg; SAR (8g) = 1.18 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.9 %

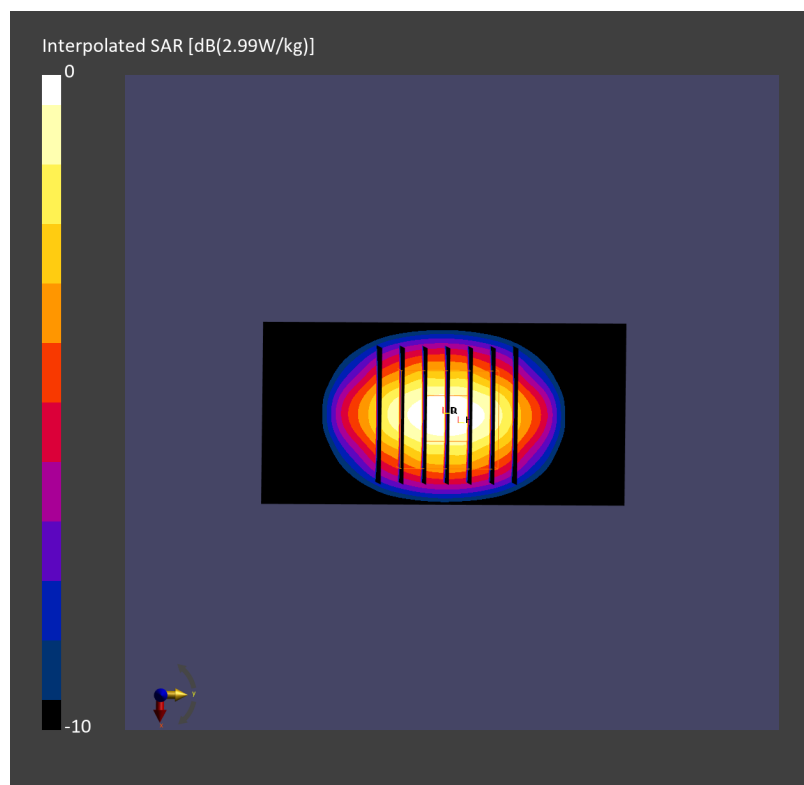

Date: 2024-10-14

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_241014 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 38.1$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.02, 7.36, 6.95); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.10 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5


mm

Power Drift = -0.00 dB

SAR (1g) = 2.59 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.6 %

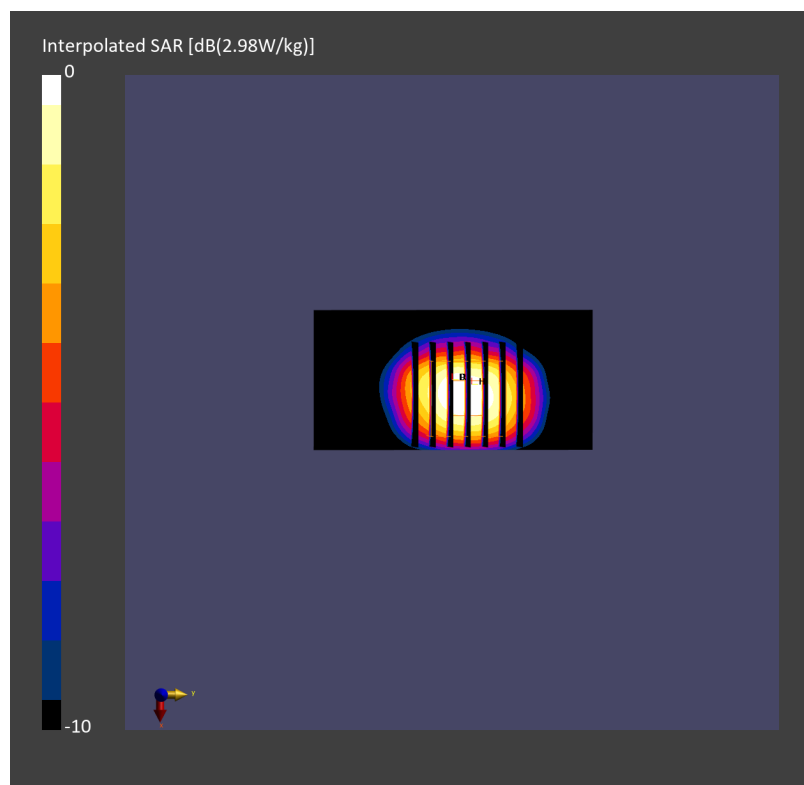

Date: 2024-10-16

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_241016 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.98$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.02, 7.36, 6.95); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.25 W/kg; SAR (10g) = 1.01 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5


mm

Power Drift = 0.00 dB

SAR (1g) = 2.52 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.4 %

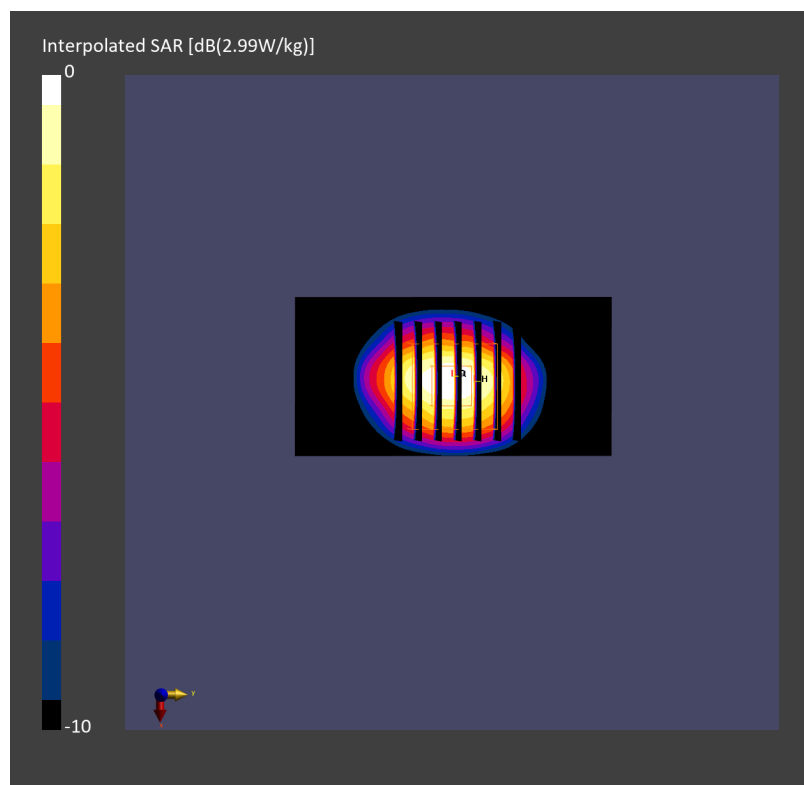

Date: 2024-10-21

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_241021 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.02, 7.36, 6.95); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.21 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5


mm

Power Drift = -0.06 dB

SAR (1g) = 2.71 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 80.2 %

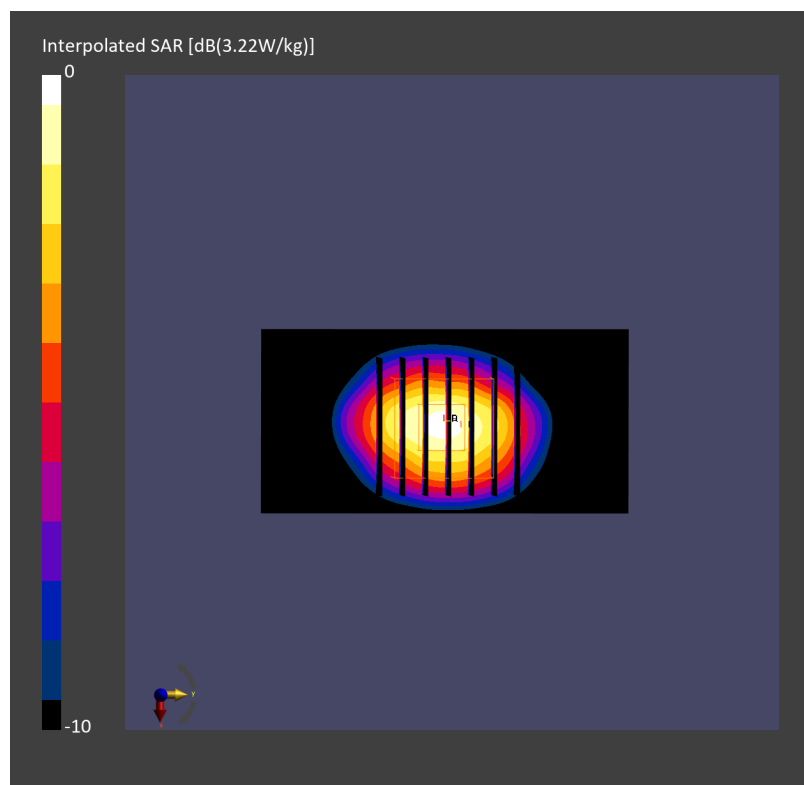

Date: 2024-10-28

System Check_Head_2600MHz**DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL_2600_241028 Medium parameters used: $f = 2600.000$ MHz; $\sigma = 2.00$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(7.02, 7.36, 6.95); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.43 W/kg; SAR (10g) = 1.26 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5


mm

Power Drift = 0.05 dB

SAR (1g) = 2.53 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.27 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.8 %

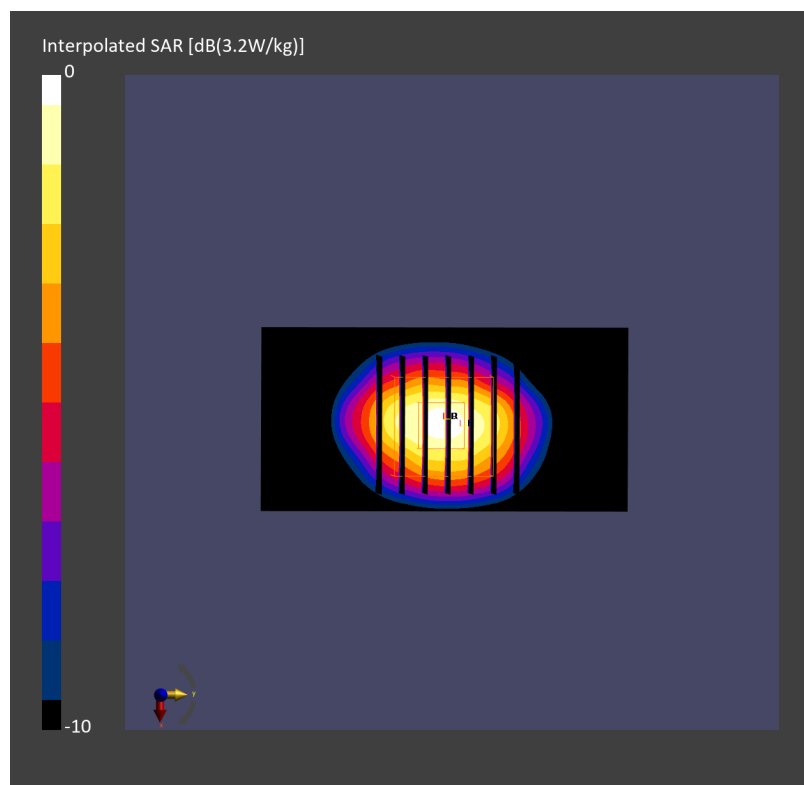

Date: 2024-10-22

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_241022 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.89$ S/m; $\epsilon_r = 38.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.03); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.01 W/kg; SAR (10g) = 1.19 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.12 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 74.2 %

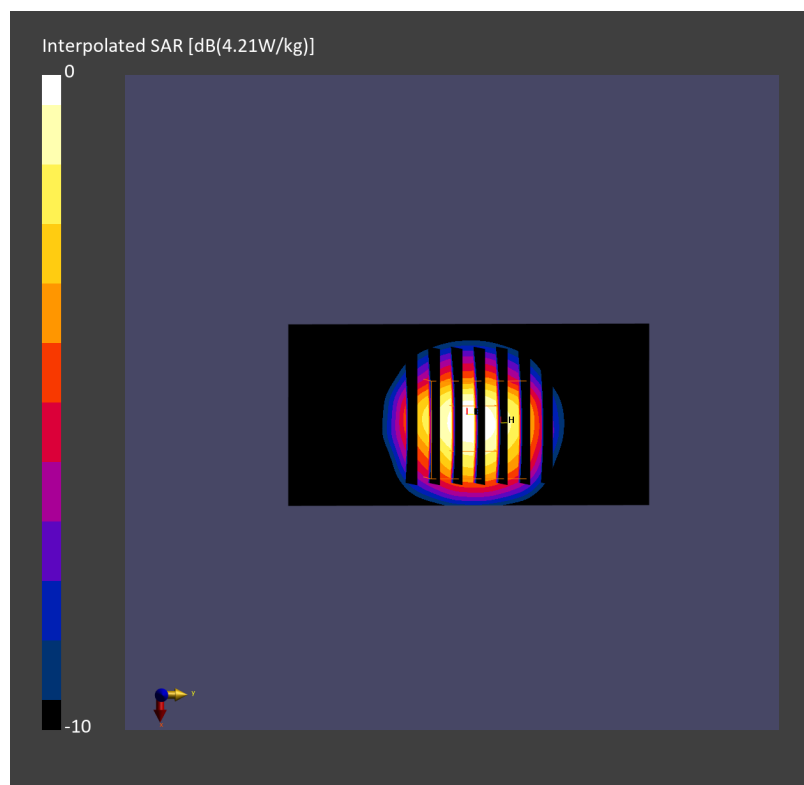

Date: 2024-10-24

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_241024 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.88$ S/m; $\epsilon_r = 37.9$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.03); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.25 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.28 W/kg; SAR (8g) = 1.41 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

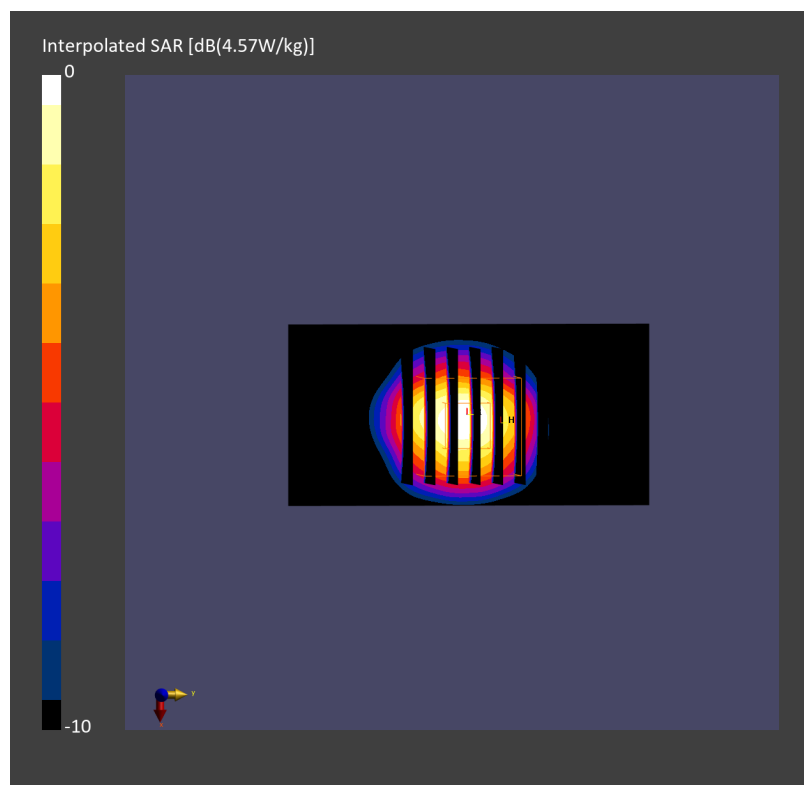

Date: 2024-10-27

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_241027 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.88$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.28, 6.16, 6.53); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.34 W/kg; SAR (10g) = 1.27 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.26 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

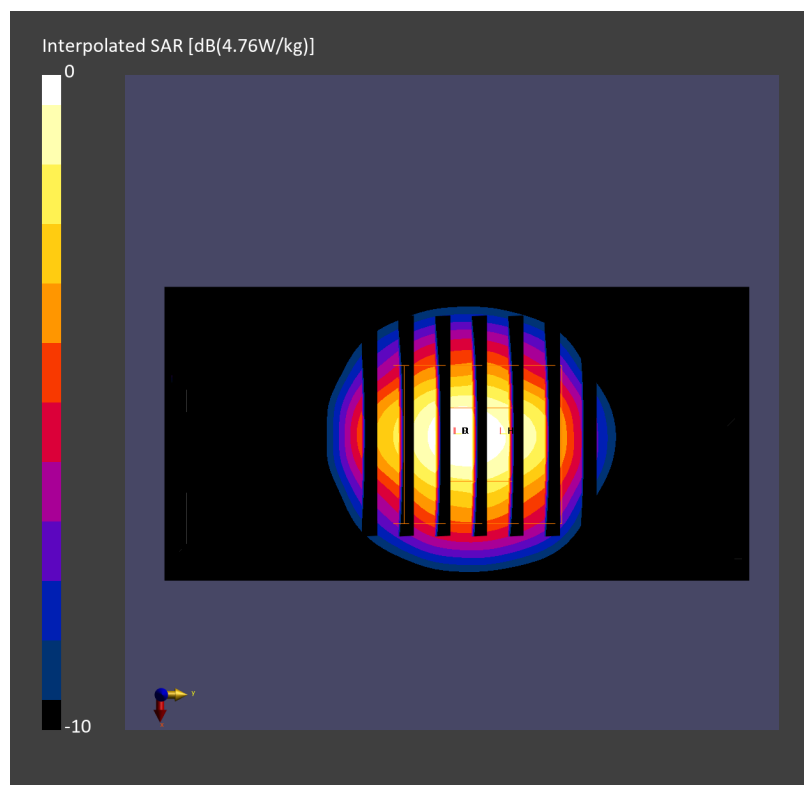

Date: 2024-10-29

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_241029 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.87$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.28, 6.16, 6.53); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.25 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.8 %

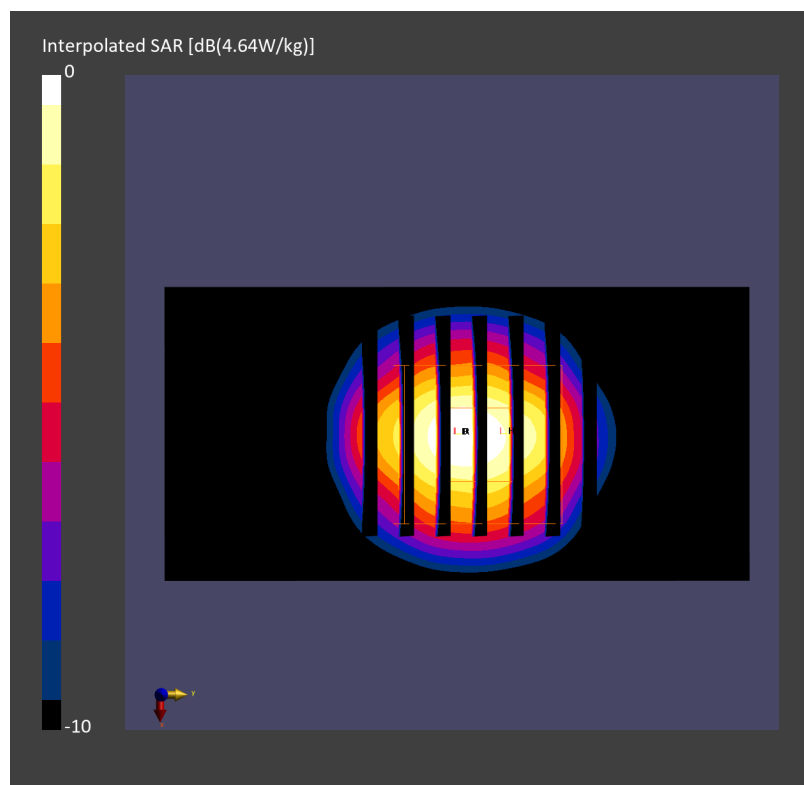

Date: 2024-10-30

System Check_Head_3500MHz**DUT: D3500V2 - SN1036**

Communication System: CW; Frequency: 3500.000 MHz

Medium: HSL_3500_241030 Medium parameters used: $f = 3500.000$ MHz; $\sigma = 2.86$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.03); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.23 W/kg; SAR (10g) = 1.25 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.25 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 76.7 %

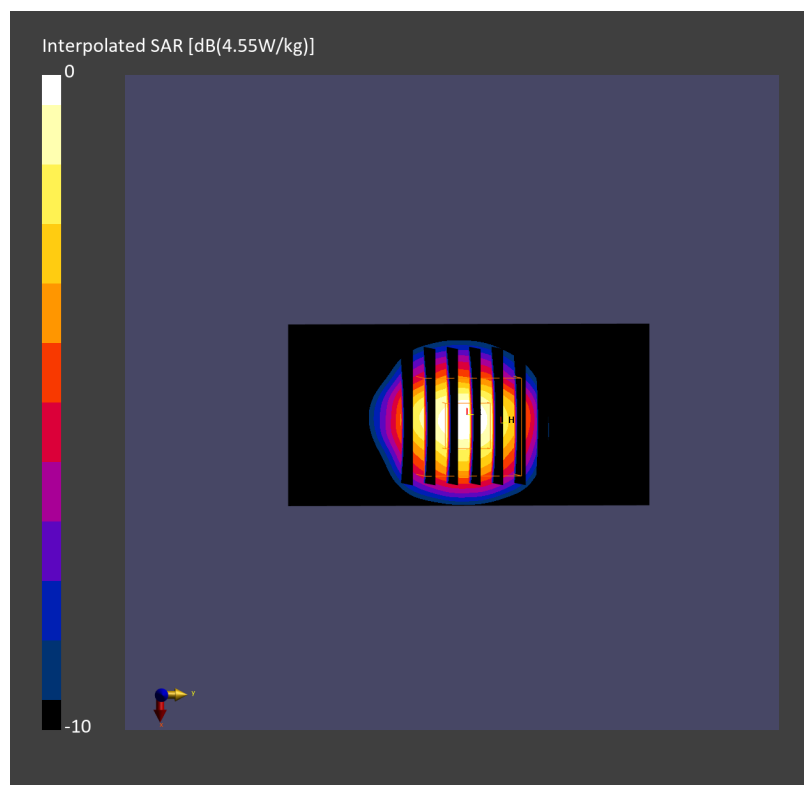

Date: 2024-10-23

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_241023 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.08$ S/m; $\epsilon_r = 37.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.02); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.35 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.2 %

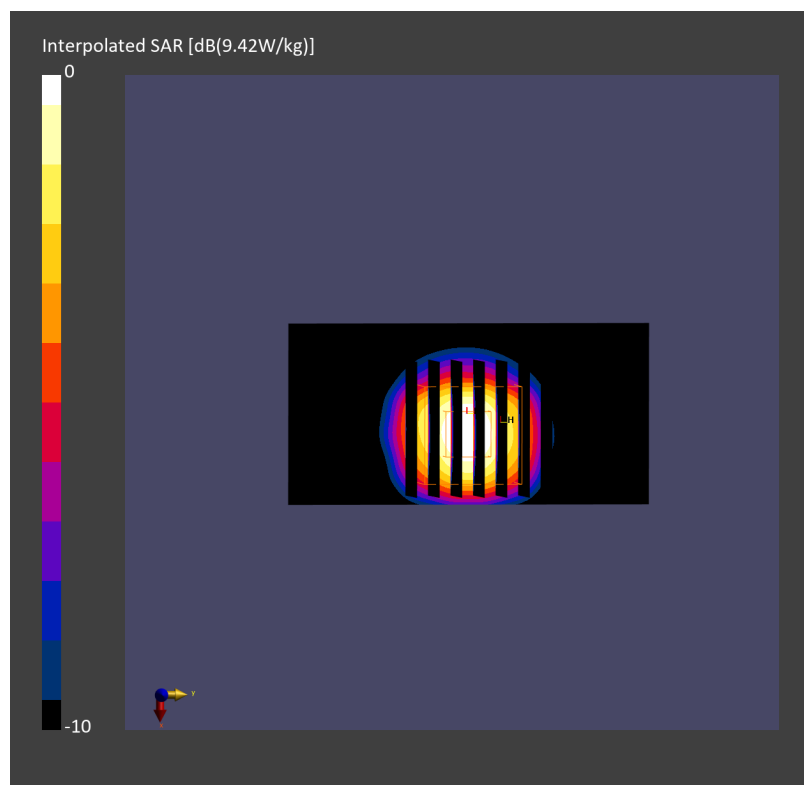

Date: 2024-10-24

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_241024 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.06$ S/m; $\epsilon_r = 37.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.02); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.23 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 3.33 W/kg; SAR (8g) = 1.39 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 73.9 %

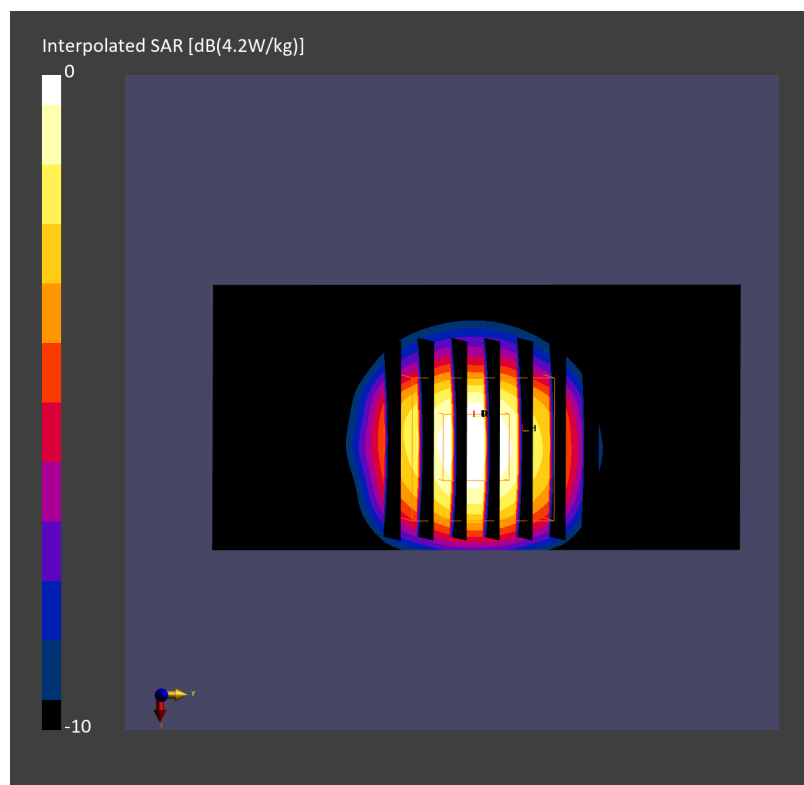

Date: 2024-10-27

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_241027 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.09$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.3, 6.18, 6.55); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.19 W/kg; SAR (10g) = 1.20 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.26 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 76.3 %

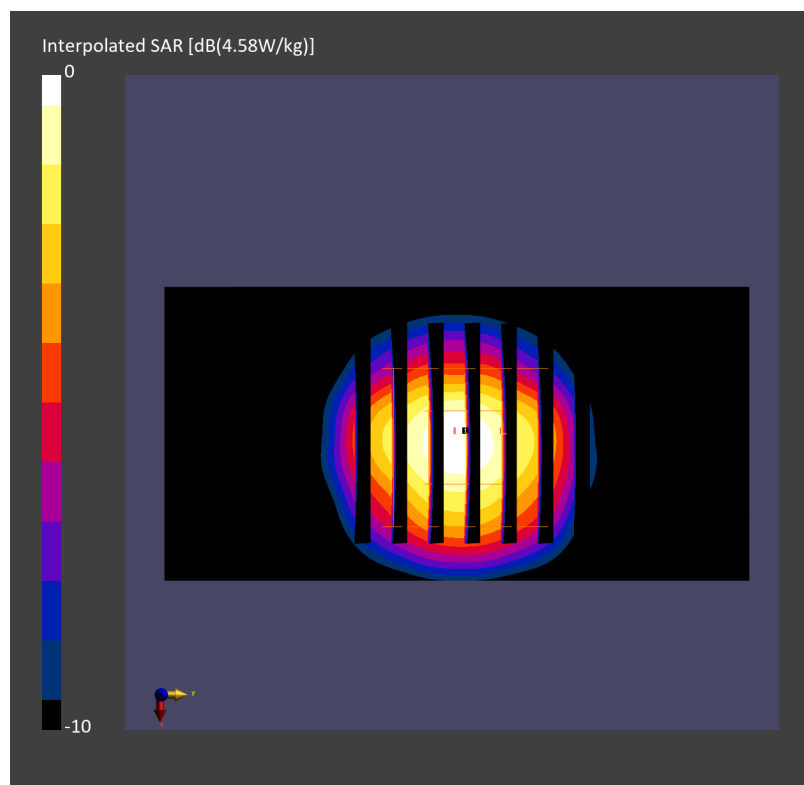

Date: 2024-10-29

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3900_241029 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.06$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.3, 6.18, 6.55); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.19 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.23 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.19 W/kg

Smallest distance from peaks to all points 3 dB below = 8.3 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

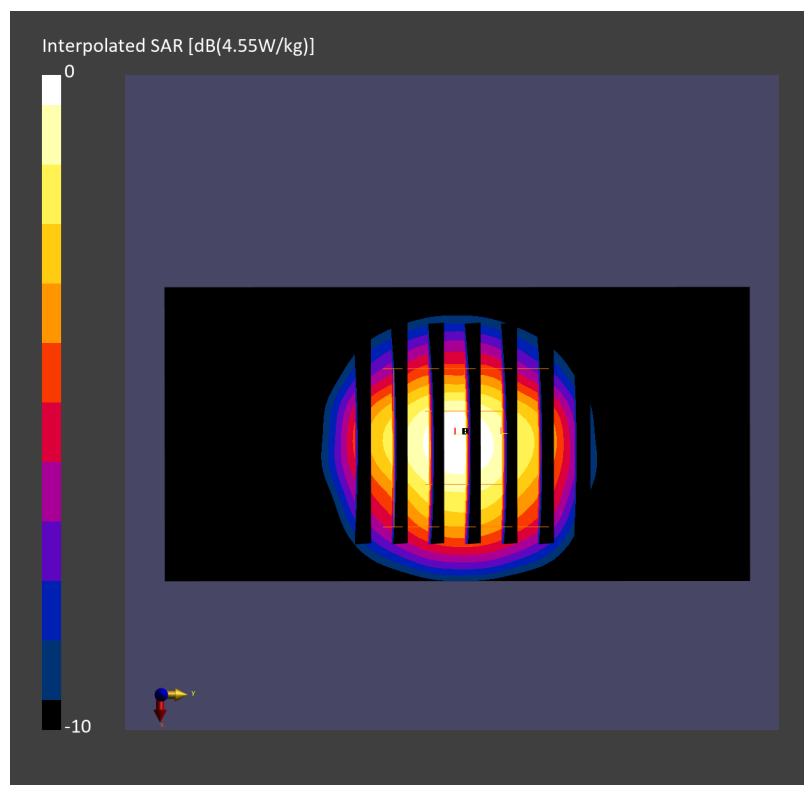

Date: 2024-10-30

System Check_Head_3700MHz**DUT: D3700V2 - SN1006**

Communication System: CW; Frequency: 3700.000 MHz

Medium: HSL_3700_241030 Medium parameters used: $f = 3700.000$ MHz; $\sigma = 3.05$ S/m; $\epsilon_r = 37.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7439; ConvF(6.08, 6.38, 6.02); Calibrated: 2024-08-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.07 W/kg; SAR (10g) = 1.17 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.19 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.18 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 72.9 %

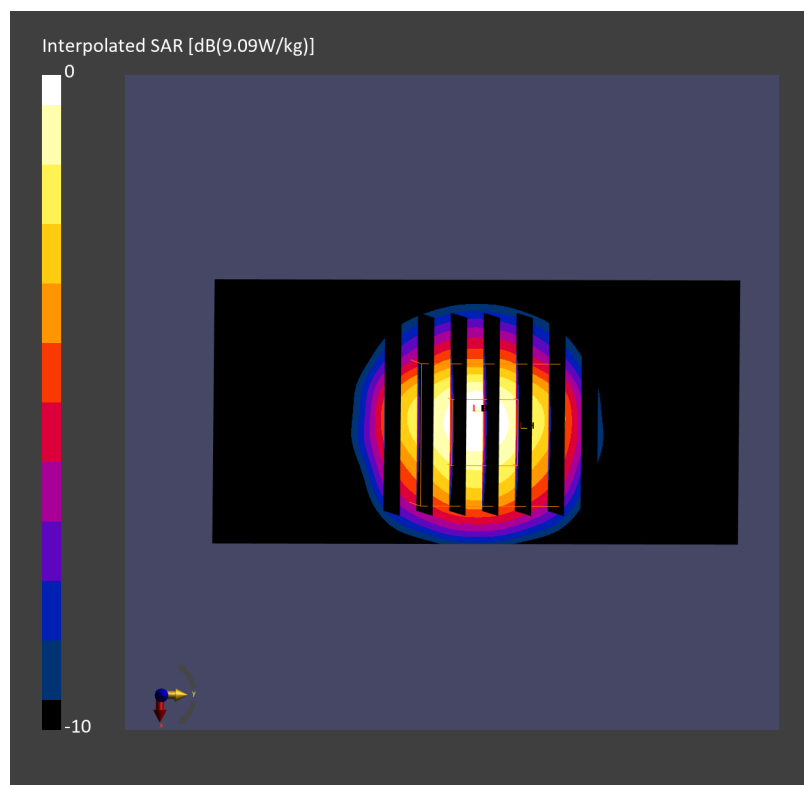

Date: 2024-10-27

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_241027 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.29$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.16, 6.04, 6.41); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.16 W/kg;


Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.30 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 75.0 %

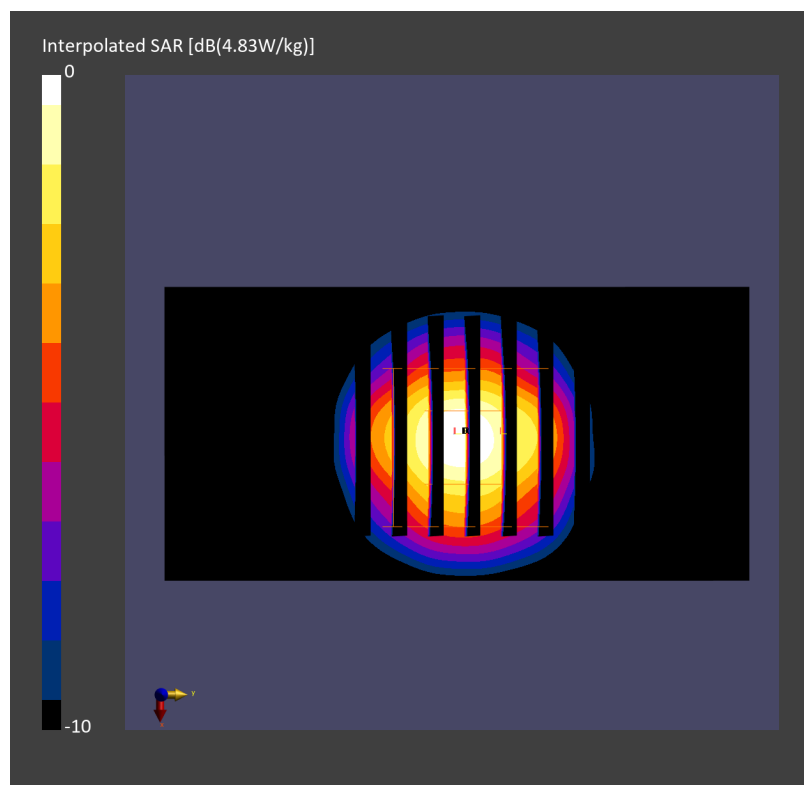

Date: 2024-10-29

System Check_Head_3900MHz**DUT: D3900V2 - SN1017**

Communication System: CW; Frequency: 3900.000 MHz

Medium: HSL_3900_241029 Medium parameters used: $f = 3900.000$ MHz; $\sigma = 3.24$ S/m; $\epsilon_r = 37.5$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.16, 6.04, 6.41); Calibrated: 2024-09-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2024-08-14
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.22 W/kg; SAR (10g) = 1.14 W/kg;

Pin=17.0dBm/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.25 W/kg; SAR (8g) = 1.31 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.0 mm

Ratio of SAR at M2 to SAR at M1 = 74.5 %

