

HAC_E_Dipole_835_160815**DUT: HAC-Dipole 835 MHz**

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ S/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³

Ambient Temperature : 23.4 °C

DASY5 Configuration

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2016/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2016/5/12
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7373)

E Scan - measurement distance from the probe sensor center to CD835 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x361x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 115.1 V/m; Power Drift = 0.02 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 109.1 V/m

Average value of Total=(109.1+99.87) / 2 = 104.485 V/m

PMF scaled E-field



Grid 1 M4 106.8 V/m	Grid 2 M4 109.1 V/m	Grid 3 M4 106.7 V/m
Grid 4 M4 57.78 V/m	Grid 5 M4 59.53 V/m	Grid 6 M4 58.83 V/m
Grid 7 M4 97.41 V/m	Grid 8 M4 99.87 V/m	Grid 9 M4 98.35 V/m

Cursor:

Total = 109.1 V/m

E Category: M4

Location: 0, -77.5, 9.7 mm

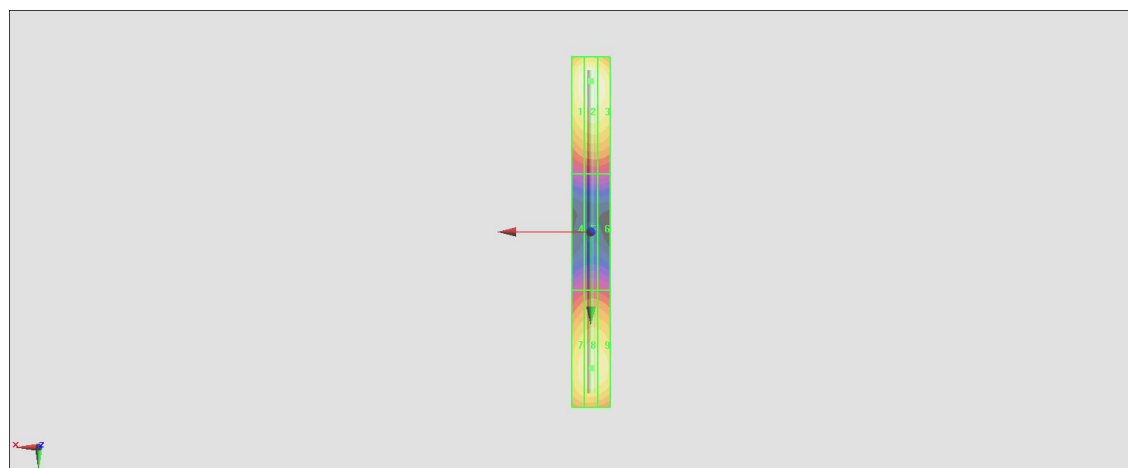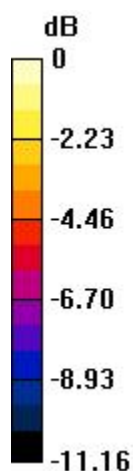

0 dB = 109.1 V/m = 40.76 dBV/m

HAC_E_Dipole_1880_160815**DUT: HAC Dipole 1880 MHz**

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ S/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³

Ambient Temperature : 23.4 °C

DASY5 Configuration

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2016/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2016/5/12
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7373)

E Scan - measurement distance from the probe sensor center to CD1880 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 137.2 V/m; Power Drift = 0.00 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 89.28 V/m

Average value of Total=(86.68+89.28) / 2 = 87.98 V/m

PMF scaled E-field



Grid 1 M3 85.31 V/m	Grid 2 M3 86.68 V/m	Grid 3 M3 85.31 V/m
Grid 4 M3 67.37 V/m	Grid 5 M3 68.87 V/m	Grid 6 M3 68.08 V/m
Grid 7 M3 87.30 V/m	Grid 8 M3 89.28 V/m	Grid 9 M3 87.84 V/m

Cursor:

Total = 89.28 V/m

E Category: M3

Location: 0, 31, 9.7 mm

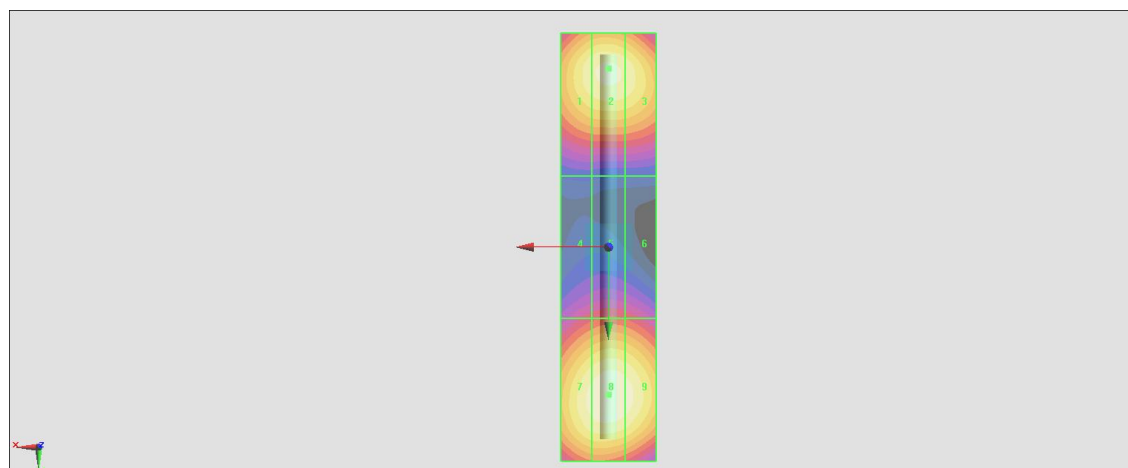

0 dB = 89.28 V/m = 39.02 dBV/m

HAC_E_Dipole_2600_160815**DUT: HAC Dipole 2600 MHz**

Communication System: CW ; Frequency: 2600 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ S/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³

Ambient Temperature : 23.4 °C

DASY5 Configuration

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2016/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2016/5/12
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7373)

E Scan - measurement distance from the probe sensor center to CD2600 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 74.10 V/m; Power Drift = 0.00 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 94.18 V/m

Average value of Total=(87.64+94.17) / 2 = 90.905 V/m

PMF scaled E-field



Grid 1 M3 86.56 V/m	Grid 2 M3 87.64 V/m	Grid 3 M3 86.09 V/m
Grid 4 M3 87.67 V/m	Grid 5 M3 90.24 V/m	Grid 6 M3 89.57 V/m
Grid 7 M3 91.86 V/m	Grid 8 M3 94.17 V/m	Grid 9 M3 93.10 V/m

Cursor:

Total = 94.17 V/m

E Category: M3

Location: -0.5, 20.5, 9.7 mm

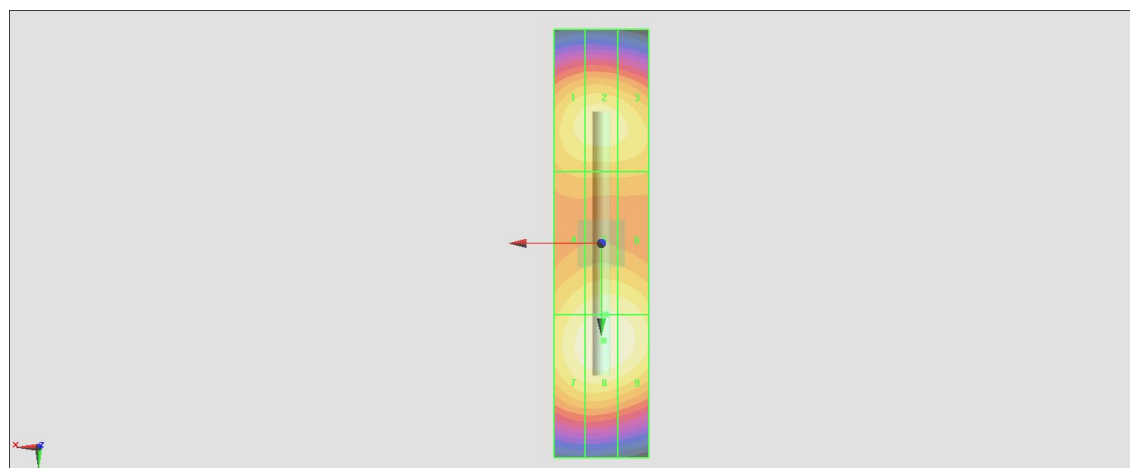

0 dB = 94.17 V/m = 39.48 dBV/m