


Specific Absorption Rate (SAR) Test Report
for
Senton Enterprises Limited
on the
Family Radio Service
Model Number: 99152

Test Report: EME-070003
Issue date: Jan. 23, 2007

Total No of Pages Contained in this Report: 67

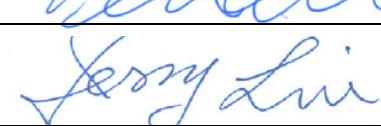

Tested by: Kevin Chen	
Reviewed by: Jerry Liu	

Review Date: Jan. 23, 2007

All services undertaken are subject to the following general policy: Reports are submitted for exclusive use of the client to whom they are addressed. Their significance is subject to the adequacy and representative character of the samples and to the comprehensiveness of the tests, examinations or surveys made. This report shall not be reproduced except in full, without written consent of Intertek Testing Services, Taiwan Ltd.

Table of Contents

1.0 General information	3
1.1 Client Information.....	3
1.2 Equipment under test (EUT).....	4
1.3 Test plan reference.....	4
1.4 Test configuration	5
1.5 Modifications required for compliance.....	6
2.0 SAR Evaluation.....	7
2.1 SAR Limits	7
2.2 Configuration Photographs	8
2.3 SAR measurement system	11
2.4 SAR measurement system validation	12
2.5 Test Result	19
3.0 Test Equipment	21
3.1 Equipment List.....	21
3.2 Tissue Simulating Liquid	22
3.3 E-Field Probe and 450 Balanced Dipole Antenna Calibration	25
4.0 Measurement Uncertainty	26
5.0 Warning Label Information - USA	28
6.0 References	29
7.0 Document History	30
APPENDIX A - SAR Evaluation Data.....	31
APPENDIX B - Photographs.....	40
APPENDIX C - E-Field Probe and 450MHz Balanced Dipole Antenna Calibration Data.....	43

1.0 General information

The Senton sample device, model # 99152 was evaluated in accordance with the requirements for compliance testing defined in FCC OET Bulletin 65, Supplement C (Edition 01-01). Testing was performed at the Intertek Testing Services facility in Hsinchu, Taiwan. The maximum output power declared by the Senton.

The EUT was evaluated in a face-held configuration with the front of the radio placed parallel to the outer surface of the planar. A 2.5cm separation distance was maintained between the front side of the EUT and the outer surface of the planar phantom for the duration of the test.

The EUT was tested in a body-worn configuration with the rear of the radio placed parallel to outer surface of the planar phantom. The attached plastic belt-clip was touching the planar phantom.

For the evaluation, the dosimetric assessment system INDEXSAR SARA2 was used. The phantom employed was the box phantom of 2 mm thick in one wall. The total uncertainty for the evaluation of the spatial peak SAR values averaged over a cube of 1g tissue mass had been assessed for this system to be $\pm 20.6\%$.

The device was tested in unmodulated continuous transmit operation (Continuous Wave at 100% duty cycle) with the transmit key constantly depressed. For a push-to-talk device, the 50% duty cycle compensation reported assumes a transmit/ receive cycle of equal time base.

In summary, the maximum spatial peak SAR value for the sample device averaged over 1g was found to be:

Phantom	Position	SAR _{1g} , W/kg
2 mm thick box phantom wall for evaluation	EUT front to the phantom, 25 mm separation. 462MHz band _channel 4	0.064 W/kg

In conclusion, the tested Sample device was found to be in compliance with the requirements defined in OET Bulletin 65, Supplement C (Edition 01-01) for head and body configurations.

1.1 Client Information

The 99152 has been tested at the request of:

Applicant: **Senton Enterprises Limited**
Flat10, 17/F., Fotan Ind. Centre, 26-28 Au Pui Wan St., Fo Tan, Shatin, N.T.
Hong Kong

1.2 Equipment under test (EUT)**Product Descriptions:**

Equipment	Family Radio Service		
Trade Name	SENTON	Model No:	99152
FCC ID	PEG99152	S/N No.	Not Labeled
Category	<i>Portable</i>	RF Exposure	Uncontrolled Environment
Frequency Band	462.5625 – 462.7125 MHz for FRS 467.5625 – 467.7125 MHz for FRS 462.5500 – 462.7250 MHz for GMRS	System	F3E

EUT Antenna Description			
Type	Integral/ helix	Configuration	Fixed
Dimensions	43 mm length	Gain	0 dBi
Location	Embedded		

Use of Product : Family Radio Service**Manufacturer:** XIAMEN NETCOM ELECTRONIC Co., LTD**Production is planned:** [X] Yes, [] No**EUT receive date:** Jan. 02, 2007**EUT status:** Normal operating condition**Test start date:** Jan. 09, 2007**Test end date:** Jan. 09, 2007**1.3 Test plan reference**

FCC Rule: Part 2.1093, FCC's OET Bulletin 65, Supplement C (Edition 01-01) and IEEE 1528

1.4 Test configuration

Please refer to section 2.2 figure 2 ~ 5

1.4.1 Support equipment & EUT antenna position

Support Equipment				
Item #	Equipment	Brand	Model No.	S/N
1	N/A	N/A	N/A	N/A



1.4.2 Test Condition

During tests the worst-case data (max RF coupling) was determined with following conditions:

Usage	Operates with a built-in test mode by client	Distance between antenna axis at the joint and the liquid surface:	For head, EUT front to phantom, 25 mm separation.	
Simulating human Head/ Body	Head and Body	EUT Battery	New with 4 Alkaline batteries	
E.R.P. for 462MHz Band	Channel	Frequency MHz	Before SAR Test (dBm)	After SAR Test (dBm)
	Mid Channel – 4	462.6375	20.56	20.52
E.R.P. for 467MHz Band	Channel	Frequency MHz	Before SAR Test (dBm)	After SAR Test (dBm)
	Mid Channel – 11	467.6375	20.24	20.23

The spatial peak SAR values were assessed for middle operating channels, defined by the manufacturer.

The EUT was transmitted continuously during the test (Continuous Wave at 100% duty cycle). For a push-to-talk device, the 50% duty cycle compensation reported assumes a transmit/ receive cycle of equal time base.

The EUT take general alkaline batteries as its power source. Each test was proceeded with new batteries.

1.5 Modifications required for compliance

The EUT has no modifications during test.

2.0 SAR Evaluation

The evaluation of the result analysis was based on software: SARA2 Version 2.41VPM (**Virtual Probe Miniaturization**).

2.1 SAR Limits

The following FCC limits for SAR apply to devices operate in General Population/Uncontrolled Exposure environment:



EXPOSURE (General Population/Uncontrolled Exposure environment)	SAR (W/kg)
Average over the whole body	0.08
Spatial Peak (1g)	1.60
Spatial Peak for hands, wrists, feet and ankles (10g)	4.00



2.2 Configuration Photographs

SAR Measurement Test Setup

Figure 1: Test System

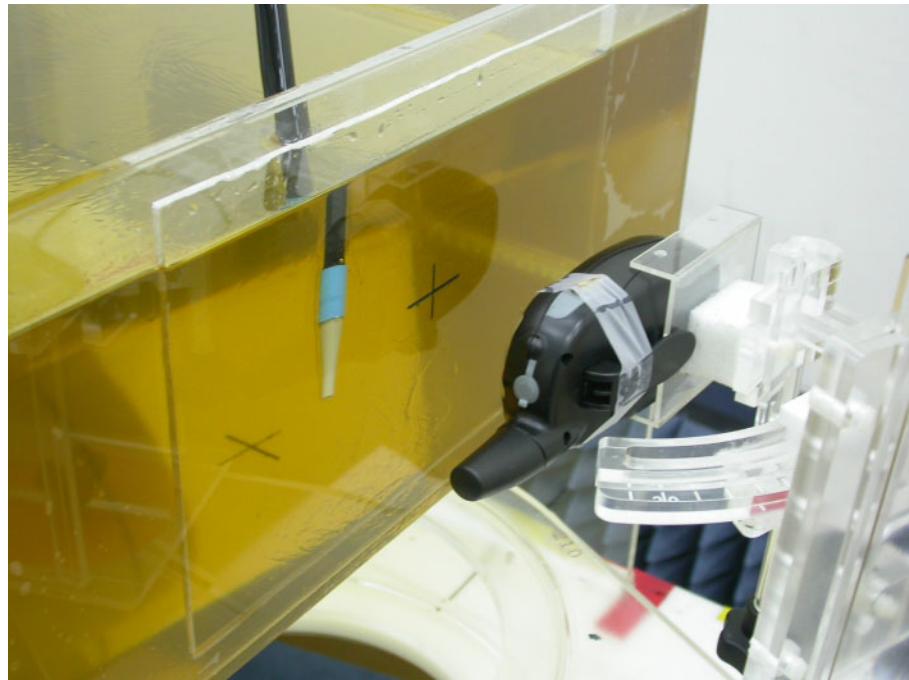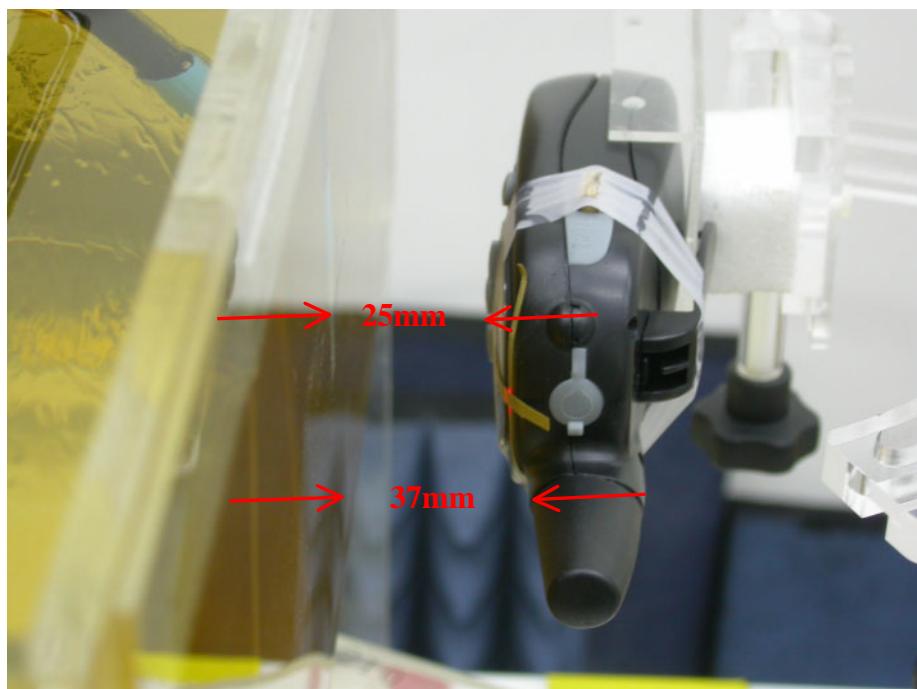

SAR Measurement Test Setup**Figure 2: For head, EUT front to phantom, 25 mm separation****SAR Measurement Test Setup****Figure 3: For head, EUT front to phantom, 25 mm separation – Zoom In**

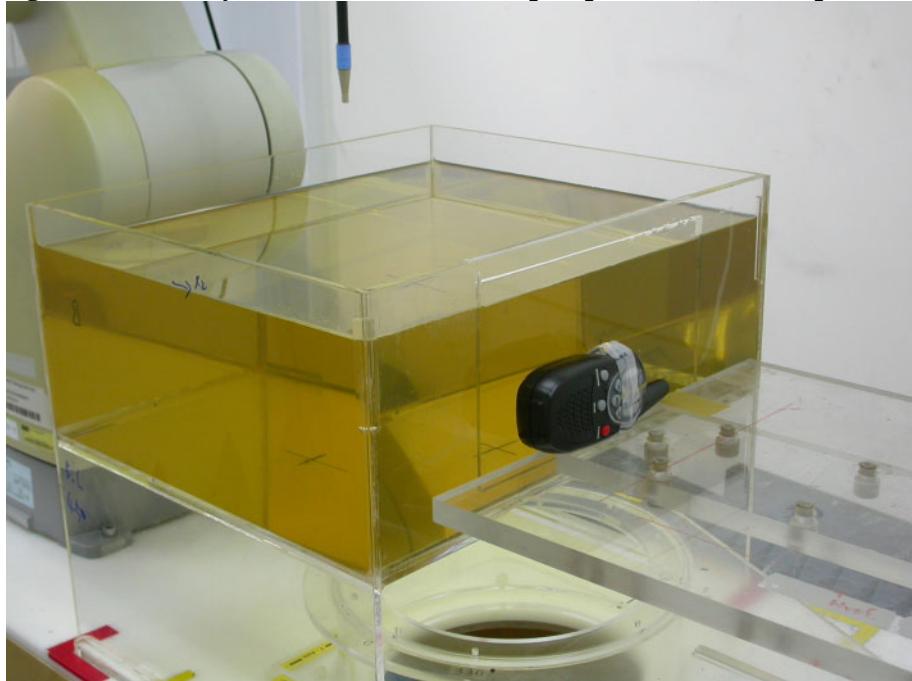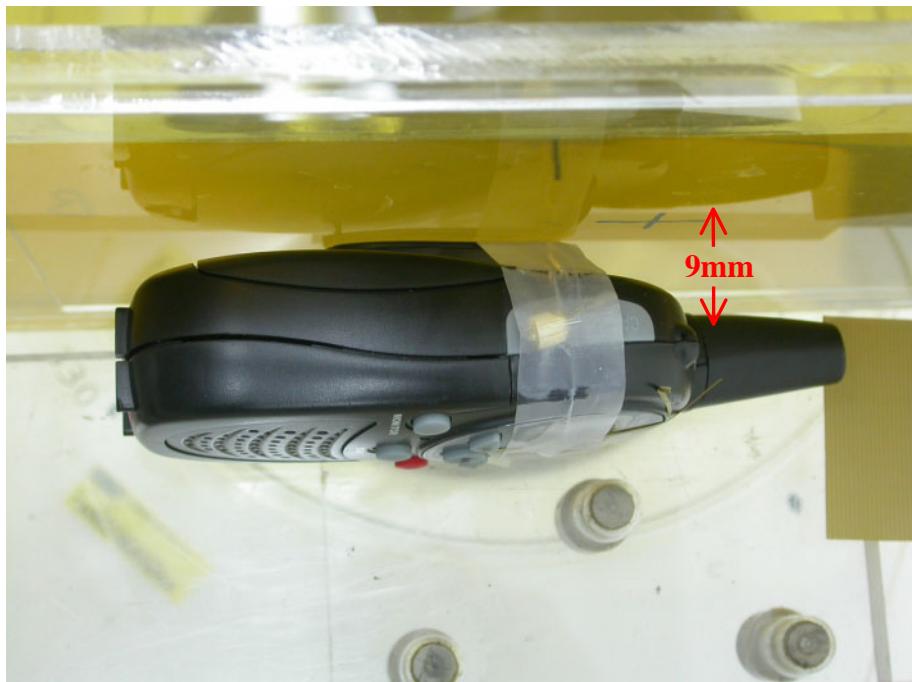SAR Measurement Test Setup**Figure 4: For body, EUT rear with belt-clip to phantom, 0 mm separation****SAR Measurement Test Setup****Figure 5: For body, EUT rear with belt-clip to phantom, 0 mm separation-Zoon In**

2.3 SAR measurement system

Robot system specification

The SAR measurement system being used is the IndexSAR SARA2 system, which consists of a Mitsubishi RV-E2 6-axis robot arm and controller, IndexSAR probe and amplifier and SAM phantom Head Shape. The robot is used to articulate the probe to programmed positions inside the phantom head to obtain the SAR readings from the DUT.

The system is controlled remotely from a PC, which contains the software to control the robot and data acquisition equipment. The software also displays the data obtained from test scans.

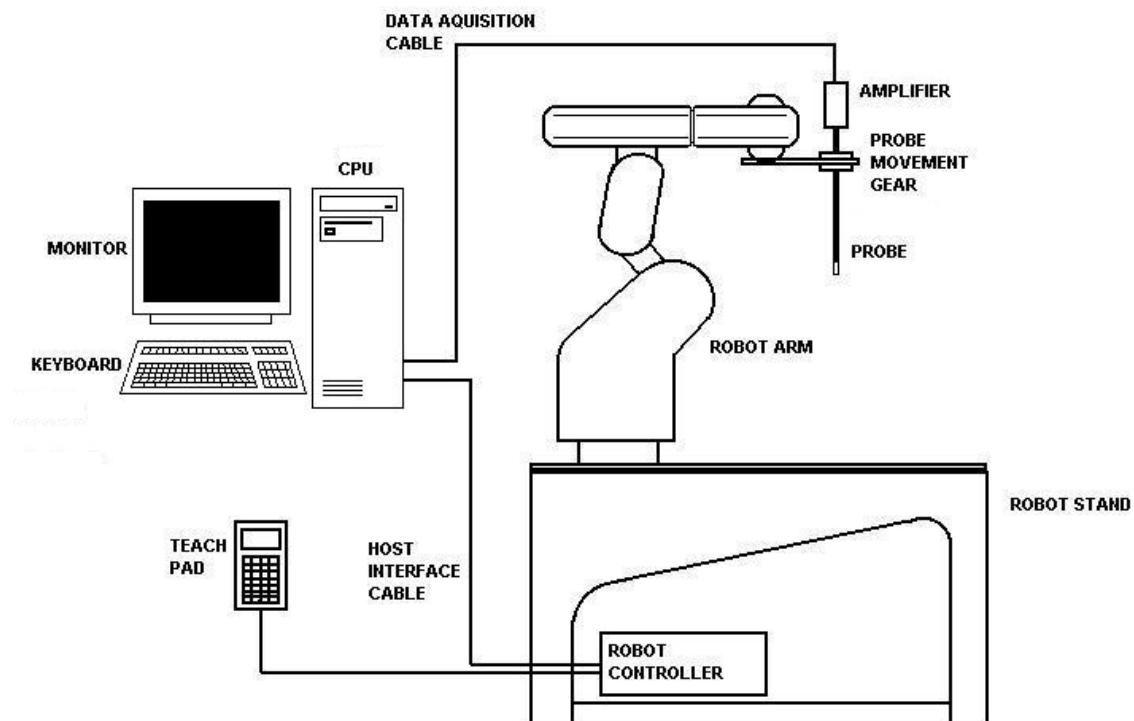


Figure 1: Schematic diagram of the SAR measurement system

The position and digitised shape of the phantom heads are made available to the software for accurate positioning of the probe and reduction of set-up time.

The SAM phantom heads are individually digitised using a Mitutoyo CMM machine to a precision of 0.02mm. The data is then converted into a shape format for the software, providing an accurate description of the phantom shell. In operation, the system first does an area (2D) scan at a fixed depth within the liquid from the inside wall of the phantom. When the maximum SAR point has been found, the system will then carry out a 3D scan centred at that point to determine volume averaged SAR level.

The first 2 measurements points in a direction perpendicular to the surface of the phantom during the zoom scan and closest to the phantom surface, were only 3.5mm and the probe is kept at greater than half a diameter from the surface.

2.4 SAR measurement system validation


Prior to the assessment, the system was verified to the $\pm 10\%$ of the specifications by using the system validation equipments. The validation was performed at 450 MHz on the bottom side of box phantom.

Procedures

The SAR evaluation was performed with the following procedures:

- a. The SAR distribution was measured at the exposed side of the bottom of the box phantom and was measured at a distance of 15 mm for 300 ~ 1000 MHz and 10 mm for 1000 ~ 3000 MHz from the inner surface of the shell. The feed power was 1/5W.
- b. The dimension for this cube is 32 mm x 32 mm x 34 mm was assessed by measuring 5 x 5 x 7 points. On the basis of this data set, the spatial peak SAR value was evaluated with the following procedure:
 - i) The data at the surface were extrapolated, since the center of the dipoles is 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measurement point is 5 mm. The extrapolation was based on a least square algorithm. A polynomial of the fourth order was calculated through the points in Z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.
 - ii) The maximum interpolated value was searched with a straightforward algorithm. Around this maximum, the SAR values averaged over the spatial volumes (1g or 10g) were computed using the 3-D spline interpolation algorithm. The 3-D spline is composed of three one-dimensional splines with the “Not a knot” condition (in x, y and z directions). The volume was integrated with the trapezoidal algorithm. 1000 points (10 x 10 x 10) were interpolated to calculate the average.
 - iii) All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.

The test scan procedure for system validation also apply to the general scan procedure except for the set-up position. For general scan, the EUT was placed at the side of phantom. For validation scan, the dipole antenna was placed at the bottom of phantom.

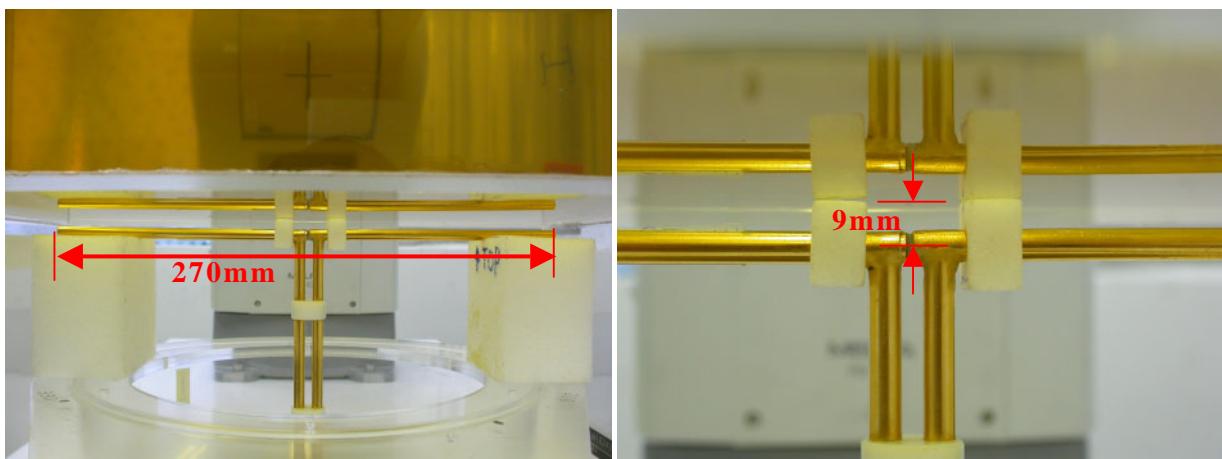

2.4.1 System Validation result

System Validation (450 MHz Head)				
Frequency MHz	Operating Mode	Target SAR_{1g} (W/kg)	Measured SAR_{1g} (W/kg)	Deviation ($\pm 10\%$)
450	CW	4.9	4.78	-2.449%

Please see the plot below:

System Validation (450 MHz Body)				
Frequency MHz	Operating Mode	Target SAR_{1g} (W/kg)	Measured SAR_{1g} (W/kg)	Deviation ($\pm 10\%$)
450	CW	4.9	5.19	5.92%


Please see the plot below

Head Liquid System Validation

Date:	2007/1/8	Position:	Bottom to the Phantom
Filename:	450Head validation.txt	Phantom:	HeadBox3-450_HL-val..csv
Device Tested:	450Head validation	Head Rotation:	0
Antenna:	450 Dipole Antenna	Test Frequency:	450MHz
Shape File:	none.csv	Power Level:	23 dBm

Probe:	0136																
Cal File:	SN0136_450_CW_HEAD																
Cal Factors:	<table border="1"> <tr> <th></th> <th>X</th> <th>Y</th> <th>Z</th> </tr> <tr> <td>Air</td> <td>490</td> <td>377</td> <td>387</td> </tr> <tr> <td>DCP</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Lin</td> <td>.299</td> <td>.299</td> <td>.299</td> </tr> </table>		X	Y	Z	Air	490	377	387	DCP	20	20	20	Lin	.299	.299	.299
	X	Y	Z														
Air	490	377	387														
DCP	20	20	20														
Lin	.299	.299	.299														
Amp Gain:	2																
Averaging:	1																
Batteries Replaced:	-																

Liquid:	15.5cm
Type:	450 MHz Head
Conductivity:	0.889
Relative Permittivity:	44.239
Liquid Temp (deg C):	23
Ambient Temp (deg C):	23
Ambient RH (%):	55
Density (kg/m3):	1000
Software Version:	2.41VPM
Crest Factor = 1	

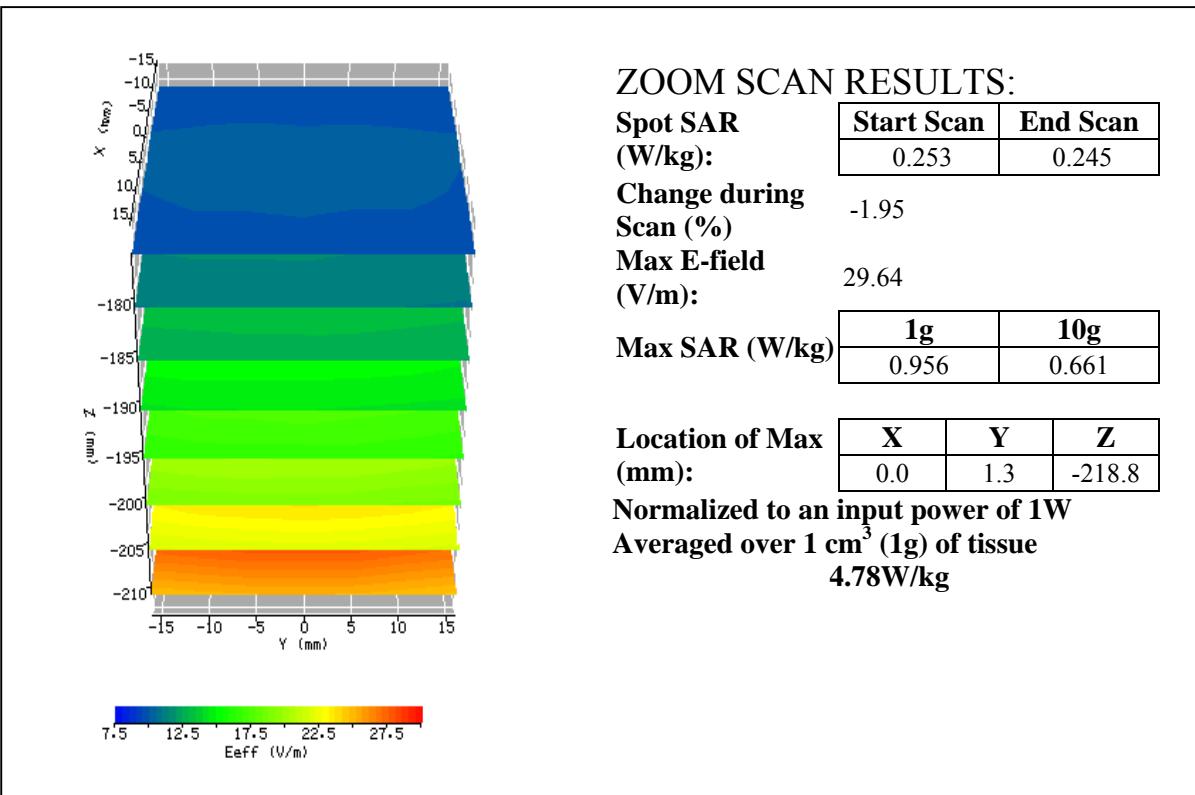


Body Liquid System Validation

Date:	2007/1/8	Position:	Bottom to the Phantom
Filename:	450Body validation.txt	Phantom:	HeadBox3-450_BL-val..csv
Device Tested:	450Body validation	Head Rotation:	0
Antenna:	450 Dipole Antenna	Test Frequency:	450MHz
Shape File:	none.csv	Power Level:	23 dBm

Probe:	0136																
Cal File:	SN0136_450_CW_BODY																
Cal Factors:	<table border="1"> <thead> <tr> <th></th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>Air</td> <td>490</td> <td>377</td> <td>387</td> </tr> <tr> <td>DCP</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Lin</td> <td>.298</td> <td>.298</td> <td>.298</td> </tr> </tbody> </table>		X	Y	Z	Air	490	377	387	DCP	20	20	20	Lin	.298	.298	.298
	X	Y	Z														
Air	490	377	387														
DCP	20	20	20														
Lin	.298	.298	.298														
Amp Gain:	2																
Averaging:	1																
Batteries Replaced:	-																

Liquid:	15.5cm
Type:	450 MHz Body
Conductivity:	1.9236
Relative Permittivity:	57.371
Liquid Temp (deg C):	23
Ambient Temp (deg C):	23
Ambient RH (%):	55
Density (kg/m³):	1000
Software Version:	2.41VPM
Crest Factor = 1	

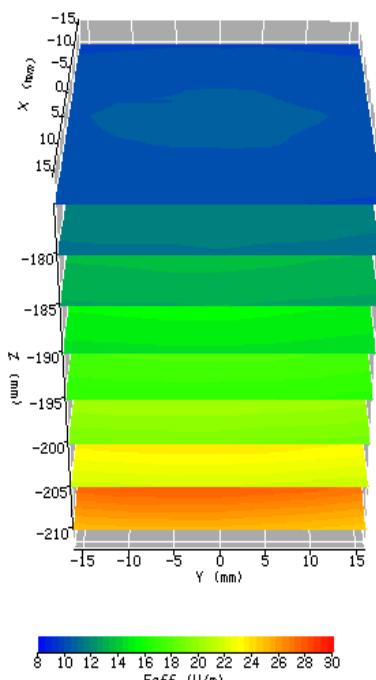

ZOOM SCAN RESULTS:

Spot SAR (W/kg):	Start Scan	End Scan
	0.280	0.274

Change during Scan (%) -1.91

Max E-field (V/m): 29.66

Max SAR (W/kg)	1g	10g
	1.038	0.719

Location of Max (mm):	X	Y	Z
	0.0	1.3	-218.2

**Normalized to an input power of 1W
Averaged over 1 cm³ (1g) of tissue
5.19W/kg**

2.4.2 System Performance Check result

System performance check (450 MHz Head)				
Frequency MHz	Operating Mode	Target SAR_{1g} (W/kg)	Measured SAR_{1g} (W/kg)	Deviation (±10%)
450	CW	4.9	4.78	-2.449%

Deviation (±10%) = (measured – target)/target

Please see the plot below:

System Validation (450 MHz Body)				
Frequency MHz	Operating Mode	Target SAR_{1g} (W/kg)	Measured SAR_{1g} (W/kg)	Deviation (±10%)
450	CW	4.9	5.19	5.92%


Deviation (±10%) = (measured – target)/target

Please see the plot below:

Head Liquid System Performance Check

Date:	2007/1/8	Position:	Bottom to the phantom
Filename:	450 Head per. check.txt	Phantom:	HeadBox3-450_HL-val..csv
Device Tested:	450 performance check	Head Rotation:	0
Antenna:	450 dipole ant.	Test Frequency:	450MHz
Shape File:	none.csv	Power Level:	23 dBm


Probe:	0136	Liquid:	15.5cm																
Cal File:	SN0136_450_CW_HEAD	Type:	450 MHz Head																
Cal Factors:	<table border="1"> <thead> <tr> <th></th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>Air</td> <td>490</td> <td>377</td> <td>387</td> </tr> <tr> <td>DCP</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Lin</td> <td>.299</td> <td>.299</td> <td>.299</td> </tr> </tbody> </table>		X	Y	Z	Air	490	377	387	DCP	20	20	20	Lin	.299	.299	.299	Conductivity:	0.889
	X	Y	Z																
Air	490	377	387																
DCP	20	20	20																
Lin	.299	.299	.299																
Amp Gain:	2	Relative Permittivity:	44.239																
Averaging:	1	Liquid Temp (deg C):	23																
Batteries Replaced:	-	Ambient Temp (deg C):	22																
		Ambient RH (%):	56																
		Density (kg/m3):	1000																
		Software Version:	2.41VPM																

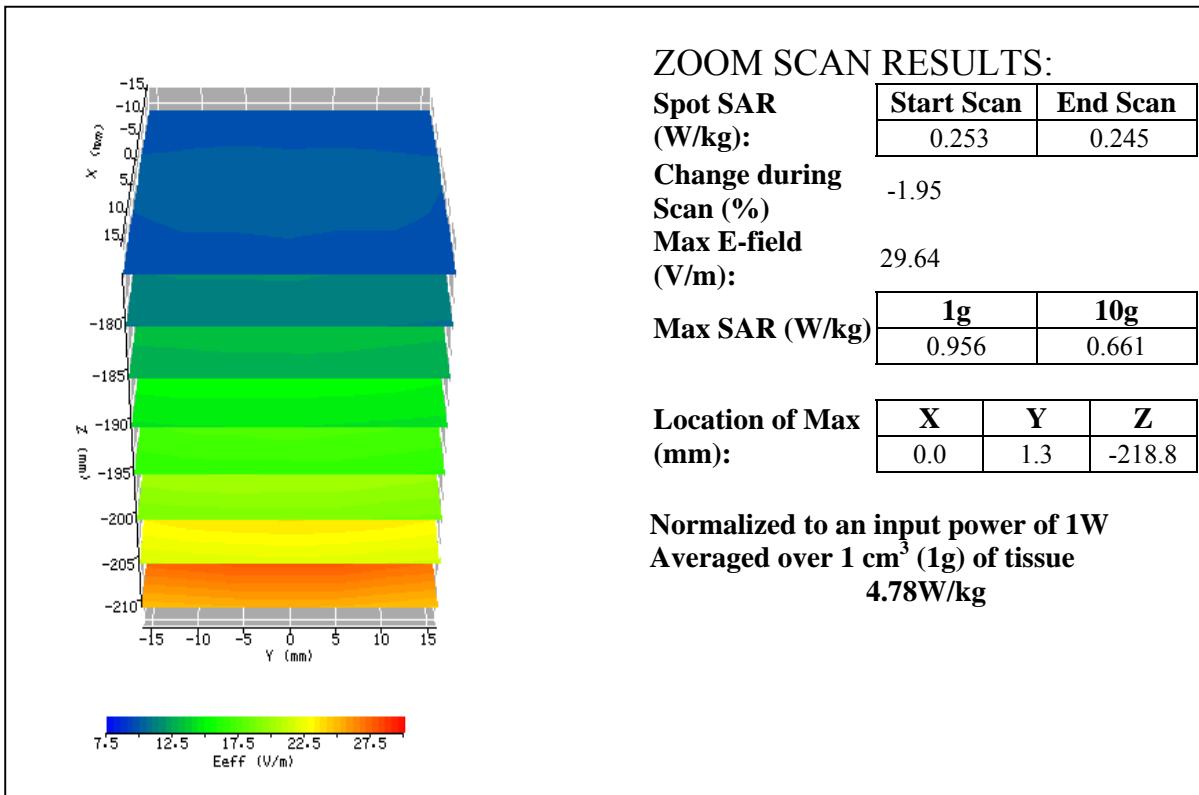

Body Liquid System Performance Check

Date:	2007/1/8	Position:	Bottom to the phantom
Filename:	450 Body per. check.txt	Phantom:	HeadBox5-450_BL-val..csv
Device Tested:	450B performance check	Head Rotation:	0
Antenna:	450 dipole ant.	Test Frequency:	450MHz
Shape File:	none.csv	Power Level:	23 dBm

Probe:	0136	Liquid:	15.5cm																
Cal File:	SN0136_450_CW_BODY	Type:	450 MHz Body																
Cal Factors:	<table border="1"> <tr> <th></th> <th>X</th> <th>Y</th> <th>Z</th> </tr> <tr> <td>Air</td> <td>490</td> <td>377</td> <td>387</td> </tr> <tr> <td>DCP</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Lin</td> <td>.298</td> <td>.298</td> <td>.298</td> </tr> </table>		X	Y	Z	Air	490	377	387	DCP	20	20	20	Lin	.298	.298	.298	Conductivity:	1.9236
	X	Y	Z																
Air	490	377	387																
DCP	20	20	20																
Lin	.298	.298	.298																
Amp Gain:	2	Relative Permittivity:	57.371																
Averaging:	1	Liquid Temp (deg C):	23																
Batteries		Ambient Temp (deg C):	22																
Replaced:	-	Ambient RH (%):	56																
		Density (kg/m³):	1000																
		Software Version:	2.41VPM																

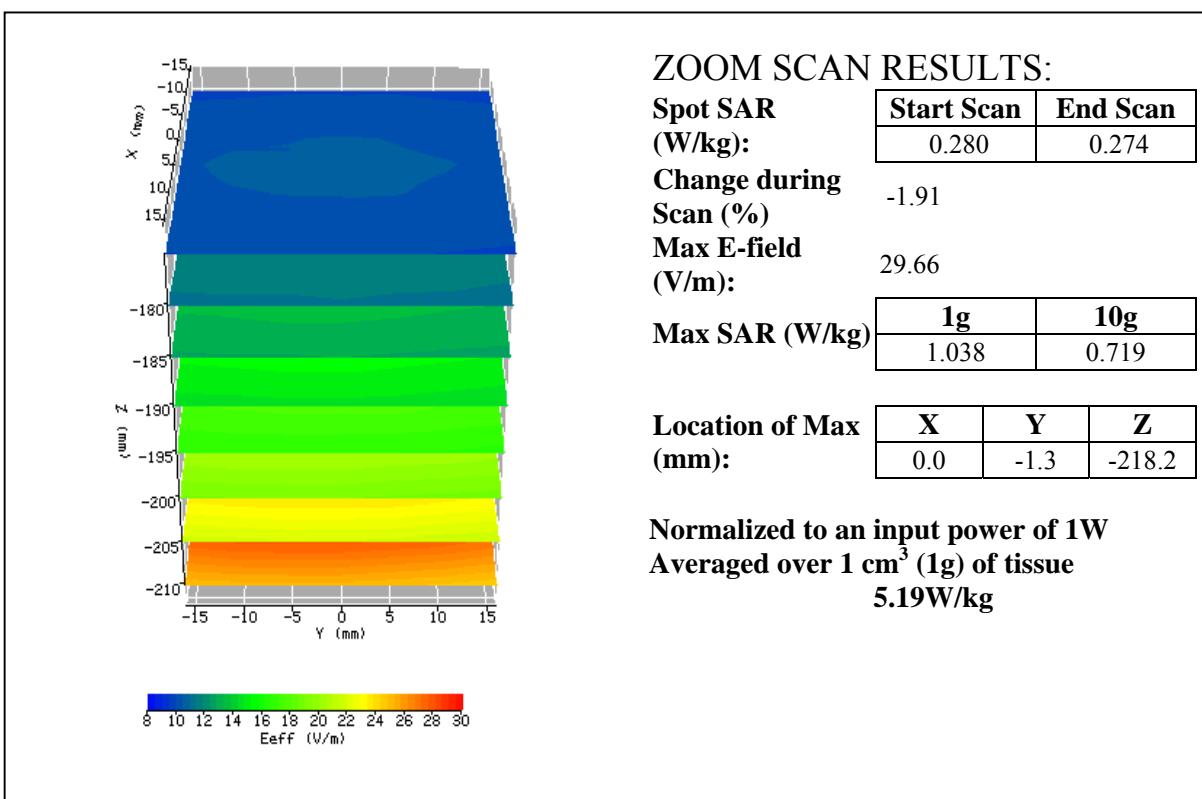

2.5 Test Result

The results on the following page(s) were obtained when the device was tested in the condition described in this report. Detailed measurement data and plots, which reveal information about the location of the maximum SAR with respect to the device, are reported in Appendix A.

Measurement Results

Trade Name:	SENTON	Model No.:	99152
Serial No.:	Not Labeled	Test Engineer:	Kevin Chen
TEST CONDITIONS			
Ambient Temperature	23 °C	Relative Humidity	50 %
Test Signal Source	Test Mode	Signal Modulation	F3E
Output Power Before SAR Test	See section 1.4.2	Output Power After SAR Test	See section 1.4.2
Test Duration	23 min. each scan	Number of Battery Change	new alkaline batteries for each Scan

Test Mode: Body evaluation with belt-clip

EUT Position								
Channel (MHz)	Operating Mode	Crest Factor	Description	Distance (mm)	Measured SAR_{1g} (W/kg)		Plot Number	
					Duty Cycle			
					100%	50%		
462.6375 (CH_4)	F3E	1	Rear to phantom	0	0.122	0.061	1	
467.6375 (CH_11)	F3E	1	Rear to phantom	0	0.051	0.026	2	

Test Mode: Head evaluation

EUT Position								
Channel (MHz)	Operating Mode	Crest Factor	Description	Distance (mm)	Measured SAR_{1g} (W/kg)		Plot Number	
					Duty Cycle			
					100%	50%		
462.6375 (CH_4)	F3E	1	Front to phantom	25	0.128	0.064	3	
467.6375 (CH_11)	F3E	1	Front to phantom	25	0.070	0.035	4	

3.0 Test Equipment

3.1 Equipment List

The Specific Absorption Rate (SAR) tests were performed with the INDEXSAR SARA2 SYSTEM.

The following major equipment/components were used for the SAR evaluations:

SAR Measurement System			
EQUIPMENT	SPECIFICATIONS	Intertek ID No.	LAST CAL. DATE
Balanced Validation dipole	450MHz	EC381-1	01/2007
Controller	Mitsubishi CR-E116	EP320-1	N/A
Robot	Mitsubishi RV-E2	EP320-2	N/A
	Repeatability: $\pm 0.04\text{mm}$; Number of Axes: 6		
E-Field Probe	IXP-050	EC356	03/2006
	Frequency Range: 450MHz ~ 2450MHz Probe outer diameter: 5.2 mm; Length: 350 mm; Distance between the probe tip and the dipole center: 2.7 mm		
Data Acquisition	SARA2	N/A	N/A
	Processor: Pentium 4; Clock speed: 1.5GHz; OS: Windows XP; I/O: two RS232; Software: SARA2 Ver. 2.41VPM (Virtual Probe Minaturisation)		
Phantom	2 mm wall thickness box phantom in one wall	N/A	N/A
	Shell Material: clear Perspex; Thickness: $2 \pm 0.1\text{ mm}$; Capacity: $336 \times 397 \times 173\text{ (W x L x D)}$ mm ³ ; Dielectric constant: less than 2.85 above 500MHz;		
Device holder	Material: clear Perspex	N/A	N/A
	Dielectric constant: less than 2.85 above 500MHz		
Simulated Tissue	Mixture	N/A	01/08/2007
	Please see section 3.2 for details		
Vector Network Analyzer	HP 8753B HP 85046A	EC375	08/19/2006
	300k to 3GHz		
Signal Generator	R&S SMR27	EC354	08/16/2006
	10M to 27GHz, <120dBuV		
Wideband Peak Power Meter/ Sensor	Anritsu ML2497A with MA2491A Power sensor	EC396	10/19/2006
	Frequency Range: 100MHz~18GHz		

3.2 Tissue Simulating Liquid

The head and body tissue parameters should be used to test operating frequency band of transmitters. When a transmission band overlaps with one of the target frequencies, the tissue dielectric parameters of the tissue medium at the middle of a device transmission band should be within $\pm 5\%$ of the parameters specified at that target frequency.

3.2.1 Body Tissue Simulating Liquid

Body Ingredients Frequency (450 MHz)		
Water		51.16%
Salt		1.49%
Sugar		46.78%
HEC (Hydroxyethyl Cellulose)		0.52%
Bactericide		0.05%

The dielectric parameters were verified prior to assessment using the HP 85046A dielectric probe kit and the HP 8753B network Analyzer. The dielectric parameters were:

Frequency (MHz)	Temp. ()	ϵ_r / Relative Permittivity			σ / Conductivity (mho/m)			ρ *(kg/m ³)
		measured	target	($\pm 5\%$)	measured	target	($\pm 5\%$)	
450	23	57.37	56.7	1.18%	0.968	0.94	-2.98%	1000

* Worst-case assumption

3.2.2 Head Tissue Simulating Liquid

Head Ingredients Frequency (450 MHz)		
Water		38.56%
Salt		3.95%
Sugar		56.32%
HEC (Hydroxyethyl Cellulose)		0.98%
Bactericide		0.19%


The dielectric parameters were verified prior to assessment using the HP 85046A dielectric probe kit and the HP 8753B network Analyzer. The dielectric parameters were:

Frequency (MHz)	Temp. ()	ϵ_r / Relative Permittivity			σ / Conductivity (mho/m)			ρ *(kg/m ³)
		measured	target	($\pm 5\%$)	measured	target	($\pm 5\%$)	
450	23	44.238	43.5	1.70%	0.889	0.87	2.18%	1000

* Worst-case assumption


3.2.3 Body Liquid results

Date: 8 Jan. 2007	Temperature: 23.0	Type: 450 MHz/ body (FCC)	Tested by: Kevin
410, 57.8258633921, -0.9343893523		450, 57.3706902832, -0.9680085988	
411, 57.9323058658, -0.9335154502		451, 57.3565134382, -0.9699671111	
412, 57.8376927694, -0.9344099206		452, 57.2932295319, -0.9692890836	
413, 57.8873937683, -0.9357126398		453, 57.327793038, -0.9705975306	
414, 57.8618402329, -0.9367120171		454, 57.2491484511, -0.9755678907	
415, 57.8969366971, -0.9366993545		455, 57.317380345, -0.9730055428	
416, 57.8471116591, -0.9382168063		456, 57.177034431, -0.9737782332	
417, 57.8328170858, -0.936698843		457, 57.2359027131, -0.9749554013	
418, 57.8471012399, -0.939439524		458, 57.2078559771, -0.9749637394	
419, 57.7669019729, -0.941618338		459, 57.19371937, -0.9778964705	
420, 57.7853822475, -0.9410353437		460, 57.1916346589, -0.9784264168	
421, 57.8123674026, -0.943380196		461, 57.1579134088, -0.9790019782	
422, 57.7819320359, -0.941712636		462, 57.2371628105, -0.9789561193	
423, 57.8123570665, -0.9452529604		463, 57.0865610962, -0.9791116532	
424, 57.8074398695, -0.9426087611		464, 57.1566825729, -0.9831042151	
425, 57.7861340841, -0.944682663		465, 56.992441771, -0.9840483334	
426, 57.6291867398, -0.9467903967		466, 57.104286616, -0.984266917	
427, 57.6906233717, -0.9470179599		467, 57.0677367043, -0.9822545056	
428, 57.6885205485, -0.946124973		468, 57.0998668902, -0.9838396183	
429, 57.7261292233, -0.9495004201		469, 57.0458762966, -0.9863411462	
430, 57.5814556498, -0.9508946805		470, 57.0109941579, -0.9872657377	
431, 57.696559445, -0.9503672952		471, 56.9948287357, -0.9874745143	
432, 57.668286978, -0.9540938903		472, 56.9319438917, -0.988965965	
433, 57.5883356192, -0.9503634816		473, 56.9501570539, -0.9913060145	
434, 57.536819018, -0.952277806		474, 56.7885795753, -0.9901823218	
435, 57.56991113867, -0.9536042542		475, 56.9269794268, -0.9894921325	
436, 57.66397110337, -0.9546220952		476, 56.8662422184, -0.994446914	
437, 57.5434518006, -0.9575988968		477, 56.8844343618, -0.9922565753	
438, 57.5343630673, -0.9582576287		478, 56.7959062542, -0.9933965859	
439, 57.5301688122, -0.9576506659		479, 56.9513936641, -0.9940101435	
440, 57.3859863559, -0.9613263883		480, 56.7785485499, -0.9930139867	
441, 57.488825529, -0.9604703073		481, 56.768889513, -0.9971308615	
442, 57.5522102279, -0.9634052312		482, 56.7778564105, -0.996647456	
443, 57.4442572403, -0.9606245023		483, 56.747965663, -0.9991196689	
444, 57.3780866089, -0.9649194342		484, 56.7853648707, -0.9976823952	
445, 57.3590296523, -0.961324244		485, 56.7107716605, -0.999460246	
446, 57.4002611178, -0.9620423663		486, 56.6431577433, -1.0006955736	
447, 57.4433043403, -0.9682989742		487, 56.6243448783, -1.0016847471	
448, 57.4763429239, -0.9679117152		488, 56.6847102804, -1.0032863083	
449, 57.3544331237, -0.9664014382		489, 56.6987108631, -1.0050205245	
		490, 56.7662867229, -1.0045396124	

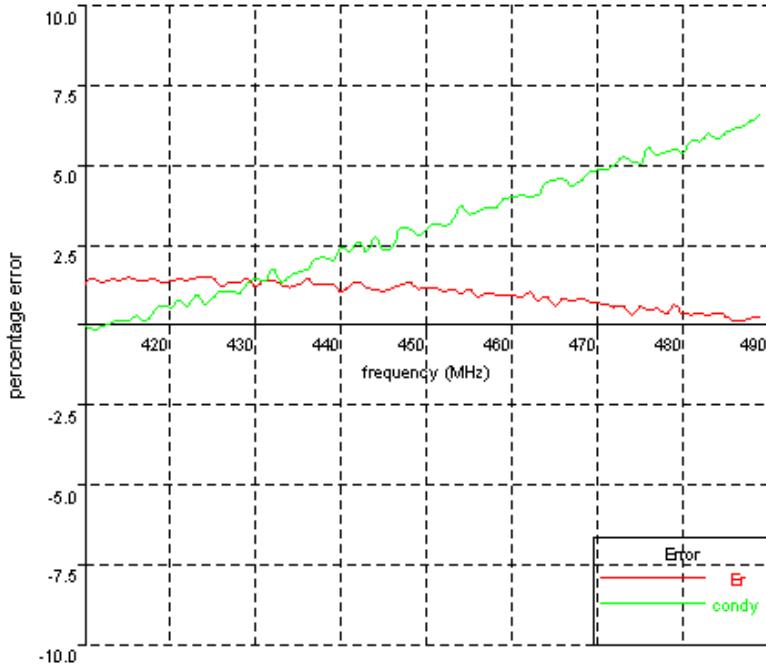

3.2.4 Head Liquid results

Date: 8 Jan. 2007	Temperature: 23.0	Type: 450 MHz/ head	Tested by: Kevin
410, 45.1101910826, -0.8523135212 411, 45.1822466688, -0.8537192943 412, 45.0712695497, -0.8520678419 413, 45.1432629657, -0.8549114965 414, 45.0046145597, -0.8565303416 415, 45.0432878572, -0.8578603607 416, 45.077064851, -0.8577723386 417, 45.0328008734, -0.8592735302 418, 45.0472073673, -0.8581636842 419, 44.9627105148, -0.8592362718 420, 44.9147383662, -0.8613916014 421, 44.913101224, -0.8624898605 422, 44.9185581658, -0.8621275889 423, 44.8508330027, -0.8646570892 424, 44.8839194312, -0.8664238611 425, 44.88555545, -0.8660138478 426, 44.8950052118, -0.8650980649 427, 44.811773863, -0.8688748462 428, 44.7903596393, -0.8685442881 429, 44.7211975589, -0.8705418648 430, 44.7507346567, -0.871714268 431, 44.715482638, -0.87194715 432, 44.6748303969, -0.8746574831 433, 44.7115905673, -0.8715588885 434, 44.6824308522, -0.8724242034 435, 44.6472326393, -0.8745087642 436, 44.676339353, -0.8757967358 437, 44.5835675539, -0.8768912582 438, 44.579775524, -0.8779921519 439, 44.5924116967, -0.8793034901 440, 44.5157989368, -0.8793149472 441, 44.5338278354, -0.8805549481 442, 44.4540749063, -0.8830485642 443, 44.4906534306, -0.8807389738 444, 44.4109778199, -0.8806314935 445, 44.4419298755, -0.8837742131 446, 44.5019264809, -0.8856526027 447, 44.3472798849, -0.88734356 448, 44.3293192365, -0.8889684905 449, 44.3277034328, -0.8878135439	450, 44.2389907067, -0.8892429694 451, 44.3128849953, -0.8918765166 452, 44.2616657879, -0.8913613764 453, 44.2133134572, -0.8915553419 454, 44.0612758405, -0.8950268253 455, 44.2067827415, -0.8960085533 456, 44.0920734995, -0.8930590904 457, 44.1099307892, -0.8950501767 458, 44.0079368506, -0.8967216782 459, 44.0921582929, -0.8984247659 460, 44.0000045095, -0.896439303 461, 43.9843216522, -0.8988611296 462, 44.1047354056, -0.9019503102 463, 43.9423918607, -0.9018224488 464, 43.9623246052, -0.9017242875 465, 43.8798627108, -0.9023380601 466, 43.8121065548, -0.9039452868 467, 43.8749839544, -0.9042188362 468, 43.8404218011, -0.9061550649 469, 43.8173419763, -0.90745658 470, 43.8350879998, -0.9080534351 471, 43.8613665912, -0.9096500751 472, 43.8436027377, -0.9104945507 473, 43.7105392245, -0.9107120951 474, 43.7571376317, -0.909712916 475, 43.6819599288, -0.9120345951 476, 43.6851443436, -0.9152218653 477, 43.6711655836, -0.9143611046 478, 43.5761863676, -0.9147482259 479, 43.6334237229, -0.9170665599 480, 43.602925984, -0.9165297226 481, 43.5333018806, -0.9168612193 482, 43.5401781585, -0.9169286529 483, 43.5042940141, -0.9187193565 484, 43.4798062473, -0.9193451167 485, 43.4658931932, -0.9214273258 486, 43.4375458888, -0.922226331 487, 43.3873384453, -0.9203714907 488, 43.3188164828, -0.9235950629 489, 43.3295158172, -0.9254539417 490, 43.3597141522, -0.92664975		

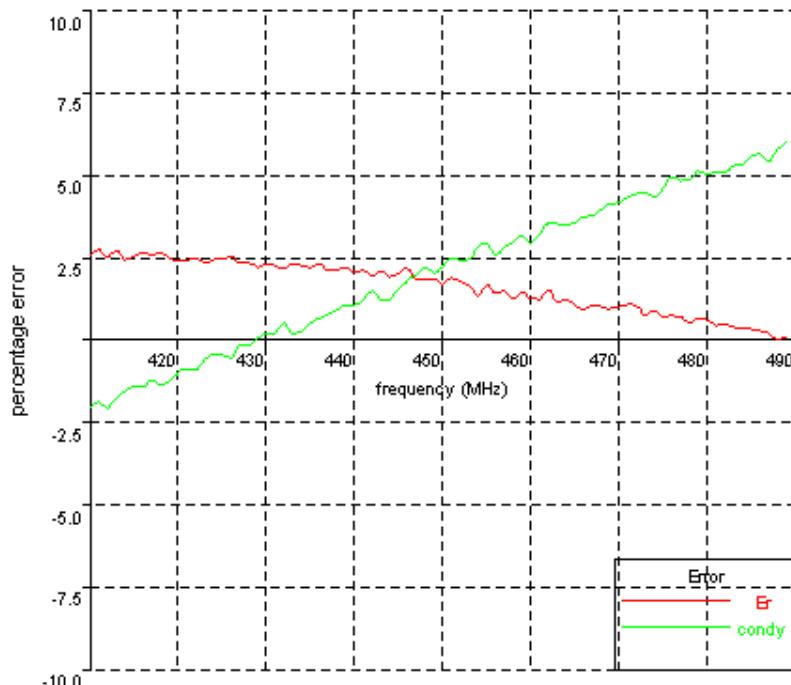

3.3 E-Field Probe and 450 Balanced Dipole Antenna Calibration

Probe calibration factors and dipole antenna calibration are included in Appendix C.

4.0 Measurement Uncertainty

The uncertainty budget has been determined for the INDEXSAR SARA2 measurement system according to IEEE P1528 documents [3] and is given in the following table. The extended uncertainty (95% confidence level) was assessed to be 20.6 % for SAR measurement, and the extended uncertainty (95% confidence level) was assessed to be 20.2 % for system performance check.

Table 1 Exposure Assessment Uncertainty

Example of measurement uncertainty assessment SAR measurement

a	b	c	d	e	f	g	h	i	
Uncertainty Component	Sec.	Tol. (+/-)	Prob. Dist.	Divisor (descrip)	Divisor (value)	c1 (1g)	c1 (10g)	Standard Uncertainty (%) 1g	Standard Uncertainty (%) 10g
		(dB)	(%)						
Measurement System									
Probe Calibration	E2.1		2.5	N	1 or k	1	1	2.50	2.50
Axial Isotropy	E2.2	0.25	5.93	5.93	R	$\sqrt{3}$	1.73	0	0.00
Hemispherical Isotropy	E2.2	0.45	10.92	10.92	R	$\sqrt{3}$	1.73	1	6.30
Boundary effect	E2.3		4	4.00	R	$\sqrt{3}$	1.73	1	2.31
Linearity	E2.4	0.04	0.93	0.93	R	$\sqrt{3}$	1.73	1	0.53
System Detection Limits	E2.5		1	1.00	R	$\sqrt{3}$	1.73	1	0.58
Readout Electronics	E2.6		1	1.00	N	1 or k	1.00	1	1.00
Response time	E2.7		0	0.00	R	$\sqrt{3}$	1.73	1	0.00
Integration time	E2.8		1.4	1.40	R	$\sqrt{3}$	1.73	1	0.81
RF Ambient Conditions	E6.1		3	3.00	R	$\sqrt{3}$	1.73	1	1.73
Probe Positioner Mechanical Tolerance	E6.2		0.6	0.60	R	$\sqrt{3}$	1.73	1	0.35
Probe Position wrt. Phantom Shell	E6.3		3	3.00	R	$\sqrt{3}$	1.73	1	1.73
SAR Evaluation Algorithms	E5		8	8.00	R	$\sqrt{3}$	1.73	1	4.62
Test Sample Related									
Test Sample Positioning	E4.2		2	2.00	N	1	1.00	1	2.00
Device Holder Uncertainty	E4.1		2	2.00	N	1	1.00	1	2.00
Output Power Variation	6.6.2		5	5.00	R	$\sqrt{3}$	1.73	1	2.89
Phantom and Tissue Parameters									
Phantom Uncertainty (shape and thickness)	E3.1		4	4.00	R	$\sqrt{3}$	1.73	1	2.31
Liquid conductivity (Deviation from target)	E3.2		5	5.00	R	$\sqrt{3}$	1.73	0.64	0.43
Liquid conductivity (measurement uncert.)	E3.3		1.1	1.10	N	1	1.00	0.64	0.43
Liquid permittivity (Deviation from target)	E3.2		5	5.00	R	$\sqrt{3}$	1.73	0.6	0.49
Liquid permittivity (measurement uncert.)	E3.3		1.1	1.10	N	1	1.00	0.6	0.49
Combined standard uncertainty					RSS				10.5
Expanded uncertainty		(95% Confidence Level)			k=2				20.6
									20.3

Table 2 System Check (Verification)

Example of measurement uncertainty assessment for system performance check

a	b	c	d	e	f	g	h	i	
Uncertainty Component	Sec.	Tol. (+/-)	Prob. Dist.	Divisor (descrip)	Divisor (value)	c1 (1g)	c1 (10g)	Standard Uncertainty (%) 1g	Standard Uncertainty (%) 10g
		(dB)	(%)						
Measurement System									
Probe Calibration	E2.1		2.5	N	1 or k	1	1	2.50	2.50
Axial Isotropy	E2.2	0.25	5.93	5.93	R	$\sqrt{3}$	1.73	0	0.00
Hemispherical Isotropy	E2.2	0.45	10.92	10.92	R	$\sqrt{3}$	1.73	1	6.30
Boundary effect	E2.3		4	4.00	R	$\sqrt{3}$	1.73	1	2.31
Linearity	E2.4	0.04	0.93	0.93	R	$\sqrt{3}$	1.73	1	0.53
System Detection Limits	E2.5		1	1.00	R	$\sqrt{3}$	1.73	1	0.58
Readout Electronics	E2.6		1	1.00	N	1 or k	1.00	1	1.00
Response time	E2.7		0	0.00	R	$\sqrt{3}$	1.73	1	0.00
Integration time	E2.8		1.4	1.40	R	$\sqrt{3}$	1.73	1	0.81
RF Ambient Conditions	E6.1		3	3.00	R	$\sqrt{3}$	1.73	1	1.73
Probe Positioner Mechanical Tolerance	E6.2		0.6	0.60	R	$\sqrt{3}$	1.73	1	0.35
Probe Position wrt. Phantom Shell	E6.3		3	3.00	R	$\sqrt{3}$	1.73	1	1.73
SAR Evaluation Algorithms	E5		8	8.00	R	$\sqrt{3}$	1.73	1	4.62
Dipole									
Dipole axis to liquid distance	8, E4.2		2	2.00	N	1	1.00	1	2.00
Input power and SAR drift measurement	8, 6.6.2		5	5.00	R	$\sqrt{3}$	1.73	1	2.89
Phantom and Tissue Parameters									
Phantom Uncertainty (thickness)	E3.1		4	4.00	R	$\sqrt{3}$	1.73	1	2.31
Liquid conductivity (Deviation from target)	E3.2		5	5.00	R	$\sqrt{3}$	1.73	0.64	1.85
Liquid conductivity (measurement uncert.)	E3.3		1.1	1.10	N	1	1.00	0.64	0.43
Liquid permittivity (Deviation from target)	E3.2		5	5.00	R	$\sqrt{3}$	1.73	0.6	0.49
Liquid permittivity (measurement uncert.)	E3.3		1.1	1.10	N	1	1.00	0.6	0.49
Combined standard uncertainty					RSS				10.3
Expanded uncertainty	(95% Confidence Level)				k=2				20.2
									19.9

5.0 Warning Label Information - USA

See user manual.

6.0 References

- [1] ANSI, *ANSI/IEEE C95.1-1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3kHz to 300 GHz*, The Institute of electrical and Electronics Engineers, Inc., New York, NY 10017, 1999
- [2] Federal Communications Commission, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Supplement C to OET Bulletin 65, Washington, D.C. 20554, 1997
- [3] IEEE Standards Coordinating Committee 34, "IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", IEEE Std 1528TM-2003
- [4] Industry Canada, "Evaluation Procedure for Mobile and Portable Radio Transmitters with respect to Health Canada's Safety Code 6 for Exposure of Humans to Radio Frequency Fields", Radio Standards Specification RSS-102 Issue 1 (Provisional): September 1999.

7.0 Document History

Revision/ Job Number	Writer Initials	Date	Change
N/A	S.L.	Jan. 25, 2007	Original document
	S.L.	Feb. 12, 2007	Update

APPENDIX A - SAR Evaluation Data


Power drift is the measurement of power drift of the device over one complete SAR scan.

To assess the drift of the power of the device under test, a SAR measurement was made in the middle of the zoom scan volume at the start of the scan and a measurement at this point was then also made after the measurement scan. The difference between the two measurements should be less than 5%.

Plot #1(1/2)

Date / Time:	2007/1/9	Position:	Rear side 0mm to phantom
Filename:	ch4_body0mm.txt	Phantom:	HeadBox6-450_BL-test.csv
Device Tested:	99152	Head Rotation:	0
Antenna:	Helix	Test Frequency:	Ch4_462.6375MHz
Shape File:	99152-R.csv	Power Level:	20.56 dBm


Probe:	0136	Liquid:	15.5cm																
Cal File:	SN0136_450_CW_BODY	Type:	450 MHz Body																
Cal Factors:	<table border="1"> <tr> <th></th> <th>X</th> <th>Y</th> <th>Z</th> </tr> <tr> <td>Air</td> <td>490</td> <td>377</td> <td>387</td> </tr> <tr> <td>DCP</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Lin</td> <td>.298</td> <td>.298</td> <td>.298</td> </tr> </table>		X	Y	Z	Air	490	377	387	DCP	20	20	20	Lin	.298	.298	.298	Conductivity:	0.968
	X	Y	Z																
Air	490	377	387																
DCP	20	20	20																
Lin	.298	.298	.298																
Amp Gain:	2	Relative Permittivity:	57.371																
Averaging:	1	Liquid Temp (deg C):	23																
Batteries	-	Ambient Temp (deg C):	23																
Replaced:	-	Ambient RH (%):	50																
		Density (kg/m3):	1000																
		Software Version:	2.41VPM																

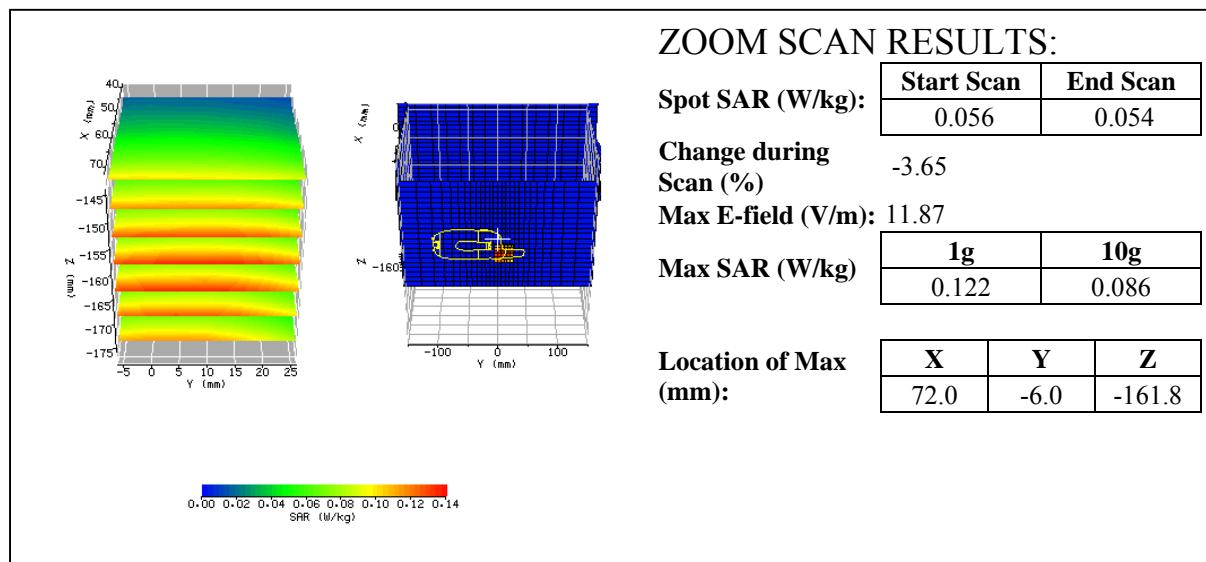

Plot #1(2/2)

AREA SCAN:


	Min	Max	Steps
Scan Extent:			
Y	-50.0	50.0	10.0
Z	-185.0	-125.0	6.0

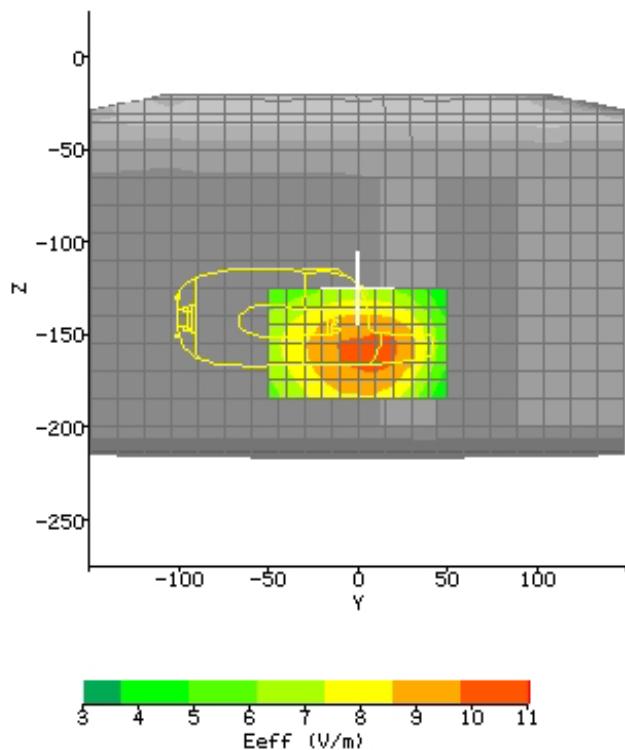

Plot #2(1/2)

Date:	2007/1/9	Position:	Rear side 0mm to phantom
Filename:	ch11_body0mm.txt	Phantom:	HeadBox6-450_BL-test.csv
Device Tested:	99152	Head Rotation:	0
Antenna:	Helix	Test Frequency:	Ch4_467.6375MHz
Shape File:	99152-R.csv	Power Level:	20.24 dBm

Probe:	0136	Liquid:	15.5cm																
Cal File:	SN0136_450_CW_BODY	Type:	450 MHz Body																
Cal Factors:	<table border="1"> <tr> <th></th> <th>X</th> <th>Y</th> <th>Z</th> </tr> <tr> <td>Air</td> <td>490</td> <td>377</td> <td>387</td> </tr> <tr> <td>DCP</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Lin</td> <td>.298</td> <td>.298</td> <td>.298</td> </tr> </table>		X	Y	Z	Air	490	377	387	DCP	20	20	20	Lin	.298	.298	.298	Conductivity:	0.968
	X	Y	Z																
Air	490	377	387																
DCP	20	20	20																
Lin	.298	.298	.298																
Amp Gain:	2	Relative Permittivity:	57.371																
Averaging:	1	Liquid Temp (deg C):	23																
Batteries	-	Ambient Temp (deg C):	23																
Replaced:	-	Ambient RH (%):	50																
		Density (kg/m3):	1000																
		Software Version:	2.41VPM																

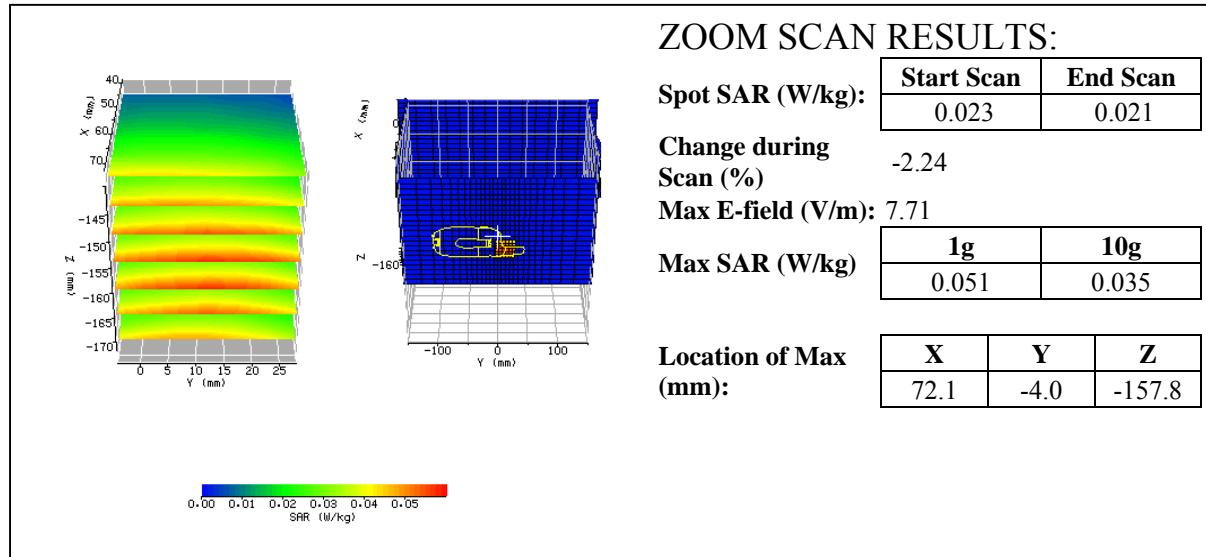


Plot #2(2/2)

AREA SCAN:

Scan Extent:


	Min	Max	Steps
Y	-50.0	50.0	10.0
Z	-185.0	-125.0	6.0

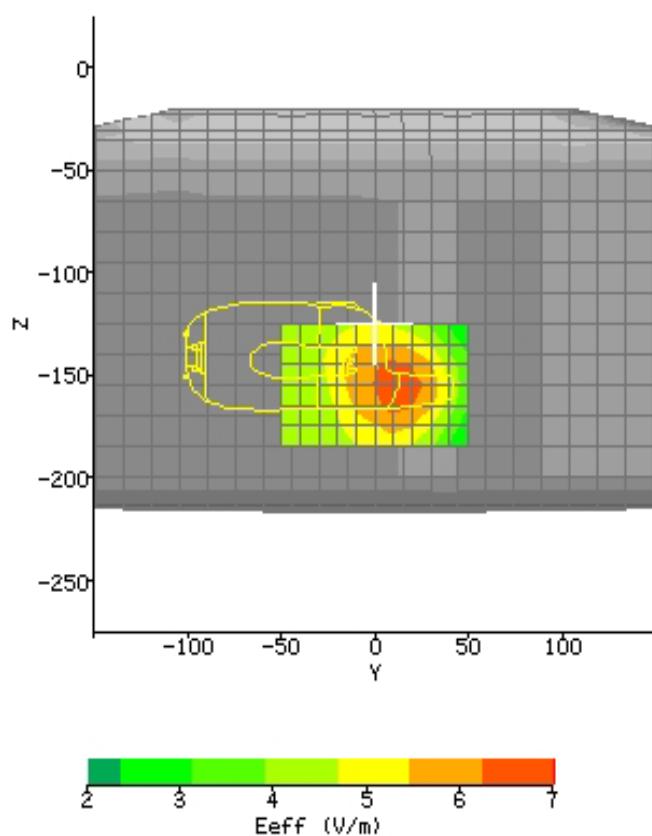

Plot #3(1/2)


Date:	2007/1/9	Position:	Front side 25mm to phantom
Filename:	ch4_head25mm.txt	Phantom:	HeadBox4-450_HL-test.csv
Device Tested:	99152	Head Rotation:	0
Antenna:	Helix	Test Frequency:	Ch4_462.6375MHz
Shape File:	99152-F.csv	Power Level:	20.56 dBm

Probe:	0136	Liquid:	15.5cm															
Cal File:	SN0136_450_CW_HEAD	Type:	450 MHz Head															
Cal Factors:	<table border="1"> <thead> <tr> <th></th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>Air</td> <td>490</td> <td>377</td> <td>387</td> </tr> <tr> <td>DCP</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Lin</td> <td>.299</td> <td>.299</td> <td>.299</td> </tr> </tbody> </table>		X	Y	Z	Air	490	377	387	DCP	20	20	20	Lin	.299	.299	.299	
	X	Y	Z															
Air	490	377	387															
DCP	20	20	20															
Lin	.299	.299	.299															
Amp Gain:	2	Conductivity:	0.889															
Averaging:	1	Relative Permittivity:	44.239															
Batteries	-	Liquid Temp (deg C):	23															
Replaced:	-	Ambient Temp (deg C):	23															
		Ambient RH (%):	50															
		Density (kg/m³):	1000															
		Software Version:	2.41VPM															

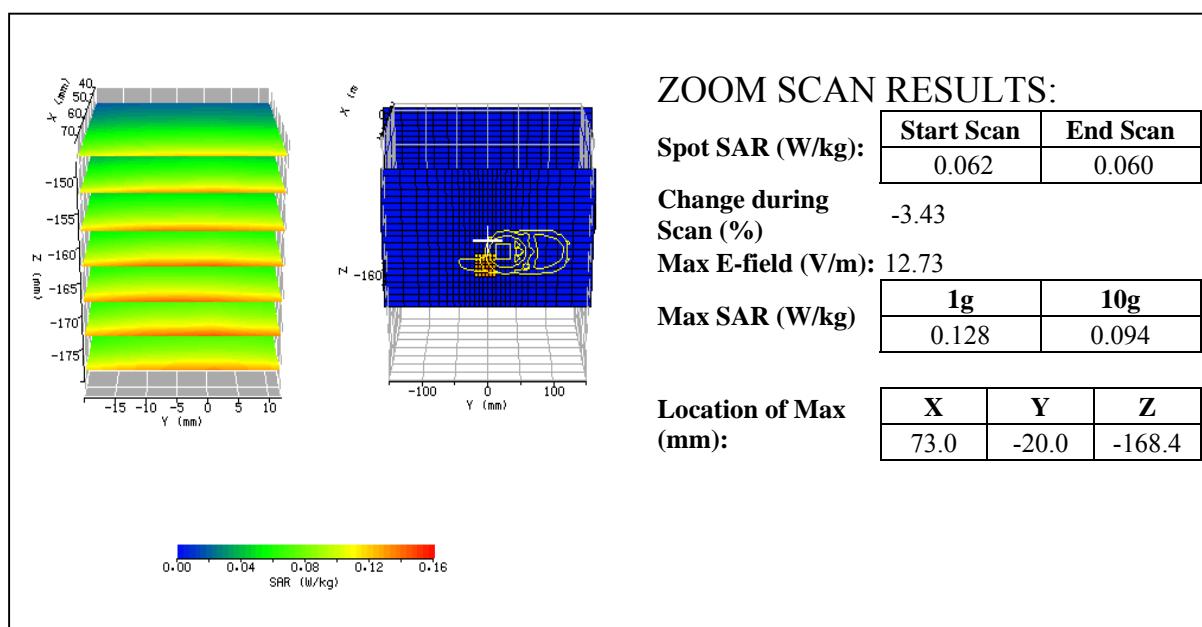

AREA SCAN:

	Min	Max	Steps
Y	-50.0	50.0	10.0
Z	-195.0	-125.0	7.0

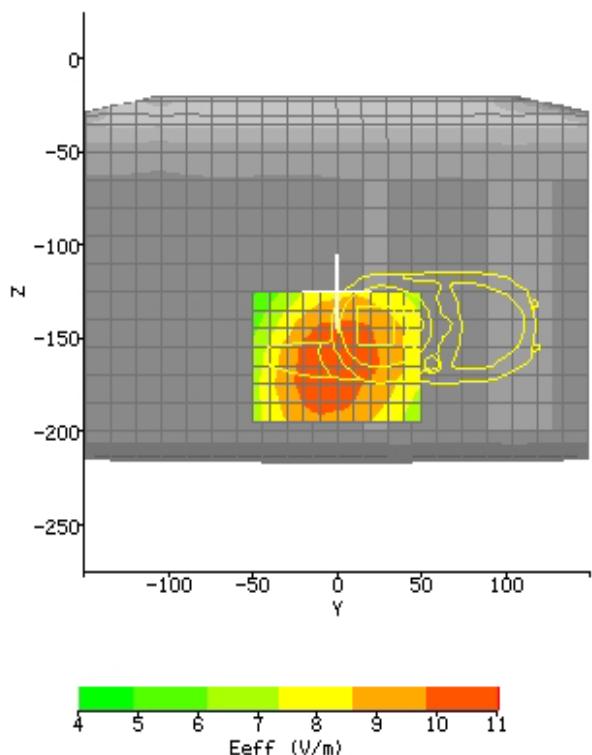


FCC ID. : PEG99152

Report No.: EME-070003
Page 38 of 67

Plot #4(1/2)

Date:	2007/1/9	Position:	Front side 25mm to phantom
Filename:	ch11_head25mm.txt	Phantom:	HeadBox4-450_HL-test.csv
Device Tested:	99152	Head Rotation:	0
Antenna:	Helix	Test Frequency:	Ch11_467.6375MHz
Shape File:	99152-F.csv	Power Level:	20.24 dBm


Probe:	0136	Liquid:	15.5cm															
Cal File:	SN0136_450_CW_HEAD	Type:	450 MHz Head															
Cal Factors:	<table border="1"> <thead> <tr> <th></th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>Air</td> <td>490</td> <td>377</td> <td>387</td> </tr> <tr> <td>DCP</td> <td>20</td> <td>20</td> <td>20</td> </tr> <tr> <td>Lin</td> <td>.299</td> <td>.299</td> <td>.299</td> </tr> </tbody> </table>		X	Y	Z	Air	490	377	387	DCP	20	20	20	Lin	.299	.299	.299	
	X	Y	Z															
Air	490	377	387															
DCP	20	20	20															
Lin	.299	.299	.299															
Amp Gain:	2	Conductivity:	0.889															
Averaging:	1	Relative Permittivity:	44.239															
Batteries Replaced:	-	Liquid Temp (deg C):	23															
		Ambient Temp (deg C):	23															
		Ambient RH (%):	50															
		Density (kg/m3):	1000															
		Software Version:	2.41VPM															

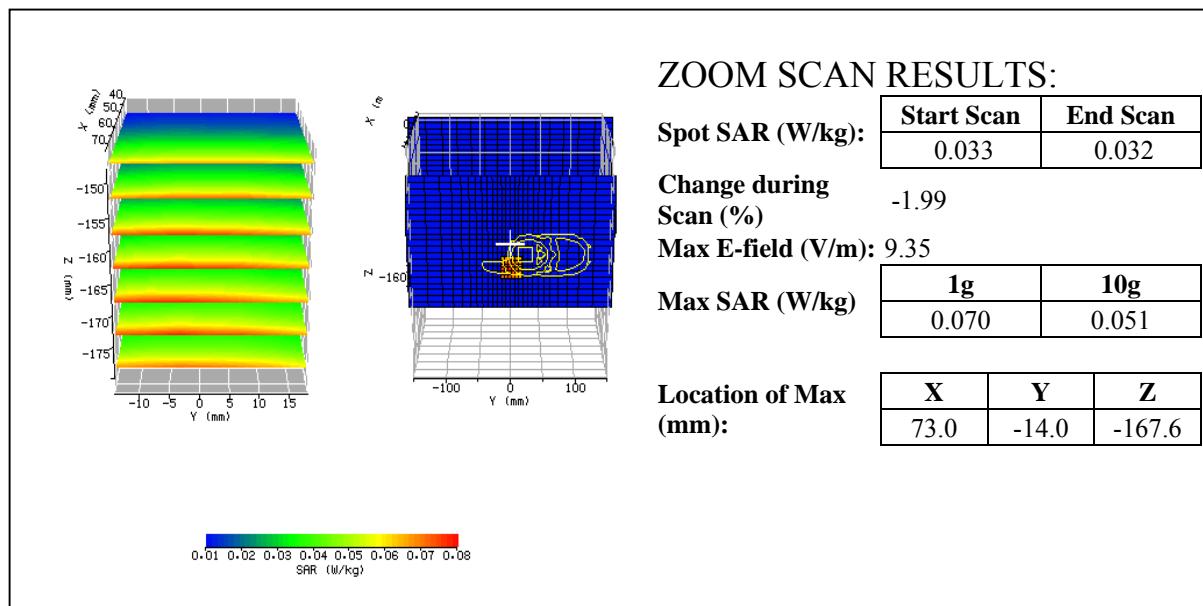

Plot #4(2/2)

AREA SCAN:

	Min	Max	Steps
Scan Extent:			
Y	-50.0	50.0	10.0
Z	-195.0	-125.0	7.0

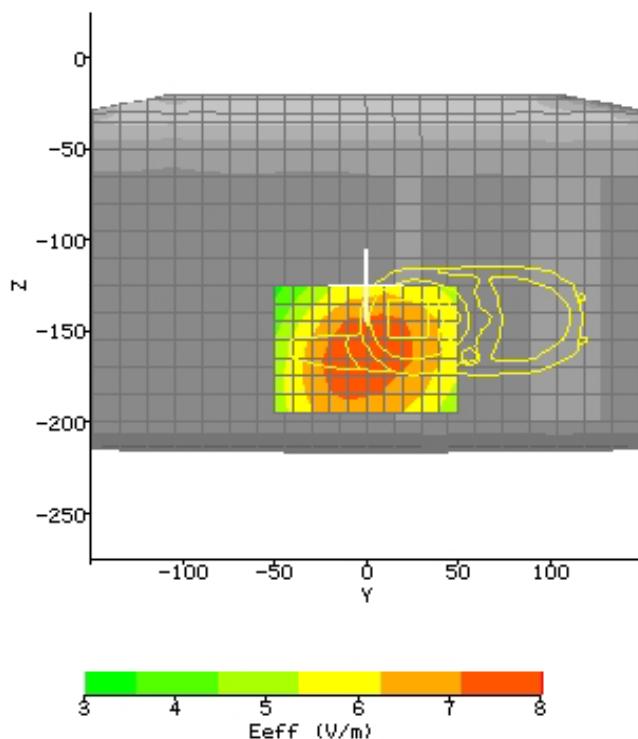

APPENDIX B - Photographs



(Belt-clip)



(Belt-clip)



(Battery)



APPENDIX C - E-Field Probe and 450MHz Balanced Dipole Antenna Calibration Data

**IndexSAR Limited***Oakfield House**Cudworth Lane***Newdigate***Surrey RH5 5BG***Tel: +44 (0) 1306 632 870****Fax: +44 (0) 1306 631 834****e-mail: enquiries@indexsar.com****Calibration Certificate 0603/0136**
Dosimetric E-field Probe**Type:** **IXP-050****Manufacturer:** **IndexSAR, UK****Serial Number:** **0136****Place of Calibration:** **IndexSAR, UK**

IndexSAR Limited hereby declares that the IXP-050 Probe named above has been calibrated for conformity to the IEEE 1528 and CENELEC EN 50361 standards on the date shown below.

Date of Initial Calibration: **8th March 2006**

The probe named above will require a calibration check on the date shown below.

Next Calibration Date: **March 2007**

The calibration was carried out using the methods described in the calibration document. Where applicable, the standards used in the calibration process are traceable to the UK's National Physical Laboratory.

Calibrated By:*A. Brinklow***Approved By:***M.J. Main*

Please keep this certificate with the calibration document. When the probe is sent for a calibration check, please include the calibration document.




IMMERSIBLE SAR PROBE

CALIBRATION REPORT

Part Number: IXP – 050

S/N 0136

March 2006

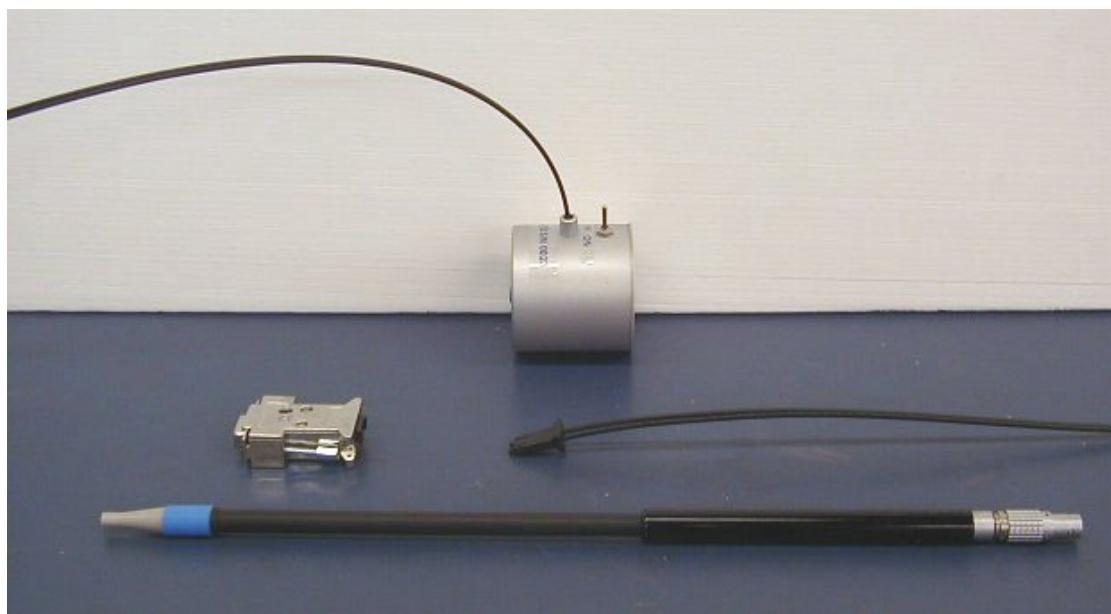

**Indexsar Limited
Oakfield House
Cudworth Lane
Newdigate
Surrey RH5 5BG**

Tel: +44 (0) 1306 632 870

Fax: +44 (0) 1306 631 834

e-mail: enquiries@indexsar.com

INTRODUCTION

This Report presents measured calibration data for a particular Indexsar SAR probe (S/N 0136) and describes the procedures used for characterisation and calibration.

Indexsar probes are characterised using procedures that, where applicable, follow the recommendations of CENELEC [1] and IEEE [2] standards. The procedures incorporate techniques for probe linearisation, isotropy assessment and determination of liquid factors (conversion factors). Calibrations are determined by comparing probe readings with analytical computations in canonical test geometries (waveguides) using normalised power inputs.

Each step of the calibration procedure and the equipment used is described in the sections below.

CALIBRATION PROCEDURE

1. Objectives

The calibration process comprises three stages

- 1) Determination of the channel sensitivity factors which optimise the probe's overall rotational isotropy in brain fluid across a range of frequencies
- 2) At each frequency of interest, application of these channel sensitivity factors to model the exponential decay of SAR in a waveguide fluid cell, and hence derive the liquid conversion factors at that frequency
- 3) Determination of the effective tip radius and angular offset of the X channel which together optimise the probe's spherical isotropy in 900MHz brain fluid

2. Probe output

The probe channel output signals are linearised in the manner set out in Refs [1] and [2]. The following equation is utilized for each channel:

$$U_{lin} = U_{o/p} + U_{o/p}^2 / DCP \quad (1)$$

where U_{lin} is the linearised signal, $U_{o/p}$ is the raw output signal in voltage units and DCP is the diode compression potential in similar voltage units.

DCP is determined from fitting equation (1) to measurements of U_{lin} versus source feed power over the full dynamic range of the probe. The DCP is a characteristic of the Schottky diodes used as the sensors. For the IXP-050 probes with CW signals the DCP values are typically 0.10V (or 20 in the voltage units used by Indexsar software, which are V*200).

In turn, measurements of E-field are determined using the following equation (where output voltages are also in units of V*200):

$$E_{liq}^2 (V/m) = U_{linx} * Air\ Factor_x * Liq\ Factor_x + U_{liny} * Air\ Factor_y * Liq\ Factor_y + U_{linz} * Air\ Factor_z * Liq\ Factor_z \quad (3)$$

Here, "Air Factor" represents each channel's sensitivity, while "Liq Factor" represents the

enhancement in signal level when the probe is immersed in tissue-simulant liquids at each frequency of interest.

3. Selecting channel sensitivity factors to optimise isotropic response

After manufacture, the first stage of the calibration process is to balance the three channels' Air Factor values, thereby optimising the probe's overall axial response ("rotational isotropy").

To do this, a 900MHz waveguide containing head-fluid simulant is selected. Like all waveguides used during probe calibration, this particular waveguide contains two distinct sections: an air-filled launcher section, and a liquid cell section, separated by a dielectric matching window designed to minimise reflections at the air-liquid interface.

The waveguide stands in an upright position and the liquid cell section is filled with 900MHz brain fluid to within 10 mm of the open end. The depth of liquid ensures there is negligible radiation from the waveguide open top and that the probe calibration is not influenced by reflections from nearby objects.

During the measurement, a TE_{01} mode is launched into the waveguide by means of an N-type-to-waveguide adapter. The probe is then lowered vertically into the liquid until the tip is exactly 10mm above the centre of the dielectric window. This particular separation ensures that the probe is operating in a part of the waveguide where boundary corrections are not necessary.

Care must also be taken that the probe tip is centred while rotating.

The exact power applied to the input of the waveguide during this stage of the probe calibration is immaterial since only relative values are of interest while the probe rotates. However, the power must be sufficiently above the noise floor and free from drift.

The dedicated Indexsar calibration software rotates the probe in 10 degree steps about its axis, and at each position, an Indexsar 'Fast' amplifier samples the probe channels 500 times per second for 0.4 s. The raw $U_{o/p}$ data from each sample are packed into 10 bytes and transmitted back to the PC controller via an optical cable. U_{linx} , U_{liny} and U_{linz} are derived from the raw $U_{o/p}$ values and written to an Excel template.

Once data have been collected from a full probe rotation, the Air Factors are adjusted using a special Excel Solver routine to equalise the output from each channel and hence minimise the rotational isotropy. This automated approach to optimisation removes the effect of human bias.

Figure 5 represents the output from each diode sensor as a function of probe rotation angle. The directionality of the orthogonally-arranged sensors can be checked by analysing the data using dedicated Indexsar software, which displays the data in 3D format, a representative image of which is shown in Figure 3. The left-hand side of this diagram shows the individual channel outputs after linearisation (see above). The program uses these data to balance the channel outputs and then applies an optimisation process, which makes fine adjustments to the channel factors for optimum isotropic response.

4. Determination of Conversion ("Liquid") Factors at each frequency of interest

A lookup table of conversion factors for a probe allows a SAR value to be derived at the measured frequencies, and for either brain or body fluid-simulant.

The method by which the conversion factors are assessed is based on the comparison between measured and analytical rates of decay of SAR with height above a dielectric window. This way, not only can the conversion factors for that frequency/fluid combination be determined, but an allowance can also be made for the scale and range of boundary layer effects.

The theoretical relationship between the SAR at the cross-sectional centre of the lossy waveguide as a function of the longitudinal distance (z) from the dielectric separator is given by Equation 4:

$$SAR(z) = \frac{4(P_f - P_b)}{\rho ab\delta} e^{-2z/\delta} \quad (4)$$

Here, the density ρ is conventionally assumed to be 1000 kg/m^3 , ab is the cross-sectional area of the waveguide, and P_f and P_b are the forward and reflected power inside the lossless section of the waveguide, respectively. The penetration depth δ (which is the reciprocal of the waveguide-mode attenuation coefficient) is a property of the lossy liquid and is given by Equation (5).

$$\delta = \left[\text{Re} \left\{ \sqrt{(\pi/a)^2 + j\omega\mu_o(\sigma + j\omega\epsilon_o\epsilon_r)} \right\} \right]^{-1} \quad (5)$$

where σ is the conductivity of the tissue-simulant liquid in S/m , ϵ_r is its relative permittivity, and ω is the radial frequency (rad/s). Values for σ and ϵ_r are obtained prior to each waveguide test using an Indexsar DiLine measurement kit, which uses the TEM method as recommended in [2]. σ and ϵ_r are both temperature- and fluid-dependent, so are best measured using a sample of the tissue-simulant fluid immediately prior to the actual calibration.

Wherever possible, all DiLine and calibration measurements should be made in the open laboratory at $22 \pm 2.0^\circ\text{C}$; if this is not possible, the values of σ and ϵ_r should reflect the actual temperature. Values employed for calibration are listed in the tables below.

By ensuring the liquid height in the waveguide is at least three penetration depths, reflections at the upper surface of the liquid are negligible. The power absorbed in the liquid is therefore determined solely from the waveguide forward and reflected power.

Different waveguides are used for 835/900MHz, 1800/1900MHz, 2450MHz and 5200/5800MHz measurements. Table A.1 of [1] can be used for designing calibration waveguides with a return loss greater than 20 dB at the most important frequencies used for personal wireless communications, and better than 15dB for frequencies greater than 5GHz. Values for the penetration depth for these specific fixtures and tissue-simulating mixtures are also listed in Table A.1.

According to [1], this calibration technique provides excellent accuracy, with standard uncertainty of less than 3.6% depending on the frequency and medium. The calibration itself is reduced to power measurements traceable to a standard calibration procedure. The practical limitation to the frequency band of 800 to 5800 MHz because of the

waveguide size is not severe in the context of compliance testing.

During calibration, the probe is lowered carefully until it is just touching the cross-sectional centre of the dielectric window. 200 samples are then taken and written to an Excel template file before moving the probe vertically upwards. This cycle is repeated 50 times. The vertical separation between readings is determined from practical considerations of the expected SAR decay rate, and range from 1mm steps at low frequency, through 0.5mm at 2450MHz, down to 0.2mm at 5GHz.

Once the data collection is complete, a Solver routine is run which optimises the measured-theoretical fit by varying the conversion factor, and the boundary correction size and range.

For 450 MHz calibrations, the response of the probe-under-test is compared with the equivalent response of a probe whose 450MHz characteristics have been determined by NPL. The conversion factor of the probe-under-test can then be deduced.

5. Measurement of Spherical Isotropy

The setup for measuring the probe's spherical isotropy is shown in Figure 2.

A box phantom containing 900MHz head fluid is irradiated by a vertically-polarised, tuned dipole, mounted to the side of the phantom on the robot's seventh axis. During calibration, the spherical response is generated by rotating the probe about its axis in 20 degree steps and changing the dipole polarisation in 10 degree steps.

By using the VPM technique discussed below, an allowance can also be made for the effect of E-field gradient across the probe's spatial extent. This permits values for the probe's effective tip radius and X-channel angular offset to be modelled until the overall spherical isotropy figure is optimised.

The dipole is connected to a signal generator and amplifier via a directional coupler and power meter. As with the determination of rotational isotropy, the absolute power level is not important as long as it is stable.

The probe is positioned within the fluid so that its sensors are at the same vertical height as the centre of the source dipole. The line joining probe to dipole should be perpendicular to the phantom wall, while the horizontal separation between the two should be small enough for VPM corrections to be applicable, without encroaching near the boundary layer of the phantom wall. VPM corrections require a knowledge of the fluid skin depth. This is measured during the calibration by recording the E-field strength while systematically moving the probe away from the dipole in 2mm steps over a 20mm range.

VPM (Virtual Probe Miniaturisation)

SAR probes with 3 diode-sensors in an orthogonal arrangement are designed to display an isotropic response when exposed to a uniform field. However, the probes are ordinarily used for measurements in non-uniform fields and isotropy is not assured when the field gradients are significant compared to the dimensions of the tip containing the three orthogonally-arranged dipole sensors.

It becomes increasingly important to assess the effects of field gradients on SAR probe readings when higher frequencies are being used. For Indexsar IXP-050 probes, which are of 5mm tip diameter, field gradient effects are minor at GSM frequencies, but are major above 5GHz. Smaller probes are less affected by field gradients and so probes, which are

significantly less than 5mm diameter, would be better for applications above 5GHz.

The IndexSAR report IXS0223 describes theoretical and experimental studies to evaluate the issues associated with the use of probes at arbitrary angles to surfaces and field directions. Based upon these studies, the procedures and uncertainty analyses referred to in P1528 are addressed for the full range of probe presentation angles.

In addition, generalized procedures for correcting for the finite size of immersible SAR probes are developed. Use of these procedures enables application of schemes for virtual probe miniaturization (VPM) – allowing probes of a specific size to be used where physically-smaller probes would otherwise be required.


Given the typical dimensions of 3-channel SAR probes presently available, use of the VPM technique extends the satisfactory measurement range to higher frequencies.

CALIBRATION FACTORS MEASURED FOR PROBE S/N 0136

The probe was initially calibrated by the National Physical Laboratory (NPL) at 900, 1800 and 2450 MHz in liquid samples representing both brain liquid and body fluid at these frequencies. Additional calibrations were performed at Indexsar at 450, 835 and 1900 MHz. In both cases, the calibration was for CW signals only, and the axis of the probe was parallel to the direction of propagation of the incident field i.e. end-on to the incident radiation. The axial isotropy of the probe was measured by rotating the probe about its axis in 10 degree steps through 360 degrees in this orientation.

The reference point for the calibration is in the centre of the probe's cross-section at a distance of 2.7 mm from the probe tip in the direction of the probe amplifier. A value of 2.7 mm should be used for the tip to sensor offset distance in the software. The distance of 2.7mm for assembled probes has been confirmed by taking X-ray images of the probe tips (see Figure 8).

It is important that the diode compression point and air factors used in the software are the same as those quoted in the results tables, as these are used to convert the diode output voltages to a SAR value.

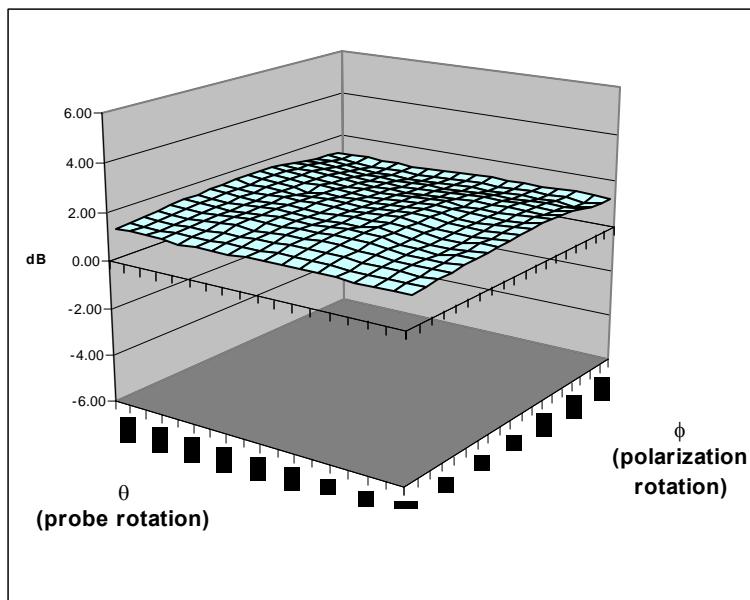

Surface Isotropy diagram of IXP-050 Probe S/N 0136 at 900MHz after VPM (rotational isotropy axial +/-0.05dB, spherical isotropy +/-0.24dB)[†]

Probe tip radius	1.25
X Ch. Angle to red dot	0

Frequency	Head		Body	
	Bdy. Corrn. – f(0)	Bdy. Corrn. – d(mm)	Bdy. Corrn. – f(0)	Bdy. Corrn. – d(mm)
	-	-	-	-
835	0.71	1.8	1.01	1.5
900	0	1	0	1
1800	0	1	0	1
1900	1.08	1.2	0.68	2.3
2450	0	1	0	1

[†] Based on previous measurements

SUMMARY OF CALIBRATION FACTORS FOR PROBE IXP-050 S/N 0136

Spherical isotropy measured at 900MHz [†]	0.24	(+/-) dB
--	------	----------

	X	Y	Z	
Air Factors	490	377	387	(V*200)
CW DCPs	20	20	20	(V*200)
DSSS [†]	20	20	20	(V*200)
GSM [‡]	8	9.5	11.2	(V*200)
CDMA [†]	20	20	20	(V*200)

Freq (MHz)	Axial Isotropy		SAR ConvF		Notes	
	(+/- dB)		(liq/air)			
	Head	Body	Head	Body		
450	-	-	0.299	0.298	1,3	
835	0.05	0.04	0.284	0.304	1,2,3	
900	0.05	0.04	0.281	0.299	1,2,4	
1800	0.06	0.06	0.344	0.369	1,2,4	
1900	0.06	0.06	0.320	0.399	1,2,3	
2450	0.05	0.10	0.356	0.435	1,2,4	

Notes	
1)	Calibrations done at 22°C +/-2°C
2)	Waveguide calibration
3)	Calibrated by Indexsar
4)	Calibrated by NPL

[†] Based on previous measurements

[‡] GSM factor not used with IXP-020 'fast' probe amplifier

PROBE SPECIFICATIONS

Indexsar probe 0136, along with its calibration, is compared with CENELEC and IEEE standards recommendations (Refs [1] and [2]) in the Tables below. A listing of relevant specifications is contained in the tables below:

Dimensions	S/N 0136	CENELEC [1]	IEEE [2]
Overall length (mm)	350		
Tip length (mm)	10		
Body diameter (mm)	12		
Tip diameter (mm)	5.2	8	8
Distance from probe tip to dipole centers (mm)	2.7		

Dynamic range	S/N 0136	CENELEC [1]	IEEE [2]
Minimum (W/kg)	0.01	<0.02	0.01
Maximum (W/kg) N.B. only measured to > 100 W/kg on representative probes	>100	>100	100

Isotropy (measured at 900MHz)	S/N 0136	CENELEC [1]	IEEE [2]
Axial rotation with probe normal to source (+/- dB)	0.06 Max (See table above)	0.5	0.25
Spherical isotropy covering all orientations to source (+/- dB)	0.24	1.0	0.50

Construction	Each probe contains three orthogonal dipole sensors arranged on a triangular prism core, protected against static charges by built-in shielding, and covered at the tip by PEEK cylindrical enclosure material. No adhesives are used in the immersed section. Outer case materials are PEEK and heat-shrink sleeving.
Chemical resistance	Tested to be resistant to glycol and alcohol containing simulant liquids but probes should be removed, cleaned and dried when not in use.

REFERENCES

- [1] CENELEC, EN 50361, July 2001. Basic Standard for the measurement of specific absorption rate related to human exposure to electromagnetic fields from mobile phones.
- [2] IEEE 1528, Recommended practice for determining the spatial-peak specific absorption rate (SAR) in the human body due to wireless communications devices: Experimental techniques.

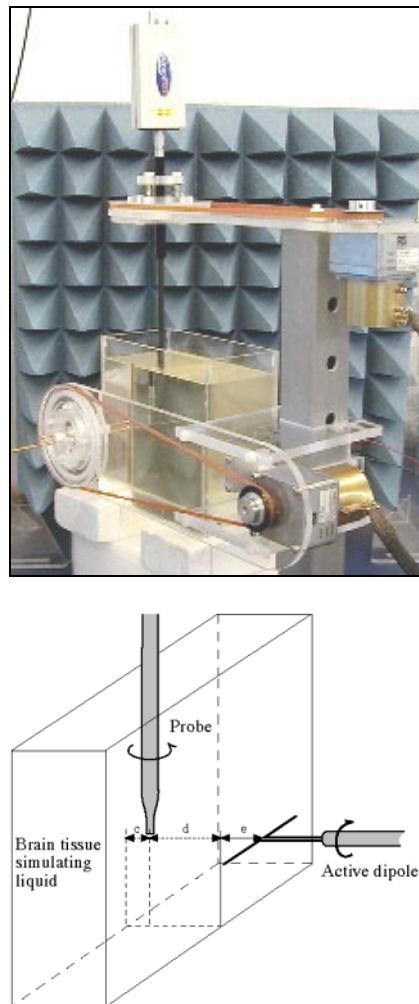


Figure 1. Spherical isotropy jig showing probe, dipole and box filled with simulated brain liquid (see Ref [2], Section A.5.2.1)

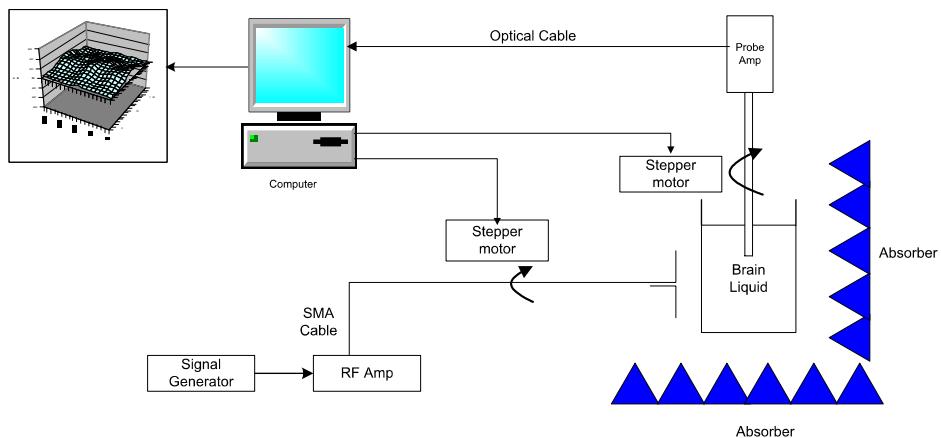


Figure 2. Schematic diagram of the test geometry used for isotropy determination

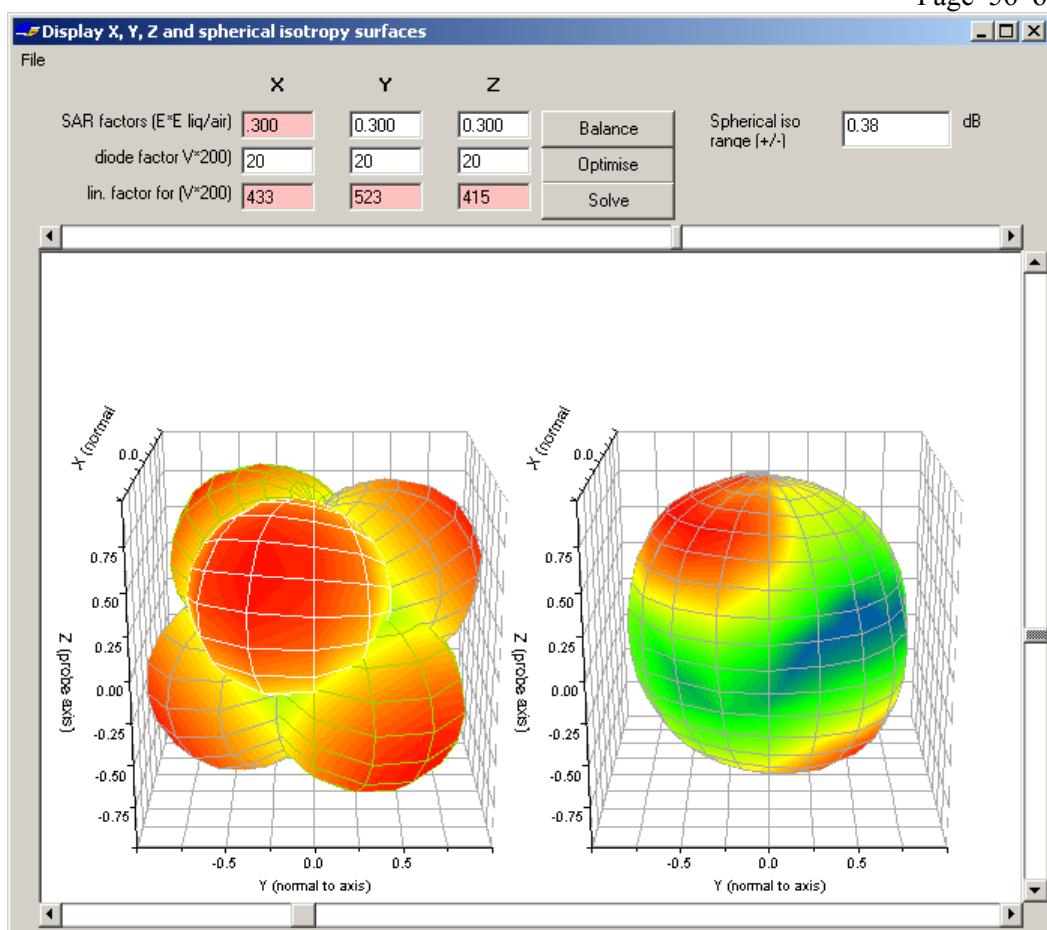


Figure 3. Typical graphical representation of a probe's response to fields applied from each direction. The diagram on the left shows the individual response characteristics of each of the three channels and the diagram on the right shows the resulting probe sensitivity in each direction. The colour range in the figure images the lowest values as blue and the maximum values as red. For the probe S/N 0136, this range is (+/-) 0.24dB.

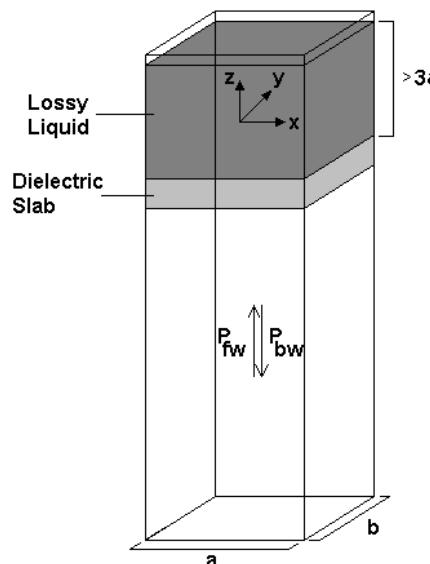


Figure 4. Geometry used for waveguide calibration (after Ref [2]. Section A.3.2.2)

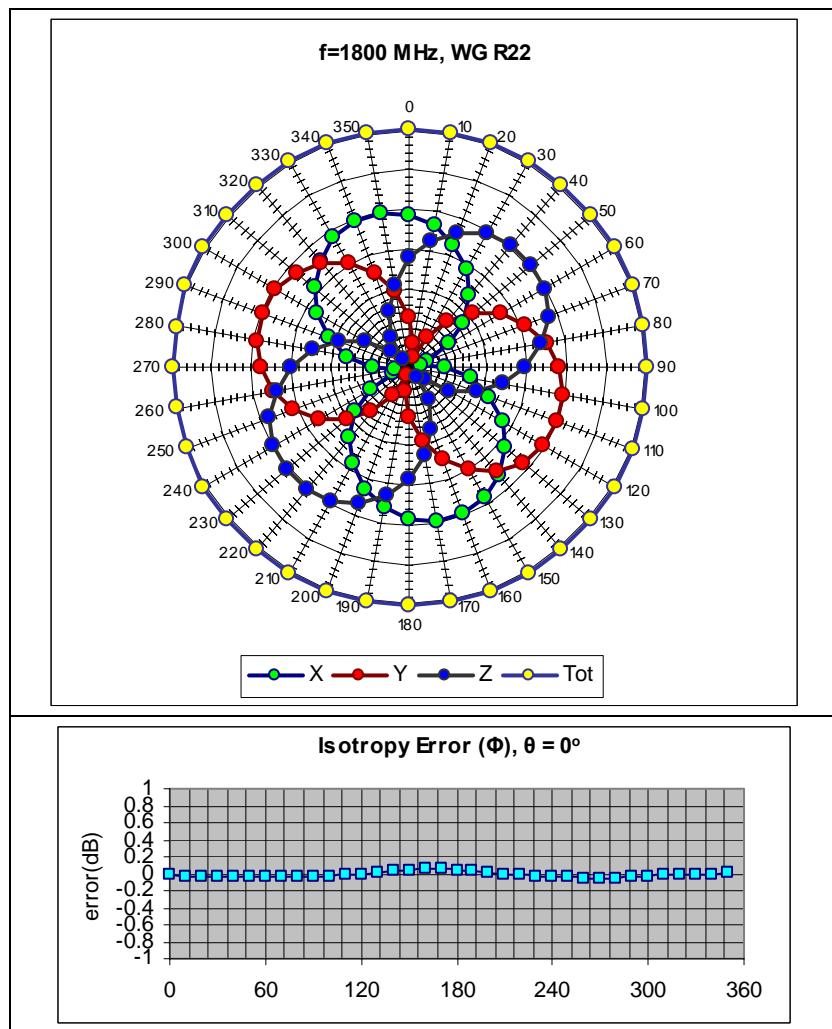


Figure 5. Example of the rotational isotropy of probe S/N 0136 obtained by rotating the probe in a liquid-filled waveguide at 2450 MHz. Similar distributions are obtained at the other test frequencies (1800 and 1900 MHz) both in brain liquids and body fluids (see summary table)

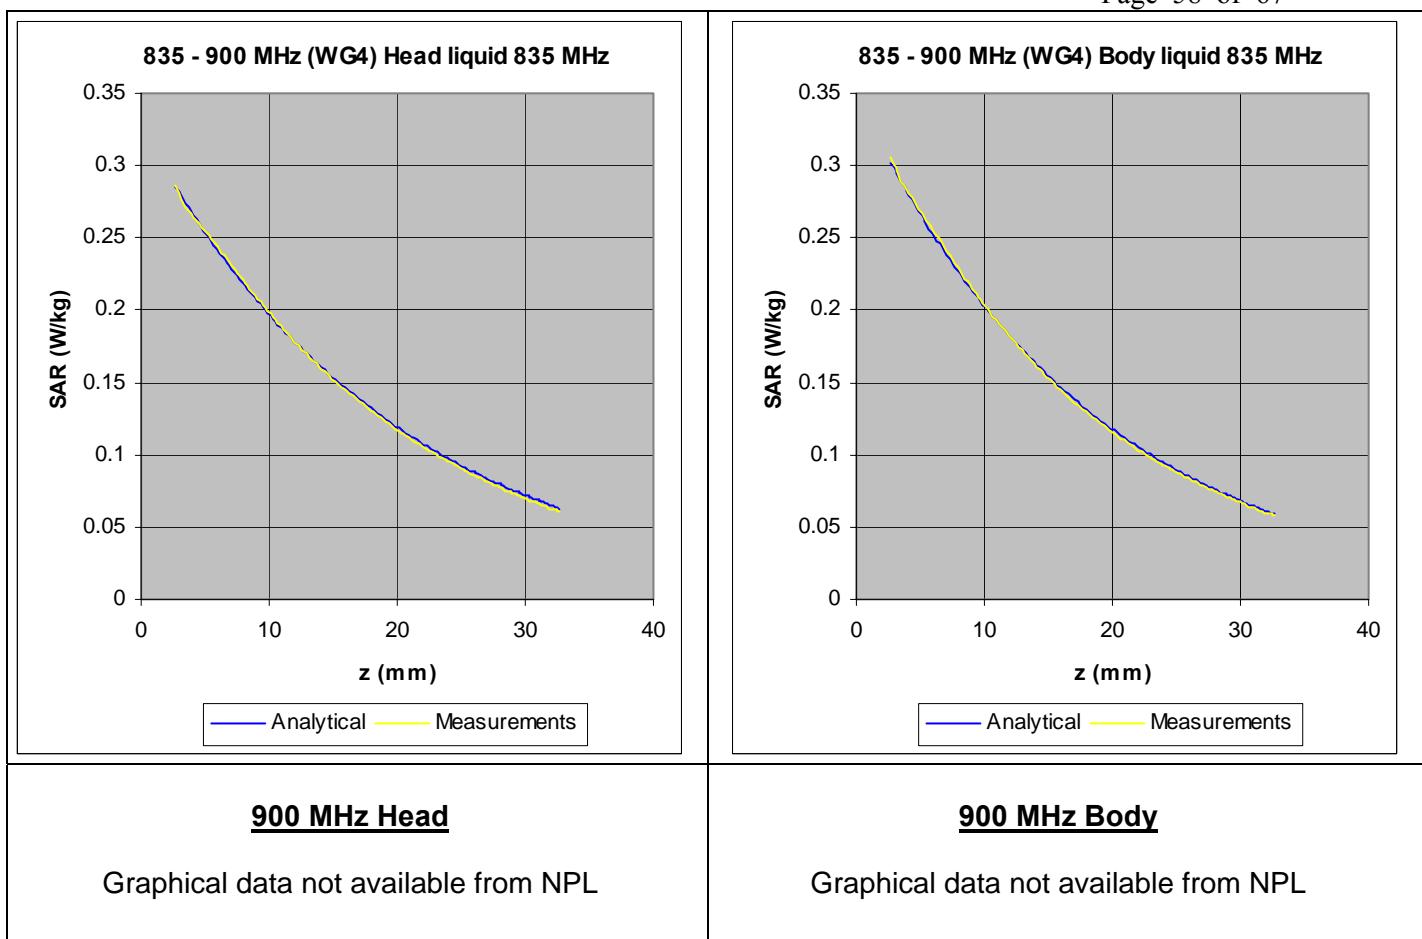


Figure 6. The measured SAR decay function along the centreline of the WG4 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.

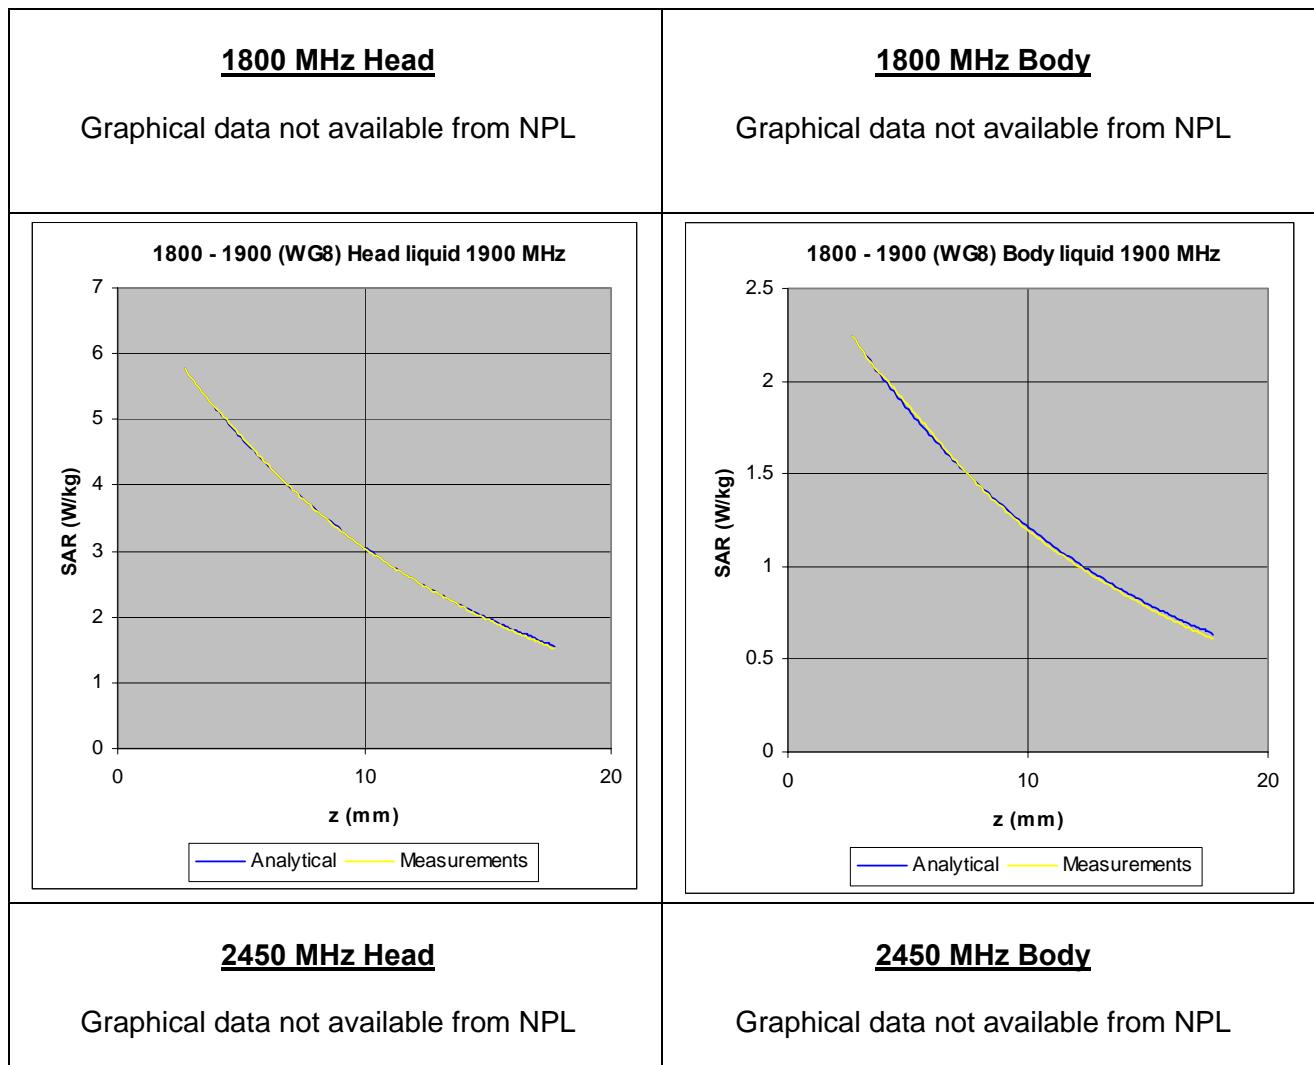


Figure 7. The measured SAR decay function along the centreline of the R22 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.

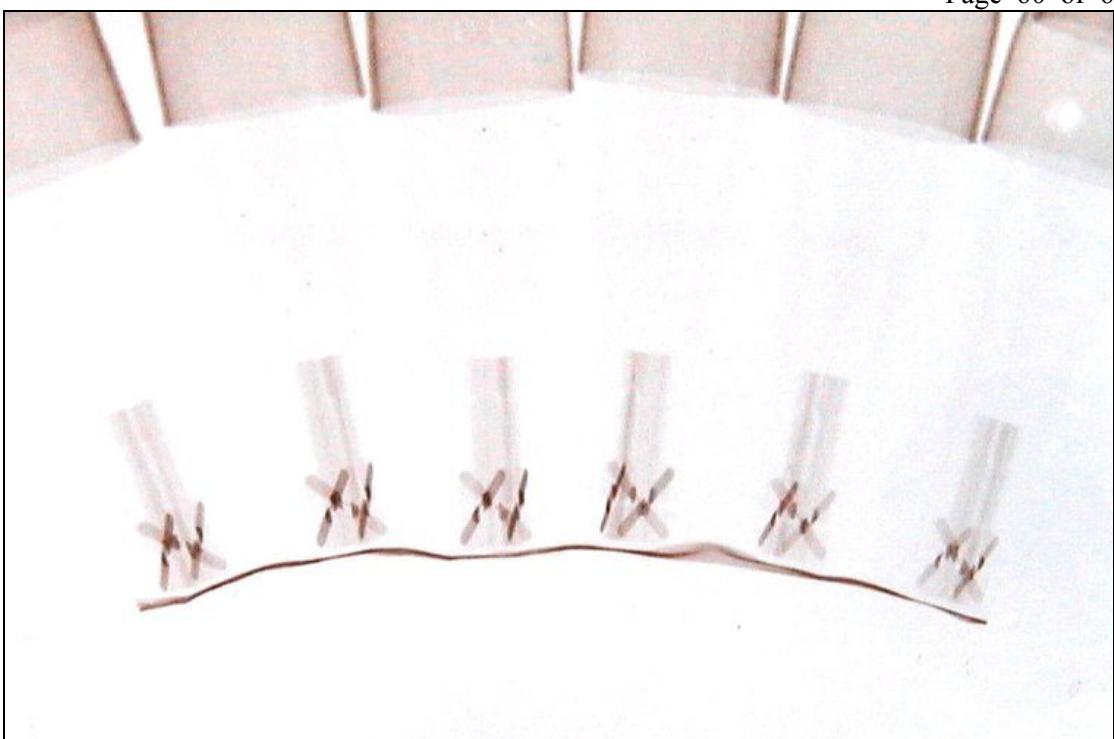


Figure 8: X-ray positive image of 5mm probes

Table indicating the dielectric parameters of the liquids used for calibrations at each frequency

<i>Liquid used</i>	<i>Relative permittivity (measured)</i>	<i>Conductivity (S/m) (measured)</i>
835 MHz BRAIN	41.53	0.89
835 MHz BODY	48.72	1.02
900 MHz BRAIN	40.8	0.95
900 MHz BODY	56.5	1.02
1800 MHz BRAIN	40.5	1.38
1800 MHz BODY	53.5	1.56
1900 MHz BRAIN	38.63	1.47
1900 MHz BODY	54.00	1.66
2450 MHz BRAIN	38.5	1.85
2450 MHz BODY	53.4	1.99



Indexsar Limited
Oakfield House
Cudworth Lane
Newdigate
Surrey RH5 5BG
Tel: +44 (0) 1306 632 870
Fax: +44 (0) 1306 631 834
e-mail: enquiries@indexsar.com

Calibration Certificate

Type: **IXD-045**

Manufacturer: **IndexSAR, UK**

Serial Number: **0010**

Place of Calibration: **IndexSAR, UK**

Date of Initial Calibration: **16th January 2006**

The calibration was carried out using the methods described in the calibration document.
Where applicable, the standards used in the calibration process are traceable to the UK's National Physical Laboratory.

Calibrated By:

A handwritten signature in black ink, appearing to read "M.J. Mainf".

Approved By:




Report No. SN0010_450
January 2006

INDEXSAR

450MHz validation Dipole
Type IXD-045 S/N 0010

Performance measurements

- *MI Manning*

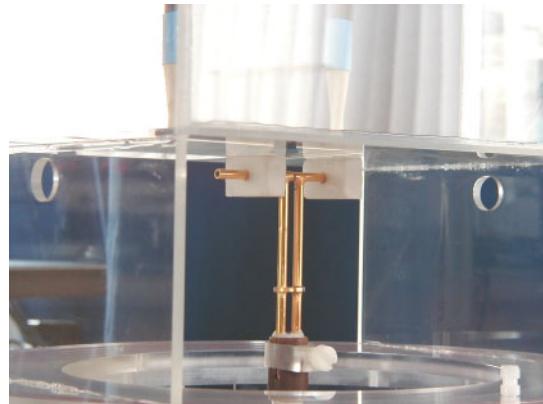

**Indexsar, Oakfield House, Cudworth Lane,
Newdigate, Surrey RH5 5BG. UK.**

Tel: +44 (0) 1306 633870 Fax: +44 (0) 1306 631834
e-mail: enquiries@indexsar.com

1. Measurement Conditions

Measurements were performed using a box-shaped phantom made of PMMA with dimensions designed to meet the accuracy criteria for reasonably-sized phantoms that do not have liquid capacities substantially in excess of the volume of liquid required for the frequency of 450MHz.

An Anritsu MS4623B vector network analyser was used for the return loss measurements.

The dipole was placed in a special holder made of low-permittivity, low-loss materials. This holder enables the dipole to be positioned accurately in the centre of the base of the Indexsar box-phantom used for flat-surface testing and validation checks.

The validation dipoles are used with special spacers made from a low-permittivity, low-loss foam material. These spacers are fitted to the dipole arms to ensure that, when the dipole is offered up to the phantom surface, the spacing between the dipole and the liquid surface is accurately aligned according to the guidance in the relevant standards documentation. The spacers are rectangular with a central hole equal to the dipole arm diameter and dimensioned so that the longer side can be used to ensure a spacing of 15mm from the liquid in the phantom (for tests at 900MHz and below) and the shorter side can be used for tests at 1800MHz and above to ensure a spacing of 10mm from the liquid in the phantom. The spacers are made on a CNC milling machine with an accuracy of 1/40th mm but they may suffer wear and tear and need to be replaced periodically. The material used is Rohacell, which has a relative permittivity of approx. 1.05 and a negligible loss tangent.

The apparatus supplied by Indexsar for dipole validation tests thus includes:

Balanced dipoles for each frequency required are dimensioned according to the guidelines given in IEEE 1528 [1]. The dipoles are made from semi-rigid 50 Ohm co-ax, which is joined by soldering and is gold-plated subsequently. The constructed dipoles are easily deformed, if mis-handled, and periodic checks need to be made of their symmetry.

Rohacell foam spacers designed for presenting the dipoles to 2mm thick PMMA box phantoms (or 6mm thick for 450MHz). These components also suffer wear and tear and should be replaced when the central hole is a loose-fit on the dipole arms or if the edges are too worn to ensure accurate alignment. The standard spacers are dimensioned for use with 2mm wall thickness (additional spacers are available for 4mm and 6mm wall thicknesses).

2. Dipole validation SAR Measurement


A SAR validation check was performed with the box-phantom located on the SARA2 side-bench of the SARA2 robot system. Tests were then conducted at a feed power level of approx. 0.25W. The actual power level was recorded and used to normalise the results obtained to the standard input power conditions of 1W (forward power). The ambient temperature was 17°C +/- 1°C and the relative humidity was 40% during the measurements.

The phantom was filled with a 450MHz brain liquid using a recipe from [1], which had the following electrical parameters (measured using an Indexsar DiLine kit) at 450MHz:

Relative Permittivity **43.78**
Conductivity **0.79 S/m**

The SARA2 software version 2.41 VPM was used with an Indexsar probe (S/N 0137) previously calibrated using waveguides by the National Physical Laboratory (NPL) [2].

The 3D validation measurement made using the dipole at the bottom of the phantom box is shown below:

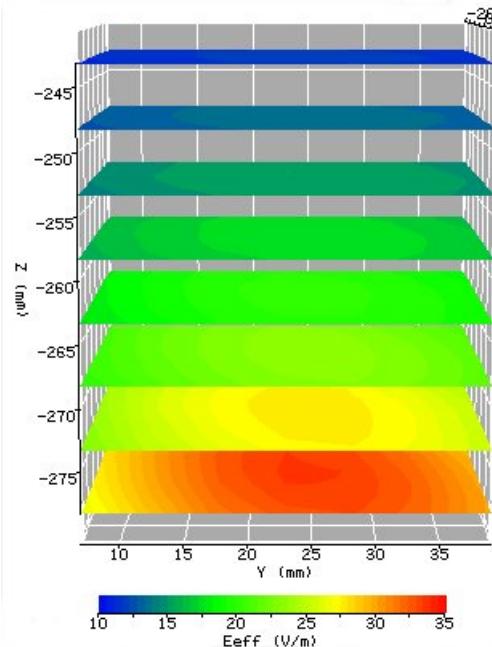

The results, normalised to an input power of 1W (forward power) were:

Averaged over 1 cm³ (1g) of tissue **4.748 W/kg**
Averaged over 10cm³ (10g) of tissue **3.252 W/kg**


These results can be compared with the reference values for 450MHz from Table 8.1 in [1]. The agreement is within 3%.

3. Dipole impedance and return loss

The dipoles are designed to have low return loss ONLY when presented against a lossy-phantom at the specified distance. A Vector Network Analyser (VNA) was used to perform a return loss measurement on the specific dipole when in the measurement-location against the box phantom. The distance was as specified in the standard i.e. 15mm from the liquid (for 450MHz). The Indexsar foam spacers (described above) were used to ensure this condition during measurement.

The impedance was measured at the SMA-connector with the network analyser. The following parameters were measured:

Return loss at 450MHz **-26.506 dB**

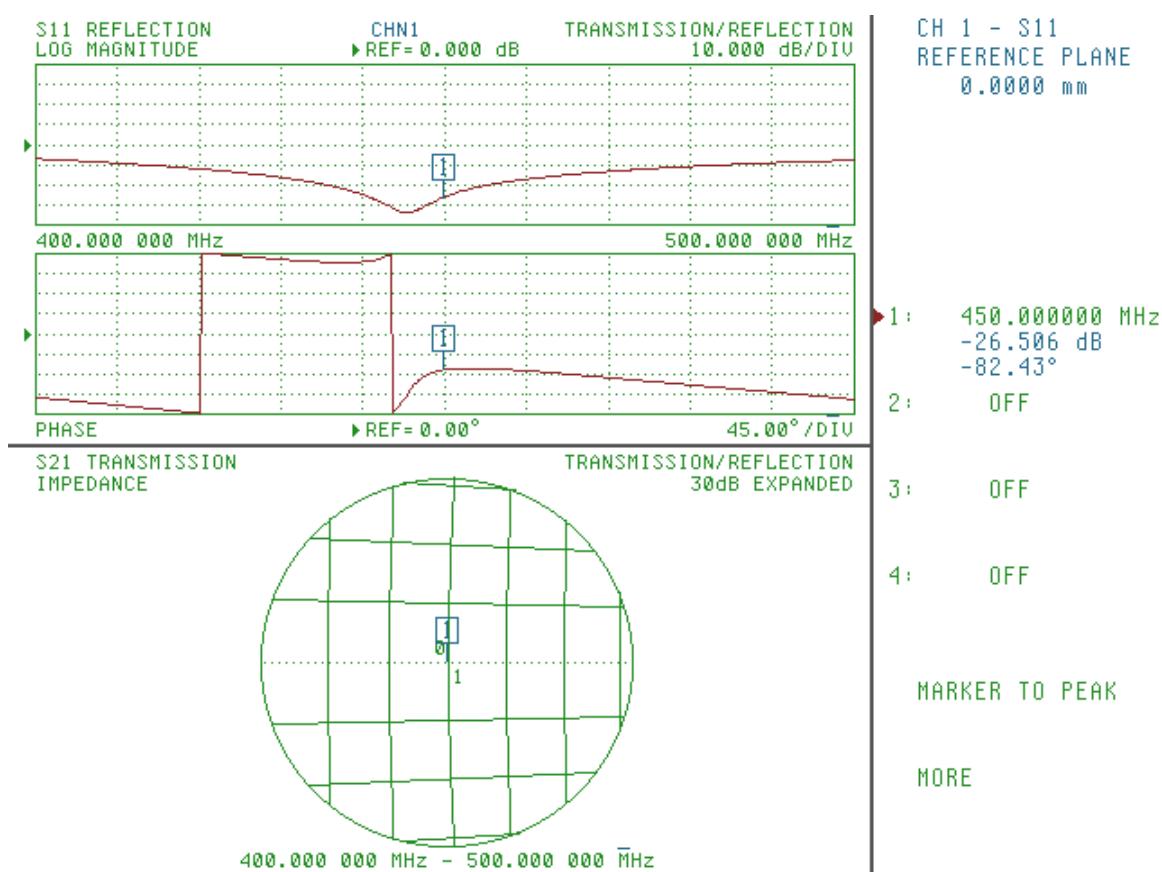

4. Dipole handling

The dipoles are made from standard, copper-sheathed coaxial cable. In assembly, the sections are joined using ordinary soft soldering. This is necessary to avoid excessive heat input in manufacture, which would destroy the polythene dielectric used for the cable. The consequence of the construction material and the assembly technique is that the dipoles are fragile and can be deformed by rough handling. Conversely, they can be straightened quite easily as described in this report.

If a dipole is suspected of being deformed, a normal workshop lathe can be used as an alignment jig to restore the symmetry. To do this, the dipole is first placed in the headstock of the lathe (centred on the plastic or brass spacers) and the headstock is rotated by hand (do NOT use the motor). A marker (lathe tool or similar) is brought up close to the end of one dipole arm and then the headstock is rotated by 0.5 rev. to check the opposing arm. If they are not balanced, judicious deformation of the arms can be used to restore the symmetry.

If a dipole has a failed solder joint, the dipole can be fixed down in such a way that the arms are co-linear and the joint re-soldered with a reasonably powerful electrical soldering iron. Do not use gas soldering irons. After such a repair, electrical tests must be performed as described below.

Please note that, because of their construction, the dipoles are short-circuited for DC signals.

5. Tuning the dipole

The dipole dimensions are based on calculations that assumed specific liquid dielectric properties. If the liquid dielectric properties are somewhat different, the dipole tuning will also vary. A pragmatic way of accounting for variations in liquid properties is to 'tune' the dipole (by applying minor variations to its effective length). For this purpose, Indexsar can supply short brass tube lengths to extend the length of the dipole and thus 'tune' the dipole. It cannot be made shorter without removing a bit from the arm. An alternative way to tune the dipole is to use copper shielding tape to extend the effective length of the dipole. Do both arms equally.

It should be possible to tune a dipole as described, whilst in place in the measurement position as long as the user has access to a VNA for determining the return loss.

6. References

- [1] Recommended practice for determining the peak spatial-average specific absorption rate (SAR) in the human body due to wireless communications devices: Measurement Techniques. IEEE Std. 1528.
- [2] National Physical Laboratory Certificate of Calibration: SAR Probe Indexsar IXP-050 (S/N 0137). Report No. E050602032 dated 10th June 2005.