

HAC_E_Dipole_835_160312

DUT: HAC-Dipole 835 MHz

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1
 Medium: Air Medium parameters used: $\sigma = 0$ S/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³
 Ambient Temperature : 23.5 °C

DASY5 Configuration

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2016/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2016/2/18
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

E Scan - measurement distance from the probe sensor center to CD835 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x361x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 123.6 V/m; Power Drift = -0.01 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 115.3 V/m

Average value of Total=(115.3+107.2) / 2 = 111.25 V/m

PMF scaled E-field



Grid 1 M4 111.1 V/m	Grid 2 M4 115.3 V/m	Grid 3 M4 114.1 V/m
Grid 4 M4 61.34 V/m	Grid 5 M4 62.81 V/m	Grid 6 M4 61.97 V/m
Grid 7 M4 105.4 V/m	Grid 8 M4 107.2 V/m	Grid 9 M4 105.4 V/m

Cursor:

Total = 115.3 V/m

E Category: M4

Location: -1, -78, 9.7 mm

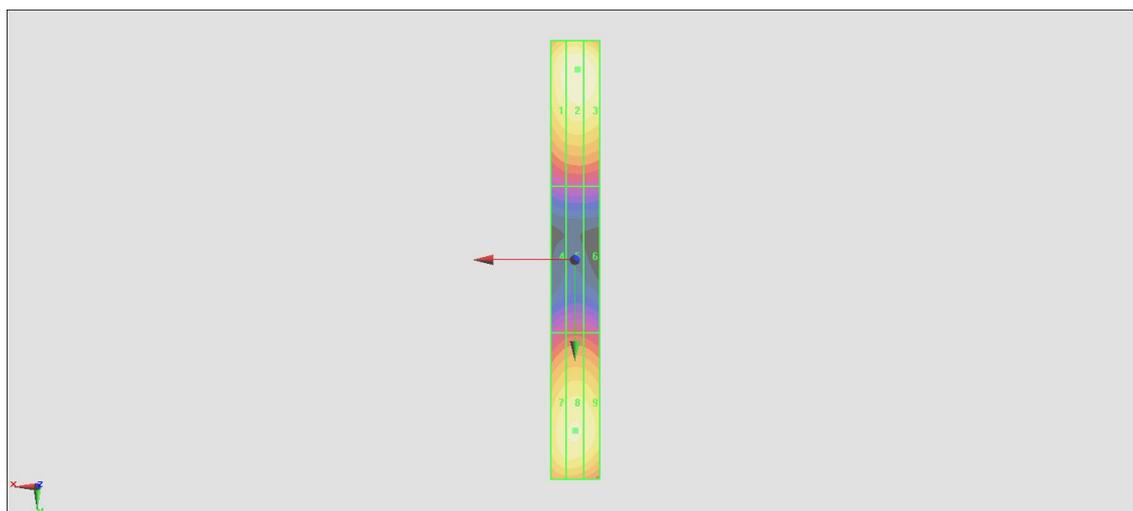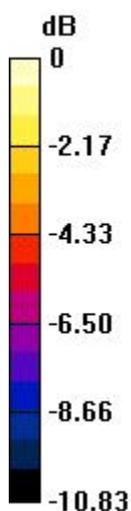

0 dB = 115.3 V/m = 41.24 dBV/m

HAC_E_Dipole_1880_160312

DUT: HAC Dipole 1880 MHz

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1
 Medium: Air Medium parameters used: $\sigma = 0$ S/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³
 Ambient Temperature : 23.5 °C

DASY5 Configuration

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2016/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn778; Calibrated: 2016/2/18
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

E Scan - measurement distance from the probe sensor center to CD1880 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 144.8 V/m; Power Drift = 0.02 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 92.16 V/m

Average value of Total=(91.84+92.16) / 2 = 92 V/m

PMF scaled E-field



Grid 1 M3 90.61 V/m	Grid 2 M3 91.84 V/m	Grid 3 M3 90.28 V/m
Grid 4 M3 70.80 V/m	Grid 5 M3 72.19 V/m	Grid 6 M3 71.48 V/m
Grid 7 M3 90.63 V/m	Grid 8 M3 92.16 V/m	Grid 9 M3 90.26 V/m

Cursor:

Total = 92.16 V/m

E Category: M3

Location: 0, 31, 9.7 mm

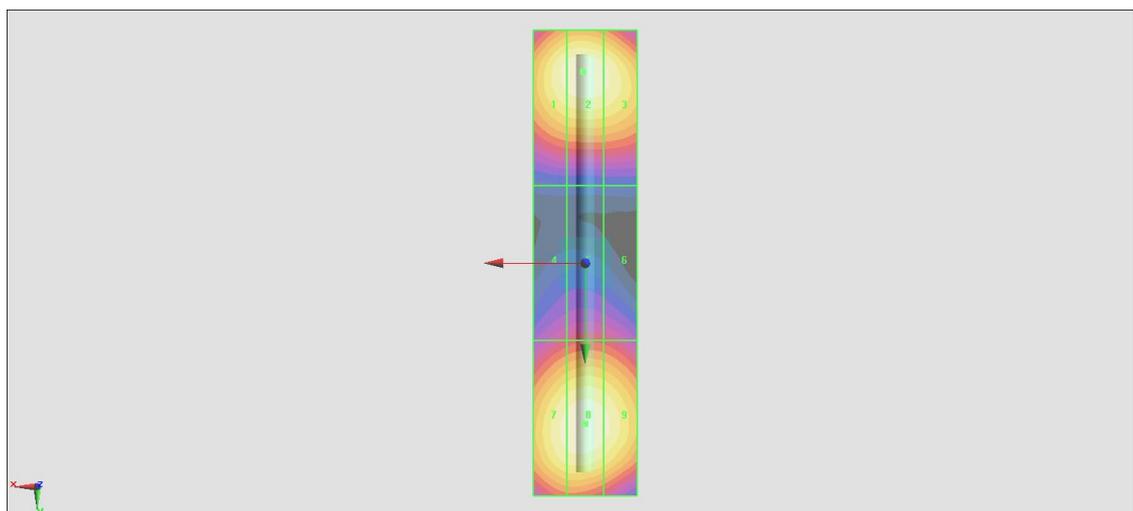

0 dB = 92.16 V/m = 39.29 dBV/m

HAC_E_Dipole_2600_160321

DUT: HAC Dipole 2600 MHz

Communication System: CW ; Frequency: 2600 MHz; Duty Cycle: 1:1

Medium: Air Medium parameters used: $\sigma = 0$ S/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³

Ambient Temperature : 23.5 °C

DASY5 Configuration

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2016/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn495; Calibrated: 2015/5/22
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

E Scan - measurement distance from the probe sensor center to CD2600 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 74.24 V/m; Power Drift = -0.01 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 93.84 V/m

Average value of Total=(93.84+84.55) / 2 = 89.195 V/m

PMF scaled E-field


Grid 1 M3 92.16 V/m	Grid 2 M3 93.84 V/m	Grid 3 M3 92.42 V/m
Grid 4 M3 90.09 V/m	Grid 5 M3 91.43 V/m	Grid 6 M3 89.97 V/m
Grid 7 M3 83.06 V/m	Grid 8 M3 84.55 V/m	Grid 9 M3 83.64 V/m

Cursor:

Total = 93.84 V/m

E Category: M3

Location: 0, -19.5, 9.7 mm

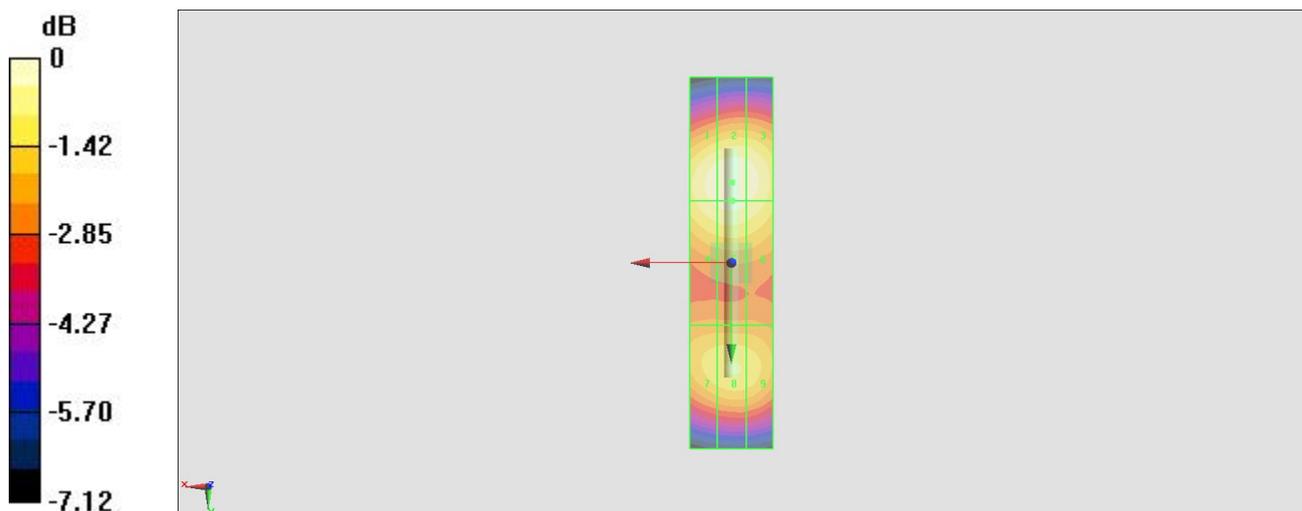

0 dB = 93.84 V/m = 39.45 dBV/m