

GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 12 Middle Frequency

Communication System: GSM 1900+GPRS(2Up); Frequency: 1880 MHz; Duty Cycle: 1:4

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.54$ mho/m; $\epsilon_r = 53.2$; $\rho = 1000$ kg/m³

Probe: ET3DV6 - SN1531; ConvF(4.64, 4.64, 4.64);

Electronics: DAE3 Sn452;

Test Position 12 Middle/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.213 mW/g

Test Position 12 Middle/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 16.8 V/m; Power Drift = -0.089 dB

Peak SAR (extrapolated) = 1.22 W/kg

SAR(1 g) = 0.294 mW/g; SAR(10 g) = 0.118 mW/g

Maximum value of SAR (measured) = 0.349 mW/g

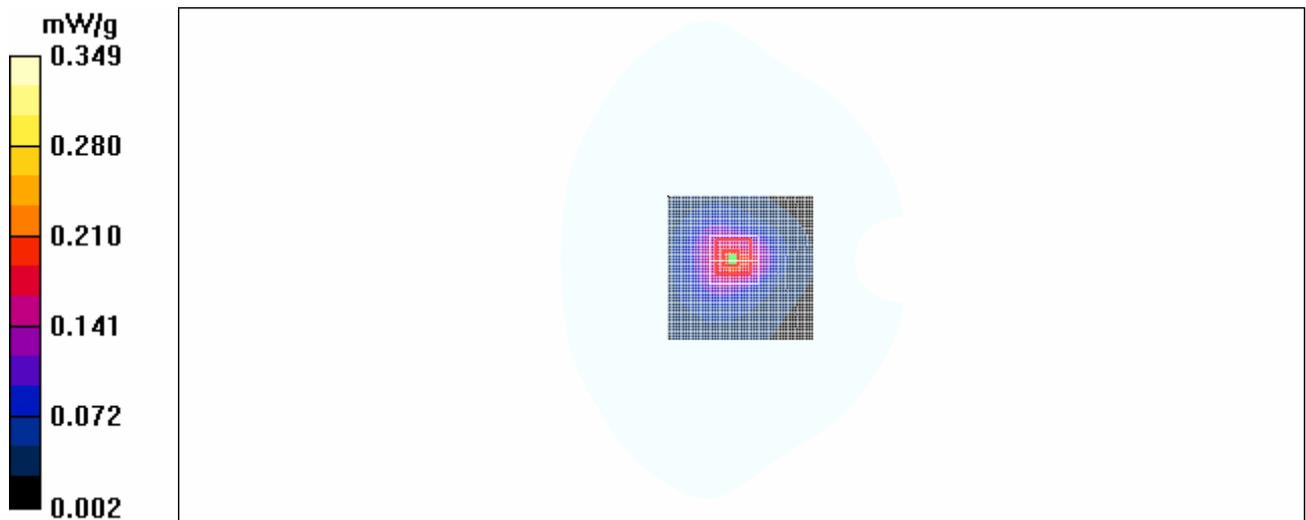


Figure 85 GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 12 Channel 661

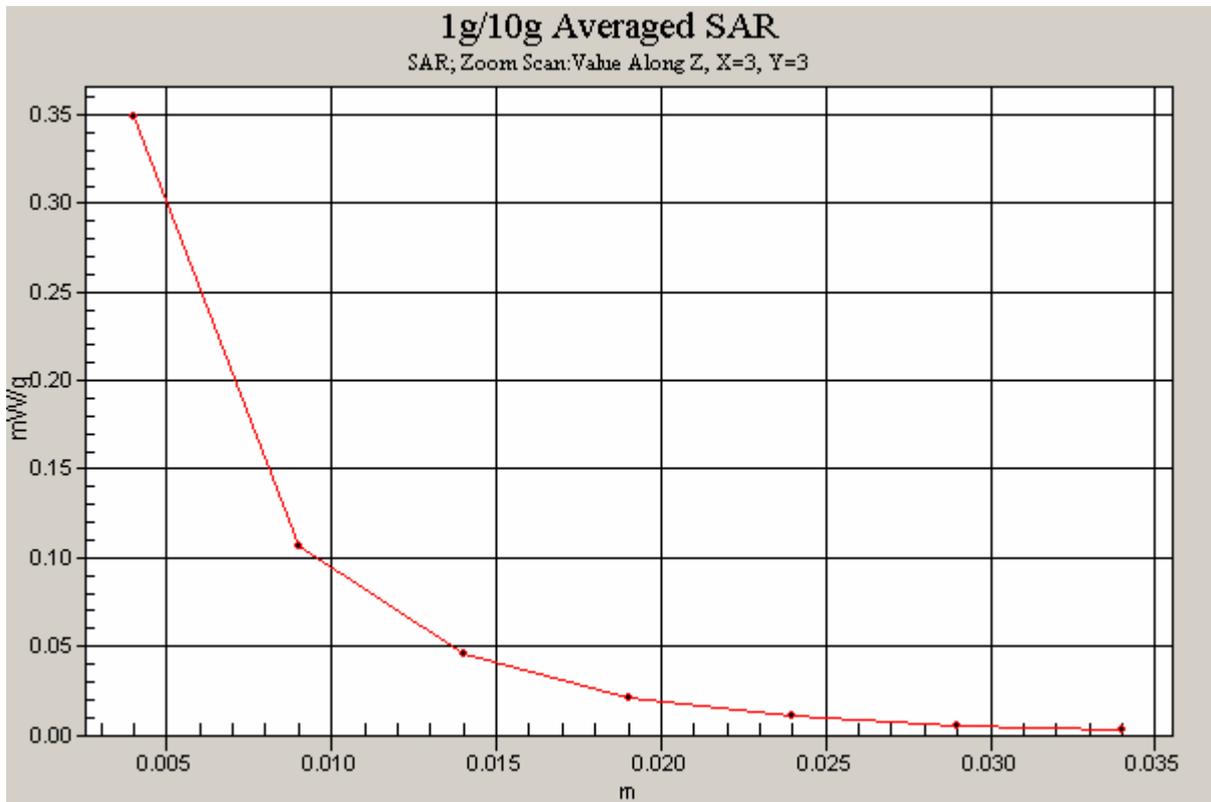


Figure 86 Z-Scan at power reference point [GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 12 Channel 661]

GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 13 Middle Frequency

Communication System: GSM 1900+GPRS(2Up); Frequency: 1880 MHz; Duty Cycle: 1:4

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.52$ mho/m; $\epsilon_r = 52.8$; $\rho = 1000$ kg/m³

Probe: ET3DV6 - SN1531; ConvF(4.64, 4.64, 4.64);

Electronics: DAE3 Sn452;

Test Position 13 Middle/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.468 mW/g

Test Position 13 Middle/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 15.5 V/m; Power Drift = -0.015 dB

Peak SAR (extrapolated) = 0.657 W/kg

SAR(1 g) = 0.432 mW/g; SAR(10 g) = 0.269 mW/g

Maximum value of SAR (measured) = 0.466 mW/g

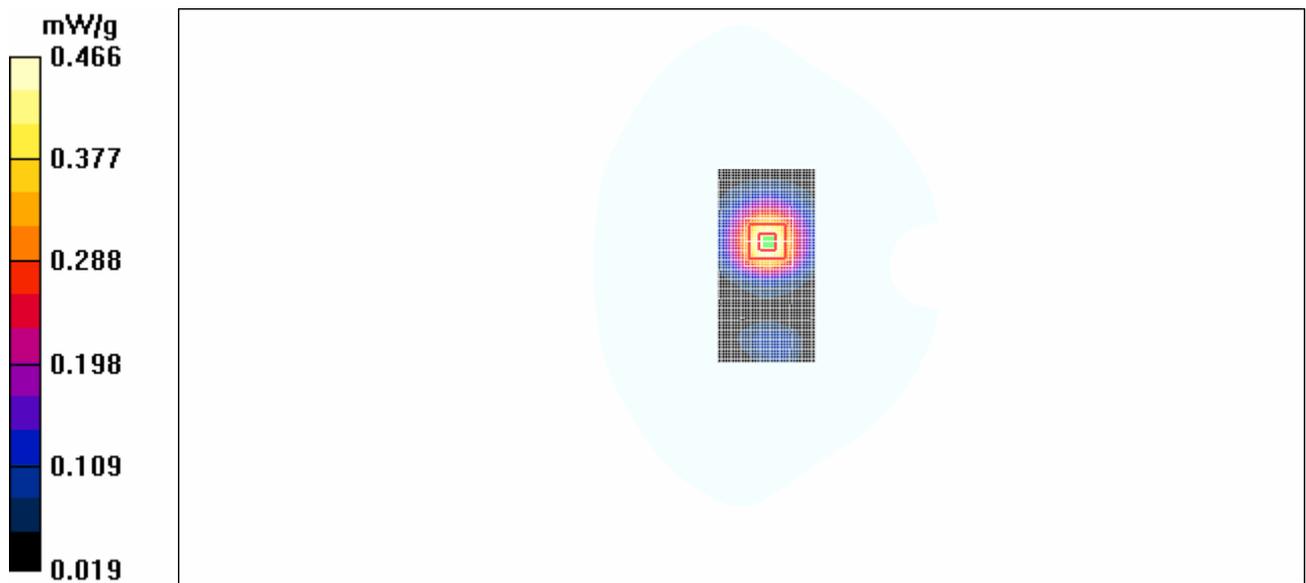


Figure 87 GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 13 Channel 661

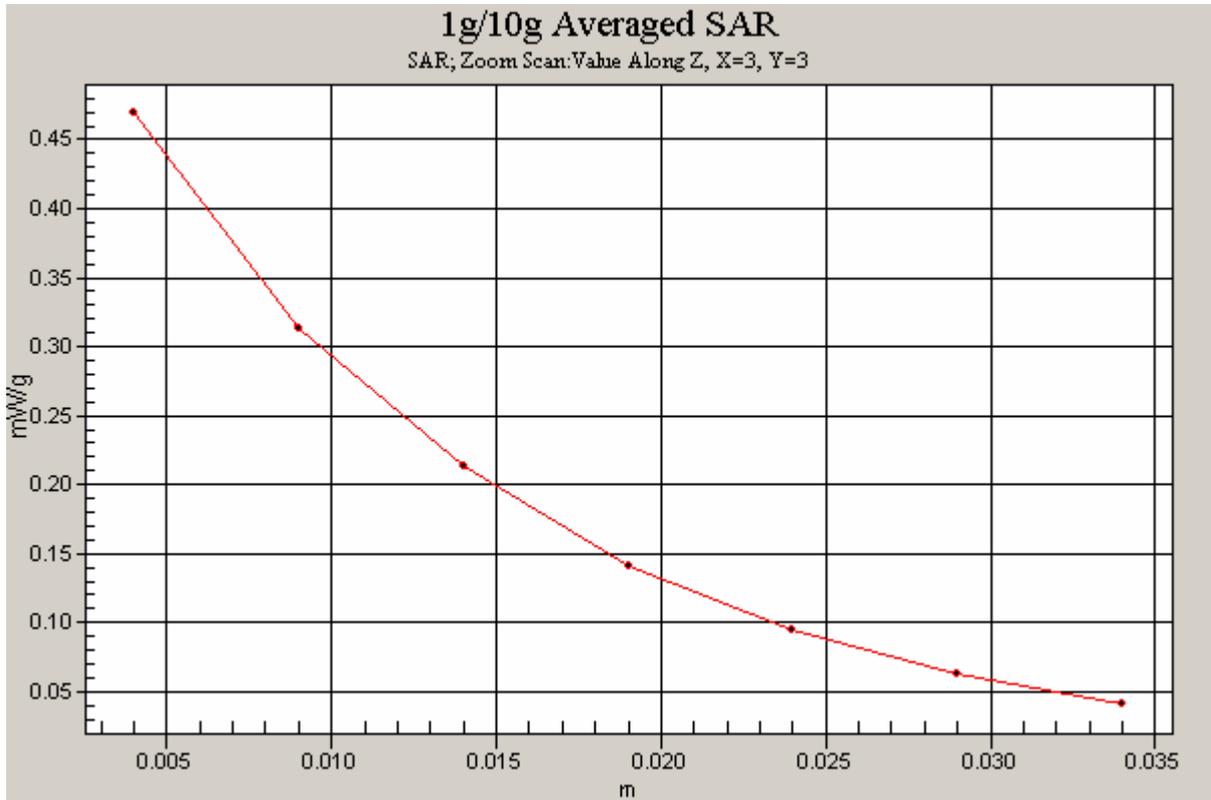


Figure 88 Z-Scan at power reference point [GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 13 Channel 661]

GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 14 Middle Frequency

Communication System: GSM 1900+GPRS(2Up); Frequency: 1880 MHz; Duty Cycle: 1:4

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.54$ mho/m; $\epsilon_r = 53.2$; $\rho = 1000$ kg/m³

Probe: ET3DV6 - SN1531; ConvF(4.64, 4.64, 4.64);

Electronics: DAE3 Sn452;

Test Position 14 Middle/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.113 mW/g

Test Position 14 Middle/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 6.68 V/m; Power Drift = 0.015 dB

Peak SAR (extrapolated) = 0.459 W/kg

SAR(1 g) = 0.097 mW/g; SAR(10 g) = 0.054 mW/g

Maximum value of SAR (measured) = 0.107 mW/g

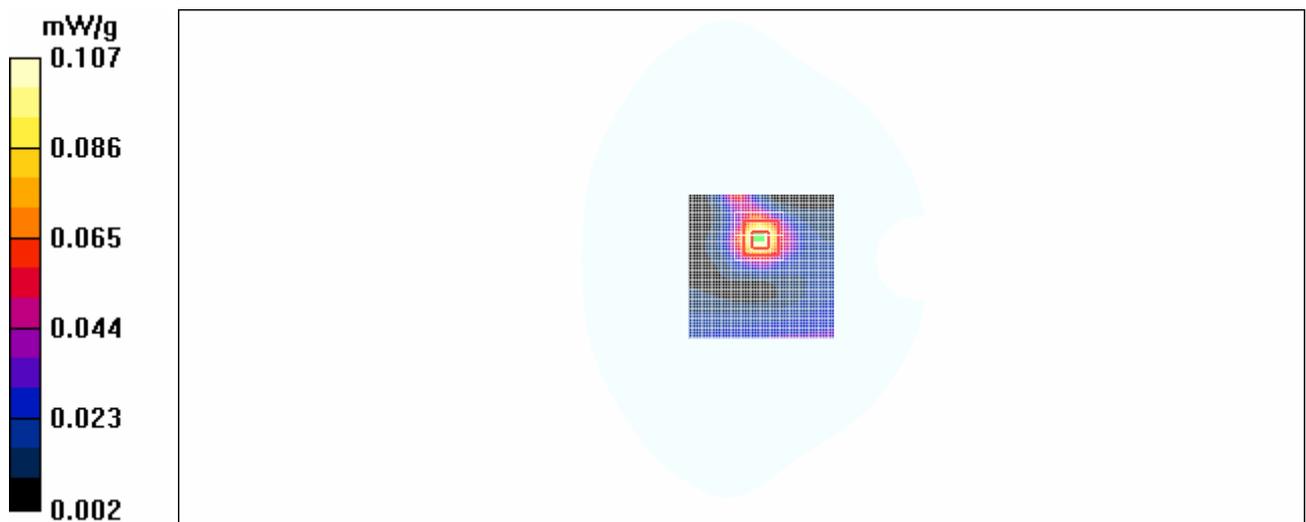


Figure 89 GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 14 Channel 661

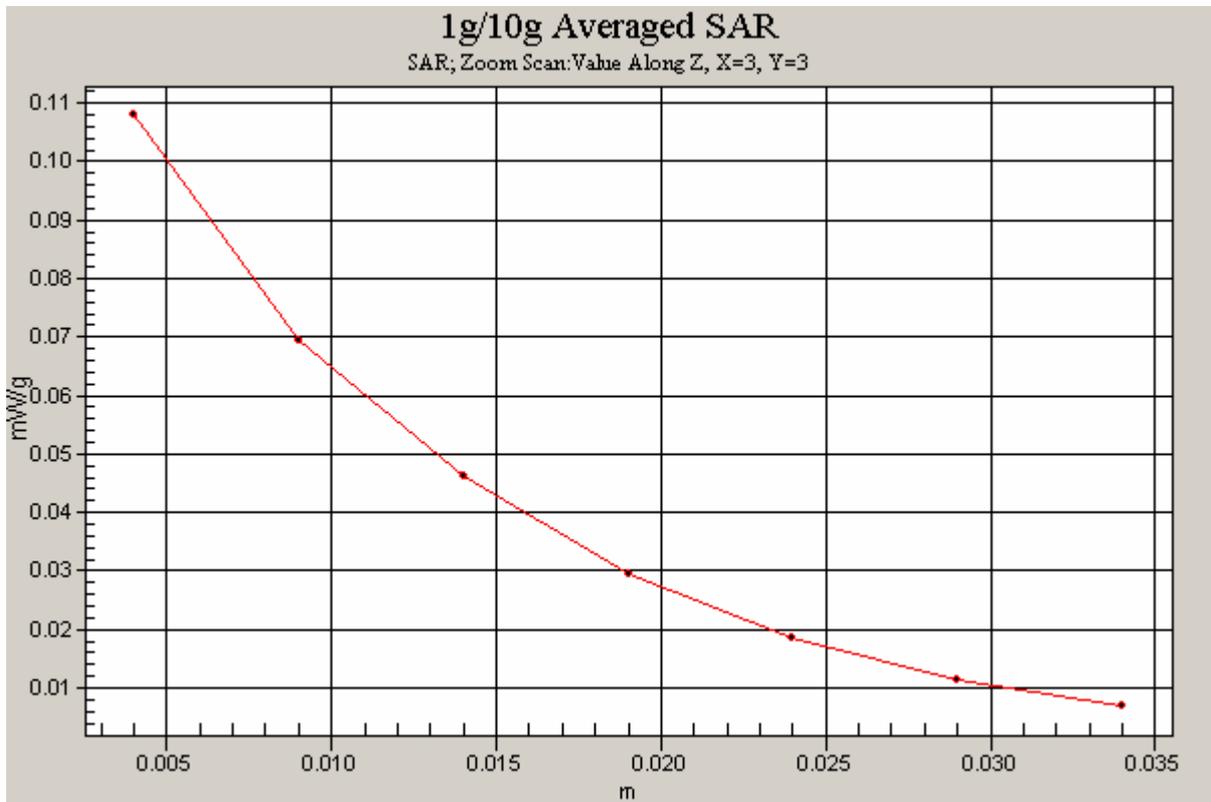


Figure 90 Z-Scan at power reference point [GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 14 Channel 661]

GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 15 Middle Frequency

Communication System: GSM 1900+GPRS(2Up); Frequency: 1880 MHz; Duty Cycle: 1:4

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.52$ mho/m; $\epsilon_r = 52.8$; $\rho = 1000$ kg/m³

Probe: ET3DV6 - SN1531; ConvF(4.64, 4.64, 4.64);

Electronics: DAE3 Sn452;

Test Position 15 Middle/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.295 mW/g

Test Position 15 Middle/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 18.8 V/m; Power Drift = -0.083 dB

Peak SAR (extrapolated) = 1.60 W/kg

SAR(1 g) = 0.367 mW/g; SAR(10 g) = 0.146 mW/g

Maximum value of SAR (measured) = 0.434 mW/g

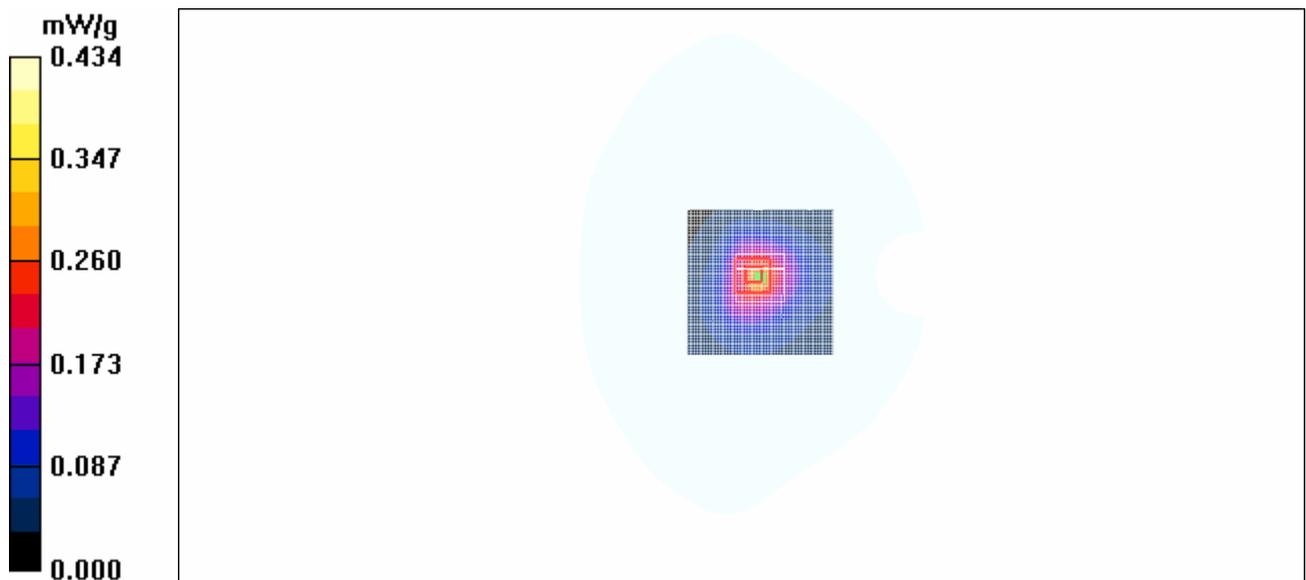


Figure 91 GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 15 Channel 661

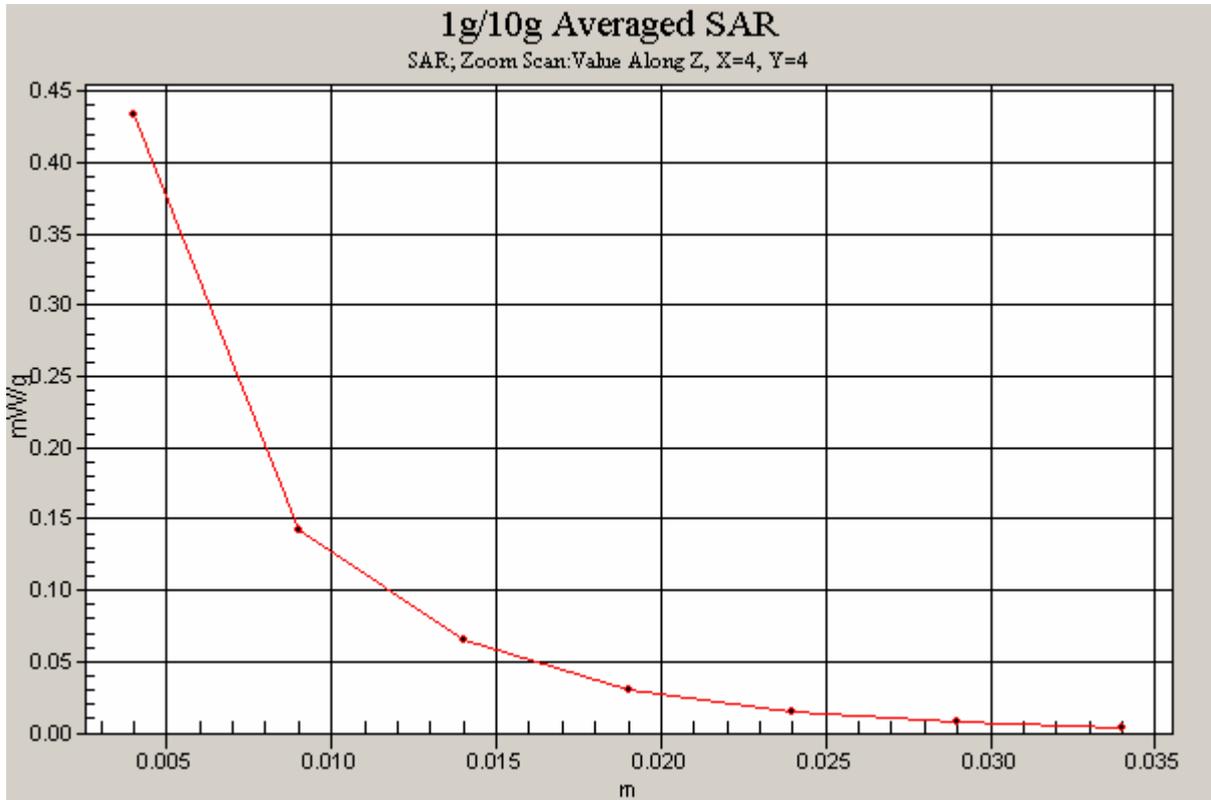


Figure 92 Z-Scan at power reference point [GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 15 Channel 661]

GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 16 Middle Frequency

Communication System: GSM 1900+GPRS(2Up); Frequency: 1880 MHz; Duty Cycle: 1:4

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.54$ mho/m; $\epsilon_r = 53.2$; $\rho = 1000$ kg/m³

Probe: ET3DV6 - SN1531; ConvF(4.64, 4.64, 4.64);

Electronics: DAE3 Sn452;

Test Position 16 Middle/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.693 mW/g

Test Position 16 Middle/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 21.2 V/m; Power Drift = -0.142 dB

Peak SAR (extrapolated) = 0.881 W/kg

SAR(1 g) = 0.588 mW/g; SAR(10 g) = 0.362 mW/g

Maximum value of SAR (measured) = 0.638 mW/g

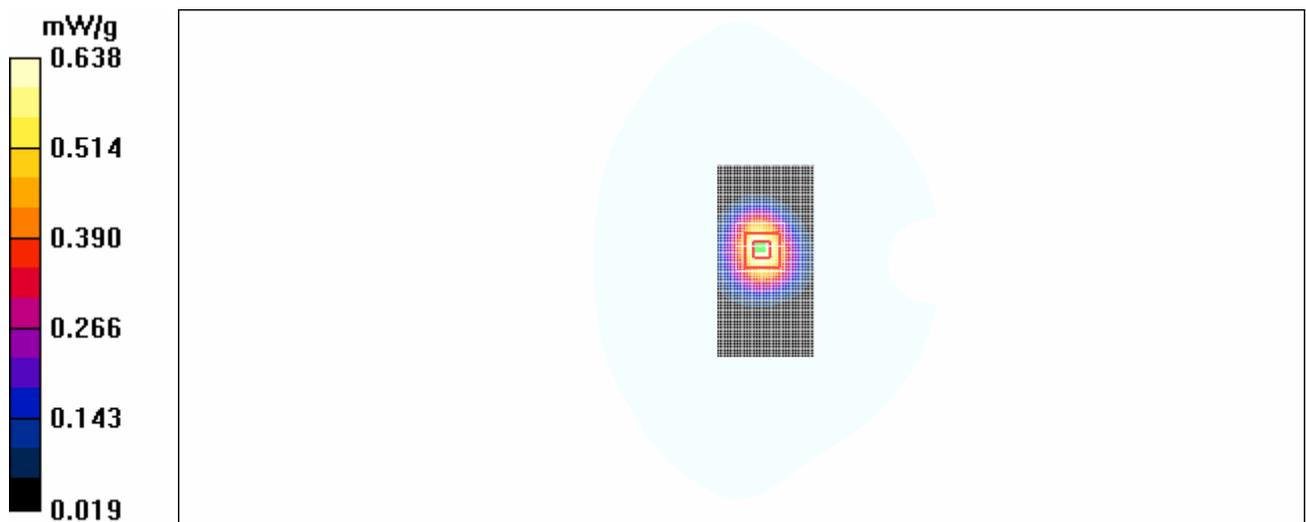


Figure 93 GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 16 Channel 661

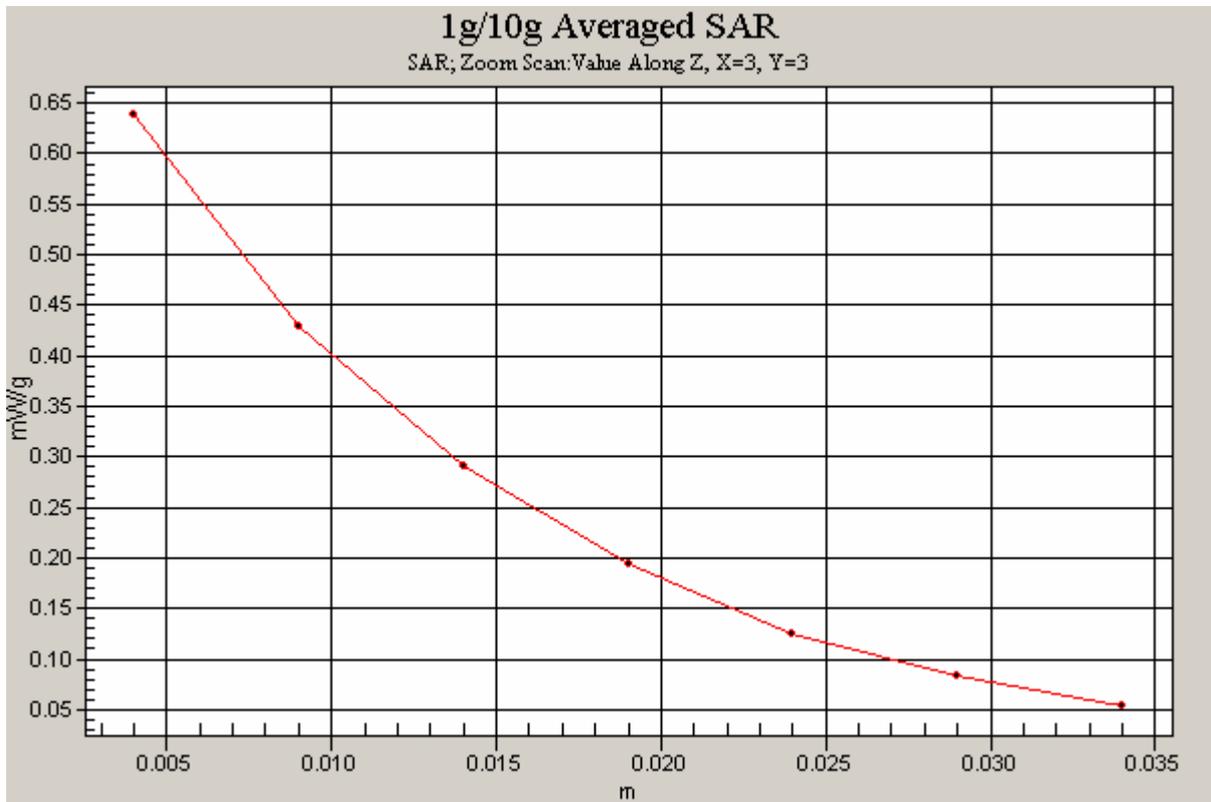


Figure 94 Z-Scan at power reference point [GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 16 Channel 661]

GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 17 Middle Frequency

Communication System: GSM 1900+GPRS(2Up); Frequency: 1880 MHz; Duty Cycle: 1:4

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.54$ mho/m; $\epsilon_r = 53.2$; $\rho = 1000$ kg/m³

Probe: ET3DV6 - SN1531; ConvF(4.64, 4.64, 4.64);

Electronics: DAE3 Sn452;

Test Position 17 Middle/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.696 mW/g

Test Position 17 Middle/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 21.1 V/m; Power Drift = -0.037 dB

Peak SAR (extrapolated) = 1.67 W/kg

SAR(1 g) = 0.639 mW/g; SAR(10 g) = 0.391 mW/g

Maximum value of SAR (measured) = 0.686 mW/g

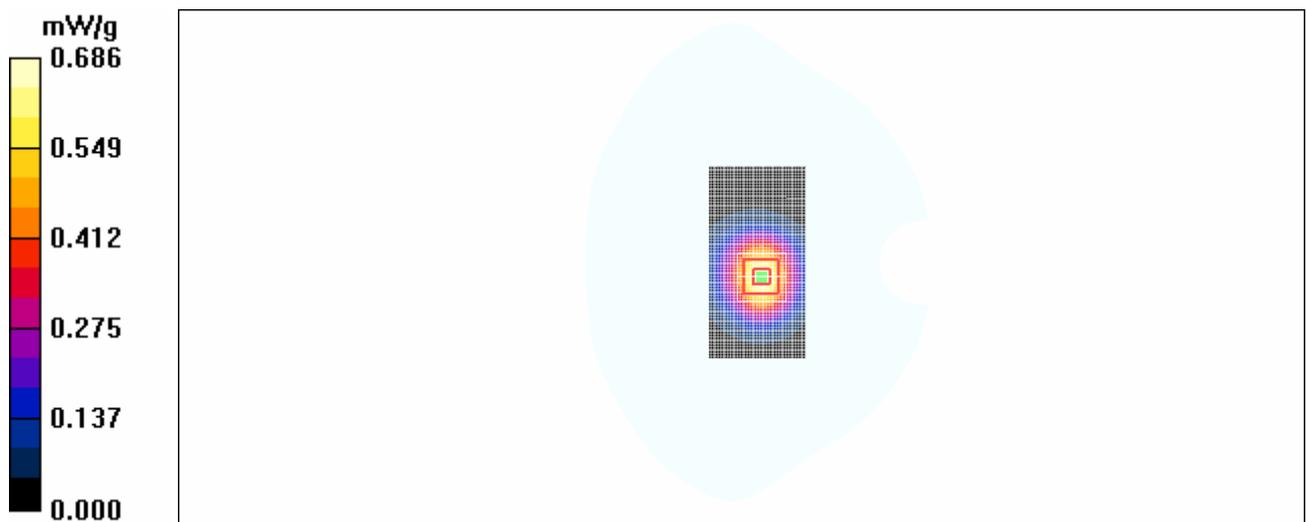


Figure 95 GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 17 Channel 661

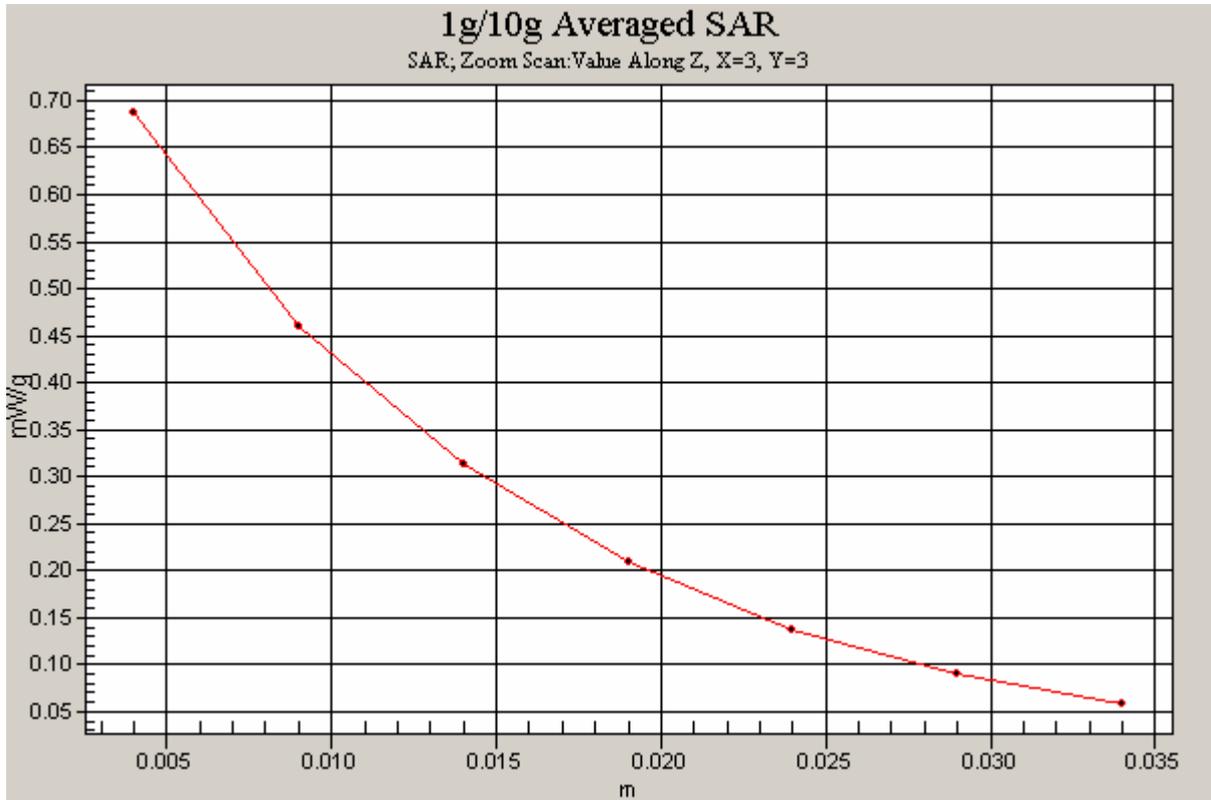


Figure 96 Z-Scan at power reference point [GSM 1900 GPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 17 Channel 661]

GSM 1900 EGPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 11 Middle Frequency

Communication System: GSM 1900+EGPRS(2Up); Frequency: 1880 MHz; Duty Cycle: 1:4

Medium parameters used: $f = 1880$ MHz; $\sigma = 1.54$ mho/m; $\epsilon_r = 53.2$; $\rho = 1000$ kg/m³

Probe: ET3DV6 - SN1531; ConvF(4.64, 4.64, 4.64);

Electronics: DAE3 Sn452;

Test Position 11 Middle/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.581 mW/g

Test Position 11 Middle/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 17.1 V/m; Power Drift = 0.052 dB

Peak SAR (extrapolated) = 0.741 W/kg

SAR(1 g) = 0.469 mW/g; SAR(10 g) = 0.271 mW/g

Maximum value of SAR (measured) = 0.521 mW/g

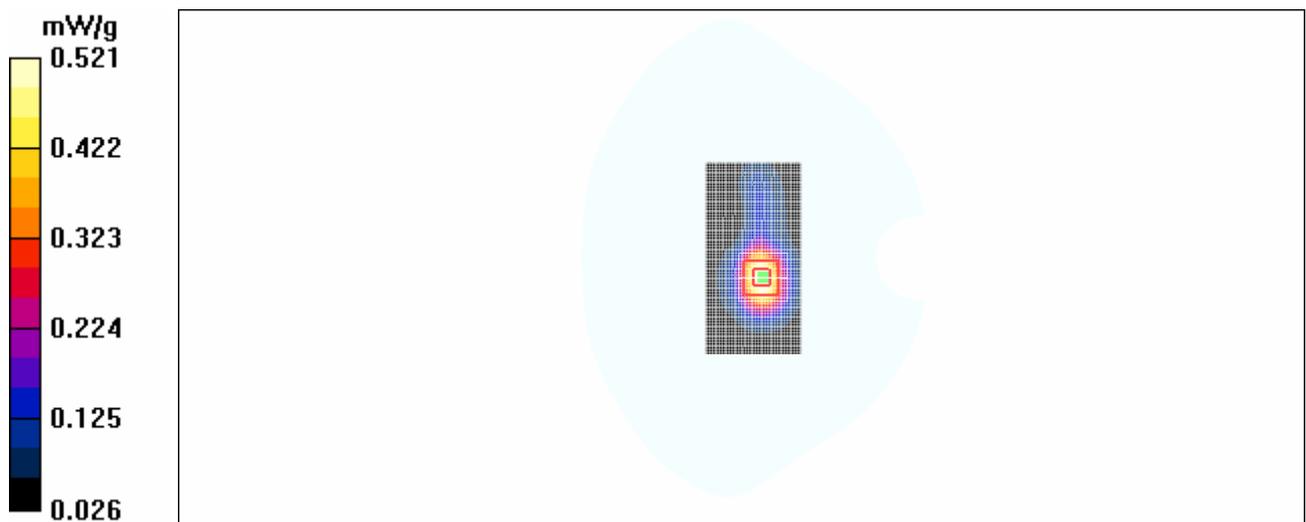


Figure 97 GSM 1900 EGPRS (2 timeslots in uplink) with BenQ Joy book R55v Test Position 11 Channel 661

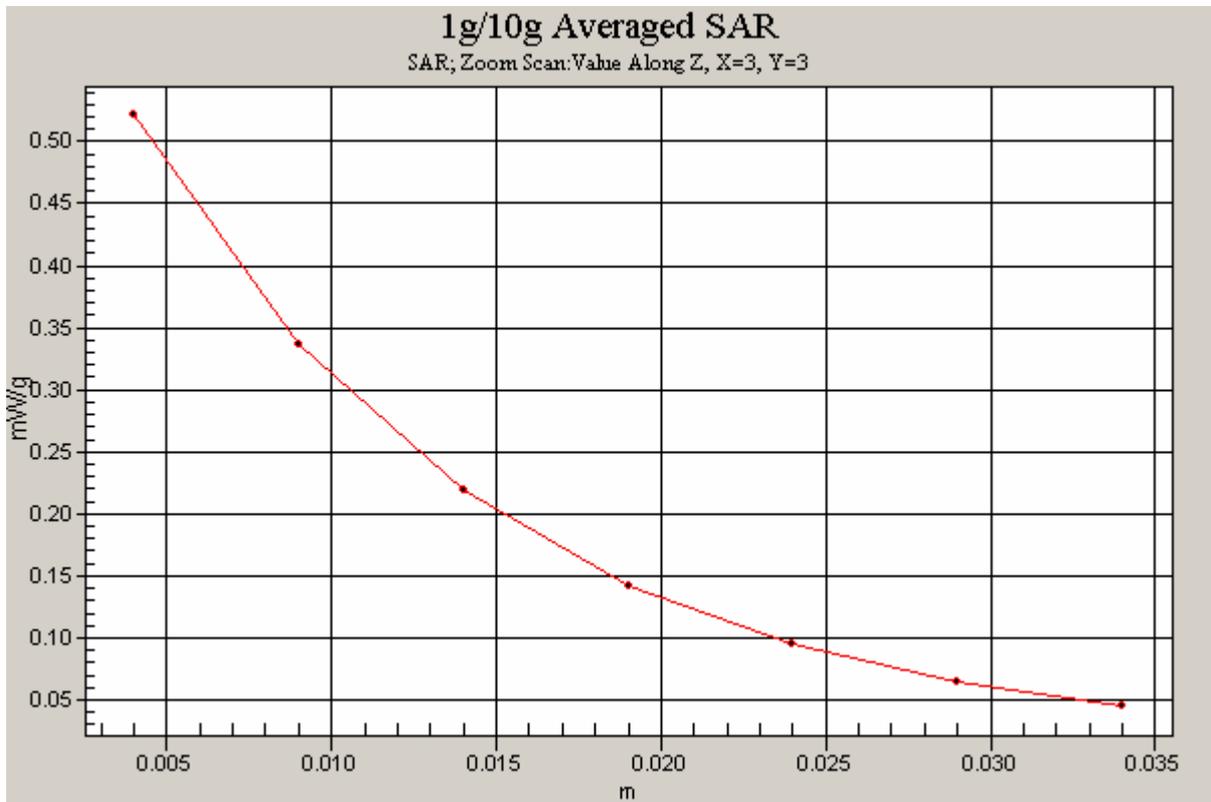


Figure 98 Z-Scan at power reference point [GSM 1900 EGPRS (2 timeslots in uplink) with BenQ Joy book R55V Test Position 11 Channel 661]

ANNEX D: SYSTEM VALIDATION RESULTS

System Performance Check at 835 MHz

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 443

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Head 835MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.92 \text{ mho/m}$; $\epsilon_r = 41.94$; $\rho = 1000 \text{ kg/m}^3$

- Probe: ET3DV6 - SN1531; ConvF(6.85, 6.85, 6.85);

- Electronics: DAE3 Sn452;

d=15mm, Pin=250mW/Area Scan (61x81x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 2.54 mW/g


d=15mm, Pin=250mW/Zoom Scan (7x7x7) /Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 55.0 V/m; Power Drift = -0.061 dB

Peak SAR (extrapolated) = 3.44 W/kg

SAR(1 g) = 2.34 mW/g; SAR(10 g) = 1.53 mW/g

Maximum value of SAR (measured) = 2.52 mW/g

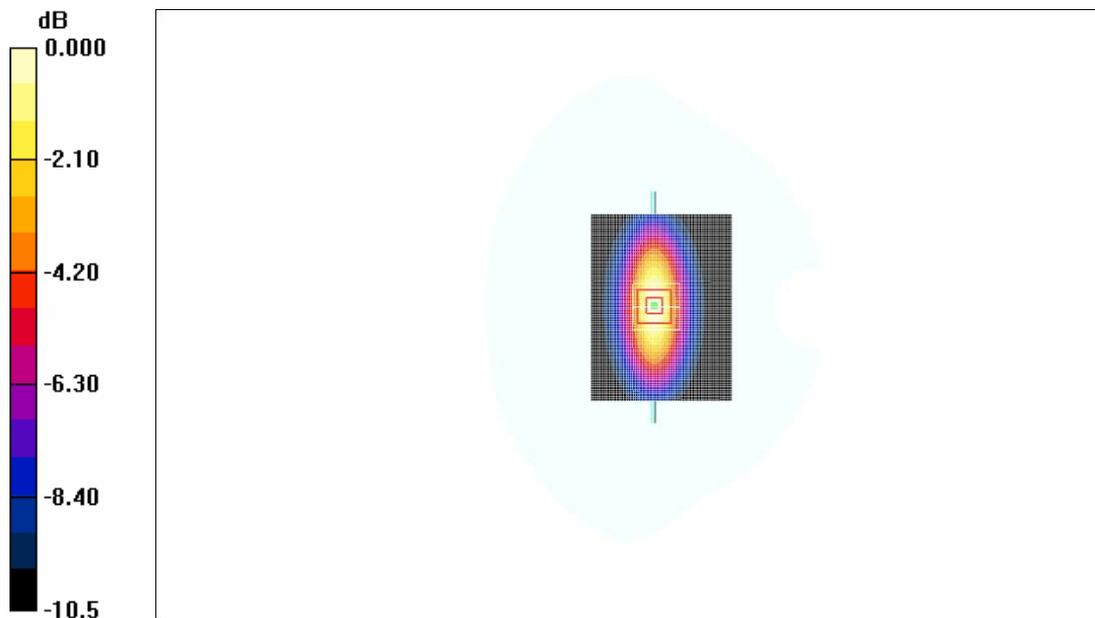

0 dB = 2.52mW/g

Figure 99 System Performance Check 835MHz 250mW

System Performance Check at 1900 MHz

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d018

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.43$ mho/m; $\epsilon_r = 40.09$; $\rho = 1000$ kg/m³

Probe: ET3DV6 - SN1531; ConvF(5.15, 5.15, 5.15);

Electronics: DAE3 Sn452;

d=10mm, Pin=250mW 2/Area Scan (101x121x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 10.8 mW/g

d=10mm, Pin=250mW 2/Zoom Scan (7x7x7) /Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 92.8 V/m; Power Drift = -0.018 dB

Peak SAR (extrapolated) = 16.0 W/kg

SAR(1 g) = 9.36 mW/g; SAR(10 g) = 4.93 mW/g

Maximum value of SAR (measured) = 10.7 mW/g

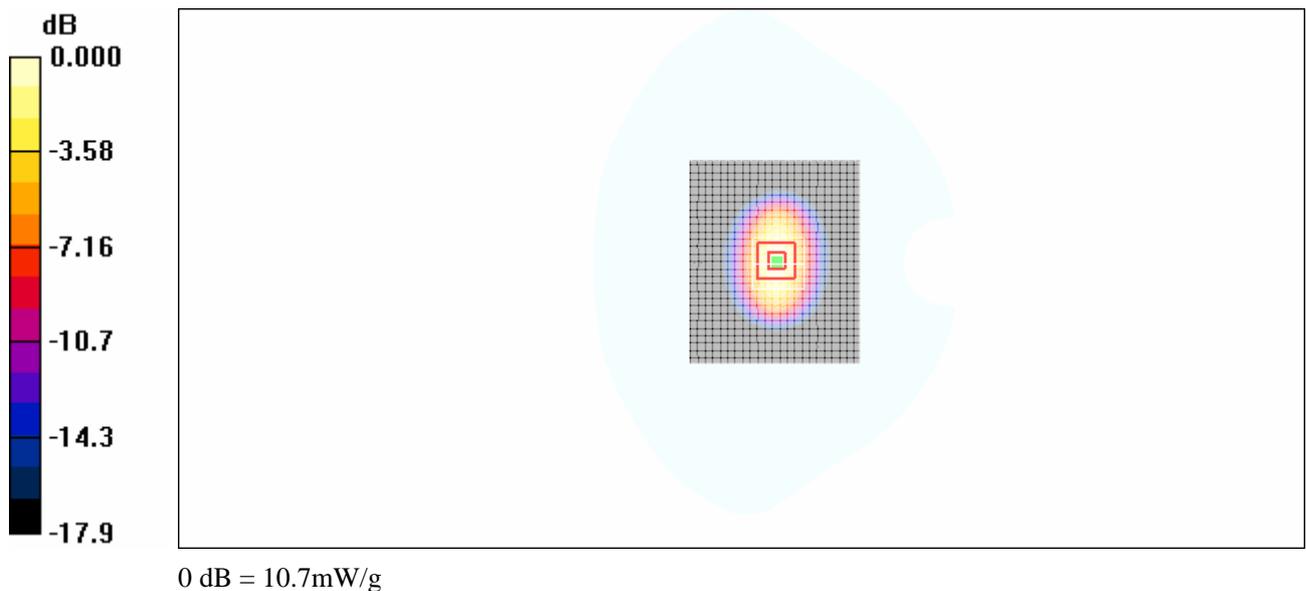


Figure 100 System Performance Check 1900MHz 250mW

TA Technology (Shanghai) Co., Ltd. Test Report

No. RZA2008-0528FCC

Page 127 of 155

ANNEX E: PROBE CALIBRATION CERTIFICATE

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **ATL (Auden)**

Certificate No: **ET3-1531_Jan08**

CALIBRATION CERTIFICATE

Object: **ET3DV6 - SN:1531**

Calibration procedure(s): **QA CAL-01.v6 and QA CAL-12.v5
Calibration procedure for dosimetric E-field probes**

Calibration date: **January 29, 2008**

Condition of the calibrated item: **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&PE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Power sensor E4412A	MY41495277	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Power sensor E4412A	MY41498087	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Reference 3 dB Attenuator	SN: S5054 (3c)	8-Aug-07 (METAS, No. 217-00719)	Aug-08
Reference 20 dB Attenuator	SN: S5088 (20b)	29-Mar-07 (METAS, No. 217-00671)	Mar-08
Reference 30 dB Attenuator	SN: S5129 (30b)	8-Aug-07 (METAS, No. 217-00720)	Aug-08
Reference Probe ES3DV2	SN: 3013	2-Jan-08 (SPEAG, No. ES3-3013_Jan08)	Jan-09
DAE4	SN: 654	20-Apr-07 (SPEAG, No. DAE4-654_Apr07)	Apr-08

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Oct 07)	In house check: Oct-09
Network Analyzer HP 8753E	US37300565	18-Oct-01 (SPEAG, in house check Oct-07)	In house check: Oct-08

Calibrated by:	Name	Function	Signature
	Kaja Pokovic	Technical Manager	
Approved by:	Niels Kuster	Quality Manager	

Issued: January 29, 2008

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ET3-1531_Jan08

Page 1 of 9

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
Polarization ϕ	ϕ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}:** Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not effect the E²-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP_{x,y,z}:** DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

ET3DV6 SN:1531

January 29, 2008

Probe ET3DV6

SN:1531

Manufactured:	July 15, 2000
Last calibrated:	January 22, 2007
Recalibrated:	January 29, 2008

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

