

# Appendix D

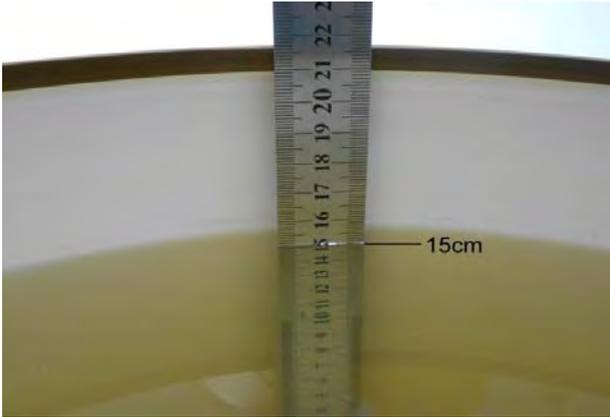
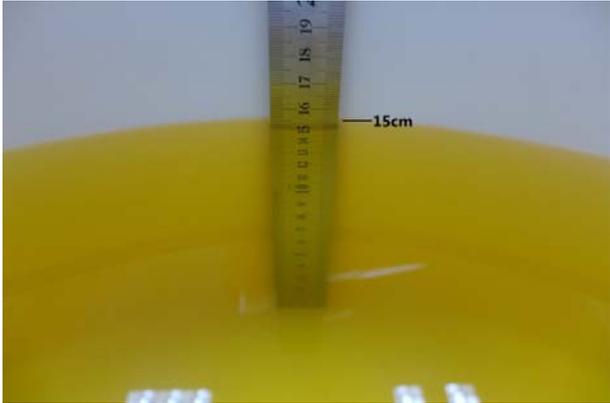
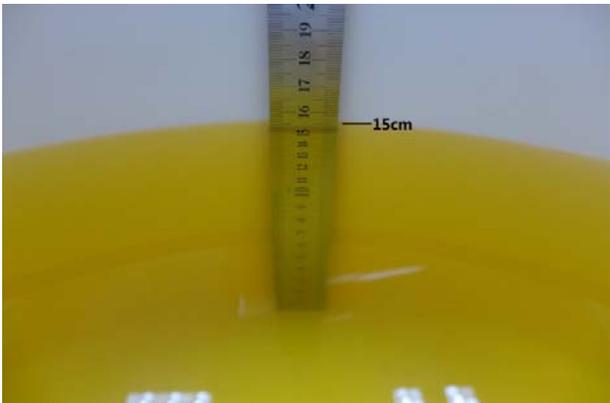
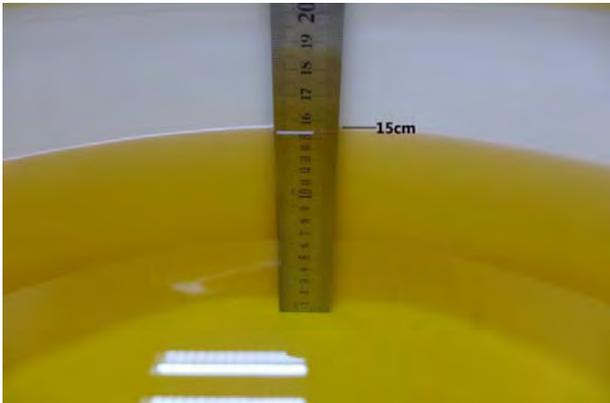
## Photographs

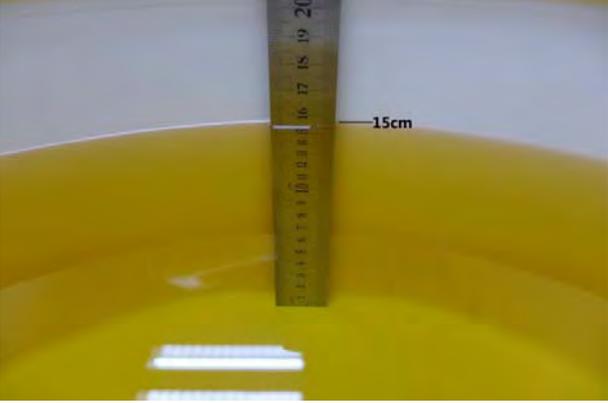
1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System



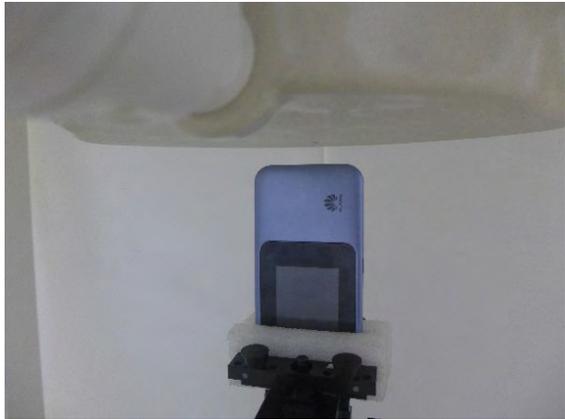
## 2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Body 835	Photo 2: Tissue Simulant Liquid for Body 1750
	
Photo 3: Tissue Simulant Liquid for Body 1900	Photo 4: Tissue Simulant Liquid for Body 2450
	

<b>Photo 5: Tissue Simulant Liquid for Body 2600</b>	<b>N/A</b>
	<p>N/A</p>

### 3. Photographs of EUT test position

<p>Photo 6: Front side 10mm</p>	<p>Photo 7: Back side 10mm</p>
	
<p>Photo 8: Front side 16mm</p>	<p>Photo 9: Back side 16mm</p>
	
<p>Photo 10: Front side 22mm</p>	<p>Photo 11: Back side 22mm</p>
	

<p><b>Photo 12: Right side 10mm</b></p>	<p><b>Photo 13: Right side 20mm</b></p>
	
<p><b>Photo 14: Right side 24mm</b></p>	<p><b>Photo 15: Top side 10mm</b></p>
	
<p><b>Photo 16: Bottom side 10mm</b></p>	<p><b>N/A</b></p>
	<p><b>N/A</b></p>

#### 4. EUT Constructional Details

