

ET3DV6 SN:1531

January 29, 2008

# Probe ET3DV6

## SN:1531

Manufactured:	July 15, 2000
Last calibrated:	January 22, 2007
Recalibrated:	January 29, 2008

Calibrated for DASY Systems


(Note: non-compatible with DASY2 system!)



ET3DV6 SN:1531

January 29, 2008

### Frequency Response of E-Field (TEM-Cell: If1110 EXX, Waveguide: R22)



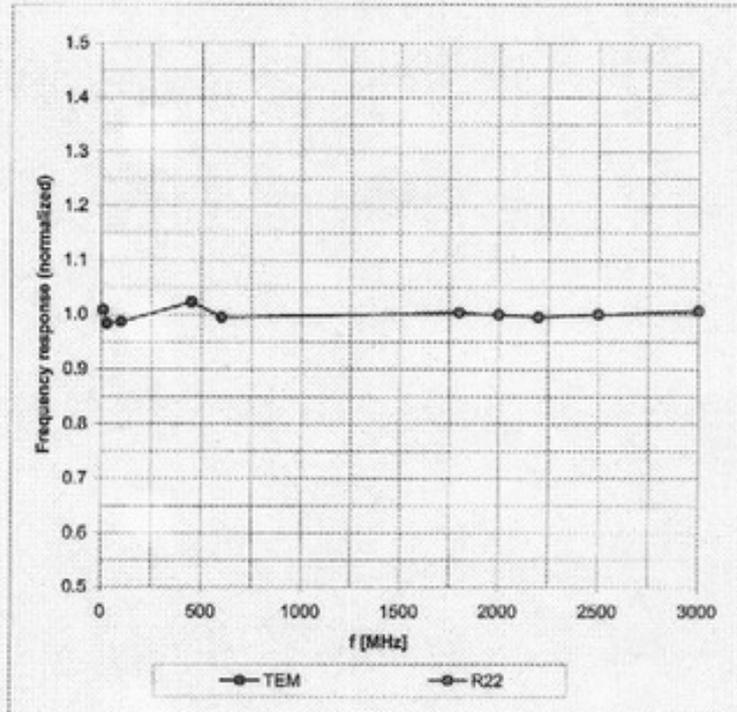


Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

ET3DV6 SN:1531

January 29, 2008

Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$

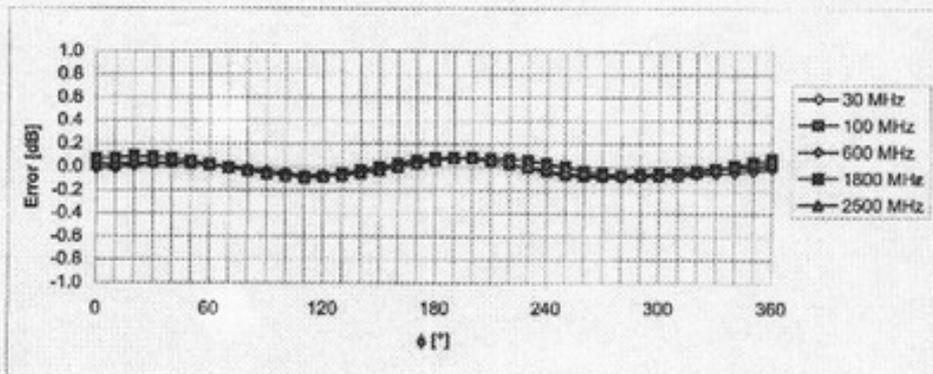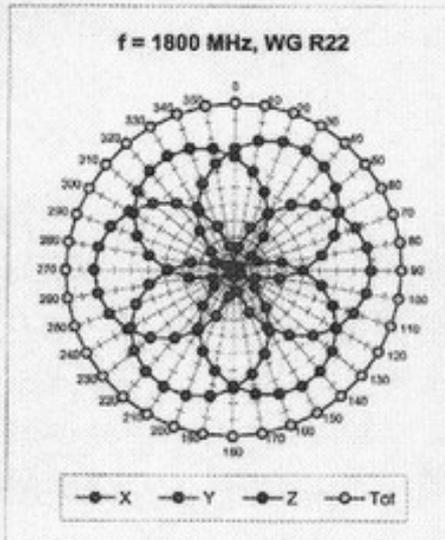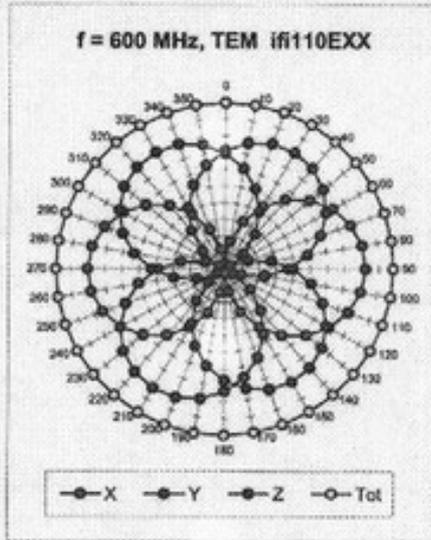


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

ET3DV6 SN:1531

January 29, 2008

**Dynamic Range  $f(\text{SAR}_{\text{head}})$**   
(Waveguide R22,  $f = 1800$  MHz)

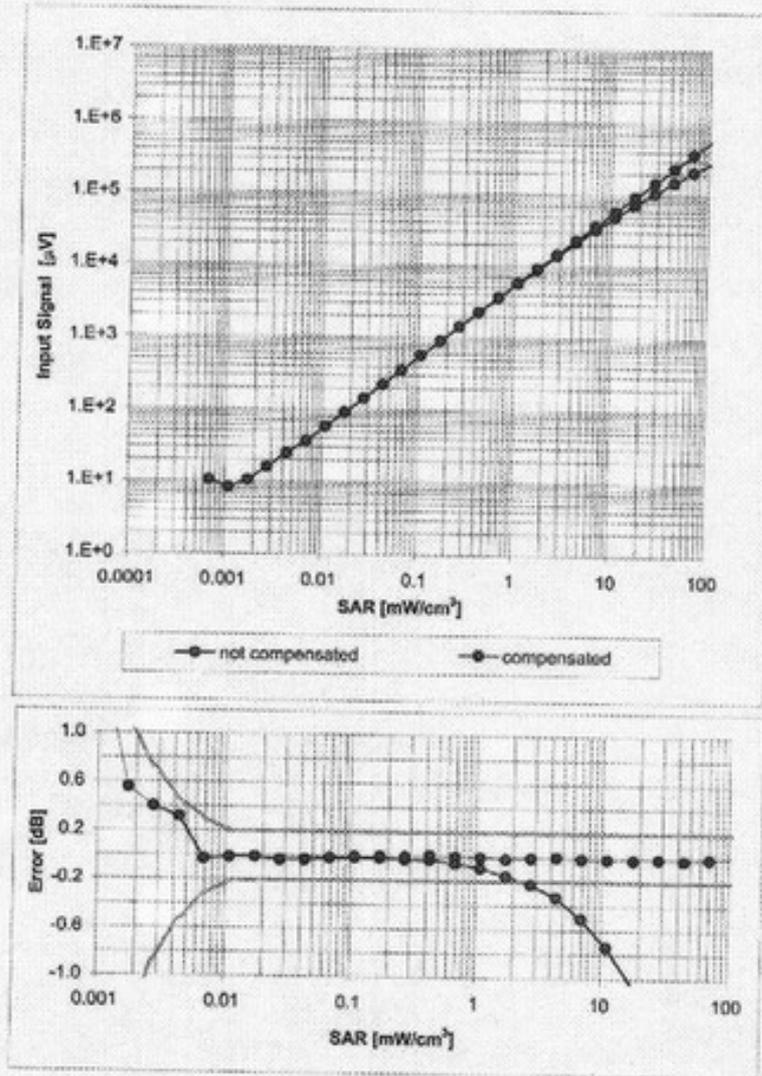


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

ET3DV6 SN:1531

January 29, 2008

### Conversion Factor Assessment

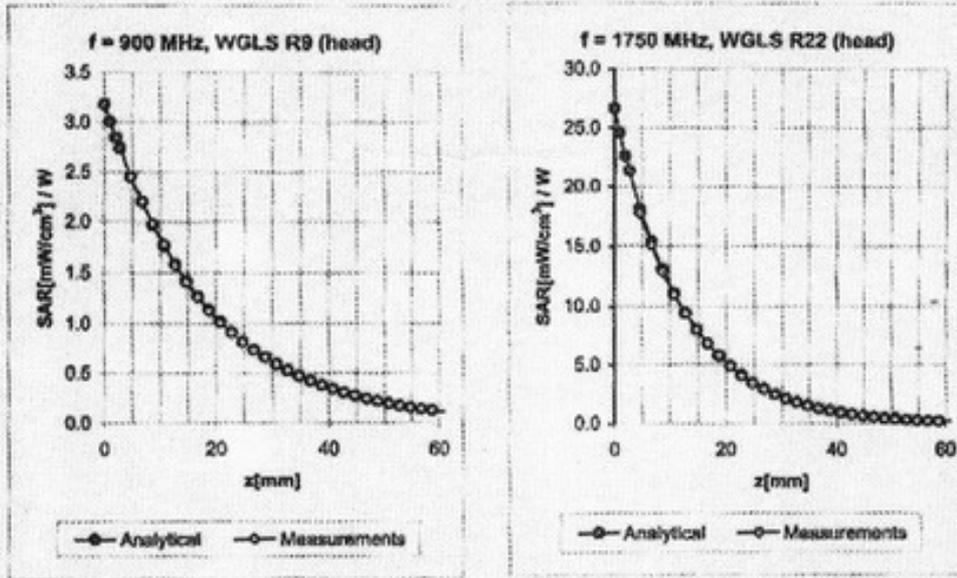

f [MHz]	Validity [MHz] <sup>©</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.27	2.89	6.85 ± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.52	2.56	5.42 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.49	2.89	5.15 ± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.35	2.82	6.52 ± 11.0% (k=2)
1750	± 50 / ± 100	Body	53.4 ± 5%	1.49 ± 5%	0.56	2.68	4.97 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.88	2.07	4.64 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.66	2.16	4.10 ± 11.8% (k=2)


<sup>©</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

ET3DV6 SN:1531

January 29, 2008

### Deviation from Isotropy in HSL

Error ( $\phi$ ,  $\theta$ ),  $f = 900$  MHz

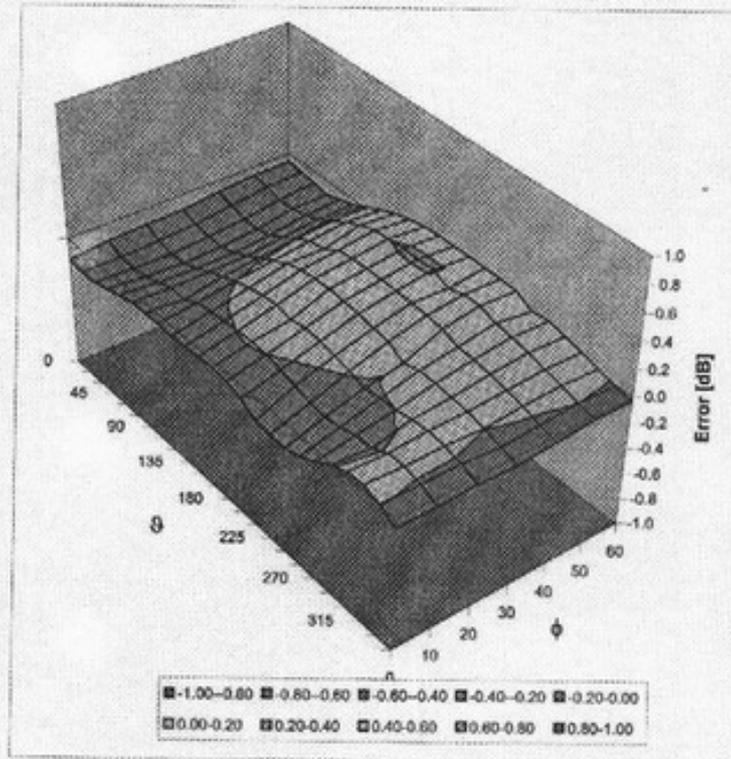

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )

**TA Technology (Shanghai) Co., Ltd.**  
**Test Report**

No. RZA2008-1054FCC

Page 83of 95

**ANNEX F : D835V2 DIPOLE CALIBRATION CERTIFICATE**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **TMC China**

Certificate No: **D835V2-443\_Dec07**

**CALIBRATION CERTIFICATE**

Object	<b>D835V2-SN: 443</b>
Calibration procedure(s)	<b>QA CAL-05.v6 Calibration procedure for dipole validation kits</b>
Calibration date:	<b>December 9, 2007</b>
Condition of the calibrated item	<b>In Tolerance</b>

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements(SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted at an environment temperature (22±3)°C and humidity<70%

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Data (Calibrated by, Certification NO.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	13-Sep-07 (METAS, NO. 217-00608)	Sep-08
Power sensor 8481A	US37292783	13-Sep-07 (METAS, NO. 217-00608)	Sep-08
Reference 20 dB Attenuator	SN:5086 (20g )	12-Jul-07 (METAS, NO. 217-00591)	Jul-08
Reference 10 dB Attenuator	SN:5047_2 (10r)	12-Jul-07 (METAS, NO. 217-00591)	Jul-08
DAE4	SN:601	30-Jan-07 (SPEAG, NO.DAE4-601_Jan07)	Jan-08
Reference Probe ET3DVB (HF)	SN: 1507	19-Sep-07 (SPEAG, NO. ET3-1507_Sep07)	Sep-08
Secondary Standards	ID#	Check Data (in house)	Scheduled Calibration
Power sensor HP 8481A	MY41092317	18-Oct-02(SPEAG, in house check Oct-07)	In house check: Oct-09
RF generator Agilent E4421B	MY41000878	11-May-05(SPEAG, in house check Nov-07)	In house check: Nov-09
Network Analyzer HP 8753E	US37390585S4208	18-Oct-01(SPEAG, in house check Oct-07)	In house check: Oct-08

	Name	Function	Signature
Calibrated by:	<b>Marcel Fehr</b>	Laboratory Technician	
Approved by:	<b>Katja Pokovic</b>	Technical Director	

Issued: **December 10, 2007**

This calibration certificate shall not be reported except in full without written approval of the laboratory.

# TA Technology (Shanghai) Co., Ltd. Test Report

No. RZA2008-1054FCC

Page 84 of 95

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8904 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

- DASY4 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature during test	(21.2 ± 0.2) °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.43 mW / g
SAR normalized	normalized to 1W	9.72 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	9.70 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.56 mW / g
SAR normalized	normalized to 1W	6.24 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	6.31 mW / g ± 16.5 % (k=2)

<sup>1</sup>Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"