

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY4	V4.7
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom V4.9	
<b>Distance Dipole Center - TSL</b>	15 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	835 MHz $\pm$ 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	<b>Temperature</b>	<b>Permittivity</b>	<b>Conductivity</b>
<b>Nominal Head TSL parameters</b>	22.0 °C	41.5	0.90 mho/m
<b>Measured Head TSL parameters</b>	(22.0 $\pm$ 0.2) °C	41.4 $\pm$ 6 %	0.91 mho/m $\pm$ 6 %
<b>Head TSL temperature during test</b>	(21.5 $\pm$ 0.2) °C	----	----

### SAR result with Head TSL

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	2.43 mW / g
SAR normalized	normalized to 1W	9.72 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	<b>9.65 mW /g <math>\pm</math> 17.0 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	1.57 mW / g
SAR normalized	normalized to 1W	6.28 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	<b>6.25 mW /g <math>\pm</math> 16.5 % (k=2)</b>

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

### Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Body TSL parameters</b>	22.0 °C	55.2	0.97 mho/m
<b>Measured Body TSL parameters</b>	(22.0 ± 0.2) °C	54.9 ± 6 %	0.98 mho/m ± 6 %
<b>Body TSL temperature during test</b>	(21.5 ± 0.2) °C	----	----

### SAR result with Body TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.46 mW / g
SAR normalized	normalized to 1W	9.84 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	<b>9.75 mW /g ± 17.0 % (k=2)</b>

SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.60 mW / g
SAR normalized	normalized to 1W	6.40 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	<b>6.36 mW /g ± 16.5 % (k=2)</b>

<sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.1 $\Omega$ -3.5 j $\Omega$
Return Loss	- 25.5dB

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.6 $\Omega$ - 5.3 j $\Omega$
Return Loss	-25.8dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	2.572 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 3, 2001

**DASY4 Validation Report for Head TSL**

Date/Time: 25.10.2009 10:26:37

Test laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; serial: D835V2-SN: 443**

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Head 835 MHz;

Medium parameters used:  $f=835$  MHz;  $\sigma=0.91$  mho/m;  $\epsilon_r=41.4$ ;  $\rho=1000$ kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6-SN1507(HF); ConvF(6.01,6.01,6.01); Calibrated: 17.10.2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.1\_2009
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA;
- Measurement SW: DASY, V4.7 Build 53; Post processing SW: SEMCAD, V1.8 Build 172


**Pin = 250 mW; d = 15 mm/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.5 V/m; Power Drift = 0.048 dB

Peak SAR (extrapolated) = 3.76 W/kg


**SAR(1 g) = 2.43 mW/g; SAR(10 g) = 1.57 mW/g**

Maximum value of SAR (measured) = 2.75 mW/g

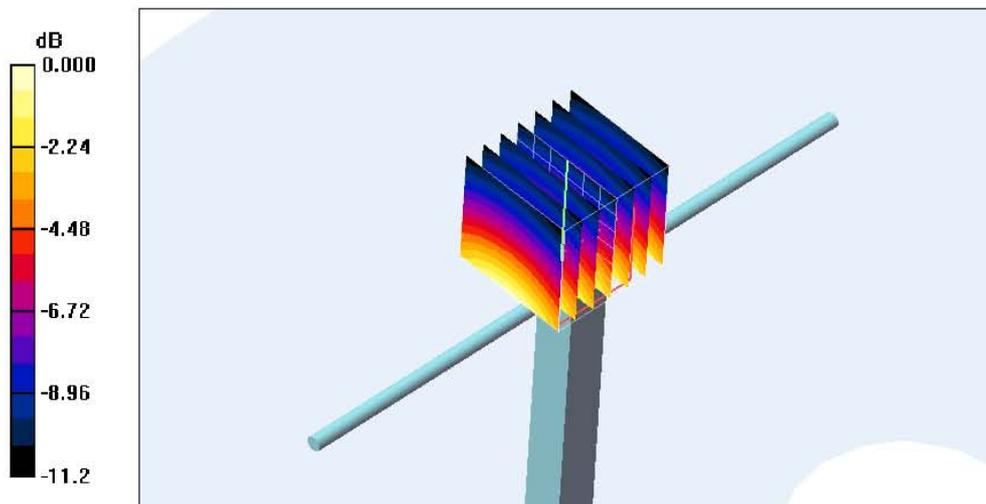

0 dB = 2.75mW/g

Impedance measurement Plot for Head TSL

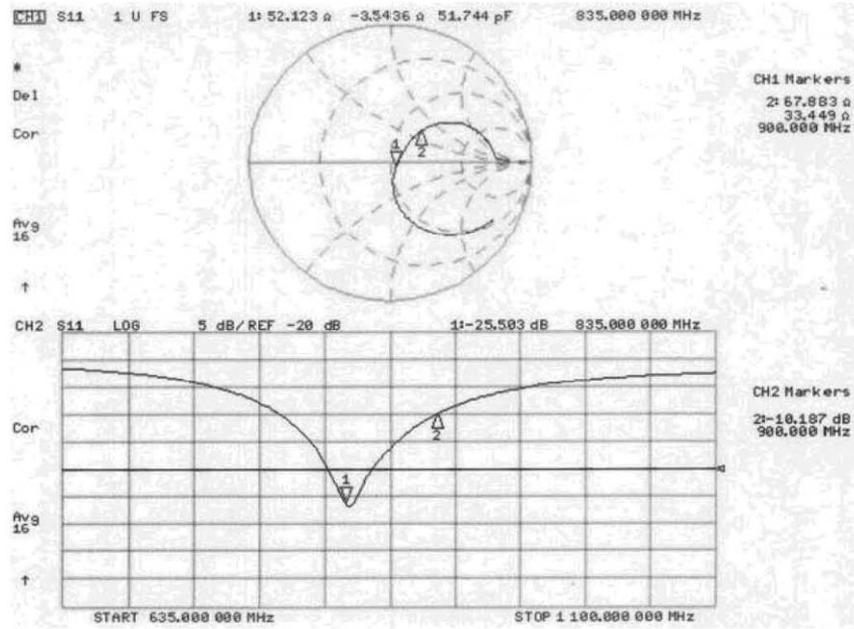

**DASY4 Validation Report for Body TSL**

Date/Time: 25.10.2009 14:47:03

Test laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; serial: D835V2-SN: 443**

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: Body 835 MHz;

Medium parameters used:  $f=835$  MHz;  $\sigma=0.98$  mho/m;  $\epsilon_r=54.9$ ;  $\rho= 1000\text{kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6-SN1507(HF); ConvF(5.75,5.75,5.75); Calibrated: 17.10.2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.1\_2009
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA;
- Measurement SW: DASY, V4.7 Build 53; Post processing SW: SEMCAD, V1.8 Build 172


**Pin = 250 mW; d = 15 mm/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.9 V/m; Power Drift = 0.061 dB


Peak SAR (extrapolated) = 3.80 W/kg

**SAR(1 g) = 2.46 mW/g; SAR(10 g) = 1.60 mW/g**

Maximum value of SAR (measured) = 2.78 mW/g

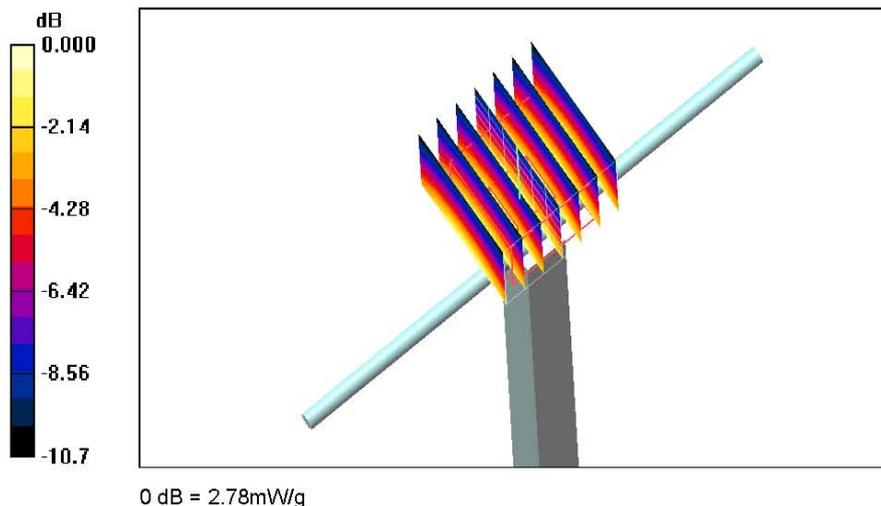

Impedance measurement Plot for Body TSL

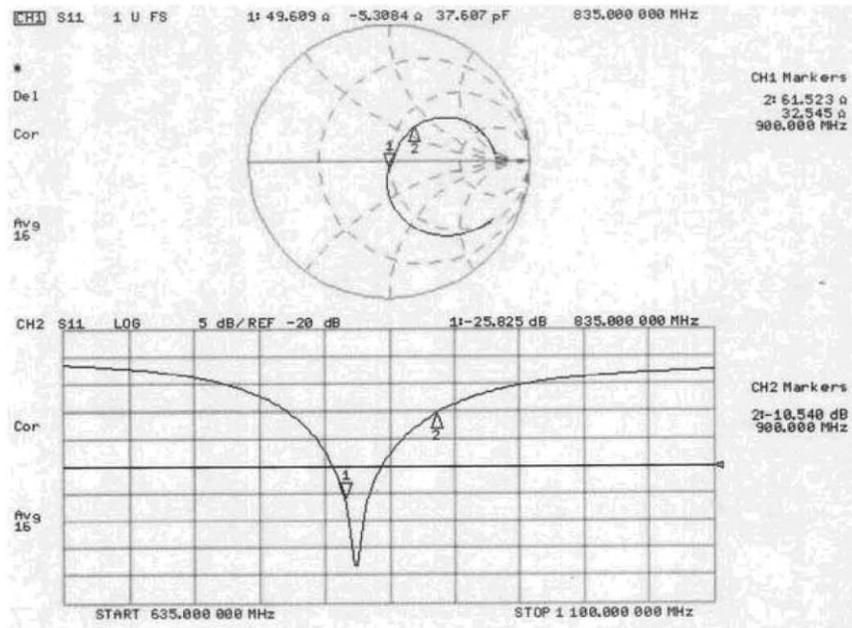

### 1900 MHz Dipole Calibration Certificate

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **TMC China**

Certificate No: **D1900V2-541\_Oct09**

CALIBRATION CERTIFICATE																																															
Object	D1900V2-SN: 541																																														
Calibration procedure(s)	QA CAL-05.v6 Calibration procedure for dipole validation kits																																														
Calibration date:	October 26, 2009																																														
Condition of the calibrated item	In Tolerance																																														
<p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted at an environment temperature (22±3)°C and humidity&lt;70%</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID#</th> <th>Cal Data (Calibrated by, Certification NO.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter EPM-442A</td> <td>GB37480704</td> <td>01-Oct-09 (METAS, NO. 217-00608)</td> <td>Oct-10</td> </tr> <tr> <td>Power sensor 8481A</td> <td>US37292783</td> <td>01-Oct-09 (METAS, NO. 217-00608)</td> <td>Oct-10</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN:5086 (20g )</td> <td>08-Aug-09 (METAS, NO. 217-00591)</td> <td>Aug-10</td> </tr> <tr> <td>Reference 10 dB Attenuator</td> <td>SN:5047_2 (10r)</td> <td>08-Aug-09 (METAS, NO. 217-00591)</td> <td>Aug-10</td> </tr> <tr> <td>DAE4</td> <td>SN:601</td> <td>28-Jan-09 (SPEAG, NO.DAE4-601_Jan09)</td> <td>Jan-10</td> </tr> <tr> <td>Reference Probe ET3DV6 (HF)</td> <td>SN: 1507</td> <td>17-Oct-09 (SPEAG, NO. ET3-1507_Oct09)</td> <td>Oct-10</td> </tr> <tr> <th>Secondary Standards</th> <th>ID#</th> <th>Check Data (in house)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Power sensor HP 8481A</td> <td>MY41092317</td> <td>18-Oct-02(SPEAG, in house check Oct-09)</td> <td>In house check: Oct-10</td> </tr> <tr> <td>RF generator Aglient E4421B</td> <td>MY41000676</td> <td>11-May-05(SPEAG, in house check Nov-07)</td> <td>In house check: Nov -09</td> </tr> <tr> <td>Network Analyzer HP 8753E</td> <td>US37390585S4206</td> <td>18-Oct-01(SPEAG, in house check Oct-09)</td> <td>In house check: Oct -10</td> </tr> </tbody> </table>				Primary Standards	ID#	Cal Data (Calibrated by, Certification NO.)	Scheduled Calibration	Power meter EPM-442A	GB37480704	01-Oct-09 (METAS, NO. 217-00608)	Oct-10	Power sensor 8481A	US37292783	01-Oct-09 (METAS, NO. 217-00608)	Oct-10	Reference 20 dB Attenuator	SN:5086 (20g )	08-Aug-09 (METAS, NO. 217-00591)	Aug-10	Reference 10 dB Attenuator	SN:5047_2 (10r)	08-Aug-09 (METAS, NO. 217-00591)	Aug-10	DAE4	SN:601	28-Jan-09 (SPEAG, NO.DAE4-601_Jan09)	Jan-10	Reference Probe ET3DV6 (HF)	SN: 1507	17-Oct-09 (SPEAG, NO. ET3-1507_Oct09)	Oct-10	Secondary Standards	ID#	Check Data (in house)	Scheduled Calibration	Power sensor HP 8481A	MY41092317	18-Oct-02(SPEAG, in house check Oct-09)	In house check: Oct-10	RF generator Aglient E4421B	MY41000676	11-May-05(SPEAG, in house check Nov-07)	In house check: Nov -09	Network Analyzer HP 8753E	US37390585S4206	18-Oct-01(SPEAG, in house check Oct-09)	In house check: Oct -10
Primary Standards	ID#	Cal Data (Calibrated by, Certification NO.)	Scheduled Calibration																																												
Power meter EPM-442A	GB37480704	01-Oct-09 (METAS, NO. 217-00608)	Oct-10																																												
Power sensor 8481A	US37292783	01-Oct-09 (METAS, NO. 217-00608)	Oct-10																																												
Reference 20 dB Attenuator	SN:5086 (20g )	08-Aug-09 (METAS, NO. 217-00591)	Aug-10																																												
Reference 10 dB Attenuator	SN:5047_2 (10r)	08-Aug-09 (METAS, NO. 217-00591)	Aug-10																																												
DAE4	SN:601	28-Jan-09 (SPEAG, NO.DAE4-601_Jan09)	Jan-10																																												
Reference Probe ET3DV6 (HF)	SN: 1507	17-Oct-09 (SPEAG, NO. ET3-1507_Oct09)	Oct-10																																												
Secondary Standards	ID#	Check Data (in house)	Scheduled Calibration																																												
Power sensor HP 8481A	MY41092317	18-Oct-02(SPEAG, in house check Oct-09)	In house check: Oct-10																																												
RF generator Aglient E4421B	MY41000676	11-May-05(SPEAG, in house check Nov-07)	In house check: Nov -09																																												
Network Analyzer HP 8753E	US37390585S4206	18-Oct-01(SPEAG, in house check Oct-09)	In house check: Oct -10																																												
	Name	Function	Signature																																												
Calibrated by:	Marcel Fehr	Laboratory Technician																																													
Approved by:	Katja Pokovic	Technical Director																																													
Issued: October 26, 2009																																															
This calibration certificate shall not be reported except in full without written approval of the laboratory.																																															

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

**Glossary:**

TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY4 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY4	V4.7
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom V4.9	
<b>Distance Dipole Center - TSL</b>	10 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	1900 MHz $\pm$ 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	40.0	1.40 mho/m
<b>Measured Head TSL parameters</b>	(22.0 $\pm$ 0.2) °C	39.7 $\pm$ 6 %	1.41 mho/m $\pm$ 6 %
<b>Head TSL temperature during test</b>	(21.5 $\pm$ 0.2) °C	----	----

### SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.97 mW / g
SAR normalized	normalized to 1W	39.9 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	<b>39.6 mW /g <math>\pm</math> 17.0 % (k=2)</b>

SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.12 mW / g
SAR normalized	normalized to 1W	20.5 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	<b>20.4 mW /g <math>\pm</math> 16.5 % (k=2)</b>

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

### Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Body TSL parameters</b>	22.0 °C	53.3	1.52 mho/m
<b>Measured Body TSL parameters</b>	(22.0 ± 0.2) °C	52.3 ± 6 %	1.51 mho/m ± 6 %
<b>Body TSL temperature during test</b>	(21.5 ± 0.2) °C	----	----

### SAR result with Body TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.4 mW / g
SAR normalized	normalized to 1W	41.6 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	<b>41.3 mW /g ± 17.0 % (k=2)</b>

SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.29 mW / g
SAR normalized	normalized to 1W	21.2 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	<b>21.1 mW /g ± 16.5 % (k=2)</b>

<sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	$54.4\Omega + 5.8j\Omega$
Return Loss	- 23.0dB

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	$47.6\Omega + 7.0j\Omega$
Return Loss	- 22.4dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.883 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 4, 2001