


To make the mobile emits maximum power; the output power of CMU200 would be adjusted to minimum power with the sensitivity of the mobile station to build steady connection with mobile station. The power level control parameter in the CMU200 is "0", it means "all up" and requires mobile station to emit with maximum power.

4.2 SAR Measurement Set-up

These measurements were performed with the automated near-field scanning system DASY4 Professional from Schmid & Partner Engineering AG (SPEAG). The system is based on a high precision robot (working range greater than 0.9m) which positions the probes with a positional repeatability of better than $\pm 0.02\text{mm}$. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines (length =300mm) to the data acquisition unit.

A cell controller system contains the power supply, robot controller, teaches pendant (Joystick), and remote control, is used to drive the robot motors. The PC consists of the Micron Pentium III 800 MHz computer with Windows 2000 system and SAR Measurement Software DASY4, A/D interface card, monitor, mouse, and keyboard. The Stäubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

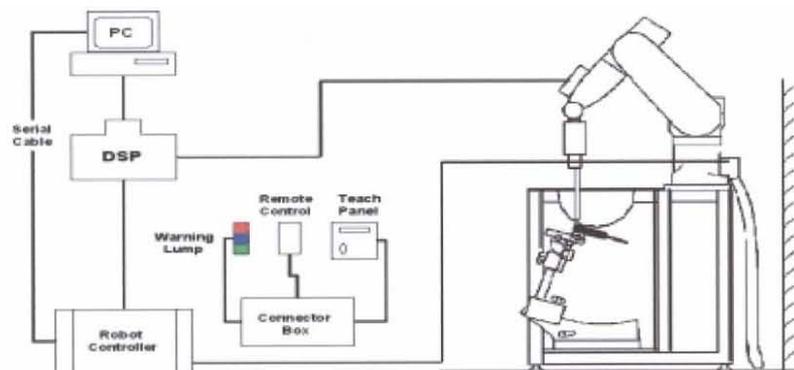

Picture 2: SAR Lab Test Measurement Set-up

The DAE consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer.


4.3 Dasy4 E-field Probe System

The SAR measurements were conducted with the dosimetric probe ET3DV6 (manufactured by

SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe has been calibrated according to the standard procedure with an accuracy of better than $\pm 10\%$. The spherical isotropy was evaluated and found to be better than $\pm 0.25\text{dB}$.

ET3DV6 Probe Specification

Construction	Symmetrical design with triangular core Built-in optical fiber for surface detection System(ET3DV6 only) Built-in shielding against static charges PEEK enclosure material(resistant to organic solvents, e.q., glycol)
Calibration	In air from 10 MHz to 2.5 GHz In brain and muscle simulating tissue at frequencies of 450MHz, 900MHz and 1.8GHz (accuracy $\pm 8\%$) Calibration for other liquids and frequencies upon request
Frequency	10 MHz to > 6 GHz; Linearity: $\pm 0.2\text{ dB}$ (30 MHz to 3 GHz)
Directivity	$\pm 0.2\text{ dB}$ in brain tissue (rotation around probe axis) $\pm 0.4\text{ dB}$ in brain tissue (rotation normal probe axis)
Dynamic Range	5u W/g to > 100mW/g; Linearity: $\pm 0.2\text{ dB}$
Surface Detection	$\pm 0.2\text{ mm}$ repeatability in air and clear liquids over diffuse reflecting surface(ET3DV6 only)
Dimensions	Overall length: 330mm Tip length: 16mm Body diameter: 12mm Tip diameter: 6.8mm Distance from probe tip to dipole centers: 2.7mm
Application	General dosimetry up to 3GHz Compliance tests of mobile phones Fast automatic scanning in arbitrary phantoms

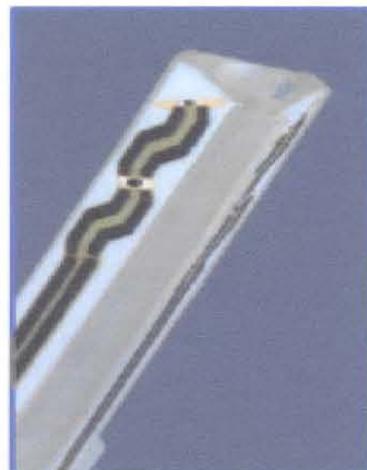

Picture 3: ET3DV6 E-field Probe



Picture4:ET3DV6 E-field probe

4.4 E-field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure with accuracy better than $\pm 10\%$. The spherical isotropy was evaluated and found to be better than $\pm 0.25\text{dB}$. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a wave guide above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

Where: Δt = Exposure time (30 seconds),

C = Heat capacity of tissue (brain or muscle),

ΔT = Temperature increase due to RF exposure.

Or

$$SAR = \frac{|E|^2 \sigma}{\rho}$$

Where: σ = Simulated tissue conductivity,

ρ = Tissue density (kg/m³).

Note: Please see Annex E to check the probe calibration certificate.



Picture 5: Device Holder

4.5 Other Test Equipment

4.5.1 Device Holder for Transmitters

In combination with the Generic Twin Phantom V3.0, the Mounting Device (POM) enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation points is the ear opening. The devices can be easily, accurately, and repeat ably positioned according to the FCC and CENELEC specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).

4.5.2 Phantom

The Generic Twin Phantom is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow all predefined phantom positions and measurement grids by the complete setup of manually teaching three points in the robot.

Shell Thickness 2±0.1 mm

Filling Volume Approx. 20 liters

Dimensions 810 x 1000 x 500 mm (H x L x W)

Available Special



Picture6:Generic Twin Phantom

4.6 Equivalent Tissues

The liquid used for the frequency range of 800-2000 MHz consisted of water, sugar, salt and Cellulose. The liquid has previously been proven to be suited for worst-case. The Table 4 shows the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the IEEE 1528.

Table 4. Composition of the Head Tissue Equivalent Matter

MIXTURE %	FREQUENCY 835MHz		
Water	41.45		
Sugar	56.0		
Salt	1.45		
Preventol	0.1		
Cellulose	1.0		
Dielectric Parameters Target Value	f=835MHz	$\epsilon=41.5$	$\sigma=0.90$
MIXTURE %	FREQUENCY 1900MHz		
Water	55.242		
Glycol monobutyl	44.452		
Salt	0.306		
Dielectric Parameters Target Value	f=1900MHz	$\epsilon=40.0$	$\sigma=1.40$

Table 5. Composition of the Body Tissue Equivalent Matter

MIXTURE %	FREQUENCY 835MHz		
Water	52.5		
Sugar	45.0		
Salt	1.4		
Preventol	0.1		
Cellulose	1.0		
Dielectric Parameters Target Value	f=835MHz	$\epsilon=55.2$	$\sigma=0.97$
MIXTURE %	FREQUENCY 1900MHz		
Water	69.91		
Glycol monobutyl	29.96		
Salt	0.13		
Dielectric Parameters Target Value	f=1900MHz	$\epsilon=53.3$	$\sigma=1.52$

4.7 System Specifications

4.7.1 Robotic System Specifications

Specifications

Positioner: Stäubli Unimation Corp. Robot Model: RX90L

Repeatability: ± 0.02 mm

No. of Axis: 6

Data Acquisition Electronic (DAE) System

Cell Controller

Processor: Pentium III

Clock Speed: 800 MHz

Operating System: Windows 2000

Data Converter

Features: Signal Amplifier, multiplexer, A/D converter, and control logic

Software: DASY4 software

Connecting Lines: Optical downlink for data and status info.

Optical uplink for commands and clock

5 CHARACTERISTICS OF THE TEST

5.1 Applicable Limit Regulations

EN 50360–2001: Product standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones.

It specifies the maximum exposure limit of **2.0 W/kg** as averaged over any 10 gram of tissue for portable devices being used within 20 cm of the user in the uncontrolled environment.

ANSI C95.1–1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz.

It specifies the maximum exposure limit of **1.6 W/kg** as averaged over any 1 gram of tissue for portable devices being used within 20 cm of the user in the uncontrolled environment.

5.2 Applicable Measurement Standards

EN 50361–2001: Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones.

IEEE 1528–2003: Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques.

IEC 62209-1: Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures –Part 1: Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)

OET Bulletin 65 (Edition 97-01) and Supplement C(Edition 01-01): Additional Information for

Evaluating Compliance of Mobile and Portable Devices with FCC Limits.

They specify the measurement method for demonstration of compliance with the SAR limits for such equipments.

6 LABORATORY ENVIRONMENT

Table 6: The Ambient Conditions during EMF Test

Temperature	Min. = 15 °C, Max. = 30 °C
Relative humidity	Min. = 30%, Max. = 70%
Ground system resistance	< 0.5 Ω
Ambient noise is checked and found very low and in compliance with requirement of standards.	
Reflection of surrounding objects is minimized and in compliance with requirement of standards.	

7 CONDUCTED OUTPUT POWER MEASUREMENT

7.1 Summary

During the process of testing, the EUT was controlled via Rhode & Schwarz Digital Radio Communication tester (CMU-200) to ensure the maximum power transmission and proper modulation. This result contains conducted output power and ERP for the EUT. In all cases, the measured peak output power should be greater and within 5% than EMI measurement.

7.2 Conducted Power

7.2.1 Measurement Methods

The EUT was set up for the maximum output power. The channel power was measured with Agilent Spectrum Analyzer E4440A. These measurements were done at 3 channels, 1013, 384 and 777 before SAR test and after SAR test.

7.2.2 Measurement result

Table 7: Conducted Power Measurement Results

CDMA 835	Conducted Power		
	Channel 1013	Channel 384	Channel 777
Before Test (dBm)	24.2	24.1	24.1
After Test (dBm)	24.1	24.0	24.1
CDMA 1900	Conducted Power		
	Channel 1175	Channel 600	Channel 25
Before Test (dBm)	24.0	24.0	24.3
After Test (dBm)	24.1	23.9	24.2

7.2.3 Power Drift

To control the output power stability during the SAR test, DASY4 system calculates the power drift by measuring the E-field at the same location at the beginning and at the end of the measurement for each test position. These drift values can be found in Table 11 to Table 12 labeled as: (Power Drift [dB]). This ensures that the power drift during one measurement is within 5%.

8 TEST RESULTS

8.1 Dielectric Performance

Table 8: Dielectric Performance of Head Tissue Simulating Liquid

Measurement is made at temperature 24.5 °C and relative humidity 40%. Liquid temperature during the test: 24.0°C			
/	Frequency	Permittivity ϵ	Conductivity σ (S/m)
Target value	835 MHz	41.5	0.90
	1900 MHz	40.0	1.40
Measurement value (Average of 10 tests)	835 MHz	40.1	0.928
	1900 MHz	39.6	1.37

Table 9: Dielectric Performance of Body Tissue Simulating Liquid

Measurement is made at temperature 24.5 °C and relative humidity 40%. Liquid temperature during the test: 24.0°C			
/	Frequency	Permittivity ϵ	Conductivity σ (S/m)
Target value	835 MHz	55.2	0.97
	1900 MHz	53.3	1.52
Measurement value (Average of 10 tests)	835 MHz	56.0	0.977
	1900 MHz	52.1	1.53

8.2 System Validation

Table 10: System Validation

Measurement is made at temperature 24.5 °C, relative humidity 40%, input power 250 mW. Liquid temperature during the test: 24.0°C					
Liquid parameters		Frequency	Permittivity ϵ		Conductivity σ (S/m)
		835 MHz	40.1		0.928
		1900 MHz	39.6		1.37
Verification results	Frequency	Target value (W/kg)		Measurement value (W/kg)	
		10 g Average	1 g Average	10 g Average	1 g Average
	835 MHz	1.55	2.375	1.62	2.48
1900 MHz	5.125	9.925	5.27	9.91	

Note: Target Values used are one fourth of those in IEEE Std 1528-2003 (feeding power is normalized to 1 Watt), i.e. 250 mW is used as feeding power to the validation dipole (SPEAG using).

8.3 Summary of Measurement Results

Table 11: SAR Values (Head, 835 MHz Band)

Limit of SAR (W/kg)	10 g Average	1 g Average	Power Drift (dB)
	2.0	1.6	
Test Case	Measurement Result (W/kg)		
	10 g Average	1 g Average	
Left hand, Touch cheek, Top frequency(See Fig.1)	0.178	0.351	-0.200
Left hand, Touch cheek, Mid frequency(See Fig.3)	0.154	0.306	-0.200
Left hand, Touch cheek, Bottom frequency(See Fig.5)	0.178	0.359	-0.200
Left hand, Tilt 15 Degree, Top frequency(See Fig.7)	0.052	0.073	-0.108
Left hand, Tilt 15 Degree, Mid frequency(See Fig.9)	0.049	0.067	-0.085
Left hand, Tilt 15 Degree, Bottom frequency(See Fig.11)	0.059	0.082	-0.188
Right hand, Touch cheek, Top frequency(See Fig.13)	0.383	0.619	-0.200
Right hand, Touch cheek, Mid frequency(See Fig.15)	0.337	0.540	0.003
Right hand, Touch cheek, Bottom frequency(See Fig.17)	0.416	0.658	-0.200
Right hand, Tilt 15 Degree, Top frequency(See Fig.19)	0.073	0.100	0.198
Right hand, Tilt 15 Degree, Mid frequency(See Fig.21)	0.070	0.098	0.200
Right hand, Tilt 15 Degree, Bottom frequency(See Fig.23)	0.099	0.135	-0.167

Table 12: SAR Values (Body, 835 MHz Band)

Limit of SAR (W/kg)	10 g Average	1 g Average	Power Drift (dB)
	2.0	1.6	
Test Case	Measurement Result (W/kg)		
	10 g Average	1 g Average	
Body, Towards Ground, Top frequency(See Fig.25)	0.267	0.404	-0.118
Body, Towards Ground, Mid frequency(See Fig.27)	0.260	0.387	-0.123
Body, Towards Ground, Bottom frequency(See Fig.29)	0.377	0.562	-0.200