

Appendix D

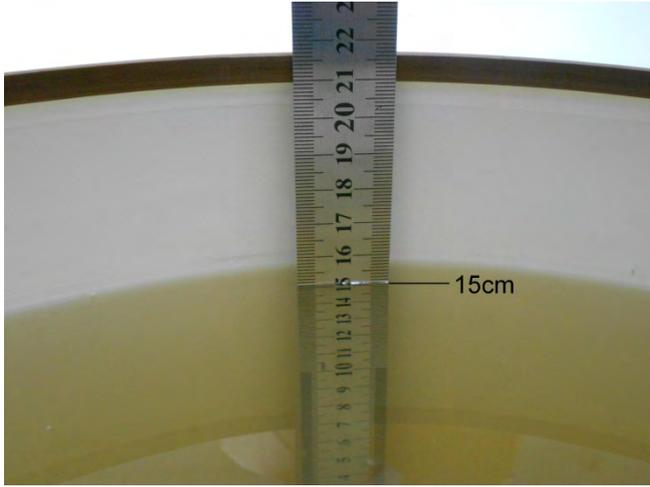
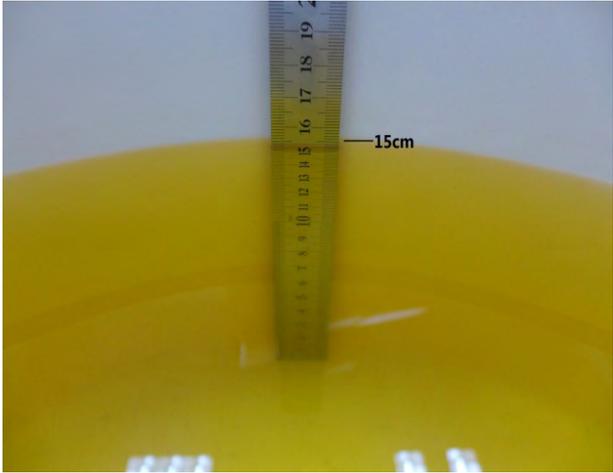
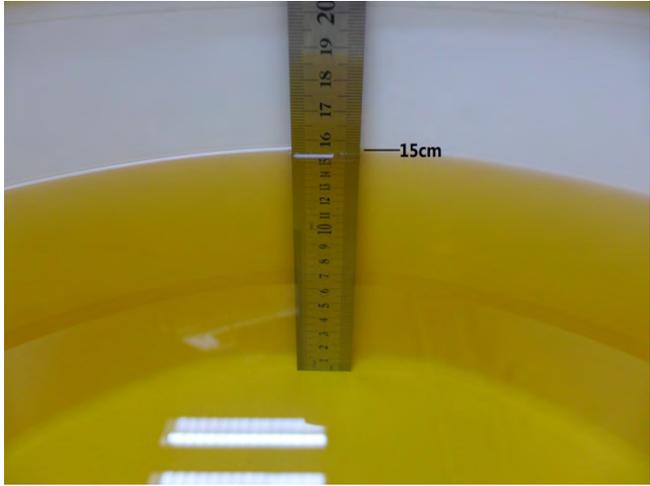
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

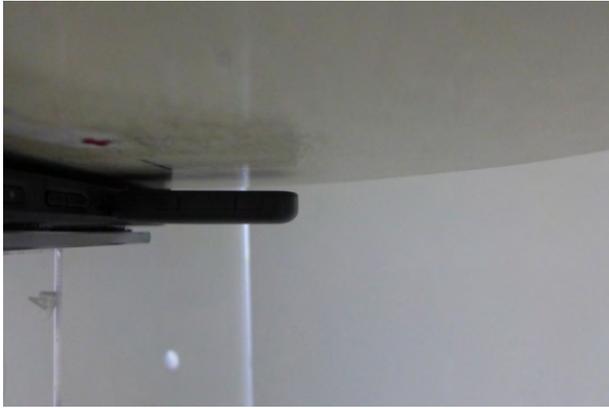
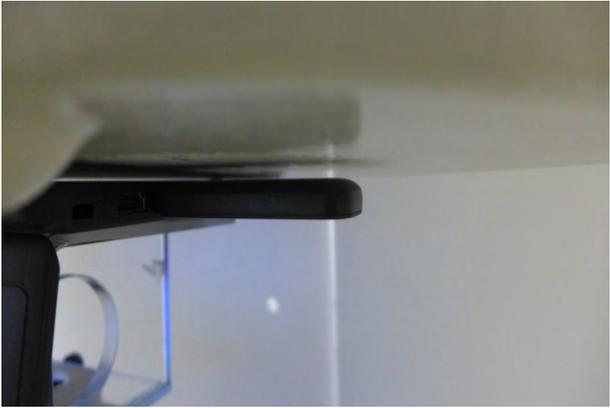
1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Body 835</p>	<p>Photo 2: Tissue Simulant Liquid for Body 1900</p>
	
<p>Photo 3: Tissue Simulant Liquid for Body 2600</p>	<p>N/A</p>
	<p>N/A</p>

3. Photographs of EUT test position

<p>Photo 4: Front side 5mm</p>	<p>Photo 5: Back side 5mm</p>
	
<p>Photo 6: Left side 5mm</p>	<p>Photo 7: Right side 5mm</p>
	
<p>Photo 8: Top side 5mm</p>	
	

4. EUT Constructional Details

Photo 9: Front View



Photo 10: Back View

