



## **Accredited testing laboratory**

**CNAS Registration number: L0310**

**Appendix to test report no. SYBH(Z-SAR)096082009  
Calibration data, Phantom certificate  
and detail information of the DASY5 System**



## Table of Content

1	Calibration report "Probe EX3DV4".....	3
2	Calibration report "1800 MHz System validation.....	11
3	Calibration report "1900 MHz System validation dipole".....	18
4	Calibration report "835 MHz System validation dipole".....	25
5	Calibration certificate of Data Acquisition Unit (DAE).....	32
6	Application Note System Performance Check.....	37



1 Calibration report "Probe EX3DV4"

信息产业部通信计量中心 **TMC**  

Telecommunication Metrology Center of MII

Add: No.52 Hanyuanbei Road, Haidian District, Beijing, 100083, China  
 Tel: +86-10-62303288-2082 Fax: +86-10-62304793  
 E-mail: Info@emcite.com Http://www.emcite.com

检测 CNAS L0442

Client **Huawei** Certificate No: **EX3-3641\_May09**

### CALIBRATION CERTIFICATE

Object: EX3DV4 - SN: 3641

Calibration Procedure(s): TMC-XZ-01-028  
Calibration procedure for dosimetric E-field probes

Calibration date: May 14, 2009




Condition of the calibrated item: In Tolerance

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	SN.	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRVD	101253	19-Jun-08 (TMC, No.JZ08-248)	Jun-09
Power sensor NRV-Z5	100333	19-Jun-08 (TMC, No. JZ08-248)	Jun-09
Reference Probe EX3DV4	SN 3631	13-Dec-08(SPEAG, No.ES3-3631_Dec08)	Dec-09
DAE4	SN 771	21-Nov-08(SPEAG, No.DAE4-771_Nov08)	Nov-09
RF generator E4438C	MY45092879	18-Jun-08(TMC, No.JZ08-302)	Jun-09
Network Analyzer 8753E	US38433212	03-Aug-08(TMC, No.JZ08-056)	Aug-09

	Name	Function	Signature
Calibrated by:	Lin Hao	SAR Test Engineer	
Reviewed by:	Qi Dianyuan	SAR Project Leader	
Approved by:	Lu Bingsong	Deputy Director of the laboratory	

Issued: May 15, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-3641\_May09 Page 1 of 8

Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100083, China  
Tel: +86-10-62303288-2082 Fax: +86-10-62304793  
E-mail: Info@emcite.com Http://www.emcite.com

## Glossary:

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
Polarization $\phi$	$\phi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis(at measurement center), i.e., $\theta = 0$ is normal to probe axis

## Calibration is Performed According to the Following Standards:

- YD/T 1644.1-2007, Human exposure to radio frequency fields from handheld and body-mounted wireless communication devices—human models, instrumentation, and procedures part 1: procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)
- IEEE 1528-2003, IEEE Recommended Practice for Determining the Peak Spatial- Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques Annex A
- IEC 62209-1-2005, Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 300 MHz to 6 GHz. Annex B

## Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900\text{MHz}$  in TEM-cell;  $f > 1800\text{MHz}$ : waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub>\* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800\text{MHz}$ ) and inside waveguide using analytical field distributions based on power measurements for  $f > 800\text{MHz}$ . The same setups are used for assessment of the parameters applied for boundary compensation (alpha,depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub>\* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50\text{MHz}$  to  $\pm 100\text{MHz}$ .
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100083, China  
 Tel: +86-10-62303288-2082 Fax: +86-10-62304793  
 E-mail: Info@emcite.com Http://www.emcite.com

## DASY – Parameters of Probe: EX3DV4 SN:3641

Sensitivity in Free Space <sup>A</sup>			Diode Compression <sup>B</sup>	
NormX	0.36 ± 10.1%	μ V/(V/m) <sup>2</sup>	DCP X	83mV
NormY	0.36 ± 10.1%	μ V/(V/m) <sup>2</sup>	DCP Y	89mV
NormZ	0.41 ± 10.1%	μ V/(V/m) <sup>2</sup>	DCP Z	89mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)  
 Please see Page 7

### Boundary Effect

TSL	900MHz	Typical SAR gradient: 5% per mm		
	Sensor Center to Phantom Surface Distance	2.0 mm	3.0 mm	
	SARbe[%] Without Correction Algorithm	8.5	4.2	
	SARbe[%] With Correction Algorithm	0.4	0.1	
TSL	1810MHz	Typical SAR gradient: 10% per mm		
	Sensor Center to Phantom Surface Distance	2.0 mm	3.0 mm	
	SARbe[%] Without Correction Algorithm	7.6	3.8	
	SARbe[%] With Correction Algorithm	0.2	0.1	

### Sensor Offset

Probe Tip to Sensor Center 1.0 mm


The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100083, China  
Tel: +86-10-62303288-2082 Fax: +86-10-62304793  
E-mail: Info@emcite.com Http://www.emcite.com



## Frequency Response of E-Field

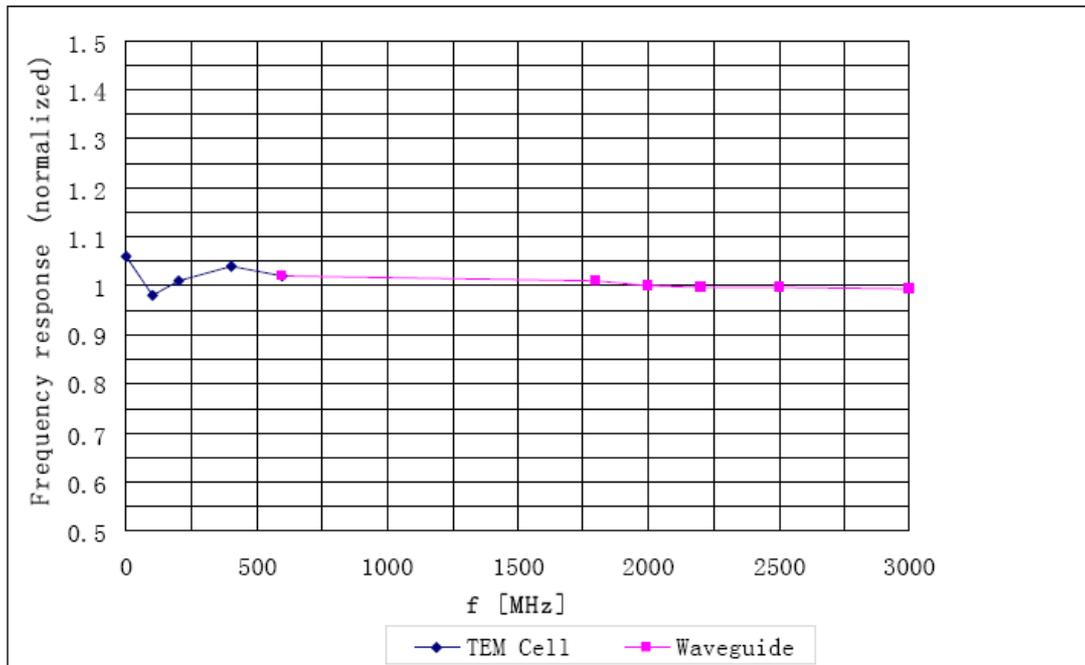

Uncertainty of Frequency Response of E-field:  $\pm 5.0\%$  (k=2)

Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100083, China  
Tel: +86-10-62303288-2082 Fax: +86-10-62304793  
E-mail: Info@emcite.com Http://www.emcite.com


### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

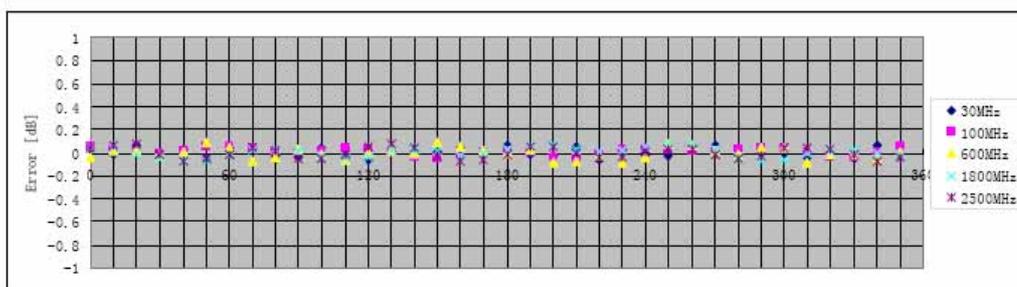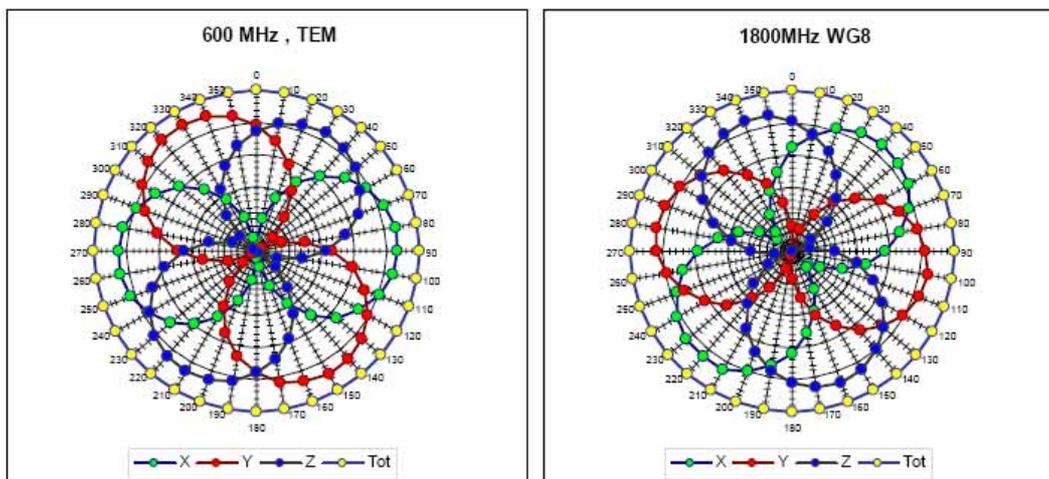

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)

Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100083, China  
Tel: +86-10-62303288-2082 Fax: +86-10-62304793  
E-mail: Info@emcite.com Http://www.emcite.com


### Dynamic Range $f(\text{SAR}_{\text{head}})$ (Waveguide: WG8, $f = 1800 \text{ MHz}$ )

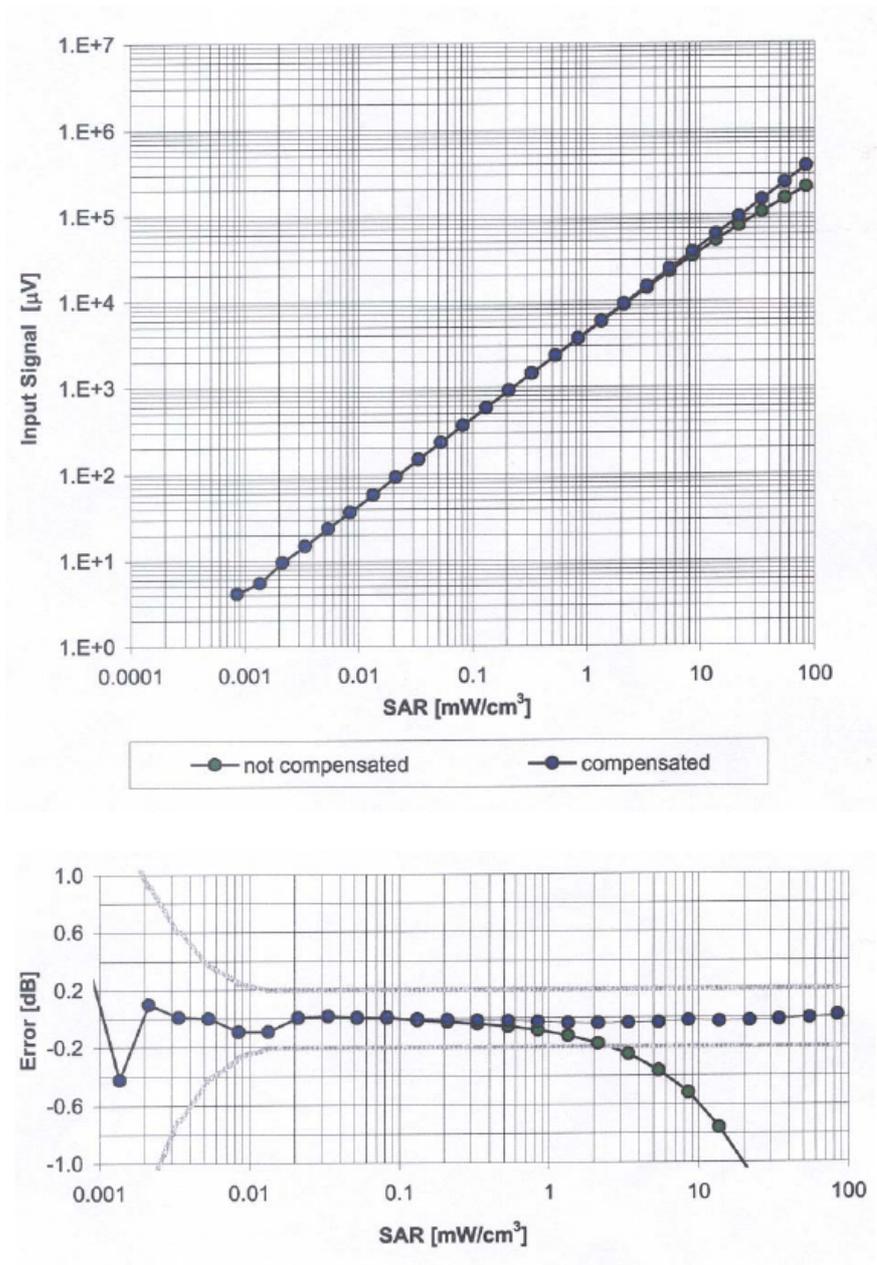

Uncertainty of Linearity Assessment:  $\pm 0.5\%$  ( $k=2$ )

Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100083, China  
 Tel: +86-10-62303288-2082 Fax: +86-10-62304793  
 E-mail: Info@emcite.com Http://www.emcite.com

## Conversion Factor Assessment

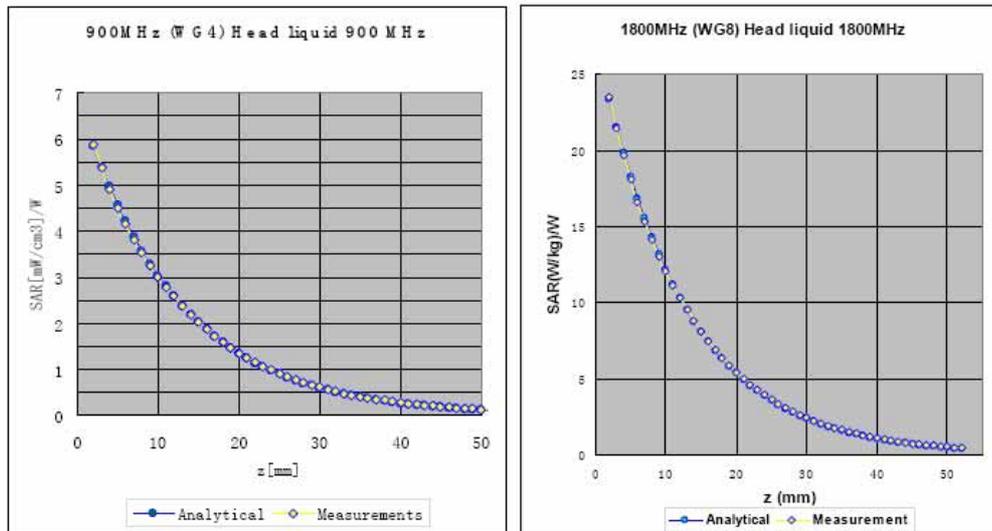


f[MHz]	Validity[MHz] <sup>C</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF	Uncertainty
835	± 50 / ± 100	Head	41.5 ± 5%	0.90 ± 5%	0.20	1.05	9.13	± 11.0% (k=2)
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.55	0.69	9.02	± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.21	1.24	7.74	± 11.0% (k=2)
1900	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.20	1.05	7.66	± 11.0% (k=2)
2000	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.21	1.25	7.53	± 11.0% (k=2)
835	± 50 / ± 100	Body	55.2 ± 5%	0.97 ± 5%	0.69	0.64	9.09	± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.45	0.83	8.93	± 11.0% (k=2)
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.20	1.05	7.62	± 11.0% (k=2)
1900	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.26	1.08	7.22	± 11.0% (k=2)
2000	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.21	1.24	7.39	± 11.0% (k=2)

<sup>C</sup> The validity of ±100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100083, China  
Tel: +86-10-62303288-2082 Fax: +86-10-62304793  
E-mail: Info@emcite.com Http://www.emcite.com

## Deviation from Isotropy

Error (  $\phi$  ,  $\theta$  ), f = 900 MHz

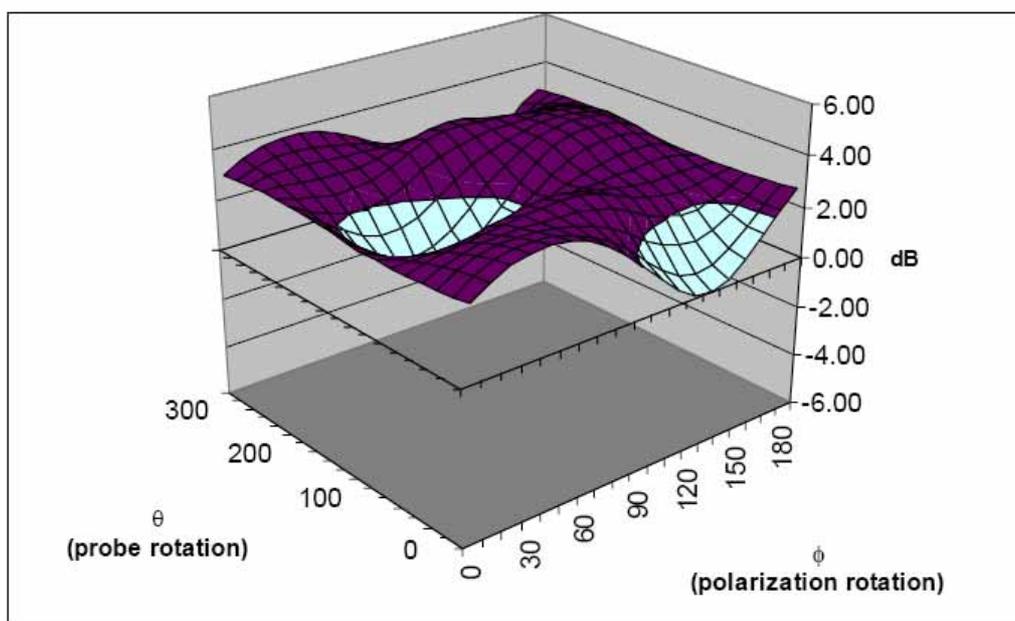

**Uncertainty of Spherical Isotropy Assessment:  $\pm 2.5\%$  (k=2)**

## 2 Calibration report “1800 MHz System validation





信息产业部通信计量中心  
Telecommunication Metrology Center of MII

Client: **Huawei**      Certificate No: **D1800V2-2d157\_May09**

### CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d157**

Calibration Procedure(s): **TMC-XZ-01-027  
Calibration procedure for dipole validation kits**

Calibration date: **May 27, 2009**




Condition of the calibrated item: **In Tolerance**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRVD	101253	19-Jun-08 (TMC, No.JZ08-248)	Jun-09
Power sensor NRV-Z5	100333	19-Jun-08 (TMC, No. JZ08-248)	Jun-09
Reference Probe ES3DV3	SN 3149	08-Dec-08(SPEAG, No.ES3-3149_Dec08)	Dec-09
DAE4	SN 771	21-Nov-08(SPEAG, No.DAE4-771_Nov08)	Nov-09
RF generator E4438C	MY45092879	18-Jun-08(TMC, No.JZ08-302)	Jun-09
Network Analyzer 8753E	US38433212	03-Aug-08(TMC, No.JZ08-056)	Aug-09

	Name	Function	Signature
Calibrated by:	Lin Hao	SAR Test Engineer	
Reviewed by:	Qi Dianyuan	SAR Project Leader	
Approved by:	Lu Bingsong	Deputy Director of the laboratory	

Issued: May 27, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D1800V2-2d157\_May09
Page 1 of 7

**Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
N/A	not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.0
Extrapolation	Advanced Extrapolation	
Phantom	2mm Oval Phantom ELI4	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz $\pm$ 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	40.6 $\pm$ 6 %	1.35mho/m $\pm$ 6 %
Head TSL temperature during test	(22.5 $\pm$ 0.2) °C	----	----

### SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.23 mW / g
SAR normalized	normalized to 1W	36.9 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	37.9 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	4.90 mW / g
SAR normalized	normalized to 1W	19.6 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	19.9 mW / g $\pm$ 16.5 % (k=2)

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

### Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.3 ± 6%	1.46mho/m ± 6 %
Body TSL temperature during test	(22.4 ± 0.2) °C	---	---

### SAR result with Body TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.80 mW / g
SAR normalized	normalized to 1W	38.4 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	39.2 mW / g ± 17.0 % (k=2)

SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.13 mW / g
SAR normalized	normalized to 1W	20.5 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	20.7 mW / g ± 16.5 % (k=2)

---

<sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	$45.5 \Omega + 4.2 j \Omega$
Return Loss	- 25.2dB

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	$46.7 \Omega + 7.4 j \Omega$
Return Loss	- 22.1dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.624 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### DASY5 Validation Report for Head TSL

Date/Time: 2009-5-27 9:05:32

Test Laboratory: TMC, Beijing, China

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: SN: 2d157

Communication System: CW Frequency: 1800 MHz Duty Cycle: 1:1

Medium: Head 1900MHz

Medium parameters used:  $f = 1800$  MHz;  $\sigma = 1.35$  mho/m;  $\epsilon_r = 40.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

#### DASY5 Configuration:

- Probe: ES3DV3 - SN3149; ConvF(5.18, 5.18, 5.18); Calibrated: 08.12.08
- Electronics: DAE4 Sn771; Calibration: 21.11.08
- Phantom: 2mm Oval Phantom ELI4; Type: QDOVA001BB
- Measurement SW: DASY5, V5.0 Build 119.9; Postprocessing SW: SEMCAD, V13.2 Build 87

Pin=250mW; d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 62.9 V/m; Power Drift = -0.095 dB

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 9.23 mW/g; SAR(10 g) = 4.9 mW/g

Maximum value of SAR (measured) = 10.4 mW/g

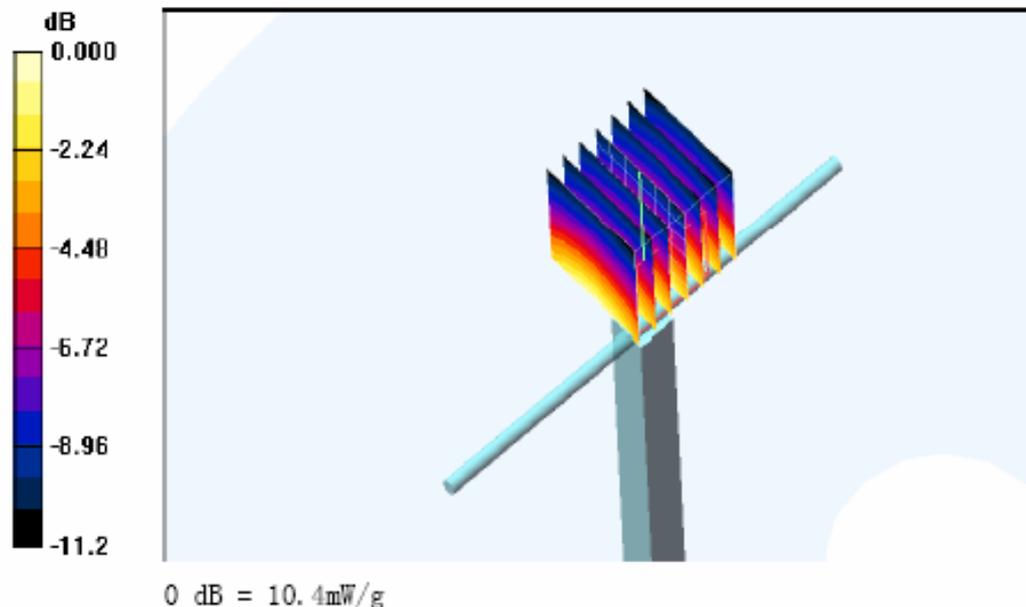

### DASY5 Validation Report for Body TSL

Date/Time: 2009-5-27 12:58:30

Test Laboratory: TMC, Beijing, China

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: SN: 2d157

Communication System: CW Frequency: 1800 MHz Duty Cycle: 1:1

Medium: Body 1900MHz

Medium parameters used:  $f = 1800$  MHz;  $\sigma = 1.46$  mho/m;  $\epsilon_r = 53.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

#### DASY5 Configuration:

- Probe: ES3DV3 - SN3149; ConvF(4.97, 4.97, 4.97); Calibrated: 08.12.08
- Electronics: DAE4 Sn771; Calibration: 21.11.08
- Phantom: 2mm Oval Phantom ELI4; Type: QDOVA001BB
- Measurement SW: DASY5, V5.0 Build 119.9; Postprocessing SW: SEMCAD, V13.2 Build 87

Pin=250mW; d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.4 V/m; Power Drift = -0.150 dB

Peak SAR (extrapolated) = 17.0 W/kg

SAR(1 g) = 9.6 mW/g; SAR(10 g) = 5.13 mW/g

Maximum value of SAR (measured) = 10.8 mW/g

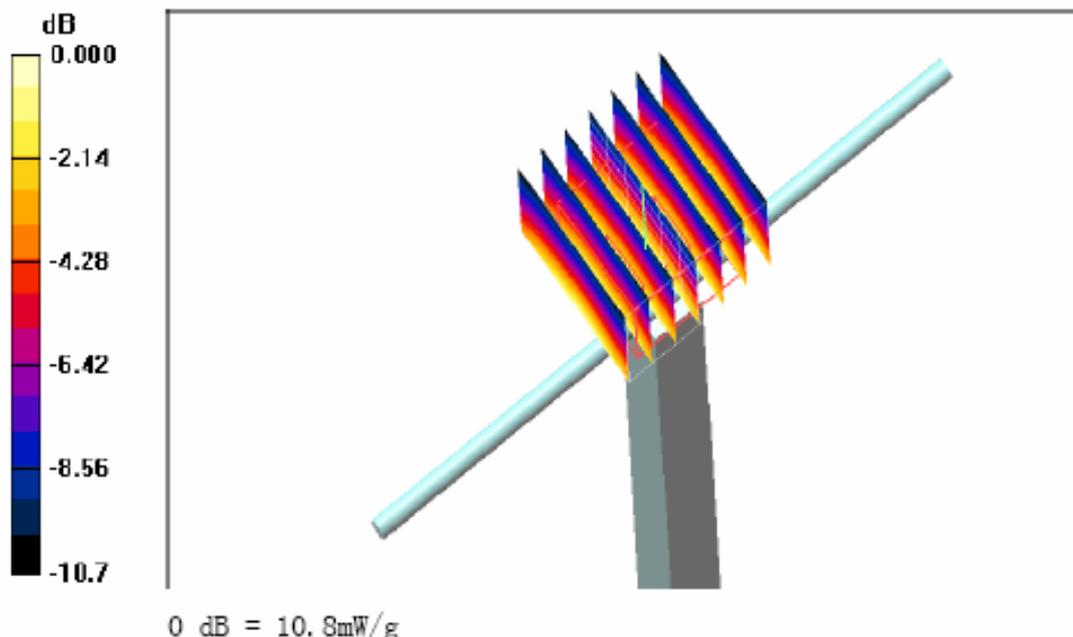



### 3 Calibration report “1900 MHz System validation dipole”





信息产业部通信计量中心  
Telecommunication Metrology Center of MII

Client: **Huawei** Certificate No: **D1900V2-5d091\_May09**

#### CALIBRATION CERTIFICATE

Object: D1900V2 - SN: 5d091

Calibration Procedure(s): TMC-XZ-01-027  
Calibration procedure for dipole validation kits

Calibration date: May 28, 2009

Condition of the calibrated item: In Tolerance



This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRVD	101253	19-Jun-08 (TMC, No.JZ08-248)	Jun-09
Power sensor NRV-Z5	100333	19-Jun-08 (TMC, No. JZ08-248)	Jun-09
Reference Probe ES3DV3	SN 3149	08-Dec-08(SPEAG No.ES3-3149_Dec08)	Dec-09
DAE4	SN 771	21-Nov-08(SPEAG No.DAE4-771_Nov08)	Nov-09
RF generator E4438C	MY45092879	18-Jun-08(TMC, No.JZ08-302)	Jun-09
Network Analyzer 8753E	US38433212	03-Aug-08(TMC, No.JZ08-056)	Aug-09

	Name	Function	Signature
Calibrated by:	Lin Hao	SAR Test Engineer	
Reviewed by:	Qi Dianyuan	SAR Project Leader	
Approved by:	Lu Bingsong	Deputy Director of the laboratory	

Issued: May 28, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D1900V2-5d091\_May09 Page 1 of 7

**Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
N/A	not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY5	V5.0
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	2mm Oval Phantom ELI4	
<b>Distance Dipole Center - TSL</b>	10 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	1900 MHz $\pm$ 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	40.0	1.40 mho/m
<b>Measured Head TSL parameters</b>	(22.0 $\pm$ 0.2) °C	40.3 $\pm$ 6 %	1.39mho/m $\pm$ 6 %
<b>Head TSL temperature during test</b>	(22.1 $\pm$ 0.2) °C	----	----

### SAR result with Head TSL

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	9.60 mW / g
SAR normalized	normalized to 1W	38.4 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	<b>38.7 mW / g <math>\pm</math> 17.0 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	5.10 mW / g
SAR normalized	normalized to 1W	20.4 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	<b>20.5 mW / g <math>\pm</math> 16.5 % (k=2)</b>

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"