



Annex 3 Calibration parameters

3.1 Data Acquisition Unit (DAE4)-852

工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT

Add: No.52 Huiyuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: Info@emctc.com Http://www.emctc.com

Client **Huawei** Certificate No: DAE4-852_Dec10

CALIBRATION CERTIFICATE

Object

DAE4 - SN: 852

Calibration Procedure(s)

TMC-XZ-01-029
Calibration procedure for the data acquisition electronics (DAE)

Calibration date:

December 24, 2010

Condition of the calibrated item

In Tolerance

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Multimeter 3458A	MY45041463	12-Nov-10 (TMC, No: DLsc2010-1115)	Nov-11
DC POWER SUPPLY 66321D	MY43001657	12-Nov-10 (TMC, No: JZ10-290)	Nov-11

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Calibrator Box	/	19-Jun-10 (TMC, in house check)	In house check Jun-11

Calibrated by:

Name

Lin Hao

Function

SAR Test Engineer

Signature

Reviewed by:

Name

Qi Dianyuan

Function

SAR Project Leader

Signature

Approved by:

Name

Xiao Li

Function

Deputy Director of the laboratory

Signature

Issued: December 24, 2010

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Add: No.52 Huiyuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: Info@emc.itc.com [Http://www.emc.itc.com](http://www.emc.itc.com)

Glossary:

DAE	data acquisition electronics
Connector angle	information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters:

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters contain technical information as a result from the performance test and require no uncertainty.
- DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
- Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
- Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
- AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage.
- Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.



工业和信息化部通信计量中心 TMC
Telecommunication Metrology Center of MIIT

Add: No.52 Huiyuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: info@emcicc.com Http://www.emcicc.com

DC Voltage Measurement

A/D - Converter Resolution nominal
High Range: 1LSB = 8.1 μ V, full range = -100...+300 mV
Low Range: 1LSB = 61nV, full range = -1,...,+3mV
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	405.142 $\pm$ 0.1% (κ =2)	405.214 $\pm$ 0.1% (κ =2)	404.005 $\pm$ 0.1% (κ =2)
Low Range	3.97599 $\pm$ 0.7% (κ =2)	3.96438 $\pm$ 0.7% (κ =2)	3.95613 $\pm$ 0.7% (κ =2)

Connector Angle

Connector Angle to be used in DASY system	159 $^{\circ}$ $\pm$ 1 $^{\circ}$
---	-----------------------------------



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIT

Add: No.52 Huguangbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079
E-mail: Info@emcrite.com

Fax: +86-10-62304793
Http://www.emcrite.com

Appendix
1. DC Voltage Linearity

High Range		Input (μ V)	Reading (μ V)	Error (%)
Channel X	+ Input	200000	200000.2	0.00
Channel X	+ Input	20000	20002.75	0.01
Channel X	- Input	20000	-20003.08	0.02
Channel Y	+ Input	200000	200000	0.00
Channel Y	+ Input	20000	20003.19	0.02
Channel Y	- Input	20000	-20002.40	0.01
Channel Z	+ Input	200000	200001.2	0.00
Channel Z	+ Input	20000	20004.27	0.02
Channel Z	- Input	20000	-20003.2	0.02

Low Range		Input (μ V)	Reading (μ V)	Error (%)
Channel X	+ Input	2000	1999.7	-0.02
Channel X	+ Input	200	199.66	-0.06
Channel X	- Input	200	-200.49	0.28
Channel Y	+ Input	2000	1999.8	0.00
Channel Y	+ Input	200	199.45	-0.26
Channel Y	- Input	200	-200.24	0.08
Channel Z	+ Input	2000	2000	0.00
Channel Z	+ Input	200	199.57	-0.30
Channel Z	- Input	200	-200.83	0.49

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μ V)	Low Range Average Reading (μ V)
Channel X	200	3.41	3.47
	- 200	-2.60	-3.15
Channel Y	200	0.18	-0.37
	- 200	-0.66	-1.12
Channel Z	200	-9.70	-10.08
	- 200	7.88	8.23



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT

Add: No.52 Huiyuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: info@emclic.com <http://www.emclic.com>

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	2.61	-0.38
Channel Y	200	0.59	-	2.46
Channel Z	200	-1.93	0.24	-

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16130	16437
Channel Y	15975	16211
Channel Z	15978	16034

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec
Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation(μV)
Channel X	0.57	-1.04	1.91	0.45
Channel Y	-1.03	-1.90	-0.06	0.39
Channel Z	1.12	-0.11	1.94	0.38

6. Input Offset Current

Nominal Input Circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	201.1
Channel Y	0.2000	198.9
Channel Z	0.2000	200.4



3.2 Probe ES3DV3-3168

工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: Info@emcite.com Http://www.emcite.com

Client **Huawei** Certificate No: **ES3-3168_Dec10**

CALIBRATION CERTIFICATE

Object

ES3DV3 - SN: 3168

Calibration Procedure(s)

TMC-XZ-01-028
Calibration procedure for dosimetric E-field probes

Calibration date:

December 23, 2010

Condition of the calibrated item

In Tolerance

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	SN.	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRVD	102083	11-Sep-10 (TMC, No.JZ10-443)	Sep-11
Power sensor NRV-Z5	100542	11-Sep-10 (TMC, No. JZ10-443)	Sep-11
Reference Probe EX3DV4	SN 3631	13-Dec-10 (TMC, No. JZ10-657)	Dec-11
DAE4	SN 771	21-Nov-10 (TMC, No. JZ10-653)	Nov-11
RF generator E4438C	MY49070393	13-Nov-10 (TMC, No. JZ10-394)	Nov-11
Network Analyzer 8753E	US38433212	04-Aug-10 (TMC, No. JZ10-056)	Aug-11

Calibrated by:

Name

Lin Hao

Function

SAR Test Engineer

Signature

Reviewed by:

Name

Qi Dianyuan

Function

SAR Project Leader

Signature

Approved by:

Name

Xiao Li

Function

Deputy Director of the laboratory

Signature

Issued: December 23, 2010

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

工业和信息化部通信计量中心



Telecommunication Metrology Center of MIIT

Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2079

Fax: +86-10-62304793

E-mail: tinfo@emcrite.com

Http://www.emcrite.com

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
Polarization ϕ	ϕ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}: Assessed for E-field polarization $\theta = 0$ ($f \leq 900\text{MHz}$ in TEM-cell; $f > 1800\text{MHz}$: waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not effect the E^2 -field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800\text{MHz}$) and inside waveguide using analytical field distributions based on power measurements for $f > 800\text{MHz}$. The same setups are used for assessment of the parameters applied for boundary compensation (alpha,depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from $\pm 50\text{MHz}$ to $\pm 100\text{MHz}$.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.



工业和信息化部通信计量中心 TMC
Telecommunication Metrology Center of MIIT
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: Info@cmctc.com Http://www.cmctc.com

DASY – Parameters of Probe: ES3DV3 SN:3168

Sensitivity in Free Space ^A			Diode Compression ^B	
NormX	1.04±10.1%	μ V/(V/m) ²	DCP X	85mV
NormY	1.19±10.1%	μ V/(V/m) ²	DCP Y	88mV
NormZ	1.02±10.1%	μ V/(V/m) ²	DCP Z	83mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)
Please see Page 8

Boundary Effect

TSL	900MHz	Typical SAR gradient: 5% per mm		
Sensor Center to Phantom Surface Distance		3.0 mm	4.0 mm	
SARbe[%]	Without Correction Algorithm	3.8	1.4	
SARbe[%]	With Correction Algorithm	0.8	0.6	
TSL	1750MHz	Typical SAR gradient: 10% per mm		
Sensor Center to Phantom Surface Distance		3.0 mm	4.0 mm	
SARbe[%]	Without Correction Algorithm	6.7	3.6	
SARbe[%]	With Correction Algorithm	0.3	0.2	

Sensor Offset

Probe Tip to Sensor Center	2.0 mm
----------------------------	--------


The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).
^B Numerical linearization parameter: uncertainty not required.



工业和信息化部通信计量中心 TMC
Telecommunication Metrology Center of MIIT
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: Info@emcite.com Http://www.emcite.com

Frequency Response of E-Field


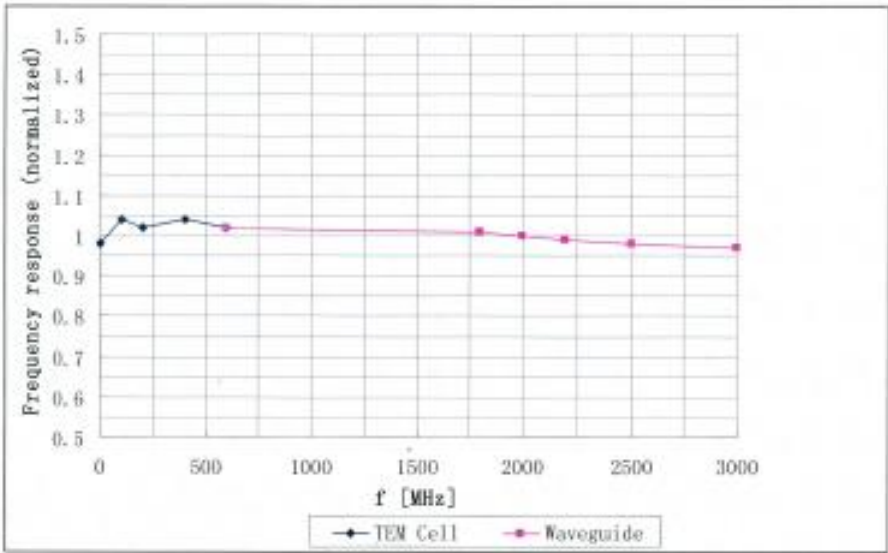


Uncertainty of Frequency Response of E-field: $\pm 5.0\%$ (k=2)



工业和信息化部通信计量中心 TMC
Telecommunication Metrology Center of MIIT
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: Info@emcitz.com Http://www.emcitz.com

Receiving Pattern (ϕ), $\theta = 0^\circ$

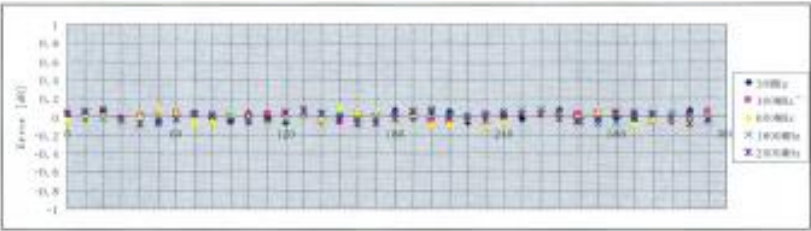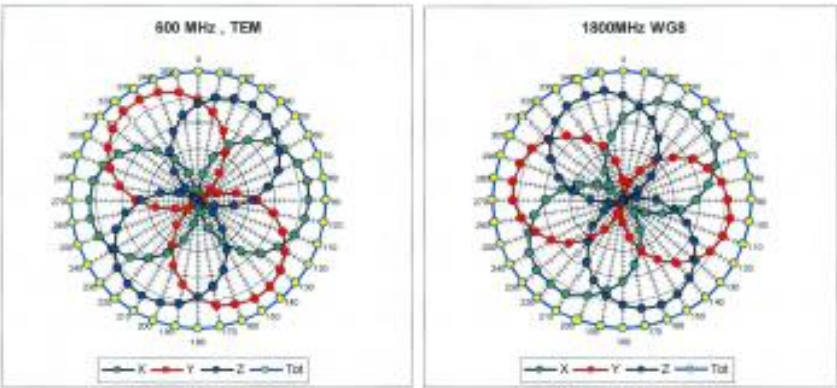


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)



工业和信息化部通信计量中心 TMC
Telecommunication Metrology Center of MIIT
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: info@emcite.com Http://www.emcite.com

Dynamic Range f(SAR_{head})
(Waveguide: WG8, f = 1750 MHz)

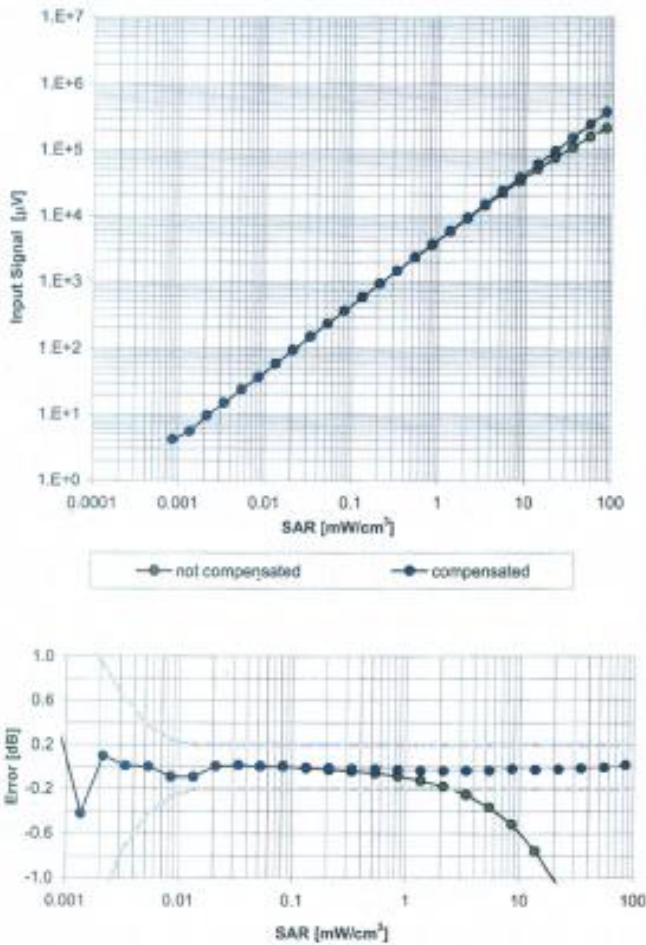


Uncertainty of Linearity Assessment: $\pm 0.5\%$ (k=2)




工业和信息化部通信计量中心 TMC
Telecommunication Metrology Center of MIIT
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: Info@emcrite.com Http://www.emcrite.com

Conversion Factor Assessment

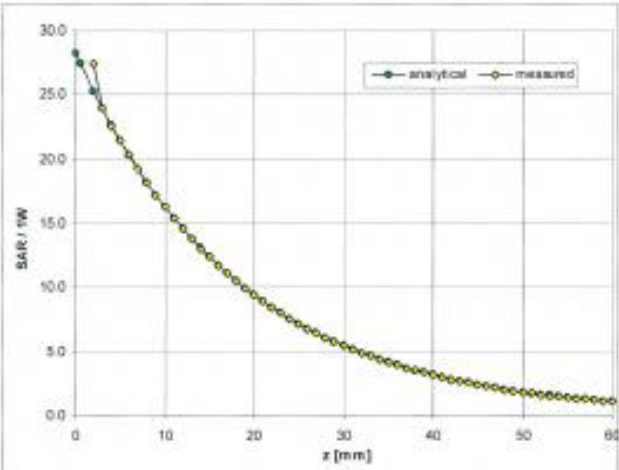

900MHz

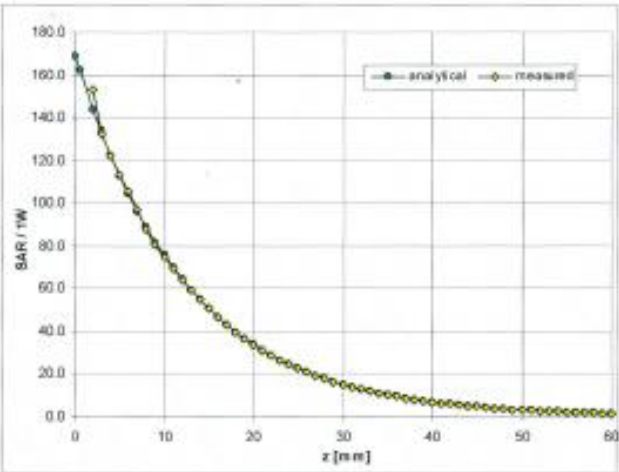

1900MHz


Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2079 Fax: +86-10-62304791
 E-mail: Info@emcrite.com Http://www.emcrite.com

Freq	Frequency	ϵ	σ	ϵ	σ	Sensitivity X sensor			Sensitivity Y sensor			Sensitivity Z sensor			Uncertainty
[MHz]	Range	target	[S/m]	used	used	ConvF	Alpha	Depth	ConvF	Alpha	Depth	ConvF	Alpha	Depth	k=2
		$\pm 5\%$	$\pm 5\%$												
Probe Conversion Factors: Head Tissue Liquid															
850	$\pm 50 / \pm 100$	41.5	0.92	42.0	0.91	5.98	0.28	1.92	5.98	0.28	1.92	5.98	0.28	1.92	$\pm 11\%$
900	$\pm 50 / \pm 100$	41.5	0.97	41.5	0.95	5.89	0.28	2.04	5.89	0.28	2.04	5.89	0.28	2.04	$\pm 11\%$
1750	$\pm 50 / \pm 100$	40.08	1.37	39.7	1.35	5.12	0.42	1.57	5.12	0.42	1.57	5.12	0.42	1.57	$\pm 11\%$
1900	$\pm 50 / \pm 100$	40.0	1.40	40.5	1.35	4.97	0.48	1.63	4.97	0.48	1.63	4.97	0.48	1.63	$\pm 11\%$
2000	$\pm 50 / \pm 100$	40.0	1.40	40.2	1.45	4.83	0.44	1.66	4.83	0.44	1.66	4.83	0.44	1.66	$\pm 11\%$
2300	$\pm 50 / \pm 100$	39.47	1.67	40.4	1.71	4.59	0.29	2.36	4.59	0.29	2.36	4.59	0.29	2.36	$\pm 11\%$
2450	$\pm 50 / \pm 100$	39.2	1.80	39.4	1.82	4.45	0.51	1.38	4.45	0.51	1.38	4.45	0.51	1.38	$\pm 11\%$
2600	$\pm 50 / \pm 100$	39.01	1.96	38.7	2.05	4.32	0.68	2.92	4.32	0.68	2.92	4.32	0.68	2.92	$\pm 11\%$
Probe Conversion Factors: Body Tissue Liquid															
850	$\pm 50 / \pm 100$	55.2	0.99	54.6	1.03	5.92	0.32	1.88	5.92	0.32	1.88	5.92	0.32	1.88	$\pm 11\%$
900	$\pm 50 / \pm 100$	55.0	1.05	54.0	1.08	5.83	0.43	1.52	5.83	0.43	1.52	5.83	0.43	1.52	$\pm 11\%$
1750	$\pm 50 / \pm 100$	53.4	1.49	53.2	1.42	4.99	0.43	1.74	4.99	0.43	1.74	4.99	0.43	1.74	$\pm 11\%$
1900	$\pm 50 / \pm 100$	53.3	1.52	52.8	1.54	4.61	0.43	1.76	4.61	0.43	1.76	4.61	0.43	1.76	$\pm 11\%$
2000	$\pm 50 / \pm 100$	53.3	1.52	53.6	1.58	4.56	0.41	1.67	4.56	0.41	1.67	4.56	0.41	1.67	$\pm 11\%$
2300	$\pm 50 / \pm 100$	52.8	1.85	52.3	1.77	4.38	0.33	2.18	4.38	0.33	2.18	4.38	0.33	2.18	$\pm 11\%$
2450	$\pm 50 / \pm 100$	52.7	1.95	51.9	1.95	4.24	0.66	2.92	4.24	0.66	2.92	4.24	0.66	2.92	$\pm 11\%$
2600	$\pm 50 / \pm 100$	52.5	2.16	51.9	2.26	4.16	0.35	1.91	4.16	0.35	1.91	4.16	0.35	1.91	$\pm 11\%$



工业和信息化部通信计量中心 TMC
Telecommunication Metrology Center of MIIT
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304793
E-mail: Info@emcite.com Http://www.emcite.com

Deviation from Isotropy
Error (ϕ , θ), $f = 900$ MHz

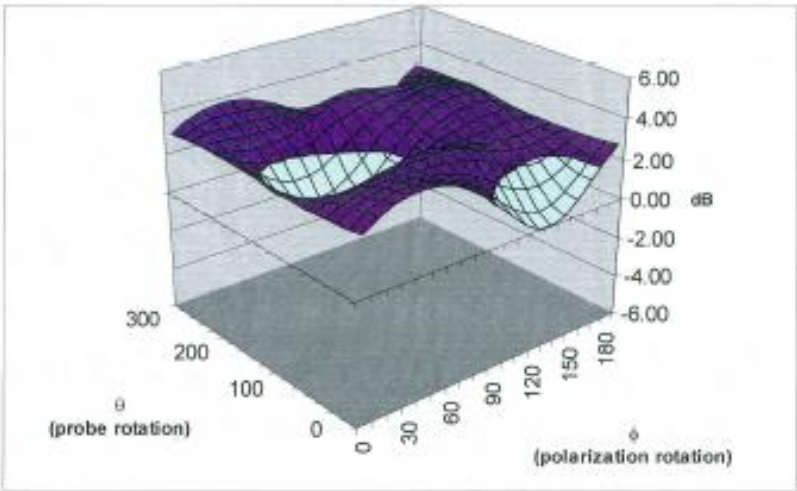

Uncertainty of Spherical Isotropy Assessment: $\pm 2.5\%$ ($k=2$)



3.3 835 MHz System validation dipole

工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT

Client **Huawei** Certificate No: **D835V2-4d095_Feb11**

CALIBRATION CERTIFICATE

Object

D835V2 - SN: 4d095

Calibration Procedure(s)

TMC-XZ-01-027
Calibration procedure for dipole validation kits

Calibration date:

February 23, 2011

Condition of the calibrated item

In Tolerance

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRVD	101253	18-Jun-10 (TMC, No.JZ10-248)	Jun-11
Power sensor NRV-Z5	100333	18-Jun-10 (TMC, No. JZ10-248)	Jun-11
Reference Probe ES3DV3	SN 3149	25-Sep-10 (SPEAG, No.ES3-3149_Sep10)	Sep-11
DAE4	SN 771	21-Nov-10 (TMC, No.JZ10-653)	Nov-11
RF generator E4438C	MY45092879	17-Jun-10 (TMC, No.JZ10-302)	Jun-11
Network Analyzer 8753E	US38433212	02-Aug-10 (TMC, No.JZ10-056)	Aug-11

	Name	Function	Signature
Calibrated by:	Lin Hao	SAR Test Engineer	
Reviewed by:	Qi Dianyuan	SAR Project Leader	
Approved by:	Lu Bingsong	Deputy Director of the laboratory	

Issued: February 23, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM _{x,y,z}
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2.157
Extrapolation	Advanced Extrapolation	
Phantom	2mm Oval Phantom ELI4	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.9 ± 6 %	0.93mho/m ± 6 %
Head TSL temperature during test	(22.5 ± 0.2) °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.39 mW / g
SAR normalized	normalized to 1W	9.56 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	9.42 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.54 mW / g
SAR normalized	normalized to 1W	6.16 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	6.13 mW / g ± 16.5 % (k=2)

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.8 ± 6%	1.00mho/m ± 6 %
Body TSL temperature during test	(22.4 ± 0.2) °C	-----	-----

SAR result with Body TSL

SAR averaged over 1 cm^3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.47 mW / g
SAR normalized	normalized to 1W	9.88 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	9.56 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm^3 (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.61 mW / g
SAR normalized	normalized to 1W	6.44 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	6.28 mW /g ± 16.5 % (k=2)

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$47.2\Omega + 7.0\text{ j}\Omega$
Return Loss	- 22.3dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$46.5\Omega + 3.4\text{ j}\Omega$
Return Loss	- 25.9dB

General Antenna Parameters and Design

Electrical Delay (one direction)	3.184 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



DASY5 Validation Report for Head TSL

Date/Time: 2011-2-23 9:15:24

Test Laboratory: TMC, Beijing, China

DUT: Dipole 835 MHz; Type: D835V2; Serial: SN: 4d095

Communication System: CW Frequency: 835 MHz Duty Cycle: 1:1

Medium: Head 835MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.93 \text{ mho/m}$; $\epsilon_r = 41.9$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3149; ConvF(6.56, 6.56, 6.56); Calibrated: 25.09.10
- Electronics: DAE4 Sn771; Calibration: 21.11.10
- Phantom: 2mm Oval Phantom EL14; Type: QDOVA001BB
- Measurement SW: DASY5, V5.2.157; Postprocessing SW: SEMCAD, V14.0 Build 57

Pin=250mW; d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 56.3 V/m; Power Drift = 0.104 dB

Peak SAR (extrapolated) = 3.475 W/kg

SAR(1 g) = 2.39 mW/g; SAR(10 g) = 1.54 mW/g

Maximum value of SAR (measured) = 2.56 mW/g


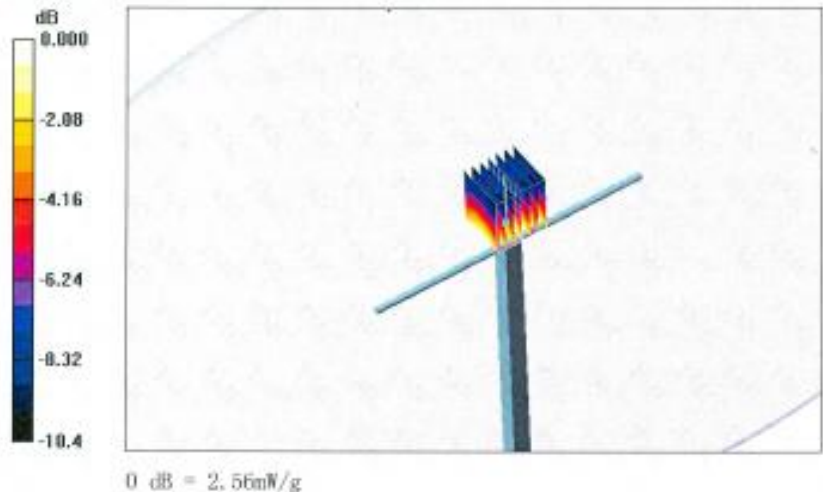




工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Impedance Measurement Plot for Head TSL

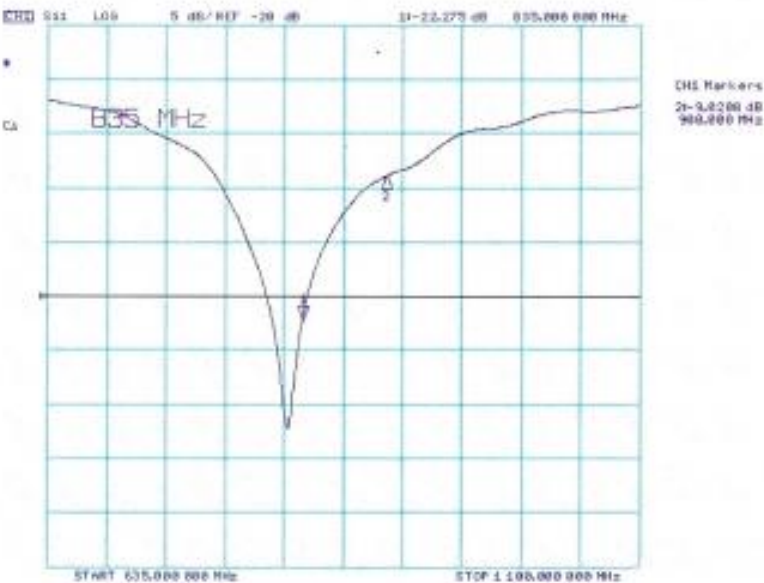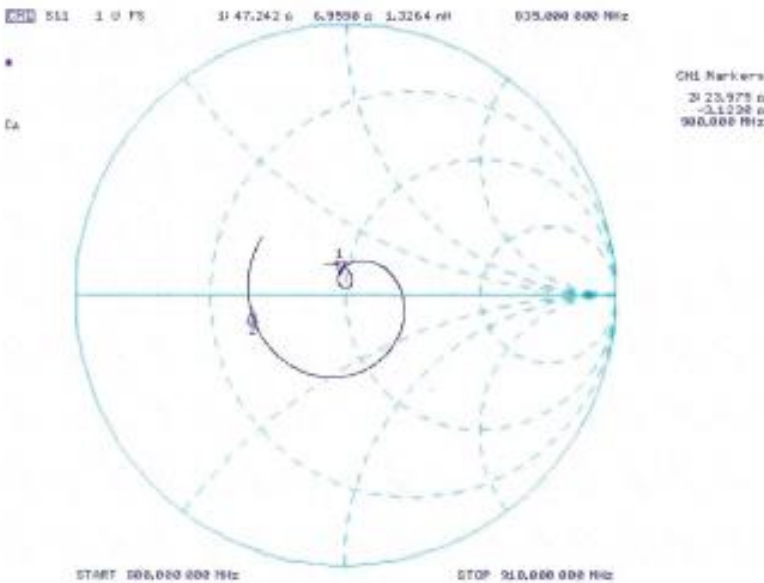



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



DASY5 Validation Report for Body TSL

Date/Time: 2011-2-23 10:36:18

Test Laboratory: TMC, Beijing, China

DUT: Dipole 835 MHz; Type: D835V2; Serial: SN: 4d095

Communication System: CW Frequency: 835 MHz Duty Cycle: 1:1

Medium: Body 835MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 1 \text{ mho/m}$; $\epsilon_r = 53.8$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3149; ConvF(6.22, 6.22, 6.22); Calibrated: 25.09.10
- Electronics: DAE4 Sn771; Calibration: 21.11.10
- Phantom: 2mm Oval Phantom EL34; Type: QDOVA001BB
- Measurement SW: DASY5, V5.2.157; Postprocessing SW: SEMCAD, V14.0 Build 57

Pin=250mW; d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 41.7 V/m; Power Drift = -0.065 dB

Peak SAR (extrapolated) = 3.475 W/kg

SAR(1 g) = 2.47 mW/g; SAR(10 g) = 1.61 mW/g

Maximum value of SAR (measured) = 2.68 mW/g

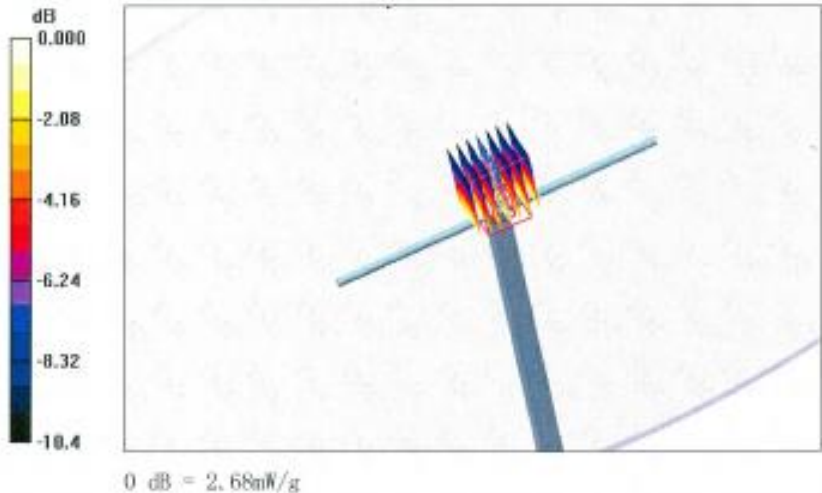




工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Impedance Measurement Plot for Body TSL

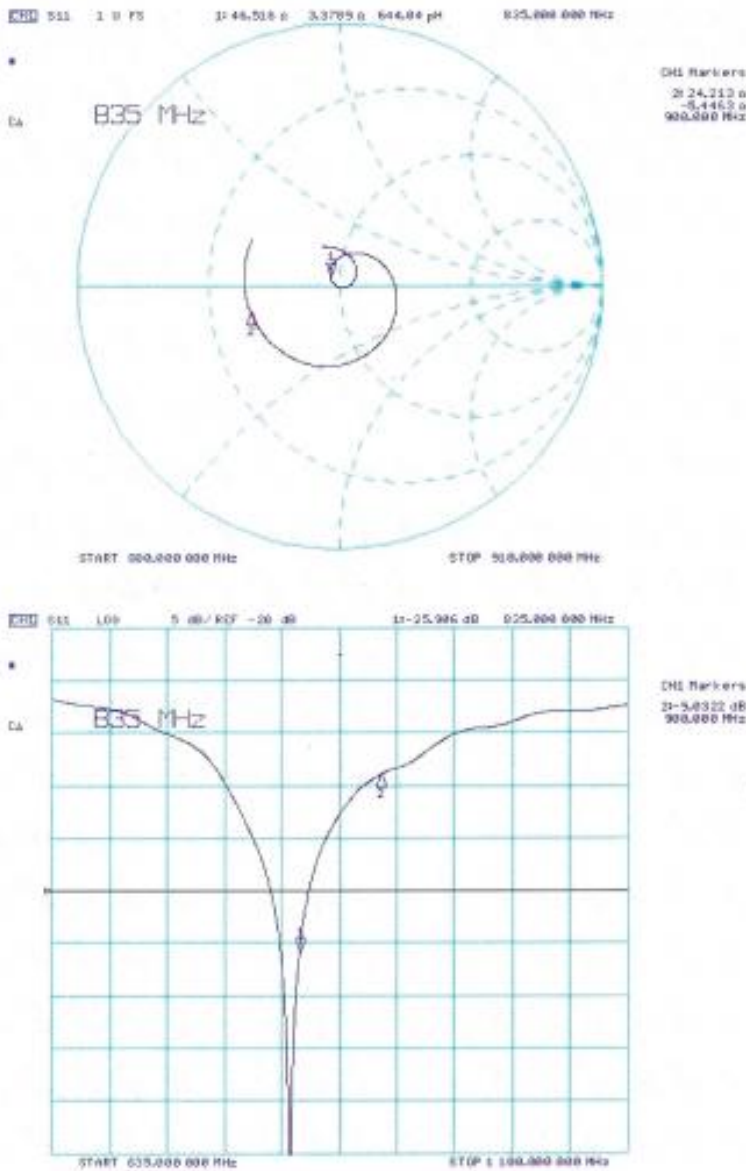



3.4 1900 MHz System validation dipole

工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT

Client **Huawei** Certificate No: **D1900V2-5d091_Feb11**

CALIBRATION CERTIFICATE

Object

D1900V2 - SN: 5d091

Calibration Procedure(s)

TMC-XZ-01-027
Calibration procedure for dipole validation kits

Calibration date.

February 23, 2011

Condition of the calibrated item

In Tolerance

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRVD	101253	18-Jun-10 (TMC, No.JZ10-248)	Jun-11
Power sensor NRV-Z5	100333	18-Jun-10 (TMC, No. JZ10-248)	Jun-11
Reference Probe ES3DV3	SN 3149	25-Sep-10 (SPEAG, No.ES3-3149_Sep10)	Sep-11
DAE4	SN 771	21-Nov-10 (TMC, No.JZ10-653)	Nov-11
RF generator E4438C	MY45092879	17-Jun-10 (TMC, No.JZ10-302)	Jun-11
Network Analyzer 8753E	US38433212	02-Aug-10 (TMC, No.JZ10-056)	Aug-11

Calibrated by:

Name

Lin Hao

Function

SAR Test Engineer

Signature

Reviewed by:

Name

Qi Dianyuan

Function

SAR Project Leader

Signature

Approved by:

Name

Lu Bingsong

Function

Deputy Director of the laboratory

Signature

Issued: February 23, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D1900V2-5d091_Feb11

Page 1 of 9

工业和信息化部通信计量中心
Telecommunication Metrology Center of MII



Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM _{x,y,z}
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2.157
Extrapolation	Advanced Extrapolation	
Phantom	2mm Oval Phantom EL14	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.8 $\pm$ 6 %	1.39mho/m $\pm$ 6 %
Head TSL temperature during test	(22.1 $\pm$ 0.2) °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.90 mW / g
SAR normalized	normalized to 1W	39.6 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	39.1 mW /g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.10 mW / g
SAR normalized	normalized to 1W	20.4 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	20.2 mW /g $\pm$ 16.5 % (k=2)

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.7 ± 6%	1.58mho/m ± 6 %
Body TSL temperature during test	(21.9 ± 0.2) °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm^3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.2 mW / g
SAR normalized	normalized to 1W	40.8 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	39.2 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm^3 (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.24 mW / g
SAR normalized	normalized to 1W	21.0 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	20.5 mW /g ± 16.5 % (k=2)

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.2Ω - 2.3 jΩ
Return Loss	- 32.5dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.6Ω - 6.1 jΩ
Return Loss	- 24.2dB

General Antenna Parameters and Design

Electrical Delay (one direction)	4.089 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



DASY5 Validation Report for Head TSL

Date/Time: 2011-2-23 16:07:52

Test Laboratory: TMC, Beijing, China

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: SN: 5d091

Communication System: CW Frequency: 1900 MHz Duty Cycle: 1:1

Medium: Head 1900MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.39$ mho/m; $\epsilon_r = 38.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 - SN3149; ConvF(5.03, 5.03, 5.03); Calibrated: 25.09.10
- Electronics: DAE4 Sn771; Calibration: 21.11.10
- Phantom: 2mm Oval Phantom ELI4; Type: QDOVA001BB
- Measurement SW: DASY5, V5.2.157; Postprocessing SW: SEMCAD, V14.0 Build 57

Pin=250mW; d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.4 V/n; Power Drift = 0.048 dB

Peak SAR (extrapolated) = 17.75 W/kg

SAR(1 g) = 9.9 mW/g; SAR(10 g) = 5.1 mW/g

Maximum value of SAR (measured) = 11.0 mW/g


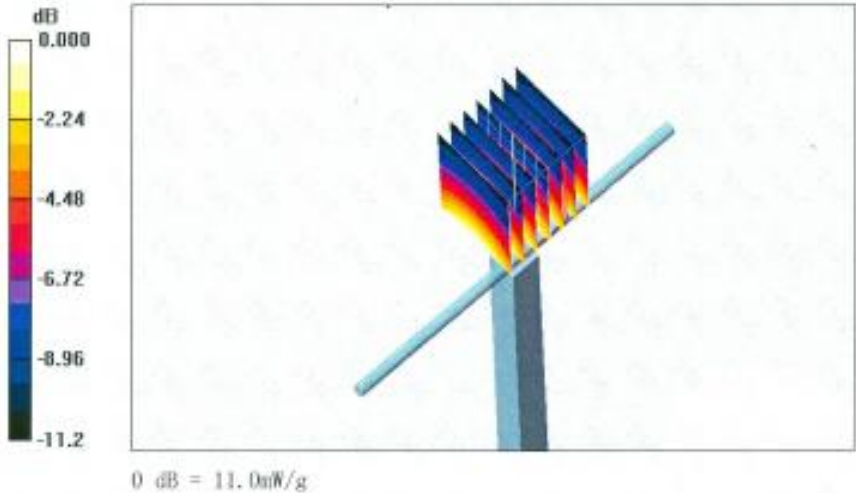




工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Impedance Measurement Plot for Head TSL

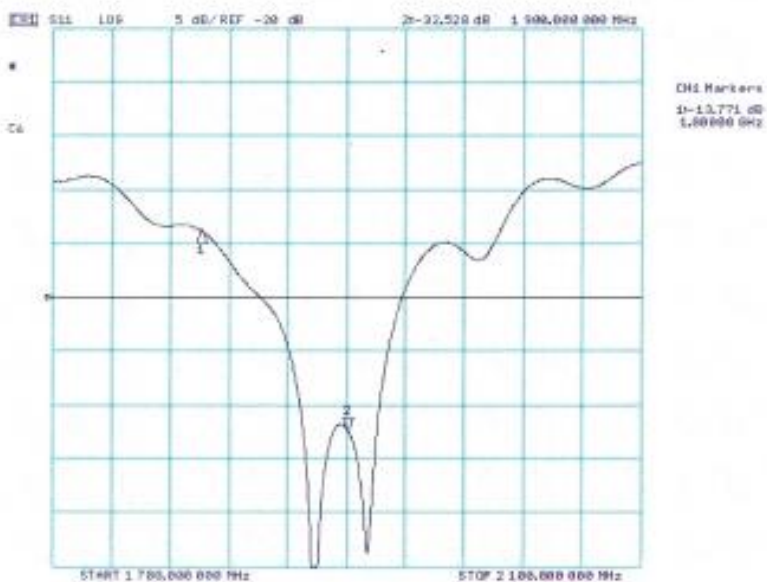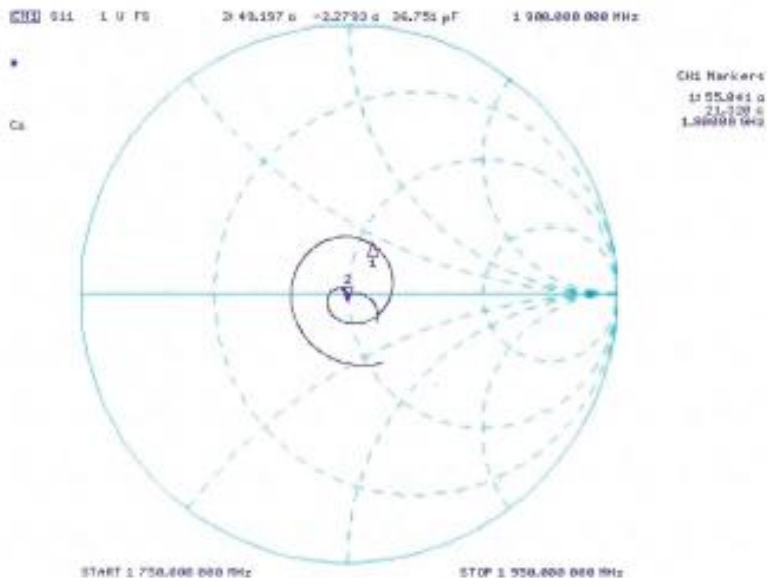

Certificate No: D1900V2-5d091_Feb11

Page 7 of 9



工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



DASY5 Validation Report for Body TSL

Date/Time: 2011-2-23 16:58:35

Test Laboratory: TMC, Beijing, China

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: SN: 5d091

Communication System: CW Frequency: 1900 MHz Duty Cycle: 1:1

Medium: Body 1900MHz

Medium parameters used: $f = 1900 \text{ MHz}$; $\sigma = 1.58 \text{ mho/m}$; $\epsilon_r = 51.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES30V3 - SN3149; ConvF(4.68, 4.68, 4.68); Calibrated: 25.09.10
- Electronics: DAE4 Sn771; Calibration: 21.11.10
- Phantom: 2mm Oval Phantom EL34; Type: QDOVA001BB
- Measurement SW: DASY5, V5.2.157; Postprocessing SW: SEMCAD, V14.0 Build 57

$P_{in}=250\text{mW}$; $d=10\text{mm}$ /Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 55.3 V/m; Power Drift = -0.076 dB

Peak SAR (extrapolated) = 17.15 W/kg

$\text{SAR}(1 \text{ g}) = 10.2 \text{ mW/g}$; $\text{SAR}(10 \text{ g}) = 5.24 \text{ mW/g}$

Maximum value of SAR (measured) = 12.0 mW/g

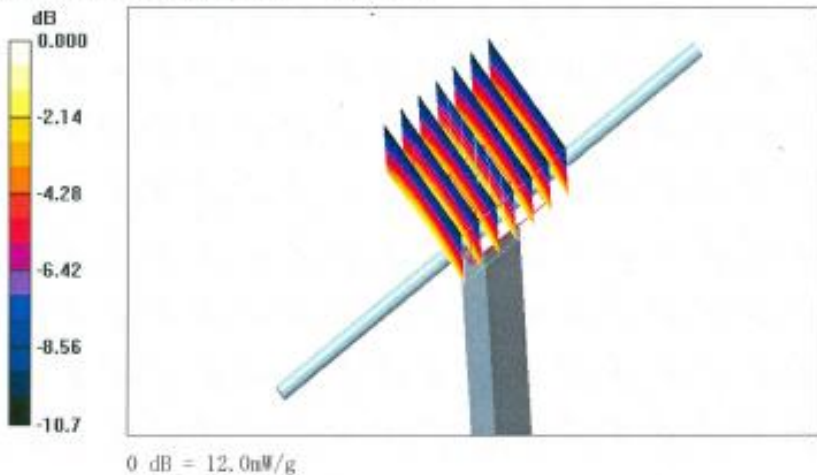




工业和信息化部通信计量中心
Telecommunication Metrology Center of MIIT



Impedance Measurement Plot for Body TSL

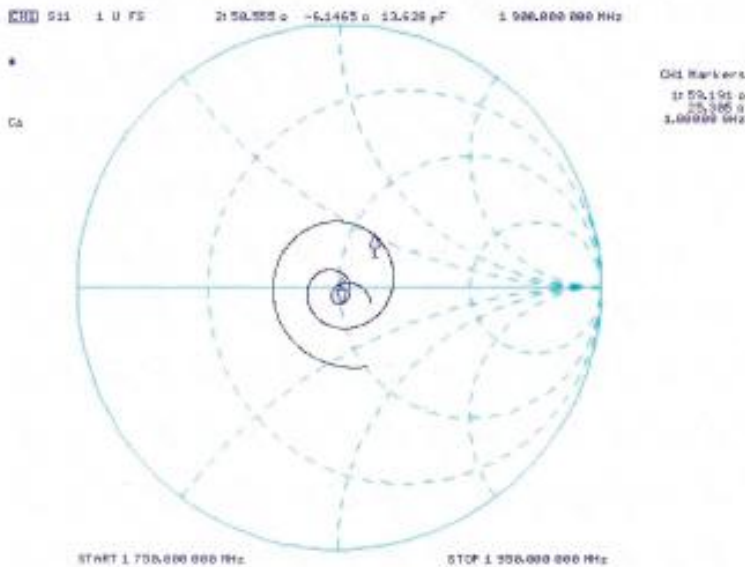



3.4 2450 MHz System validation dipole

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland

S

Schweizerischer Kalibrierdienst

C

Service suisse d'étalonnage

S

Servizio svizzero di taratura

S

Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client: Huawei Shenzhen (Auden)

Certificate No.: D2450V2-860_Mar11

CALIBRATION CERTIFICATE

Object

D2450V2 - SN: 860

Calibration procedure(s)

QA CAL-05.v8
Calibration procedure for dipole validation kits

Calibration date:

March 08, 2011

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GS37483704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01286)	Oct-11
Reference 20 dB Attenuator	SN: 5066 (20g)	30-Mar-10 (No. 217-01156)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES3DV3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390565 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by:

Name

Dirce Ilev

Function

Laboratory Technician

Signature

Approved by:

Name

Katja Pokovic

Technical Manager

issued: March 9, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D2450V2-860_Mar11

Page 1 of 9

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland	 	S Schweizerischer Kalibrierdienst C Service suisse d'étalonnage S Servizio svizzero di taratura S Swiss Calibration Service
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 108
Glossary: TSL tissue simulating liquid ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured		
Calibration is Performed According to the Following Standards: a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005 c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65		
Additional Documentation: d) DASY4/5 System Handbook		
Methods Applied and Interpretation of Parameters: • <i>Measurement Conditions:</i> Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • <i>Antenna Parameters with TSL:</i> The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • <i>Feed Point Impedance and Return Loss:</i> These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • <i>Electrical Delay:</i> One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • <i>SAR measured:</i> SAR measured at the stated antenna input power. • <i>SAR normalized:</i> SAR as measured, normalized to an input power of 1 W at the antenna connector. • <i>SAR for nominal TSL parameters:</i> The measured TSL parameters are used to calculate the nominal SAR result.		
Certificate No: D2450V2-860_Mar11		Page 2 of 9

Measurement Conditions

DASY system configuration, as far as not given on page 1

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.7 $\pm$ 6 %	1.72 mho/m $\pm$ 6 %
Head TSL temperature during test	(21.0 $\pm$ 0.2) °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 mW / g
SAR normalized	normalized to 1W	52.8 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.7 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.19 mW / g
SAR normalized	normalized to 1W	24.8 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.9 mW / g $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.5 ± 6 %	1.92 mho/m ± 6 %
Body TSL temperature during test	(21.0 ± 0.2) °C	-----	-----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.2 mW / g
SAR normalized	normalized to 1W	52.8 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	52.8 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ² (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.13 mW / g
SAR normalized	normalized to 1W	24.5 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	24.5 mW / g ± 16.5 % (k=2)

Appendix**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	$54.0 \Omega + 2.2 j\Omega$
Return Loss	- 27.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$49.0 \Omega + 4.9 j\Omega$
Return Loss	- 26.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.163 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	April 23, 2010

DASY5 Validation Report for Head TSL

Date/Time: 07.03.2011 14:59:52

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:860

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.73$ mho/m; $\epsilon_r = 38.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)


Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 102.4 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 26.918 W/kg

SAR(1 g) = 13.2 mW/g; SAR(10 g) = 6.19 mW/g

Maximum value of SAR (measured) = 16.865 mW/g

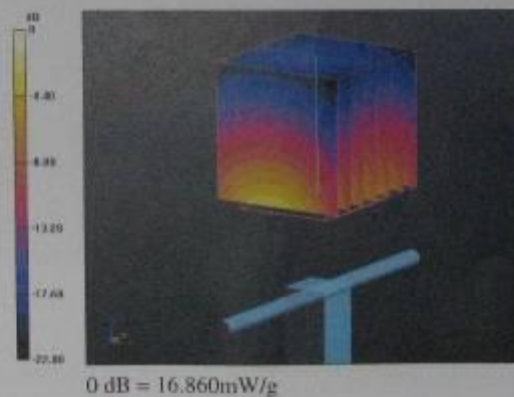

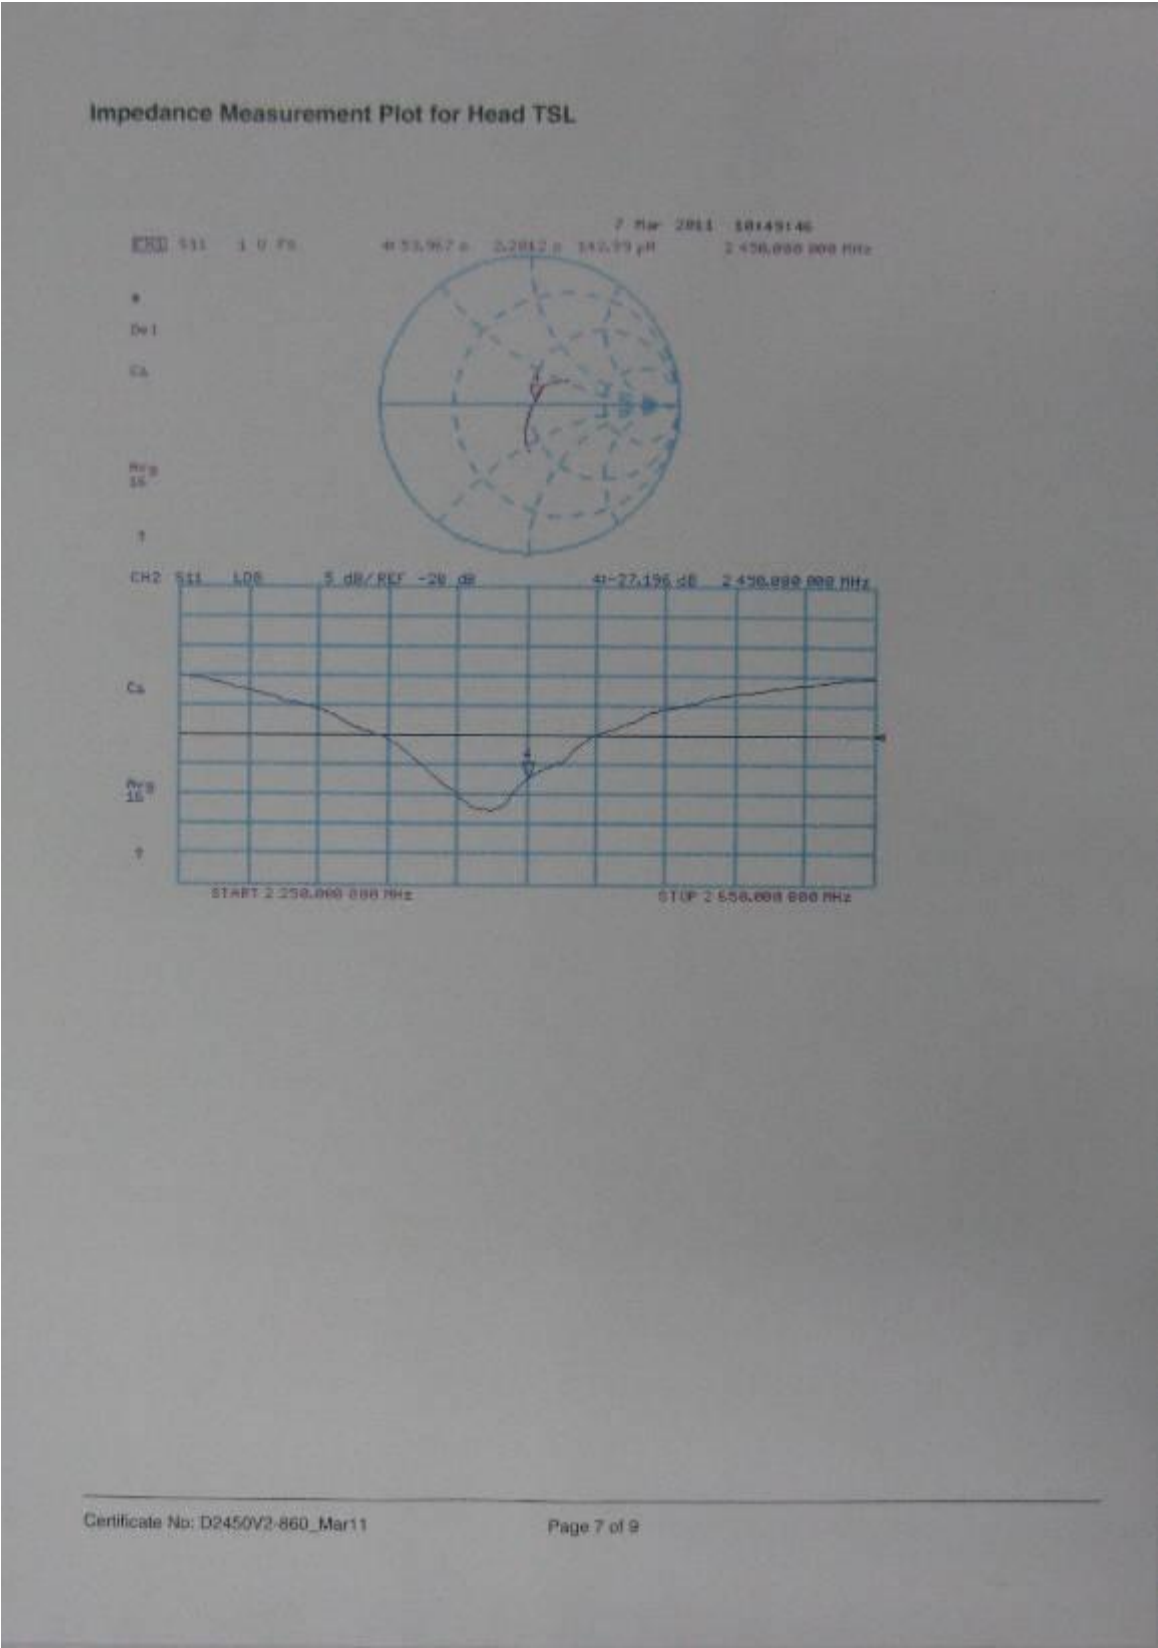

DASY5 Validation Report for Body TSL

Date/Time: 08.03.2011 14:50:47

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:860

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U12 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.93$ mho/m; $\epsilon_r = 51.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY52, V52.6.2 Build (424)
- Postprocessing SW: SEMCAD X, V14.4.4 Build (2829)

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement
grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.448 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 27.953 W/kg

SAR(1 g) = 13.2 mW/g; SAR(10 g) = 6.13 mW/g

Maximum value of SAR (measured) = 17.417 mW/g

