
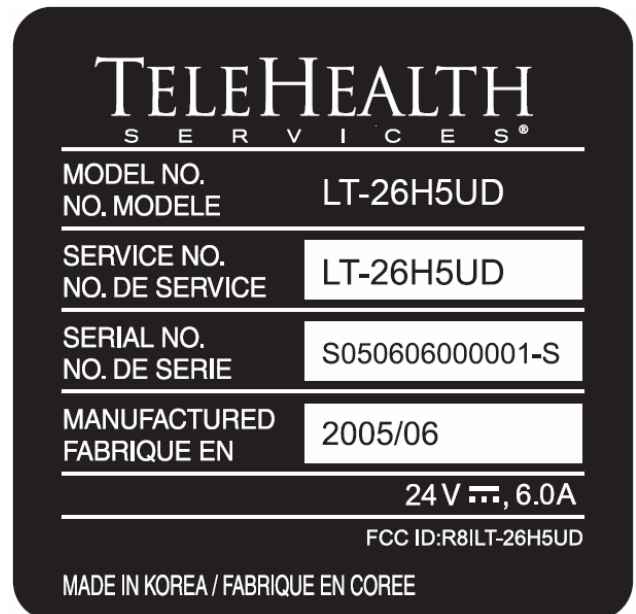


APPENDIX C
: ID SAMPLE LABEL & LOCATION


LABELLING REQUIREMENTS

The label shown shall be permanently affixed at a conspicuous location on the device and be readily visible to the user at the time of purchase.

■ ID Label

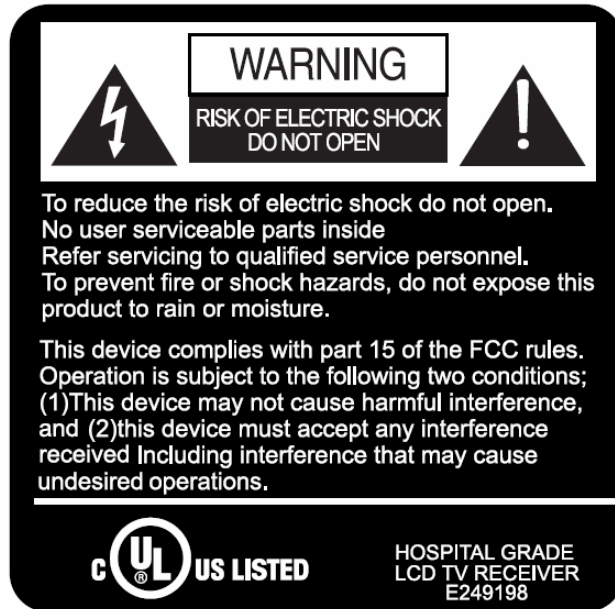

■ ID Label Location of EUT

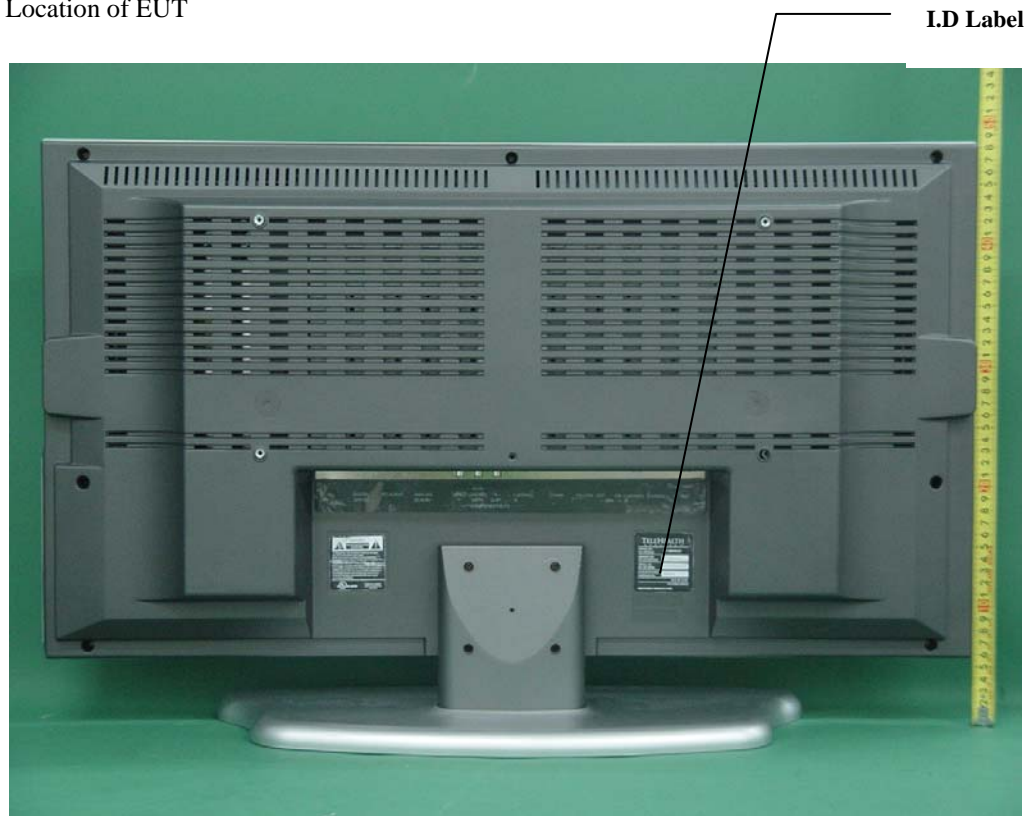

EUT Type: 26" Hospital Grade WIDE LCD TV

FCC ID : R8ILT-26H5UD