

DASY5 Validation Report for Body TSL

Date: 05.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 853

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 50.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.42, 4.42, 4.42); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.672 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 27.2 W/kg


SAR(1 g) = 12.9 W/kg; SAR(10 g) = 5.93 W/kg

Maximum value of SAR (measured) = 16.9 W/kg

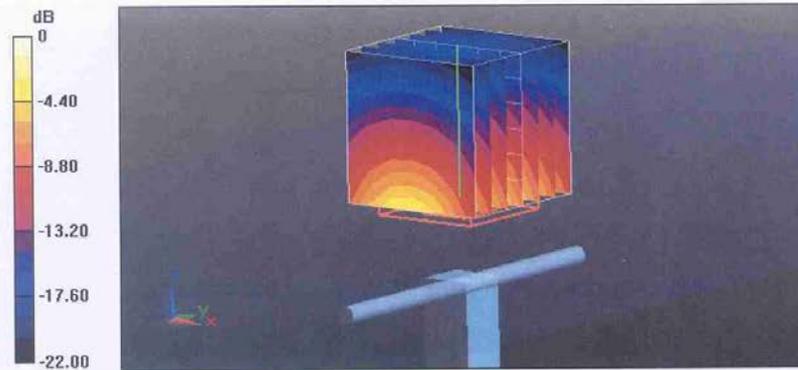

0 dB = 16.9 W/kg = 12.28 dBW/kg

Impedance Measurement Plot for Body TSL

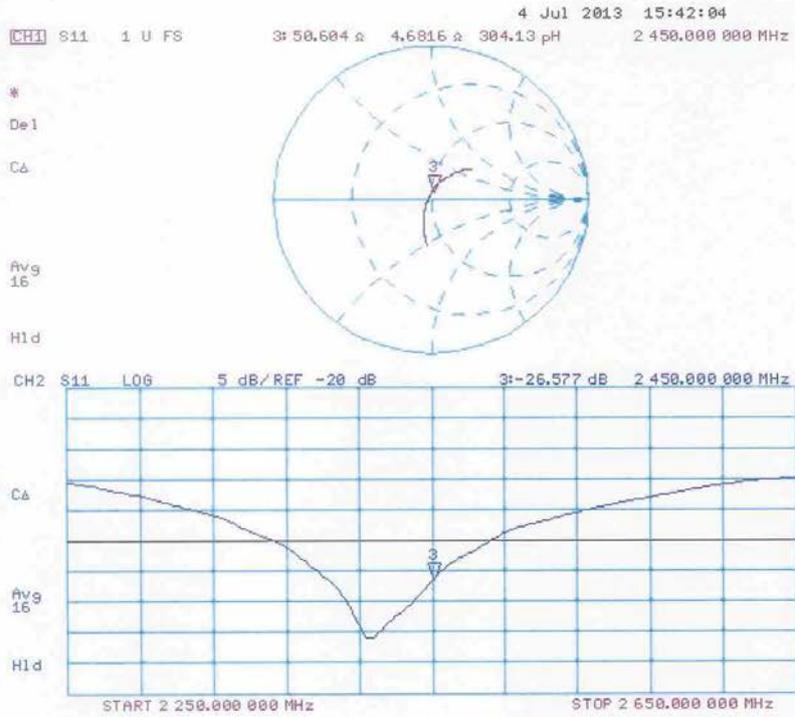

ANNEX I DIPOLE QUALIFICATION FOR THE EXTENDED 3-YEAR CALIBRATION INTERVAL

I1 Dipole 835

The information and documentation below are provided to qualify the extended 3-year calibration interval of dipole.

I1.1 List of Equipment

No.	Name	Type	Serial Number
01	Network analyzer	E5071C	MY46110673
02	Power meter	NRVD	102083
03	Power sensor	NRV-Z5	100542
04	Signal Generator	E4438C	MY49070393
05	Amplifier	60S1G4	0331848
06	E-field Probe	SPEAG EX3DV4	3846
07	DAE	SPEAG DAE4	771
08	Dipole Validation Kit	SPEAG D835V2	443

I1.2 Results of Impedance, Return-loss and System validation

Dipole 835 - Head

		Year		Deviation	Limit
		2012	2013		
Impedance	Real (Ω)	50.8	53.6	2.8 Ω	Deviation < 5 Ω
	Imaginary (Ω)	-6.7	-2.2	4.5 Ω	Deviation < 5 Ω
Return-loss (dB)		-23.5	-23.3	0.2dB	Deviate < 0.2dB
System validation	10g	1.52	1.56	2.63%	Deviation < 10%
	1g	2.33	2.38	2.15%	Deviation < 10%

Dipole 835 - Body

		Year		Deviation	Limit
		2012	2013		
Impedance	Real (Ω)	46.8	49.1	2.3 Ω	Deviation < 5 Ω
	Imaginary (Ω)	-7.8	-3.7	4.1 Ω	Deviation < 5 Ω
Return-loss (dB)		-21.2	-21.4	-0.2dB	Deviate < 0.2dB
System validation	10g	1.59	1.61	1.26%	Deviation < 10%
	1g	2.42	2.42	0.00%	Deviation < 10%

According to the above tables, it is not necessary to recalibration the dipoles in 2013.