
Appendix B – System Check Plots

Test Date : 2024-03-13 | Ambient Temp : 22.4 °C | Tissue Temp : 21.3 °C

System Performance Check**System Performance Check at 2450 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D2450	1087	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	2450.000	8.20	1.87	41.5

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2179	HBBL-600-10000	EX3DV4 - SN7650 / 2023-05-22	DAE4 Sn1741 / 2023-08-23

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	2.41	2.37
psSAR-10g [W/kg]	1.12	1.12
Power Drift [dB]		0.01
TSL Correction	Positive only	Positive only

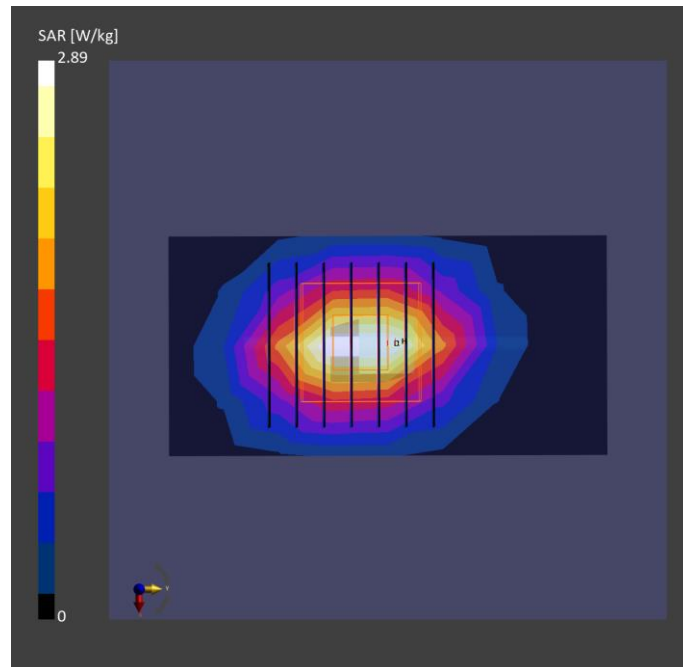

Test Date : 2024-03-14 | Ambient Temp : 22.7 °C | Tissue Temp : 21.2 °C

System Performance Check**System Performance Check at 5250 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHz	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5250.000	5.91	4.61	37.5

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2179	HBBL-600-10000	EX3DV4 - SN7650 / 2023-05-22	DAE4 Sn1741 / 2023-08-23

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.41	3.61
psSAR-10g [W/kg]	1.02	1.06
Power Drift [dB]		0.01
TSL Correction	Positive only	Positive only

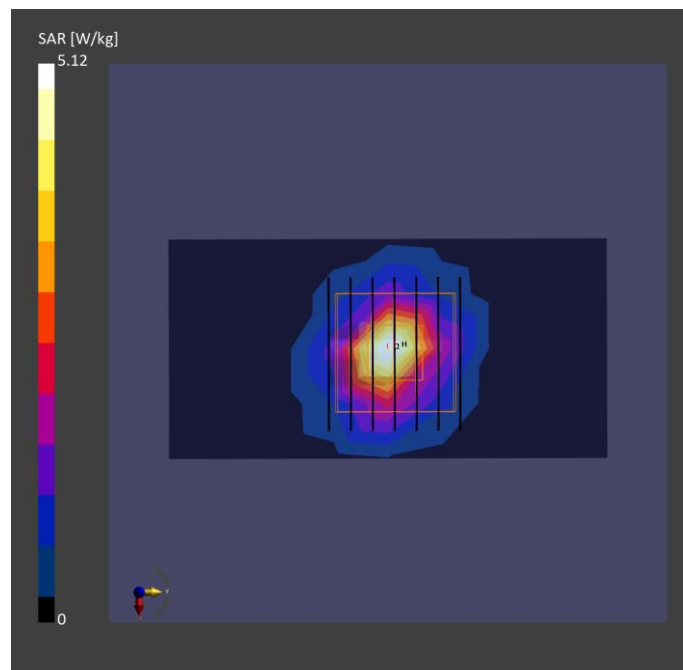

Test Date : 2024-03-15 | Ambient Temp : 22.6 °C | Tissue Temp : 21.1 °C

System Performance Check**System Performance Check at 5600 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHz	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5600.000	5.25	5.02	36.5

Hardware Setup


Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2179	HBBL-600-10000	EX3DV4 - SN7650 / 2023-05-22	DAE4 Sn1741 / 2023-08-23

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.49	3.78
psSAR-10g [W/kg]	1.04	1.08
Power Drift [dB]		-0.04
TSL Correction	Positive only	Positive only

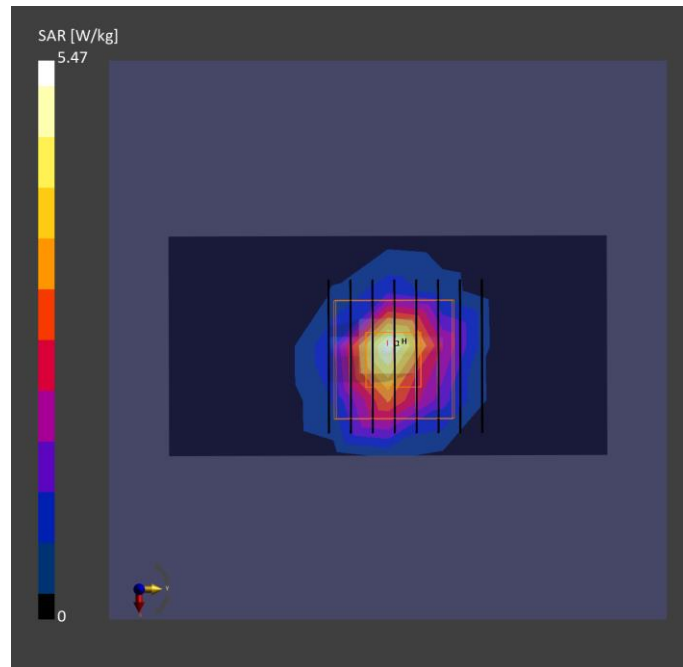

Test Date : 2024-03-15 | Ambient Temp : 22.6 °C | Tissue Temp : 21.1 °C

System Performance Check**System Performance Check at 5800 MHz****Verification Source Properties**

Manufacturer	Model No.	Serial No.	Input Power [dBm]
SPEAG	D5GHz	1358	17.0

Exposure Conditions

Phantom Section	Group	Frequency [MHz]	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	CW	5800.000	5.28	4.96	37.0

Hardware Setup

Phantom	Tissue Simulating Liquid	Probe / Calibration Date	DAE / Calibration Date
ELI V8.0 (20deg probe tilt) - 2180	HBBL-600-10000	EX3DV4 - SN7650 / 2023-05-22	DAE4 Sn1741 / 2023-08-23

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR-1g [W/kg]	3.35	3.68
psSAR-10g [W/kg]	0.989	1.08
Power Drift [dB]		-0.03
TSL Correction	Positive only	Positive only

