

omnipod®
DASH™

INSULIN MANAGEMENT SYSTEM



Podder's handbook

USER GUIDE

Contacts and Important Information

Customer Care

1-800-591-3455 — 24 hours/7 days

1-978-600-7850 when calling from outside the United States of America

Customer Care Fax: 877-467-8538

Website: myomnipod.com

Address: Insulet Corporation

100 Nagog Park, Acton MA 01720

Emergency Services: Dial 911 (USA only; not available in all communities)

PDM Model PDM-USA1-D001-MG-USA1

Serial Number _____

Omnipod DASH™ Insulin Management System Start Date _____

Healthcare Provider

Name _____

Address _____

Phone _____

Email _____

Omnipod® System Trainer

Name _____

Address _____

Phone _____

Email _____

Health Insurance

Name _____

Address _____

Phone _____

Policy Number _____

Pharmacy

Name _____

Address _____

Phone _____

Email _____

© 2018-2020 Insulet Corporation. Omnipod, the Omnipod logo, DASH, the DASH logo, and Podder are trademarks or registered trademarks of Insulet Corporation. All rights reserved. The Bluetooth® word mark and logos are registered trademarks owned by the Bluetooth SIG, Inc. and any use of such marks by Insulet Corporation is under license. Contour is a registered trademark of Ascensia Diabetes Care. All other trademarks are the property of their respective owners. The use of third party trademarks does not constitute an endorsement or imply a relationship or other affiliation. Patent information at www.insulet.com/patents.

Contents

Introductionxi
About This User Guidexi
Indications and Contraindicationsxii
General Warningsxii
Working with Your Healthcare Providerxiii
Safety Featuresxiv

Getting Started

1 Your Omnipod DASH™ Insulin Management System	1
Welcome	1
The Pod and PDM	2
Navigating Screens and Entering Information	4
Touchscreen Basics	4
Entering Numbers and Text	5
Navigation Icons and Navigation Shorthand	7
The Status Bar	9
The PDM's Lock and PIN Screens	10
The PDM's Home Screen	12
Dashboard tab	13
Basal tab / Temp Basal tab	14
Pod Info tab	15
Last BG section	16
Last bolus section	17
Bolus button	17
The Home Page's Menu	18
PDM Messages to You	20
Alarms	20
Notifications	20
Confirmation Messages	20
2 Initial PDM Setup	21
The Omnipod DASH™ PDM Kit	21
Preparing for Your Training	21

Contents

General PDM Settings.....	23
Turning on and personalizing the PDM.....	23
Enter a PIN	24
Set the time zone and time	25
Set the date.....	26
Basal Insulin Settings.....	26
Maximum Basal Rate	26
Create a Basal Program.....	27
Temp basal configuration.....	29
Blood Glucose Settings	30
Upper and lower limits for BG Goal Range.....	30
Pair to a BG meter	31
Bolus Calculator Settings.....	32
Turn the Bolus Calculator on or off.....	32
Target BG and Correct Above values.....	33
Minimum BG for Calcs.....	34
Insulin to Carb Ratio	34
Correction Factor	35
Reverse Correction	35
Duration of Insulin Action.....	35
Other Bolus Settings	36
Maximum Bolus	36
Extended bolus setting.....	36
PDM Setup Complete.....	36

User Guide

3 Changing Your Pod.....	37
Beginning the Pod Change Process	37
First Time Activating a Pod.....	38
Deactivate an Active Pod	38
No Active Pod	39
Preliminary Pod Change Steps.....	40
Fill the Syringe with Insulin.....	41
Fill, Pair, and Apply the Pod	42
Fill the Pod with insulin.....	42
Pair the PDM and Pod	43
Prepare the Pod site	44
Remove the Pod's blue cap	46
Apply the Pod	47
Begin insulin delivery.....	47
Check the Infusion Site.....	48
Avoid Infusion Site Infections	49
More Information about Pod Use.....	50

4 Entering Blood Glucose Readings	51
About Blood Glucose Testing	51
Entering Your Blood Glucose Reading from a Paired BG Meter	51
Entering Your Blood Glucose Reading Manually	53
Tagging Your Blood Glucose Reading	54
How Blood Glucose Readings are Displayed	55
5 Delivering a Bolus of Insulin	57
Bolusing with the Bolus Calculator	57
Enter your meal information	57
Enter your blood glucose reading	58
Delivering an immediate or extended bolus	59
Manually-calculated Bolus	62
Tracking the Progress of a Bolus	64
Altering a Bolus in Progress	65
Using the Food Library	66
Add carbs to the Bolus Calculator	67
Search for a food on the BROWSE list	69
Create a list of favorite foods on the MY FOODS list	70
Removing foods from the MY FOODS list	73
6 Modifying Basal Insulin Delivery	75
Using Temporary Basal Rates	75
Activate a temp basal	75
Activate a temp basal preset	77
Cancel a temp basal	77
Switching to a Different Basal Program	78
Suspending and Resuming Insulin Delivery	79
7 Managing Programs and Presets	81
Basal Programs	81
Create a new Basal Program	81
Review all Basal Programs	82
Edit or rename a Basal Program	83
Delete a Basal Program	85
Temp Basal Presets	85
Create a new temp basal preset	85
Edit or rename a temp basal preset	86
Delete a temp basal preset	87
Bolus Presets	87
Create a new bolus preset	87
Edit or rename a bolus preset	88
Delete a bolus preset	88

Contents

8 Browsing Your PDM Records	89
Notifications & Alarms Screens	89
Overview of the Insulin and BG History Screens	90
Date Selection.....	91
Summary Section.....	92
Details Section	94
Blood glucose details.....	95
Bolus details	95
Carbs details	97
Basal rate details.....	97
Pod details.....	98
Insulin suspended and resumed details	98
Time change details.....	98
Date change details	98
9 Adjusting Settings	99
PDM Device Settings.....	99
Network connectivity	99
Screen display	101
Lock screen	102
Date and time, and language	102
Diagnostics	105
Software update (Wireless update)	106
Pod Sites Setting	108
Reminder Settings	109
Pod expiration	109
Low reservoir level.....	109
Pod Auto-off.....	109
Check BG after Bolus reminders.....	110
Missed bolus reminders	110
Confidence reminders	112
Program reminders.....	112
Custom reminders.....	112
Blood Glucose Settings	114
BG Goal Range.....	114
Pairing, unpairing, or renaming a BG meter	114
Basal and Temp Basal Settings.....	116
Maximum Basal Rate	116
Temp basal	116
Bolus Delivery Settings.....	117
Maximum Bolus	117
Extended bolus.....	117
Bolus Calculator settings	117

Reference

10 Alarms, Notifications, and Communication Errors	121
Overview	121
Responding to Alarms	122
Responding to Notifications	122
Priority and Predictability of Alarms and Notifications	123
Sounds and Vibrations	124
Hazard Alarm List	125
Advisory Alarm List.....	128
Notifications List	129
Informational Signals List	131
Communication Errors.....	132
Error when canceling a bolus	133
Error when sending insulin instructions to the Pod	133
Error when activating a Pod.....	134
Error when deactivating a Pod.....	134
Silencing an Alarm	135
Pod alarm.....	135
PDM alarm.....	135
11 Taking Care of Your PDM and Pod	137
Pod and Insulin Care	137
Pod and insulin storage	137
Pods and the environment.....	137
Cleaning your Pod.....	138
PDM Care.....	138
PDM storage.....	139
PDM and the environment.....	139
Cleaning your PDM.....	140
If you drop the PDM	141
PDM Battery Care	141
Safe use of the PDM battery.....	141
Charging the PDM battery	142
Inserting or replacing the PDM battery	143
12 Understanding PDM and Pod Function.....	145
PDM and Pod Interactions	145
Pod actions controlled by the PDM	145
What the Pod can do between PDM instructions	148
Auto-off.....	148
PDM and Paired BG Meter Interaction.....	149

Contents

Basal Insulin Delivery.....	149
Basal Programs	150
Temporary basal rates	151
Methods to temporarily stop insulin delivery.....	154
Immediate and Extended Boluses.....	155
About Manually-Calculated Boluses.....	155
The Bolus Calculator	156
Bolus Calculator boluses	156
When the Bolus Calculator does not work.....	157
Factors used in the Bolus Calculator's calculations	157
Insulin on board (IOB)	160
Bolus Calculator equations.....	162
Bolus Calculator rules.....	163
Overview of the Bolus Calculator CALCULATIONS screen.....	164
Bolus Calculator examples	166
Calculations for History Summaries	171
Blood glucose summaries.....	171
Insulin delivery summaries.....	172
13 Living with Diabetes.....	173
Daily Activities.....	173
Infusion site checks.....	173
Check your blood glucose frequently.....	174
Prepare for Emergencies	175
Traveling and Vacations.....	175
Keep supplies accessible	176
Plan for changing time zones	176
Airports and flying.....	176
Avoid Lows, Highs, and DKA	178
General precautions.....	178
Hypoglycemia (low blood glucose).....	178
Hyperglycemia (high blood glucose)	181
Diabetic ketoacidosis (DKA).....	184
Handling Special Situations	185
Sick days	185
Exercising, playing sports, or working hard	186
X-rays, MRIs, and CT scans.....	186
Surgery or hospitalization.....	186

Appendix	187
Troubleshooting PDM Startup.....	187
Summary of Settings and Options.....	188
Pod Specifications.....	189
PDM Specifications	191
Protection from Over-infusion or Under-infusion	192
Omnipod DASH™ System Label Symbols	193
Omnipod DASH™ System Notice Concerning Interference.....	194
Electromagnetic Compatibility	194
Customer's Bill of Rights.....	197
Warranty.....	199
HIPAA Privacy Notice.....	202
Glossary	207
Index.....	213

This page intentionally left blank.

Introduction

About This User Guide

Caution: This *User Guide* is intended for use only with Personal Diabetes Manager (PDM) model PDM-USA1-D001-MG-USA1. To learn which version of the PDM you have, turn it over. If you see "PDM-USA1-D001-MG-USA1" on the back of the PDM, this is the correct *User Guide*. If you do not see it, call Customer Care.

Note: Screen images shown in this *User Guide* are examples only and are not suggestions for user settings. Always consult with your healthcare provider to determine the appropriate settings for you.

Healthcare and treatment are complex subjects requiring the services of qualified healthcare providers. This *User Guide* is informational only and not intended as medical or healthcare advice or recommendations to be used for diagnosis, treatment, or for any other individual needs. This *User Guide* is not a substitute for medical or healthcare advice, recommendations, and/or services from a qualified healthcare provider. This *User Guide* may not be relied upon in any way in connection with your personal healthcare, related decisions, and treatment. All such decisions and treatment should be discussed with a qualified healthcare provider who is familiar with your individual needs.

This *User Guide* is periodically updated. Visit www.myomnipod.com to see the most recent version and to find other helpful information. To access the User Guide in Spanish, see www.myomnipod.com.

For instructions about how to use the CONTOUR® NEXT ONE Blood Glucose Monitoring System, see the CONTOUR® NEXT ONE Blood Glucose Monitoring System *User Guide*.

Term	Meaning
Warning	Alerts you to the possibility of injury, death, or other serious adverse reactions associated with the use or misuse of the device.
Caution	Alerts you to the possibility of a problem with the device associated with its use or misuse. Such problems include device malfunctions, device failure, damage to the device, or damage to other property.
Note	Provides helpful information.
Tip	Offers a suggestion for successful use of the device.

Introduction

Indications and Contraindications

Caution: Federal (US) law restricts this device to sale by or on the order of a physician.

Indications for use

The Omnipod DASH™ Insulin Management System is intended for subcutaneous delivery of insulin at set and variable rates for the management of diabetes mellitus in persons requiring insulin.

Additionally, the Omnipod DASH™ System is interoperable with a compatible blood glucose meter to receive and display blood glucose measurements.

Contraindications

Insulin pump therapy is NOT recommended for people who are:

- Unable to monitor blood glucose levels as recommended by their healthcare provider
- Unable to maintain contact with their healthcare provider
- Unable to use the Omnipod DASH™ System according to instructions

General Warnings

Warnings:

Rapid-acting U-100 insulin: The Omnipod DASH™ System is designed to use rapid-acting U-100 insulin. The following U-100 rapid-acting insulin analogs have been tested and found to be safe for use in the Pod: NovoLog® (insulin aspart), Fiasp® (insulin aspart), Humalog® (insulin lispro), Admelog® (insulin lispro), and Apidra® (insulin glulisine). NovoLog, Fiasp, Humalog, and Admelog are compatible with the Omnipod DASH™ System for use up to 72 hours (3 days). Apidra is compatible with the Omnipod DASH™ System for use up to 48 hours (2 days). Before using a different insulin with the Omnipod DASH™ System, check the insulin drug label and consult your healthcare provider. Refer to the insulin labeling and follow your healthcare provider's directions for how often to replace the Pod. Fiasp has a faster initial absorption than other rapid-acting U-100 insulins; always consult with your healthcare provider and refer to the insulin labeling prior to use.

Read all the instructions provided in this *User Guide* before using the Omnipod DASH™ System. Monitor your blood glucose with the guidance of your healthcare provider. Undetected hyperglycemia or hypoglycemia can result without proper monitoring.

Warnings:

Not recommended for individuals with hearing loss. Always verify your ability to hear Pod/PDM alarms and notifications.

If you are unable to use the Omnipod DASH™ System according to instructions, you may be putting your health and safety at risk. Talk with your healthcare provider if you have questions or concerns about using the Omnipod DASH™ System properly.

After use, parts of the device are considered biohazardous and can potentially transmit infectious diseases.

If you are having symptoms that are not consistent with your blood glucose test results and you have followed all instructions described in this *User Guide*, contact your healthcare provider.

The Omnipod DASH™ System should NOT be used at low atmospheric pressure (below 700 hPa). You could encounter such low atmospheric pressures at high elevations, such as when mountain climbing or living at elevations above 10,000 feet (3,000 meters).

The Omnipod DASH™ System should NOT be used in oxygen rich environments (greater than 25% oxygen) or at high atmospheric pressure (above 1060 hPa), both of which can be found in a hyperbaric chamber. Hyperbaric, or high pressure, chambers are sometimes used to promote healing of diabetic ulcers, or to treat carbon monoxide poisoning, certain bone and tissue infections, and decompression sickness.

Working with Your Healthcare Provider

Insulin pump therapy requires substantial caregiver involvement, especially with children. Work with your healthcare provider to establish diabetes management guidelines and settings that best fit your, or your child's, needs. These may include:

Insulin-to-Carbohydrate (IC) Ratio: Number of grams of carbohydrate covered by one unit of insulin. For example, if your Insulin-to-Carbohydrate Ratio is 1 to 15, then you need to deliver one unit of insulin to cover every 15 grams of carbohydrate you eat.

Correction (or Sensitivity) Factor: How much one unit of insulin lowers your blood glucose. For example, if your Correction Factor is 50, one unit of insulin lowers your blood glucose by 50 mg/dL.

Target Blood Glucose (Target BG): The blood glucose level you want to achieve. For example, you may want to keep your blood glucose close to 100 mg/dL.

Duration of Insulin Action: The length of time that insulin remains active and available in your body after a correction or meal bolus.

Introduction

Your healthcare provider is a valuable resource. You will rely on him or her for critical information about your Omnipod DASH™ System, especially during the first few weeks and months. When you have questions about diabetes management after starting on the Omnipod DASH™ System, do not hesitate to talk with your healthcare provider.

For technical questions about your Omnipod DASH™ System setup or operation, or to order Omnipod DASH™ System products and supplies, you can call Customer Care 24 hours a day, 7 days a week. See the first page of this *User Guide* for your Customer Care contact information.

For technical questions about your CONTOUR® NEXT ONE Blood Glucose Monitoring System setup or operation, or to order CONTOUR® NEXT ONE BG meter products or supplies, see the CONTOUR® NEXT ONE instructions for use for Customer Service contact information.

Your healthcare provider will give you all the tools and training you need to be successful with the Omnipod DASH™ System. As you become actively involved in your diabetes management, you can enjoy the flexibility that is possible with the Omnipod DASH™ System.

Being actively involved means to frequently monitor your blood glucose levels, to learn how to operate your Omnipod DASH™ System, to practice proper techniques, and to visit your healthcare provider regularly.

Safety Features

The Omnipod DASH™ System's safety features include:

Automatic priming, safety checks, and insertion

When you activate a new Pod, the Omnipod DASH™ System automatically primes and performs safety checks on the Pod, then inserts and primes the cannula (a small, thin tube). These safety checks take only a few seconds.

The Omnipod DASH™ System also performs safety checks on the Personal Diabetes Manager (PDM) whenever the PDM is awake. If it detects any problems in the PDM or the Pod—or in the communication between them—it informs you with vibrations or beeps and on-screen messages.

Alarms and notifications

For your safety, the Omnipod DASH™ System provides a range of alarms and notifications to tell you that your attention is needed or to warn you of hazardous situations. For a description of the PDM's alarms and notifications, see "Alarms, Notifications, and Communication Errors" on page 121.

Note: Brief alarm and notification messages appear on the Lock screen. You must unlock the screen and enter your personal identification number (PIN) to see the full alarm messages.

Note: Wake up your PDM periodically to confirm that there are no notification or alarm messages that require a response.

Warning: Do NOT attempt to use the Omnipod DASH™ System before you receive training. Inadequate training could put your health and safety at risk.

Software updates

Occasionally, an update may be provided for the PDM software. The PDM periodically checks for software updates if Wi-Fi is on. For information about checking for and installing software updates, see "Software update (Wireless update)" on page 106.

This page intentionally left blank.

CHAPTER 1

Your Omnipod DASH™ Insulin Management System

Welcome

The Omnipod DASH™ Insulin Management System is a continuous insulin delivery system that provides all the proven benefits of continuous subcutaneous insulin infusion (CSII) therapy.

Features of the Omnipod DASH™ System include:

No tubing: There is no tubing connecting the Pod to the Personal Diabetes Manager (PDM). You can wear the Pod under your clothes and carry the PDM separately. You can swim wearing the Pod and leave the PDM on dry land. The Pod is waterproof to 25 feet (7.6 meters) for up to 60 minutes (IP28).

Bolus Calculator: If your blood glucose is high or if you are planning to eat, the PDM's Bolus Calculator can suggest a bolus dose based on your individual settings.

Glucose readings: Your PDM can pair to and record blood glucose readings from the CONTOUR® NEXT ONE BG meter via Bluetooth® wireless technology. While the CONTOUR NEXT ONE BG meter is the only BG meter compatible for pairing to the PDM, you can also manually enter blood glucose readings from any BG meter into the PDM.

Recordkeeping: The PDM displays up to 90 days of information, including basal rates, bolus doses, carbohydrates, alarms, and blood glucose entries.

The *Getting Started* section of this book gives an overview of the basic operation and setup of the Omnipod DASH™ System. The *User Guide* section gives step-by-step instructions for using the Omnipod DASH™ System. The *Reference* section explains how the Omnipod DASH™ System works.

Terms and conventions used in this *User Guide*

Screen	Area of the PDM that displays menus, instructions, and messages.
Menu	List of options on the screen.
Icon	An image on the screen that indicates a menu option or that provides information.
Button	Physical buttons on the PDM, such as the Power button. Also, areas of the screen that you can tap to perform an action.
Field	The area of a screen where you enter information.

1 Omnipod DASH™ Insulin Management System

The Pod and PDM


The Omnipod DASH™ System is made up of two primary parts: The Pod, which delivers insulin to your body, and the Personal Diabetes Manager (PDM), which lets you control the Pod.

The Pod

The Pod is a lightweight device that you fill with insulin and wear directly on your body. The Pod receives insulin delivery instructions from the PDM. The Pod then delivers insulin into your body through a small, flexible tube called a cannula.

The Pod is applied to your skin with an adhesive, similar to an adhesive bandage.

The Pod that is used with the Omnipod DASH™ System has a blue needle cap.

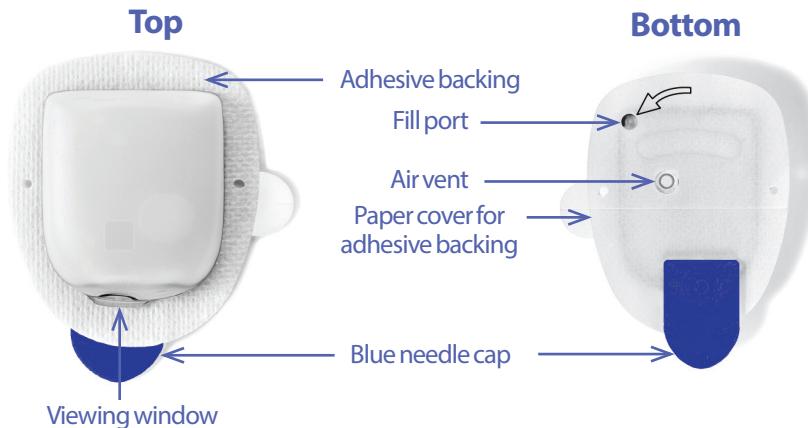

Omnipod DASH™ Insulin Management System 1

The Personal Diabetes Manager (PDM)

The PDM is a handheld device that controls and monitors the Pod's operations using wireless technology.



Navigating Screens and Entering Information

This section explains how to use the touchscreen, how to enter numbers or text into the PDM, and how this *User Guide* describes moving between PDM screens.

Touchscreen Basics

The PDM displays messages and options for you on its touchscreen. You communicate with the PDM by tapping or swiping your finger on the touchscreen.

Tapping and swiping

The basic instructions for interacting with the touchscreen are explained here.



Tap

Touch the screen, then lift your finger up.



Swipe

Touch a starting point and move your finger up, down, left, or right.

Note: Scrolling and swiping are related actions. When you swipe up, the screen display scrolls up to show items that are currently off-screen.

Note: A screen protector may decrease the touchscreen sensitivity.

Screen time-out and brightness

The PDM screen turns black, called timing-out, after a period of inactivity. To control the screen time-out and brightness settings, see "Screen display" on page 101. The PDM screen dims 6-10 seconds before it times out. If the screen dims, touch the screen briefly to prevent the screen from timing out.

Entering Numbers and Text

Tapping fields to enter data

Fields allow you to specify values to be used by the PDM. Tapping an editable field (which is either framed by a box or underlined) opens a keypad, number pad or scroll wheel. Tap the letters or numbers or scroll the wheel to enter data for use in that field.

8 g ← Editable fields are underlined or framed by a box.

1 ← Non-editable fields are not underlined or framed by a box.

Tapping blue and underlined text brings up a screen where you can view an explanation or enter data.

Using a keypad

Tapping in an editable field brings up a keypad. To bring up a different keypad, tap the ?123, ABC, or =< in the lower left of a keypad.



Tap a character to add it to the text field.

Touch a letter in the top row for a second to display other options such as a number or an accented letter such as é.

Tap the up-arrow () to toggle between uppercase and lowercase letters. Tap the up-arrow twice in rapid succession to type in ALL CAPITALS mode. Tap the up-arrow one more time to exit ALL CAPITALS mode.

Tap the spacebar icon () to add a space between characters.

Tap the backspace icon () to delete the most recent entry from the entry field.

Tap the green checkmark () to close the keypad when you have finished entering your text.

~ ` | . √ π ÷ × ¶ Δ
£ ¢ € ¥ ^ ° = { }
?123 \ © ® ™ % [] ✖
ABC , < [] > . ✓

Note: The PDM considers CAPITAL and lowercase letters to be the same. In other words, the PDM considers "WEEKEND" and "weekend" to be the same name.

1 Omnipod DASH™ Insulin Management System

Using a number pad

1	2	3	-
4	5	6	,
7	8	9	☒
.	0	—	✓

Tap a number to add it to the entry field. Tap the period (.) to add a decimal point. Tap the backspace icon (☒) to delete the most recent entry from the entry field. The comma (,), dash (-), and underscore (_) are not used.

Tap the green checkmark (✓) to accept the entered number. You can also tap outside the number pad to accept the entered number.

Using a scroll wheel


0.85	U/hr
0.80	U/hr
0.75	U/hr
0.70	U/hr
0.65	U/hr

Place your finger on the scroll wheel. Move your finger up to select a smaller number and down to select a larger number. The faster you move your finger, the faster the wheel will scroll.

When your desired selection is shown in the center of the wheel, select the value by tapping it or by tapping outside the scroll wheel.

Using a slider

Use sliders to select a value from a scale. Place your finger on the small open circle and move your finger until your desired value is displayed. Depending on the on-screen graphic, you may move your finger vertically or in a circle to move the slider. Move your finger up or clockwise for a larger number and down or counterclockwise for a smaller number. Lift your finger when the desired value is displayed.

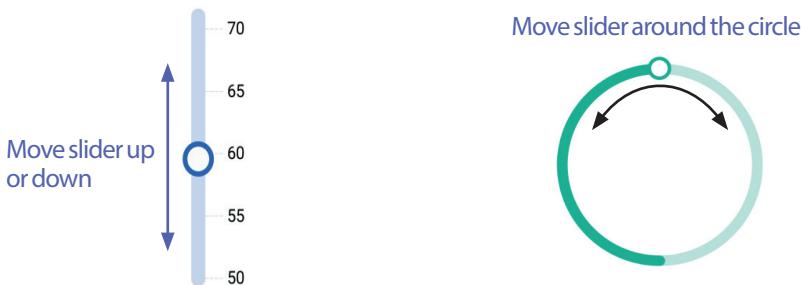

Selecting, Adding, and Deleting Items

Toggles

-  Tap a toggle to change the selection from one side to the other.
-  Toggles allow you to choose between two options or to turn a feature on or off. The toggle is on the right side and blue when a feature is on, and on the left and gray when a feature is off.


Checkboxes, radio buttons, and drop-down lists



Checkboxes are squares. Tap a checkbox to check or uncheck it. You can check more than one checkbox in a list.



Radio buttons are circles. Tap a radio button to select it. A dot appears inside the selected radio button. You can select only one radio button at a time. To deselect a radio button, tap the radio button next to a different option.

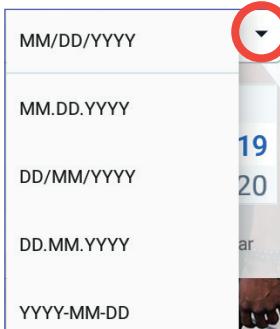

Drop-down lists are indicated by a down or up arrow next to an item. The currently selected setting appears to the left of the drop-down arrow. To select a different option, tap the down arrow to show the drop-down list of options. To replace the currently selected option at the top, tap the desired option from the drop-down list.

Tap the up arrow to hide the list of options.



A plus symbol in a circle indicates that you can add an item to a list. Tap the plus symbol to add the item to the list.



A red x in a circle indicates that you can remove an item from a list. To remove the item, tap the red x.

Navigation Icons and Navigation Shorthand

The PDM has buttons below the screen that can be used for navigation. In addition, some screen icons can be used for navigation.

Back arrow and back button

Many screens display a "back" arrow icon in the upper left corner.

Tapping the back arrow returns to the previous screen.



Tapping the left-hand button below the PDM screen generally also returns to the previous screen.



Note: The middle and right-hand buttons below the PDM screen have no function.

Options icon



The Options icon (⋮) appears on the right-side of certain lists. Tapping the Options icon brings up a list of options relevant to the item on that row.

1 Omnipod DASH™ Insulin Management System

Navigation shorthand

The *User Guide* uses the ">" symbol to indicate navigating from one screen to another. For example, the following notation:

- Menu icon (≡) > Pod > CHANGE POD

tells you to:

1. Tap the Menu icon (≡) in the upper left of the Home screen.
2. Tap Pod to open the Pod screen.
3. Tap CHANGE POD.

- Menu icon (≡) > History:Insulin & BG History

tells you to:

1. Tap the Menu icon (≡) in the upper left of the Home screen.
2. Expand the History entry, if it is collapsed, by tapping anywhere in the row with the word "History."

When expanded, selections for the Notifications & Alarms history screen and the Insulin & BG History screen appear.

3. Tap Insulin & BG History.

- Settings icon (⚙) > Reminders > Pod Expiration


tells you to:

1. Tap the Settings icon (⚙) in the upper right of the Home screen.
2. Tap Reminders.
3. Tap Pod Expiration.

The Status Bar

Most screens have a status bar that shows you:

- The Pod status, including how much insulin is left in an active Pod
- Whether a temp basal rate is running
- Whether the PDM will vibrate for selected notifications
- The Bluetooth® icon
- If Wi-Fi is on, the strength of the Wi-Fi signal
- The status of the PDM's battery
- The current time

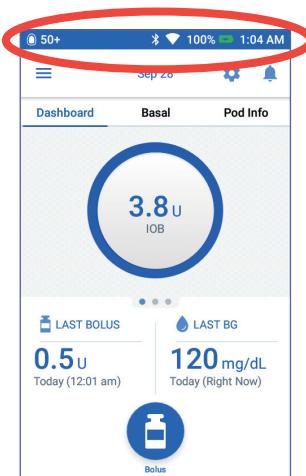

Status bar icon definitions:

 More than 50 units in Pod

 Airplane mode on

 Between 50 and 26 units in Pod

 Vibration mode on

 Between 25 and 5 units in Pod

 Bluetooth® setting on

 Less than 5 units in Pod

 Wi-Fi on: strong signal

 PDM unable to communicate with Pod; units in Pod shown as " - " when unable to communicate.

 Wi-Fi on: good signal

 No active Pod

 Wi-Fi on: fair signal

 Temp basal rate active

 Wi-Fi on: low signal

 Wi-Fi on: no signal

The PDM's battery icons, during normal operation and while charging, are:

  100% to 31% charge

  30% to 16% charge

  15% to 0% charge

1 Omnipod DASH™ Insulin Management System

For charging instructions, see "Charge the battery" on page 22.

The PDM's Lock and PIN Screens

After you set up your PDM, the Lock and PIN screens appear whenever you wake up your PDM. The Lock and PIN screens help confirm that you are using the correct PDM.

The Lock screen displays:

- Your selected background image
- Your customized message
- The amount of insulin on board, if the Bolus Calculator is on
- Today's date
- Any alarm or notification messages


Warning: Always identify the PDM as yours before using it. Using someone else's PDM can result in incorrect insulin delivery for both of you.

Unlock your PDM

In the remainder of this *User Guide*, instructions to "wake up" or "unlock" the PDM mean to do the following:

1. Press the Power button briefly. See the PDM image on page 3 for the location of the Power button.
2. Unlock the Lock screen by either swiping left to right or by swiping up from the bottom. The PIN screen appears.
3. Enter your 4-digit PIN.
4. Tap the checkmark. The Home screen or your most recent screen appears.

Note: If a hazard alarm or an advisory alarm is occurring, the alarm message appears.

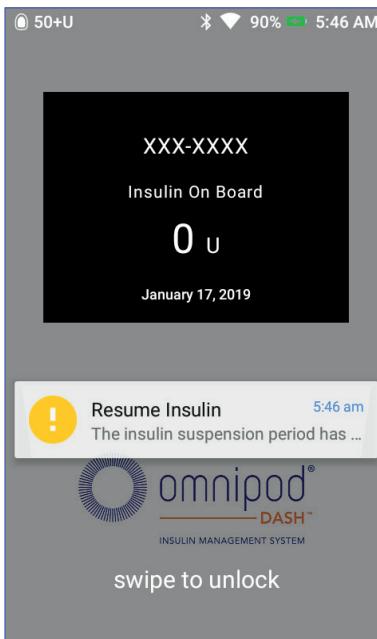

Lock your PDM

To lock your PDM when you are finished using it:

1. Press the Power button briefly. This locks the PDM by putting it to sleep.
2. Store your PDM in a safe, accessible location.

Caution: Only press the Power button briefly. If the PDM asks if you would like to "Power off," tap outside the message to cancel the instruction. Once you begin using your PDM, do not turn the power off. The PDM can sound an alarm only when powered on.

Forgot your PIN?

You can use the last four digits of the PDM's serial number as an alternate PIN:


1. Find the serial number next to the **SN** icon on the back of your PDM.
2. Note the last four digits of the serial number.
3. Enter those four digits on the PIN screen and tap the checkmark.

If you have problems with your PIN, call Customer Care.

1 Omnipod DASH™ Insulin Management System

The PDM's Home Screen

The Home screen provides information about recent boluses, blood glucose values, the active basal rate, and the active Pod. It also provides access to the PDM functions, alarm information, and settings. The Home screen also has a Bolus button to give quick access to the bolus screen.

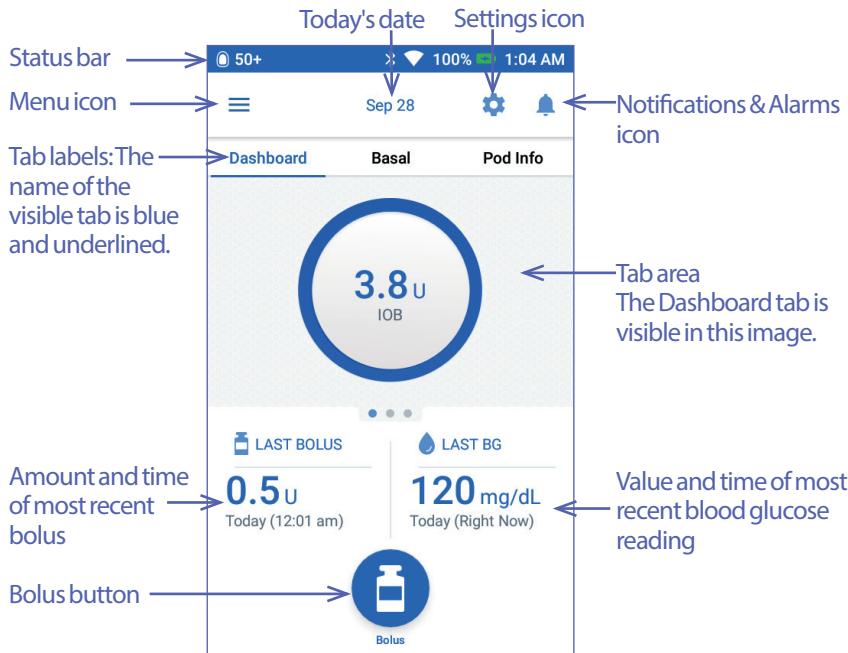

The tab area of the Home screen can display bolus information on the Dashboard, basal information, or Pod information. To change which information is displayed:

- Tap Dashboard, Basal, or Pod Info to display each tab.
- Swipe right or swipe left in the middle section to move between the tabs.

Note: If an immediate bolus is running, a bolus progress bar is shown on the Home screen, and the Bolus button and three tabs are not visible (see "Immediate bolus progress" on page 64). A button to cancel the bolus is visible.

Dashboard tab

The Dashboard tab is available if the Bolus Calculator is on and is usually not available if the Bolus Calculator is off.

When the Bolus Calculator is on


When the Bolus Calculator is on, the Dashboard tab displays:

- IOB (insulin on board), when IOB is available.
- IOB is Not Available, when the Bolus Calculator is disabled. Tap the  icon for a list of reasons for the Bolus Calculator to be disabled.

A progress bar appears when a bolus is in progress (see "Tracking the Progress of a Bolus" on page 64).

When the Bolus Calculator is off

When the Bolus Calculator is off, there are usually only two tabs: Basal and Pod Info. The Dashboard tab displays only when an extended bolus is running (see "Tracking the Progress of a Bolus" on page 64).

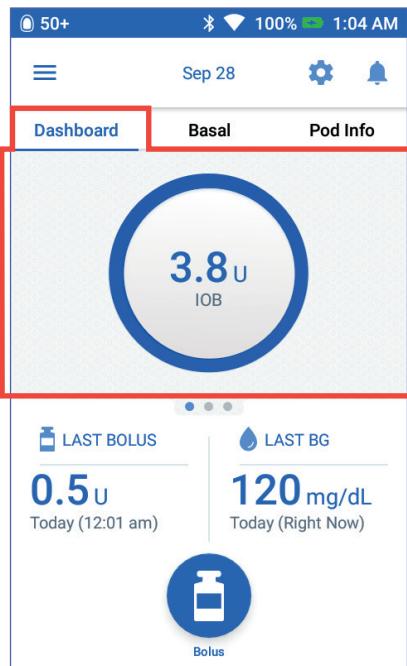

1 Omnipod DASH™ Insulin Management System

Basal tab / Temp Basal tab

This tab is labeled Basal or Temp Basal, depending on whether a Basal Program or temp basal is active.

Basal Program

By default, the Basal tab shows the name and graph of the active Basal Program.

A label below the Basal Program's name indicates whether the listed Basal Program is:

- Active—This program is running on the active Pod.
- Suspended—This program will resume when you resume insulin delivery.
- Current—There is no active Pod. This program will be sent to your next Pod during activation.

When there is an active Basal Program, a green line marks the current time. The numbers above the graph indicate the basal rate for each time segment.


The total daily amount of basal insulin is shown beneath the graph.

This total is the amount of insulin that the active Basal Program is scheduled to deliver in a 24-hour period. This total does not account for temp basals or boluses. To see the total amount of insulin that your Pod has actually delivered, including temp basals and boluses, see "Overview of the Insulin and BG History Screens" on page 90.

Tap **VIEW** to see details about other Basal Programs (see page 81).

Temp basal

If a temp basal is running, the Basal tab is labeled Temp Basal and is highlighted in green. It displays the temp basal graph and allows you to cancel the temp basal.

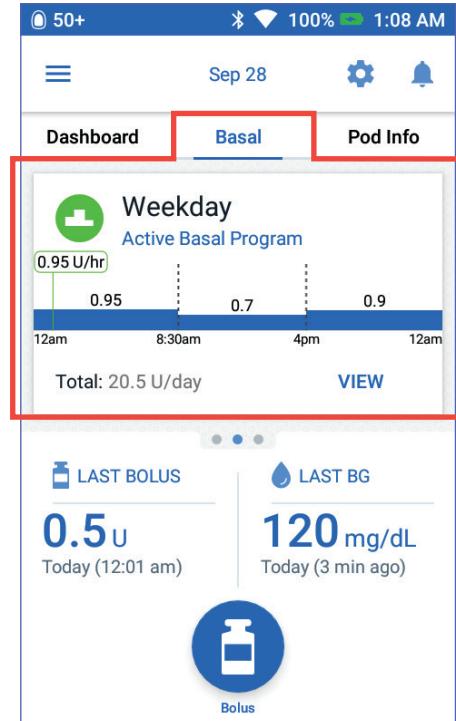

Pod Info tab

The Pod Info tab shows whether there is an active Pod, and, if so, how much insulin is left in the Pod and when the Pod will expire.

If the PDM cannot communicate with an active Pod, the Pod Info tab says "No Pod Communication." Tap the  icon for a list of reasons why the PDM may not be able to communicate with the Pod.

Note: Even when there is no communication, the Pod continues delivering insulin according to the instructions it was given. See "What the Pod can do between PDM instructions" on page 148 for details.

Tip: *Bringing the PDM and the active Pod within 5 feet of one another may quickly restore their communication.*



If there is no active Pod, the Pod Info tab says "No Active Pod." To set up a new Pod, see "Changing Your Pod" on page 37.

If there is an active Pod, tap VIEW POD DETAILS to bring up a screen that lets you deactivate or change your Pod.

The VIEW POD DETAILS screen shows:

- Amount of insulin in the Pod.
- Time of the last successful communication between the PDM and Pod.
- Date and time of the Pod's expiration.
- Any active reminders.
- A CHANGE POD button.

Tip: *You can also access this screen by tapping Menu icon (≡) > Pod.*

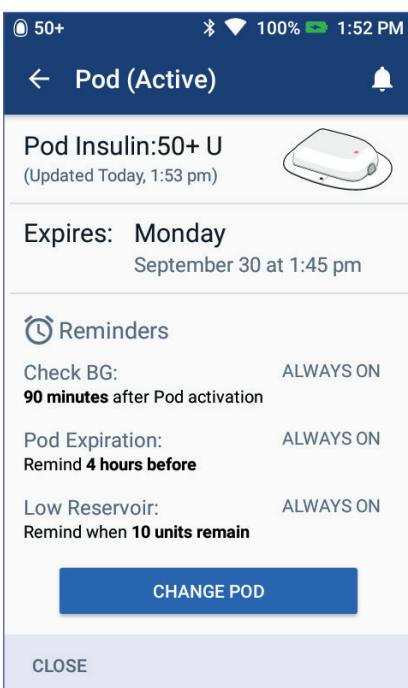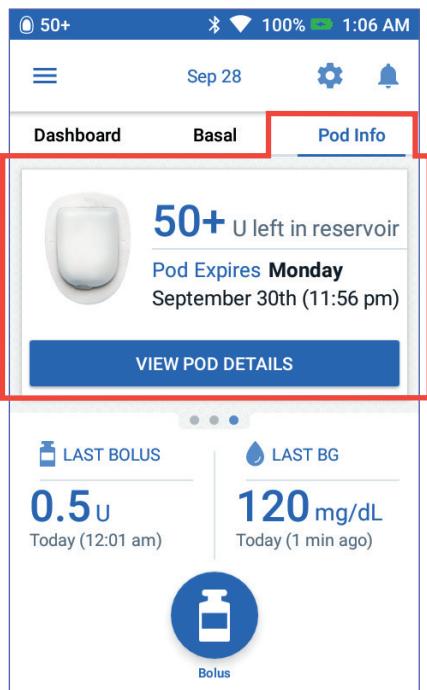

1 Omnipod DASH™ Insulin Management System

When your Pod will expire soon, a yellow Change Pod soon banner appears on the Pod Info tab. The yellow banner appears 12 hours before Pod expiration or at the time of your Pod expiration reminder, whichever is earlier.



Dashboard Basal Pod Info

Change Pod soon

27 U left in reservoir

Pod Expires Today
September 28th (1:20 pm)

VIEW POD DETAILS

At six hours before Pod expiration, a red Change Pod banner appears on the Pod Info tab.



Dashboard Basal Pod Info

Change Pod


15 U left in reservoir

Pod Expires Today
September 28th (7:18 am)

VIEW POD DETAILS

When less than five units of insulin remain in the Pod, a red Low Reservoir banner appears on the Pod Info tab. If the Pod will expire soon and there are less than five units of insulin in the Pod, the red Low Reservoir banner is displayed on the Pod Info tab.

Note: If you change the date or time, the Pod expiration date and time are adjusted to match the new date and time.

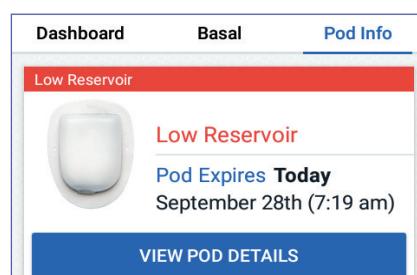

Dashboard Basal Pod Info

Low Reservoir

Low Reservoir

Pod Expires Today
September 28th (7:19 am)

VIEW POD DETAILS

Last BG section

The lower right side of the Home screen displays the value and time of your most recent blood glucose reading.



LAST BOLUS
0.5 U
Today (12:01 am)


LAST BG
120 mg/dL
Today (Right Now)

Last bolus section

The lower left side of the Home screen displays bolus information.

Between boluses

When a bolus is not being delivered, the section is labeled LAST BOLUS and shows the amount and time of the most recent bolus.

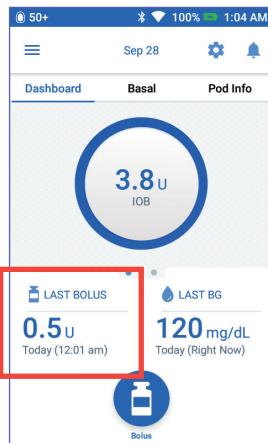

During a bolus when the Bolus Calculator is on

When a bolus is being delivered and the Bolus Calculator is on, the last bolus information is replaced by an estimate of the Insulin on Board (IOB):

- During an immediate bolus, the IOB estimate is updated every ten seconds.
- During an extended bolus, the IOB estimate includes IOB from previous boluses, an estimate of the amount already delivered from the ongoing bolus, and the amount projected to be delivered within the time period defined by your Duration of Insulin Action setting.

During a bolus when the Bolus Calculator is off

When a bolus is being delivered and the Bolus Calculator is off, the lower left of the screen shows the amount of the preceding bolus (not the ongoing bolus).

Bolus information if the PDM cannot communicate with the Pod

If the Pod is out of range of the PDM, and the PDM cannot confirm the recent bolus amount, an estimated bolus amount is shown. Once the Pod is in range again and the bolus delivery is confirmed, the confirmed bolus amount is shown.

Estimated and unconfirmed bolus amounts

The PDM estimates bolus amounts during an ongoing bolus and when the Pod is out of range. A gray icon (⚠) marks estimated bolus amounts. A yellow icon (⚠) marks unconfirmed bolus amounts (see "When the Pod has not confirmed bolus delivery" on page 97).

Bolus button

The Bolus button at the bottom of the Home screen provides access to the bolus screen. The Bolus button does not appear while an immediate bolus is being delivered, or when the Bolus Calculator is off and there is no active Pod.



1 Omnipod DASH™ Insulin Management System

The Home Page's Menu

The Menu on the Home page lets you access most of the PDM's functions. To display the Menu:

- Tap the Menu icon (≡) in the upper left corner of the Home screen.
- Place your finger on the far left of the PDM, and swipe right across the screen. Swipe left to hide the Menu.

Tap an option on the Menu to bring up the related screen.

Tip: *The Menu extends beyond the bottom of the screen. Swipe up or down to see all parts of the Menu.*

Frequent tasks

The first section of the Menu gives access to frequent tasks: activating a temp basal, changing your Pod, entering a blood glucose reading, and suspending or resuming insulin.

Special situations:


- Set Temp Basal is grayed-out if there is no active Pod, insulin is suspended, or a temp basal is already running.
- Set Temp Basal does not appear if the temp basal setting is turned off.
- Suspend Insulin changes to Resume Insulin if insulin delivery is suspended.
- Suspend Insulin is grayed-out if there is no active Pod.

Manage Programs & Presets

The next section allows you to create or activate Basal Programs, temp basal presets, and bolus presets (see "Managing Programs and Presets" on page 81).

Special situations:

- Temp Basal Presets is only visible if the temp basal setting is on.
- Bolus Presets is only visible if the Bolus Calculator setting is off.

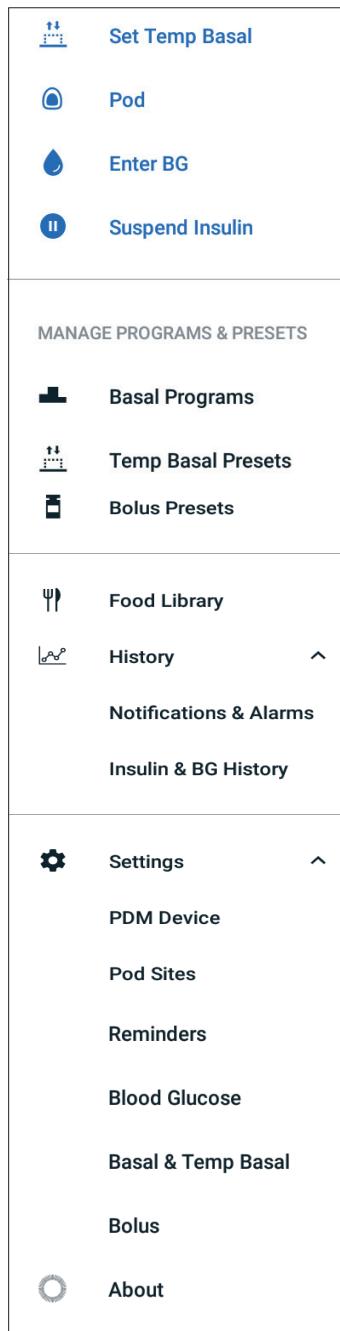

Food library

The Food Library option allows you to look up the carbohydrate content of various foods and to create food favorites (see "Using the Food Library" on page 66).

History menu

Tap the down arrow (▽) next to History to reveal the submenu:

- Notifications & Alarms history (see page 89)
- Insulin & BG History (see page 90)

Tip: Tap the bell icon (🔔 or 🔔 4) at the top-right of many screens to open the Notifications & Alarms history screen.

Settings menu

Tap the down arrow (▽) next to Settings to reveal the submenu:

- PDM Device
- Pod Sites
- Reminders
- Blood Glucose
- Basal & Temp Basal
- Bolus

Tip: Tap the Settings icon (⚙️) at the top of the Home screen to open the Settings portion of the Menu.

These settings allow you to change the time and date, turn Wi-Fi on or off, create or remove reminders, pair to a BG meter, turn the Bolus Calculator on or off, and much more. For more information, see "Adjusting Settings" on page 99.

About screen

The About screen displays details about your PDM, such as the software revision number, the Customer Care phone number, the PDM serial number, the Pod version number, the time of the most recent PDM-Pod communication, and other device and legal information.

Note: You can also find the PDM's serial number next to the **SN** icon on the back of your PDM.

1 Omnipod DASH™ Insulin Management System

PDM Messages to You

The PDM can deliver alarm messages, notifications, and confirmation messages.

Alarms

Hazard alarms and advisory alarms require your immediate attention (see "Alarms, Notifications, and Communication Errors" on page 121). If you ignore an alarm, you could develop hypoglycemia or hyperglycemia.

Hazard alarms (⚠) are accompanied by a continuous vibration or tone and interrupt anything else the PDM is doing except another hazard alarm. For example, a hazard alarm is issued if the Pod runs out of insulin.

Advisory alarms (🟡) alert you to some aspect of the PDM or Pod that needs your attention in the near future. For example, if the level of insulin in your Pod is getting low, the PDM issues an advisory alarm.

Notifications


Notifications (⌚) remind you about actions you may want to perform (see "Notifications List" on page 129). For example, you can set a reminder to tell you to measure your blood glucose after a specified amount of time.

Confirmation Messages

The PDM confirms that an instruction was successful by displaying a green banner with a confirmation message. The confirmation message disappears after several seconds.

Tip: *Swipe to the right on the message to dismiss it sooner.*

If an instruction is not successful, then the PDM displays a communication error message (see "Communication Errors" on page 132).

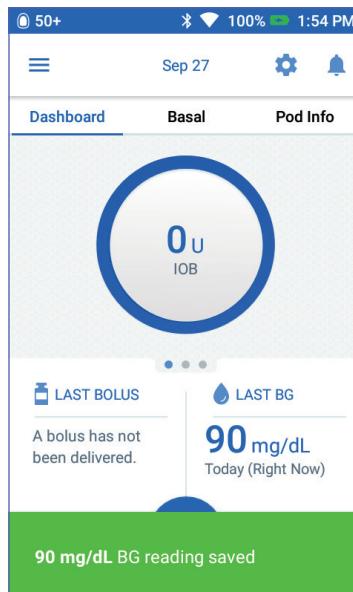

CHAPTER 2

Initial PDM Setup

This chapter guides you through setting up your first PDM or a replacement PDM.

If you are setting up a replacement PDM, be sure to unpair any BG meters paired to your old PDM before setting up your new PDM (see "Pairing, unpairing, or renaming a BG meter" on page 114). Then go to "Charge the battery" on page 22.

The Omnipod DASH™ PDM Kit

Your initial shipment contains the Omnipod DASH™ PDM Kit and other items needed to begin using the Omnipod DASH™ Insulin Management System.

After you unpack the Omnipod DASH™ PDM Kit, use the "Contents" label on the side of the box to make sure you have everything.

The Omnipod DASH™ PDM Kit contains:

- PDM & rechargeable battery
- USB cable & charger
- User Guide
- Carry case
- Quick Start Guide

You can obtain Pods by contacting Customer Care (see the first page of this *User Guide* for contact information).

Preparing for Your Training

If you are a first-time Omnipod DASH™ System user, you need to meet with your Omnipod DASH™ System Trainer to set up your Personal Diabetes Manager (PDM) and first Pod.

If you have used an Omnipod® Insulin Management System in the past and are upgrading to the Omnipod DASH™ System, contact Customer Care to find out about an online training module you can use before setting up your new system.

To get a head start on learning about the Omnipod DASH™ System, review this *User Guide*, including the "Introduction" on page xi, "Your Omnipod DASH™ Insulin Management System" on page 1, and "Taking Care of Your PDM and Pod" on page 137.

2 Initial PDM Setup

Warnings:

Do NOT use the Omnipod DASH™ System before you have been trained. Inadequate training could put your health and safety at risk.

Follow your healthcare provider's instructions for initializing the PDM. Improper setup could put your health and safety at risk.

Note: Keep an emergency kit with you at all times to quickly respond to a diabetes emergency (see "Prepare for Emergencies" on page 175).

Charge the battery

It is important to charge the PDM's battery before setting up your Omnipod DASH™ System:

1. Install the rechargeable battery in the PDM, if necessary (see "Inserting or replacing the PDM battery" on page 143).
2. Assemble the charger by plugging the charger cable's USB Type A plug into the charger's wall adapter.

Caution: Only use the micro-USB charger that came with the PDM.

3. Plug the charger into a wall outlet.
4. Plug the charger cable's USB Micro-B plug into the PDM's Micro-B USB port.
5. Charge the PDM until the battery level icon shows 100% charge (see "The Status Bar" on page 9).
6. Disconnect the charger from the PDM and the wall outlet.

Caution: Only use the rechargeable battery that came with your PDM or an Insulet authorized replacement. Contact Customer Care if you have questions.

Items needed when you meet with your Omnipod DASH™ System Trainer

- Your PDM
- Two Pods
- *This User Guide*
- The blood glucose meter that came with your PDM (recommended) or another blood glucose meter
- Test strips and a lancing device (available from many pharmacies)
- Vial of rapid-acting U-100 insulin
- Alcohol prep swabs

- Instructions from your healthcare provider with PDM settings tailored to your needs. These settings include Basal Program, IC Ratio, Correction Factor, Target BG values, and Duration of Insulin Action.

General PDM Settings

Although PDM setup is easy, if you are a first-time user, your trainer must guide you through the setup process. You can adjust these settings later as needed.

Tip: Use the pages at the end of this User Guide to write down all of your settings. This list will be helpful if you ever need to reset or replace your PDM.

Note: Tapping the back arrow () returns you to the previous screen. However tapping the CANCEL button in any of these setup steps takes you to the first screen of each section and erases any entries in that section. A popup screen warns you that you could lose these entries.

Turning on and personalizing the PDM

- Turn on the PDM by pressing and holding the Power button on the right side until the Omnipod® logo appears. The PDM runs through a series of checks.

Caution: Do not turn off the PDM power. The PDM must be ON in order to sound an alarm. If you press the Power button for too long, the PDM will display a menu with a Power Off option. Do NOT tap Power Off. Tap outside the menu to dismiss it and to keep the PDM on.

Note: You can press the Power button briefly to toggle the PDM between the wake and sleep modes. Omnipod DASH™ System alarms will also wake the PDM from sleep mode.

- When a screen with the Omnipod DASH™ logo appears, use your finger to swipe from left to right across the screen.

Note: If you see an unexpected screen instead of the Omnipod DASH™ logo screen, see "Troubleshooting PDM Startup" on page 187.

- Tap a language to select your preferred language for the PDM screens. Then tap the arrow (>).

Note: The Food Library is only available when English is the selected language.

- Review the terms and conditions (ToU - terms of use), including the End User License Agreement (EULA), Warranty, and Legal Notices as follows:

- a. Tap the HIPAA Privacy Policy, EULA, ToU, and Warranty link to read the Omnipod DASH™ System's legal notices and privacy policy. Then tap AGREE.

2 Initial PDM Setup

- b. Tap the box to add a checkmark.
- c. Tap CONTINUE.

Note: If you are under 18, your parent or guardian must accept for you.

5. Tap BEGIN SETUP.
6. Tap letters on the keypad to enter a personalized screen message (see "Selecting, Adding, and Deleting Items" on page 6). Then tap the checkmark.

Note: You must enter at least one character.

Tip: Including a contact phone number in the message could help in recovering a misplaced PDM.

7. Tap CONTINUE.
- A screen appears showing several background images.
8. Swipe right or left to see more images. Tap on your preferred image, then tap CONTINUE.



Note: When you wake up your PDM, you will see your personalized screen message and background image. Always confirm that the PDM is yours before using it.

Enter a PIN

To protect against unintentional screen touches, you must create a 4-digit personal identification number or PIN.

1. Choose four numbers to be your PIN. You will use this PIN number every time you wake up your PDM. You may want to record the PIN in a safe place.

Tip: To keep the PIN visible, tap the eye icon located to the right of the PIN entry fields. To hide the number, tap the eye icon again.

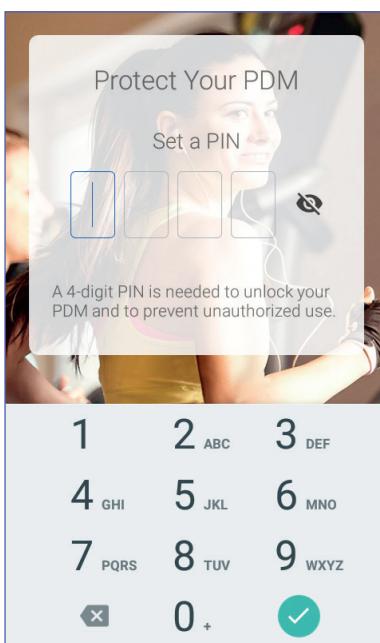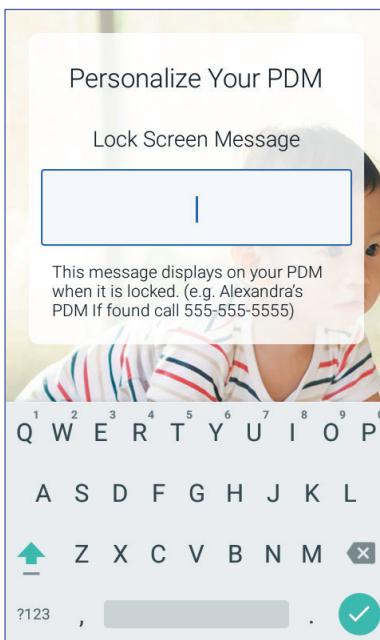


2. On the number pad, tap each number of your PIN. Then tap the checkmark.
3. Enter the same four numbers again to confirm your PIN. Tap the checkmark. If the second PIN entry does not match the first, you must repeat the above steps.

Set the time zone and time

To set the current time zone and time:

1. Tap Select One to show the list of time zones.
2. Tap your time zone. You may need to swipe up or down to find your time zone.
3. Tap CONTINUE.
4. Tap the 12 hr / 24 hr toggle to choose your preferred time display. For example, six hours before midnight is:
 - 6:00 PM in 12 hr display
 - 18:00 in 24 hr display
5. Place your finger on the Hour scroll wheel. Slide your finger up or down to scroll the wheel up or down. Stop scrolling when the correct hour appears in the center of the wheel.
6. Scroll the Minute scroll wheel up or down until the correct minute appears in the center of the scroll wheel.
7. If using 12 hr time, scroll the right-most field and select AM or PM.
8. Review the time and tap CONTINUE.

Caution: Check that you have set the time correctly. The time setting affects the operation of several Omnipod DASH™ System features and can impact your insulin delivery.

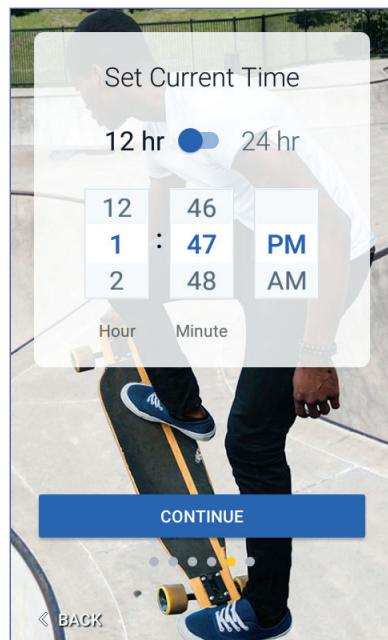


2 Initial PDM Setup

Set the date

On the Set Current Date screen:

1. Tap MM/DD/YYYY to display a list of date formats. Tap the desired date format.
2. Set the Month, Day, and Year fields by scrolling their respective wheels one at a time.
3. Review the date and date format, then tap CONTINUE.
4. On the Confirm Time & Date screen, review the time zone, time, and date. If correct, tap CONTINUE.

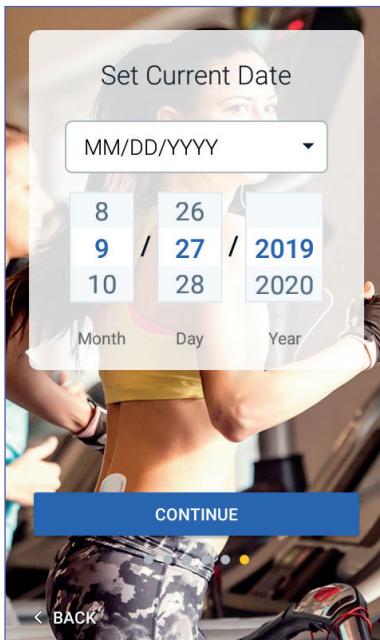

Basal Insulin Settings


Maximum Basal Rate

The Maximum Basal Rate sets the upper limit of any basal insulin rate that you can use.

1. Tap SET UP PROFILE.
2. Review the description of basal insulin, then tap the arrow (>).
3. Tap the Max Basal Rate field.
4. Scroll to your desired Maximum Basal Rate. When the correct number is in the center of the scroll wheel, tap the number to select it.

Tip: *Alternatively, tapping outside of the scroll wheel selects the value in the center of the scroll wheel.*

5. Tap NEXT.

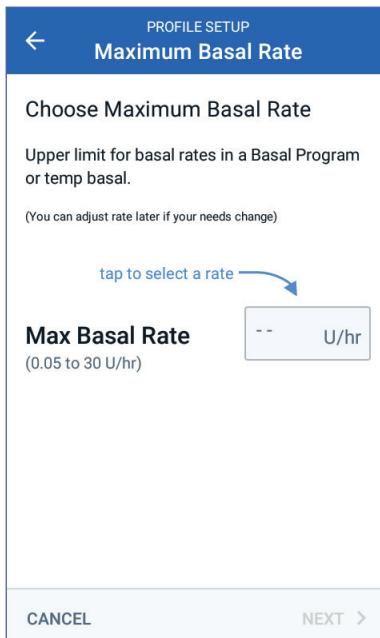

You can adjust your Maximum Basal Rate later, if your needs change.

Create a Basal Program


The next step is to define a Basal Program. For a description of basal rates, basal segments, and Basal Programs, see "Basal Insulin Delivery" on page 149.

Name and tag the Basal Program

1. Review the description of Basal Programs, then tap NEXT.
2. The default name for the Basal Program is Basal 1. To change the name, tap the Program Name field and enter the new name (see "Selecting, Adding, and Deleting Items" on page 6) and then tap the checkmark.
3. Optional: To add a visual icon to your Basal Program, tap one of the tags. Tap the tag a second time to deselect it.
4. Tap NEXT.

Define the first segment

1. The Start Time for the first segment is always midnight. Tap the End Time field and scroll to select the desired end time.
2. Tap the Basal Rate field and scroll to select the basal rate for the segment.

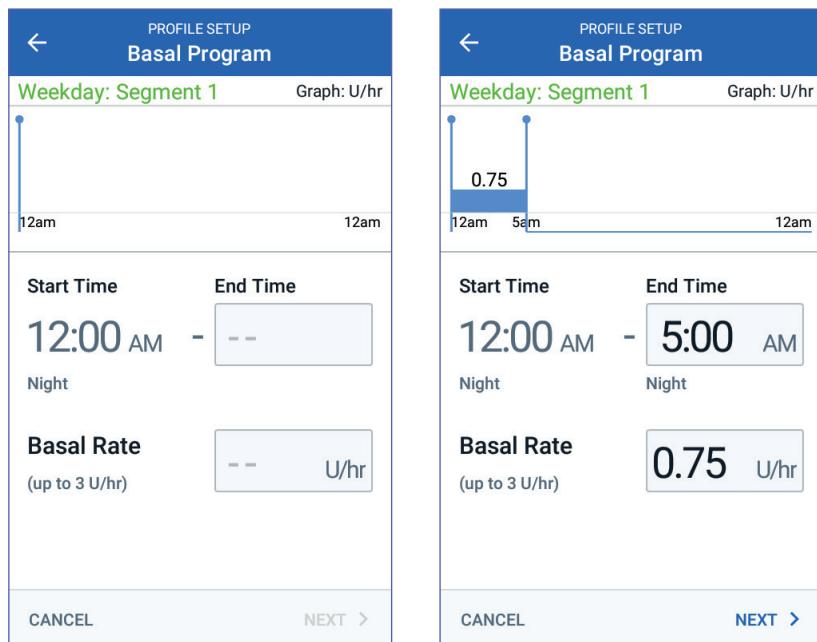

The Maximum Basal Rate that you entered earlier is displayed under the Basal Rate text. You cannot enter a basal rate greater than this number.

2 Initial PDM Setup

Note: The two vertical blue lines on the graph near the top of the screen show the start and end time for the basal segment. The selected basal rate for the segment is shown between the two vertical lines.

3. Check the values of your start and end times and the basal rate. Then tap NEXT.

Define additional segments

If the Basal Program does not cover 24-hours, you must add additional segments:

1. Tap the End Time field and select the duration of the next segment.
2. Tap the Basal Rate field and select the basal rate for the segment.
3. Review the segment details and the graph.
4. Tap NEXT to move to the next segment.
5. Repeat the preceding steps as needed until your final segment ends at midnight.

After specifying a basal rate for the final segment, your Basal Program is complete.

Review the Basal Program

The next screen summarizes the start and end times, duration, and basal rate for each segment of the Basal Program.

1. Tap CONTINUE to review your Basal Program.

2. Check that the graph and the individual segment values are correct.

The total daily amount of basal insulin to be delivered by this Basal Program is listed below the graph.

3. To change an end time or basal rate for a segment:


- a. Tap the row containing the segment you would like to change.

- b. Tap the End Time field, and enter the new end time for the segment.

- c. Tap the Basal Rate field, and enter the desired basal rate.

- d. Tap NEXT.

- e. Then define the end time and basal rate for any following segments, as needed.

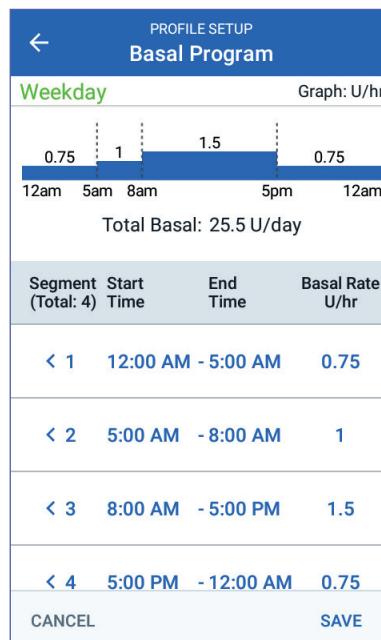

4. To add a new segment:
 - a. Tap the row containing the start time of the new segment.
 - b. Tap the End Time field, and enter the start time of the new segment as the end time of this segment.
 - c. Change the basal rate, if necessary.
 - d. Tap NEXT.
 - e. Then define the end time and basal rate for any following segments, as needed.
5. To delete a segment:
 - a. Note the end time of the segment you want to delete.
 - b. Tap the segment that precedes the segment you want to delete.
 - c. Tap the End Time field, and enter the end time of the segment you want to delete. This 'overwrites' the segment you want to delete.
 - d. Tap NEXT.
 - e. Then define the end time and basal rate for any following segments, as needed.
6. When the Basal Program is correct, tap SAVE.

Note: If the basal rate for a segment is 0 U/hr, the PDM displays a message calling this to your attention. Tap OK if the 0 U/hr rate is correct. Otherwise, tap CANCEL and edit the segment with the 0 U/hr rate.

Note: To create additional Basal Programs after setup is complete, see page 81.

Temp basal configuration

For a description of temporary basal rates, also called temp basals, see page 151.

1. If you want the ability to use temp basals, tap the toggle to the "on" position. The toggle is in the "on" position when it is in the right-hand position and is blue.

If you turn temp basals on, percentages are used by default. To specify temp basals as a flat rate (U/hr), see "Temp basal" on page 116.

2. Tap NEXT.

2 Initial PDM Setup

Blood Glucose Settings

The blood glucose settings define what blood glucose readings are considered in range and allow you to pair to a CONTOUR® NEXT ONE BG meter.

Upper and lower limits for BG Goal Range

You can set the upper and lower limits of your BG Goal Range by using the number pad or the slider:

1. Review the description of blood glucose levels, then tap the arrow (>).
2. To define the lower limit, tap the Lower Limit field and type the number using the number pad.
3. To define the upper limit, tap the Upper Limit field or slide the upper (yellow) circle.
4. Review your upper and lower limits, and tap NEXT to save them.

Tip: *Alternatively, you can touch the lower (red) circle with your finger and slide it up or down.*



Pair to a BG meter

If desired, you can pair your PDM to a CONTOUR® NEXT ONE BG meter (BG meter). Once paired, blood glucose readings can be transmitted via Bluetooth® wireless technology from your BG meter to your PDM.

Note: If you do not want to pair to a BG meter, tap SKIP. Then go to "Bolus Calculator Settings" on page 32

To pair a BG meter:

1. Turn off your BG meter, and place it within six feet of your PDM.
2. Turn on the blue light on your BG meter. To do so, press and hold the OK button on the BG meter until its white light changes to a flashing blue light.
3. On the PDM, tap START SEARCH.



The PDM displays the model and serial number of any CONTOUR® NEXT ONE BG meters that are in range and available for pairing.

4. Turn your BG meter over to find its seven digit serial number. Verify that this number matches the one on the PDM screen.
5. On the PDM, tap PAIR below your BG meter's serial number.

A Successfully Paired message appears.

Note: If the BG meter is paired to another PDM, see "Pairing, unpairing, or renaming a BG meter" on page 114.

6. Tap OK. Verify that your BG meter is listed as paired.

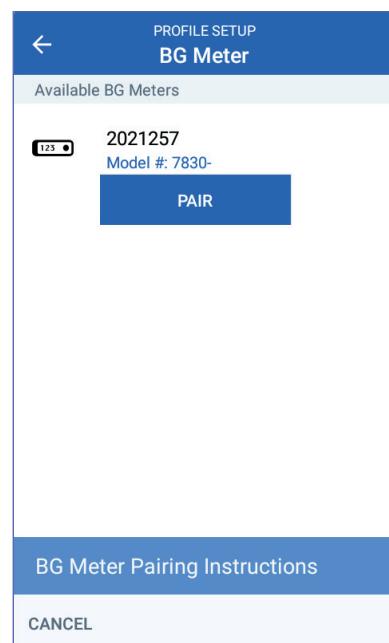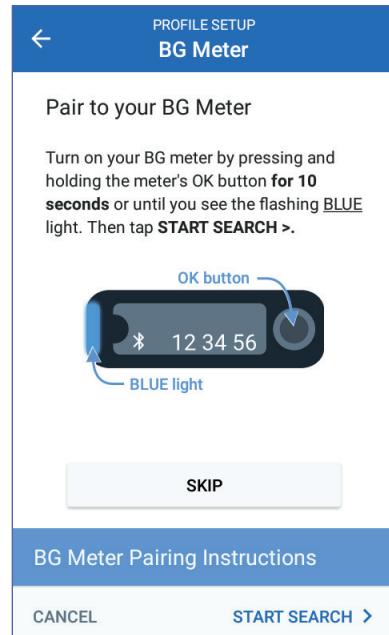

2 Initial PDM Setup

7. Optional: Rename your paired BG meter:
 - a. Tap the Options icon (⋮) next to the paired BG meter. Then tap Edit.
 - b. Tap the Name field and use the keypad to enter a new name for your BG meter, then tap the checkmark.
 - c. Tap SAVE.
8. Tap NEXT.

Caution: After pairing, the PDM controls the date, time and BG goal/target range on your paired BG meter. To avoid mislabeling of history records, make all changes to date and time on your PDM, not on your BG meter.

Bolus Calculator Settings

The Bolus Calculator suggests boluses based on your current blood glucose value and any food you are about to eat (see "The Bolus Calculator" on page 156).

Turn the Bolus Calculator on or off

1. Review the description of insulin boluses, then tap the arrow (>).
2. Toggle the Bolus Calculator setting on or off:
 - Select the On position (blue and to the right) to have the Bolus Calculator suggest boluses.
 - Select the Off position (gray and to the left) to turn off the Bolus Calculator. You will have to calculate your own bolus amounts.
3. Tap NEXT.
4. If you turned the Bolus Calculator off, skip to "Other Bolus Settings" on page 36.

Target BG and Correct Above values

The Bolus Calculator aims to bring your blood glucose to the Target BG value if your current blood glucose level is above the Correct Above value. You can establish up to eight different blood glucose targets for different times of day.

Define the segments

Setting values for each segment follows the same pattern that you used to create your Basal Program:

1. Review the description of Target BG and Correct Above, then tap NEXT.
2. Tap the End Time field and enter an end time for the segment.
3. Tap the Target BG field and specify the Target BG for that segment.
4. Tap the Correct Above field and specify the Correct Above value for that segment.
5. Tap NEXT.
6. Repeat the above steps as needed until you have specified values for the segment that ends at midnight.

PROFILE SETUP
Target BG & Correct Above

Segment 1

Start Time: 12:00 AM End Time: ---
Night

Target BG (70 to 200 mg/dL): --- mg/dL

Correct Above (Target BG to 200 mg/dL): --- mg/dL

CANCEL NEXT >

Review the Target BG and Correct Above values

1. Review the segments for the full 24 hour profile.
2. To change any of the entries:
 - a. Tap the row containing the entry to be changed and enter the corrected value.
 - b. Review and correct as needed any remaining segments.
3. When the segments and values are correct, tap SAVE.

PROFILE SETUP
Target BG & Correct Above

Review the values entered for each time segment.

Start Time	End Time	Target BG mg/dL	Correct Above mg/dL
12:00 AM	6:00 PM	100	110
6:00 PM	12:00 AM	105	115

CANCEL SAVE

2 Initial PDM Setup

Minimum BG for Calcs

If your blood glucose level is below the Minimum BG for Calcs that you specify, the Bolus Calculator is disabled (see "The Bolus Calculator" on page 156).

1. To enter your Minimum BG for Calcs, tap the Min BG for Calcs field and enter the number on the number pad.

Tip: *Alternatively, touch the blue circle and slide it to the desired number.*

2. Tap NEXT.

PROFILE SETUP

Min BG for Calcs


Set Min BG for Calcs

If your blood glucose is below your Minimum BG for Calculations (Min BG for Calcs), the Bolus Calculator is disabled so that it does not suggest a bolus.

Min BG for Calcs

70 mg/dL

(50 to 70 mg/dL)



CANCEL

NEXT >

Insulin to Carb Ratio

Your Insulin to Carbohydrate Ratio, or "IC Ratio," defines how many carbohydrates are covered by one unit of insulin. The Bolus Calculator uses the IC Ratio to calculate the meal portion of a suggested bolus. You can create up to eight IC Ratio segments per day.

1. Review the description of IC Ratio, then tap NEXT.
2. Enter the end time.
3. Enter the IC Ratio value in the 1 Unit of Insulin Covers field.
4. Tap NEXT.
5. Add additional segments as necessary until the final end time is midnight.
6. Review your 24-hour IC Ratio segments. Tap any entry to correct it.
7. When the segments and values are correct, tap SAVE.

PROFILE SETUP

Insulin to Carb Ratio

Segment 1

Start Time

12:00 AM

End Time

Night

1 Unit of Insulin Covers

(1 to 150 g carbs)

CANCEL

NEXT >

Correction Factor

Your Correction Factor defines how much one unit of insulin lowers your blood glucose level. The Bolus Calculator uses the Correction Factor to calculate the correction portion of a suggested bolus. You can create up to eight Correction Factor segments per day.

1. Review the description of Correction Factor, then tap NEXT.
2. Enter the end time.
3. Enter the Correction Factor in the 1 Unit of Insulin Decreases BG by field.
4. Tap NEXT.
5. Add additional segments as necessary until the final end time is midnight.
6. Review your Correction Factor segments. Tap any entry to correct it.
7. When the segments and values are correct, tap SAVE.

PROFILE SETUP

Correction Factor

Segment 1

Start Time: 12:00 AM

End Time: Night

1 Unit of Insulin Decreases BG by (1 to 400 mg/dL)

CANCEL NEXT >

Reverse Correction

There may be times when you are about to eat and your blood glucose level is below your Target BG level. If Reverse Correction is on, the Bolus Calculator decreases a suggested meal bolus to help counteract your low blood glucose.

1. Toggle the Reverse Correction button on or off:
 - Select the On position if you want the Bolus Calculator to reduce the suggested meal bolus when your blood glucose is below your Target BG.
 - Select the Off position if you do not want the Bolus Calculator to adjust the suggested meal bolus based on a low blood glucose value.
2. Tap NEXT.

Duration of Insulin Action

The Duration of Insulin Action is the length of time that insulin stays active in your body. The Bolus Calculator uses this setting to determine how much insulin remains in your body from previous boluses (called insulin on board or IOB).

2 Initial PDM Setup

1. Tap the Duration of Insulin Action field and use the scroll wheel to specify your Duration of Insulin Action.
2. Tap NEXT.

Other Bolus Settings

The remaining bolus settings are used whether the Bolus Calculator is on or off.

Maximum Bolus

The PDM will not let you request a bolus above the Maximum Bolus setting. You will see a message if the Bolus Calculator calculates a bolus that is above this amount.

1. Tap the Max Bolus field and use the number pad to specify your Maximum Bolus. Tap the checkmark to close the number pad.
2. Tap NEXT.

Extended bolus setting

Extending a bolus means that a meal bolus can be delivered over a prolonged period of time. For a description of the extended bolus feature, see page 155.

1. Toggle the Extended Bolus button to turn the extended bolus feature on or off.
2. Tap COMPLETE.
The PDM restarts.

PDM Setup Complete

Congratulations! Your PDM is now ready for use. When you are ready to activate your first Pod, go to "First Time Activating a Pod" on page 38.

Tip: To adjust the PDM screen time-out or screen brightness, see "Screen display" on page 101.

Note: Confidence reminders and program reminders are turned on by default. These reminders cause the PDM or Pod to beep at the beginning and end of boluses and temp basals, and also once an hour during a long-lasting bolus or temp basal. For more information, see "Confidence reminders" and "Program reminders" on page 112.

CHAPTER 3

Changing Your Pod

Beginning the Pod Change Process

Changing your Pod consists of deactivating your current Pod and activating a new Pod.

Your Pod should be changed at least once every 48 to 72 hours (2 to 3 days) or after delivering 200 units of insulin. Consult with your healthcare provider and refer to the insulin labeling to determine if you should change your Pod more often.

Warnings:

Do NOT use a Pod if you are sensitive to or have allergies to acrylic adhesives, or have fragile or easily damaged skin.

Because the Pod uses only rapid-acting U-100 insulin, you are at increased risk for developing hyperglycemia if insulin delivery is interrupted. Severe hyperglycemia can quickly lead to diabetic ketoacidosis (DKA). DKA can cause symptoms such as abdominal pain, nausea, vomiting, breathing difficulties, shock, coma, or death. If insulin delivery is interrupted for any reason, you may need to replace the missing insulin. Ask your healthcare provider for instructions for handling interrupted insulin delivery, which may include an injection of rapid-acting insulin.

The Pod and its accessories, including the needle cap, contain small parts that may be dangerous if swallowed. Be careful to keep these small parts away from young children.

The steps for deactivating or activating a Pod depend on whether you have an active Pod or not:

- If this is your first time activating a Pod, go to "First Time Activating a Pod" on page 38.
- If you currently have an active Pod, go to "Deactivate an Active Pod" on page 38.
- If you have already deactivated your most recent Pod, go to "No Active Pod" on page 39.

Tip: *Software updates require that you deactivate your Pod. Connect to Wi-Fi periodically so the PDM can check for software updates. If there is a "Wireless Update" message on the Lock screen, be sure to install the software update after you deactivate your Pod (see "Software update (Wireless update)" on page 106).*

3 Changing Your Pod

First Time Activating a Pod

Your Omnipod DASH™ System trainer will help you set up your first Pod.

After completing the PDM setup flow, the Home screen displays "No Active Pod."

1. Tap SET UP NEW POD.
2. Go to "Preliminary Pod Change Steps" on page 40.

Deactivate an Active Pod


To deactivate and remove an active Pod:

1. Navigate to the Pod change screen:
Home > Pod Info tab > VIEW POD DETAILS
or
Menu icon (≡) > Pod
2. Tap CHANGE POD, then tap DEACTIVATE POD.

If a temp basal or extended bolus was running, it is canceled now.

If you see a communication error message, see "Error when deactivating a Pod" on page 134.

Warning: Do NOT apply a new Pod until you have deactivated and removed the old Pod. A Pod that has not been deactivated properly can continue to deliver insulin as programmed, putting you at risk of over infusion and possible hypoglycemia.

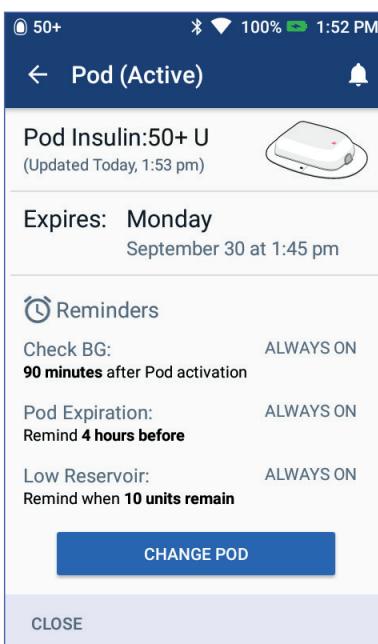

3. When the green banner tells you to remove your Pod, remove the deactivated Pod from your body:
 - a. Gently lift the edges of the adhesive tape from your skin and remove the entire Pod.


Tip: Remove the Pod slowly to help avoid possible skin irritation.

 - b. Use soap and water to remove any adhesive that remains on the skin, or, if necessary, use an adhesive remover.
 - c. Check the infusion site for signs of infection (see "Avoid Infusion Site Infections" on page 49).
 - d. Dispose of the used Pod according to local waste disposal regulations.
4. To activate a new Pod, tap SET UP NEW POD.
5. Go to "Preliminary Pod Change Steps" on page 40.

No Active Pod

If you have no active Pod and are ready to activate a new Pod:

1. Navigate to the Pod change screen:
Home > Pod Info tab > SET UP NEW POD
or
Menu icon (≡) > Pod >
SET UP NEW POD
2. Go to "Preliminary Pod Change Steps" on page 40.

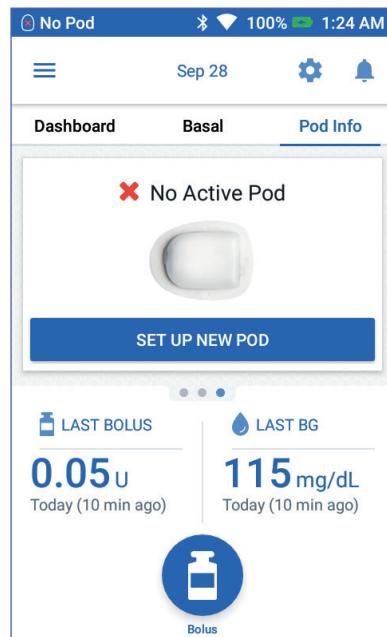

3 Changing Your Pod

Preliminary Pod Change Steps

Warnings:

NEVER use insulin that is cloudy; it may be old or inactive. Always follow the insulin manufacturer's instructions for use. Failure to use rapid-acting U-100 insulin, or using insulin that has expired or is inactive, could put your health at risk.

Do NOT apply or use a Pod if the sterile packaging is open or damaged, or if the Pod has been dropped after removal from the package, as this may increase the risk of infection. Pods are sterile unless the packaging has been opened or damaged.

Do NOT apply or use a Pod that is damaged in any way. A damaged Pod may not work properly.

Do NOT use a Pod if it is past the expiration date on the package.

To minimize the possibility of site infection, do NOT apply a Pod without first using aseptic technique. This means to:



- Wash your hands.
- Clean the insulin vial with an alcohol prep swab.
- Clean the infusion site with soap and water or an alcohol prep swab.
- Keep sterile materials away from any possible germs.

1. Gather the necessary supplies:
 - A vial of rapid-acting U-100 insulin cleared for use in the Omnipod DASH™ System
 - An unopened DASH™ Pod (look for the Omnipod DASH™ logo on the Pod tray lid)
 - Alcohol prep swabs
 - Your Omnipod DASH™ PDM
2. Wash your hands before starting and keep them clean throughout the Pod change process.
3. Check the insulin for signs of deterioration according to the manufacturer's instructions for use.
4. Check the Pod's packaging for damage. If undamaged, open it and inspect the Pod for signs of damage.
5. If the insulin or Pod is below 50°F (10°C), allow it to warm up to room temperature before proceeding.

Fill the Syringe with Insulin


The next step is to fill the syringe that came with the Pod (the "fill syringe") with insulin:

1. Use an alcohol prep swab to clean the top of the insulin vial.
2. Securely twist the fill needle onto the fill syringe.
3. Pull outward to remove the protective cap from the needle. Save the cap; you will need it later.
4. Determine how much insulin you will put into the Pod. For example, to use the Pod for 72 hours, determine how much insulin you will use over the next 72 hours. Your healthcare provider can help you determine the correct amount.



Note: The Pod requires a minimum of 85 units of rapid-acting U-100 insulin to begin operation. The Pod can deliver up to 200 units of rapid-acting U-100 insulin.

5. Draw air into the fill syringe up to the amount of insulin you want.
6. Insert the needle into the insulin vial and inject the air. Injecting air makes it easier to withdraw insulin from the vial.
7. Turn the vial of rapid-acting U-100 insulin and the fill syringe upside down. Pull down on the plunger to withdraw the desired amount of insulin from the vial into the fill syringe.
 - Fill the syringe at least to the MIN (minimum) fill line.
 - To fill the Pod with enough insulin to deliver 200 units, pull the plunger down until it stops. This will be below the 200 mark.
8. With the needle still in the vial, flick the side of the syringe with your fingertip to dislodge any air bubbles so they collect at the top of the syringe. Then push in the plunger to expel any air bubbles out of the syringe and into the insulin vial. Pull down on the plunger again, if necessary, to refill the fill syringe to the desired amount of insulin.

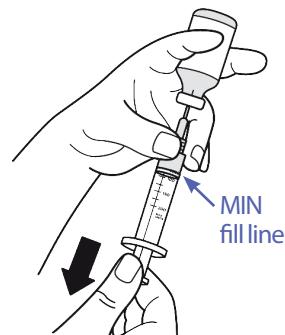

Warning: Make sure there are no air bubbles or pockets of air in the fill syringe before filling a Pod with insulin. Air transferred from the fill syringe into the Pod may result in interrupted insulin delivery.

3 Changing Your Pod

9. Remove the needle from the vial.

Fill, Pair, and Apply the Pod

Warning: Before filling a Pod, ensure that no other Pods are being activated within 5 feet (1.5 m) of your PDM.

Caution: Be sure to insert the fill syringe into the fill port and not any other location on the Pod. Do not insert the fill syringe more than once into the fill port. Only use the fill syringe and needle that came with your Pod. The fill syringe is intended for single use only and should only be used with the Omnipod DASH™ System.


Fill the Pod with insulin

To fill the Pod with insulin (screen step 1):

1. Locate the arrow on the underside of the Pod. The arrow points to the insulin fill port.
2. Insert the fill syringe straight down—not at an angle—into the fill port.
3. Depress the fill syringe plunger to transfer the insulin into the Pod.
4. Listen for two beeps from the Pod during the filling process. Be sure to completely empty the fill syringe, even after hearing the two beeps.

Note: The Pod must contain a minimum of 85 units of insulin in order to function. The Pod beeps twice after it has been filled with 85 units of insulin. If you have filled the Pod with more than 85 units and still do not hear the two beeps, please call Customer Care.

Note: After filling the Pod, continue to the next step immediately. If two hours pass before pairing the filled Pod to the PDM, the Pod becomes unusable.

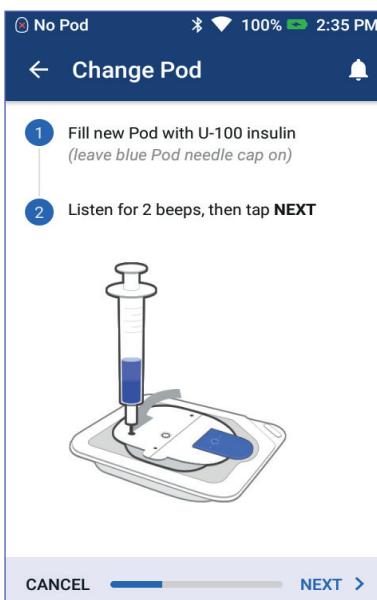

Warnings:

NEVER use a Pod if you feel resistance when you depress the plunger. This condition can result in interrupted insulin delivery.


NEVER inject air into the fill port. Doing so may result in unintended or interrupted insulin delivery.

5. Remove the needle from the insulin fill port. The port is self-sealing; insulin will not leak after the needle is removed.
6. Place the protective cap back on the syringe needle and remove the needle from the fill syringe.

Pair the PDM and Pod

To pair the PDM and Pod (screen step 2):

1. Place the PDM next to the Pod so they are touching. The Pod should be in its plastic tray during this process.
2. Tap NEXT.
 - If more than one filled DASH Pod is in range, the PDM informs you of this. Move at least five feet (1.5 m) away from any other DASH Pod and tap TRY AGAIN.
 - If only one Pod is in range, the Omnipod DASH™ System performs a series of safety checks and primes the Pod.
3. Listen for the tone from the PDM that indicates that the Pod is paired to the PDM and is ready to be applied.

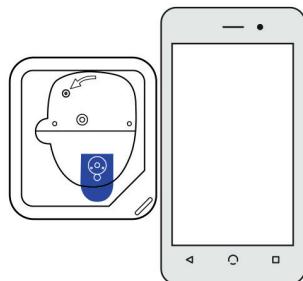

Note: After pairing, the PDM should always be able to communicate with a Pod that is up to 5 feet (1.5 m) away. Depending on the location, the PDM may be able to communicate with a Pod that is as much as 50 feet (15 meters) away.

Note: After pairing, the Pod beeps every 5 minutes until you apply it. If you do not apply it within 60 minutes after pairing, the Pod becomes unusable.

If you see a communication error message when you attempt to pair your Pod, see "Communication Errors" on page 132.