

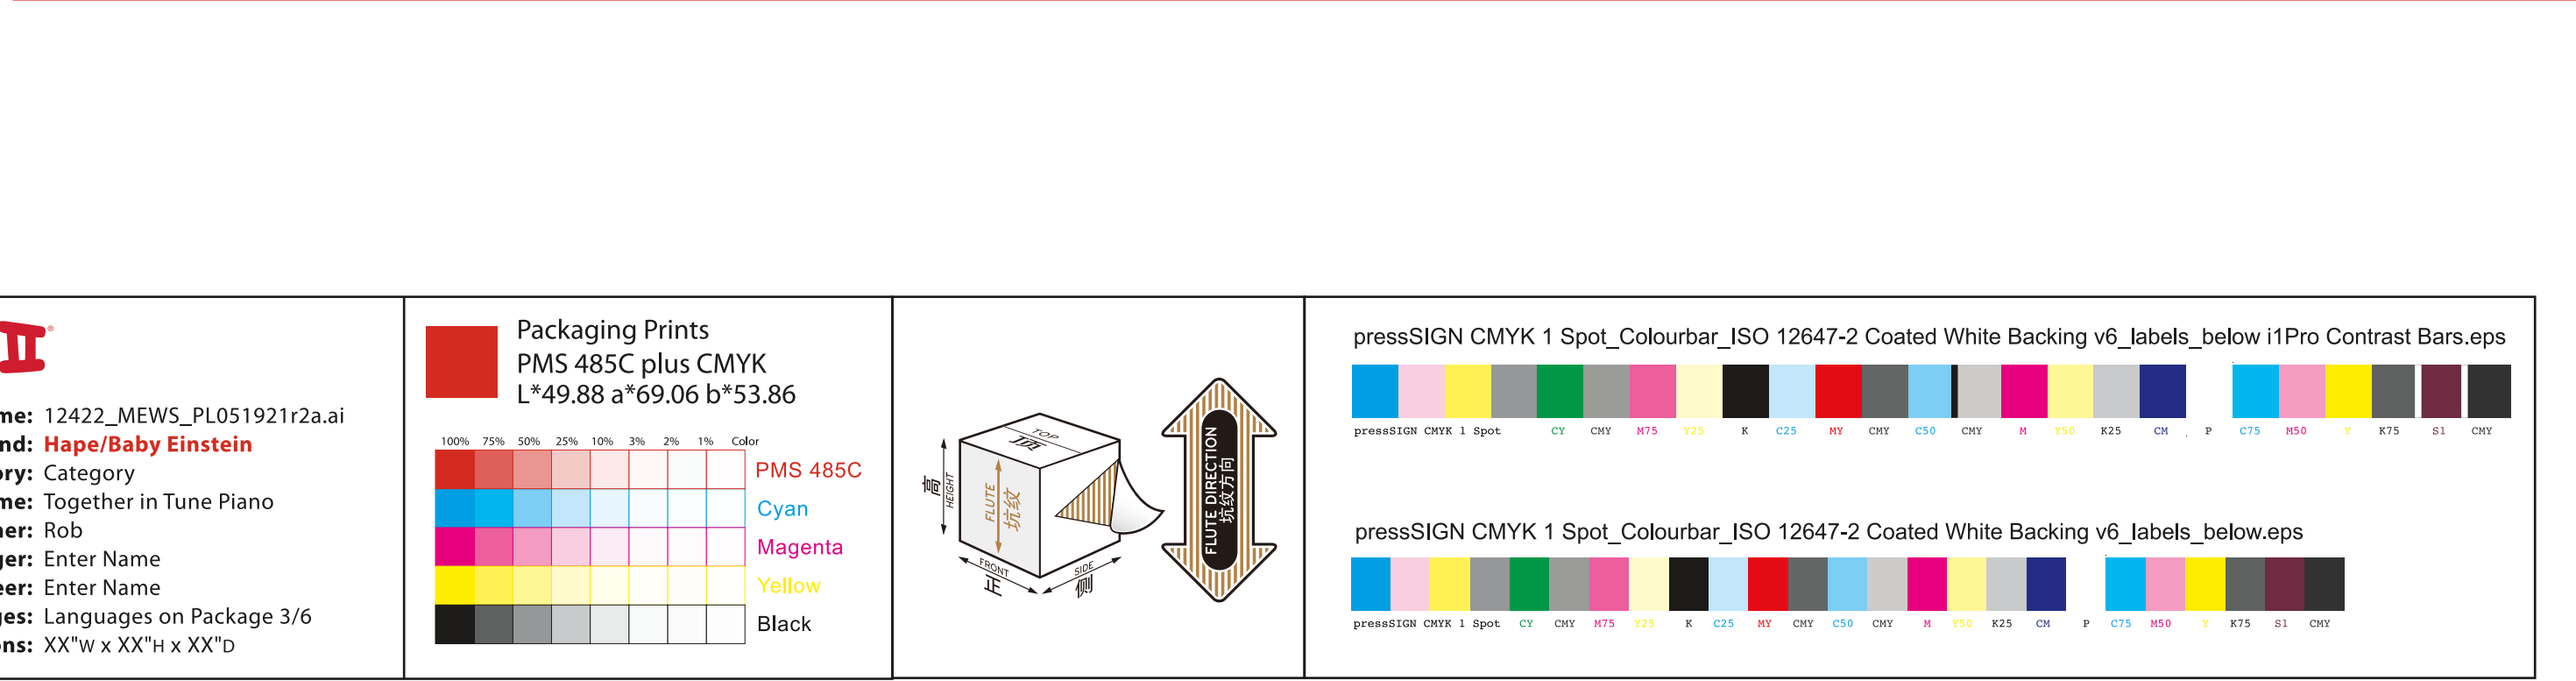
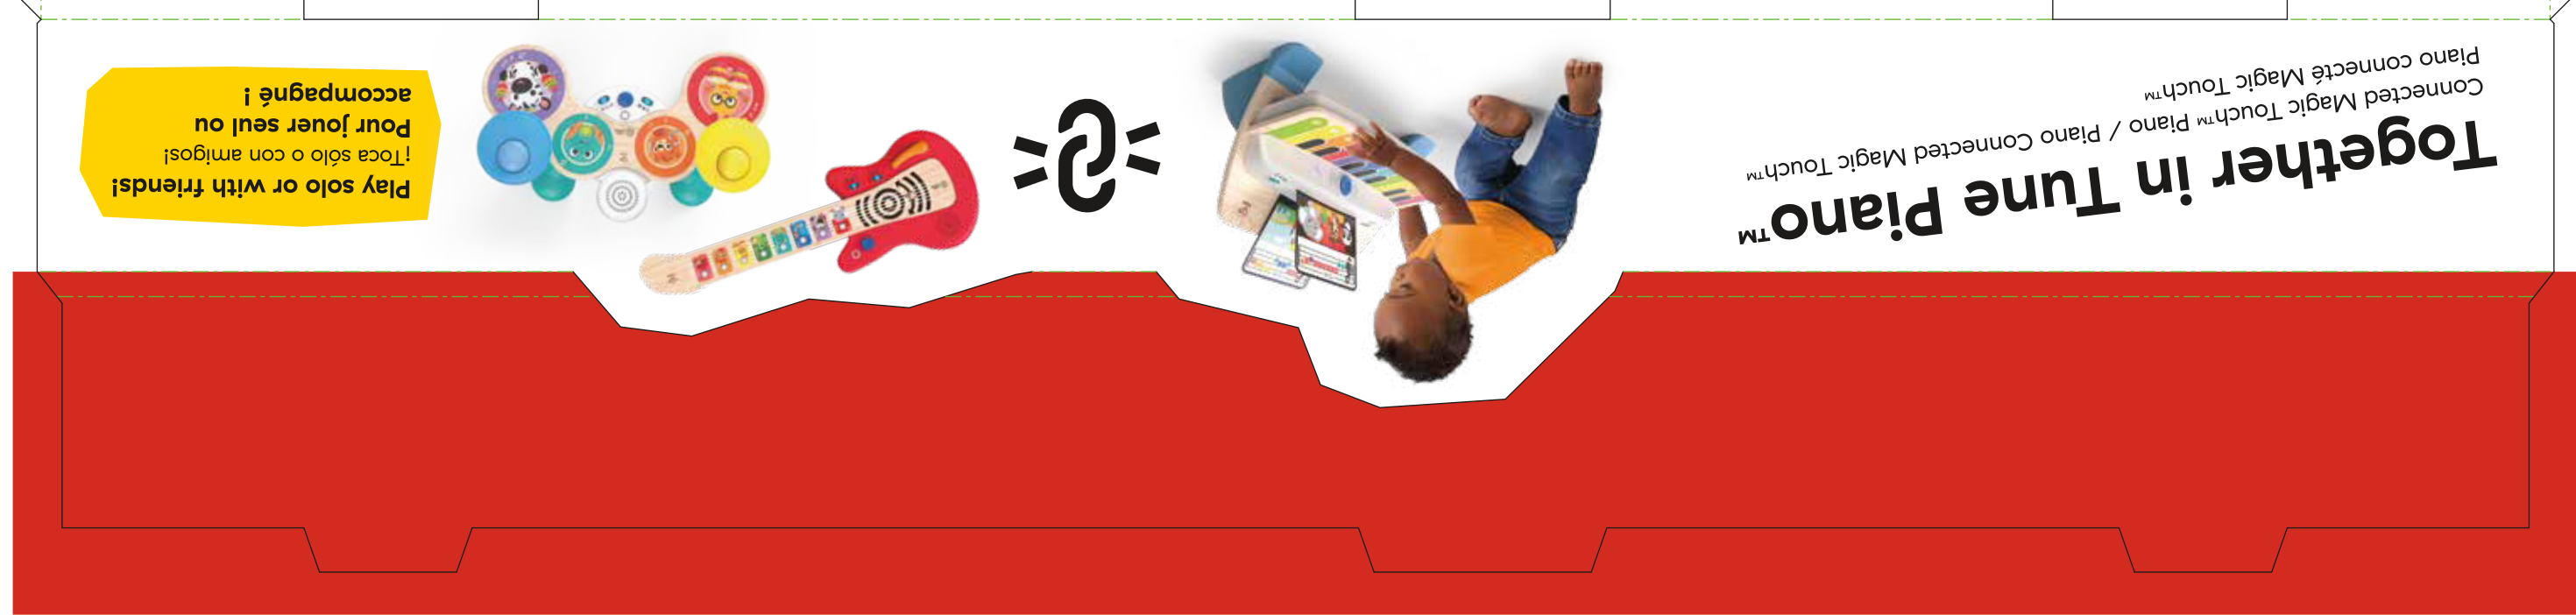


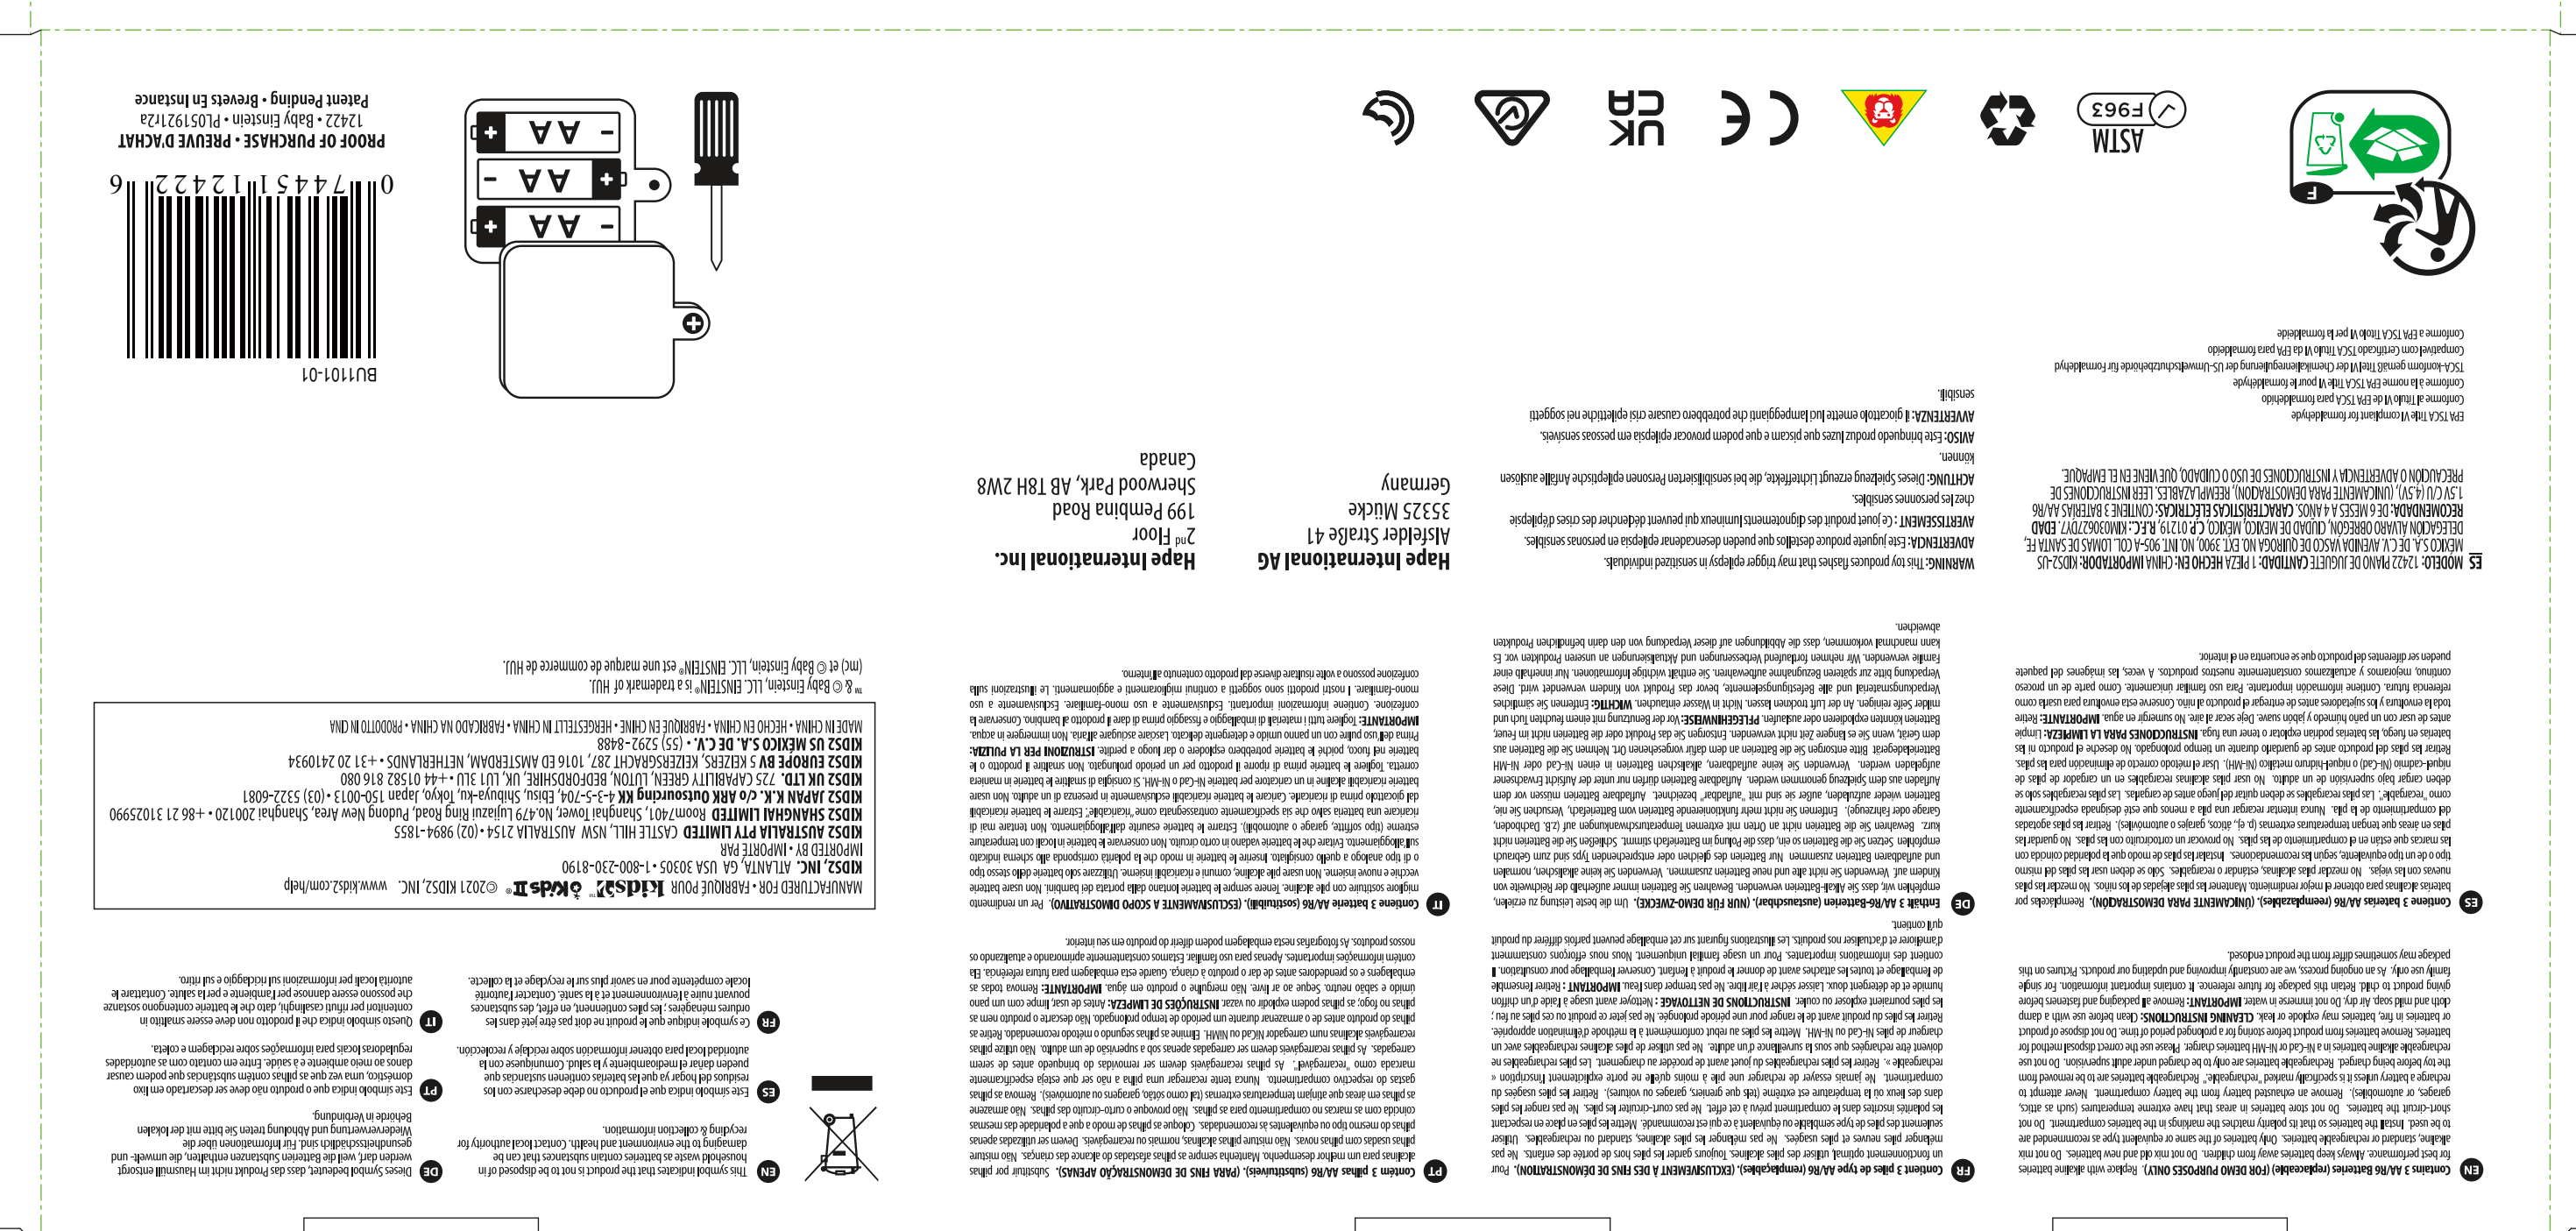

There are two color bars on this proof and in the art file. One to be used with X-rite i1 Pro Spectrophotometer. The other can be used with most other spectrophotometers. Printers must repeat one of the two color bars all the way across the width (gripper edge) of the press sheets on sample runs and production runs. Failure to comply will result in the remaking of film and/or plates at your cost.

此印刷品及设计文件包含两种颜色条。一种适用于X-rite i1 Pro分光光度计。另一种适用于其它大部分的分光光度计。在打样或批量生产时，印刷厂必须选择其一种颜色条重复放置直到覆盖整张纸的宽度（叼口处），没有按照上述要求导致数量出现差异，出版商将自行承担印刷厂责任。

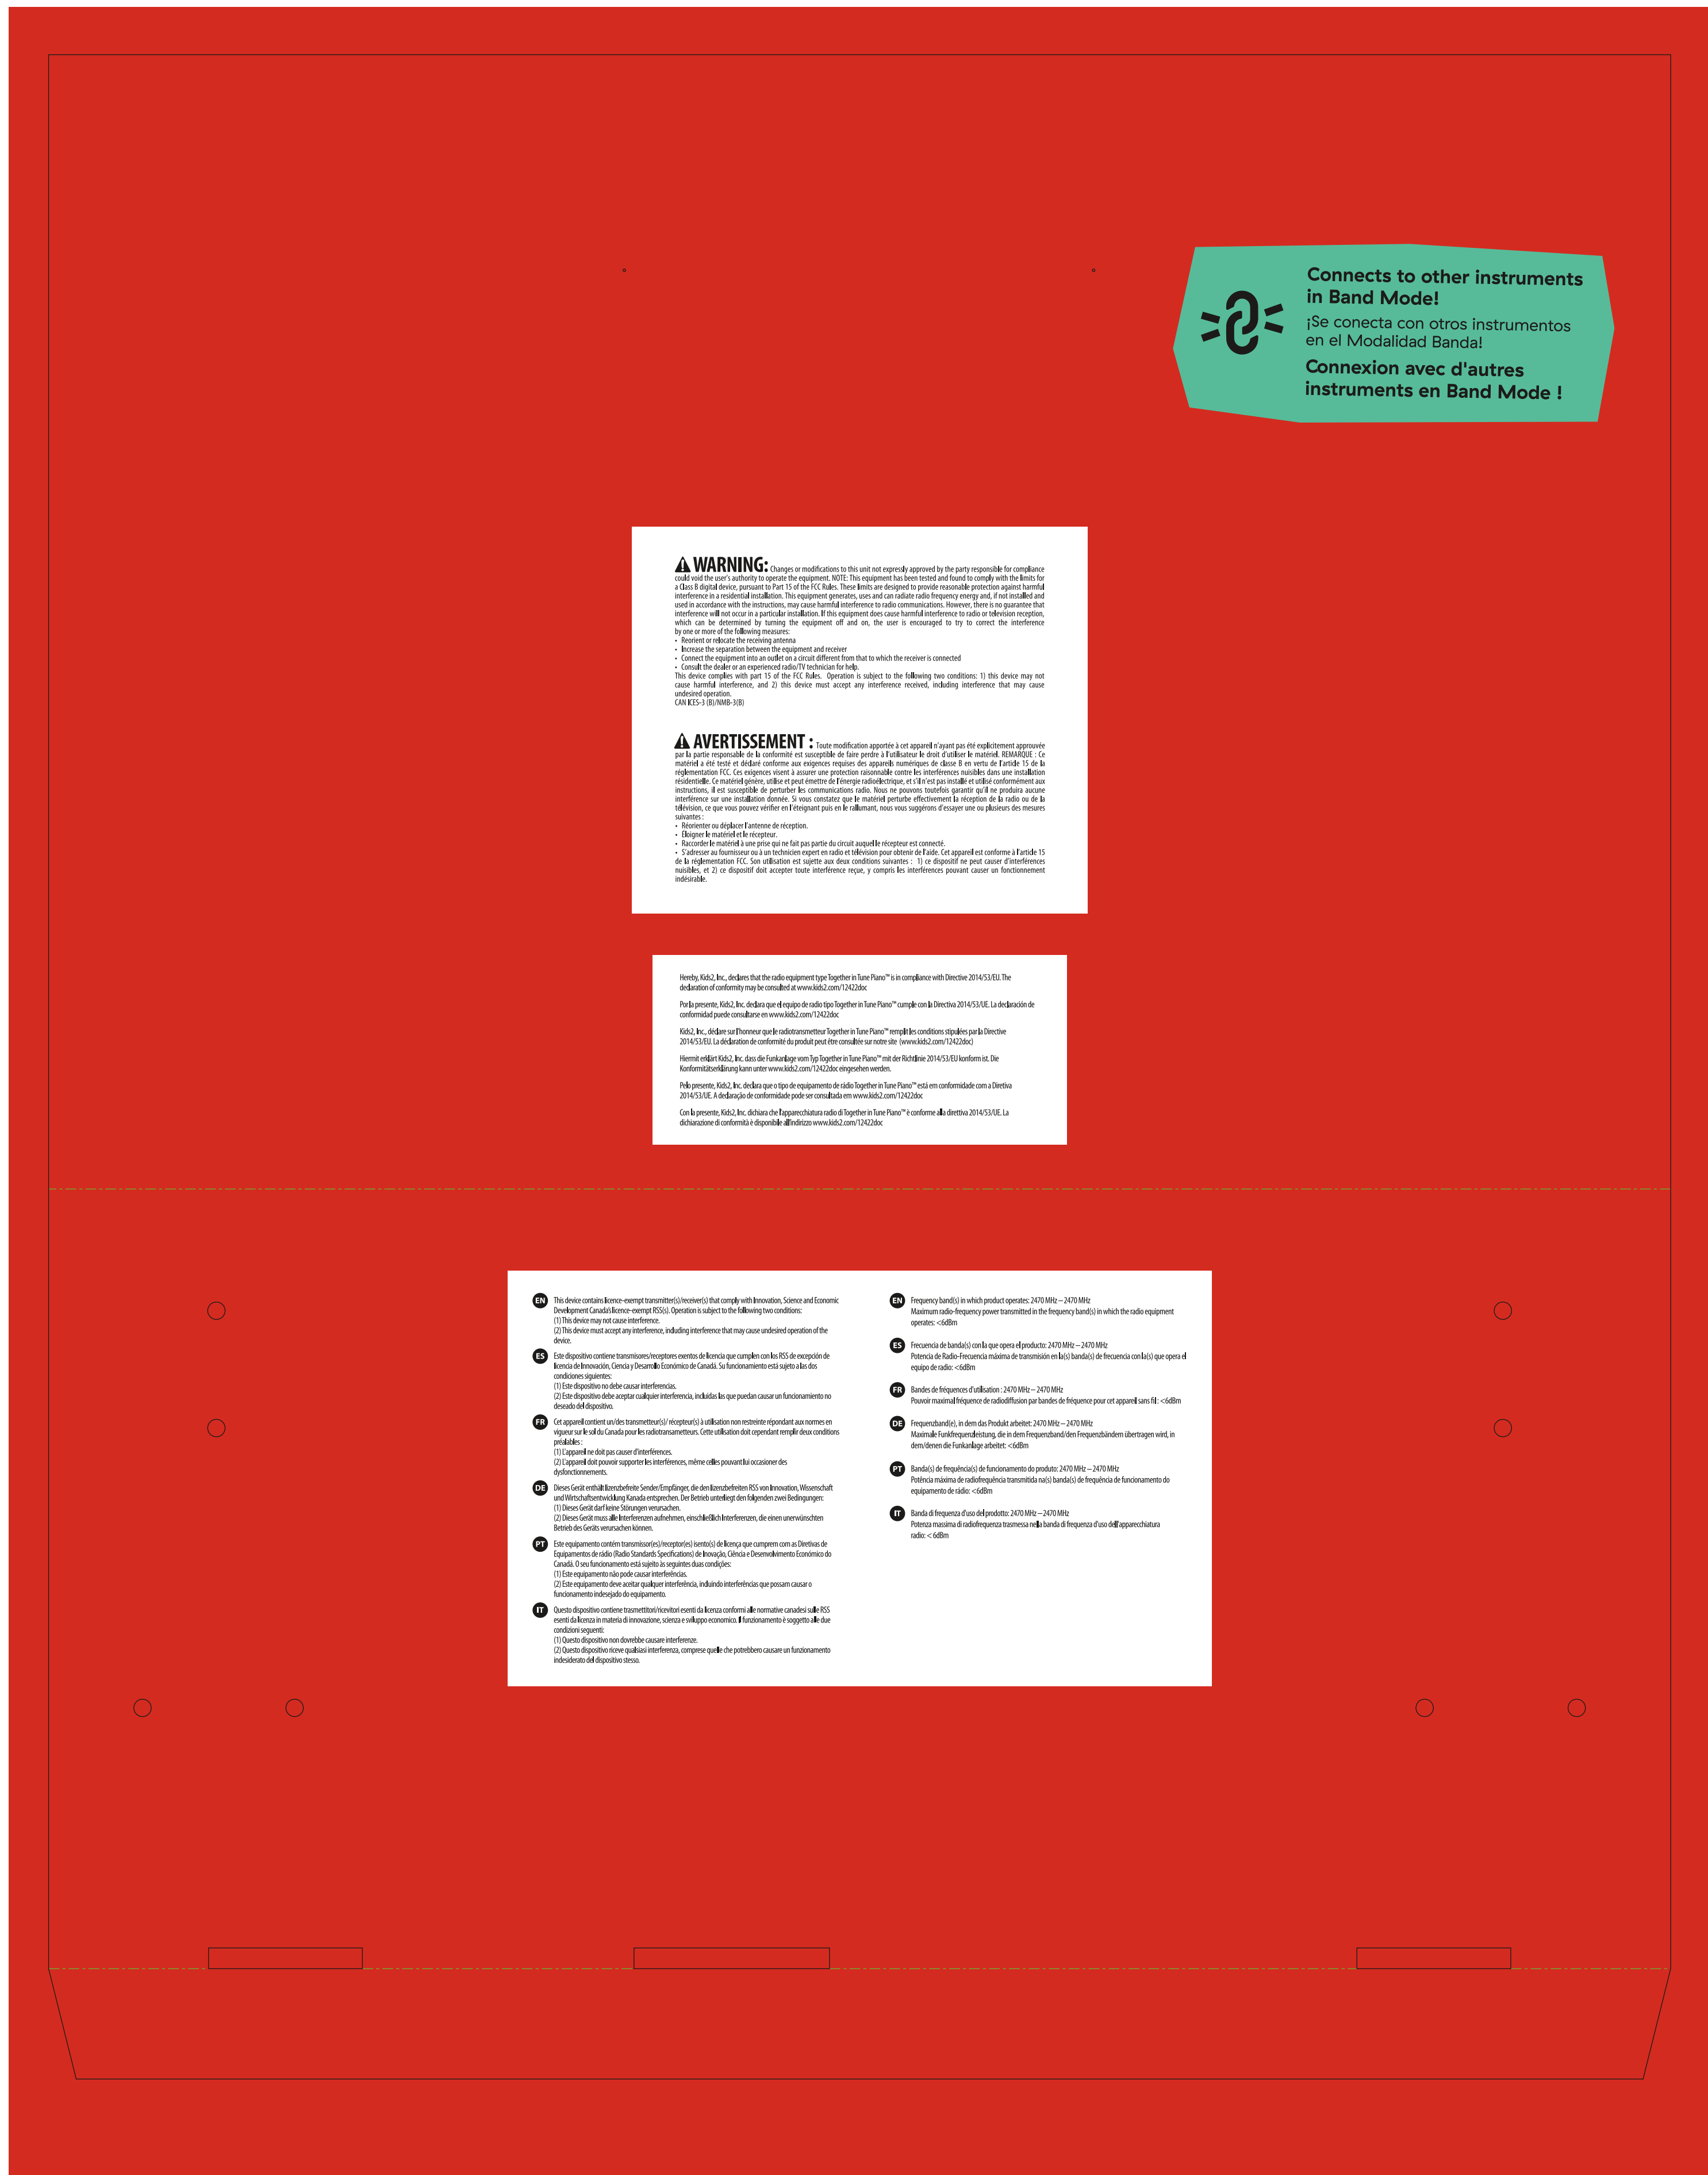

please secure the toy using cable ties

hole locations will be created by manufacturer