

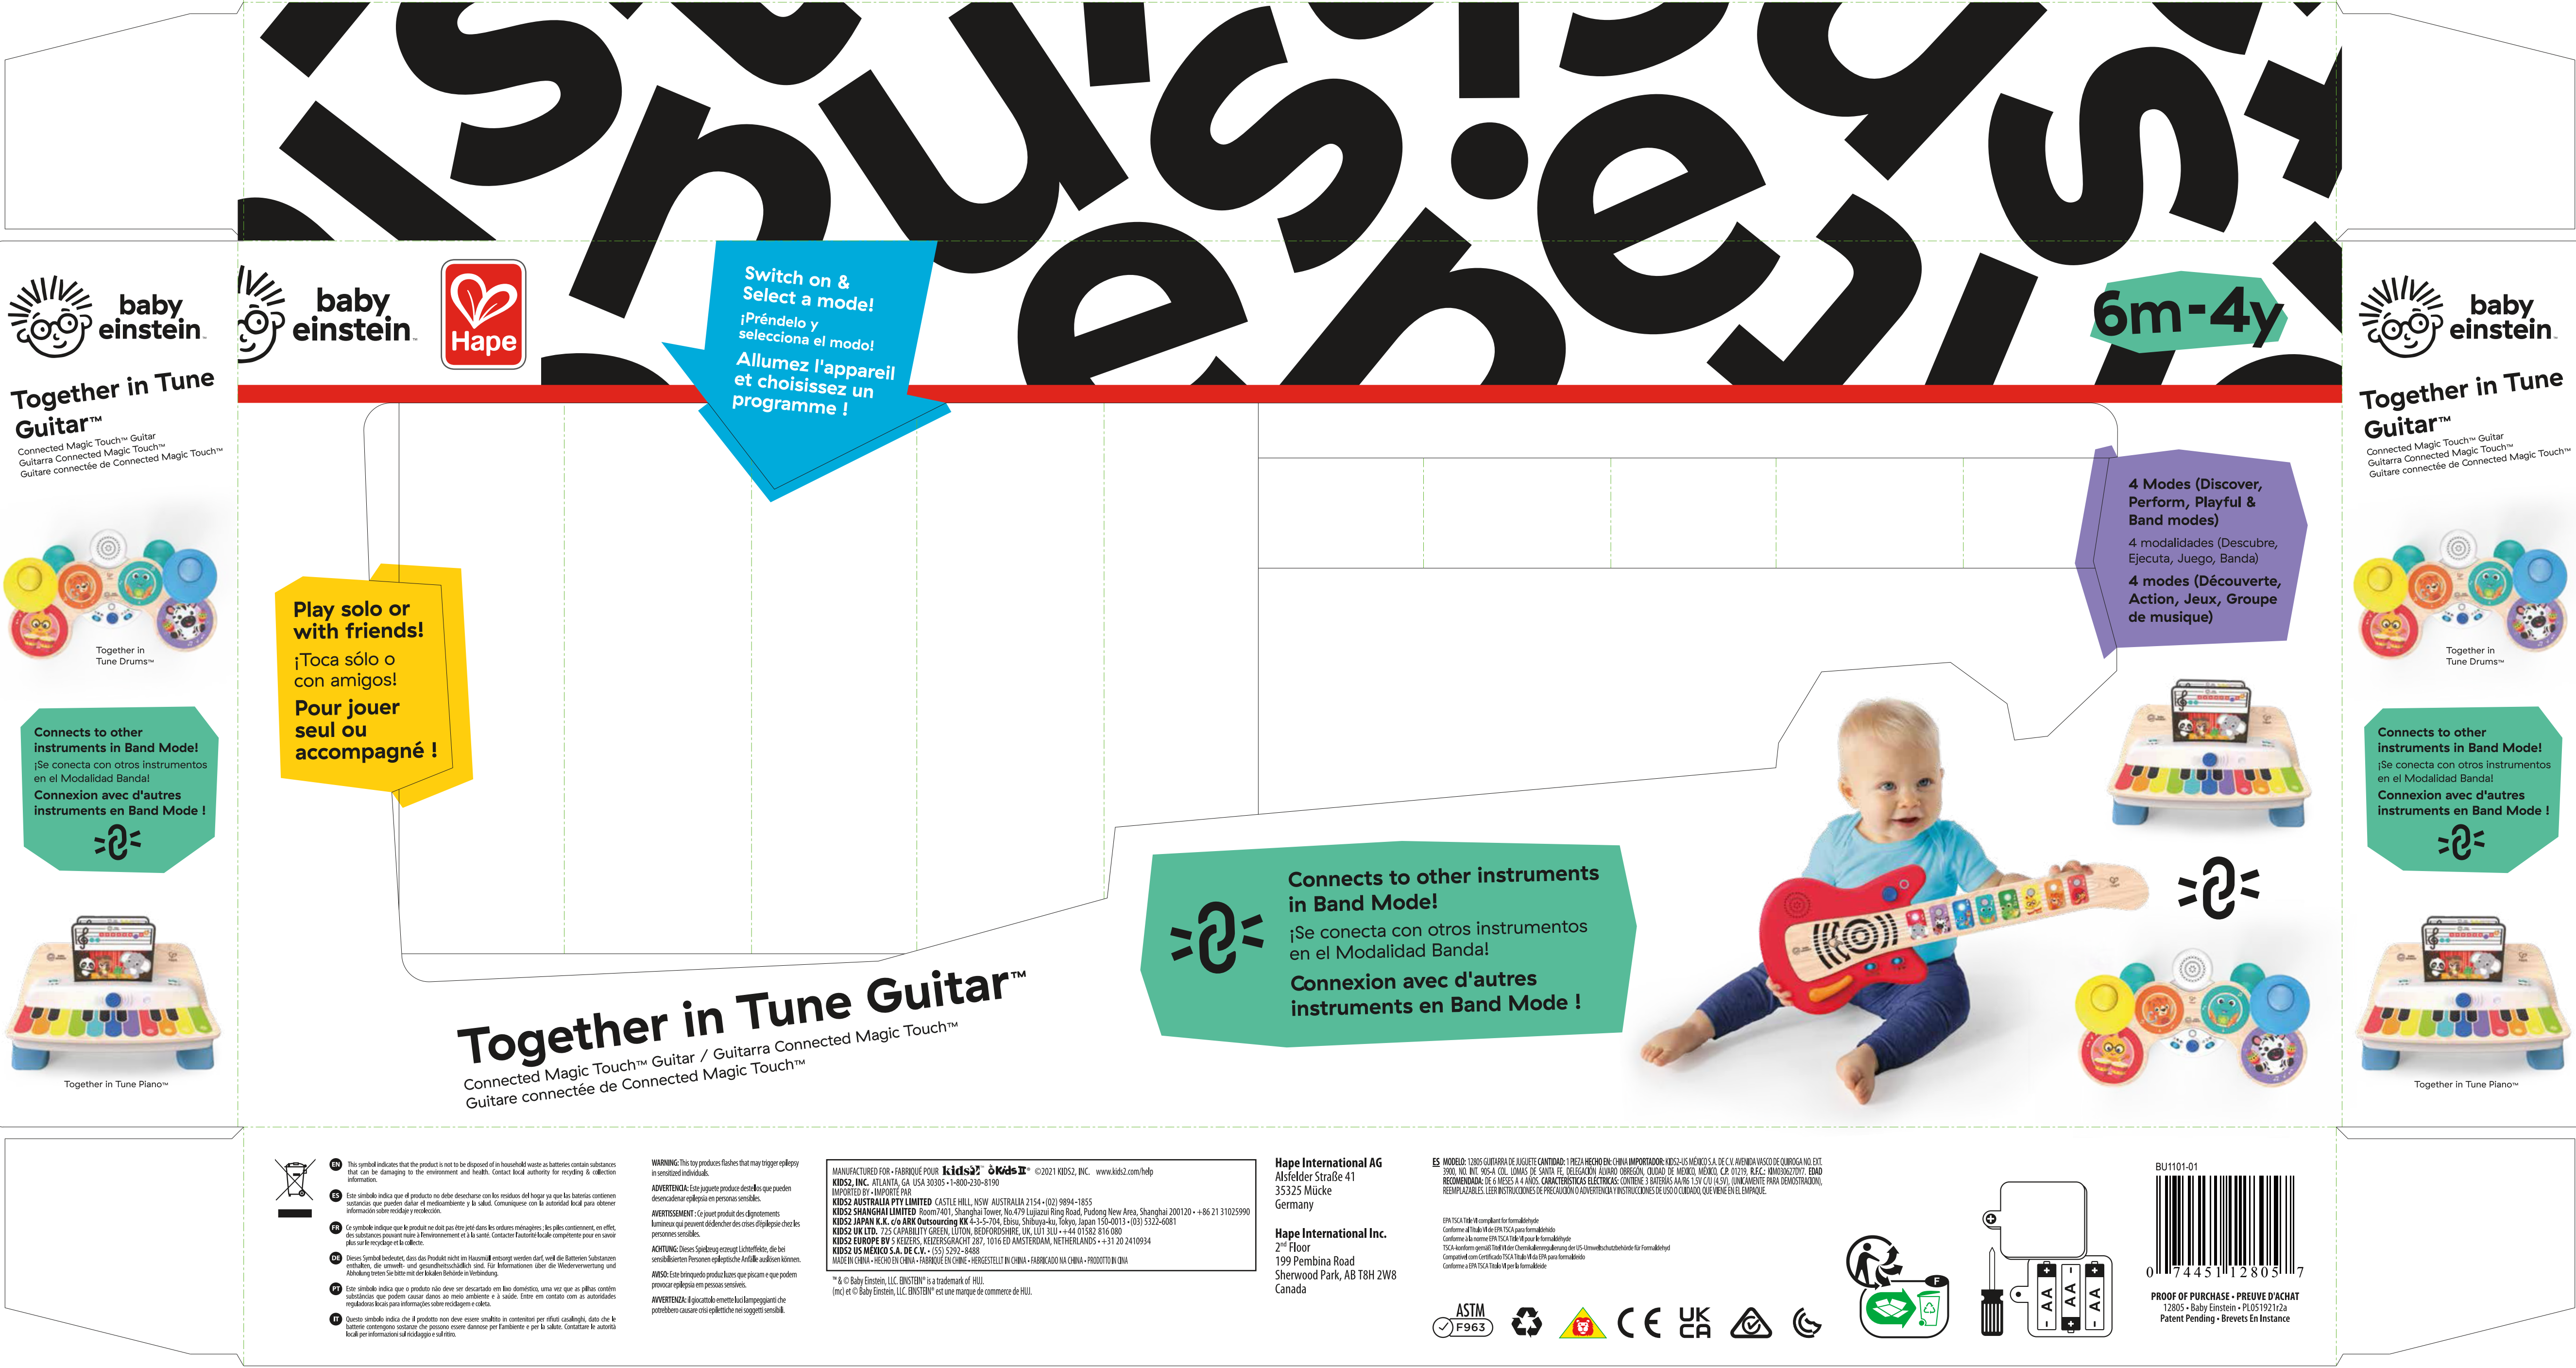


There are two color bars on this proof and in the art file. One to be used with X-rite i1 Pro Spectrophotometer. The other can be used with most other spectrophotometers. Printers must repeat one of the two color bars all the way across the width of the press sheet on sample run and production run. Failure to comply will result in the remaining of film and/or plates in your cost. 数据图以及设计文件也包含了两种色标。一种适用于X-rite i1 Pro分光光度计。另一种适用于其它大部分分光光度计。在打样或批量生产时，印刷厂必须重复其中一种色标并贯穿整张及印刷量最高的整张（即100%）。否则印刷上浪费更多纸张数量且影响。出版商将使用印刷厂沟通。

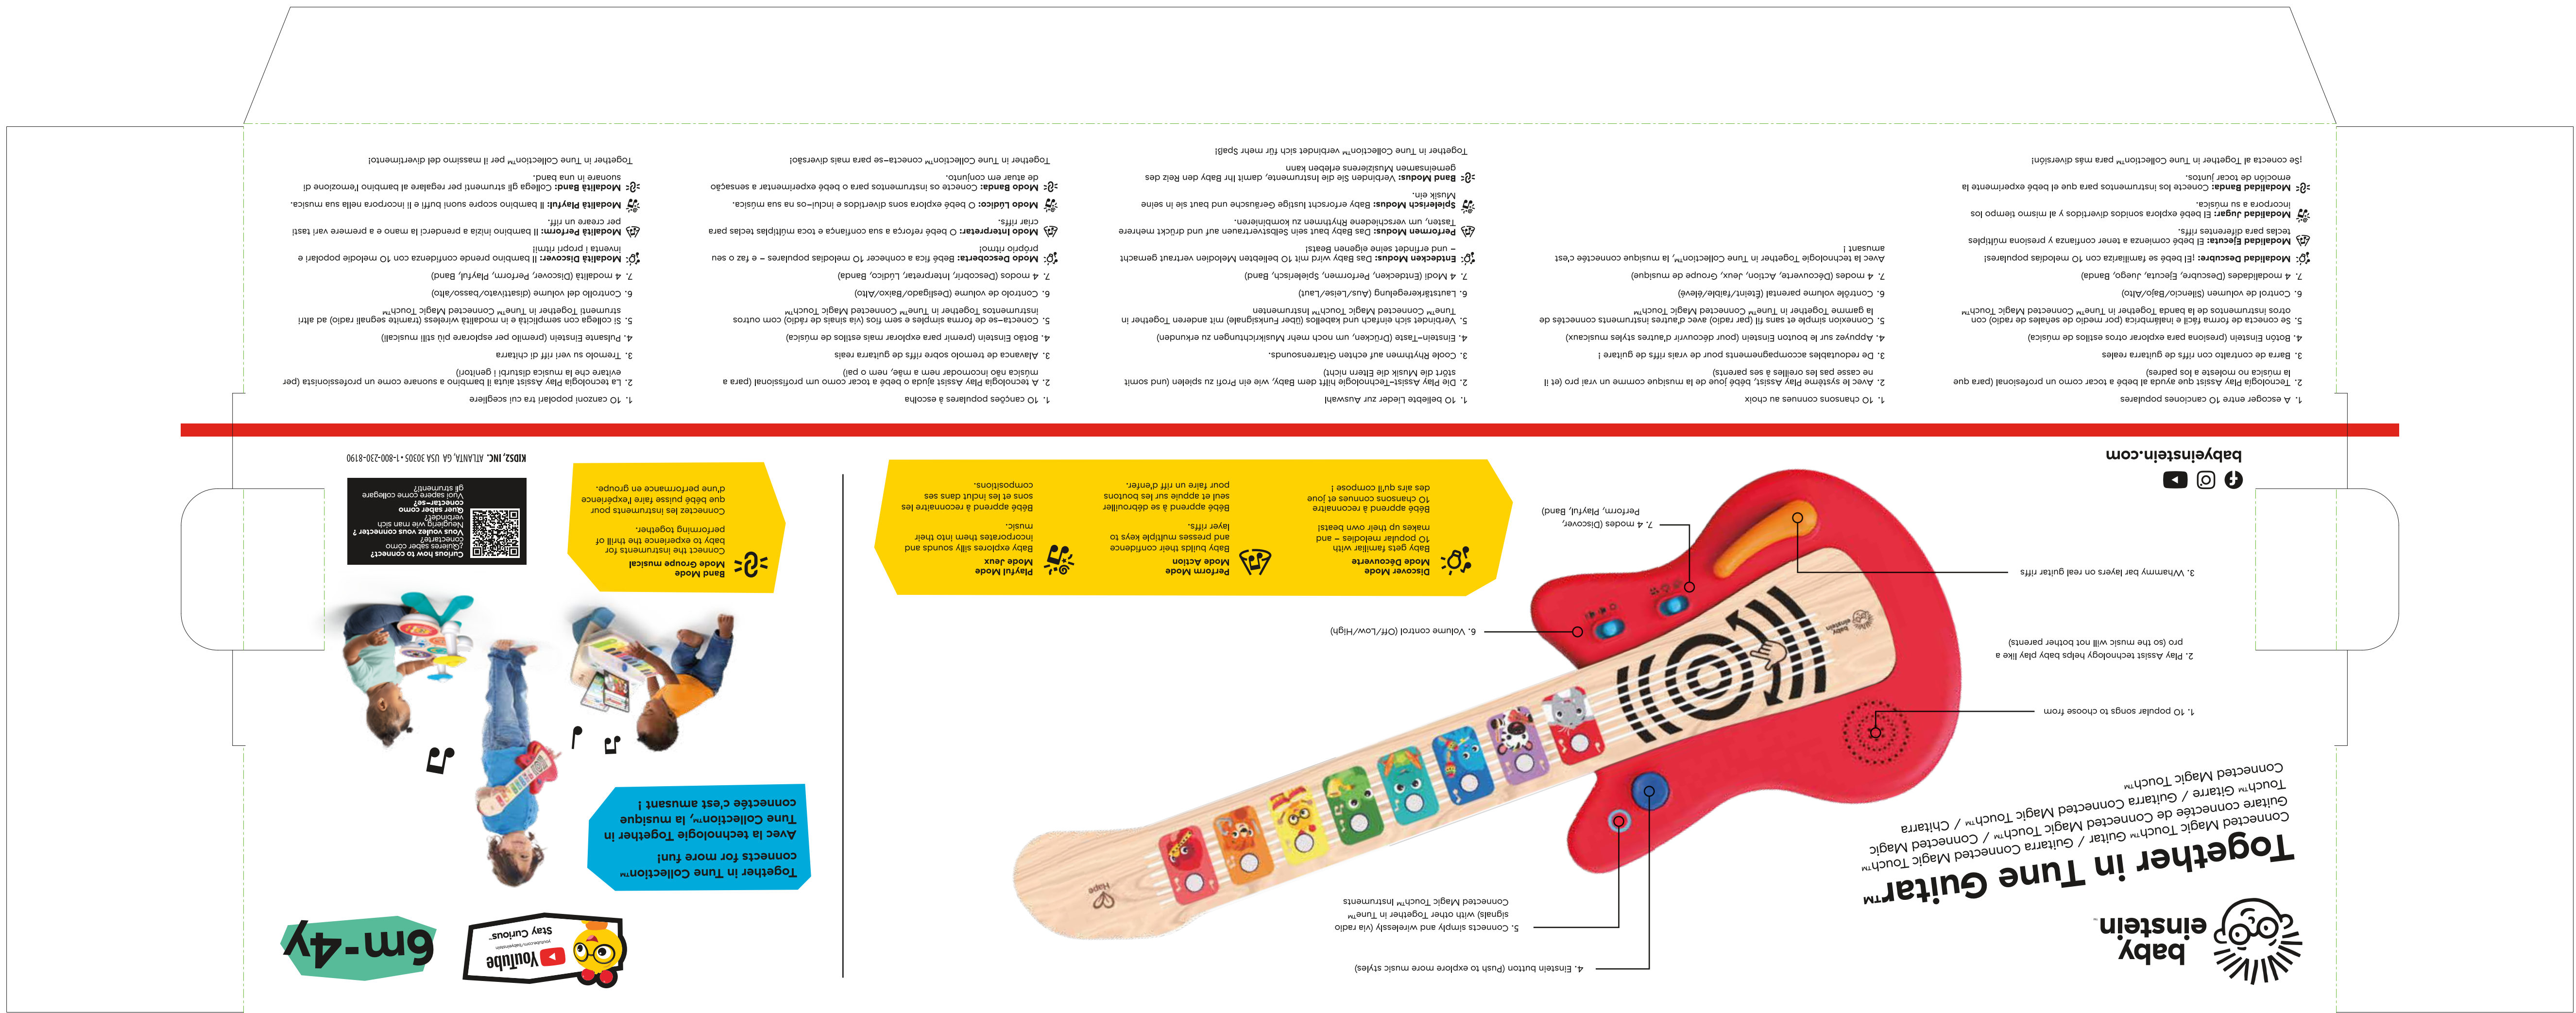

please secure the toy using cable ties
hole locations will be created by manufacturer

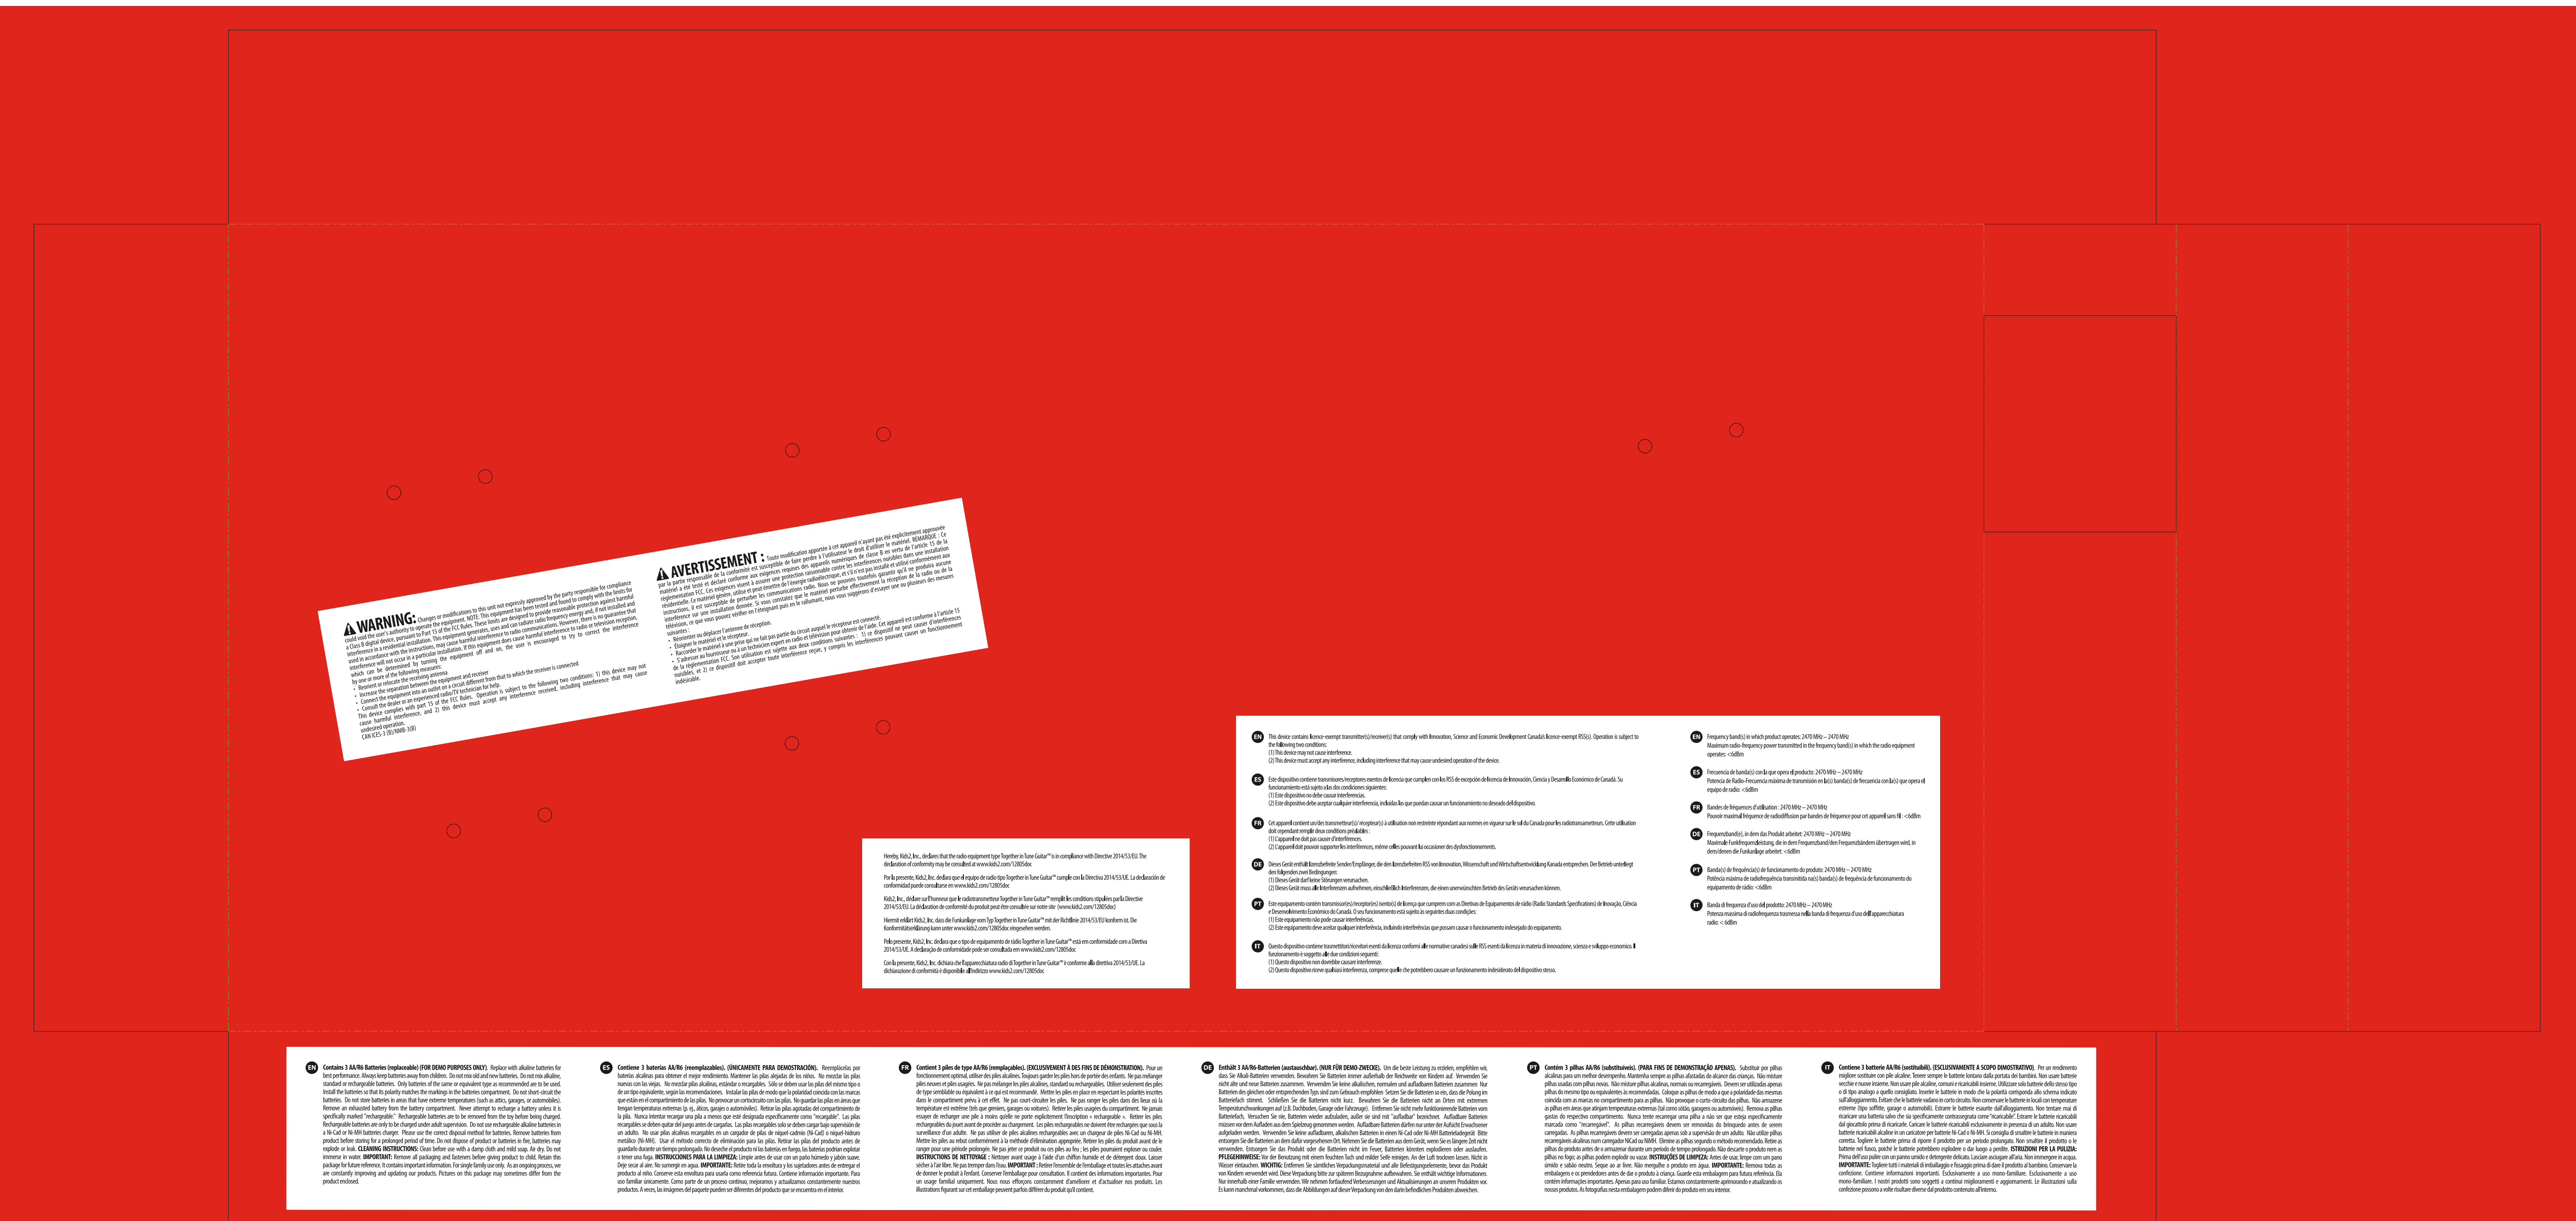