

EX3DV4 Sn:3708

EX3DV4- SN:3708 November 10, 2016

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>f</sup>	Conductivity (S/m) <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>h</sup> (mm)	Unc (k=2)
900	41.5	0.97	9.05	9.05	9.05	0.48	0.90	± 12.0 %
1810	40.0	1.40	7.84	7.84	7.84	0.36	0.80	± 12.0 %
2000	40.0	1.40	7.85	7.85	7.85	0.31	0.80	± 12.0 %
2450	39.2	1.80	7.11	7.11	7.11	0.29	0.95	± 12.0 %
5200	36.0	4.66	5.53	5.53	5.53	0.35	1.80	± 13.1 %
5300	35.9	4.76	5.30	5.30	5.30	0.35	1.80	± 13.1 %
5500	35.6	4.96	5.00	5.00	5.00	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.81	4.81	4.81	0.40	1.80	± 13.1 %
5800	35.3	5.27	5.01	5.01	5.01	0.40	1.80	± 13.1 %

<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2); else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 200 MHz respectively. Above 3 GHz frequency validity can be extended to ± 110 MHz.  
<sup>f</sup> At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.  
<sup>g</sup> AlphaDepth are determined during calibration. SPEAC warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3 & 6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-3708\_Nov16 Page 5 of 11

EX3DV4- SN:3708 November 10, 2016

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708

Calibration Parameter Determined in Body Tissue Simulating Media


f (MHz) <sup>c</sup>	Relative Permittivity <sup>f</sup>	Conductivity (S/m) <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>h</sup> (mm)	Unc (k=2)
900	55.0	1.05	9.10	9.10	9.10	0.48	0.80	± 12.0 %
1810	53.3	1.52	7.79	7.79	7.79	0.44	0.80	± 12.0 %
2000	53.3	1.52	7.71	7.71	7.71	0.43	0.80	± 12.0 %
2450	52.7	1.95	7.27	7.27	7.27	0.45	0.80	± 12.0 %
5200	49.0	5.30	4.62	4.62	4.62	0.45	1.90	± 13.1 %
5300	48.9	5.42	4.51	4.51	4.51	0.45	1.90	± 13.1 %
5500	48.6	5.65	4.07	4.07	4.07	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.95	3.95	3.95	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.13	4.13	4.13	0.50	1.90	± 13.1 %

<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2); else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 200 MHz respectively. Above 3 GHz frequency validity can be extended to ± 110 MHz.  
<sup>f</sup> At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.  
<sup>g</sup> AlphaDepth are determined during calibration. SPEAC warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3 & 6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-3708\_Nov16 Page 6 of 11

EX3DV4- SN:3708 November 10, 2016

Frequency Response of E-Field  
(TEM-Cell:if110 EXX, Waveguide: R22)


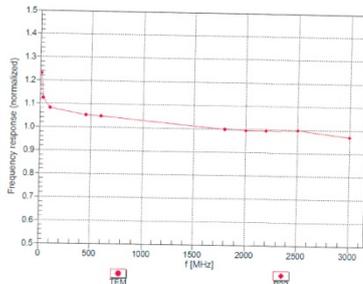


Uncertainty of Frequency Response of E-Field: ± 6.3% (k=2)

Certificate No: EX3-3708\_Nov16 Page 7 of 11

EX3DV4- SN:3708 November 10, 2016

Receiving Pattern (φ), θ = 0°

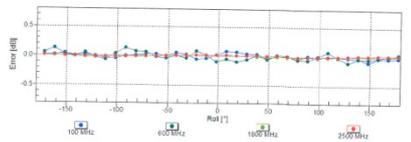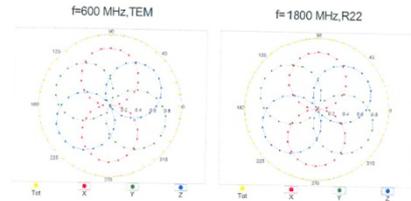


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3708\_Nov16 Page 8 of 11


EX3DV4 Sn:3708

EX3DV4- SN:3708 November 10, 2016

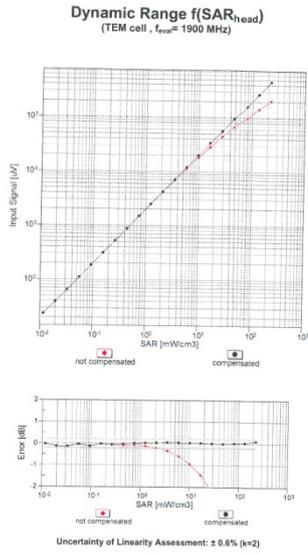

Certificate No: EX3-3708\_Nov16 Page 9 of 11

EX3DV4- SN:3708 November 10, 2016

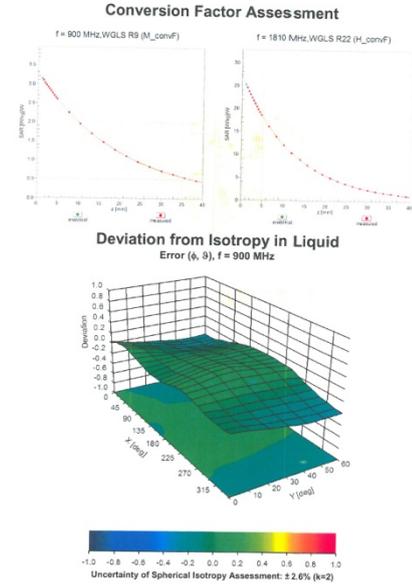

Certificate No: EX3-3708\_Nov16 Page 10 of 11

EX3DV4- SN:3708 November 10, 2016

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3708**

**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	-1.9
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Certificate No: EX3-3708\_Nov16 Page 11 of 11

D750V3 Sn:1101

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates  
Accreditation No.: SCS 0108

Client: SRTC (Vitec) Certificate No.: D750V3-1101\_Oct16

**CALIBRATION CERTIFICATE**

Object: D750V3 - SN:1101

Calibration procedure(s): QA CAL-05.v9  
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: October 24, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability given on the following pages are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 0.2 °C and humidity < 70%.

Calibration Equipment used (MTE critical for calibration):

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-291	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-291	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (20k)	05-Apr-16 (No. 217-02290)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 08327	05-Apr-16 (No. 217-02293)	Apr-17
Reference Probe EX320V4	SN: 7349	15-Jun-16 (No. EX3-7349_Jun16)	Jun-17
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16

Secondary Standards	ID #	Check Date (In house)	Scheduled Check
Power meter EPM-442A	SN: 08317480704	07-Oct-15 (In house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (In house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY10102317	07-Oct-15 (In house check Oct-16)	In house check: Oct-18
RF generator RAS SMT-06	SN: 100972	15-Jun-16 (In house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37300585	18-Oct-15 (In house check Oct-16)	In house check: Oct-17

Calibrated by: Lorif Kiyasar, Laboratory Technician, Signature: *Lorif Kiyasar*

Approved by: Katja Pokovic, Technical Manager, Signature: *Katja Pokovic*

This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: October 25, 2016

Certificate No: D750V3-1101\_Oct16 Page 1 of 8

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates  
Accreditation No.: SCS 0108

Client: SRTC (Vitec) Certificate No.: D750V3-1101\_Oct16

Glossary:  
TSL tissue simulating liquid  
ConvF sensitivity in TSL / NORM x,y,z  
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 86564, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:  
e) DAS4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D750V3-1101\_Oct16 Page 2 of 8

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASYS	V52 8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular/Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

Temperature	Permittivity	Conductivity	
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.1 ± 6 %	0.92 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.11 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	8.19 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.38 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.39 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

Temperature	Permittivity	Conductivity	
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.6 ± 6 %	0.97 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.17 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	8.62 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.44 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	5.72 W/kg ± 18.5 % (k=2)

Certificate No: D750V3-1101\_Oct16 Page 3 of 8

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	55.4 Ω ± 0.2 Ω
Return Loss	- 25.9 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	50.8 Ω ± 2.4 Ω
Return Loss	- 32.0 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.034 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	July 05, 2013

Certificate No: D750V3-1101\_Oct16 Page 4 of 8

D750V3 Sn:1101

DASY5 Validation Report for Head TSL

Date: 24.10.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1101


Communication System: UID 0 - CW; Frequency: 750 MHz  
Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.92$  S/m;  $\epsilon_r = 41.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.07, 10.07, 10.07); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 58.05 V/m; Power Drift = 0.00 dB  
Peak SAR (extrapolated) = 3.14 W/kg  
SAR(1 g) = 2.11 W/kg; SAR(10 g) = 1.38 W/kg  
Maximum value of SAR (measured) = 2.80 W/kg

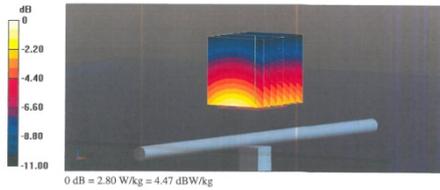

Certificate No: D750V3-1101\_Oct16

Page 5 of 8

Impedance Measurement Plot for Head TSL

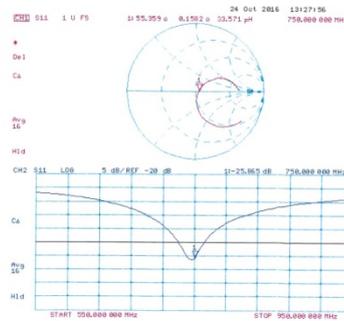

Certificate No: D750V3-1101\_Oct16

Page 6 of 8

DASY5 Validation Report for Body TSL

Date: 24.10.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1101


Communication System: UID 0 - CW; Frequency: 750 MHz  
Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.97$  S/m;  $\epsilon_r = 55.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.99, 9.99, 9.99); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 56.73 V/m; Power Drift = -0.00 dB  
Peak SAR (extrapolated) = 3.19 W/kg  
SAR(1 g) = 2.17 W/kg; SAR(10 g) = 1.44 W/kg  
Maximum value of SAR (measured) = 2.85 W/kg

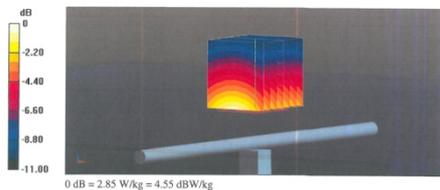

Certificate No: D750V3-1101\_Oct16

Page 7 of 8

Impedance Measurement Plot for Body TSL

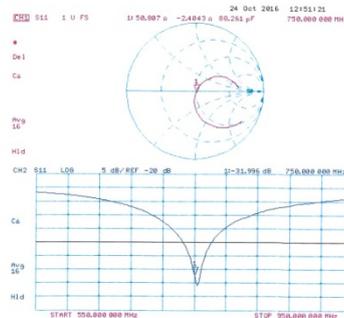

Certificate No: D750V3-1101\_Oct16

Page 8 of 8

D835V2 Sn:4d023

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates  
Accreditation No.: SCS 0108

Client: SRTC (Vitec) Certificate No: D835V2-4d023\_Oct16

**CALIBRATION CERTIFICATE**

Object: D835V2 - SN:4d023

Calibration procedure(s): QA CAL-05-VG  
Calibration procedure for dipole validation kits above 700 MHz.

Calibration date: October 24, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 0.2 °C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5088 (20k)	05-Apr-16 (No. 217-02292)	Apr-17
Type N mismatch combination	SN: 3047.2 / 06327	05-Apr-16 (No. 217-02293)	Apr-17
Reference Probe EX32V4	SN: 7369	15-Jun-16 (No. D32-7349_Jun16)	Jun-17
DAE4	SN: 601	30-Dec-15 (No. DAE4-601_Dec15)	Dec-16

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: G837480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP #481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP #811A	SN: MY41029317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SM4-06	SN: 100972	15-Jun-16 (in house check Oct-16)	In house check: Oct-18
Network Analyser HP #7533E	SN: US37300585	19-Oct-01 (in house check Oct-16)	In house check: Oct-17

Calibrated by: Lef Kysner, Laboratory Technician, Signature: *Lef Kysner*

Approved by: Katja Pokovic, Technical Manager, Signature: *Katja Pokovic*

Issued: October 25, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates  
Accreditation No.: SCS 0108

Client: SRTC (Vitec) Certificate No: D835V2-4d023\_Oct16

Glossary:  
TSL: tissue simulating liquid  
ConvF: sensitivity in TSL / NORM x,y,z  
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:  
e) DASy4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASy system configuration, as far as not given on page 1.

DASy Version	DASy5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.8 ± 6 %	0.85 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.47 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.45 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.59 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.14 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	0.99 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.44 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.82 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.60 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.33 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	53.4 Ω - 1.9 jΩ
Return Loss	-28.4 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	49.3 Ω + 5.1 jΩ
Return Loss	-25.8 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.389 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	December 17, 2004

D835V2 Sn:4d023

DASY5 Validation Report for Head TSL

Date: 24.10.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d023


Communication System: UID 0 - CW; Frequency: 835 MHz  
Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.95$  S/m;  $\epsilon_r = 40.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.72, 9.72); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 61.72 V/m; Power Drift = 0.03 dB  
Peak SAR (extrapolated) = 3.72 W/kg  
SAR(1 g) = 2.47 W/kg; SAR(10 g) = 1.59 W/kg  
Maximum value of SAR (measured) = 3.30 W/kg

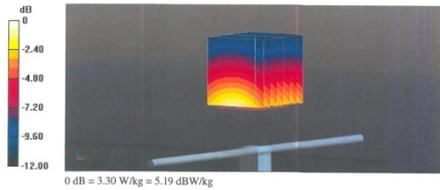

Certificate No: D835V2-4d023\_Oct16

Page 5 of 8

Impedance Measurement Plot for Head TSL

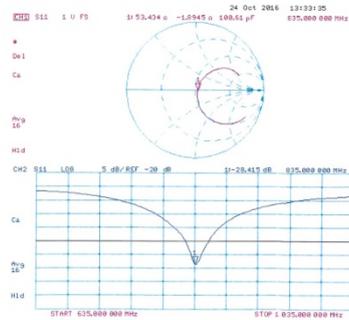

Certificate No: D835V2-4d023\_Oct16

Page 6 of 8

DASY5 Validation Report for Body TSL

Date: 24.10.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d023


Communication System: UID 0 - CW; Frequency: 835 MHz  
Medium parameters used:  $f = 835$  MHz;  $\sigma = 0.99$  S/m;  $\epsilon_r = 55.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.73, 9.73); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 59.97 V/m; Power Drift = 0.01 dB  
Peak SAR (extrapolated) = 3.54 W/kg  
SAR(1 g) = 2.44 W/kg; SAR(10 g) = 1.6 W/kg  
Maximum value of SAR (measured) = 3.19 W/kg

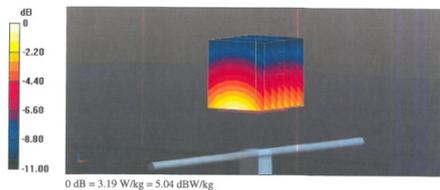

Certificate No: D835V2-4d023\_Oct16

Page 7 of 8

Impedance Measurement Plot for Body TSL

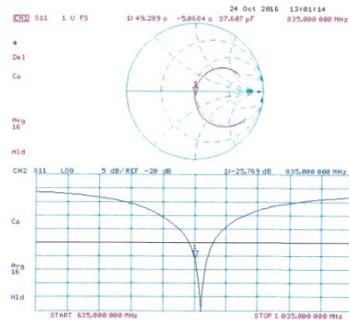

Certificate No: D835V2-4d023\_Oct16

Page 8 of 8

D1900V2 Sn:5d113

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client: SRTC (Vitec)

Certificate No: D1900V2-5d113\_Oct16

**CALIBRATION CERTIFICATE**

Object: D1900V2 - SN:5d113  
Calibration procedure(s): QA CAL-05.v0  
Calibration procedure for dipole validation kits above 700 MHz  
Calibration date: October 31, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-231	SN: 103344	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-231	SN: 103345	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (SN)	05-Apr-16 (No. 217-02292)	Apr-17
Type-A mismatch combination	SN: 5041.2 / 06327	15-Jun-16 (No. 13057369, Jun16)	Jun-17
Reference Probe EXD0V4	SN: 7349	30-Dec-16 (No. DAE4401_Dec16)	Dec-16
DAEA	SN: 801		

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: G637480704	07-Oct-16 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8441A	SN: US37292763	07-Oct-16 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8441A	SN: MV41092317	07-Oct-16 (in house check Oct-16)	In house check: Oct-18
RF generator RAS SMT-06	SN: 100972	15-Jun-16 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8733E	SN: US37390585	18-Oct-16 (in house check Oct-16)	In house check: Oct-17

Calibrated by: Jeton Kastalli, Laboratory Technician  
Approved by: Kapa Pokovic, Technical Manager  
Issued: October 31, 2016

Certificate No: D1900V2-5d113\_Oct16 Page 1 of 8

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

TSL: tissue simulating liquid  
CorvF: sensitivity in TSL / NORM x,y,z  
N/A: not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 85664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d113\_Oct16 Page 2 of 8

**Measurement Conditions**

DASY system configuration, as far as not given on page 1

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	49.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.7 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.2 ± 6 %	1.48 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.80 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	39.8 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.23 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.1 W/kg ± 16.5 % (k=2)

Certificate No: D1900V2-5d113\_Oct16 Page 3 of 8

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	51.1 Ω ± 6.5 Ω
Return Loss	-23.8 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	47.0 Ω ± 7.2 Ω
Return Loss	-21.9 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.200 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	July 24, 2009

Certificate No: D1900V2-5d113\_Oct16 Page 4 of 8

D1900V2 Sn:5d113

DASY5 Validation Report for Head TSL

Date: 31.10.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d113


Communication System: UID 0 - CW; Frequency: 1900 MHz  
Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.39$  S/m;  $\epsilon_r = 40.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.99, 7.99, 7.99); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 108.4 V/m; Power Drift = -0.02 dB  
Peak SAR (extrapolated) = 19.0 W/kg  
SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.3 W/kg  
Maximum value of SAR (measured) = 15.7 W/kg

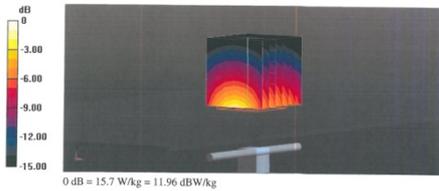

Certificate No: D1900V2-5d113\_Oct16

Page 5 of 8

Impedance Measurement Plot for Head TSL

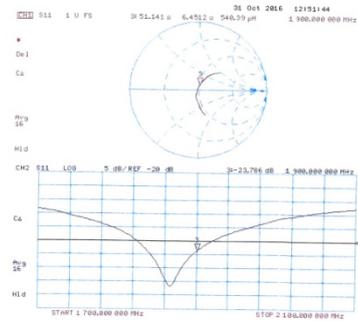

Certificate No: D1900V2-5d113\_Oct16

Page 6 of 8

DASY5 Validation Report for Body TSL

Date: 31.10.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d113


Communication System: UID 0 - CW; Frequency: 1900 MHz  
Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.48$  S/m;  $\epsilon_r = 53.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.03, 8.03, 8.03); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 104.5 V/m; Power Drift = -0.09 dB  
Peak SAR (extrapolated) = 17.2 W/kg  
SAR(1 g) = 9.8 W/kg; SAR(10 g) = 5.23 W/kg  
Maximum value of SAR (measured) = 14.7 W/kg

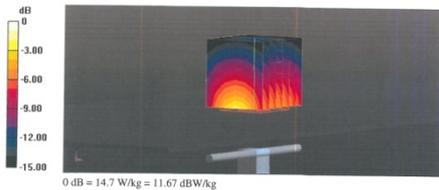

Certificate No: D1900V2-5d113\_Oct16

Page 7 of 8

Impedance Measurement Plot for Body TSL

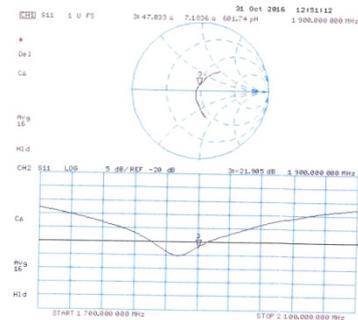

Certificate No: D1900V2-5d113\_Oct16

Page 8 of 8

D2450V2 Sn:738

Calibration Laboratory of Schmid & Partner Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
S Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client: SRTC (Vitec) Certificate No: D2450V2-738\_Oct16

**CALIBRATION CERTIFICATE**

Object: D2450V2 - SN:738  
Calibration procedure(s): QA CAL-05.v9  
Calibration date: October 25, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104178	06-Apr-18 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103844	06-Apr-18 (No. 217-02298)	Apr-17
Power sensor NRP-Z91	SN: 103845	06-Apr-18 (No. 217-02299)	Apr-17
Reference 20 dB Attenuator	SN: 5058 (804)	05-Apr-18 (No. 217-02292)	Apr-17
Type-N mismatch combination	SN: 5047.2 / 06327	05-Apr-18 (No. 217-02296)	Apr-17
Reference Probe EX20V4	SN: 7348	15-Jun-18 (No. E30-7349_Jun18)	Jun-17
DAEA	SN: 601	30-Dec-18 (No. DAE4-601_Dec18)	Dec-16

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: G18748/04	07-Oct-18 (in house check Oct-18)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292703	07-Oct-18 (in house check Oct-18)	In house check: Oct-18
Power sensor HP 8481A	SN: MVA1020217	07-Oct-18 (in house check Oct-18)	In house check: Oct-18
RF generator RAS SMF-06	SN: 100972	15-Jun-18 (in house check Oct-18)	In house check: Oct-18
Network Analyzer HP 8733E	SN: US37300585	18-Oct-18 (in house check Oct-18)	In house check: Oct-17

Calibrated by: Claudio Lauber, Laboratory Technician  
Approved by: Kata Piskovic, Technical Manager

Certificate No: D2450V2-738\_Oct16 Page 1 of 8

Calibration Laboratory of Schmid & Partner Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
S Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client: SRTC (Vitec) Certificate No: D2450V2-738\_Oct16

**Glossary:**

TSL: tissue simulating liquid  
Conv/F: sensitivity in TSL: NORM x,y,z  
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:  
e) DASY4/5 System Handbook

- Methods Applied and Interpretation of Parameters:**
- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
  - **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
  - **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
  - **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
  - **SAR measured:** SAR measured at the stated antenna input power.
  - **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
  - **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-738\_Oct16 Page 2 of 8

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.2 ± 6 %	1.87 mho/m ± 8 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	51.2 W/kg ± 17.0 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.3 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.0 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	50.8 W/kg ± 17.0 % (k=2)

Certificate No: D2450V2-738\_Oct16 Page 3 of 8

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	53.6 Ω ± 2.1 Ω
Return Loss	-27.8 dB

**Antenna Parameters with Body TSL**

Impedance, transformed to feed point	49.7 Ω ± 5.9 Ω
Return Loss	-24.5 dB

**General Antenna Parameters and Design**

Electrical Delay (one direction)	1.157 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	August 26, 2003

Certificate No: D2450V2-738\_Oct16 Page 4 of 8

D2450V2 Sn:738

DASY5 Validation Report for Head TSL

Date: 25.10.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:738


Communication System: UID 0 - CW; Frequency: 2450 MHz  
Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.87$  S/m;  $\epsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.72, 7.72, 7.72); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 111.7 V/m; Power Drift = -0.00 dB  
Peak SAR (extrapolated) = 26.4 W/kg  
SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.07 W/kg  
Maximum value of SAR (measured) = 21.4 W/kg

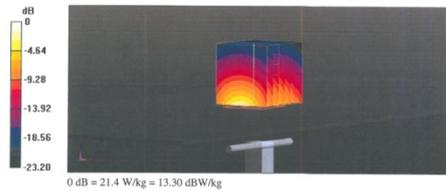

Certificate No: D2450V2-738\_Oct16

Page 5 of 8

Impedance Measurement Plot for Head TSL

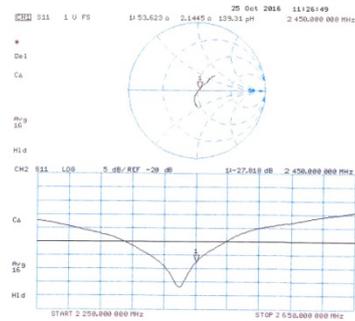

Certificate No: D2450V2-738\_Oct16

Page 6 of 8

DASY5 Validation Report for Body TSL

Date: 25.10.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:738


Communication System: UID 0 - CW; Frequency: 2450 MHz  
Medium parameters used:  $f = 2450$  MHz;  $\sigma = 2.02$  S/m;  $\epsilon_r = 51.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.79, 7.79, 7.79); Calibrated: 15.06.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 107.3 V/m; Power Drift = -0.04 dB  
Peak SAR (extrapolated) = 26.0 W/kg  
SAR(1 g) = 13 W/kg; SAR(10 g) = 6.08 W/kg  
Maximum value of SAR (measured) = 21.3 W/kg

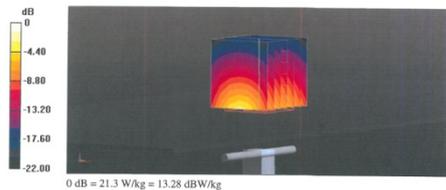

Certificate No: D2450V2-738\_Oct16

Page 7 of 8

Impedance Measurement Plot for Body TSL

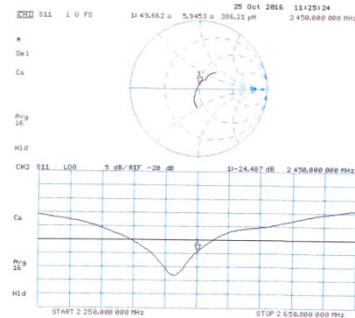

Certificate No: D2450V2-738\_Oct16

Page 8 of 8

D2600V2 Sn:1089

Calibration Laboratory of  
Schindler & Partner  
Engineering AG  
Zougstrasse 43, 8034 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service Suisse de Calibration  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates  
Accreditation No.: SCS 0108

Client: Sony Mobile CN (Vitec) Certificate No: D2600V2-1089\_Jul16

**CALIBRATION CERTIFICATE**

**Object:** D2600V2 - SN: 1089

**Calibration procedure(s):** QA-CAL-05-V9  
Calibration procedure for dipole validation kits above 700 MHz

**Calibration date:** July 13, 2016

This calibration certificate documents the traceability to national standards, which realize the physical units of measurement (SI).  
The measurement and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the clean laboratory facility, environmental temperature (20 ± 0.5) °C and humidity < 75%.

Calibration Equipment used (MATE except for calibration):

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104776	06-Apr-16 (No.: 217-02089-20089)	Apr-17
Power sensor NRP-Z91	SN: 100014	06-Apr-16 (No.: 217-02090)	Apr-17
Power sensor NRP-Z91	SN: 100016	06-Apr-16 (No.: 217-02090)	Apr-17
Reference 20-dB Attenuator	SN: 3658 (20k)	06-Apr-16 (No.: 217-02090)	Apr-17
Feed Point Impedance Comparator	SN: 13412 (30k)	19-Apr-16 (No.: 217-02090)	Apr-17
Reference Probe EPC2000	SN: 7246	17-Jan-16 (No.: ECR-7396-Jul16)	Jan-17
SAS1	SN: 101 (01)	30-Jan-15 (No.: IAE4-601)	Dec-16

Secondary Standards	ID#	Check Date (in use)	Scheduled Check
Power meter EPM-4101	NO: 1081480104	07-Oct-15 (No.: 217-02033)	In-house check: Oct-16
Power sensor HP-3487A	NO: 1051390103	07-Oct-15 (No.: 217-02072)	In-house check: Oct-16
Power sensor HP-3487A	NO: 1051390117	07-Oct-15 (No.: 217-02072)	In-house check: Oct-16
Attenuator 10kS-5011 (0)	NO: 1100107	15-Jan-15 (No.: 1004-7060-Jul-15)	In-house check: Jul-16
Reference Probe HP-1017V	NO: 1021390109	18-Oct-15 (In-house check: Jul-15)	In-house check: Jul-16

Submitted by: **Anton Kestner** (Laboratory Technician)

Approved by: **Kolja Pokorski** (Technical Manager)

Issue Date: July 14, 2016

Calibration Laboratory of  
Schindler & Partner  
Engineering AG  
Zougstrasse 43, 8034 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service Suisse de Calibration  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates  
Accreditation No.: SCS 0108

Client: Sony Mobile CN (Vitec) Certificate No: D2600V2-1089\_Jul16

**Glossary:**

TSL: Issue simulating liquid

CorrF: sensitivity in TSL / IORFA x,y,z

NA: not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- IEEE Std 1529-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- DASY4.5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

**Measurement Conditions**

DASY system configuration, as far as not given on page 1:

DASY Version	Power	Mag. SAR
4.5.0	10W	10W

Extrapolation	Antenna	Phantom
100%	Multi-Use Flat Phantom	Multi-Use Flat Phantom

Distance Dipole Center - TSL: 10 mm with Spacer

Zoom Scan Resolution: 4x, 4y, 4z (4x5 mm)

Frequency: 2600 MHz ± 1.594%

**Head TSL parameters**

The following parameters and calculations were applied:

Parameter	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	79.0	1.66 mho/m
Measured Head TSL parameters	22.0 ± 0.2 °C	77.5 ± 6 %	2.02 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	Value
SAR measured	250 mW input power	14.6 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	57.1 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	Value
SAR measured	250 mW input power	6.46 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	25.5 W/kg ± 16.5 % (k=2)

**Body TSL parameters**

The following parameters and calculations were applied:

Parameter	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.0	2.16 mho/m
Measured Body TSL parameters	22.0 ± 0.2 °C	51.4 ± 6 %	2.20 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

**SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	Value
SAR measured	250 mW input power	13.6 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	53.7 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	Value
SAR measured	250 mW input power	6.16 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	24.1 W/kg ± 16.5 % (k=2)

**Appendix (Additional assessments outside the scope of SCS 0108)**

**Antenna Parameters with Head TSL**

Parameter	Value
Impedance, transformed to feed point	48.5 Ω ± 6.8 Ω
Return Loss	-23.0 dB

**Antenna Parameters with Body TSL**

Parameter	Value
Impedance, transformed to feed point	45.8 Ω ± 6.0 Ω
Return Loss	-22.3 dB

**General Antenna Parameters and Design**

Parameter	Value
Electrical Delay (one direction)	1.146 ns

After long term use with 10W radiated power, only a slight warming of the dipole near the feedpoint can be measured.  
The dipole is made of standard serrated coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.  
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

Parameter	Value
Manufactured by	SPEAC
Manufactured on	March 15, 2014

D2600V2 Sn:1089

DASY5 Validation Report for Head TSL

Date: 11/07/2016

Test Laboratory: SPFAF, Zurich, Switzerland

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1089


Communication System: UTD 0 - CW; Frequency: 2600 MHz  
Medium parameters used:  $f = 2600 \text{ MHz}$ ;  $n = 2.02 \text{ S/m}$ ;  $\epsilon = 37.5$ ;  $\rho = 1000 \text{ kg/m}^3$   
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.56, 7.56); Calibrated: 15.06.2016
- Sensor Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 S2.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue(Pin=250 mW, d=10mm/Zoom Scan (7x7)/Cube 0):


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 117.2 V/m; Power Drift = 0.01 dB  
Peak SAR (extrapolated) = 11.2 W/kg  
SAR(1 g) = 14.6 W/kg; SAR(10 g) = 6.46 W/kg  
Maximum value of SAR (measured) = 25.0 W/kg

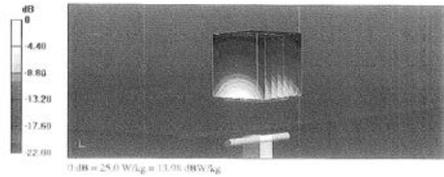

File Name: 11090707-1089-1108

Page 6 of 8

Impedance Measurement Plot for Head TSL

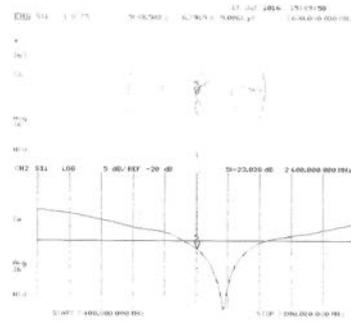

File Name: 11090707-1089-1108

Page 6 of 8

DASY5 Validation Report for Body TSL

Date: 07/07/2016

Test Laboratory: SPFAF, Zurich, Switzerland

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1089


Communication System: UTD 0 - CW; Frequency: 2600 MHz  
Medium parameters used:  $f = 2600 \text{ MHz}$ ;  $n = 2.2 \text{ S/m}$ ;  $\epsilon = 51.4$ ;  $\rho = 1000 \text{ kg/m}^3$   
Phantom section: Flat Section  
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.48, 7.48); Calibrated: 15.06.2016
- Sensor Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.12.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 S2.8.8(1258); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue(Pin=250 mW, d=10mm/Zoom Scan (7x7)/Cube 0):


Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 105.3 V/m; Power Drift = -0.07 dB  
Peak SAR (extrapolated) = 27.8 W/kg  
SAR(1 g) = 13.6 W/kg; SAR(10 g) = 6.06 W/kg  
Maximum value of SAR (measured) = 21.9 W/kg

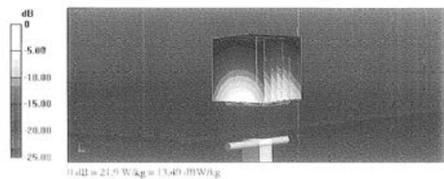

File Name: 11090707-1089-1108

Page 7 of 8


Impedance Measurement Plot for Body TSL

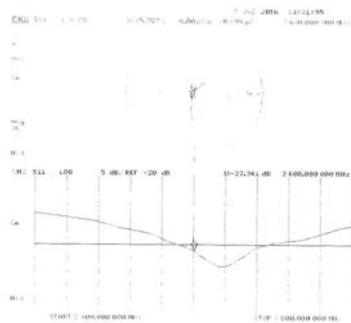


File Name: 11090707-1089-1108

Page 8 of 8


## ANNEX C - PHOTOGRAPH

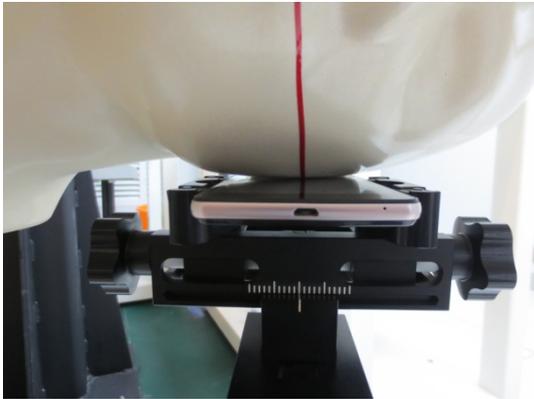


Cheek position, left side

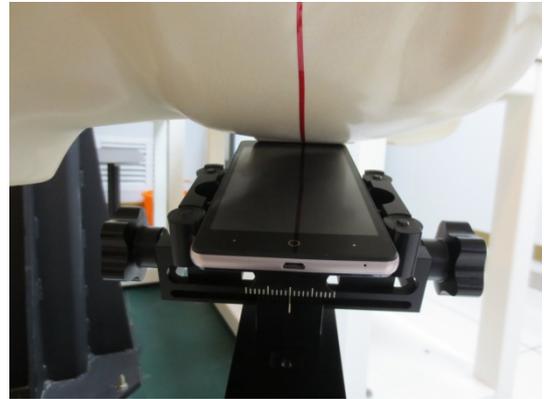

Tilt position, left side

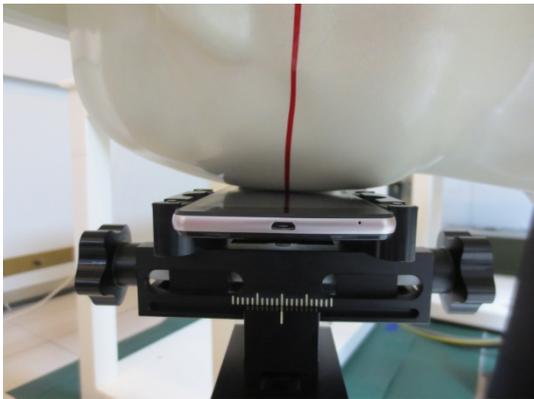

Cheek position, Right side

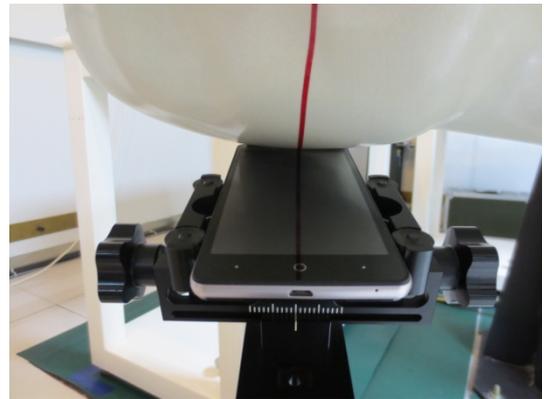


Tilt position, Right side



FLAT position, Towards phantom



FLAT position, Towards ground

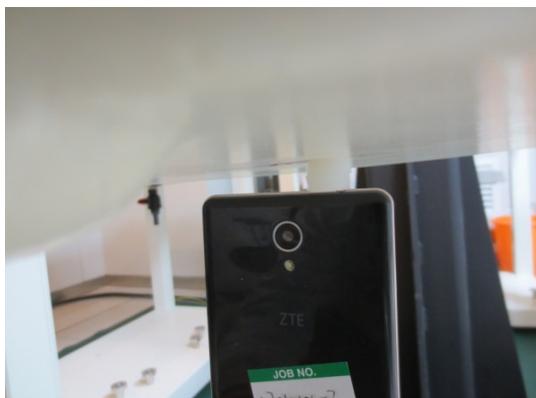


FLAT position, EDGE1



FLAT position, EDGE2



FLAT position, EDGE3

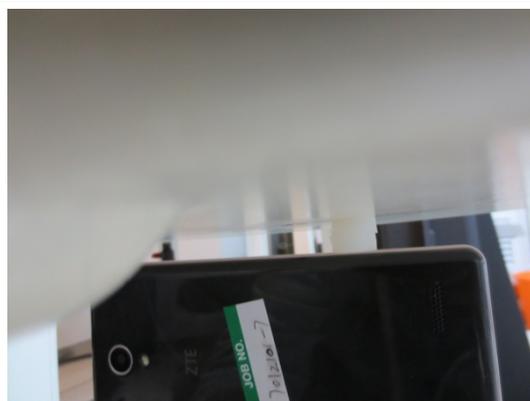

FLAT position, EDGE4



10mm Spacer

---End of Test Report---