



EX3DV4- SN:3898

June 27, 2017

|           |                                                                     |   |      |       |       |      |       |         |
|-----------|---------------------------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10508-AAB | LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.32 | 66.43 | 15.89 | 2.23 | 80.0  | ± 9.6 % |
|           |                                                                     | Y | 3.37 | 66.80 | 16.20 |      | 80.0  |         |
|           |                                                                     | Z | 3.21 | 66.16 | 15.86 |      | 80.0  |         |
| 10509-AAB | LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)   | X | 3.55 | 68.19 | 16.49 | 2.23 | 80.0  | ± 9.6 % |
|           |                                                                     | Y | 3.64 | 68.78 | 16.90 |      | 80.0  |         |
|           |                                                                     | Z | 3.42 | 67.89 | 16.49 |      | 80.0  |         |
| 10510-AAB | LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.74 | 66.59 | 16.18 | 2.23 | 80.0  | ± 9.6 % |
|           |                                                                     | Y | 3.77 | 66.88 | 16.45 |      | 80.0  |         |
|           |                                                                     | Z | 3.63 | 66.30 | 16.15 |      | 80.0  |         |
| 10511-AAB | LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.82 | 66.51 | 16.18 | 2.23 | 80.0  | ± 9.6 % |
|           |                                                                     | Y | 3.85 | 66.78 | 16.44 |      | 80.0  |         |
|           |                                                                     | Z | 3.71 | 66.23 | 16.15 |      | 80.0  |         |
| 10512-AAB | LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)   | X | 3.53 | 68.87 | 16.64 | 2.23 | 80.0  | ± 9.6 % |
|           |                                                                     | Y | 3.65 | 69.60 | 17.11 |      | 80.0  |         |
|           |                                                                     | Z | 3.39 | 68.55 | 16.65 |      | 80.0  |         |
| 10513-AAB | LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.62 | 66.62 | 16.20 | 2.23 | 80.0  | ± 9.6 % |
|           |                                                                     | Y | 3.66 | 66.94 | 16.48 |      | 80.0  |         |
|           |                                                                     | Z | 3.51 | 66.32 | 16.17 |      | 80.0  |         |
| 10514-AAB | LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.68 | 66.43 | 16.16 | 2.23 | 80.0  | ± 9.6 % |
|           |                                                                     | Y | 3.72 | 66.71 | 16.42 |      | 80.0  |         |
|           |                                                                     | Z | 3.58 | 66.13 | 16.13 |      | 80.0  |         |
| 10515-AAB | IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)           | X | 0.99 | 63.31 | 14.64 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                     | Y | 1.01 | 63.68 | 14.99 |      | 150.0 |         |
|           |                                                                     | Z | 0.99 | 63.31 | 14.65 |      | 150.0 |         |
| 10516-AAB | IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 99pc duty cycle)         | X | 0.57 | 68.71 | 16.68 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                     | Y | 0.65 | 71.13 | 18.13 |      | 150.0 |         |
|           |                                                                     | Z | 0.57 | 68.55 | 16.63 |      | 150.0 |         |
| 10517-AAB | IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 99pc duty cycle)          | X | 0.82 | 64.86 | 15.16 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                     | Y | 0.85 | 65.57 | 15.72 |      | 150.0 |         |
|           |                                                                     | Z | 0.83 | 64.83 | 15.16 |      | 150.0 |         |
| 10518-AAB | IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle)           | X | 4.32 | 66.96 | 16.17 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                     | Y | 4.35 | 67.04 | 16.27 |      | 150.0 |         |
|           |                                                                     | Z | 4.31 | 66.97 | 16.19 |      | 150.0 |         |
| 10519-AAB | IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 99pc duty cycle)          | X | 4.46 | 67.11 | 16.26 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                     | Y | 4.49 | 67.19 | 16.35 |      | 150.0 |         |
|           |                                                                     | Z | 4.45 | 67.12 | 16.27 |      | 150.0 |         |
| 10520-AAB | IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 99pc duty cycle)          | X | 4.32 | 67.04 | 16.17 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                     | Y | 4.35 | 67.12 | 16.27 |      | 150.0 |         |
|           |                                                                     | Z | 4.31 | 67.04 | 16.19 |      | 150.0 |         |
| 10521-AAB | IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 99pc duty cycle)          | X | 4.25 | 66.99 | 16.15 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                     | Y | 4.28 | 67.08 | 16.25 |      | 150.0 |         |
|           |                                                                     | Z | 4.24 | 66.99 | 16.16 |      | 150.0 |         |
| 10522-AAB | IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 99pc duty cycle)          | X | 4.29 | 67.08 | 16.22 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                     | Y | 4.32 | 67.17 | 16.32 |      | 150.0 |         |
|           |                                                                     | Z | 4.27 | 67.07 | 16.22 |      | 150.0 |         |

Certificate No: EX3-3898\_Jun17

Page 30 of 38



EX3DV4- SN:3898

June 27, 2017

|           |                                                            |   |      |       |       |      |       |         |
|-----------|------------------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10523-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 99pc duty cycle) | X | 4.24 | 67.16 | 16.19 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.27 | 67.25 | 16.30 |      | 150.0 |         |
|           |                                                            | Z | 4.23 | 67.18 | 16.21 |      | 150.0 |         |
| 10524-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 99pc duty cycle) | X | 4.25 | 67.08 | 16.24 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.28 | 67.17 | 16.34 |      | 150.0 |         |
|           |                                                            | Z | 4.24 | 67.08 | 16.25 |      | 150.0 |         |
| 10525-AAA | IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)          | X | 4.30 | 66.23 | 15.88 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.32 | 66.32 | 15.98 |      | 150.0 |         |
|           |                                                            | Z | 4.29 | 66.24 | 15.90 |      | 150.0 |         |
| 10526-AAA | IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle)          | X | 4.40 | 66.47 | 15.98 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.43 | 66.56 | 16.08 |      | 150.0 |         |
|           |                                                            | Z | 4.39 | 66.47 | 15.99 |      | 150.0 |         |
| 10527-AAA | IEEE 802.11ac WiFi (20MHz, MCS2, 99pc duty cycle)          | X | 4.34 | 66.45 | 15.93 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.37 | 66.54 | 16.03 |      | 150.0 |         |
|           |                                                            | Z | 4.33 | 66.45 | 15.94 |      | 150.0 |         |
| 10528-AAA | IEEE 802.11ac WiFi (20MHz, MCS3, 99pc duty cycle)          | X | 4.35 | 66.46 | 15.96 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.38 | 66.56 | 16.06 |      | 150.0 |         |
|           |                                                            | Z | 4.34 | 66.46 | 15.97 |      | 150.0 |         |
| 10529-AAA | IEEE 802.11ac WiFi (20MHz, MCS4, 99pc duty cycle)          | X | 4.35 | 66.46 | 15.96 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.38 | 66.56 | 16.06 |      | 150.0 |         |
|           |                                                            | Z | 4.34 | 66.46 | 15.97 |      | 150.0 |         |
| 10531-AAA | IEEE 802.11ac WiFi (20MHz, MCS6, 99pc duty cycle)          | X | 4.31 | 66.46 | 15.92 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.34 | 66.56 | 16.03 |      | 150.0 |         |
|           |                                                            | Z | 4.30 | 66.45 | 15.93 |      | 150.0 |         |
| 10532-AAA | IEEE 802.11ac WiFi (20MHz, MCS7, 99pc duty cycle)          | X | 4.20 | 66.33 | 15.86 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.23 | 66.43 | 15.96 |      | 150.0 |         |
|           |                                                            | Z | 4.19 | 66.33 | 15.87 |      | 150.0 |         |
| 10533-AAA | IEEE 802.11ac WiFi (20MHz, MCS8, 99pc duty cycle)          | X | 4.35 | 66.55 | 15.96 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.39 | 66.64 | 16.06 |      | 150.0 |         |
|           |                                                            | Z | 4.34 | 66.55 | 15.98 |      | 150.0 |         |
| 10534-AAA | IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)          | X | 4.92 | 66.42 | 16.02 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.95 | 66.49 | 16.11 |      | 150.0 |         |
|           |                                                            | Z | 4.91 | 66.42 | 16.04 |      | 150.0 |         |
| 10535-AAA | IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)          | X | 4.95 | 66.52 | 16.07 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.98 | 66.59 | 16.16 |      | 150.0 |         |
|           |                                                            | Z | 4.94 | 66.51 | 16.09 |      | 150.0 |         |
| 10536-AAA | IEEE 802.11ac WiFi (40MHz, MCS2, 99pc duty cycle)          | X | 4.85 | 66.53 | 16.05 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.87 | 66.61 | 16.14 |      | 150.0 |         |
|           |                                                            | Z | 4.84 | 66.52 | 16.07 |      | 150.0 |         |
| 10537-AAA | IEEE 802.11ac WiFi (40MHz, MCS3, 99pc duty cycle)          | X | 4.92 | 66.56 | 16.07 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.95 | 66.63 | 16.16 |      | 150.0 |         |
|           |                                                            | Z | 4.92 | 66.56 | 16.10 |      | 150.0 |         |
| 10538-AAA | IEEE 802.11ac WiFi (40MHz, MCS4, 99pc duty cycle)          | X | 4.97 | 66.48 | 16.07 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 5.00 | 66.56 | 16.15 |      | 150.0 |         |
|           |                                                            | Z | 4.96 | 66.47 | 16.09 |      | 150.0 |         |
| 10540-AAA | IEEE 802.11ac WiFi (40MHz, MCS6, 99pc duty cycle)          | X | 4.90 | 66.44 | 16.07 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                            | Y | 4.93 | 66.52 | 16.16 |      | 150.0 |         |
|           |                                                            | Z | 4.90 | 66.43 | 16.09 |      | 150.0 |         |

Certificate No: EX3-3898\_Jun17

Page 31 of 38



EX3DV4- SN:3898

June 27, 2017

|           |                                                     |   |      |       |       |      |       |         |
|-----------|-----------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10541-AAA | IEEE 802.11ac WiFi (40MHz, MCS7, 99pc duty cycle)   | X | 4.90 | 66.40 | 16.03 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 4.92 | 66.46 | 16.11 |      | 150.0 |         |
|           |                                                     | Z | 4.89 | 66.39 | 16.04 |      | 150.0 |         |
| 10542-AAA | IEEE 802.11ac WiFi (40MHz, MCS8, 99pc duty cycle)   | X | 5.05 | 66.48 | 16.09 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.07 | 66.55 | 16.17 |      | 150.0 |         |
|           |                                                     | Z | 5.04 | 66.48 | 16.10 |      | 150.0 |         |
| 10543-AAA | IEEE 802.11ac WiFi (40MHz, MCS9, 99pc duty cycle)   | X | 5.12 | 66.59 | 16.17 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.15 | 66.65 | 16.25 |      | 150.0 |         |
|           |                                                     | Z | 5.12 | 66.59 | 16.19 |      | 150.0 |         |
| 10544-AAA | IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)   | X | 5.27 | 66.48 | 16.01 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.30 | 66.55 | 16.09 |      | 150.0 |         |
|           |                                                     | Z | 5.27 | 66.47 | 16.03 |      | 150.0 |         |
| 10545-AAA | IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle)   | X | 5.43 | 66.89 | 16.18 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.46 | 66.97 | 16.26 |      | 150.0 |         |
|           |                                                     | Z | 5.43 | 66.89 | 16.20 |      | 150.0 |         |
| 10546-AAA | IEEE 802.11ac WiFi (80MHz, MCS2, 99pc duty cycle)   | X | 5.30 | 66.59 | 16.04 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.33 | 66.66 | 16.12 |      | 150.0 |         |
|           |                                                     | Z | 5.30 | 66.57 | 16.05 |      | 150.0 |         |
| 10547-AAA | IEEE 802.11ac WiFi (80MHz, MCS3, 99pc duty cycle)   | X | 5.39 | 66.74 | 16.11 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.41 | 66.81 | 16.19 |      | 150.0 |         |
|           |                                                     | Z | 5.39 | 66.75 | 16.14 |      | 150.0 |         |
| 10548-AAA | IEEE 802.11ac WiFi (80MHz, MCS4, 99pc duty cycle)   | X | 5.49 | 67.22 | 16.33 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.52 | 67.32 | 16.42 |      | 150.0 |         |
|           |                                                     | Z | 5.48 | 67.21 | 16.34 |      | 150.0 |         |
| 10550-AAA | IEEE 802.11ac WiFi (80MHz, MCS6, 99pc duty cycle)   | X | 5.37 | 66.82 | 16.16 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.39 | 66.89 | 16.25 |      | 150.0 |         |
|           |                                                     | Z | 5.37 | 66.84 | 16.20 |      | 150.0 |         |
| 10551-AAA | IEEE 802.11ac WiFi (80MHz, MCS7, 99pc duty cycle)   | X | 5.29 | 66.55 | 15.99 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.31 | 66.62 | 16.07 |      | 150.0 |         |
|           |                                                     | Z | 5.28 | 66.52 | 16.01 |      | 150.0 |         |
| 10552-AAA | IEEE 802.11ac WiFi (80MHz, MCS8, 99pc duty cycle)   | X | 5.28 | 66.62 | 16.03 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.31 | 66.69 | 16.11 |      | 150.0 |         |
|           |                                                     | Z | 5.28 | 66.61 | 16.05 |      | 150.0 |         |
| 10553-AAA | IEEE 802.11ac WiFi (80MHz, MCS9, 99pc duty cycle)   | X | 5.33 | 66.55 | 16.02 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.35 | 66.61 | 16.10 |      | 150.0 |         |
|           |                                                     | Z | 5.32 | 66.53 | 16.04 |      | 150.0 |         |
| 10554-AAA | IEEE 1602.11ac WiFi (160MHz, MCS0, 99pc duty cycle) | X | 5.70 | 66.81 | 16.09 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.73 | 66.87 | 16.16 |      | 150.0 |         |
|           |                                                     | Z | 5.70 | 66.79 | 16.10 |      | 150.0 |         |
| 10555-AAA | IEEE 1602.11ac WiFi (160MHz, MCS1, 99pc duty cycle) | X | 5.78 | 66.99 | 16.17 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.80 | 67.06 | 16.24 |      | 150.0 |         |
|           |                                                     | Z | 5.78 | 66.97 | 16.18 |      | 150.0 |         |
| 10556-AAA | IEEE 1602.11ac WiFi (160MHz, MCS2, 99pc duty cycle) | X | 5.82 | 67.12 | 16.22 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.85 | 67.19 | 16.30 |      | 150.0 |         |
|           |                                                     | Z | 5.83 | 67.12 | 16.24 |      | 150.0 |         |
| 10557-AAA | IEEE 1602.11ac WiFi (160MHz, MCS3, 99pc duty cycle) | X | 5.78 | 67.00 | 16.18 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                     | Y | 5.80 | 67.06 | 16.25 |      | 150.0 |         |
|           |                                                     | Z | 5.78 | 66.98 | 16.19 |      | 150.0 |         |

Certificate No: EX3-3898\_Jun17

Page 32 of 38



EX3DV4- SN:3898

June 27, 2017

|           |                                                                 |   |      |       |       |      |       |         |
|-----------|-----------------------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10558-AAA | IEEE 1602.11ac WiFi (160MHz, MCS4, 99pc duty cycle)             | X | 5.77 | 67.00 | 16.19 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 5.80 | 67.07 | 16.27 |      | 150.0 |         |
|           |                                                                 | Z | 5.76 | 66.96 | 16.20 |      | 150.0 |         |
| 10560-AAA | IEEE 1602.11ac WiFi (160MHz, MCS6, 99pc duty cycle)             | X | 5.80 | 66.97 | 16.21 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 5.83 | 67.03 | 16.29 |      | 150.0 |         |
|           |                                                                 | Z | 5.80 | 66.94 | 16.23 |      | 150.0 |         |
| 10561-AAA | IEEE 1602.11ac WiFi (160MHz, MCS7, 99pc duty cycle)             | X | 5.73 | 66.94 | 16.23 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 5.76 | 67.01 | 16.31 |      | 150.0 |         |
|           |                                                                 | Z | 5.73 | 66.92 | 16.25 |      | 150.0 |         |
| 10562-AAA | IEEE 1602.11ac WiFi (160MHz, MCS8, 99pc duty cycle)             | X | 5.77 | 67.07 | 16.30 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 5.80 | 67.15 | 16.38 |      | 150.0 |         |
|           |                                                                 | Z | 5.77 | 67.04 | 16.31 |      | 150.0 |         |
| 10563-AAA | IEEE 1602.11ac WiFi (160MHz, MCS9, 99pc duty cycle)             | X | 5.88 | 67.08 | 16.27 | 0.00 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 5.91 | 67.16 | 16.35 |      | 150.0 |         |
|           |                                                                 | Z | 5.88 | 67.06 | 16.28 |      | 150.0 |         |
| 10564-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle)  | X | 4.62 | 66.91 | 16.26 | 0.46 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 4.65 | 67.00 | 16.37 |      | 150.0 |         |
|           |                                                                 | Z | 4.62 | 66.92 | 16.27 |      | 150.0 |         |
| 10565-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 99pc duty cycle) | X | 4.82 | 67.35 | 16.60 | 0.46 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 4.84 | 67.41 | 16.69 |      | 150.0 |         |
|           |                                                                 | Z | 4.81 | 67.36 | 16.62 |      | 150.0 |         |
| 10566-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 99pc duty cycle) | X | 4.65 | 67.13 | 16.38 | 0.46 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 4.68 | 67.22 | 16.48 |      | 150.0 |         |
|           |                                                                 | Z | 4.64 | 67.13 | 16.40 |      | 150.0 |         |
| 10567-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 99pc duty cycle) | X | 4.70 | 67.59 | 16.80 | 0.46 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 4.72 | 67.63 | 16.88 |      | 150.0 |         |
|           |                                                                 | Z | 4.69 | 67.60 | 16.83 |      | 150.0 |         |
| 10568-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 99pc duty cycle) | X | 4.52 | 66.74 | 16.04 | 0.46 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 4.56 | 66.86 | 16.17 |      | 150.0 |         |
|           |                                                                 | Z | 4.51 | 66.72 | 16.04 |      | 150.0 |         |
| 10569-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 99pc duty cycle) | X | 4.69 | 67.86 | 16.96 | 0.46 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 4.72 | 67.90 | 17.03 |      | 150.0 |         |
|           |                                                                 | Z | 4.69 | 67.89 | 17.00 |      | 150.0 |         |
| 10570-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 99pc duty cycle) | X | 4.68 | 67.60 | 16.83 | 0.46 | 150.0 | ± 9.6 % |
|           |                                                                 | Y | 4.71 | 67.65 | 16.91 |      | 150.0 |         |
|           |                                                                 | Z | 4.67 | 67.61 | 16.85 |      | 150.0 |         |
| 10571-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)       | X | 1.14 | 63.82 | 14.89 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 1.15 | 64.13 | 15.24 |      | 130.0 |         |
|           |                                                                 | Z | 1.12 | 63.61 | 14.84 |      | 130.0 |         |
| 10572-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)       | X | 1.14 | 64.32 | 15.21 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 1.16 | 64.65 | 15.58 |      | 130.0 |         |
|           |                                                                 | Z | 1.13 | 64.09 | 15.17 |      | 130.0 |         |
| 10573-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle)     | X | 1.07 | 74.72 | 18.97 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 1.28 | 78.28 | 20.78 |      | 130.0 |         |
|           |                                                                 | Z | 0.96 | 73.37 | 18.65 |      | 130.0 |         |
| 10574-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 90pc duty cycle)      | X | 1.18 | 68.96 | 17.73 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 1.21 | 69.63 | 18.27 |      | 130.0 |         |
|           |                                                                 | Z | 1.15 | 68.56 | 17.65 |      | 130.0 |         |

Certificate No: EX3-3898\_Jun17

Page 33 of 38



EX3DV4- SN:3898

June 27, 2017

|           |                                                                 |   |      |       |       |      |       |         |
|-----------|-----------------------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10575-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)  | X | 4.39 | 66.58 | 16.17 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.42 | 66.67 | 16.29 |      | 130.0 |         |
|           |                                                                 | Z | 4.38 | 66.59 | 16.19 |      | 130.0 |         |
| 10576-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)  | X | 4.42 | 66.82 | 16.28 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.45 | 66.90 | 16.39 |      | 130.0 |         |
|           |                                                                 | Z | 4.41 | 66.83 | 16.31 |      | 130.0 |         |
| 10577-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 90pc duty cycle) | X | 4.57 | 67.04 | 16.43 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.60 | 67.12 | 16.53 |      | 130.0 |         |
|           |                                                                 | Z | 4.56 | 67.05 | 16.45 |      | 130.0 |         |
| 10578-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 90pc duty cycle) | X | 4.49 | 67.21 | 16.56 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.51 | 67.28 | 16.65 |      | 130.0 |         |
|           |                                                                 | Z | 4.48 | 67.22 | 16.59 |      | 130.0 |         |
| 10579-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 90pc duty cycle) | X | 4.22 | 66.25 | 15.71 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.25 | 66.38 | 15.85 |      | 130.0 |         |
|           |                                                                 | Z | 4.21 | 66.24 | 15.71 |      | 130.0 |         |
| 10580-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 90pc duty cycle) | X | 4.24 | 66.27 | 15.70 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.28 | 66.41 | 15.85 |      | 130.0 |         |
|           |                                                                 | Z | 4.23 | 66.24 | 15.70 |      | 130.0 |         |
| 10581-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 90pc duty cycle) | X | 4.40 | 67.30 | 16.54 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.43 | 67.38 | 16.64 |      | 130.0 |         |
|           |                                                                 | Z | 4.39 | 67.32 | 16.57 |      | 130.0 |         |
| 10582-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 90pc duty cycle) | X | 4.14 | 65.99 | 15.46 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.18 | 66.13 | 15.62 |      | 130.0 |         |
|           |                                                                 | Z | 4.12 | 65.96 | 15.46 |      | 130.0 |         |
| 10583-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)       | X | 4.39 | 66.58 | 16.17 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.42 | 66.67 | 16.29 |      | 130.0 |         |
|           |                                                                 | Z | 4.38 | 66.59 | 16.19 |      | 130.0 |         |
| 10584-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)       | X | 4.42 | 66.82 | 16.28 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.45 | 66.90 | 16.39 |      | 130.0 |         |
|           |                                                                 | Z | 4.41 | 66.83 | 16.31 |      | 130.0 |         |
| 10585-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 90pc duty cycle)      | X | 4.57 | 67.04 | 16.43 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.60 | 67.12 | 16.53 |      | 130.0 |         |
|           |                                                                 | Z | 4.56 | 67.05 | 16.45 |      | 130.0 |         |
| 10586-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 90pc duty cycle)      | X | 4.49 | 67.21 | 16.56 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.51 | 67.28 | 16.65 |      | 130.0 |         |
|           |                                                                 | Z | 4.48 | 67.22 | 16.59 |      | 130.0 |         |
| 10587-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 90pc duty cycle)      | X | 4.22 | 66.25 | 15.71 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.25 | 66.38 | 15.85 |      | 130.0 |         |
|           |                                                                 | Z | 4.21 | 66.24 | 15.71 |      | 130.0 |         |
| 10588-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 90pc duty cycle)      | X | 4.24 | 66.27 | 15.70 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.28 | 66.41 | 15.85 |      | 130.0 |         |
|           |                                                                 | Z | 4.23 | 66.24 | 15.70 |      | 130.0 |         |
| 10589-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 90pc duty cycle)      | X | 4.40 | 67.30 | 16.54 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.43 | 67.38 | 16.64 |      | 130.0 |         |
|           |                                                                 | Z | 4.39 | 67.32 | 16.57 |      | 130.0 |         |
| 10590-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 90pc duty cycle)      | X | 4.14 | 65.99 | 15.46 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                                 | Y | 4.18 | 66.13 | 15.62 |      | 130.0 |         |
|           |                                                                 | Z | 4.12 | 65.96 | 15.46 |      | 130.0 |         |

Certificate No: EX3-3898\_Jun17

Page 34 of 38



EX3DV4- SN:3898

June 27, 2017

|           |                                                       |   |      |       |       |      |       |         |
|-----------|-------------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10591-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle) | X | 4.55 | 66.71 | 16.33 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 4.58 | 66.79 | 16.43 |      | 130.0 |         |
|           |                                                       | Z | 4.54 | 66.72 | 16.35 |      | 130.0 |         |
| 10592-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle) | X | 4.66 | 66.97 | 16.44 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 4.68 | 67.05 | 16.55 |      | 130.0 |         |
|           |                                                       | Z | 4.65 | 66.98 | 16.47 |      | 130.0 |         |
| 10593-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS2, 90pc duty cycle) | X | 4.57 | 66.83 | 16.29 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 4.60 | 66.92 | 16.40 |      | 130.0 |         |
|           |                                                       | Z | 4.56 | 66.84 | 16.31 |      | 130.0 |         |
| 10594-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS3, 90pc duty cycle) | X | 4.63 | 67.03 | 16.47 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 4.66 | 67.11 | 16.57 |      | 130.0 |         |
|           |                                                       | Z | 4.62 | 67.04 | 16.49 |      | 130.0 |         |
| 10595-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS4, 90pc duty cycle) | X | 4.59 | 67.00 | 16.37 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 4.62 | 67.08 | 16.48 |      | 130.0 |         |
|           |                                                       | Z | 4.58 | 67.00 | 16.39 |      | 130.0 |         |
| 10596-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS5, 90pc duty cycle) | X | 4.52 | 66.92 | 16.34 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 4.55 | 67.02 | 16.46 |      | 130.0 |         |
|           |                                                       | Z | 4.51 | 66.92 | 16.36 |      | 130.0 |         |
| 10597-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS6, 90pc duty cycle) | X | 4.47 | 66.79 | 16.19 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 4.50 | 66.89 | 16.31 |      | 130.0 |         |
|           |                                                       | Z | 4.46 | 66.78 | 16.20 |      | 130.0 |         |
| 10598-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS7, 90pc duty cycle) | X | 4.48 | 67.08 | 16.50 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 4.51 | 67.15 | 16.60 |      | 130.0 |         |
|           |                                                       | Z | 4.47 | 67.09 | 16.52 |      | 130.0 |         |
| 10599-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle) | X | 5.24 | 67.14 | 16.59 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 5.26 | 67.22 | 16.69 |      | 130.0 |         |
|           |                                                       | Z | 5.24 | 67.17 | 16.63 |      | 130.0 |         |
| 10600-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle) | X | 5.31 | 67.40 | 16.69 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 5.34 | 67.51 | 16.81 |      | 130.0 |         |
|           |                                                       | Z | 5.31 | 67.43 | 16.73 |      | 130.0 |         |
| 10601-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS2, 90pc duty cycle) | X | 5.24 | 67.31 | 16.67 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 5.27 | 67.39 | 16.76 |      | 130.0 |         |
|           |                                                       | Z | 5.25 | 67.36 | 16.72 |      | 130.0 |         |
| 10602-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS3, 90pc duty cycle) | X | 5.30 | 67.20 | 16.52 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 5.33 | 67.30 | 16.63 |      | 130.0 |         |
|           |                                                       | Z | 5.29 | 67.21 | 16.55 |      | 130.0 |         |
| 10603-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS4, 90pc duty cycle) | X | 5.36 | 67.49 | 16.82 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 5.39 | 67.59 | 16.92 |      | 130.0 |         |
|           |                                                       | Z | 5.35 | 67.49 | 16.85 |      | 130.0 |         |
| 10604-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS5, 90pc duty cycle) | X | 5.23 | 67.04 | 16.56 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 5.26 | 67.13 | 16.66 |      | 130.0 |         |
|           |                                                       | Z | 5.22 | 67.02 | 16.58 |      | 130.0 |         |
| 10605-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS6, 90pc duty cycle) | X | 5.29 | 67.25 | 16.66 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 5.32 | 67.35 | 16.78 |      | 130.0 |         |
|           |                                                       | Z | 5.29 | 67.26 | 16.69 |      | 130.0 |         |
| 10606-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS7, 90pc duty cycle) | X | 5.11 | 66.78 | 16.27 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                       | Y | 5.14 | 66.88 | 16.39 |      | 130.0 |         |
|           |                                                       | Z | 5.11 | 66.80 | 16.31 |      | 130.0 |         |

Certificate No: EX3-3898\_Jun17

Page 35 of 38



EX3DV4- SN:3898

June 27, 2017

|           |                                                   |   |      |       |       |      |       |         |
|-----------|---------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10607-AAA | IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle) | X | 4.40 | 66.05 | 15.97 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.43 | 66.14 | 16.08 |      | 130.0 |         |
|           |                                                   | Z | 4.39 | 66.06 | 16.00 |      | 130.0 |         |
| 10608-AAA | IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle) | X | 4.52 | 66.33 | 16.10 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.55 | 66.43 | 16.21 |      | 130.0 |         |
|           |                                                   | Z | 4.51 | 66.34 | 16.13 |      | 130.0 |         |
| 10609-AAA | IEEE 802.11ac WiFi (20MHz, MCS2, 90pc duty cycle) | X | 4.41 | 66.15 | 15.91 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.45 | 66.26 | 16.03 |      | 130.0 |         |
|           |                                                   | Z | 4.40 | 66.16 | 15.93 |      | 130.0 |         |
| 10610-AAA | IEEE 802.11ac WiFi (20MHz, MCS3, 90pc duty cycle) | X | 4.47 | 66.34 | 16.10 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.50 | 66.44 | 16.21 |      | 130.0 |         |
|           |                                                   | Z | 4.46 | 66.36 | 16.12 |      | 130.0 |         |
| 10611-AAA | IEEE 802.11ac WiFi (20MHz, MCS4, 90pc duty cycle) | X | 4.38 | 66.11 | 15.92 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.41 | 66.22 | 16.04 |      | 130.0 |         |
|           |                                                   | Z | 4.37 | 66.12 | 15.94 |      | 130.0 |         |
| 10612-AAA | IEEE 802.11ac WiFi (20MHz, MCS5, 90pc duty cycle) | X | 4.35 | 66.19 | 15.93 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.39 | 66.31 | 16.06 |      | 130.0 |         |
|           |                                                   | Z | 4.34 | 66.18 | 15.94 |      | 130.0 |         |
| 10613-AAA | IEEE 802.11ac WiFi (20MHz, MCS6, 90pc duty cycle) | X | 4.35 | 66.00 | 15.77 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.39 | 66.13 | 15.90 |      | 130.0 |         |
|           |                                                   | Z | 4.34 | 66.00 | 15.79 |      | 130.0 |         |
| 10614-AAA | IEEE 802.11ac WiFi (20MHz, MCS7, 90pc duty cycle) | X | 4.34 | 66.30 | 16.07 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.37 | 66.40 | 16.18 |      | 130.0 |         |
|           |                                                   | Z | 4.33 | 66.31 | 16.10 |      | 130.0 |         |
| 10615-AAA | IEEE 802.11ac WiFi (20MHz, MCS8, 90pc duty cycle) | X | 4.36 | 65.90 | 15.65 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 4.40 | 66.04 | 15.79 |      | 130.0 |         |
|           |                                                   | Z | 4.35 | 65.90 | 15.67 |      | 130.0 |         |
| 10616-AAA | IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle) | X | 5.03 | 66.30 | 16.16 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 5.06 | 66.38 | 16.26 |      | 130.0 |         |
|           |                                                   | Z | 5.03 | 66.31 | 16.19 |      | 130.0 |         |
| 10617-AAA | IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle) | X | 5.05 | 66.37 | 16.17 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 5.09 | 66.47 | 16.28 |      | 130.0 |         |
|           |                                                   | Z | 5.05 | 66.38 | 16.20 |      | 130.0 |         |
| 10618-AAA | IEEE 802.11ac WiFi (40MHz, MCS2, 90pc duty cycle) | X | 4.97 | 66.45 | 16.23 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 5.00 | 66.54 | 16.33 |      | 130.0 |         |
|           |                                                   | Z | 4.97 | 66.45 | 16.26 |      | 130.0 |         |
| 10619-AAA | IEEE 802.11ac WiFi (40MHz, MCS3, 90pc duty cycle) | X | 5.00 | 66.32 | 16.09 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 5.04 | 66.42 | 16.20 |      | 130.0 |         |
|           |                                                   | Z | 5.01 | 66.34 | 16.13 |      | 130.0 |         |
| 10620-AAA | IEEE 802.11ac WiFi (40MHz, MCS4, 90pc duty cycle) | X | 5.06 | 66.27 | 16.11 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 5.09 | 66.36 | 16.22 |      | 130.0 |         |
|           |                                                   | Z | 5.05 | 66.27 | 16.14 |      | 130.0 |         |
| 10621-AAA | IEEE 802.11ac WiFi (40MHz, MCS5, 90pc duty cycle) | X | 5.08 | 66.45 | 16.34 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 5.11 | 66.51 | 16.42 |      | 130.0 |         |
|           |                                                   | Z | 5.08 | 66.46 | 16.37 |      | 130.0 |         |
| 10622-AAA | IEEE 802.11ac WiFi (40MHz, MCS6, 90pc duty cycle) | X | 5.07 | 66.51 | 16.37 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                   | Y | 5.09 | 66.59 | 16.45 |      | 130.0 |         |
|           |                                                   | Z | 5.06 | 66.52 | 16.40 |      | 130.0 |         |

Certificate No: EX3-3898\_Jun17

Page 36 of 38



EX3DV4- SN:3898

June 27, 2017

|           |                                                     |   |      |       |       |      |       |         |
|-----------|-----------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10623-AAA | IEEE 802.11ac WiFi (40MHz, MCS7, 90pc duty cycle)   | X | 4.96 | 66.07 | 15.99 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 4.99 | 66.16 | 16.09 |      | 130.0 |         |
|           |                                                     | Z | 4.96 | 66.07 | 16.02 |      | 130.0 |         |
| 10624-AAA | IEEE 802.11ac WiFi (40MHz, MCS8, 90pc duty cycle)   | X | 5.15 | 66.33 | 16.19 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.18 | 66.41 | 16.29 |      | 130.0 |         |
|           |                                                     | Z | 5.15 | 66.34 | 16.22 |      | 130.0 |         |
| 10625-AAA | IEEE 802.11ac WiFi (40MHz, MCS9, 90pc duty cycle)   | X | 5.25 | 66.51 | 16.35 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.27 | 66.57 | 16.43 |      | 130.0 |         |
|           |                                                     | Z | 5.25 | 66.56 | 16.40 |      | 130.0 |         |
| 10626-AAA | IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)   | X | 5.37 | 66.32 | 16.12 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.40 | 66.40 | 16.21 |      | 130.0 |         |
|           |                                                     | Z | 5.37 | 66.32 | 16.15 |      | 130.0 |         |
| 10627-AAA | IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle)   | X | 5.58 | 66.89 | 16.38 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.61 | 66.98 | 16.48 |      | 130.0 |         |
|           |                                                     | Z | 5.58 | 66.90 | 16.42 |      | 130.0 |         |
| 10628-AAA | IEEE 802.11ac WiFi (80MHz, MCS2, 90pc duty cycle)   | X | 5.35 | 66.26 | 15.99 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.38 | 66.35 | 16.09 |      | 130.0 |         |
|           |                                                     | Z | 5.35 | 66.25 | 16.01 |      | 130.0 |         |
| 10629-AAA | IEEE 802.11ac WiFi (80MHz, MCS3, 90pc duty cycle)   | X | 5.47 | 66.50 | 16.11 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.50 | 66.59 | 16.21 |      | 130.0 |         |
|           |                                                     | Z | 5.48 | 66.54 | 16.15 |      | 130.0 |         |
| 10630-AAA | IEEE 802.11ac WiFi (80MHz, MCS4, 90pc duty cycle)   | X | 5.62 | 67.17 | 16.45 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.67 | 67.30 | 16.57 |      | 130.0 |         |
|           |                                                     | Z | 5.62 | 67.15 | 16.47 |      | 130.0 |         |
| 10631-AAA | IEEE 802.11ac WiFi (80MHz, MCS5, 90pc duty cycle)   | X | 5.65 | 67.38 | 16.76 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.68 | 67.44 | 16.84 |      | 130.0 |         |
|           |                                                     | Z | 5.65 | 67.38 | 16.79 |      | 130.0 |         |
| 10632-AAA | IEEE 802.11ac WiFi (80MHz, MCS6, 90pc duty cycle)   | X | 5.61 | 67.17 | 16.67 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.63 | 67.23 | 16.75 |      | 130.0 |         |
|           |                                                     | Z | 5.62 | 67.22 | 16.73 |      | 130.0 |         |
| 10633-AAA | IEEE 802.11ac WiFi (80MHz, MCS7, 90pc duty cycle)   | X | 5.38 | 66.36 | 16.08 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.41 | 66.43 | 16.17 |      | 130.0 |         |
|           |                                                     | Z | 5.37 | 66.34 | 16.10 |      | 130.0 |         |
| 10634-AAA | IEEE 802.11ac WiFi (80MHz, MCS8, 90pc duty cycle)   | X | 5.42 | 66.59 | 16.25 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.45 | 66.66 | 16.34 |      | 130.0 |         |
|           |                                                     | Z | 5.42 | 66.59 | 16.28 |      | 130.0 |         |
| 10635-AAA | IEEE 802.11ac WiFi (80MHz, MCS9, 90pc duty cycle)   | X | 5.25 | 65.74 | 15.52 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.29 | 65.85 | 15.64 |      | 130.0 |         |
|           |                                                     | Z | 5.25 | 65.72 | 15.54 |      | 130.0 |         |
| 10636-AAA | IEEE 1602.11ac WiFi (160MHz, MCS0, 90pc duty cycle) | X | 5.81 | 66.67 | 16.21 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.84 | 66.74 | 16.30 |      | 130.0 |         |
|           |                                                     | Z | 5.82 | 66.67 | 16.24 |      | 130.0 |         |
| 10637-AAA | IEEE 1602.11ac WiFi (160MHz, MCS1, 90pc duty cycle) | X | 5.91 | 66.92 | 16.32 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.94 | 67.00 | 16.42 |      | 130.0 |         |
|           |                                                     | Z | 5.91 | 66.92 | 16.35 |      | 130.0 |         |
| 10638-AAA | IEEE 1602.11ac WiFi (160MHz, MCS2, 90pc duty cycle) | X | 5.95 | 67.05 | 16.36 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                     | Y | 5.98 | 67.13 | 16.46 |      | 130.0 |         |
|           |                                                     | Z | 5.96 | 67.06 | 16.40 |      | 130.0 |         |

Certificate No: EX3-3898\_Jun17

Page 37 of 38



EX3DV4- SN:3898

June 27, 2017

|           |                                                        |   |      |       |       |      |       |         |
|-----------|--------------------------------------------------------|---|------|-------|-------|------|-------|---------|
| 10639-AAA | IEEE 1602.11ac WiFi (160MHz, MCS3, 90pc duty cycle)    | X | 5.90 | 66.89 | 16.33 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                        | Y | 5.93 | 66.97 | 16.42 |      | 130.0 |         |
|           |                                                        | Z | 5.90 | 66.89 | 16.36 |      | 130.0 |         |
| 10640-AAA | IEEE 1602.11ac WiFi (160MHz, MCS4, 90pc duty cycle)    | X | 5.83 | 66.70 | 16.17 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                        | Y | 5.86 | 66.79 | 16.27 |      | 130.0 |         |
|           |                                                        | Z | 5.83 | 66.67 | 16.19 |      | 130.0 |         |
| 10641-AAA | IEEE 1602.11ac WiFi (160MHz, MCS5, 90pc duty cycle)    | X | 5.95 | 66.83 | 16.26 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                        | Y | 5.98 | 66.93 | 16.36 |      | 130.0 |         |
|           |                                                        | Z | 5.95 | 66.84 | 16.29 |      | 130.0 |         |
| 10642-AAA | IEEE 1602.11ac WiFi (160MHz, MCS6, 90pc duty cycle)    | X | 5.98 | 67.06 | 16.55 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                        | Y | 6.00 | 67.13 | 16.63 |      | 130.0 |         |
|           |                                                        | Z | 5.98 | 67.06 | 16.58 |      | 130.0 |         |
| 10643-AAA | IEEE 1602.11ac WiFi (160MHz, MCS7, 90pc duty cycle)    | X | 5.81 | 66.70 | 16.25 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                        | Y | 5.84 | 66.79 | 16.35 |      | 130.0 |         |
|           |                                                        | Z | 5.81 | 66.69 | 16.27 |      | 130.0 |         |
| 10644-AAA | IEEE 1602.11ac WiFi (160MHz, MCS8, 90pc duty cycle)    | X | 5.86 | 66.86 | 16.35 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                        | Y | 5.89 | 66.95 | 16.45 |      | 130.0 |         |
|           |                                                        | Z | 5.86 | 66.84 | 16.37 |      | 130.0 |         |
| 10645-AAA | IEEE 1602.11ac WiFi (160MHz, MCS9, 90pc duty cycle)    | X | 5.99 | 66.94 | 16.36 | 0.46 | 130.0 | ± 9.6 % |
|           |                                                        | Y | 6.02 | 67.02 | 16.45 |      | 130.0 |         |
|           |                                                        | Z | 6.00 | 66.95 | 16.39 |      | 130.0 |         |
| 10646-AAC | LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,7)  | X | 6.69 | 86.81 | 28.67 | 9.30 | 60.0  | ± 9.6 % |
|           |                                                        | Y | 7.72 | 91.33 | 30.89 |      | 60.0  |         |
|           |                                                        | Z | 5.52 | 83.14 | 27.53 |      | 60.0  |         |
| 10647-AAB | LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,7) | X | 5.99 | 84.97 | 28.10 | 9.30 | 60.0  | ± 9.6 % |
|           |                                                        | Y | 6.77 | 88.96 | 30.17 |      | 60.0  |         |
|           |                                                        | Z | 4.99 | 81.44 | 26.98 |      | 60.0  |         |
| 10648-AAA | CDMA2000 (1x Advanced)                                 | X | 0.51 | 61.86 | 8.44  | 0.00 | 150.0 | ± 9.6 % |
|           |                                                        | Y | 0.54 | 62.46 | 8.97  |      | 150.0 |         |
|           |                                                        | Z | 0.50 | 61.70 | 8.25  |      | 150.0 |         |

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



## ANNEX E: Probe Calibration Certificate (SN: 3677)



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ctll@chinattl.com <http://www.chinattl.cn>




中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L0570

Client **TA(shanghai)**
Certificate No: **Z18-60093**

### CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN:3677**

Calibration Procedure(s): **FF-Z11-004-01**  
**Calibration Procedures for Dosimetric E-field Probes**

Calibration date: **May 29, 2018**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #        | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|-------------|------------------------------------------|-----------------------|
| Power Meter NRP2        | 101919      | 27-Jun-17 (CTTL, No.J17X05857)           | Jun-18                |
| Power sensor NRP-Z91    | 101547      | 27-Jun-17 (CTTL, No.J17X05857)           | Jun-18                |
| Power sensor NRP-Z91    | 101548      | 27-Jun-17 (CTTL, No.J17X05857)           | Jun-18                |
| Reference10dBAttenuator | 18N50W-10dB | 09-Feb-18(CTTL, No.J18X01133)            | Feb-20                |
| Reference20dBAttenuator | 18N50W-20dB | 09-Feb-18(CTTL, No.J18X01132)            | Feb-20                |
| Reference Probe EX3DV4  | SN 3846     | 25-Jan-18(SPEAG,No.EX3-3846_Jan18)       | Jan-19                |
| DAE4                    | SN 777      | 15-Dec-17(SPEAG, No.DAE4-777_Dec17)      | Dec -18               |

| Secondary Standards     | ID #       | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|------------------------------------------|-----------------------|
| SignalGeneratorMG3700A  | 6201052605 | 27-Jun-17 (CTTL, No.J17X05858)           | Jun-18                |
| Network Analyzer E5071C | MY46110673 | 14-Jan-18 (CTTL, No.J18X00561)           | Jan -19               |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Yu Zongying | SAR Test Engineer  |  |
| Reviewed by:   | Lin Hao     | SAR Test Engineer  |                                                                                       |
| Approved by:   | Qi Dianyuan | SAR Project Leader |                                                                                       |

Issued: May 31, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z18-60093

Page 1 of 11



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ttl@chinattl.com <http://www.chinattl.cn>

# Glossary:

|                       |                                                                                                                                        |
|-----------------------|----------------------------------------------------------------------------------------------------------------------------------------|
| TSL                   | tissue simulating liquid                                                                                                               |
| NORM <sub>x,y,z</sub> | sensitivity in free space                                                                                                              |
| ConvF                 | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                             |
| DCP                   | diode compression point                                                                                                                |
| CF                    | crest factor (1/duty_cycle) of the RF signal                                                                                           |
| A,B,C,D               | modulation dependent linearization parameters                                                                                          |
| Polarization $\Phi$   | $\Phi$ rotation around probe axis                                                                                                      |
| Polarization $\theta$ | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), $\theta=0$ is normal to probe axis |

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

## Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\theta=0$  ( $f \leq 900\text{MHz}$  in TEM-cell;  $f > 1800\text{MHz}$ : waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM( $f$ )<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A,B,C** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800\text{MHz}$ ) and inside waveguide using analytical field distributions based on power measurements for  $f > 800\text{MHz}$ . The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50\text{MHz}$  to  $\pm 100\text{MHz}$ .
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: [ttl@chinattl.com](mailto:ttl@chinattl.com) [Http://www.chinattl.cn](http://www.chinattl.cn)

# Probe EX3DV4

## SN: 3677

Calibrated: May 29, 2018

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com Http://www.chinattl.cn

## DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3677

### Basic Calibration Parameters

|                                      | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|--------------------------------------|----------|----------|----------|-----------|
| Norm( $\mu V/(V/m)^2$ ) <sup>A</sup> | 0.41     | 0.46     | 0.41     | ±10.0%    |
| DCP(mV) <sup>B</sup>                 | 99.9     | 102.7    | 102.1    |           |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A dB | B dB· $\mu V$ | C   | D dB | VR mV | Unc <sup>E</sup> (k=2) |
|-----|---------------------------|---|------|---------------|-----|------|-------|------------------------|
| 0   | CW                        | X | 0.0  | 0.0           | 1.0 | 0.00 | 152.4 | ±2.4%                  |
|     |                           | Y | 0.0  | 0.0           | 1.0 |      | 161.7 |                        |
|     |                           | Z | 0.0  | 0.0           | 1.0 |      | 152.2 |                        |

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X, Y, Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 5 and Page 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com <http://www.chinattl.cn>

## DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3677

### Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 41.9                               | 0.89                            | 9.40    | 9.40    | 9.40    | 0.40               | 0.80                    | ± 12.1%     |
| 835                  | 41.5                               | 0.90                            | 9.10    | 9.10    | 9.10    | 0.15               | 1.41                    | ± 12.1%     |
| 1750                 | 40.1                               | 1.37                            | 8.19    | 8.19    | 8.19    | 0.21               | 1.15                    | ± 12.1%     |
| 1900                 | 40.0                               | 1.40                            | 7.96    | 7.96    | 7.96    | 0.25               | 1.01                    | ± 12.1%     |
| 2300                 | 39.5                               | 1.67                            | 7.91    | 7.91    | 7.91    | 0.40               | 0.78                    | ± 12.1%     |
| 2450                 | 39.2                               | 1.80                            | 7.57    | 7.57    | 7.57    | 0.53               | 0.76                    | ± 12.1%     |
| 2600                 | 39.0                               | 1.96                            | 7.28    | 7.28    | 7.28    | 0.64               | 0.70                    | ± 12.1%     |
| 5250                 | 35.9                               | 4.71                            | 5.60    | 5.60    | 5.60    | 0.40               | 1.15                    | ± 13.3%     |
| 5600                 | 35.5                               | 5.07                            | 4.87    | 4.87    | 4.87    | 0.45               | 1.05                    | ± 13.3%     |
| 5750                 | 35.4                               | 5.22                            | 4.99    | 4.99    | 4.99    | 0.45               | 1.35                    | ± 13.3%     |

<sup>C</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ttl@chinattl.com <http://www.chinattl.cn>

## DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3677

### Calibration Parameter Determined in Body Tissue Simulating Media

| f [MHz] <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750                  | 55.5                               | 0.96                            | 9.79    | 9.79    | 9.79    | 0.40               | 0.80                    | ±12.1%      |
| 835                  | 55.2                               | 0.97                            | 9.32    | 9.32    | 9.32    | 0.15               | 1.51                    | ±12.1%      |
| 1750                 | 53.4                               | 1.49                            | 7.91    | 7.91    | 7.91    | 0.23               | 1.09                    | ±12.1%      |
| 1900                 | 53.3                               | 1.52                            | 7.70    | 7.70    | 7.70    | 0.20               | 1.18                    | ±12.1%      |
| 2300                 | 52.9                               | 1.81                            | 7.65    | 7.65    | 7.65    | 0.53               | 0.82                    | ±12.1%      |
| 2450                 | 52.7                               | 1.95                            | 7.53    | 7.53    | 7.53    | 0.37               | 1.10                    | ±12.1%      |
| 2600                 | 52.5                               | 2.16                            | 7.16    | 7.16    | 7.16    | 0.55               | 0.80                    | ±12.1%      |
| 5250                 | 48.9                               | 5.36                            | 5.04    | 5.04    | 5.04    | 0.50               | 1.55                    | ±13.3%      |
| 5600                 | 48.5                               | 5.77                            | 4.27    | 4.27    | 4.27    | 0.51               | 1.66                    | ±13.3%      |
| 5750                 | 48.3                               | 5.94                            | 4.43    | 4.43    | 4.43    | 0.50               | 1.81                    | ±13.3%      |

<sup>C</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


<sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
 E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

## Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

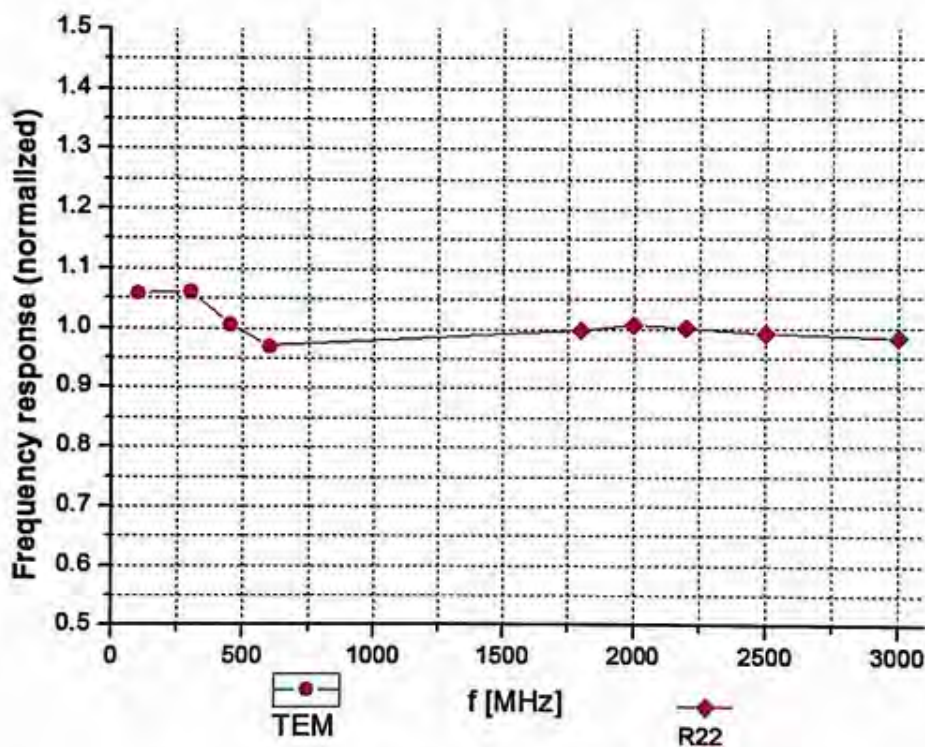

Uncertainty of Frequency Response of E-field:  $\pm 7.4\%$  (k=2)






Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ttl@chinattl.com <http://www.chinattl.cn>

## Receiving Pattern ( $\Phi$ ), $\theta=0^\circ$

f=600 MHz, TEM


f=1800 MHz, R22

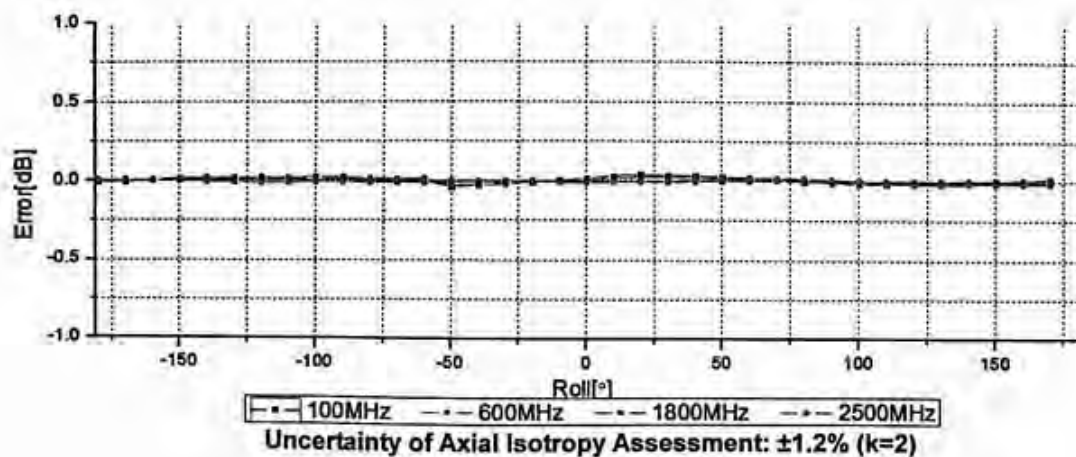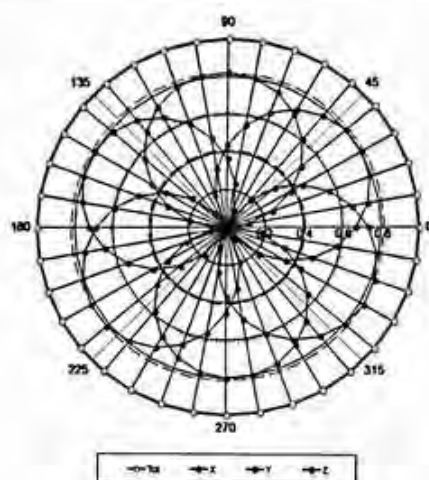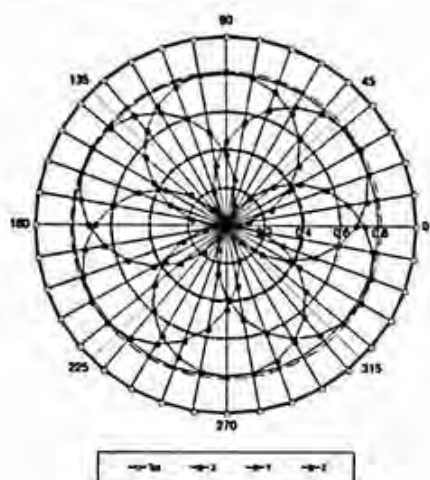



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com <http://www.chinattl.cn>

## Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f = 900 \text{ MHz}$ )

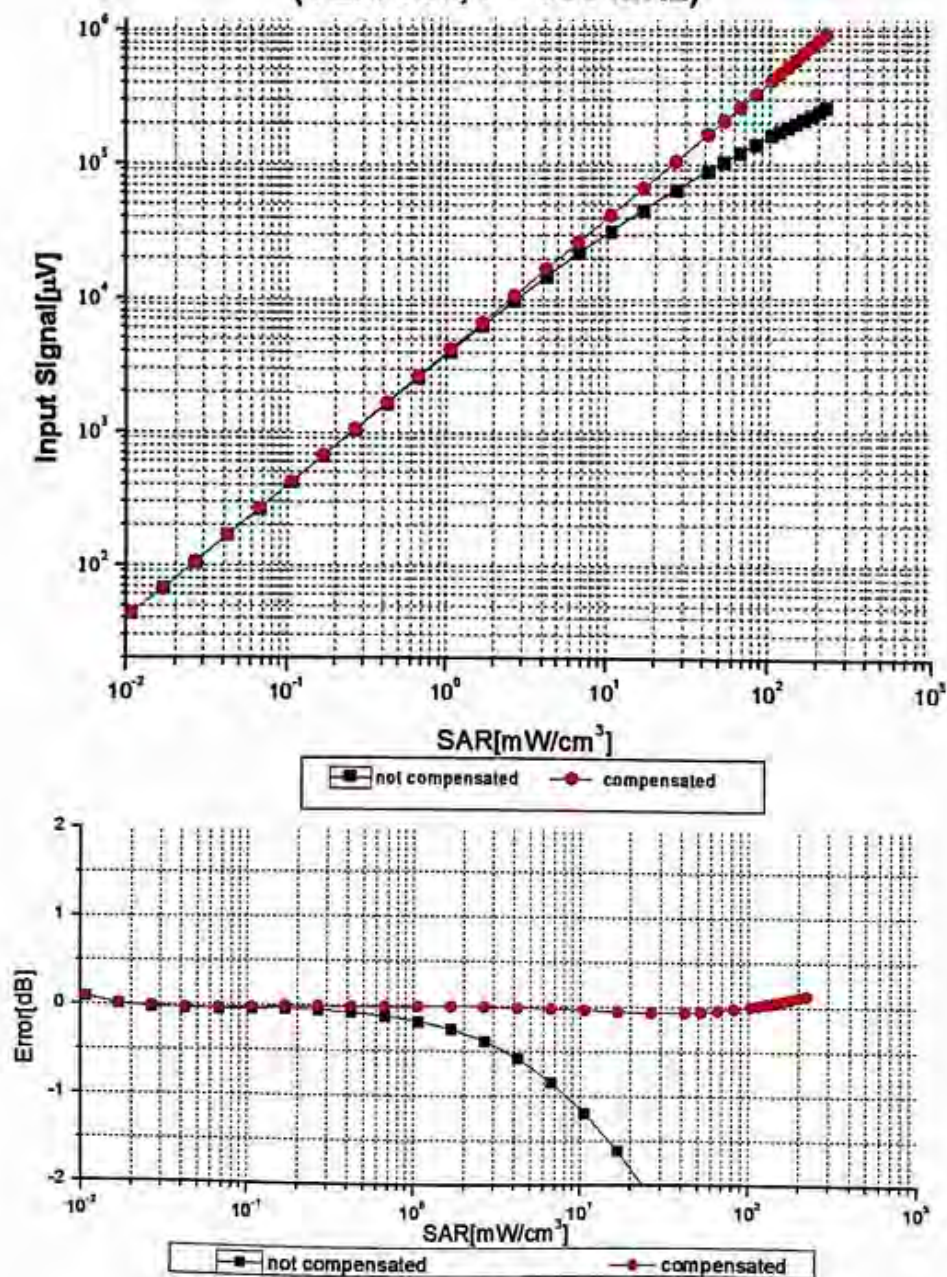

Uncertainty of Linearity Assessment:  $\pm 0.9\%$  ( $k=2$ )

Certificate No: Z18-60093

Page 9 of 11





Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cntl@chinatl.com <http://www.chinatl.cn>


## Conversion Factor Assessment

f=750 MHz, WGLS R9(H\_convF)

f=1750 MHz, WGLS R22(H\_convF)

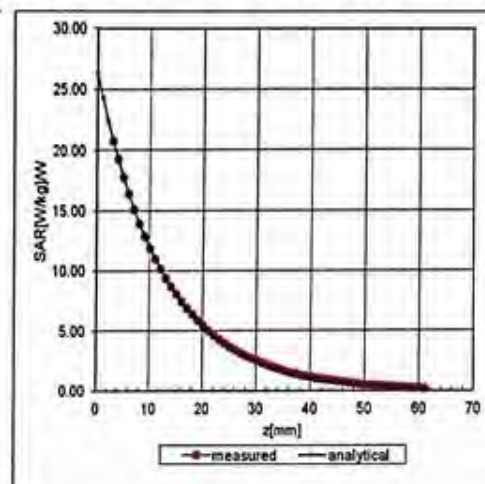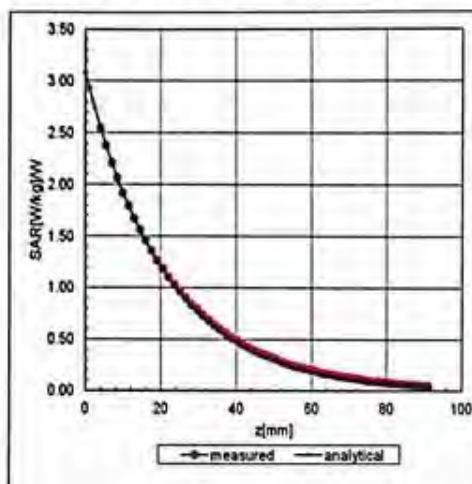

## Deviation from Isotropy in Liquid

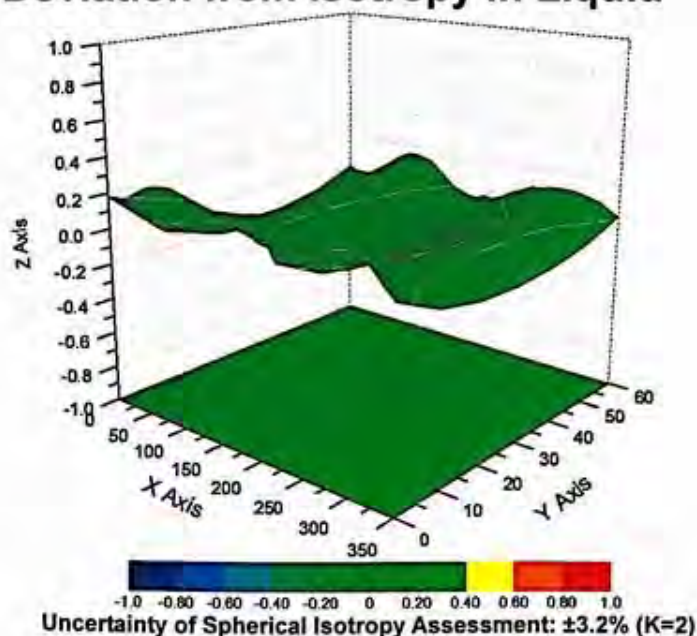

Certificate No: Z18-60093

Page 10 of 11



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
 E-mail: [ctl@chinattl.com](mailto:ctl@chinattl.com) [Http://www.chinattl.cn](http://www.chinattl.cn)

## DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3677

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | 118.3      |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disable    |
| Probe Overall Length                          | 337mm      |
| Probe Body Diameter                           | 10mm       |
| Tip Length                                    | 9mm        |
| Tip Diameter                                  | 2.5mm      |
| Probe Tip to Sensor X Calibration Point       | 1mm        |
| Probe Tip to Sensor Y Calibration Point       | 1mm        |
| Probe Tip to Sensor Z Calibration Point       | 1mm        |
| Recommended Measurement Distance from Surface | 1.4mm      |



## ANNEX F: D835V2 Dipole Calibration Certificate



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY



中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L0570

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

Client

TA(Shanghai)

Certificate No: Z17-97114

## CALIBRATION CERTIFICATE

Object

D835V2 - SN: 4d020

Calibration Procedure(s)

FF-Z11-003-01

Calibration Procedures for dipole validation kits

Calibration date:

August 28, 2017

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|------------------------------------------|-----------------------|
| Power Meter NRVD        | 102083     | 22-Sep-16 (CTTL, No.J16X06809)           | Sep-17                |
| Power sensor NRV-Z5     | 100595     | 22-Sep-16 (CTTL, No.J16X06809)           | Sep-17                |
| Reference Probe EX3DV4  | SN 3617    | 23-Jan-17(SPEAG,No.EX3-3617_Jan17)       | Jan-18                |
| DAE4                    | SN 1331    | 19-Jan-17(CTTL-SPEAG,No.Z17-97015)       | Jan-18                |
| Secondary Standards     | ID #       | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 13-Jan-17 (CTTL, No.J17X00286)           | Jan-18                |
| Network Analyzer E5071C | MY46110673 | 13-Jan-17 (CTTL, No.J17X00285)           | Jan-18                |

|                | Name        | Function           | Signature |
|----------------|-------------|--------------------|-----------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |           |
| Reviewed by:   | Lin Hao     | SAR Test Engineer  |           |
| Approved by:   | Qi Dianyuan | SAR Project Leader |           |

Issued: August 31, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97114

Page 1 of 8



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

#### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

- DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cntl@chinattl.com http://www.chinattl.cn

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |              |
|------------------------------|--------------------------|--------------|
| DASY Version                 | DASY52                   | 52.10.0.1446 |
| Extrapolation                | Advanced Extrapolation   |              |
| Phantom                      | Triple Flat Phantom 5.1C |              |
| Distance Dipole Center - TSL | 15 mm                    | with Spacer  |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm        |              |
| Frequency                    | 835 MHz $\pm$ 1 MHz      |              |

### Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 41.5           | 0.90 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 41.2 $\pm$ 6 % | 0.89 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | <1.0 °C             | ---            | ---                  |

### SAR result with Head TSL

|                                                         |                    |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL   | Condition          |                                |
| SAR measured                                            | 250 mW input power | 2.34 mW / g                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 9.45 mW / g $\pm$ 18.8 % (k=2) |
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                                |
| SAR measured                                            | 250 mW input power | 1.51 mW / g                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 6.09 mW / g $\pm$ 18.7 % (k=2) |

### Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 55.2           | 0.97 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 55.6 $\pm$ 6 % | 0.98 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | <1.0 °C             | ---            | ---                  |

### SAR result with Body TSL

|                                                         |                    |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL   | Condition          |                                |
| SAR measured                                            | 250 mW input power | 2.46 mW / g                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 9.75 mW / g $\pm$ 18.8 % (k=2) |
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | Condition          |                                |
| SAR measured                                            | 250 mW input power | 1.63 mW / g                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 6.47 mW / g $\pm$ 18.7 % (k=2) |

Certificate No: Z17-97114

Page 3 of 8



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 50.3Ω- 2.54jΩ |
| Return Loss                          | - 31.9dB      |

### Antenna Parameters with Body TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 46.8Ω- 4.57jΩ |
| Return Loss                          | - 24.8dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.495 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

# DASY5 Validation Report for Head TSL

Date: 08.28.2017

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d020

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.887 \text{ S/m}$ ;  $\epsilon_r = 41.22$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Left Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(9.73, 9.73, 9.73); Calibrated: 1/23/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)


**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 58.74V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 3.60 W/kg

SAR(1 g) = 2.34 W/kg; SAR(10 g) = 1.51 W/kg

Maximum value of SAR (measured) = 3.16 W/kg

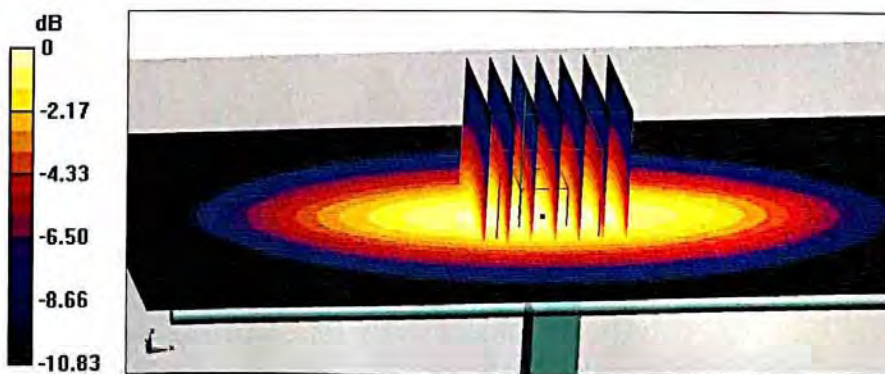


0 dB = 3.16 W/kg = 5.00 dBW/kg



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

### Impedance Measurement Plot for Head TSL

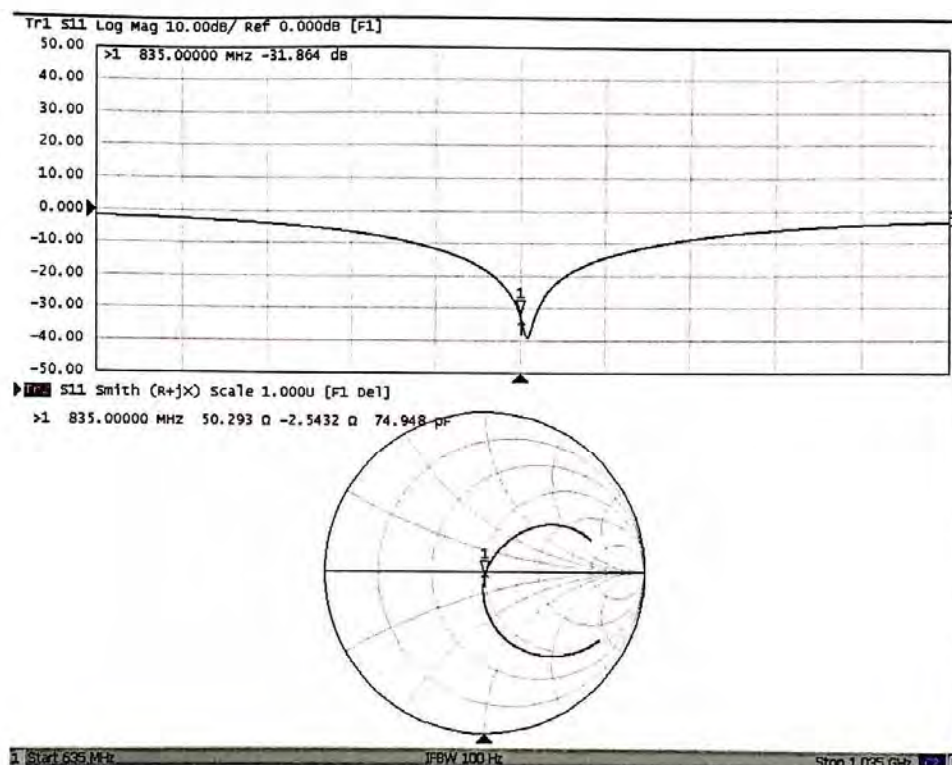

Certificate No: Z17-97114

Page 6 of 8



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

# DASY5 Validation Report for Body TSL

Date: 08.27.2017

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d020

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.984 \text{ S/m}$ ;  $\epsilon_r = 55.62$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(9.64,9.64, 9.64); Calibrated: 1/23/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)


**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 56.55 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 3.71 W/kg

SAR(1 g) = 2.46 W/kg; SAR(10 g) = 1.63 W/kg

Maximum value of SAR (measured) = 3.29 W/kg

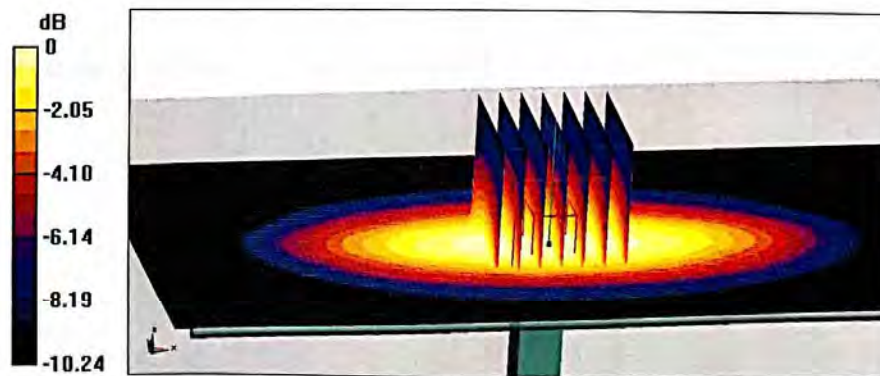


0 dB = 3.29 W/kg = 5.17 dBW/kg



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

### Impedance Measurement Plot for Body TSL

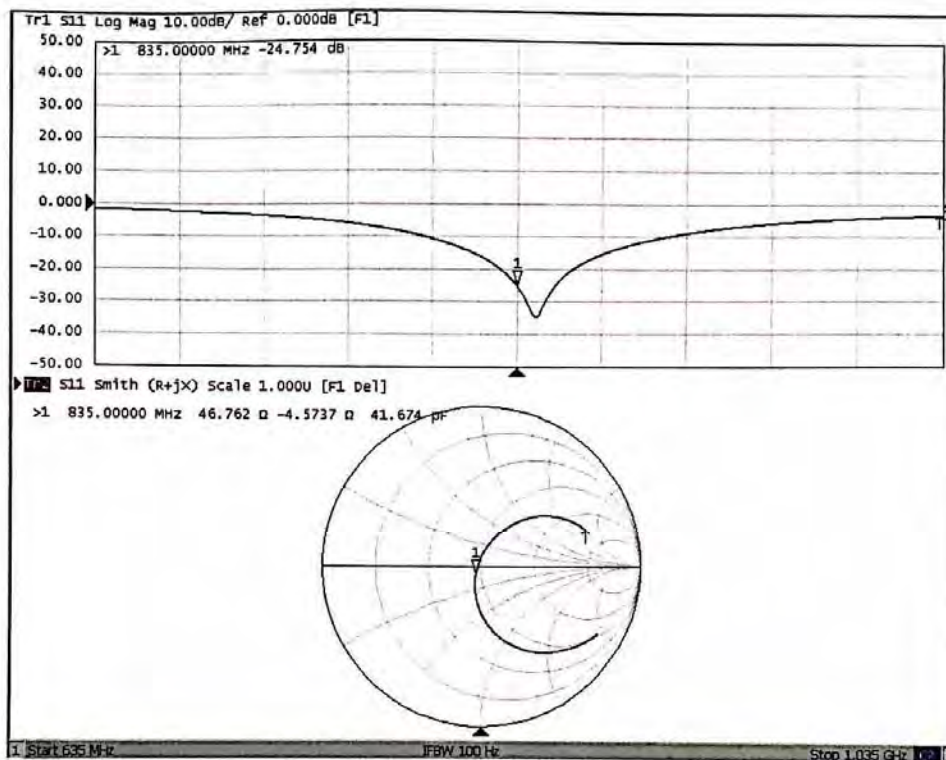



## ANNEX G: D1900V2 Dipole Calibration Certificate

In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L0570Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

Client

TA(Shanghai)

Certificate No: Z17-97115

## CALIBRATION CERTIFICATE

Object

D1900V2 - SN: 5d060

Calibration Procedure(s)

FF-Z11-003-01

Calibration Procedures for dipole validation kits

Calibration date:

August 26, 2017

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&amp;TE critical for calibration)

| Primary Standards       | ID #       | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|------------------------------------------|-----------------------|
| Power Meter NRVD        | 102083     | 22-Sep-16 (CTTL, No.J16X06809)           | Sep-17                |
| Power sensor NRV-Z5     | 100595     | 22-Sep-16 (CTTL, No.J16X06809)           | Sep-17                |
| Reference Probe EX3DV4  | SN 3617    | 23-Jan-17(SPEAG,No.EX3-3617_Jan17)       | Jan-18                |
| DAE4                    | SN 1331    | 19-Jan-17(CTTL-SPEAG,No.Z17-97015)       | Jan-18                |
| Secondary Standards     | ID #       | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 13-Jan-17 (CTTL, No.J17X00286)           | Jan-18                |
| Network Analyzer E5071C | MY46110673 | 13-Jan-17 (CTTL, No.J17X00285)           | Jan-18                |

|                | Name        | Function           | Signature |
|----------------|-------------|--------------------|-----------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |           |
| Reviewed by:   | Lin Hao     | SAR Test Engineer  |           |
| Approved by:   | Qi Dianyuan | SAR Project Leader |           |

Issued: August 30, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97115

Page 1 of 8



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

#### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz


#### Additional Documentation:

- DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |              |
|------------------------------|--------------------------|--------------|
| DASY Version                 | DASY52                   | 52.10.0.1446 |
| Extrapolation                | Advanced Extrapolation   |              |
| Phantom                      | Triple Flat Phantom 5.1C |              |
| Distance Dipole Center - TSL | 10 mm                    | with Spacer  |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm        |              |
| Frequency                    | 1900 MHz $\pm$ 1 MHz     |              |

### Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 40.0           | 1.40 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 39.9 $\pm$ 6 % | 1.41 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | <1.0 °C             | ---            | ---                  |

### SAR result with Head TSL

|                                                         |                    |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL   | Condition          |                                |
| SAR measured                                            | 250 mW input power | 10.1 mW / g                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 40.1 mW / g $\pm$ 18.8 % (k=2) |
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                                |
| SAR measured                                            | 250 mW input power | 5.19 mW / g                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 20.7 mW / g $\pm$ 18.7 % (k=2) |


### Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 53.3           | 1.52 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 53.6 $\pm$ 6 % | 1.53 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | <1.0 °C             | ---            | ---                  |

### SAR result with Body TSL

|                                                         |                    |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL   | Condition          |                                |
| SAR measured                                            | 250 mW input power | 9.90 mW / g                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 39.5 mW / g $\pm$ 18.8 % (k=2) |
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | Condition          |                                |
| SAR measured                                            | 250 mW input power | 5.21 mW / g                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 20.8 mW / g $\pm$ 18.7 % (k=2) |



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 52.0Ω+ 6.59jΩ |
| Return Loss                          | - 23.4dB      |

### Antenna Parameters with Body TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 52.7Ω+ 8.35jΩ |
| Return Loss                          | - 21.4dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.302 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: ctntl@chinattl.com http://www.chinattl.cn

# DASY5 Validation Report for Head TSL

Date: 08.26.2017

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d060

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.413$  S/m;  $\epsilon_r = 39.85$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Left Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(8.26, 8.26, 8.26); Calibrated: 1/23/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

## System Performance Check/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:


 $dx=5$ mm,  $dy=5$ mm,  $dz=5$ mm

Reference Value = 94.94 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 19.5 W/kg

SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.19 W/kg

Maximum value of SAR (measured) = 15.9 W/kg

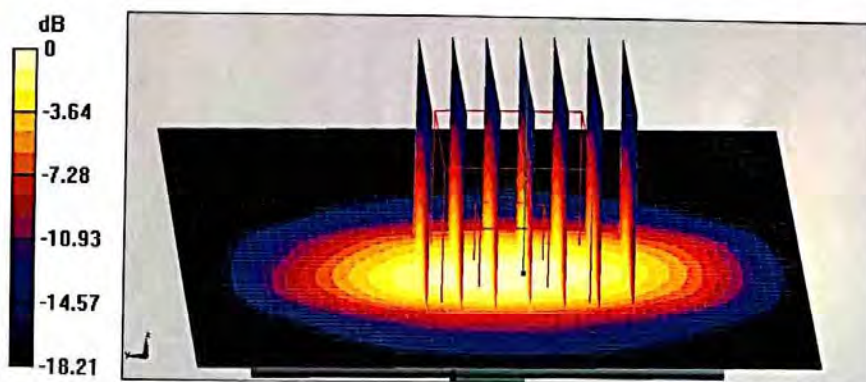


0 dB = 15.9 W/kg = 12.01 dBW/kg



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

### Impedance Measurement Plot for Head TSL

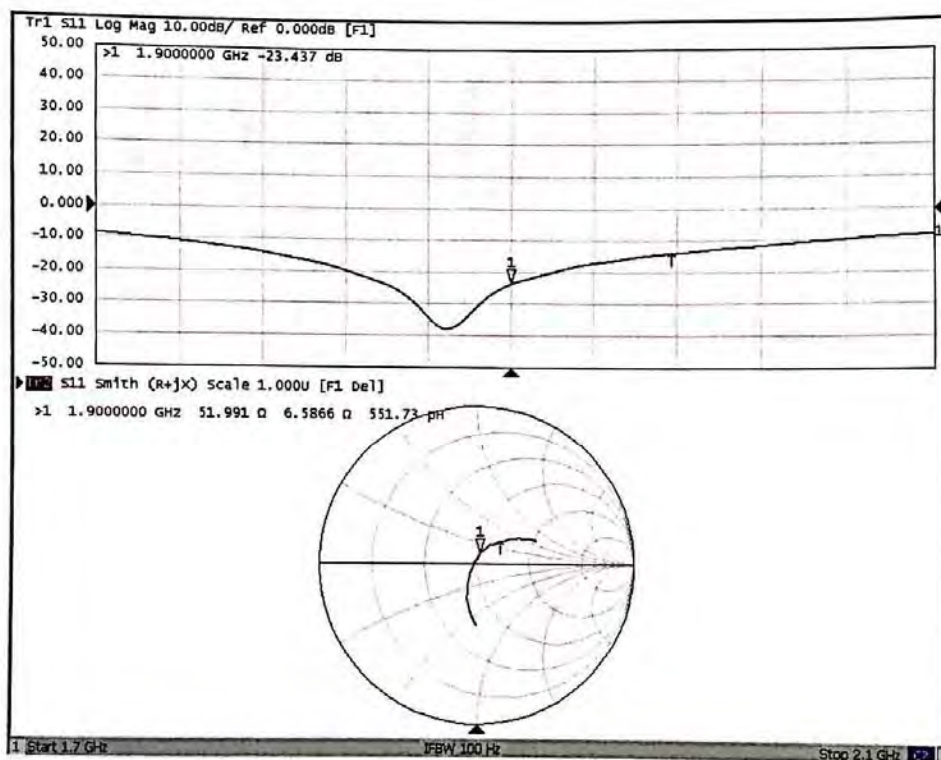



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

# DASY5 Validation Report for Body TSL

Date: 08.26.2017

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d060

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.528$  S/m;  $\epsilon_r = 53.55$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Center Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(7.95, 7.95, 7.95); Calibrated: 1/23/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

## System Performance Check/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:


dx=5mm, dy=5mm, dz=5mm

Reference Value = 91.19 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 9.9 W/kg; SAR(10 g) = 5.21 W/kg

Maximum value of SAR (measured) = 15.3 W/kg

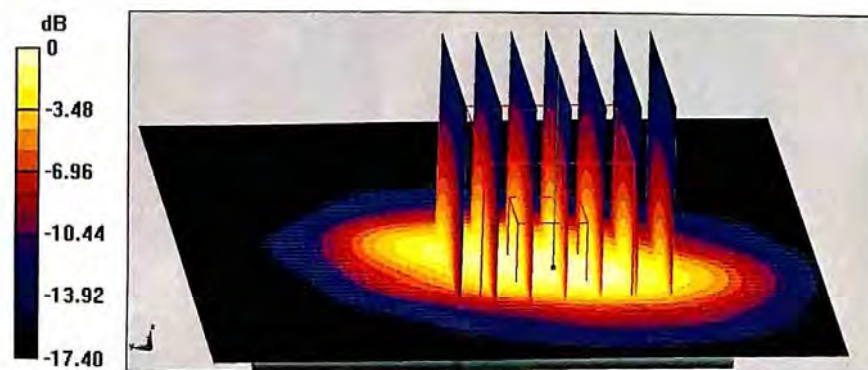


0 dB = 15.3 W/kg = 11.85 dBW/kg



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

### Impedance Measurement Plot for Body TSL

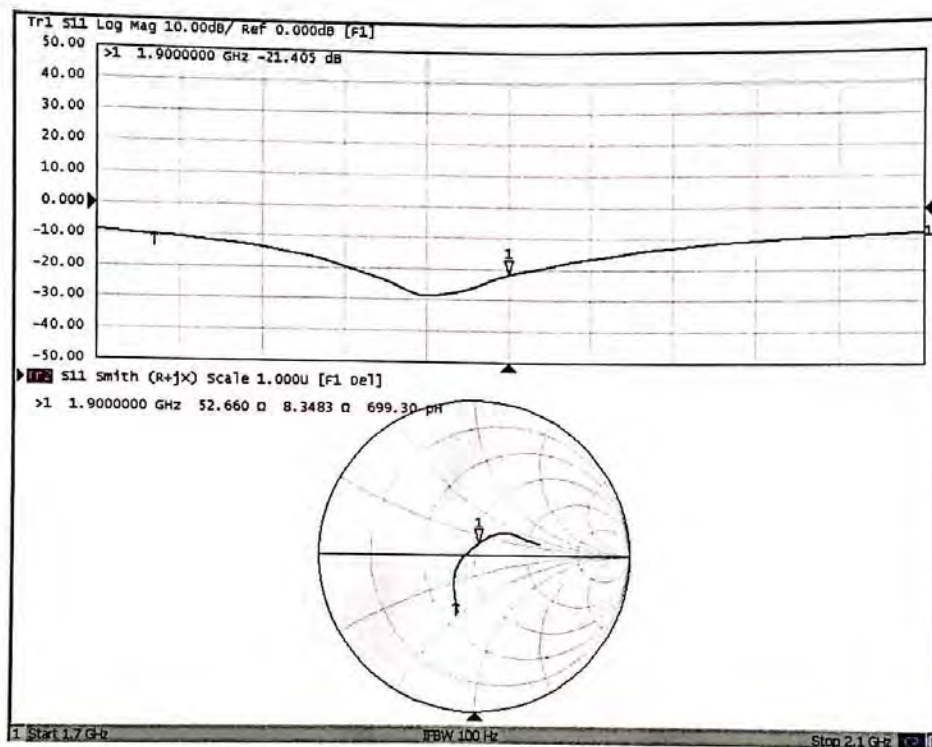



## ANNEX H: D2450V2 Dipole Calibration Certificate

In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L0570Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

Client

TA(Shanghai)

Certificate No: Z17-97116

## CALIBRATION CERTIFICATE

Object

D2450V2 - SN: 786

Calibration Procedure(s)

FF-Z11-003-01

Calibration Procedures for dipole validation kits

Calibration date:

August 29, 2017

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&amp;TE critical for calibration)

| Primary Standards       | ID #       | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|------------------------------------------|-----------------------|
| Power Meter NRVD        | 102083     | 22-Sep-16 (CTTL, No.J16X06809)           | Sep-17                |
| Power sensor NRV-Z5     | 100595     | 22-Sep-16 (CTTL, No.J16X06809)           | Sep-17                |
| Reference Probe EX3DV4  | SN 3617    | 23-Jan-17(SPEAG,No.EX3-3617_Jan17)       | Jan-18                |
| DAE4                    | SN 1331    | 19-Jan-17(CTTL-SPEAG,No.Z17-97015)       | Jan-18                |
| Secondary Standards     | ID #       | Cal Date(Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 13-Jan-17 (CTTL, No.J17X00286)           | Jan-18                |
| Network Analyzer E5071C | MY46110673 | 13-Jan-17 (CTTL, No.J17X00285)           | Jan-18                |

Calibrated by:

Name

Function

Signature

Zhao Jing

SAR Test Engineer

Reviewed by:

Lin Hao

SAR Test Engineer

Approved by:

Qi Dianyuan

SAR Project Leader

Issued: September 1, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97116

Page 1 of 8



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

#### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

- DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                          |              |
|------------------------------|--------------------------|--------------|
| DASY Version                 | DASY52                   | 52.10.0.1446 |
| Extrapolation                | Advanced Extrapolation   |              |
| Phantom                      | Triple Flat Phantom 5.1C |              |
| Distance Dipole Center - TSL | 10 mm                    | with Spacer  |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm        |              |
| Frequency                    | 2450 MHz $\pm$ 1 MHz     |              |

### Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 39.2           | 1.80 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 39.7 $\pm$ 6 % | 1.82 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | <1.0 °C             | ---            | ---                  |

### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL   | Condition          |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR measured                                            | 250 mW input power | 13.2 mW / g                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 52.6 mW / g $\pm$ 18.8 % (k=2) |
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                                |
| SAR measured                                            | 250 mW input power | 6.16 mW / g                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 24.6 mW / g $\pm$ 18.7 % (k=2) |


### Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 52.7           | 1.95 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 52.5 $\pm$ 6 % | 1.94 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | <1.0 °C             | ---            | ---                  |

### SAR result with Body TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL   | Condition          |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR measured                                            | 250 mW input power | 12.7 mW / g                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 50.8 mW / g $\pm$ 18.8 % (k=2) |
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | Condition          |                                |
| SAR measured                                            | 250 mW input power | 5.87 mW / g                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 23.5 mW / g $\pm$ 18.7 % (k=2) |



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 53.4Ω+ 4.29jΩ |
| Return Loss                          | - 25.5dB      |

### Antenna Parameters with Body TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 51.0Ω+ 6.61jΩ |
| Return Loss                          | - 23.6dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.265 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

# DASY5 Validation Report for Head TSL

Date: 08.29.2017

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 786**

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.822$  S/m;  $\epsilon_r = 39.65$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Left Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(7.74, 7.74, 7.74); Calibrated: 1/23/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)


**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 105.1 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 27.5 W/kg

**SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.16 W/kg**

Maximum value of SAR (measured) = 22.2 W/kg

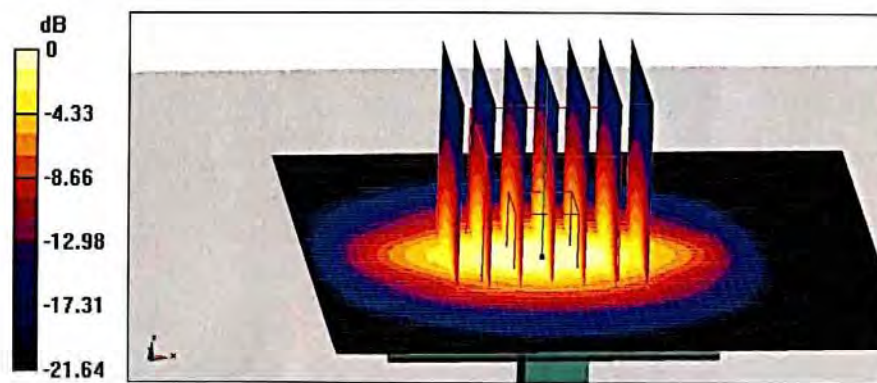


0 dB = 22.2 W/kg = 13.46 dBW/kg



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

### Impedance Measurement Plot for Head TSL

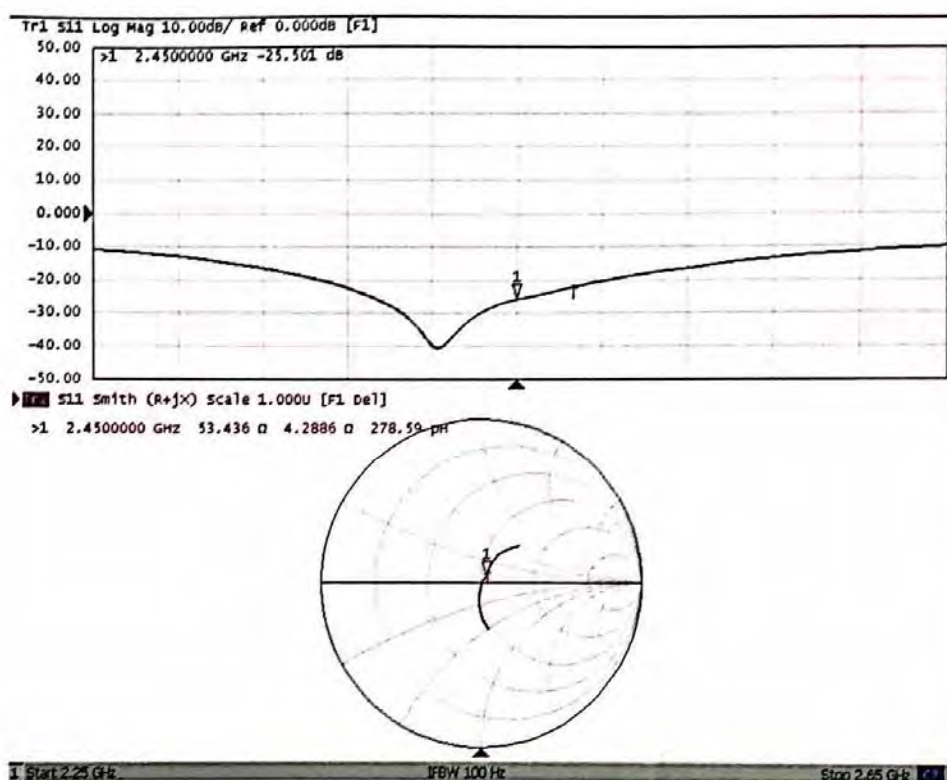



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

# DASY5 Validation Report for Body TSL

Date: 08.29.2017

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 786

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.943$  S/m;  $\epsilon_r = 52.45$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(7.8, 7.8, 7.8); Calibrated: 1/23/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 1/19/2017
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)


**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 92.28 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 27.0 W/kg

SAR(1 g) = 12.7 W/kg; SAR(10 g) = 5.87 W/kg

Maximum value of SAR (measured) = 21.5 W/kg

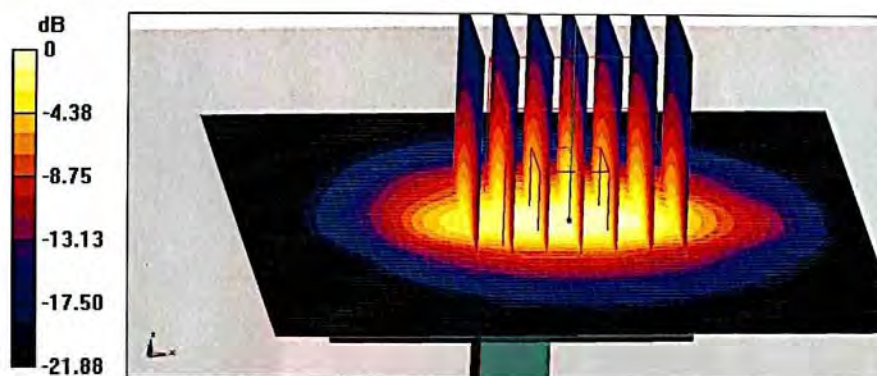


0 dB = 21.5 W/kg = 13.32 dBW/kg



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

### Impedance Measurement Plot for Body TSL

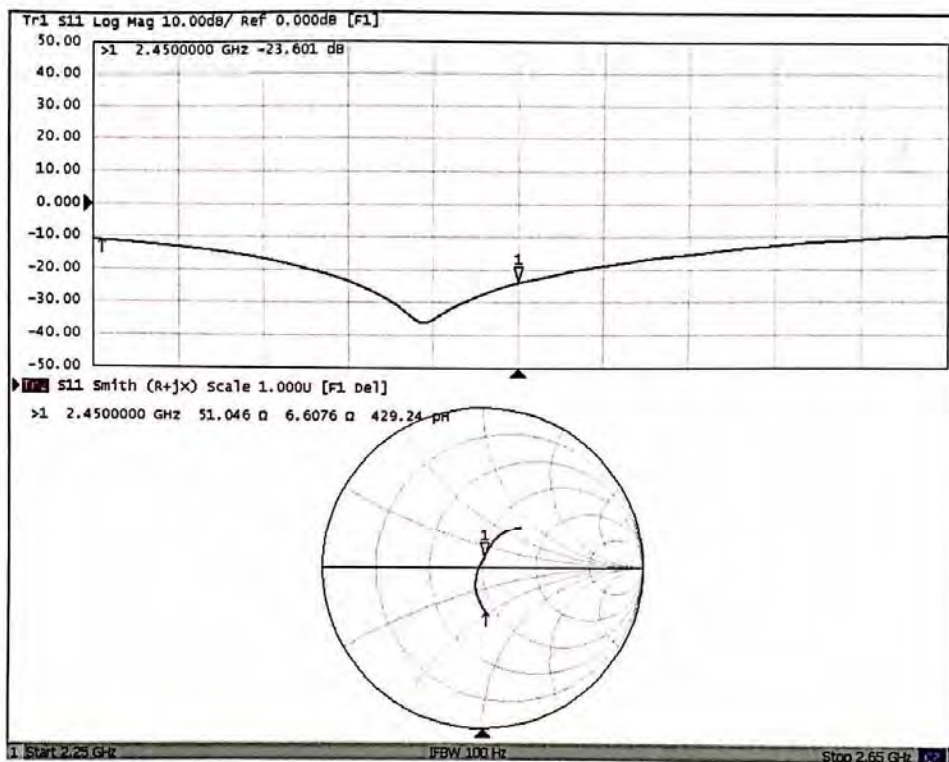

# ANNEX I: DAE4 Calibration Certificate (SN:1291)

**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
 Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client **TA-SH (Auden)**

Certificate No: DAE4-1291\_Oct17

| CALIBRATION CERTIFICATE                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |                                                                                   |                                   |                          |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------|-----------------------------------|--------------------------|-------------------|------|----------------------------|-----------------------|-------------------------------|-------------|----------------------|--------|---------------------|------|-----------------------|-----------------|---------------------------|--------------------|----------------------------|------------------------|---------------------|--------------------|----------------------------|------------------------|
| Object                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      | DAE4 - SD 000 D04 BM - SN: 1291                                                   |                                   |                          |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Calibration procedure(s)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    | QA CAL-06.v29<br>Calibration procedure for the data acquisition electronics (DAE) |                                   |                          |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Calibration date:                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           | October 31, 2017                                                                  |                                   |                          |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).<br/>           The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Keithley Multimeter Type 2001</td> <td>SN: 0810278</td> <td>31-Aug-17 (No:21092)</td> <td>Aug-18</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Auto DAE Calibration Unit</td> <td>SE UWS 053 AA 1001</td> <td>05-Jan-17 (in house check)</td> <td>In house check: Jan-18</td> </tr> <tr> <td>Calibrator Box V2.1</td> <td>SE UMS 006 AA 1002</td> <td>05-Jan-17 (in house check)</td> <td>In house check: Jan-18</td> </tr> </tbody> </table> |                                                                                   |                                   |                          | Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | Keithley Multimeter Type 2001 | SN: 0810278 | 31-Aug-17 (No:21092) | Aug-18 | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | Auto DAE Calibration Unit | SE UWS 053 AA 1001 | 05-Jan-17 (in house check) | In house check: Jan-18 | Calibrator Box V2.1 | SE UMS 006 AA 1002 | 05-Jan-17 (in house check) | In house check: Jan-18 |
| Primary Standards                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           | ID #                                                                              | Cal Date (Certificate No.)        | Scheduled Calibration    |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Keithley Multimeter Type 2001                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               | SN: 0810278                                                                       | 31-Aug-17 (No:21092)              | Aug-18                   |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Secondary Standards                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         | ID #                                                                              | Check Date (in house)             | Scheduled Check          |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Auto DAE Calibration Unit                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | SE UWS 053 AA 1001                                                                | 05-Jan-17 (in house check)        | In house check: Jan-18   |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Calibrator Box V2.1                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         | SE UMS 006 AA 1002                                                                | 05-Jan-17 (in house check)        | In house check: Jan-18   |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Calibrated by:                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              | Name<br>Eric Hainfeld                                                             | Function<br>Laboratory Technician | Signature<br>            |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| Approved by:                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                | Sven Kühn                                                                         | Deputy Manager                    |                          |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |                                                                                   |                                   | Issued: October 31, 2017 |                   |      |                            |                       |                               |             |                      |        |                     |      |                       |                 |                           |                    |                            |                        |                     |                    |                            |                        |

Certificate No: DAE4-1291\_Oct17

Page 1 of 5

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

**DAE** data acquisition electronics  
**Connector angle** information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
  - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
  - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
  - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
  - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - **Input resistance:** Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
  - **Power consumption:** Typical value for information. Supply currents in various operating modes.

**DC Voltage Measurement**

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V, full range = -100...+300 mV

Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                         | Y                         | Z                         |
|---------------------|---------------------------|---------------------------|---------------------------|
| High Range          | 402.531 $\pm$ 0.02% (k=2) | 403.204 $\pm$ 0.02% (k=2) | 403.118 $\pm$ 0.02% (k=2) |
| Low Range           | 3.97419 $\pm$ 1.50% (k=2) | 3.97827 $\pm$ 1.50% (k=2) | 3.97437 $\pm$ 1.50% (k=2) |

**Connector Angle**

|                                           |                                     |
|-------------------------------------------|-------------------------------------|
| Connector Angle to be used in DASY system | 309.5 $^{\circ}$ $\pm$ 1 $^{\circ}$ |
|-------------------------------------------|-------------------------------------|

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

| High Range        | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 200033.09                 | -1.13                        | -0.00     |
| Channel X + Input | 20005.24                  | 0.43                         | 0.00      |
| Channel X - Input | -20002.50                 | 2.70                         | -0.01     |
| Channel Y + Input | 200031.52                 | -2.54                        | -0.00     |
| Channel Y + Input | 20002.99                  | -1.90                        | -0.01     |
| Channel Y - Input | -20005.78                 | -0.47                        | 0.00      |
| Channel Z + Input | 200033.14                 | -0.98                        | -0.00     |
| Channel Z + Input | 20001.98                  | -2.75                        | -0.01     |
| Channel Z - Input | -20006.08                 | -0.65                        | 0.00      |

| Low Range         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 2001.76                   | 0.75                         | 0.04      |
| Channel X + Input | 201.56                    | 0.40                         | 0.20      |
| Channel X - Input | -198.62                   | 0.27                         | -0.14     |
| Channel Y + Input | 2001.35                   | 0.49                         | 0.02      |
| Channel Y + Input | 202.20                    | 1.16                         | 0.57      |
| Channel Y - Input | -200.25                   | -1.24                        | 0.62      |
| Channel Z + Input | 2000.49                   | -0.37                        | -0.02     |
| Channel Z + Input | 200.01                    | -0.98                        | -0.49     |
| Channel Z - Input | -200.38                   | -1.21                        | 0.61      |

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode Input Voltage (mV) | High Range Average Reading ( $\mu\text{V}$ ) | Low Range Average Reading ( $\mu\text{V}$ ) |
|-----------|--------------------------------|----------------------------------------------|---------------------------------------------|
| Channel X | 200                            | 9.58                                         | 7.76                                        |
|           | - 200                          | -6.07                                        | -8.06                                       |
| Channel Y | 200                            | 13.34                                        | 13.80                                       |
|           | - 200                          | -15.13                                       | -15.41                                      |
| Channel Z | 200                            | -16.12                                       | -16.97                                      |
|           | - 200                          | 14.39                                        | 14.53                                       |

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X ( $\mu\text{V}$ ) | Channel Y ( $\mu\text{V}$ ) | Channel Z ( $\mu\text{V}$ ) |
|-----------|--------------------|-----------------------------|-----------------------------|-----------------------------|
| Channel X | 200                | -                           | 0.30                        | -3.79                       |
| Channel Y | 200                | 6.95                        | -                           | 0.36                        |
| Channel Z | 200                | 10.83                       | 4.52                        | -                           |

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 16119            | 16474           |
| Channel Y | 15930            | 16813           |
| Channel Z | 16170            | 16434           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | 0.93               | -0.36                  | 2.05                   | 0.49                      |
| Channel Y | -0.05              | -1.46                  | 0.88                   | 0.48                      |
| Channel Z | -1.03              | -2.76                  | 1.81                   | 0.59                      |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

#### 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

#### 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |

**ANNEX J: DAE4 Calibration Certificate(SN:1317)**

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TA-SH (Auden)**

Certificate No: **DAE4-1317\_Mar18**

**CALIBRATION CERTIFICATE**

Object **DAE4 - SD 000 D04 BM - SN: 1317**

Calibration procedure(s) **QA CAL-06.v29  
Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **March 23, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                                | ID #               | Cal Date (Certificate No.) | Scheduled Calibration  |
|--------------------------------------------------|--------------------|----------------------------|------------------------|
| Keithley Multimeter Type 2001                    | SN: 0810278        | 31-Aug-17 (No:21092)       | Aug-18                 |
| Secondary Standards                              | ID #               | Check Date (in house)      | Scheduled Check        |
| Auto DAE Calibration Unit<br>Calibrator Box V2.1 | SE UWS 053 AA 1001 | 04-Jan-18 (in house check) | In house check: Jan-19 |
|                                                  | SE UMS 006 AA 1002 | 04-Jan-18 (in house check) | In house check: Jan-19 |

|                |                                  |                                          |               |
|----------------|----------------------------------|------------------------------------------|---------------|
| Calibrated by: | Name<br><b>Dominique Steffen</b> | Function<br><b>Laboratory Technician</b> | Signature<br> |
| Approved by:   | Name<br><b>Egon Kühn</b>         | Function<br><b>Deputy Manager</b>        | Signature<br> |

Issued: March 23, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **DAE4-1317\_Mar18**

Page 1 of 5

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

## Glossary

**DAE** data acquisition electronics  
**Connector angle** information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
  - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
  - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
  - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
  - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - **Input resistance:** Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
  - **Power consumption:** Typical value for information. Supply currents in various operating modes.

### DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1μV, full range = -100...+300 mV

Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                     | Y                     | Z                     |
|---------------------|-----------------------|-----------------------|-----------------------|
| High Range          | 403.713 ± 0.02% (k=2) | 404.474 ± 0.02% (k=2) | 403.834 ± 0.02% (k=2) |
| Low Range           | 3.97916 ± 1.50% (k=2) | 3.99031 ± 1.50% (k=2) | 3.96832 ± 1.50% (k=2) |

### Connector Angle

|                                           |               |
|-------------------------------------------|---------------|
| Connector Angle to be used in DASY system | 332.0 ° ± 1 ° |
|-------------------------------------------|---------------|

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

| High Range        | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 200033.59                 | -2.39                        | -0.00     |
| Channel X + Input | 20006.23                  | 0.60                         | 0.00      |
| Channel X - Input | -20003.30                 | 2.01                         | -0.01     |
| Channel Y + Input | 200032.59                 | -3.60                        | -0.00     |
| Channel Y + Input | 20003.70                  | -1.89                        | -0.01     |
| Channel Y - Input | -20004.09                 | 1.35                         | -0.01     |
| Channel Z + Input | 200035.04                 | -0.93                        | -0.00     |
| Channel Z + Input | 20005.33                  | -0.22                        | -0.00     |
| Channel Z - Input | -20006.76                 | -1.25                        | 0.01      |

| Low Range         | Reading ( $\mu\text{V}$ ) | Difference ( $\mu\text{V}$ ) | Error (%) |
|-------------------|---------------------------|------------------------------|-----------|
| Channel X + Input | 2001.75                   | 0.20                         | 0.01      |
| Channel X + Input | 200.99                    | -0.43                        | -0.21     |
| Channel X - Input | -197.13                   | 1.49                         | -0.75     |
| Channel Y + Input | 2001.26                   | -0.25                        | -0.01     |
| Channel Y + Input | 200.67                    | -0.56                        | -0.28     |
| Channel Y - Input | -199.10                   | -0.34                        | 0.17      |
| Channel Z + Input | 2000.98                   | -0.47                        | -0.02     |
| Channel Z + Input | 200.06                    | -1.17                        | -0.58     |
| Channel Z - Input | -199.95                   | -1.19                        | 0.60      |

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode Input Voltage (mV) | High Range Average Reading ( $\mu\text{V}$ ) | Low Range Average Reading ( $\mu\text{V}$ ) |
|-----------|--------------------------------|----------------------------------------------|---------------------------------------------|
| Channel X | 200                            | 11.88                                        | 10.25                                       |
|           | - 200                          | -8.69                                        | -10.35                                      |
| Channel Y | 200                            | 11.35                                        | 11.40                                       |
|           | - 200                          | -13.19                                       | -12.90                                      |
| Channel Z | 200                            | 1.73                                         | 1.34                                        |
|           | - 200                          | -2.98                                        | -3.58                                       |

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X ( $\mu\text{V}$ ) | Channel Y ( $\mu\text{V}$ ) | Channel Z ( $\mu\text{V}$ ) |
|-----------|--------------------|-----------------------------|-----------------------------|-----------------------------|
| Channel X | 200                | -                           | 2.22                        | -4.63                       |
| Channel Y | 200                | 8.79                        | -                           | 3.02                        |
| Channel Z | 200                | 10.60                       | 8.05                        | -                           |

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 15758            | 16030           |
| Channel Y | 16498            | 16052           |
| Channel Z | 16107            | 15724           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | 1.03               | -0.09                  | 2.36                   | 0.48                      |
| Channel Y | -0.33              | -1.77                  | 1.22                   | 0.54                      |
| Channel Z | -1.81              | -3.67                  | -0.40                  | 0.67                      |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

#### 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

#### 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |