



Annex A Test setup photographs

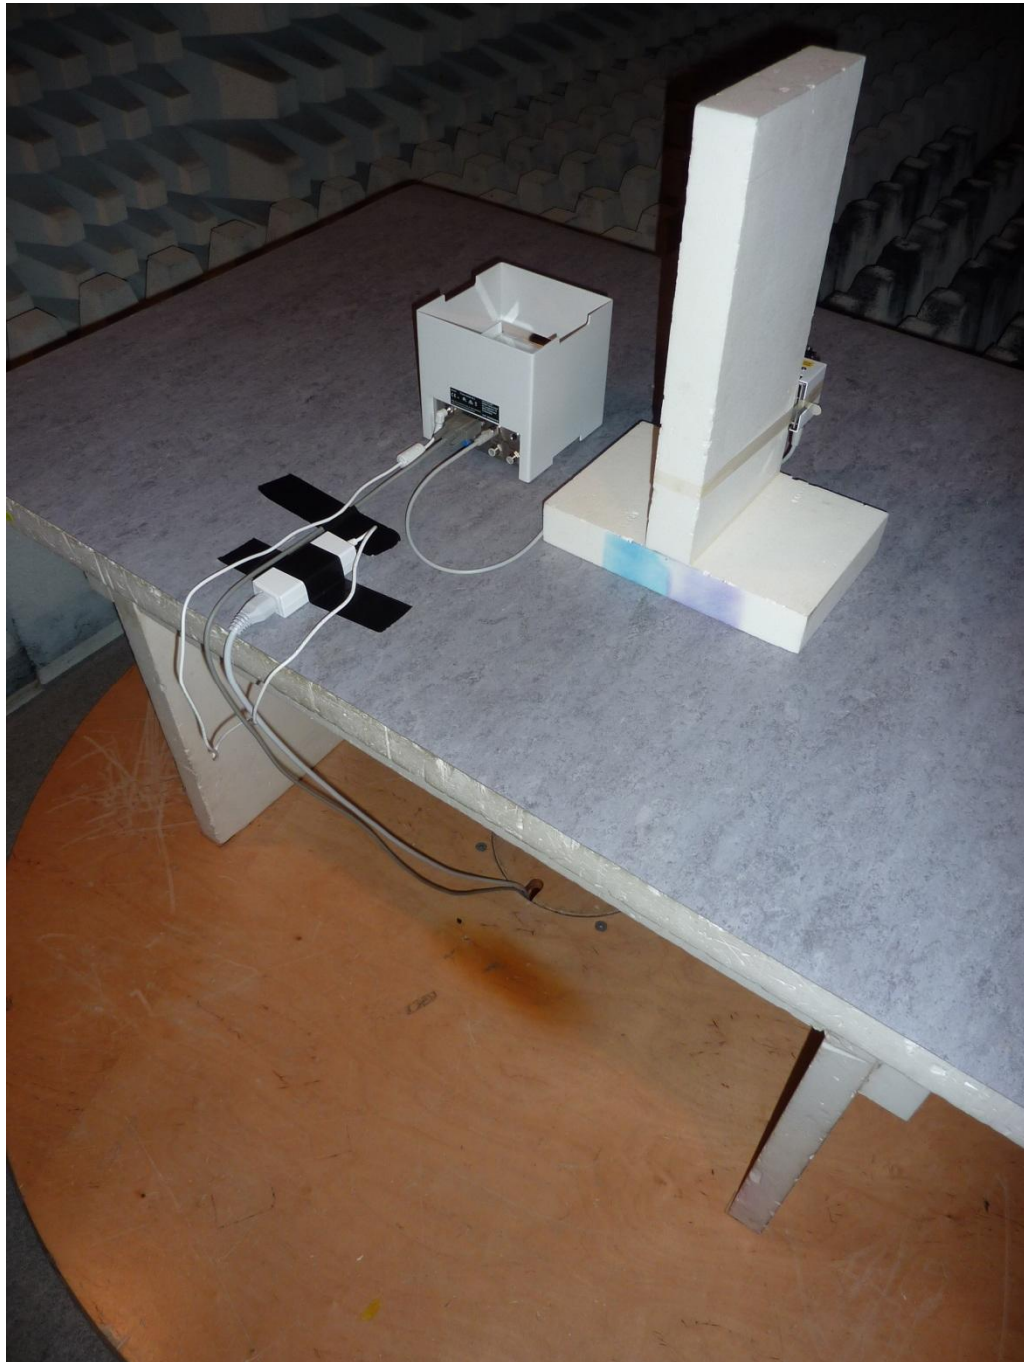

161006_1a.jpg: QLX45 Liquid Dosing Module, test setup fully anechoic chamber

Annex A Test setup photographs

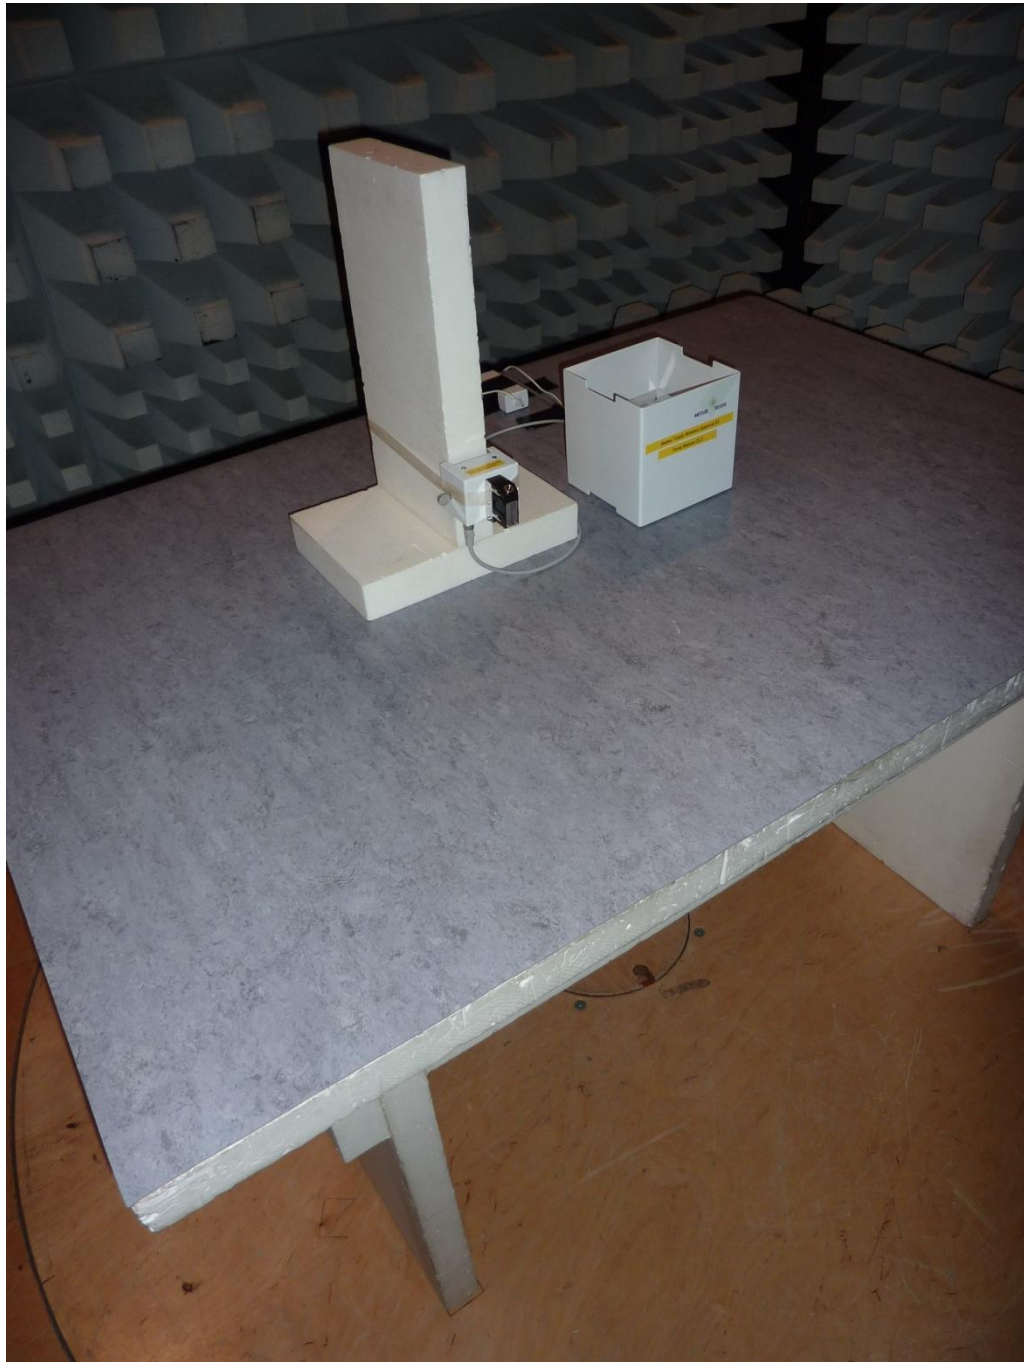


161006_1b.jpg: QLX45 Liquid Dosing Module, test setup fully anechoic chamber

Annex A Test setup photographs



161006_1c.jpg: QLX45 Liquid Dosing Module, test setup fully anechoic chamber

Annex A Test setup photographs

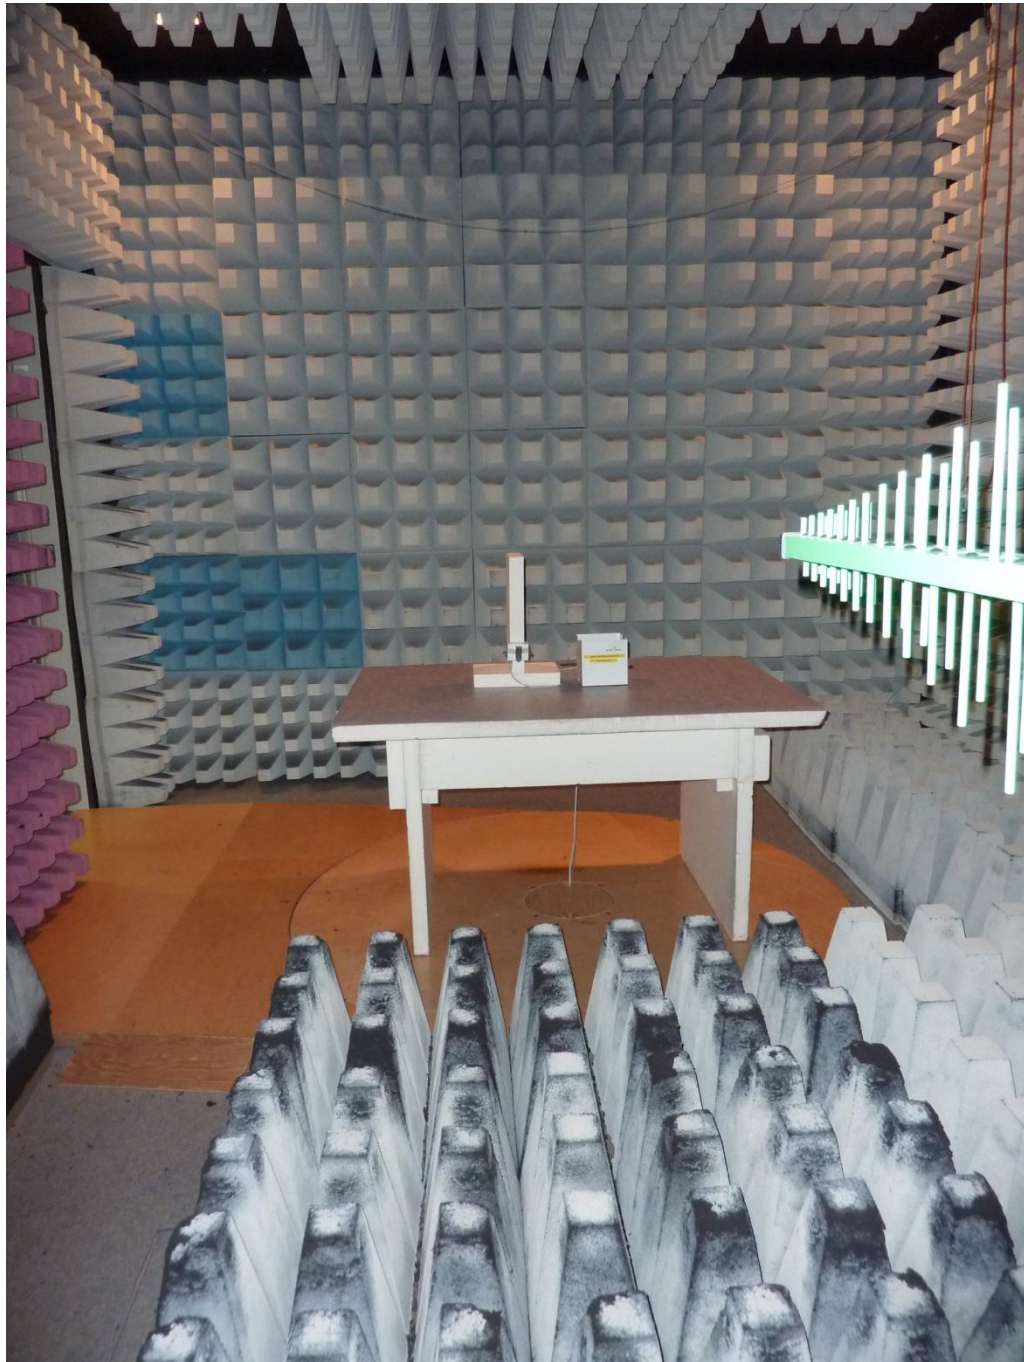

161006_1d.jpg: QLX45 Liquid Dosing Module, test setup fully anechoic chamber

Annex A Test setup photographs



161006_1e.jpg: QXL45 Liquid Dosing Module, test setup outdoor test site

Annex A Test setup photographs



161006_1f.jpg: QLX45 Liquid Dosing Module, test setup open area test site

Annex A Test setup photographs



161006_1h.jpg: QLX45 Liquid Dosing Module, test setup shielded chamber