



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

**DASY5 Validation Report for Head TSL**

Date: 08.28.2019

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1238**

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz,  
Frequency: 5750 MHz,

Medium parameters used:  $f = 5250$  MHz;  $\sigma = 4.692$  S/m;  $\epsilon_r = 35.71$ ;  $\rho = 1000$   
kg/m<sup>3</sup>, Medium parameters used:  $f = 5600$  MHz;  $\sigma = 4.992$  S/m;  $\epsilon_r = 35.42$ ;  $\rho =$   
1000 kg/m<sup>3</sup>, Medium parameters used:  $f = 5750$  MHz;  $\sigma = 5.096$  S/m;  $\epsilon_r = 35.13$ ;  $\rho =$   
1000 kg/m<sup>3</sup>,

Phantom section: Center Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(5.39, 5.39, 5.39) @ 5250 MHz; ConvF(5.06, 5.06, 5.06) @ 5600 MHz; ConvF(5.07, 5.07, 5.07) @ 5750 MHz; Calibrated: 1/31/2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1555; Calibrated: 8/22/2019
- Phantom: MFP\_V5.1C ; Type: QD 000 P51CA; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7470)


**Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 69.41 V/m; Power Drift = -0.05 dB  
Peak SAR (extrapolated) = 32.8 W/kg  
**SAR(1 g) = 7.81 W/kg; SAR(10 g) = 2.23 W/kg**  
Maximum value of SAR (measured) = 18.7 W/kg

**Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 70.02 V/m; Power Drift = 0.04 dB  
Peak SAR (extrapolated) = 35.7 W/kg  
**SAR(1 g) = 7.96 W/kg; SAR(10 g) = 2.27 W/kg**  
Maximum value of SAR (measured) = 19.2 W/kg

**Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 68.55 V/m; Power Drift = 0.02 dB  
Peak SAR (extrapolated) = 36.5 W/kg  
**SAR(1 g) = 7.86 W/kg; SAR(10 g) = 2.23 W/kg**  
Maximum value of SAR (measured) = 18.9 W/kg




Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

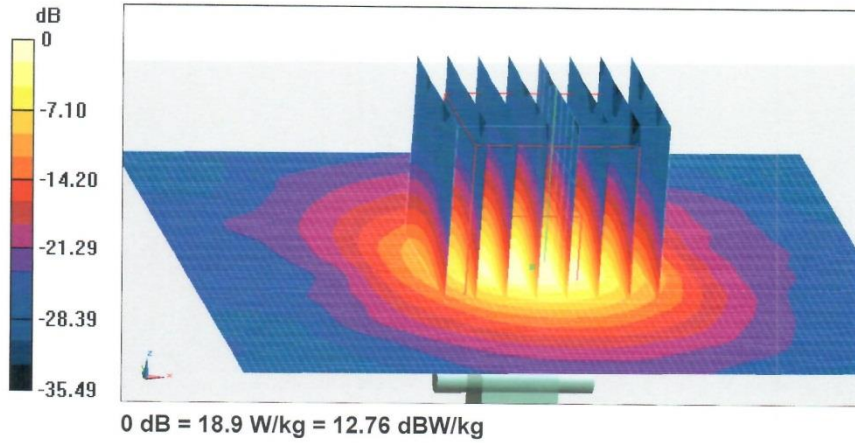



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

**Impedance Measurement Plot for Head TSL**

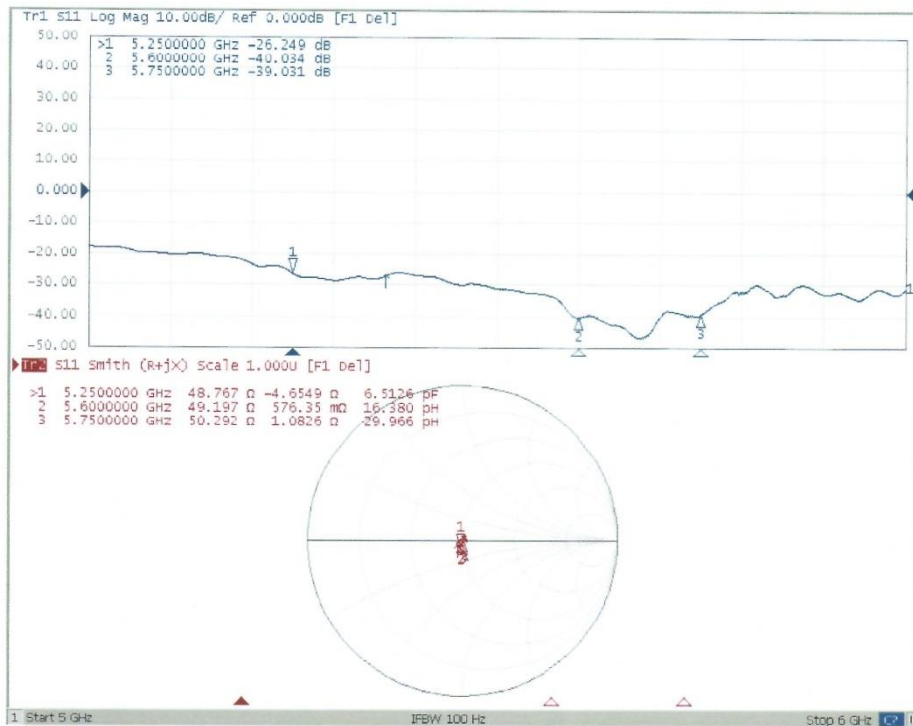



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

**DASY5 Validation Report for Body TSL**

Date: 08.29.2019

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1238**

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz,  
Frequency: 5750 MHz,

Medium parameters used: f = 5250 MHz;  $\sigma$  = 5.402 S/m;  $\epsilon_r$  = 48.05;  $\rho$  = 1000  
kg/m<sup>3</sup>, Medium parameters used: f = 5600 MHz;  $\sigma$  = 5.703 S/m;  $\epsilon_r$  = 47.61;  $\rho$  =  
1000 kg/m<sup>3</sup>, Medium parameters used: f = 5750 MHz;  $\sigma$  = 5.782 S/m;  $\epsilon_r$  = 47.49;  $\rho$   
= 1000 kg/m<sup>3</sup>,

Phantom section: Right Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(4.76, 4.76, 4.76) @ 5250 MHz; ConvF(4.23, 4.23, 4.23) @ 5600 MHz; ConvF(4.36, 4.36, 4.36) @ 5750 MHz; Calibrated: 1/31/2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1555; Calibrated: 8/22/2019
- Phantom: MFP\_V5.1C ; Type: QD 000 P51CA; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7470)


**Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan,**  
**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 54.85 V/m; Power Drift = 0.04 dB  
Peak SAR (extrapolated) = 27.5 W/kg  
**SAR(1 g) = 7.17 W/kg; SAR(10 g) = 2.04 W/kg**  
Maximum value of SAR (measured) = 16.4 W/kg

**Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan,**  
**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 56.17 V/m; Power Drift = 0.07 dB  
Peak SAR (extrapolated) = 32.3 W/kg  
**SAR(1 g) = 7.62 W/kg; SAR(10 g) = 2.18 W/kg**  
Maximum value of SAR (measured) = 18.4 W/kg

**Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan,**  
**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 55.47 V/m; Power Drift = 0.04 dB  
Peak SAR (extrapolated) = 33.2 W/kg  
**SAR(1 g) = 7.39 W/kg; SAR(10 g) = 2.1 W/kg**  
Maximum value of SAR (measured) = 18.1 W/kg



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

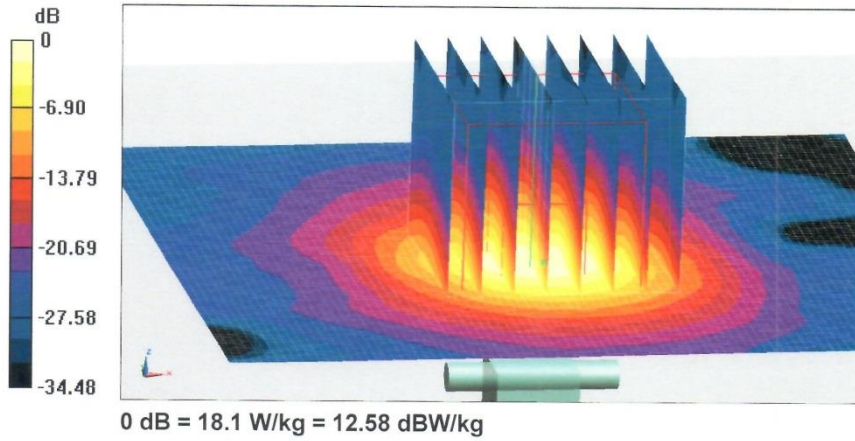






Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

**Impedance Measurement Plot for Body TSL**

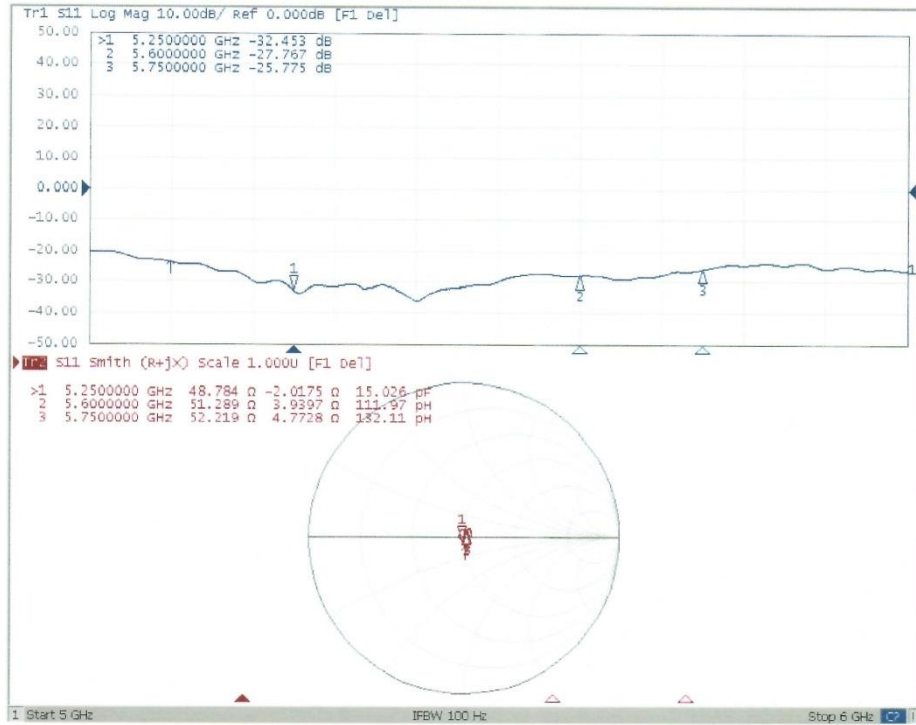

## ANNEX J Sensor Triggering Data Summary

This device was tested by the manufacturer to determine the proximity sensor triggering distances for all applicable sides and edges of the device. The measured output power at distances within  $\pm 5$  mm of the triggering points (or until touching the phantom) is included for back side and each applicable edge. The technical descriptions in the filing contain the complete set of triggering data required.

To ensure all production units are compliant, it is necessary to test SAR at a distance 1 mm less than the smallest distance between the device and SAR phantom with the device at the maximum output power (without power reduction). These SAR tests are included in addition to the SAR tests for the device touching the SAR phantom (at the reduced output power level).

We tested the power and got the different proximity sensor triggering distances for front, rear and bottom edge. The manufacturer has declared 18mm is the most conservative triggering distance for main antenna with front side, 26mm distance for rear side and 28mm distance for bottom side.

The operational description contains information explaining how this device remains compliant in the event of a sensor malfunction.

### Main Antenna (W1900, LTE Band 7)

#### Front Side

Moving device toward the phantom:

Distance(mm)	23	22	21	20	19	18	17	16	15	14	13
Main Antenna	/	/	/	/	/	20.5	20.3	20.4	20.5	20.4	20.4

Moving device away from the phantom:

Distance(mm)	23	22	21	20	19	18	17	16	15	14	13
Main Antenna	23.1	23.1	23.2	23.2	23.2	/	/	/	/	/	/

Based on the most conservative measured triggering distance of 18 mm, additional SAR measurements were required at 17 mm from the Rear side for the above modes.

#### Rear Side

Moving device toward the phantom:

Distance(mm)	31	30	29	28	27	26	25	24	23	22	21
Main Antenna	/	/	/	/	/	20.4	20.5	20.2	20.4	20.5	20.3

Moving device away from the phantom:

Distance(mm)	31	30	29	28	27	26	25	24	23	22	21
Main Antenna	23.2	23.2	23.1	23.2	23.1	/	/	/	/	/	/

Based on the most conservative measured triggering distance of 26 mm, additional SAR measurements were required at 25 mm from the Rear side for the above modes.

**Bottom Side**

Moving device toward the phantom:

Distance(mm)	33	32	31	30	29	28	27	26	25	24	23
Main Antenna	/	/	/	/	/	20.3	20.4	20.5	20.4	20.5	20.5

Moving device away from the phantom:

Distance(mm)	33	32	31	30	29	28	27	26	25	24	23
Main Antenna	23.2	23.2	23.2	23.1	23.01	/	/	/	/	/	/

Based on the most conservative measured triggering distance of 28 mm, additional SAR measurements were required at 27 mm from the Rear side for the above modes.



## ANNEX K Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole D835V2– serial no.4d057

Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2018-10-09	-27.7	/	49.6	/	-4.08	/
2019-10-06	-26.9	2.9	50.1	0.5	-3.95	0.13

Justification of Extended Calibration SAR Dipole D2450V2– serial no. 873

Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2018-10-26	-28.0	/	53.5	/	2.11	/
2019-10-22	-27.3	2.5	54.4	0.9	2.29	0.18

Justification of Extended Calibration SAR Dipole D2550V2– serial no.1010

Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2018-08-24	-25.7	/	54.9	/	-2.30	/
2019-08-22	-24.8	3.5	55.8	0.9	-2.22	0.08

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended.