

FCC 47 CFR PART 15 SUBPART C AND ANSI C63.10: 2013

TEST REPORT

For

Fall Sensor

Model: FS315-IC

Brand: 

Issued to

Instant Care, Inc.
2080 Wineridge PL, Suite A, Escondido, CA 92029

Issued by

Compliance Certification Services Inc.
Tainan Lab.

No.8, Jiucengling, Xinhua Dist., Tainan City 712, Taiwan (R.O.C.)

TEL: (06) 580-2201
FAX: (06) 580-2202

Issued Date: May 25, 2018



Note: This report shall not be reproduced except in full, without the written approval of Compliance Certification Services Inc. This document may be altered or revised by Compliance Certification Services Inc. personnel only, and shall be noted in the revision section of the document.

Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Compliance Certification Services Inc.

No.8, Jiucengling, Xinhua Dist., Tainan City 712, Taiwan (R.O.C.)
t (886) 6-580-2201 f (886) 6-580-2202

www.ccsrf.com

Member of SGS Group

REVISION HISTORY

Rev.	Issue Date	Revisions	Effect Page	Revised By
00	May 15, 2018	Initial Issue	ALL	Gina Lin
01	May 25, 2018	See the following note rev.01	ALL	Gina Lin

Note:

- ※ Rev.00 Issue Date : May 15, 2018 T180503N01-RP1
Original Report
- ※ Rev.01 Issue Date : May 25, 2018 T180503N01-RP1
Update SUPPORT EQUIPMENT.

TABLE OF CONTENTS

1. TEST RESULT CERTIFICATION	4
2. EUT DESCRIPTION.....	5
3. TEST METHODOLOGY.....	6
3.1 EUT CONFIGURATION.....	6
3.2 EUT EXERCISE.....	6
3.3 GENERAL TEST PROCEDURES	6
3.4 FCC PART 15.205 RESTRICTED BANDS OF OPERATIONS	7
3.5 DESCRIPTION OF TEST MODES	7
4. INSTRUMENT CALIBRATION	8
4.1 MEASURING INSTRUMENT CALIBRATION.....	8
4.2 MEASUREMENT EQUIPMENT USED.....	8
4.3 MEASUREMENT UNCERTAINTY	9
5. FACILITIES AND ACCREDITATIONS	10
5.1 FACILITIES.....	10
5.2 EQUIPMENT.....	10
5.3 TABLE OF ACCREDITATIONS AND LISTINGS	10
5.4 TABLE OF ACCREDITATIONS AND LISTINGS	11
6. SETUP OF EQUIPMENT UNDER TEST	12
6.1 SETUP CONFIGURATION OF EUT.....	12
6.2 SUPPORT EQUIPMENT	12
7. FCC PART 15.231 REQUIREMENTS	13
7.1 20 DB BANDWIDTH	13
7.2 LIMIT OF TRANSMISSION TIME.....	15
7.3 DUTY CYCLE	18
7.4 CENTRAL FREQUNCY	21
7.5 RADIATED EMISSIONS.....	23
7.6 POWERLINE CONDUCTED EMISSIONS	33
8. APPENDIX 1 PHOTOGRAPHS OF TEST SETUP	34

1. TEST RESULT CERTIFICATION

Product: Fall Sensor

Model: FS315-IC

Brand Name: The logo for Instant Care, featuring the word "Instant" in blue and "Care" in pink, with a small heart icon above the "i" in "Instant".

Applicant: Instant Care, Inc.

2080 Wineridge PL, Suite A, Escondido, CA 92029

Tested: April 17, 2018 ~ May 14, 2018


APPLICABLE STANDARDS	
STANDARD	TEST RESULT
FCC 47 CFR Part 15 Subpart C ANSI C63.10: 2013	No non-compliance noted

We hereby certify that:

The above equipment was tested by Compliance Certification Services Inc. The test data, data evaluation, test procedures, and equipment configurations shown in this report were made in accordance with the procedures given in ANSI C63.10: 2013 and the energy emitted by the sample EUT tested as described in this report is in compliance with conducted and radiated emission limits of FCC Rules Part 15.207, 15.209 and Part 15.231.


The test results of this report relate only to the tested sample identified in this report.

Approved by:

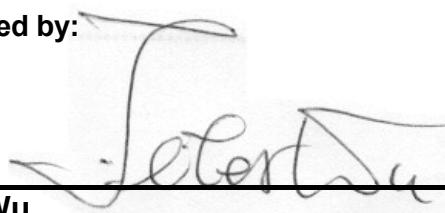A handwritten signature in black ink that appears to read "Jeter Wu".

Jeter Wu
Assistant Manager

Reviewed by:

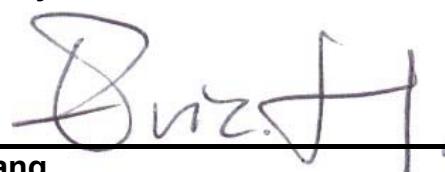A handwritten signature in black ink that appears to read "Eric Huang".

Eric Huang
Section Manager

2. EUT DESCRIPTION

Product	Fall Sensor
Model Number	FS315-IC
Brand Name	
Received Date	May 04, 2018
Frequency Range	315MHz ± 40kHz
Number of Channels	1 Channel
Type of Modulation	ASK
Power Supply	3Vdc (Powered from battery)
Antenna Type	Type: PCB Antenna Model: FS315-IC Manufacturer: Maxim Gain: -22dBi
RF Module Model	MAX7044
Software Version	V1
Hardware Version	V1
Temperature Range	-20 °C ~ +60 °C

Remark:

1. Client consigns only one model sample to test (Model Number: **FS315-IC**). Therefore, the testing Lab. just guarantees the unit, which has been tested.
2. This submittal(s) (test report) is intended for FCC ID: **XO8-IC315FS-1** filing to comply with Section 15.207, 15.209 and 15.231 of the FCC Part 15, Subpart C Rules.

3. TEST METHODOLOGY

The tests documented in this report were performed in accordance with ANSI C63.10 (2013) and FCC CFR 47 15.207, 15.209 and 15.231

3.1 EUT CONFIGURATION

The EUT configuration for testing is installed on RF field strength measurement to meet the Commissions requirement and operating in a manner that intends to maximize its emission characteristics in a continuous normal application.

3.2 EUT EXERCISE

The EUT was operated in the engineering mode to fix the TX frequency that was for the purpose of the measurements.

3.3 GENERAL TEST PROCEDURES

Conducted Emissions

The EUT is placed on the turntable, which is 0.8 m above ground plane. According to the requirements in Section 13.1.4.1 of ANSI C63.10. Conducted emissions from the EUT measured in the frequency range between 0.15 MHz and 30MHz using CISPR Quasi-peak and average detector modes.

Radiated Emissions

The EUT is placed on a turn table, which is 0.8 m above ground plane. The turntable shall rotate 360 degrees to determine the position of maximum emission level. EUT is set 3m away from the receiving antenna, which varied from 1m to 4m to find out the highest emission. And also, each emission was to be maximized by changing the polarization of receiving antenna both horizontal and vertical. In order to find out the maximum emissions, exploratory radiated emission measurements were made according to the requirements in Section 13.1.4.1 of ANSI C63.10.

3.4 FCC PART 15.205 RESTRICTED BANDS OF OPERATIONS

(a) Except as shown in paragraph (d) of this section, only spurious emissions are permitted in any of the frequency bands listed below:

MHz	MHz	MHz	GHz
0.090 □ 0.110	16.42 - 16.423	399.9 - 410	4.5 - 5.15
¹ 0.495 □ 0.505	16.69475 - 16.69525	608 - 614	5.35 - 5.46
2.1735 □ 2.1905	16.80425 - 16.80475	960 - 1240	7.25 - 7.75
4.125 - 4.128	25.5 - 25.67	1300 - 1427	8.025 - 8.5
4.17725 - 4.17775	37.5 - 38.25	1435 - 1626.5	9.0 - 9.2
4.20725 - 4.20775	73 - 74.6	1645.5 - 1646.5	9.3 - 9.5
6.215 - 6.218	74.8 - 75.2	1660 - 1710	10.6 - 12.7
6.26775 - 6.26825	108 - 121.94	1718.8 - 1722.2	13.25 - 13.4
6.31175 - 6.31225	123 - 138	2200 - 2300	14.47 - 14.5
8.291 - 8.294	149.9 - 150.05	2310 - 2390-	15.35 - 16.2
8.362 □ 8.366	156.52475 -	2483.5 - 2500	17.7 - 21.4
8.37625 - 8.38675	156.52525	2655 - 2900	22.01 - 23.12
8.41425 - 8.41475	156.7 - 156.9	3260 - 3267	23.6 - 24.0
12.29 - 12.293	162.0125 - 167.17	3332 - 3339	31.2 - 31.8
12.51975 - 12.52025	167.72 - 173.2	3345.8 - 3358	36.43 - 36.5
12.57675 - 12.57725	240 - 285	3600 - 4400	(²)
13.36 □ 13.41	322 - 335.4		

¹ Until February 1, 1999, this restricted band shall be 0.490-0.510 MHz.

² Above 38.6

(b) Except as provided in paragraphs (d) and (e), the field strength of emissions appearing within these frequency bands shall not exceed the limits shown in Section 15.209. At frequencies equal to or less than 1000 MHz, compliance with the limits in Section 15.209 shall be demonstrated using measurement instrumentation employing a CISPR quasi-peak detector. Above 1000 MHz, compliance with the emission limits in Section 15.209 shall be demonstrated based on the average value of the measured emissions. The provisions in Section 15.35 apply to these measurements.

3.5 DESCRIPTION OF TEST MODES

The EUT (Model: **FS315-IC**) had been tested under engineering test mode condition and the EUT staying in continuous transmitting mode.

Note :

- 1) The field strength of spurious emission was measured in the following position: EUT have three test modes(X, Y, Z axis).The worst emission was found in X axis and the worst case was recorded.

4. INSTRUMENT CALIBRATION

4.1 MEASURING INSTRUMENT CALIBRATION

The measuring equipment, which was utilized in performing the tests documented herein, has been calibrated in accordance with the manufacturer's recommendations for utilizing calibration equipment, which is traceable to recognized national standards.

4.2 MEASUREMENT EQUIPMENT USED

Equipment Used for Emissions Measurement

Chamber 966				
Name of Equipment	Manufacturer	Model	Serial Number	Calibration Due
Active Loop Antenna	ETS-LINDREN	6502	8905-2356	07/19/2019
Amplifier	HP	8447F	2443A01671	01/21/2019
Bi-Log Antenna	Sunol	JB1	A070506-2	02/08/2019
Cable	Rosnol+Suhner	SUCOFLEX 104PEA	SN25737 /4PEA	01/26/2019
Double Ridged Guide Horn Antenna	ETS-LINDGREN	3116	00078900	03/19/2019
EMI Test Receiver	R&S	ESCI	100782	06/11/2018
EXA Spectrum Analyzer	KEYSIGHT	N9010A	MY54430216	05/08/2019
Horn Antenna	Com-Power	AH-118	071032	04/18/2019
Pre-Amplifier	EMCI	EMC012645	980098	01/21/2019
Software	Excel			

Remark: Each piece of equipment is scheduled for calibration once a year.

4.3 MEASUREMENT UNCERTAINTY

Parameter	Uncertainty
Radiated Emission, 30 to 200 MHz Test Site : OATS-6	±3.3456dB
Radiated Emission, 200 to 1000 MHz Test Site : OATS-6	±2.6828dB
Radiated Emission, 1 to 8 GHz	± 2.6485dB
Radiated Emission, 8 to 18 GHz	± 2.6852dB
Radiated Emission, 18 to 26.5 GHz	± 2.6485dB
Radiated Emission, 26 to 40 GHz	± 3.0295dB
Power Line Conducted Emission	±1.91dB
Band Width	136.49kHz
Peak Output Power MU	±1.904dB
Band Edge MU	±0.302dBuV
Channel Separation MU	361.69Hz
Duty Cycle MU	0.064ms
Frequency Stability MU	0.223kHz

Uncertainty figures are valid to a confidence level of 95%, k=2

5. FACILITIES AND ACCREDITATIONS

5.1 FACILITIES

All measurement facilities used to collect the measurement data are located at

No.8, Jiucengling, Xinhua Dist., Tainan City 712, Taiwan (R.O.C.)

The sites are constructed in conformance with the requirements of ANSI C63.7:1992, ANSI C63.10: 2013 and CISPR Publication 22.

5.2 EQUIPMENT

Radiated emissions are measured with one or more of the following types of linearly polarized antennas: tuned dipole, biconical, log periodic, bi-log, and/or ridged waveguide, horn. Spectrum analyzers with pre-selectors and quasi-peak detectors are used to perform radiated measurements.

Conducted emissions are measured with Line Impedance Stabilization Networks and EMI Test Receivers.

Calibrated wideband preamplifiers, coaxial cables, and coaxial attenuators are also used for making measurements.

All receiving equipment conforms to CISPR Publication 16-1, "Radio Interference Measuring Apparatus and Measurement Methods."

5.3 TABLE OF ACCREDITATIONS AND LISTINGS

The test facilities used to perform radiated and conducted emissions tests are accredited by Taiwan Accreditation Foundation for the specific scope of accreditation under Lab Code: 1109 to perform Electromagnetic Interference tests according to FCC PART 15 AND CISPR 22 requirements. No part of this report may be used to claim or imply product endorsement by TAF or any agency of the Government. In addition, the test facilities are listed with Federal Communications Commission (registration no: TW1109).

5.4 TABLE OF ACCREDITATIONS AND LISTINGS

Our laboratories are accredited and approved by the following accreditation body according to ISO/IEC 17025.

Taiwan TAF

The measuring facility of laboratories has been authorized or registered by the following approval agencies.

Canada	Industry Canada
Germany	TUV NORD
Taiwan	BSMI
USA	FCC

Copies of granted accreditation certificates are available for downloading from our web site, <http://www.ccsrf.com>

6. SETUP OF EQUIPMENT UNDER TEST

6.1 SETUP CONFIGURATION OF EUT

See test photographs attached in Appendix I for the actual connections between EUT and support equipment.

6.2 SUPPORT EQUIPMENT

[EMC test]

No.	Product	Manufacturer	Model No.	Certify No.	Signal cable
1	N/A	---	---	---	---

No.	Signal cable description	
A	N/A	---

[RF test]

No.	Product	Manufacturer	Model No.	Certify No.	Signal cable
1	N/A	---	---	---	---

No.	Signal cable description	
A	N/A	---

Remark:

1. All the equipment/cables were placed in the worst-case configuration to maximize the emission during the test.
2. Grounding was established in accordance with the manufacturer's requirements and conditions for the intended use.

7. FCC PART 15.231 REQUIREMENTS

7.1 20 DB BANDWIDTH

LIMIT


The bandwidth of the emission shall be no wider than 0.25% of the center frequency for devices operating above 70 MHz and below 900 MHz. For devices operating above 900 MHz, the emission shall be no wider than 0.5% of the center frequency. Bandwidth is determined at the points 20 dB down from the modulated carrier.

MEASUREMENT EQUIPMENT USED

Name of Equipment	Manufacturer	Model	Serial Number	Calibration Due
EXA Spectrum Analyzer	KEYSIGHT	N9010A	MY54430216	05/08/2019

Remark: Each piece of equipment is scheduled for calibration once a year.

TEST CONFIGURATION

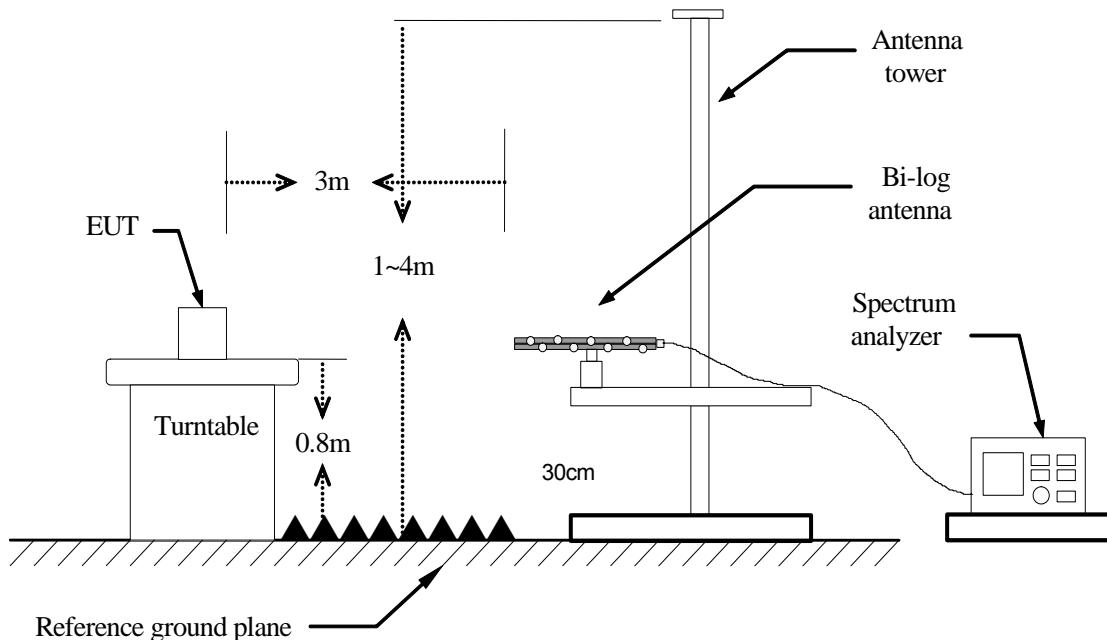

TEST PROCEDURE

The spectrum analyzer center frequency is set to the transmitter frequency. The RBW is set to 3 kHz and VBW is set 10kHz.


TEST RESULTS

No non-compliance noted.

TEST DATA

Frequency (MHz)	20dB Bandwidth (KHz)	Limit (KHz)	Result
315	7.7	787.5	PASS

Test Plot

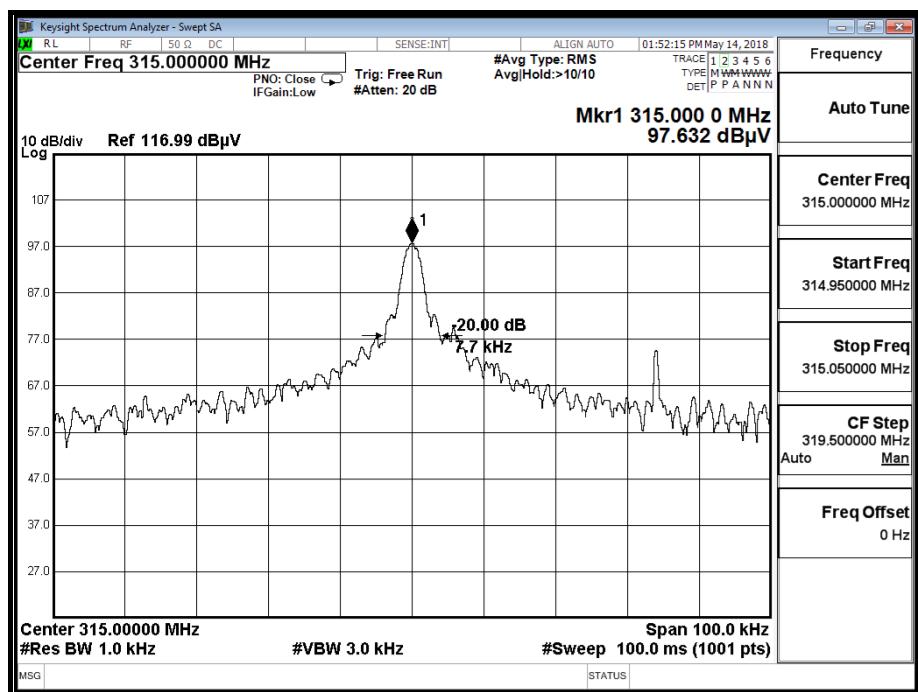

7.2 LIMIT OF TRANSMISSION TIME

LIMIT


According to 15.231, a manually operated transmitter shall employ a switch that will automatically deactivate the transmitter within not more than 5 seconds of being released.

MEASUREMENT EQUIPMENT USED

Name of Equipment	Manufacturer	Model	Serial Number	Calibration Due
EXA Spectrum Analyzer	KEYSIGHT	N9010A	MY54430216	05/08/2019

Remark: Each piece of equipment is scheduled for calibration once a year.

TEST CONFIGURATION

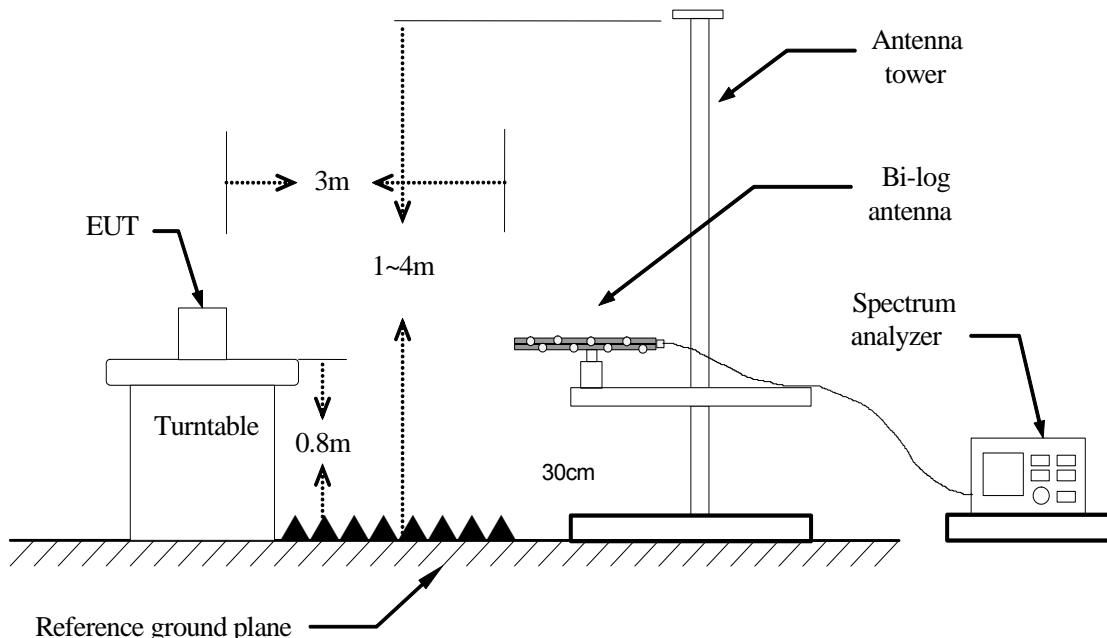

TEST PROCEDURE

The spectrum analyzer center frequency is set to the transmitter frequency. The RBW = 100kHz and VBW = 300kHz.


TEST RESULTS

No non-compliance noted.

TEST DATA

Frequency (MHz)	Transmission Time (s)	Limit (Second)	Result
315	1.6	5	PASS

Test Plot
5s

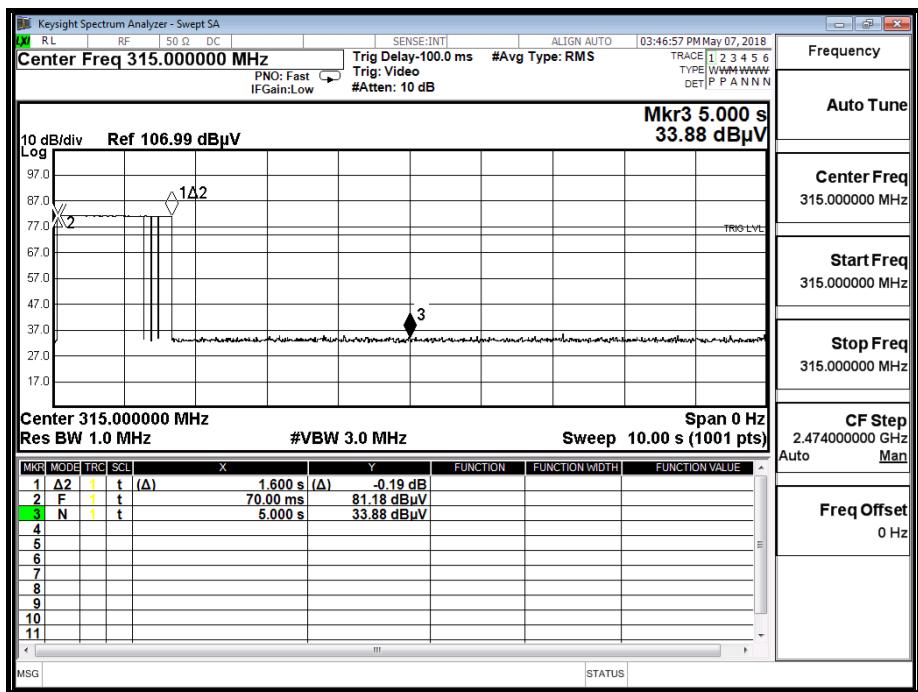

7.3 DUTY CYCLE

LIMIT


Nil (No dedicated limit specified in the Rules)

MEASUREMENT EQUIPMENT USED

Name of Equipment	Manufacturer	Model	Serial Number	Calibration Due
EXA Spectrum Analyzer	KEYSIGHT	N9010A	MY54430216	05/08/2019

Remark: Each piece of equipment is scheduled for calibration once a year.

TEST CONFIGURATION

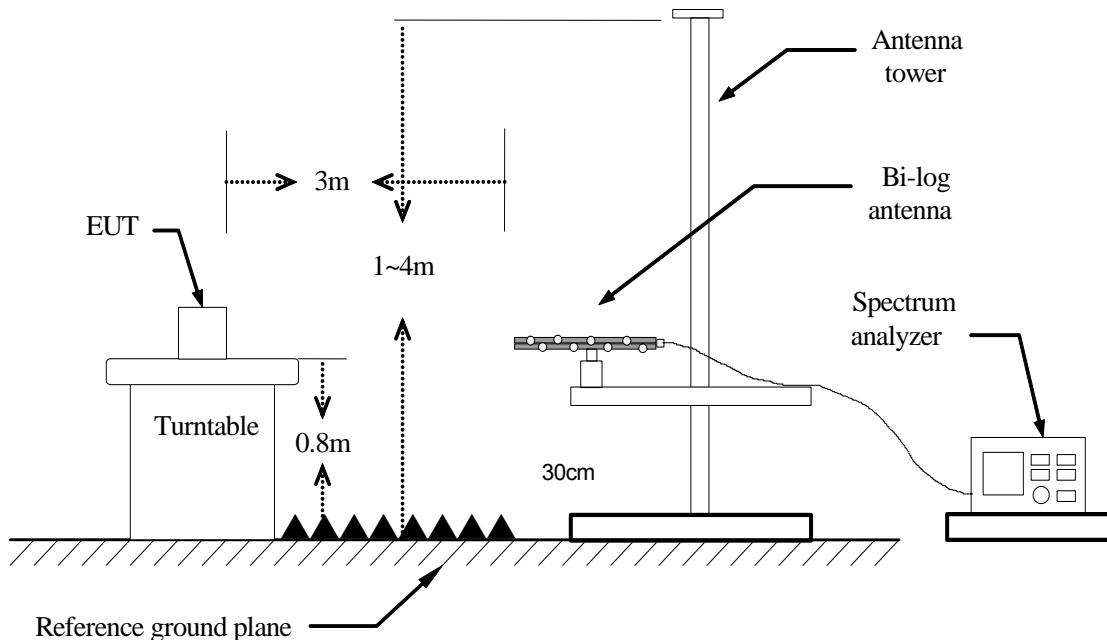

TEST PROCEDURE

1. Place the EUT on the table and set it in transmitting mode.
2. Set center frequency of spectrum analyzer = operating frequency.
3. Set the spectrum analyzer as RBW, VBW=100KHz, Span = 0Hz, a suitable Sweep Time.
4. Repeat above procedures until all frequency measured were complete.

TEST RESULTS

No non-compliance noted.

TEST DATA

	us	Times	Ton	Total Ton time(ms)
Ton1	498.000	17	8466.000	8.541
Ton2	5.000	15	75.000	
Ton3		0	0.000	
Tp				100.000


Ton	8.541
Tp(Ton+Toff)	100.000
Duty Cycle	0.085
Duty Factor	-20.000

8.541 %


Limit of bandwidth	F(MHz)*0.25% = X(kHz)
(MHz)	(k'Hz)
319.5	787.50

Test Plot


Ton1

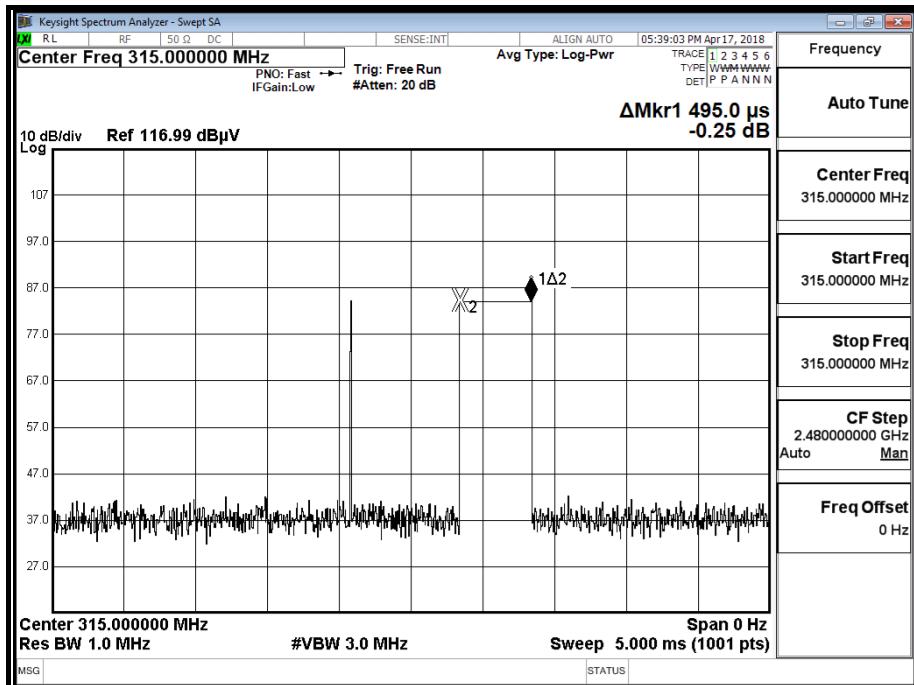

Ton2

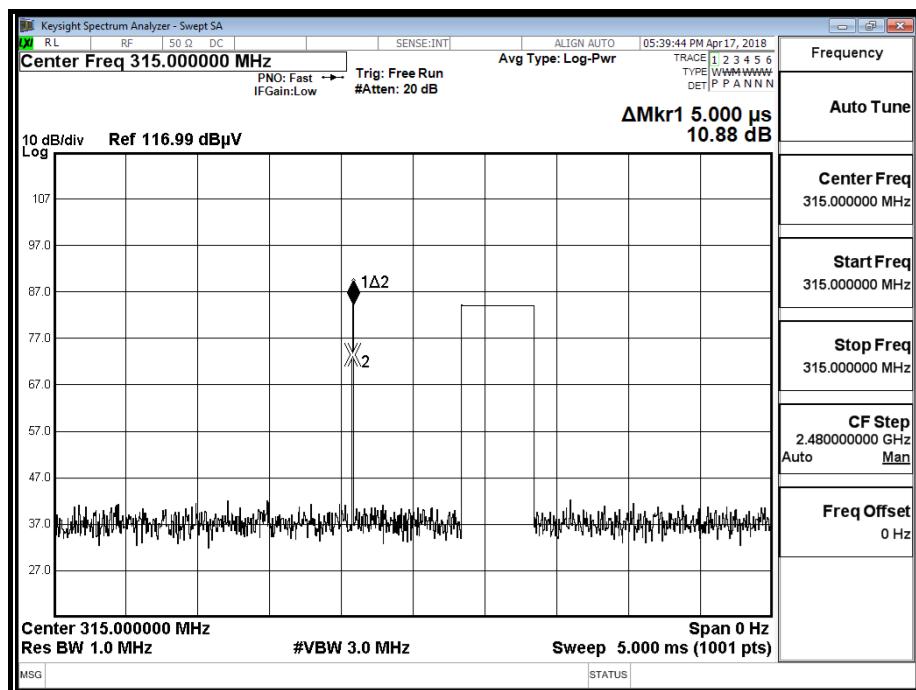

Tp

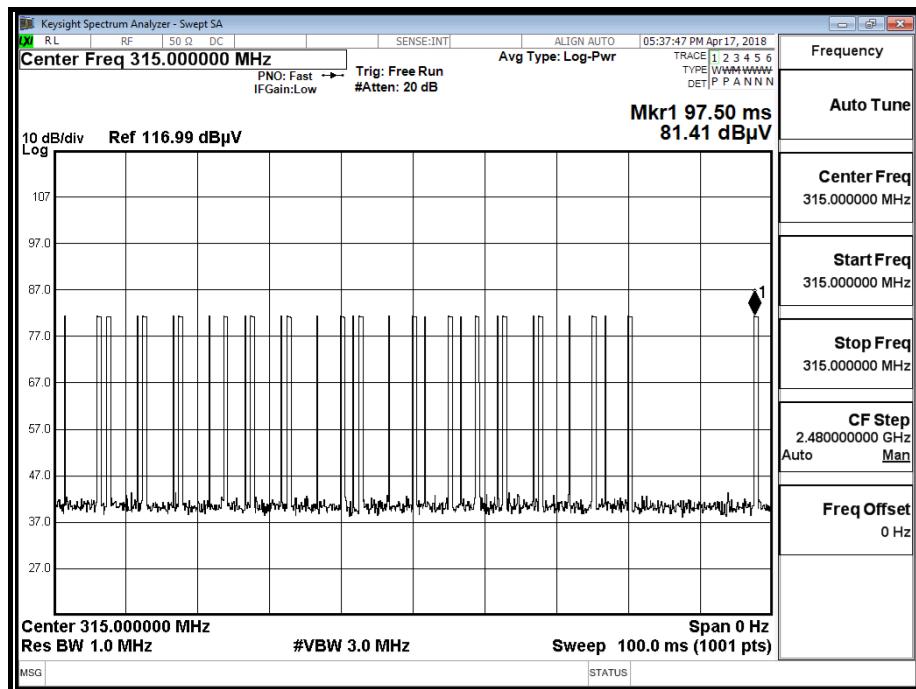


7.4 CENTRAL FREQUENCY

MEASUREMENT EQUIPMENT USED

Name of Equipment	Manufacturer	Model	Serial Number	Calibration Due
EXA Spectrum Analyzer	KEYSIGHT	N9010A	MY54430216	05/08/2019

Remark: Each piece of equipment is scheduled for calibration once a year.

TEST CONFIGURATION

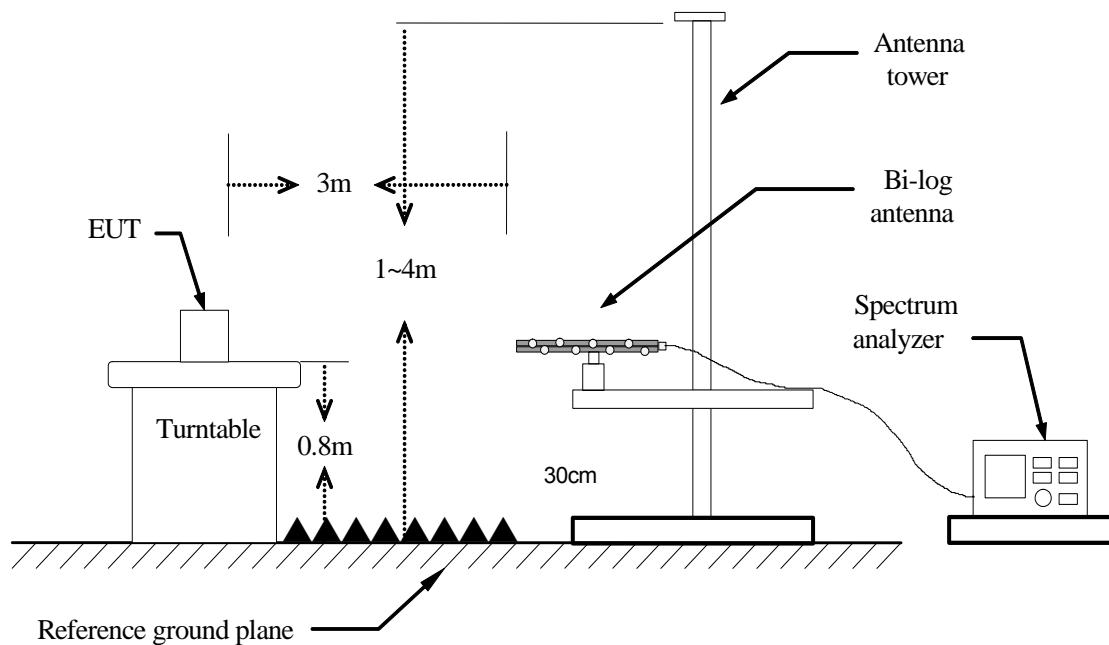

TEST PROCEDURE

The spectrum analyzer center frequency is set to the transmitter frequency. The RBW=3kHz and VBW=10kHz.

TEST RESULTS

No non-compliance noted.

TEST DATA

Frequency (MHz)	Central Frequency (MHz)	Frequency Error (MHz)
315	315	0

7.5 RADIATED EMISSIONS

LIMIT

1. Except as provided elsewhere in this Subpart, the emissions from an intentional radiator shall not exceed the field strength levels specified in the following table:

Frequency (MHz)	Field Strength (mV/m)	Field Strength (dB μ V/m at 3-meter)	Measurement Distance (m)
30-88	100*	40	3
88-216	150*	43.5	3
216-960	200*	46	3
Above 960	500	54	3

Remark: Except as provided in paragraph (g), fundamental emissions from intentional radiators operating under this Section shall not be located in the frequency bands 54□72 MHz, 76□88 MHz, 174□216 MHz or 470□806 MHz. However, operation within these frequency bands is permitted under other sections of this Part, e.g., Sections 15.231 and 15.241.

2. For intentional device, according to § 15.231, the general requirement of field strength of radiated emissions from intentional radiators at a distance of 3 meters shall not exceed the following table.

Fundamental Frequency (MHz)	Field Strength of Fundamental (μ V/M)	Field Strength of Spurious Emission
40.66-40.70	2250	225
70-130	1250	125
130-174	1250 to 3750**	125 to 375**
174-260	3750	375
260-470	3750 to 12500**	375 to 1250**
Above 470	12500	1250

Note :

1. “ ** ” linear interpolations.
2. Where F is the frequency in MHz, the formulas for calculating the maximum permitted fundamental field strengths are as follows: for the band 130-174 MHz, μ V/m at 3 meters = $56.81818(F) - 6136.3636$; for the band 260-470 MHz, μ V/m at 3 meters = $41.6667(F) - 7083.3333$. The maximum permitted unwanted emission level is 20 dB below the maximum permitted fundamental level.


MEASUREMENT EQUIPMENT USED

Chamber 966				
Name of Equipment	Manufacturer	Model	Serial Number	Calibration Due
Active Loop Antenna	ETS-LINDREN	6502	8905-2356	07/19/2019
Amplifier	HP	8447F	2443A01671	01/21/2019
Bi-Log Antenna	Sunol	JB1	A070506-2	02/08/2019
Cable	Rosnol+Suhner	SUCOFLEX 104PEA	SN25737 /4PEA	01/26/2019
Double Ridged Guide Horn Antenna	ETS-LINDGREN	3116	00078900	03/19/2019
EMI Test Receiver	R&S	ESCI	100782	06/11/2018
EXA Spectrum Analyzer	KEYSIGHT	N9010A	MY54430216	05/08/2019
Horn Antenna	Com-Power	AH-118	071032	04/18/2019
Pre-Amplifier	EMCI	EMC012645	980098	01/21/2019
Software	Excel			


Remark: Each piece of equipment is scheduled for calibration once a year.

Test Configuration

Below 1 GHz

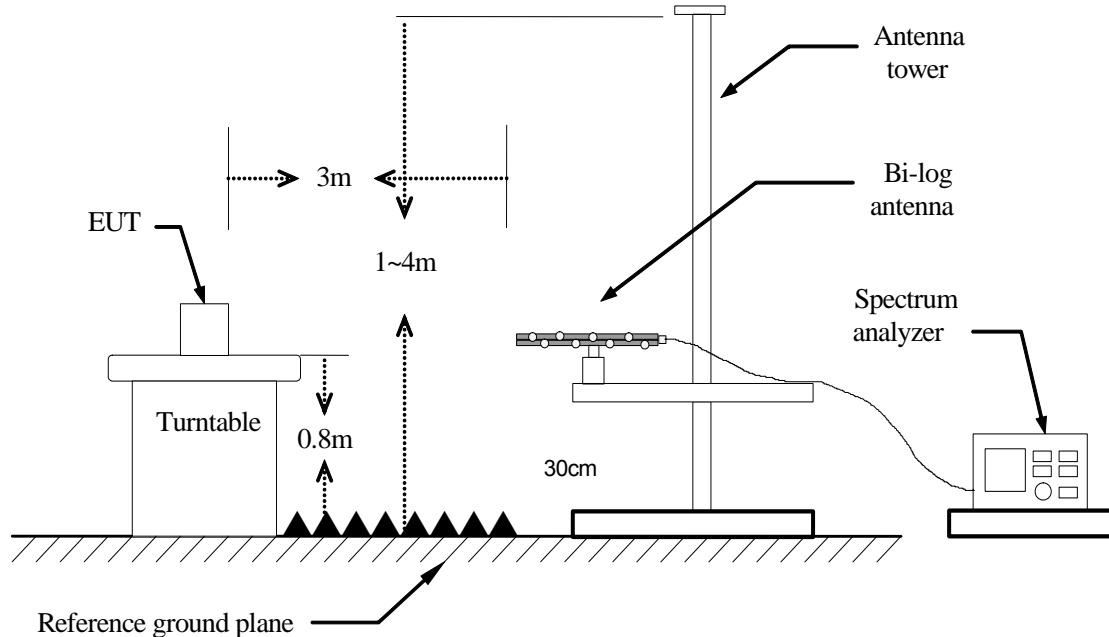

Above 1 GHz

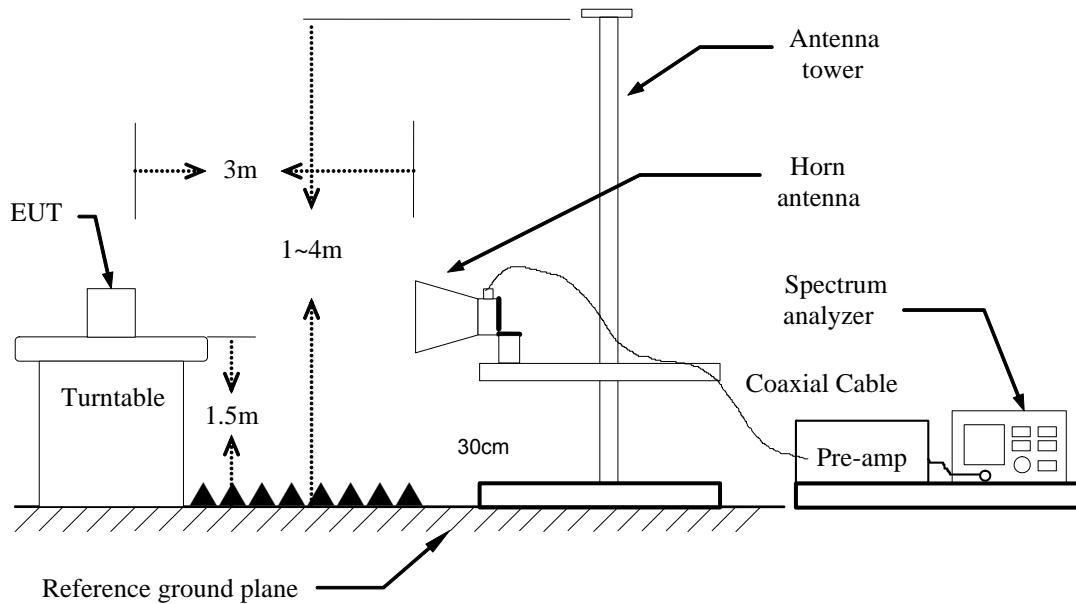

TEST PROCEDURE

1. The EUT is placed on a turntable, which is 0.8m/1.5m above ground plane.
2. The turntable shall be rotated for 360 degrees to determine the position of maximum emission level.
3. EUT is set 3m away from the receiving antenna, which is varied from 1m to 4m to find out the highest emissions.
4. Maximum procedure was performed on the six highest emissions to ensure EUT compliance.
5. And also, each emission was to be maximized by changing the polarization of receiving antenna both horizontal and vertical.
6. Set the spectrum analyzer in the following setting as:

Below 1GHz:

RBW=100kHz / VBW=300kHz / Sweep=AUTO

Above 1GHz:

- (a) PEAK: RBW=VBW=1MHz / Sweep=AUTO
- (b) AVERAGE: PEAK + DUTY FACTOR

7. Repeat above procedures until the measurements for all frequencies are complete.
8. No emission is found between lowest internal used/generated frequency to 30MHz (9kHz~30MHz)

TEST RESULTS

Below 1 GHz

Operation Mode: Normal Operation

Test Date: 2018/05/14


Temperature: 26.8 °C

Tested by: Ted Huang

Humidity: 52% RH

Polarity: Ver. / Hor.

Horizontal

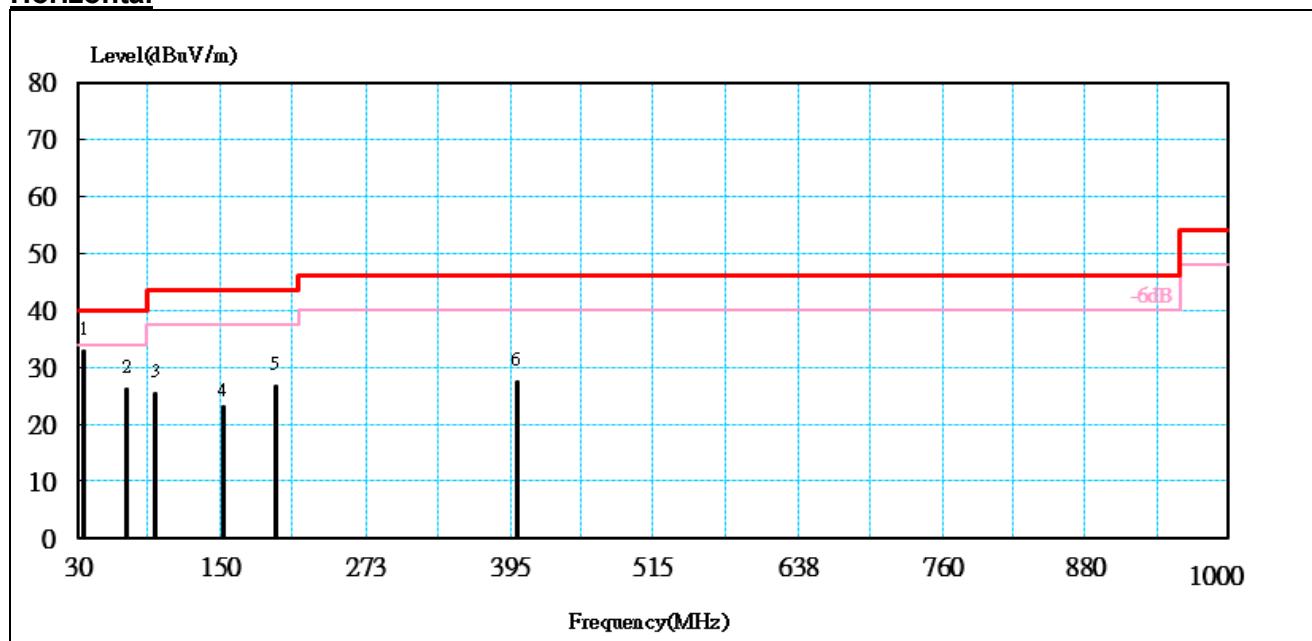

No.	Freq-Uency	Meter Reading at 3 m Level	Antenna Factor	Cable Loss	Emission at 3 m Level	Limits	Margin	Detector Mode
	(MHz)	(dB μ V)	(dB/m)	(dB)	(dB μ V/m)	(dB μ V/m)	(dB)	PK/QP
1	35.23	13.76	18.32	0.84	32.91	40.00	-7.09	QP
2	71.56	16.44	8.62	1.17	26.23	40.00	-13.77	QP
3	95.67	14.73	9.23	1.42	25.38	43.50	-18.12	QP
4	152.28	8.56	12.75	1.89	23.20	43.50	-20.30	QP
5	196.78	11.64	12.88	2.23	26.75	43.50	-16.75	QP
6	400.68	7.55	16.11	3.94	27.60	46.00	-18.40	QP

Remark:

1. No emission found between lowest internal used/generated frequency to 30MHz (9kHz~30MHz).
2. Radiated emissions measured in frequency range from 30 MHz to 1000MHz were made with an instrument using peak/quasi-peak detector mode.
3. Quasi-peak test would be performed if the peak result were greater than the quasi-peak limit or as required by the applicant.
4. Measurements above show only up to 6 maximum emissions noted, or would be lesser, with " N/A " remark, if no specific emissions from the EUT are recorded (ie: margin>20dB from the applicable limit) and considered that's already beyond the background noise floor.
5. Margin (dB) = Remark result (dB μ V/m) – Quasi-peak limit (dB μ V/m).
6. That the limit for signals below 1GHz is a QP limit and peak readings are below the QP limit.
7. The fundamental signal is not shown in the test data because measurements at fundamental frequency are shown separately and were ignored during the 30 – 1000 MHz scan.

Operation Mode: Normal Operation


Test Date: 2018/05/14

Temperature: 26.8 °C

Tested by: Ted Huang

Humidity: 52% RH

Polarity: Ver. / Hor.

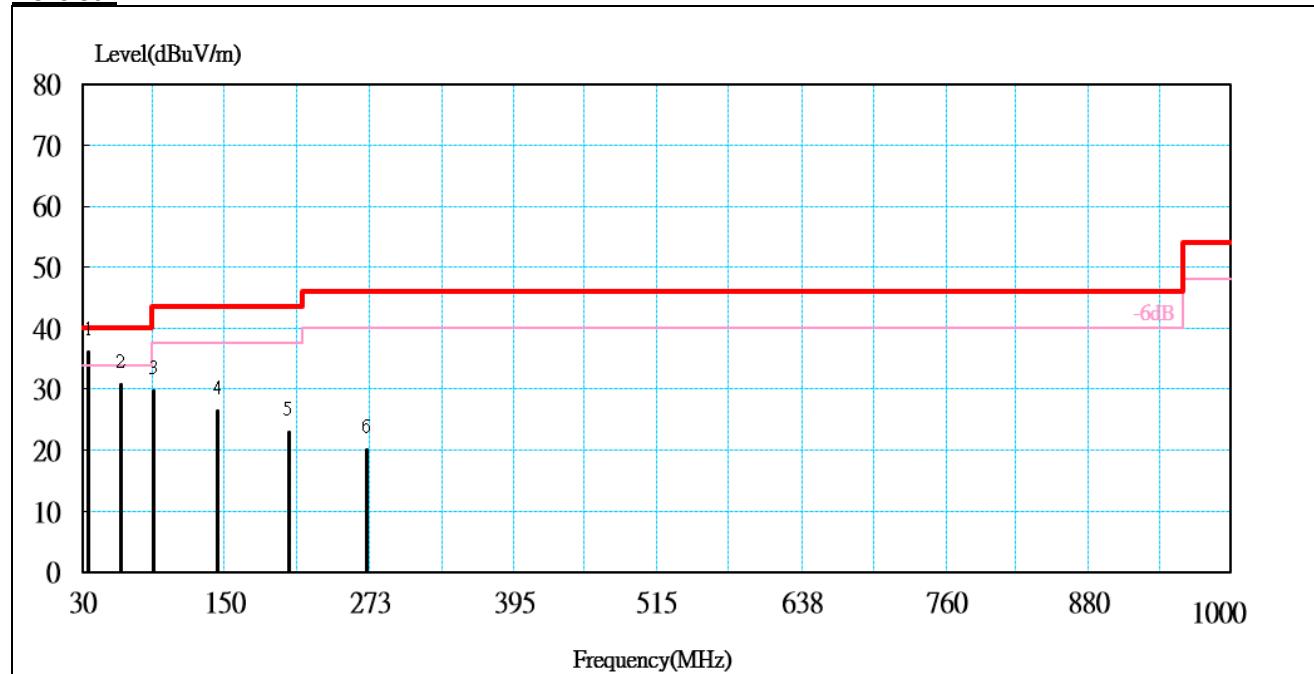Vertical


No.	Freq-Uency	Meter Reading at 3 m Level	Antenna Factor	Cable Loss	Emission at 3 m Level	Limits	Margin	Detector Mode
	(MHz)	(dB _u V)	(dB/m)	(dB)	(dB _u V/m)	(dB _u V/m)	(dB)	PK/QP
1	35.28	17.06	18.28	0.84	36.17	40.00	-3.83	QP
2	62.43	21.67	8.09	1.11	30.88	40.00	-9.12	QP
3	90.85	20.48	7.93	1.39	29.80	43.50	-13.70	QP
4	144.15	11.48	13.27	1.82	26.57	43.50	-16.93	QP
5	204.72	7.55	13.22	2.29	23.06	43.50	-20.44	QP
6	270.28	4.16	13.11	2.81	20.08	46.00	-25.92	QP

Remark:

1. No emission found between lowest internal used/generated frequency to 30MHz (9kHz~30MHz).
2. Radiated emissions measured in frequency range from 30 MHz to 1000MHz were made with an instrument using peak/quasi-peak detector mode.
3. Quasi-peak test would be performed if the peak result were greater than the quasi-peak limit or as required by the applicant.
4. Measurements above show only up to 6 maximum emissions noted, or would be lesser, with " N/A " remark, if no specific emissions from the EUT are recorded (ie: margin>20dB from the applicable limit) and considered that's already beyond the background noise floor.
5. Margin (dB) = Remark result (dB_uV/m) – Quasi-peak limit (dB_uV/m).
6. That the limit for signals below 1GHz is a QP limit and peak readings are below the QP limit.
7. The fundamental signal is not shown in the test data because measurements at fundamental frequency are shown separately and were ignored during the 30 – 1000 MHz scan.

The fundamental signal

Operation Mode: TX **Test Date:** 2018/04/17
Temperature: 26.4°C **Tested by:** Ted Huang
Humidity: 45% RH **Polarity:** Ver. / Hor.

Horizontal

Measurement Distance at 3m							Horizontal polarity		
Freq.	Reading	AF	Closs	Pre-amp	Filter	Level	Limit	Margin	Mark
(MHz)	(dB μ V)	(dB μ V)	(dB)	(dB)	(dB)	(dB μ V/m)	(dB μ V/m)	(dB)	(P/Q/A)
315.00	102.60	14.32	3.21	26.67	0.00	93.46	95.62	-2.17	P
315.00	82.60	14.32	3.21	26.67	0.00	73.46	75.62	-2.17	A

Vertical

Measurement Distance at 3m							Vertical polarity		
Freq.	Reading	AF	Closs	Pre-amp	Filter	Level	Limit	Margin	Mark
(MHz)	(dB μ V)	(dB μ V)	(dB)	(dB)	(dB)	(dB μ V/m)	(dB μ V/m)	(dB)	(P/Q/A)
315.00	90.83	14.32	3.21	26.67	0.00	81.69	95.62	-13.94	P
315.00	70.83	14.32	3.21	26.67	0.00	61.69	75.62	-13.94	A

Remark:

Margin (dB) = Remark result (dB μ V/m) – Quasi-peak limit (dB μ V/m).

Harmonic

Operation Mode:	TX	Test Date:	2018/04/17
Temperature:	26.4 °C	Tested by:	Ted Huang
Humidity:	45% RH	Polarity:	Ver. / Hor.

Horizontal

		Measurement Distance at 3m			Horizontal polarity				
Freq. (MHz)	Reading (dB μ V)	AF (dB μ V)	Closs (dB)	Pre-amp (dB)	Filter (dB)	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Mark (P/Q/A)
630.00	55.80	19.66	5.44	25.87	0.00	55.02	75.62	-20.60	P
630.00	35.80	19.66	5.44	25.87	0.00	35.02	55.62	-20.60	A
945.01	43.48	22.96	6.82	25.64	0.00	47.63	75.62	-28.00	P
945.01	23.48	22.96	6.82	25.64	0.00	27.63	55.62	-28.00	A

Vertical

		Measurement Distance at 3m			Vertical polarity				
Freq. (MHz)	Reading (dB μ V)	AF (dB μ V)	Closs (dB)	Pre-amp (dB)	Filter (dB)	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Mark (P/Q/A)
630.00	42.68	19.66	5.44	25.87	0.00	41.91	75.62	-33.72	P
630.00	22.68	19.66	5.44	25.87	0.00	21.91	55.62	-33.72	A
945.02	44.37	22.96	6.82	25.64	0.00	48.51	75.62	-27.11	P
945.02	24.37	22.96	6.82	25.64	0.00	28.51	55.62	-27.11	A

Remark:

Margin (dB) = Remark result (dB μ V/m) – Quasi-peak limit (dB μ V/m).

Above 1 GHz

Operation Mode:	TX	Test Date:	2018/04/17
Temperature:	26.4 °C	Tested by:	Ted Huang
Humidity:	45% RH	Polarity:	Ver. / Hor.

Horizontal

Freq. (MHz)	Reading (dBμV)	AF (dBμV)	Closs (dB)	Pre-amp (dB)	Filter (dB)	Level (dBμV/m)	Limit (dBμV/m)	Margin (dB)	Mark (P/Q/A)
1260.11	62.39	25.64	2.10	45.22	1.19	46.10	75.62	-29.52	P
1260.11	42.39	25.64	2.10	45.22	1.19	26.10	55.62	-29.52	A
* 1575.10	65.01	27.17	2.37	44.97	0.76	50.34	74.00	-23.66	P
* 1575.10	45.01	27.17	2.37	44.97	0.76	30.34	54.00	-23.66	A
1889.82	66.05	29.56	2.60	44.78	0.50	53.94	75.62	-21.69	P
1889.82	46.05	29.56	2.60	44.78	0.50	33.94	55.62	-21.69	A
* 2205.36	63.46	30.24	2.79	44.62	0.41	52.28	74.00	-21.72	P
* 2205.36	43.46	30.24	2.79	44.62	0.41	32.28	54.00	-21.72	A
2520.00	67.25	30.01	2.97	44.49	0.40	56.14	75.62	-19.48	P
2520.00	47.25	30.01	2.97	44.49	0.40	36.14	55.62	-19.48	A
* 2834.86	62.39	30.20	3.20	44.35	0.32	51.76	74.00	-22.24	P
* 2834.86	42.39	30.20	3.20	44.35	0.32	31.76	54.00	-22.24	A
3150.13	67.30	30.33	3.46	44.26	0.26	57.09	75.62	-18.53	P
3150.13	47.30	30.33	3.46	44.26	0.26	37.09	55.62	-18.53	A

Notes:

1. Measuring frequencies from 30 MHz to the 1GHz.
2. Radiated emissions measured in frequency range from 30 MHz to 1000MHz were made with an instrument using Peak detector mode.
3. Data of measurement within this frequency range shown “ --- ” in the table above means the reading of emissions are attenuated more than 20dB below the permissible limits or the field strength is too small to be measured.
4. The IF bandwidth of SPA between 1GHz to 4.5GHz was 1MHz.
5. Remark “*”means the Restricted band.
6. Average level=Peak level +Duty factor.

Operation Mode: TX / X Mode **Test Date:** 2018/04/17

Temperature: 26.4 °C **Tested by:** Ted Huang

Humidity: 45% RH **Polarity:** Ver. / Hor.

Vertical

Freq. (MHz)	Reading (dBμV)	AF (dBμV)	Closs (dB)	Pre-amp (dB)	Filter (dB)	Level (dBμV/m)	Limit (dBμV/m)	Margin (dB)	Mark (P/Q/A)	
1260.16	64.44	25.64	2.10	45.22	1.19	48.15	75.62	-27.47	P	
1260.16	44.44	25.64	2.10	45.22	1.19	28.15	55.62	-27.47	A	
*	1575.21	72.30	27.17	2.37	44.97	0.76	57.63	74.00	-16.37	P
*	1575.21	52.30	27.17	2.37	44.97	0.76	37.63	54.00	-16.37	A
	1889.70	65.04	29.56	2.60	44.78	0.50	52.92	75.62	-22.70	P
	1889.70	45.04	29.56	2.60	44.78	0.50	32.92	55.62	-22.70	A
*	2205.06	62.10	30.24	2.79	44.62	0.41	50.92	74.00	-23.08	P
*	2205.06	42.10	30.24	2.79	44.62	0.41	30.92	54.00	-23.08	A
	2520.21	62.43	30.01	2.97	44.49	0.40	51.32	75.62	-24.30	P
	2520.21	42.43	30.01	2.97	44.49	0.40	31.32	55.62	-24.30	A
*	2834.99	59.82	30.20	3.20	44.35	0.32	49.18	74.00	-24.82	P
*	2834.99	39.82	30.20	3.20	44.35	0.32	29.18	54.00	-24.82	A
	3150.13	60.86	30.33	3.46	44.26	0.26	50.64	75.62	-24.98	P
	3150.13	40.86	30.33	3.46	44.26	0.26	30.64	55.62	-24.98	A

Notes:

1. Measuring frequencies from 30 MHz to the 1GHz.
2. Radiated emissions measured in frequency range from 30 MHz to 1000MHz were made with an instrument using Peak detector mode.
3. Data of measurement within this frequency range shown “ --- ” in the table above means the reading of emissions are attenuated more than 20dB below the permissible limits or the field strength is too small to be measured.
4. The IF bandwidth of SPA between 1GHz to 4.5GHz was 1MHz.
5. Remark “*”means the Restricted band.
6. Average level=Peak level +Duty factor.

7.6 POWERLINE CONDUCTED EMISSIONS

LIMIT

For an intentional radiator which is designed to be connected to the public utility (AC) power line, the radio frequency voltage that is conducted back onto the AC power line on any frequency or frequencies within the band 150 kHz to 30 MHz shall not exceed 250 microvolts (The limit decreases linearly with the logarithm of the frequency in the range 0.15 MHz to 0.50 MHz). The limits at specific frequency range is listed as follows:

Frequency Range (MHz)	Limits (dB μ V)	
	Quasi-peak	Average
0.15 to 0.50	66 to 56	56 to 46
0.50 to 5	56	46
5 to 30	60	50

Compliance with this provision shall be based on the measurement of the radio frequency voltage between each power line (LINE and NEUTRAL) and ground at the power terminals.

MEASUREMENT EQUIPMENT USED

Conducted Emission room #1				
Name of Equipment	Manufacturer	Model	Serial Number	Calibration Due
BNC Coaxial Cable	CCS	BNC50	11	01/23/2019
EMI Test Receiver	R&S	ESCS 30	100348	01/30/2019
LISN	SCHWARZBECK	NNLK8130	8130124	11/30/2018
LISN	FCC	FCC-LISN-50-32-2	08009	05/07/2019
Pulse Limiter	R&S	ESH3-Z2	100116	01/23/2019
Software	e-3 (5.04211j)			

Remark: Each piece of equipment is scheduled for calibration once a year.

TEST RESULTS

* This EUT is not connect to AC Source directly. Not applicable for this test.